

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
 Data File : VX034054.D
 Acq On : 07 Feb 2023 11:03
 Operator : JC/MD
 Sample : VX0208MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK614

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

Signal : TIC: VX034054.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	27	29	32	rVB	662	491	0.08%	0.010%
2	1.368	42	46	60	rVB	58355	68256	11.71%	1.447%
3	1.666	91	95	115	rVB	42402	60118	10.32%	1.275%
4	2.307	193	200	210	rBV	125474	196345	33.70%	4.164%
5	2.447	218	223	227	rBV	152	253	0.04%	0.005%
6	2.514	227	234	240	rVV2	996	1890	0.32%	0.040%
7	2.654	255	257	260	rVB	156	202	0.03%	0.004%
8	2.739	268	271	272	rBV	150	183	0.03%	0.004%
9	2.782	274	278	283	rVV4	806	1322	0.23%	0.028%
10	2.880	290	294	297	rBB4	111	162	0.03%	0.003%
11	2.910	297	299	300	rBV4	197	188	0.03%	0.004%
12	2.941	300	304	309	rVV3	580	1215	0.21%	0.026%
13	3.087	324	328	332	rBV2	479	858	0.15%	0.018%
14	3.130	332	335	336	rVB	189	172	0.03%	0.004%
15	3.154	336	339	340	rBV2	174	160	0.03%	0.003%
16	3.282	356	360	362	rBV	157	195	0.03%	0.004%
17	3.587	408	410	414	rVB	178	193	0.03%	0.004%
18	3.678	423	425	427	rBV	172	158	0.03%	0.003%
19	3.733	431	434	437	rBV	193	203	0.03%	0.004%
20	3.843	448	452	455	rBV2	158	318	0.05%	0.007%
21	3.873	455	457	462	rVB	118	188	0.03%	0.004%
22	4.446	543	551	565	rBV	39980	113960	19.56%	2.417%
23	4.812	607	611	613	rBV2	180	204	0.04%	0.004%
24	5.050	637	650	664	rBV	80046	240053	41.20%	5.091%
25	5.178	670	671	677	rVB3	193	248	0.04%	0.005%
26	5.324	690	695	697	rBV	123	235	0.04%	0.005%
27	5.379	701	704	705	rBV	219	252	0.04%	0.005%
28	5.550	726	732	738	rVV2	707	1694	0.29%	0.036%
29	5.757	765	766	770	rBV2	194	208	0.04%	0.004%
30	5.849	778	781	782	rBV	170	157	0.03%	0.003%
31	5.867	782	784	788	rVV	129	197	0.03%	0.004%
32	5.964	788	800	816	rVV2	194521	582641	100.00%	12.356%
33	6.245	844	846	848	rVV	193	169	0.03%	0.004%
34	6.269	848	850	853	rVB	150	158	0.03%	0.003%
35	6.294	853	854	857	rBV	177	166	0.03%	0.004%
36	6.397	870	871	874	rBV	131	165	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
 Data File : VX034054.D
 Acq On : 07 Feb 2023 11:03
 Operator : JC/MD
 Sample : VX0208MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK614

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

37	6.489	883	886	888	rVB	162	164	0.03%	0.003%
38	6.629	906	909	911	rBV	177	168	0.03%	0.004%
39	6.757	919	930	946	rBV	177563	426800	73.25%	9.051%
40	7.031	974	975	979	rBV2	146	206	0.04%	0.004%
41	7.117	983	989	995	rVB5	1302	3151	0.54%	0.067%
42	7.171	997	998	1003	rBV	161	257	0.04%	0.005%
43	7.232	1006	1008	1011	rVB	178	164	0.03%	0.003%
44	7.306	1011	1020	1032	rBV	121805	268456	46.08%	5.693%
45	7.476	1044	1048	1053	rVB2	294	425	0.07%	0.009%
46	7.684	1080	1082	1086	rBB	152	218	0.04%	0.005%
47	7.726	1086	1089	1090	rBV	194	197	0.03%	0.004%
48	7.830	1105	1106	1109	rVV	162	200	0.03%	0.004%
49	8.159	1157	1160	1161	rBV	147	153	0.03%	0.003%
50	8.324	1180	1187	1198	rVV	78354	132599	22.76%	2.812%
51	8.458	1207	1209	1212	rVB	251	190	0.03%	0.004%
52	8.501	1213	1216	1217	rBV	186	177	0.03%	0.004%
53	8.543	1221	1223	1226	rVB	163	203	0.03%	0.004%
54	8.574	1226	1228	1231	rBV	232	264	0.05%	0.006%
55	8.647	1233	1240	1250	rBV	304612	483706	83.02%	10.258%
56	8.946	1284	1289	1302	rBV	56952	85210	14.62%	1.807%
57	9.196	1328	1330	1332	rBV2	179	161	0.03%	0.003%
58	9.232	1332	1336	1340	rVV	152	279	0.05%	0.006%
59	9.281	1340	1344	1348	rVB3	428	670	0.11%	0.014%
60	9.385	1355	1361	1373	rBV	161228	246599	42.32%	5.230%
61	9.702	1410	1413	1416	rVB	283	361	0.06%	0.008%
62	9.744	1418	1420	1422	rBV	227	241	0.04%	0.005%
63	9.872	1440	1441	1445	rVB2	179	215	0.04%	0.005%
64	10.049	1465	1470	1487	rVV	346984	485691	83.36%	10.300%
65	10.195	1491	1494	1500	rVV2	570	767	0.13%	0.016%
66	10.311	1509	1513	1518	rVB3	354	516	0.09%	0.011%
67	10.409	1526	1529	1532	rVB2	155	181	0.03%	0.004%
68	10.439	1532	1534	1540	rBB2	208	257	0.04%	0.005%
69	10.506	1540	1545	1546	rBV	208	250	0.04%	0.005%
70	10.646	1565	1568	1570	rBV2	327	422	0.07%	0.009%
71	10.768	1586	1588	1589	rBV2	185	151	0.03%	0.003%
72	10.957	1617	1619	1624	rVB2	351	477	0.08%	0.010%
73	11.031	1629	1631	1632	rBV	163	168	0.03%	0.004%
74	11.092	1639	1641	1643	rVB	408	321	0.06%	0.007%
75	11.122	1643	1646	1647	rBV	184	157	0.03%	0.003%
76	11.189	1652	1657	1667	rVV	232513	293369	50.35%	6.221%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
 Data File : VX034054.D
 Acq On : 07 Feb 2023 11:03
 Operator : JC/MD
 Sample : VX0208MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK614

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

77	11.311	1674	1677	1681	rVB2	1048	1370	0.24%	0.029%
78	11.457	1693	1701	1703	rBV3	421	675	0.12%	0.014%
79	11.567	1718	1719	1723	rVV2	106	167	0.03%	0.004%
80	11.677	1735	1737	1740	rBV	162	167	0.03%	0.004%
81	11.756	1745	1750	1753	rVB2	546	709	0.12%	0.015%
82	11.976	1782	1786	1788	rBV2	904	1058	0.18%	0.022%
83	12.018	1788	1793	1808	rVB	395152	507317	87.07%	10.758%
84	12.317	1837	1842	1858	rBV	371561	481787	82.69%	10.217%
85	12.451	1863	1864	1868	rVB	187	219	0.04%	0.005%
86	12.488	1868	1870	1871	rBV	215	205	0.04%	0.004%
87	12.762	1911	1915	1921	rVB2	1302	1852	0.32%	0.039%
88	13.116	1969	1973	1977	rVB2	1101	1377	0.24%	0.029%
89	13.390	2015	2018	2019	rBV	150	149	0.03%	0.003%
90	13.591	2047	2051	2056	rVB2	1772	2458	0.42%	0.052%
91	13.780	2078	2082	2089	rVB	1819	2407	0.41%	0.051%
92	13.914	2102	2104	2107	rBV2	132	167	0.03%	0.004%
93	13.963	2108	2112	2118	rVB2	1979	2547	0.44%	0.054%
94	14.128	2136	2139	2143	rBV2	1223	1611	0.28%	0.034%
95	14.353	2172	2176	2179	rBV3	201	378	0.06%	0.008%
96	14.414	2183	2186	2188	rBV	208	241	0.04%	0.005%
97	15.054	2289	2291	2294	rVB2	302	248	0.04%	0.005%
98	15.383	2343	2345	2346	rBV	448	314	0.05%	0.007%
99	15.530	2368	2369	2371	rVB2	277	162	0.03%	0.003%
100	15.731	2400	2402	2403	rBV	272	200	0.03%	0.004%




Sum of corrected areas: 4715523

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
Data File : VX034054.D
Acq On : 07 Feb 2023 11:03
Operator : JC/MD
Sample : VX0208MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK614

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

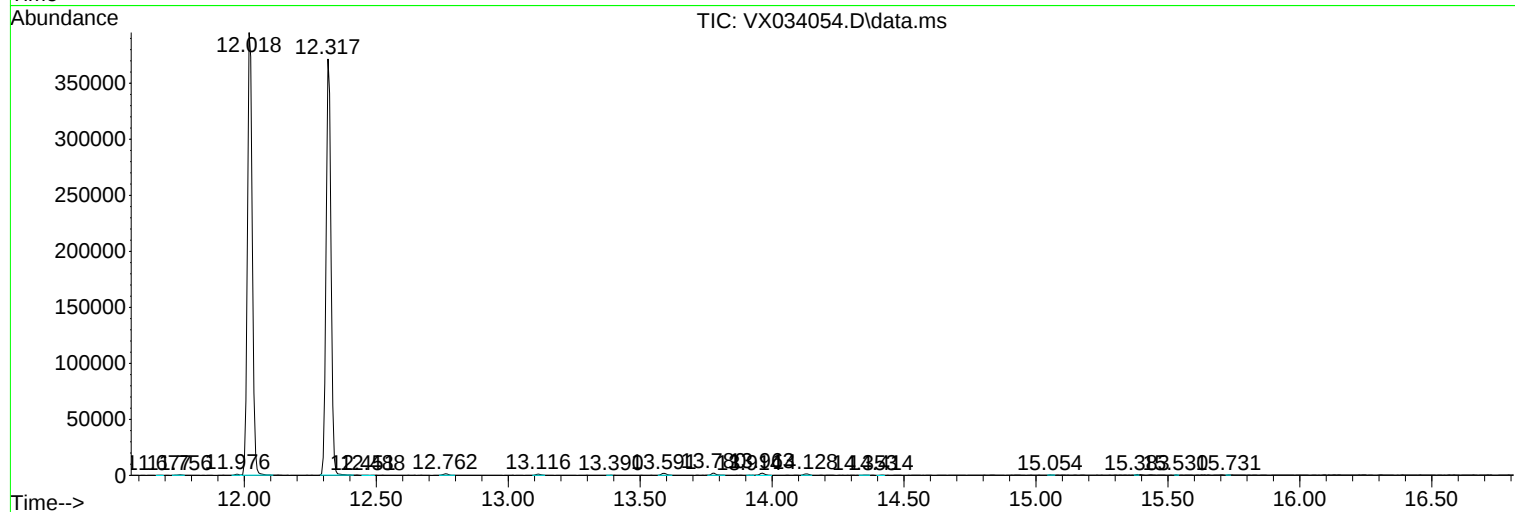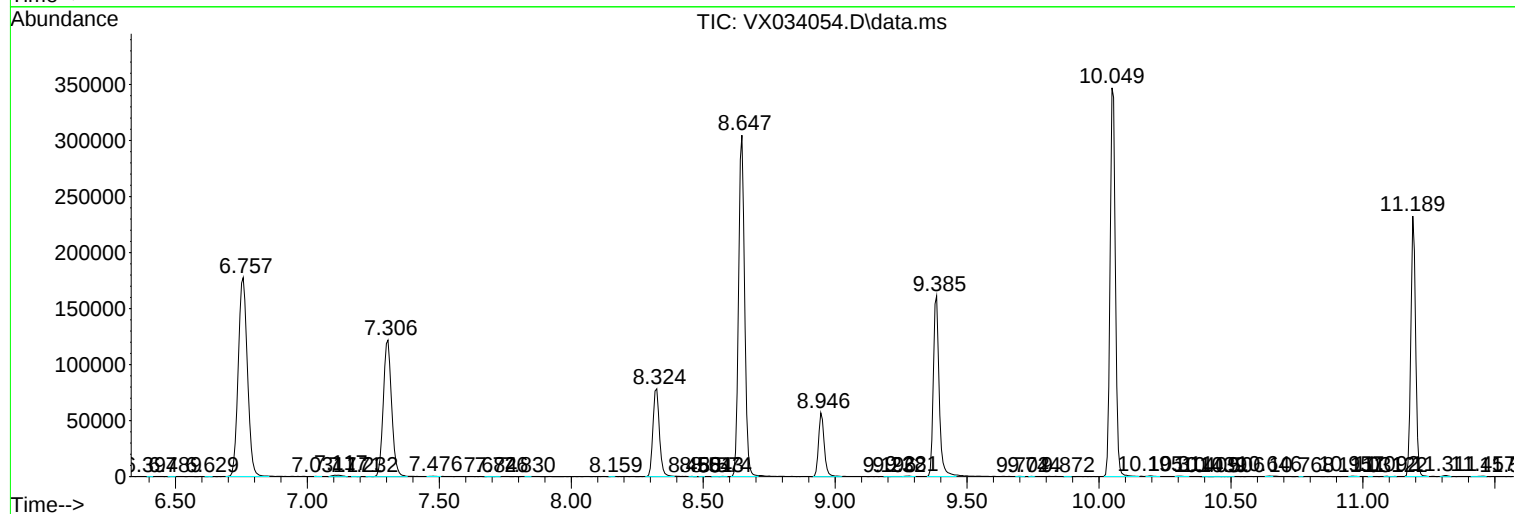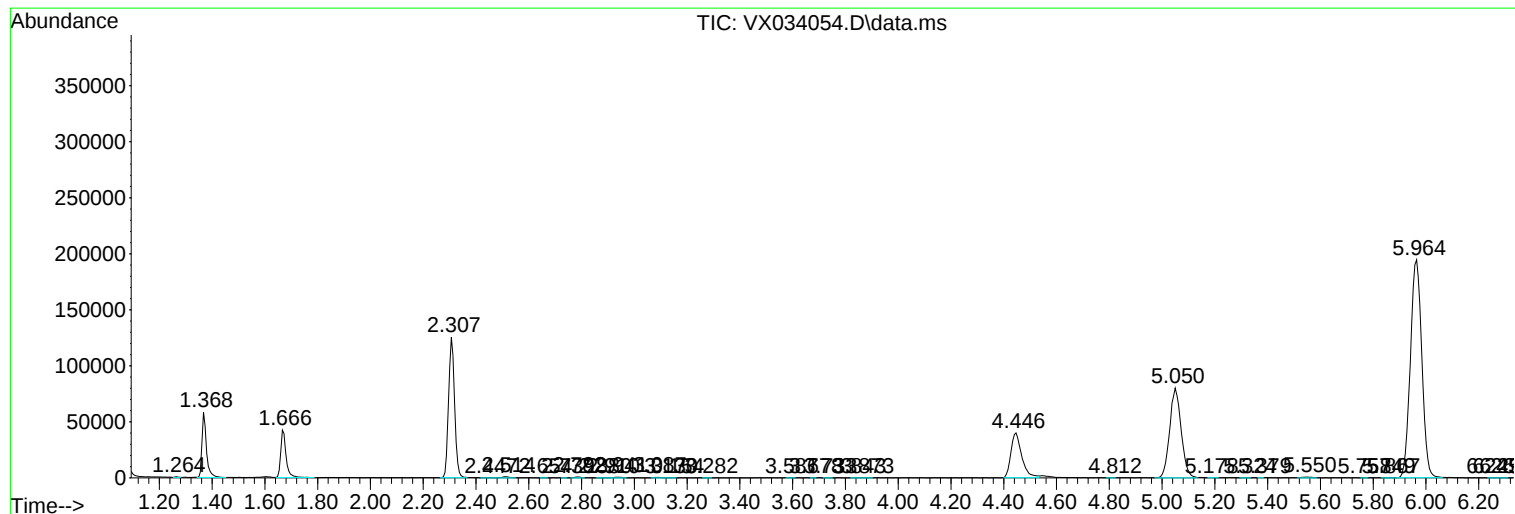

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
Data File : VX034054.D
Acq On : 07 Feb 2023 11:03
Operator : JC/MD
Sample : VX0208MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK614

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
Data File : VX034054.D
Acq On : 07 Feb 2023 11:03
Operator : JC/MD
Sample : VX0208MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK614

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc