

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
 Data File : VX034055.D
 Acq On : 07 Feb 2023 12:31
 Operator : JC/MD
 Sample : VX0208WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK615

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

Signal : TIC: VX034055.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	59	rBV	54540	61781	10.97%	1.347%
2	1.624	87	88	91	rBV2	259	262	0.05%	0.006%
3	1.666	91	95	111	rVB	41092	56093	9.96%	1.223%
4	2.197	180	182	186	rVB	166	200	0.04%	0.004%
5	2.307	193	200	209	rBV	118676	185793	32.99%	4.050%
6	2.435	220	221	226	rVB2	218	236	0.04%	0.005%
7	2.514	226	234	238	rBV2	425	821	0.15%	0.018%
8	2.563	240	242	245	rBB	136	161	0.03%	0.004%
9	2.624	250	252	253	rBV	192	144	0.03%	0.003%
10	2.666	256	259	260	rBV	185	154	0.03%	0.003%
11	2.733	267	270	273	rVB	155	194	0.03%	0.004%
12	2.788	275	279	285	rBV3	818	1532	0.27%	0.033%
13	2.941	299	304	312	rBV2	670	1645	0.29%	0.036%
14	3.123	331	334	336	rBB	142	158	0.03%	0.003%
15	3.355	370	372	374	rBB	177	156	0.03%	0.003%
16	3.495	393	395	397	rVB	194	143	0.03%	0.003%
17	3.520	397	399	401	rBV	159	146	0.03%	0.003%
18	3.648	419	420	424	rVB	151	154	0.03%	0.003%
19	3.971	471	473	475	rBV	148	152	0.03%	0.003%
20	4.209	511	512	517	rVB2	199	281	0.05%	0.006%
21	4.373	536	539	541	rVB2	168	178	0.03%	0.004%
22	4.446	541	551	564	rBV	39732	112250	19.93%	2.447%
23	4.666	584	587	590	rBV2	197	251	0.04%	0.005%
24	4.837	613	615	621	rBV2	153	203	0.04%	0.004%
25	4.910	625	627	629	rVB	165	165	0.03%	0.004%
26	4.940	629	632	633	rBV	180	179	0.03%	0.004%
27	5.056	638	651	668	rBV	74161	231119	41.04%	5.038%
28	5.452	715	716	720	rBV2	171	260	0.05%	0.006%
29	5.544	724	731	732	rBV2	805	1034	0.18%	0.023%
30	5.678	749	753	754	rVB	175	203	0.04%	0.004%
31	5.721	758	760	764	rVB	140	149	0.03%	0.003%
32	5.964	788	800	815	rBV2	187501	563136	100.00%	12.276%
33	6.196	833	838	839	rBB	212	281	0.05%	0.006%
34	6.214	839	841	844	rBV	194	227	0.04%	0.005%
35	6.550	894	896	900	rVB2	159	147	0.03%	0.003%
36	6.641	906	911	914	rBV	154	290	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
 Data File : VX034055.D
 Acq On : 07 Feb 2023 12:31
 Operator : JC/MD
 Sample : VX0208WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK615

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

37	6.757	921	930	945	rBV	181054	429605	76.29%	9.365%
38	6.989	967	968	972	rVB2	177	156	0.03%	0.003%
39	7.111	982	988	995	rBV4	1383	2778	0.49%	0.061%
40	7.226	1006	1007	1011	rBV2	168	273	0.05%	0.006%
41	7.306	1011	1020	1031	rVV	120694	258886	45.97%	5.643%
42	7.421	1038	1039	1042	rBV	168	200	0.04%	0.004%
43	7.476	1044	1048	1049	rBV2	215	243	0.04%	0.005%
44	8.251	1173	1175	1178	rBV2	227	298	0.05%	0.006%
45	8.324	1180	1187	1200	rVV	77091	126453	22.46%	2.756%
46	8.427	1202	1204	1206	rVB2	220	214	0.04%	0.005%
47	8.501	1213	1216	1217	rBV	158	147	0.03%	0.003%
48	8.647	1233	1240	1255	rVV	303860	468196	83.14%	10.206%
49	8.946	1284	1289	1300	rVV	52159	80207	14.24%	1.748%
50	9.092	1311	1313	1317	rVB	185	207	0.04%	0.005%
51	9.141	1318	1321	1324	rBV	166	248	0.04%	0.005%
52	9.275	1339	1343	1345	rVV	410	406	0.07%	0.009%
53	9.385	1355	1361	1382	rBV	160384	246496	43.77%	5.373%
54	9.574	1391	1392	1397	rBV2	277	379	0.07%	0.008%
55	9.988	1458	1460	1465	rVB	130	159	0.03%	0.003%
56	10.049	1465	1470	1483	rBV	340996	486329	86.36%	10.601%
57	10.171	1489	1490	1492	rVB	279	151	0.03%	0.003%
58	10.189	1492	1493	1498	rVB3	332	431	0.08%	0.009%
59	10.403	1525	1528	1529	rVB3	156	154	0.03%	0.003%
60	10.433	1529	1533	1534	rBV2	185	240	0.04%	0.005%
61	10.488	1539	1542	1544	rBV	188	159	0.03%	0.003%
62	10.970	1616	1621	1623	rBV2	200	299	0.05%	0.007%
63	11.043	1630	1633	1635	rBB2	124	146	0.03%	0.003%
64	11.128	1645	1647	1649	rVB	177	153	0.03%	0.003%
65	11.189	1652	1657	1665	rBV	223773	287292	51.02%	6.263%
66	11.317	1673	1678	1685	rVB2	1190	1789	0.32%	0.039%
67	11.384	1688	1689	1693	rVV2	187	181	0.03%	0.004%
68	11.427	1693	1696	1698	rVV2	151	215	0.04%	0.005%
69	11.451	1698	1700	1701	rVB	260	159	0.03%	0.003%
70	11.488	1704	1706	1709	rVV	142	139	0.02%	0.003%
71	11.665	1733	1735	1738	rBV	136	154	0.03%	0.003%
72	11.713	1741	1743	1745	rBV	227	226	0.04%	0.005%
73	11.750	1748	1749	1752	rVB	249	241	0.04%	0.005%
74	11.823	1759	1761	1765	rBV2	166	211	0.04%	0.005%
75	11.927	1776	1778	1782	rBV2	141	163	0.03%	0.004%
76	12.018	1788	1793	1805	rBV	383019	500603	88.90%	10.912%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
 Data File : VX034055.D
 Acq On : 07 Feb 2023 12:31
 Operator : JC/MD
 Sample : VX0208WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK615

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1850	rBV	361390	462869	82.19%	10.090%
78	12.457	1862	1865	1868	rBV	217	273	0.05%	0.006%
79	12.616	1889	1891	1894	rVV2	193	279	0.05%	0.006%
80	12.658	1896	1898	1902	rVV	172	251	0.04%	0.005%
81	12.762	1909	1915	1924	rBV3	1260	1983	0.35%	0.043%
82	12.847	1927	1929	1934	rBV2	106	206	0.04%	0.004%
83	12.957	1943	1947	1948	rBV	167	136	0.02%	0.003%
84	13.116	1971	1973	1975	rBV	262	216	0.04%	0.005%
85	13.164	1977	1981	1984	rBV	155	263	0.05%	0.006%
86	13.341	2005	2010	2011	rBV	119	195	0.03%	0.004%
87	13.487	2031	2034	2036	rBV2	139	187	0.03%	0.004%
88	13.591	2048	2051	2056	rBV2	385	679	0.12%	0.015%
89	13.780	2080	2082	2087	rVB2	394	553	0.10%	0.012%
90	13.817	2087	2088	2091	rBV2	159	184	0.03%	0.004%
91	13.963	2110	2112	2114	rVB	179	142	0.03%	0.003%
92	14.030	2122	2123	2127	rVB	175	146	0.03%	0.003%
93	14.097	2127	2134	2135	rBV	174	324	0.06%	0.007%
94	14.128	2135	2139	2145	rBV2	1163	1772	0.31%	0.039%
95	14.310	2168	2169	2173	rVV	164	162	0.03%	0.004%
96	14.493	2198	2199	2201	rBV	222	155	0.03%	0.003%
97	14.725	2236	2237	2241	rBV2	199	229	0.04%	0.005%
98	15.310	2331	2333	2335	rBV	270	168	0.03%	0.004%
99	15.383	2342	2345	2346	rBV2	454	482	0.09%	0.011%
100	15.828	2415	2418	2421	rBV4	270	357	0.06%	0.008%




Sum of corrected areas: 4587475

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
Data File : VX034055.D
Acq On : 07 Feb 2023 12:31
Operator : JC/MD
Sample : VX0208WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK615

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

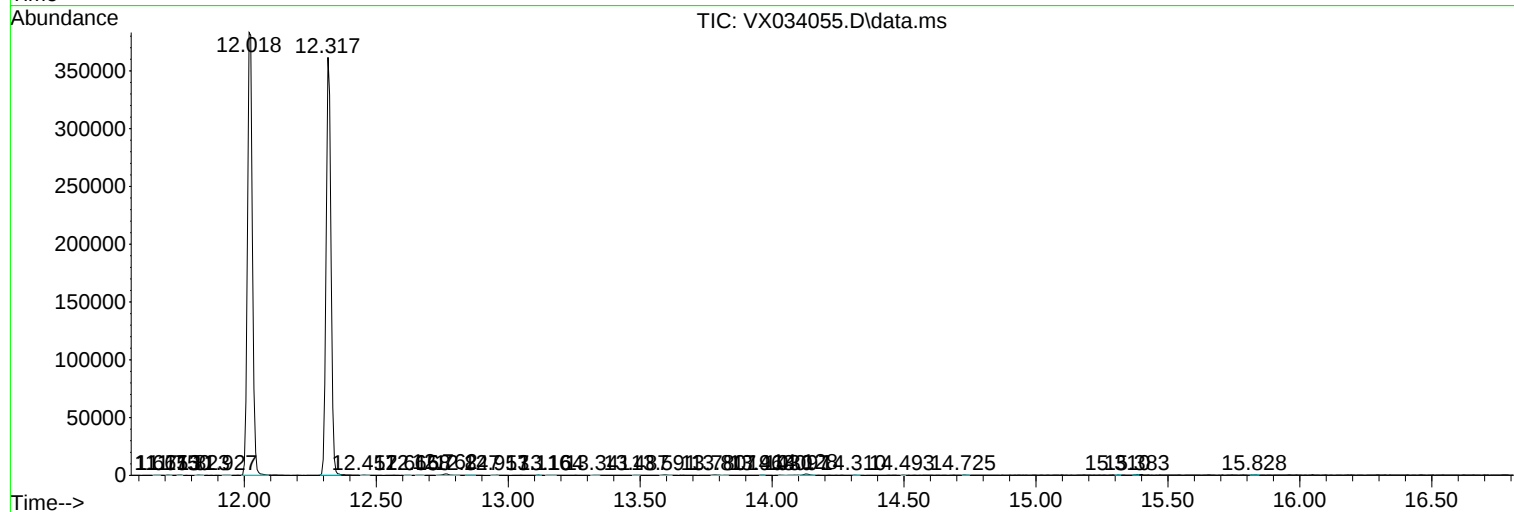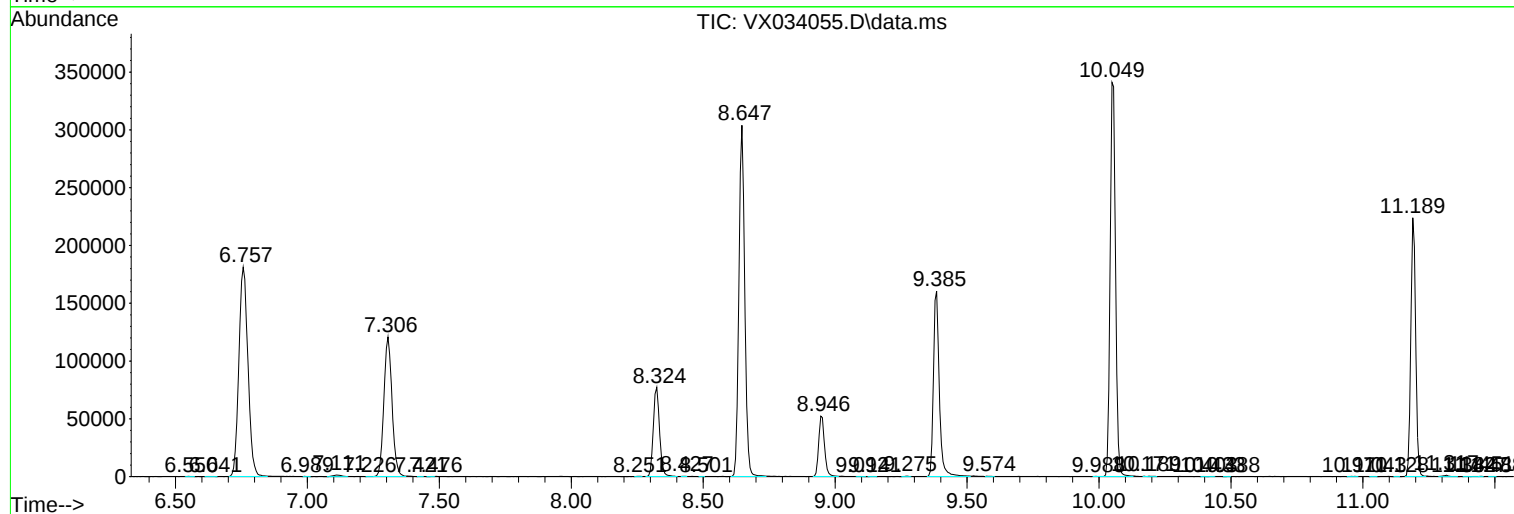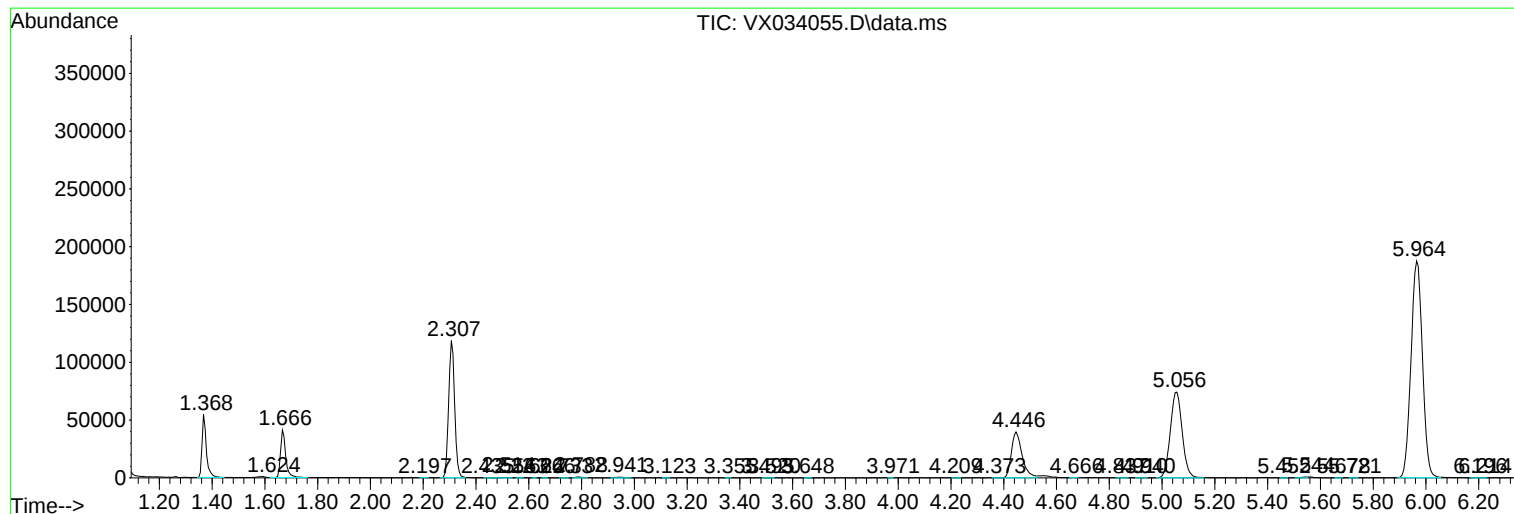

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
Data File : VX034055.D
Acq On : 07 Feb 2023 12:31
Operator : JC/MD
Sample : VX0208WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK615

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
Data File : VX034055.D
Acq On : 07 Feb 2023 12:31
Operator : JC/MD
Sample : VX0208WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK615

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc