

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
 Data File : VX034057.D
 Acq On : 07 Feb 2023 13:24
 Operator : JC/MD
 Sample : 01394-04ME
 Misc : 3.65g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C1152ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

Signal : TIC: VX034057.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	26	28	32	rBV2	827	960	0.13%	0.018%
2	1.374	43	47	65	rBV	43903	84765	11.85%	1.558%
3	1.563	69	78	79	rBV4	1634	3475	0.49%	0.064%
4	1.648	89	92	98	rBV	17423	31521	4.41%	0.579%
5	2.063	159	160	163	rBV2	161	136	0.02%	0.002%
6	2.093	163	165	168	rVB	233	226	0.03%	0.004%
7	2.215	180	185	191	rBV2	565	773	0.11%	0.014%
8	2.288	191	197	209	rBV	140644	222846	31.16%	4.096%
9	2.489	227	230	235	rBV3	324	483	0.07%	0.009%
10	2.678	258	261	264	rBV2	128	209	0.03%	0.004%
11	2.782	272	278	283	rBV2	2480	4855	0.68%	0.089%
12	2.947	298	305	310	rBV	3949	8076	1.13%	0.148%
13	3.099	329	330	335	rVB	133	149	0.02%	0.003%
14	3.245	353	354	356	rBV	225	162	0.02%	0.003%
15	3.270	356	358	361	rVB	159	211	0.03%	0.004%
16	3.428	381	384	385	rVV2	387	298	0.04%	0.005%
17	3.489	392	394	399	rBV	194	299	0.04%	0.005%
18	3.739	432	435	437	rBV2	193	235	0.03%	0.004%
19	3.904	459	462	464	rBV	111	130	0.02%	0.002%
20	4.050	484	486	487	rBV	196	156	0.02%	0.003%
21	4.160	501	504	505	rBV	114	143	0.02%	0.003%
22	4.208	509	512	513	rBV	210	220	0.03%	0.004%
23	4.465	545	554	571	rBV2	41493	135726	18.98%	2.494%
24	4.885	621	623	624	rBV2	199	146	0.02%	0.003%
25	5.056	639	651	671	rVB	90300	286638	40.08%	5.268%
26	5.196	671	674	675	rVB2	185	172	0.02%	0.003%
27	5.269	685	686	692	rBV2	118	213	0.03%	0.004%
28	5.379	700	704	705	rBV2	335	479	0.07%	0.009%
29	5.538	727	730	731	rBV2	517	556	0.08%	0.010%
30	5.848	779	781	784	rVB	176	217	0.03%	0.004%
31	5.885	784	787	788	rBV	190	156	0.02%	0.003%
32	5.964	788	800	816	rBV2	248660	715102	100.00%	13.143%
33	6.184	833	836	837	rBV2	203	200	0.03%	0.004%
34	6.208	837	840	842	rVV2	147	141	0.02%	0.003%
35	6.263	846	849	850	rBV	154	146	0.02%	0.003%
36	6.367	859	866	868	rBV5	521	1002	0.14%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
 Data File : VX034057.D
 Acq On : 07 Feb 2023 13:24
 Operator : JC/MD
 Sample : 01394-04ME
 Misc : 3.65g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C1152ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

37	6.434	873	877	878	rBV	163	141	0.02%	0.003%
38	6.513	887	890	891	rBV	128	139	0.02%	0.003%
39	6.757	921	930	946	rBV	192619	455850	63.75%	8.378%
40	6.995	966	969	971	rBV2	160	208	0.03%	0.004%
41	7.117	980	989	997	rBV4	1681	3838	0.54%	0.071%
42	7.208	997	1004	1011	rBV4	1008	2704	0.38%	0.050%
43	7.306	1011	1020	1037	rVB	149017	327692	45.82%	6.023%
44	7.476	1046	1048	1054	rBV2	364	569	0.08%	0.010%
45	7.623	1069	1072	1073	rBV2	162	160	0.02%	0.003%
46	7.683	1079	1082	1084	rBV	193	168	0.02%	0.003%
47	7.757	1092	1094	1099	rVB2	152	191	0.03%	0.004%
48	7.799	1099	1101	1105	rVB2	179	195	0.03%	0.004%
49	7.909	1117	1119	1121	rVB	181	182	0.03%	0.003%
50	7.940	1121	1124	1125	rBV	154	211	0.03%	0.004%
51	8.324	1180	1187	1201	rBV	91420	150781	21.09%	2.771%
52	8.592	1227	1231	1233	rBV3	182	288	0.04%	0.005%
53	8.647	1233	1240	1255	rBV	377957	592024	82.79%	10.881%
54	8.952	1284	1290	1300	rBV	60720	95077	13.30%	1.747%
55	9.098	1312	1314	1317	rBV	170	184	0.03%	0.003%
56	9.238	1334	1337	1339	rBV2	93	132	0.02%	0.002%
57	9.275	1340	1343	1347	rBB4	414	468	0.07%	0.009%
58	9.330	1350	1352	1354	rBV2	167	176	0.02%	0.003%
59	9.403	1356	1364	1383	rBV	148659	305530	42.73%	5.615%
60	9.653	1401	1405	1406	rBV	120	145	0.02%	0.003%
61	9.708	1412	1414	1419	rBV2	523	771	0.11%	0.014%
62	10.055	1465	1471	1487	rBV	346192	493938	69.07%	9.078%
63	10.195	1491	1494	1501	rVB3	418	746	0.10%	0.014%
64	10.311	1508	1513	1517	rBV2	567	882	0.12%	0.016%
65	10.409	1527	1529	1530	rBV2	134	137	0.02%	0.003%
66	10.555	1551	1553	1557	rBV	142	164	0.02%	0.003%
67	10.592	1557	1559	1562	rVB	116	146	0.02%	0.003%
68	10.646	1565	1568	1570	rBV2	347	328	0.05%	0.006%
69	10.701	1575	1577	1579	rBV	136	153	0.02%	0.003%
70	10.799	1589	1593	1595	rBV2	136	187	0.03%	0.003%
71	10.915	1608	1612	1613	rBV2	158	215	0.03%	0.004%
72	10.969	1619	1621	1622	rVB2	256	131	0.02%	0.002%
73	11.195	1652	1658	1668	rBV	277047	362430	50.68%	6.661%
74	11.317	1673	1678	1685	rVB3	1339	1902	0.27%	0.035%
75	11.451	1698	1700	1704	rVB	236	306	0.04%	0.006%
76	11.591	1720	1723	1724	rBV	186	161	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
 Data File : VX034057.D
 Acq On : 07 Feb 2023 13:24
 Operator : JC/MD
 Sample : 01394-04ME
 Misc : 3.65g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C1152ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

77	11.762	1747	1751	1753	rVB2	387	434	0.06%	0.008%
78	11.860	1764	1767	1769	rBV	146	171	0.02%	0.003%
79	11.975	1784	1786	1789	rBV	300	206	0.03%	0.004%
80	12.024	1789	1794	1804	rBV	430597	534734	74.78%	9.828%
81	12.195	1820	1822	1824	rBV2	181	215	0.03%	0.004%
82	12.244	1827	1830	1831	rBV2	127	141	0.02%	0.003%
83	12.323	1837	1843	1851	rBV	471109	595921	83.33%	10.952%
84	12.463	1864	1866	1870	rBV2	234	323	0.05%	0.006%
85	12.762	1911	1915	1920	rBV2	1720	2341	0.33%	0.043%
86	12.841	1925	1928	1930	rBV	173	249	0.03%	0.005%
87	13.097	1967	1970	1972	rBV	126	138	0.02%	0.003%
88	13.122	1972	1974	1976	rVB2	221	204	0.03%	0.004%
89	13.329	2006	2008	2015	rVB	186	350	0.05%	0.006%
90	13.384	2015	2017	2020	rBV2	186	179	0.03%	0.003%
91	13.524	2038	2040	2042	rBV	138	149	0.02%	0.003%
92	13.597	2047	2052	2055	rBV3	252	466	0.07%	0.009%
93	13.786	2079	2083	2087	rBV2	294	485	0.07%	0.009%
94	14.127	2135	2139	2144	rVB2	1121	1420	0.20%	0.026%
95	14.329	2171	2172	2175	rBV	186	192	0.03%	0.004%
96	14.761	2241	2243	2244	rBV	241	155	0.02%	0.003%
97	14.944	2271	2273	2276	rBV2	218	171	0.02%	0.003%
98	15.176	2309	2311	2312	rBV2	250	139	0.02%	0.003%
99	15.359	2339	2341	2342	rBV	282	205	0.03%	0.004%
100	15.389	2342	2346	2351	rVB4	698	1199	0.17%	0.022%




Sum of corrected areas: 5441059

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
Data File : VX034057.D
Acq On : 07 Feb 2023 13:24
Operator : JC/MD
Sample : 01394-04ME
Misc : 3.65g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C1152ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

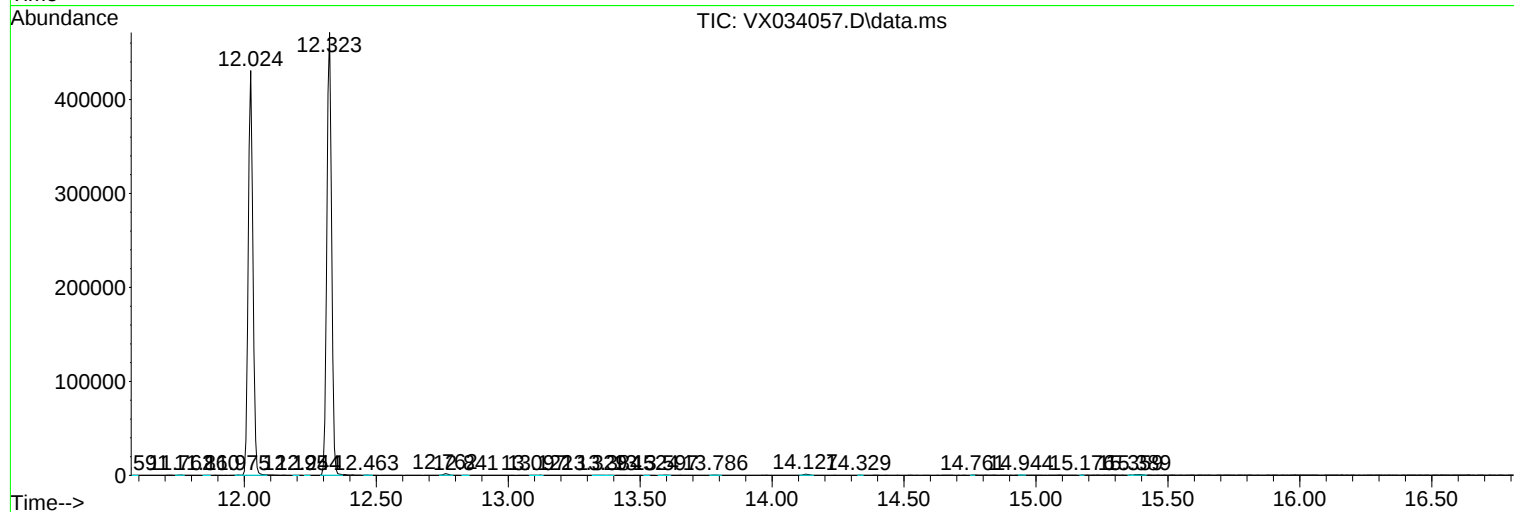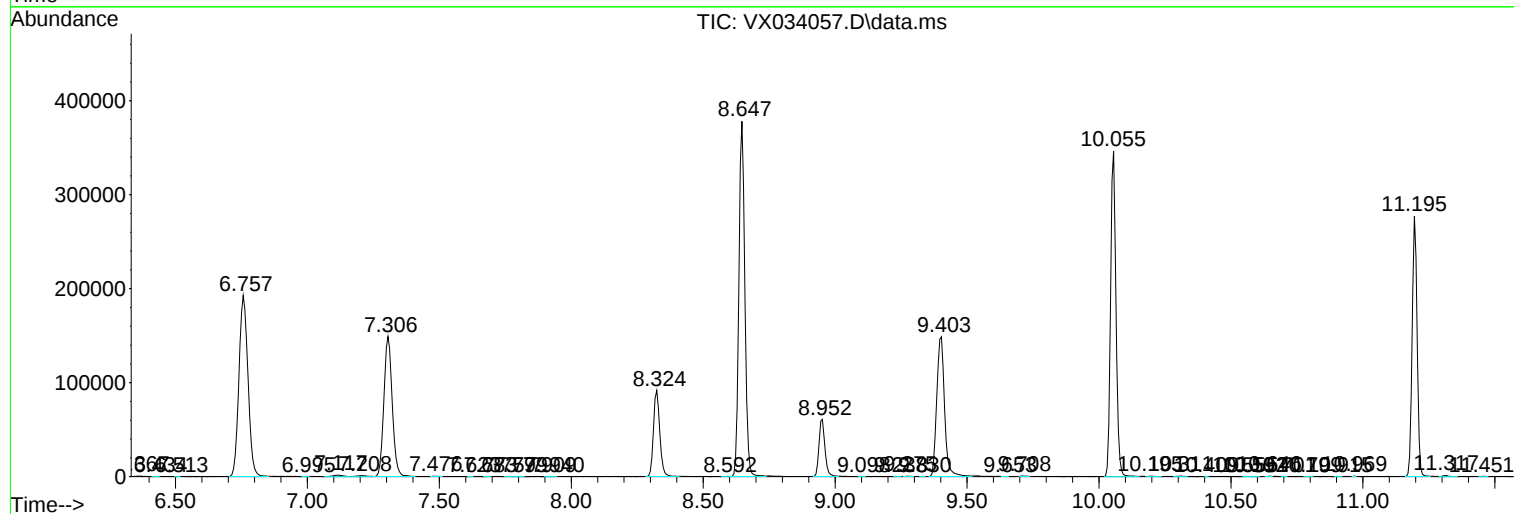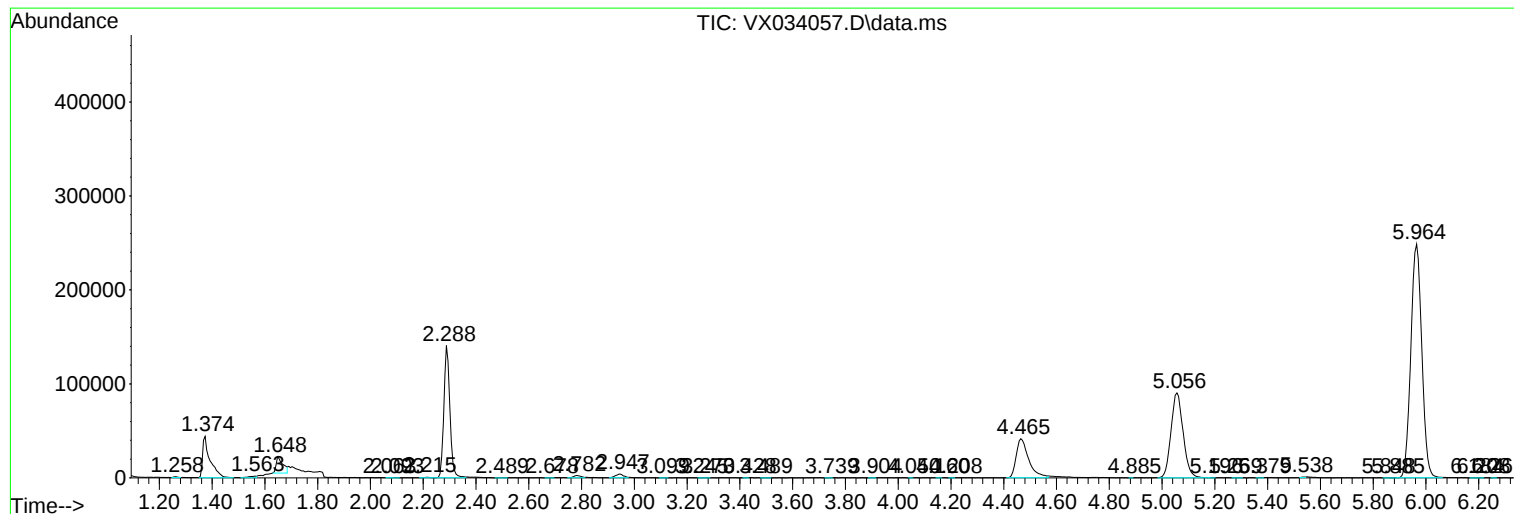

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
Data File : VX034057.D
Acq On : 07 Feb 2023 13:24
Operator : JC/MD
Sample : 01394-04ME
Misc : 3.65g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C1152ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
Data File : VX034057.D
Acq On : 07 Feb 2023 13:24
Operator : JC/MD
Sample : 01394-04ME
Misc : 3.65g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C1152ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc