

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
 Data File : VX034058.D
 Acq On : 07 Feb 2023 13:55
 Operator : JC/MD
 Sample : VIBLK612
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK612

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M

Title : VOC Analysis

Signal : TIC: VX034058.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.257	26	28	32	rVB2	738	835	0.16%	0.020%
2	1.367	42	46	59	rVB	47598	53396	9.98%	1.274%
3	1.635	88	90	91	rBV2	239	122	0.02%	0.003%
4	1.666	91	95	110	rVB	36987	50448	9.43%	1.204%
5	2.166	175	177	180	rBV	191	226	0.04%	0.005%
6	2.306	194	200	211	rBV	101838	157137	29.37%	3.750%
7	2.513	230	234	237	rVB2	297	410	0.08%	0.010%
8	2.678	258	261	263	rBV2	128	154	0.03%	0.004%
9	2.794	275	280	286	rBV4	906	1733	0.32%	0.041%
10	2.940	298	304	309	rBV3	1058	2331	0.44%	0.056%
11	3.086	326	328	330	rBV3	152	132	0.02%	0.003%
12	3.160	337	340	343	rBV2	179	205	0.04%	0.005%
13	3.251	353	355	358	rBB2	167	162	0.03%	0.004%
14	3.300	361	363	366	rBV	110	149	0.03%	0.004%
15	3.342	366	370	372	rVB	184	218	0.04%	0.005%
16	3.428	382	384	386	rBB	168	170	0.03%	0.004%
17	3.763	436	439	440	rBV	141	144	0.03%	0.003%
18	3.891	458	460	463	rBB	155	125	0.02%	0.003%
19	3.946	467	469	471	rBV	197	173	0.03%	0.004%
20	4.208	510	512	516	rVB2	133	164	0.03%	0.004%
21	4.251	516	519	522	rVB2	210	249	0.05%	0.006%
22	4.306	522	528	530	rBV	176	310	0.06%	0.007%
23	4.446	542	551	565	rBV2	38482	113289	21.18%	2.704%
24	4.720	594	596	600	rBV2	151	169	0.03%	0.004%
25	4.769	600	604	605	rVB	211	199	0.04%	0.005%
26	4.867	618	620	622	rBV	192	212	0.04%	0.005%
27	5.056	639	651	667	rBV	68640	216152	40.41%	5.159%
28	5.391	700	706	707	rBV2	594	1047	0.20%	0.025%
29	5.543	724	731	734	rBV3	1376	3033	0.57%	0.072%
30	5.757	763	766	769	rBV2	127	153	0.03%	0.004%
31	5.830	774	778	780	rBV	159	172	0.03%	0.004%
32	5.964	789	800	819	rVV2	177773	534957	100.00%	12.767%
33	6.275	849	851	853	rBV	105	134	0.03%	0.003%
34	6.311	855	857	859	rVV	133	159	0.03%	0.004%
35	6.385	867	869	873	rBV2	143	208	0.04%	0.005%
36	6.549	893	896	901	rVB	364	510	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
 Data File : VX034058.D
 Acq On : 07 Feb 2023 13:55
 Operator : JC/MD
 Sample : VIBLK612
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK612

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

37	6.671	915	916	918	rBV	190	154	0.03%	0.004%
38	6.757	921	930	948	rBV	161853	382086	71.42%	9.119%
39	6.976	964	966	968	rBV2	260	267	0.05%	0.006%
40	7.116	983	989	994	rBV4	1160	2578	0.48%	0.062%
41	7.195	1001	1002	1005	rBV	122	122	0.02%	0.003%
42	7.305	1011	1020	1032	rBV	115059	247595	46.28%	5.909%
43	7.445	1041	1043	1046	rBV	109	132	0.02%	0.003%
44	7.750	1091	1093	1096	rVB	180	124	0.02%	0.003%
45	7.781	1096	1098	1102	rVB2	156	185	0.03%	0.004%
46	7.884	1113	1115	1119	rVB	159	208	0.04%	0.005%
47	7.921	1119	1121	1123	rBV	178	218	0.04%	0.005%
48	7.988	1130	1132	1135	rBV2	109	151	0.03%	0.004%
49	8.043	1137	1141	1143	rBV2	122	139	0.03%	0.003%
50	8.323	1181	1187	1200	rBV	70634	113725	21.26%	2.714%
51	8.518	1217	1219	1220	rBV	183	131	0.02%	0.003%
52	8.579	1227	1229	1231	rVB	194	163	0.03%	0.004%
53	8.646	1234	1240	1259	rVB	270749	424196	79.30%	10.124%
54	8.817	1266	1268	1270	rBV2	184	168	0.03%	0.004%
55	8.945	1284	1289	1300	rBV	47655	73386	13.72%	1.751%
56	9.073	1307	1310	1313	rBV2	205	319	0.06%	0.008%
57	9.274	1340	1343	1347	rVB2	317	446	0.08%	0.011%
58	9.384	1355	1361	1383	rBV	162771	248075	46.37%	5.921%
59	9.640	1400	1403	1405	rVV2	187	174	0.03%	0.004%
60	9.665	1405	1407	1409	rVB	200	155	0.03%	0.004%
61	9.695	1410	1412	1417	rVB	257	349	0.07%	0.008%
62	9.738	1417	1419	1422	rVB	122	142	0.03%	0.003%
63	9.768	1422	1424	1425	rBV	139	122	0.02%	0.003%
64	10.055	1465	1471	1483	rBV	311138	423690	79.20%	10.112%
65	10.195	1492	1494	1496	rVV	217	163	0.03%	0.004%
66	10.219	1496	1498	1500	rVB2	225	172	0.03%	0.004%
67	10.311	1510	1513	1517	rVB3	361	513	0.10%	0.012%
68	10.347	1517	1519	1521	rBV	136	129	0.02%	0.003%
69	10.488	1540	1542	1543	rBV	175	123	0.02%	0.003%
70	10.506	1543	1545	1547	rBV	95	120	0.02%	0.003%
71	10.640	1565	1567	1570	rVB	142	121	0.02%	0.003%
72	10.725	1579	1581	1585	rBV2	115	152	0.03%	0.004%
73	10.829	1595	1598	1602	rBV	162	208	0.04%	0.005%
74	10.884	1605	1607	1610	rBV2	148	182	0.03%	0.004%
75	11.091	1639	1641	1646	rVB2	275	339	0.06%	0.008%
76	11.146	1646	1650	1652	rBV2	207	354	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
 Data File : VX034058.D
 Acq On : 07 Feb 2023 13:55
 Operator : JC/MD
 Sample : VIBLK612
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK612

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
 Title : VOC Analysis

77	11.189	1652	1657	1671	rVV	218567	281188	52.56%	6.711%
78	11.311	1674	1677	1681	rVB2	868	986	0.18%	0.024%
79	11.402	1690	1692	1694	rBV	155	167	0.03%	0.004%
80	11.762	1748	1751	1753	rBV	222	266	0.05%	0.006%
81	12.018	1788	1793	1804	rBV	330013	424277	79.31%	10.126%
82	12.249	1829	1831	1833	rVB	160	131	0.02%	0.003%
83	12.316	1837	1842	1850	rBV	315813	415862	77.74%	9.925%
84	12.469	1864	1867	1868	rBV2	163	168	0.03%	0.004%
85	12.512	1871	1874	1875	rBV	134	140	0.03%	0.003%
86	12.597	1884	1888	1891	rVB2	129	210	0.04%	0.005%
87	12.627	1891	1893	1897	rBV2	134	219	0.04%	0.005%
88	12.762	1912	1915	1920	rVB3	1127	1568	0.29%	0.037%
89	13.347	2009	2011	2013	rVV	187	148	0.03%	0.004%
90	13.377	2015	2016	2019	rVB	198	158	0.03%	0.004%
91	13.597	2050	2052	2055	rVB3	184	189	0.04%	0.005%
92	13.914	2102	2104	2107	rBV2	224	335	0.06%	0.008%
93	13.993	2114	2117	2120	rBV	213	305	0.06%	0.007%
94	14.127	2136	2139	2144	rBV	1095	1404	0.26%	0.034%
95	14.200	2148	2151	2152	rBV2	131	129	0.02%	0.003%
96	14.420	2183	2187	2189	rBV2	179	230	0.04%	0.005%
97	14.530	2201	2205	2207	rBV2	191	199	0.04%	0.005%
98	14.554	2207	2209	2211	rVB	224	144	0.03%	0.003%
99	14.700	2231	2233	2235	rBV	189	166	0.03%	0.004%
100	16.523	2530	2532	2533	rBV2	287	240	0.04%	0.006%




Sum of corrected areas: 4189992

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
Data File : VX034058.D
Acq On : 07 Feb 2023 13:55
Operator : JC/MD
Sample : VIBLK612
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

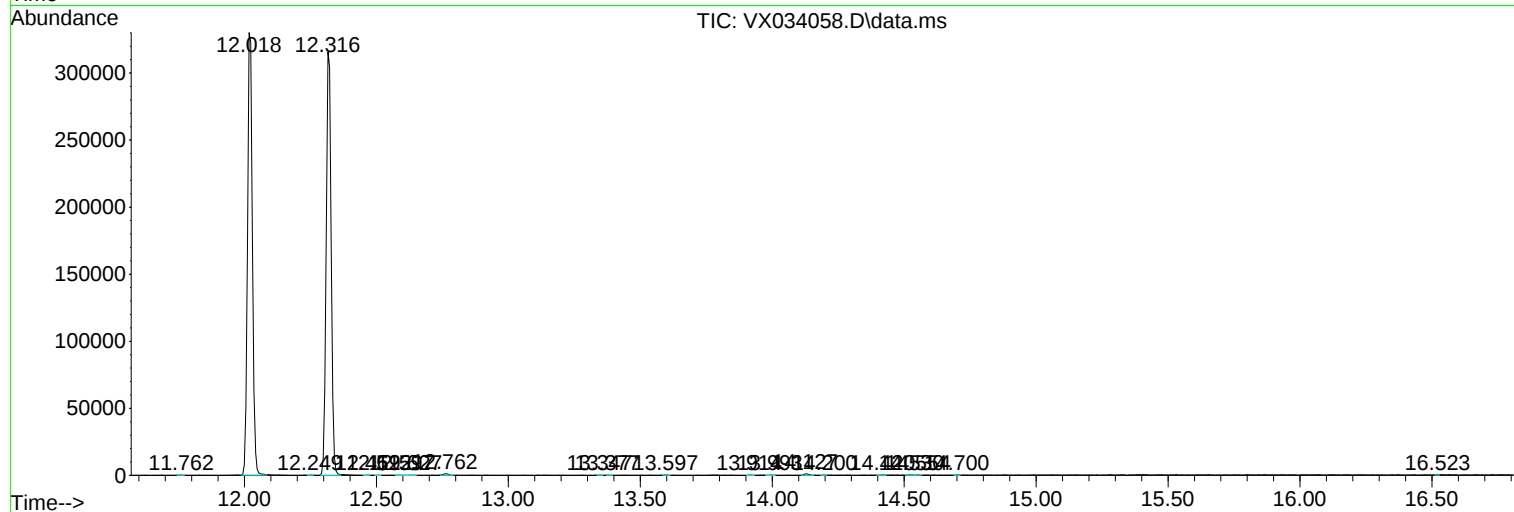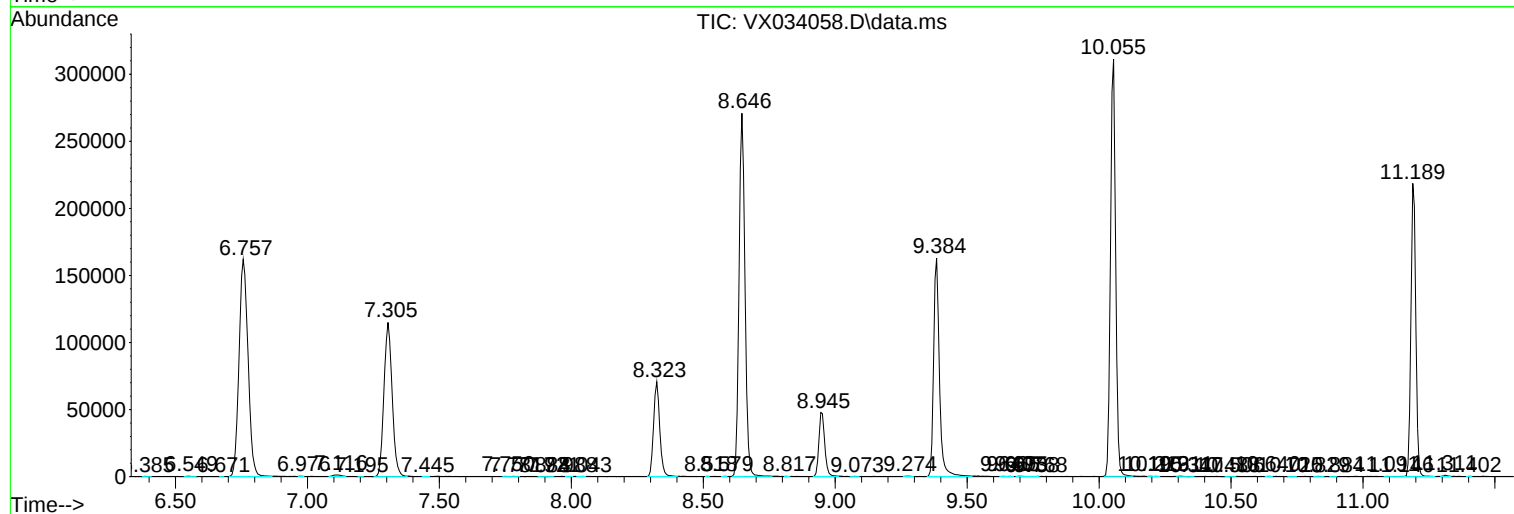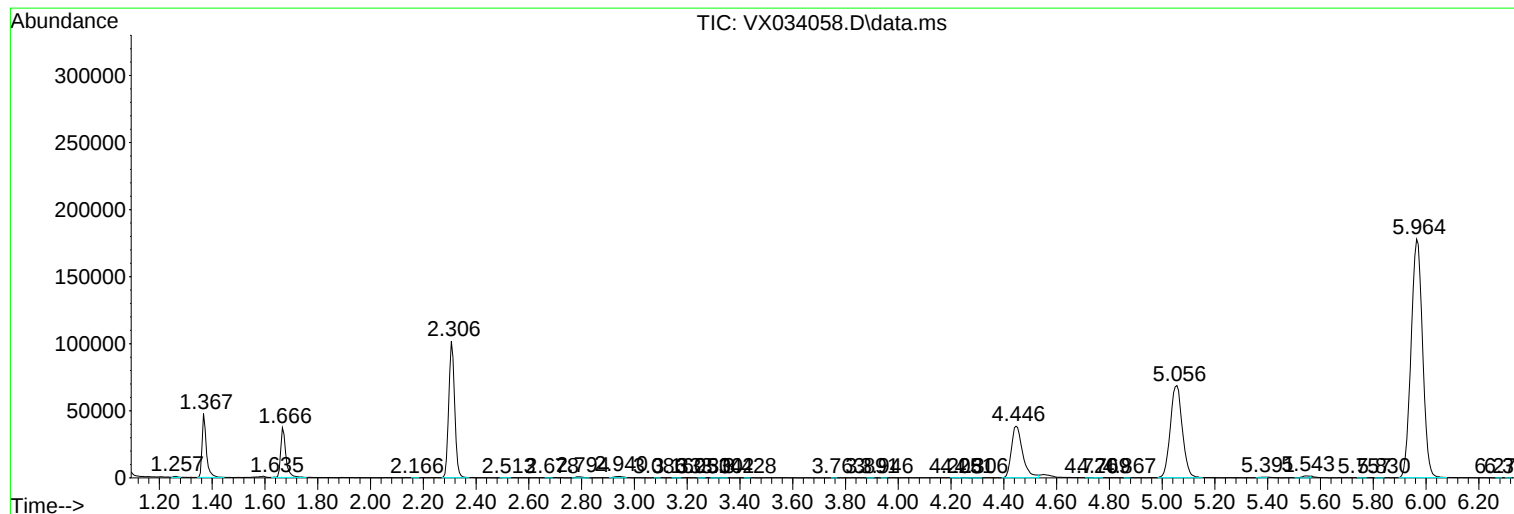

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
Data File : VX034058.D
Acq On : 07 Feb 2023 13:55
Operator : JC/MD
Sample : VIBLK612
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
Data File : VX034058.D
Acq On : 07 Feb 2023 13:55
Operator : JC/MD
Sample : VIBLK612
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML020223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc