


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020823\
 Data File : VX034052.D
 Acq On : 07 Feb 2023 08:53
 Operator : JC/MD
 Sample : BFB610
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB610

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM020223WMA.M
 Title : VOC Analysis
 Last Update : Tue Feb 07 20:42:13 2023

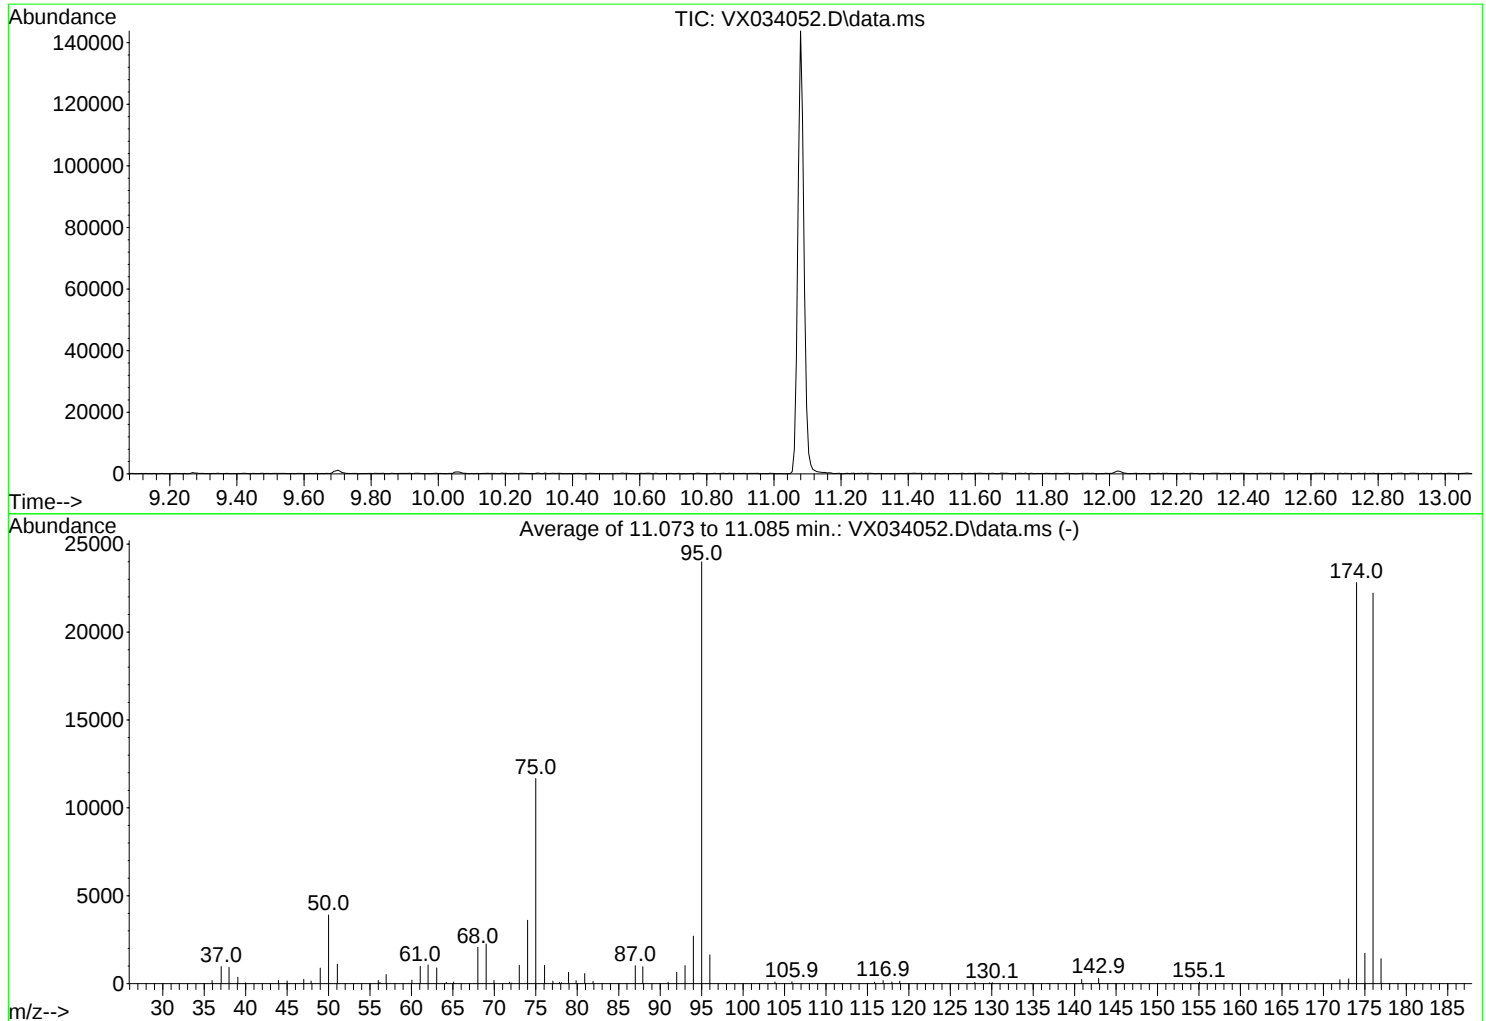

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	3905	PASS
75	95	30	80	48.6	11669	PASS
95	95	100	100	100.0	23995	PASS
96	95	5	9	6.8	1637	PASS
173	174	0.00	2	1.2	275	PASS
174	95	50	120	95.1	22821	PASS
175	174	5	9	7.6	1728	PASS
176	174	95	101	97.4	22222	PASS
177	176	5	9	6.4	1423	PASS

m/z	Abundance
40.00	70.0

Instrument :
MSVOA_X
ClientSampleId :
BFB610

m/z	Abundance
36.00	167.0
37.00	1052.0
38.00	944.0
39.10	321.0
40.10	143.0
43.90	192.0
45.00	182.0
47.00	288.0
47.90	138.0
49.00	923.0
50.00	3681.0
51.10	1018.0
56.00	212.0
56.90	524.0
60.10	185.0
61.00	854.0
62.00	1166.0
63.00	709.0
64.20	73.0
65.10	100.0
68.00	1912.0
69.00	1984.0
70.00	166.0
71.90	129.0
73.00	1007.0
74.00	2995.0
75.00	10601.0
76.00	831.0
77.00	188.0
77.80	103.0
78.90	572.0
79.80	108.0
80.90	582.0
82.00	87.0
87.00	892.0
88.10	758.0
91.00	106.0
92.00	565.0
93.00	968.0
94.00	2302.0
95.00	20208.0
96.00	1596.0
103.90	83.0
106.00	90.0
115.90	83.0
116.90	179.0
118.00	75.0
118.90	129.0
127.90	54.0
129.80	80.0
140.80	187.0
142.90	252.0
155.00	66.0
172.00	97.0
173.10	169.0
174.00	16624.0
175.00	1227.0
176.00	16155.0
177.00	1079.0

Instrument :
MSVOA_X
ClientSampleId :
BFB610

m/z	Abundance
36.00	198.0
37.10	1121.0
38.00	1158.0
39.00	502.0
40.10	107.0
44.00	194.0
44.90	161.0
47.00	269.0
47.90	177.0
49.00	947.0
50.00	4796.0
51.00	1311.0
56.00	339.0
57.00	565.0
60.00	247.0
61.10	1170.0
62.00	1145.0
63.00	1182.0
64.20	51.0
65.10	86.0
68.00	2383.0
69.00	2670.0
70.00	237.0
72.10	120.0
73.00	1253.0
74.00	4444.0
75.00	14183.0
76.00	1260.0
77.00	130.0
77.90	107.0
78.90	760.0
79.90	231.0
80.90	694.0
81.90	152.0
87.00	1365.0
87.90	1280.0
90.90	80.0
92.00	764.0
93.00	1132.0
94.00	3279.0
95.00	29072.0
96.00	1799.0
103.90	112.0
105.90	143.0
115.80	130.0
116.90	193.0
117.90	120.0
118.90	217.0
127.90	74.0
130.00	118.0
134.80	52.0
136.80	57.0
140.80	275.0
142.90	336.0
147.80	61.0
155.00	93.0
171.90	280.0
173.00	296.0
174.00	27504.0
175.00	1941.0
176.00	26848.0
177.00	1743.0
177.90	54.0

Instrument :
MSVOA_X
ClientSampleId :
BFB610

m/z	Abundance
35.90	151.0
37.00	749.0
38.00	698.0
39.00	267.0
39.90	89.0
44.00	147.0
45.10	126.0
47.10	178.0
47.90	124.0
49.00	780.0
50.00	3237.0
51.10	1014.0
56.20	225.0
57.00	460.0
60.10	161.0
61.00	934.0
62.00	884.0
63.10	790.0
64.20	88.0
65.10	91.0
68.00	1903.0
69.00	2125.0
69.90	145.0
71.80	128.0
73.00	879.0
74.00	3368.0
75.00	10222.0
76.10	1019.0
77.10	126.0
78.10	130.0
79.00	594.0
79.90	174.0
80.90	458.0
81.80	140.0
87.00	816.0
87.80	849.0
90.90	51.0
92.00	598.0
93.00	980.0
94.00	2544.0
95.00	22704.0
96.00	1516.0
103.80	103.0
105.80	104.0
115.90	70.0
116.90	142.0
118.00	93.0
119.00	102.0
128.00	57.0
129.70	92.0
130.10	71.0
140.90	242.0
142.90	321.0
155.10	81.0
171.90	146.0
172.10	167.0
173.10	359.0
174.00	24336.0
175.00	2016.0
176.00	23664.0
176.90	1446.0

Instrument :
MSVOA_X
ClientSampleId :
BFB610