

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020922\
 Data File : VX026900.D
 Acq On : 10 Feb 2022 04:29
 Operator : JC/MD
 Sample : N1447-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-138A

Quant Time: Feb 10 07:29:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 08 07:07:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	134253	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	224843	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	202691	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	84666	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	86633	53.757	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 107.520%	
35) Dibromofluoromethane	5.391	113	70048	52.292	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 104.580%	
50) Toluene-d8	8.653	98	260851	53.049	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 106.100%	
62) 4-Bromofluorobenzene	11.079	95	95010	54.882	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 109.760%	
Target Compounds						
					Qvalue	
16) Acetone	2.386	43	1955	2.762	ug/l	100
19) Methyl tert-butyl Ether	3.117	73	519921	106.908	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020922\
Data File : VX026900.D
Acq On : 10 Feb 2022 04:29
Operator : JC/MD
Sample : N1447-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-138A

Quant Time: Feb 10 07:29:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 08 07:07:46 2022
Response via : Initial Calibration




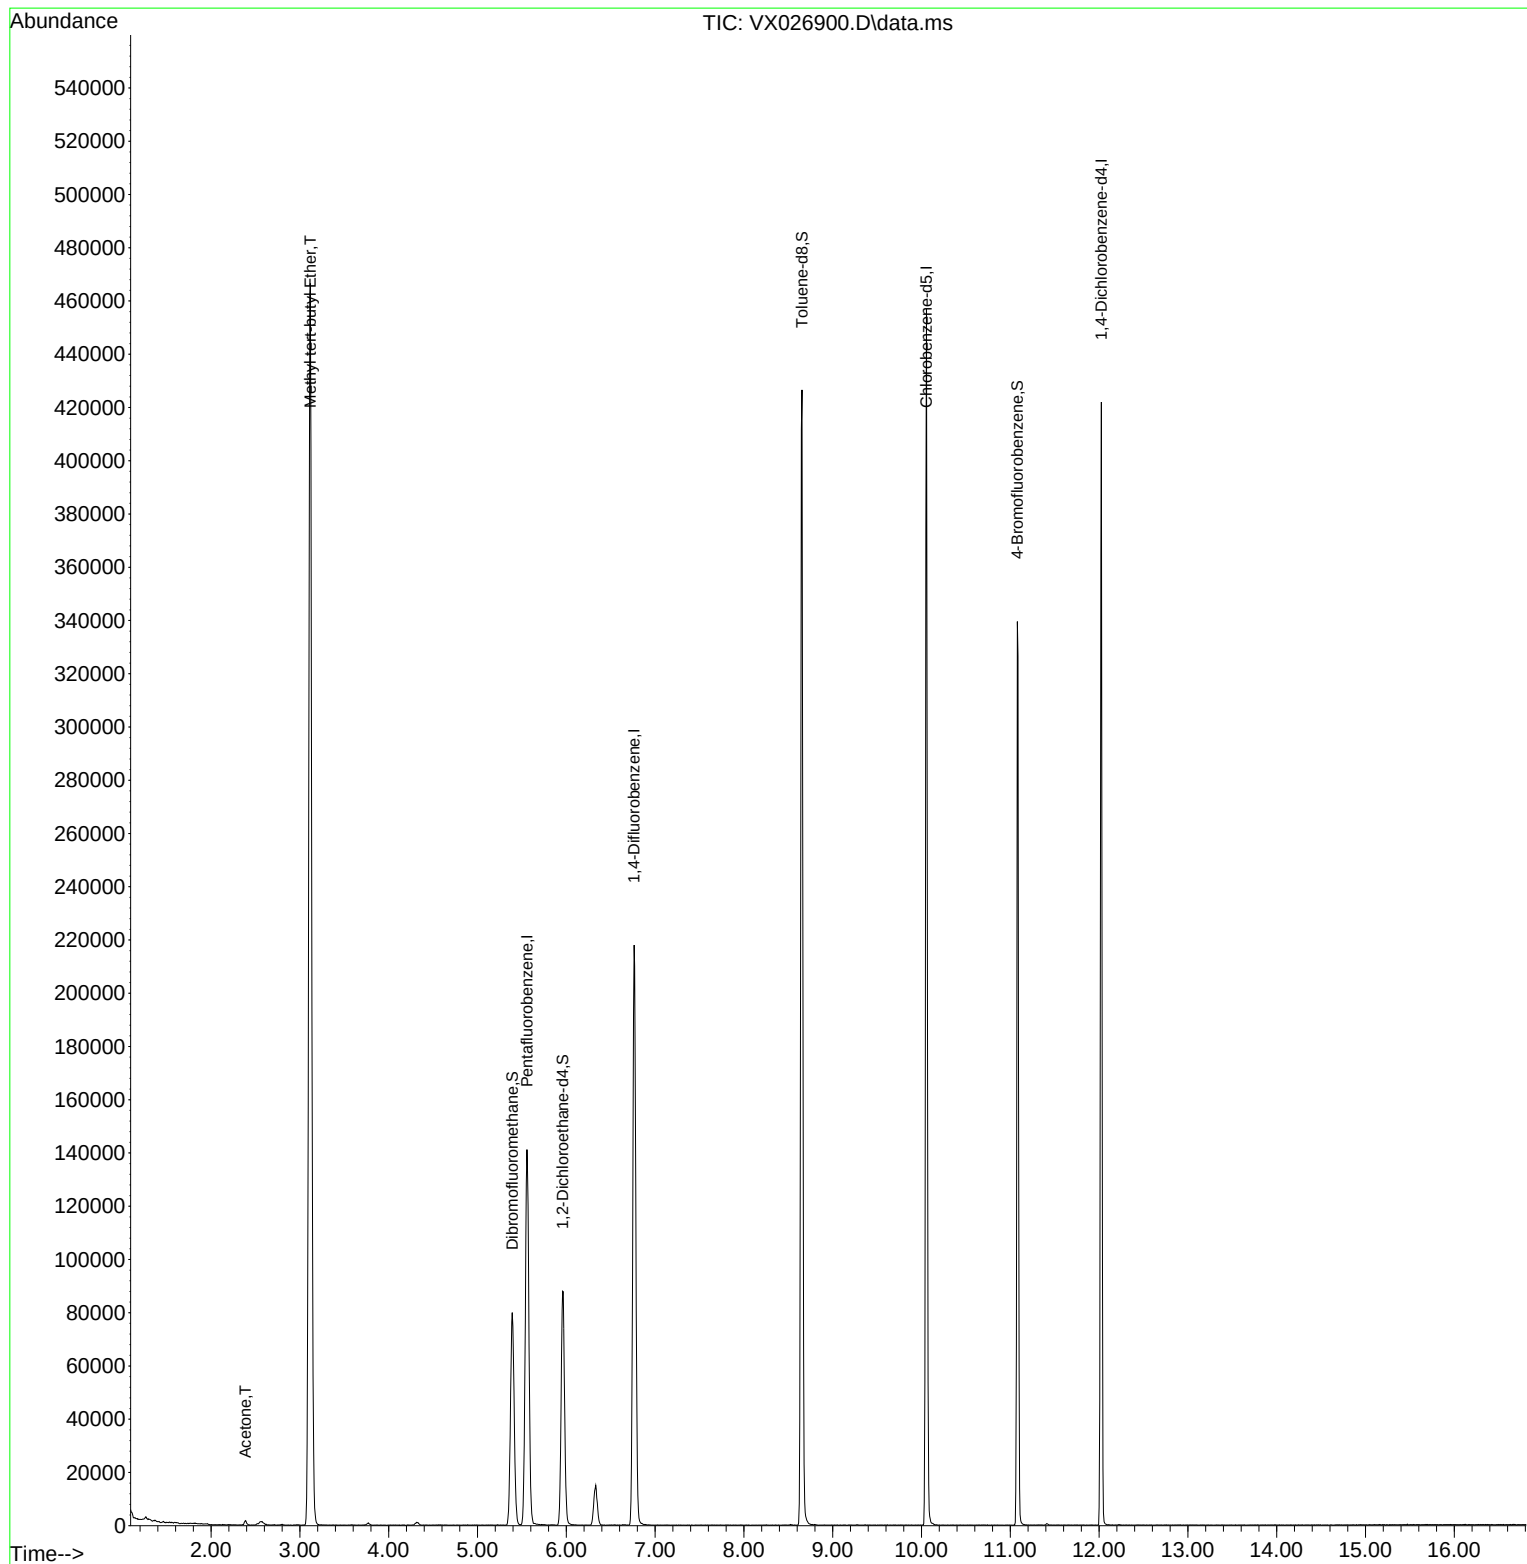


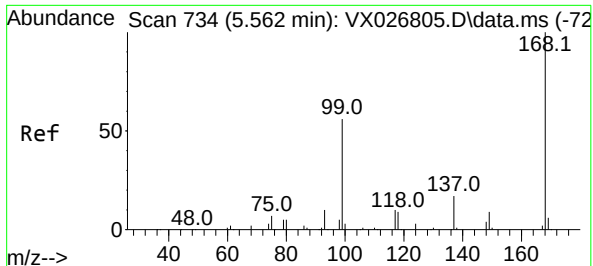

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX026900.D
Acq: 10 Feb 2022 04:29




Instrument :
MSVOA_X
ClientSampleId :
MW-138A


Tgt Ion:168 Resp: 134253
Ion Ratio Lower Upper
168 100
99 60.1 50.3 75.5

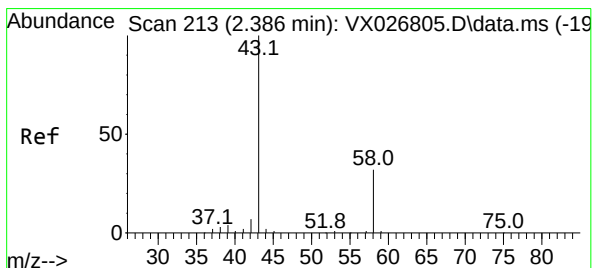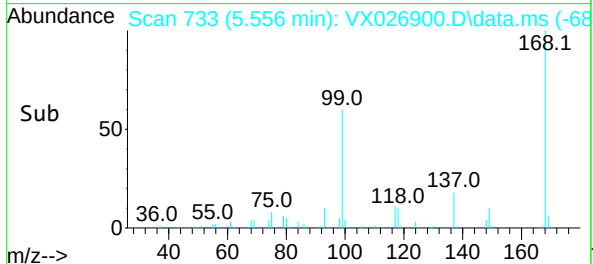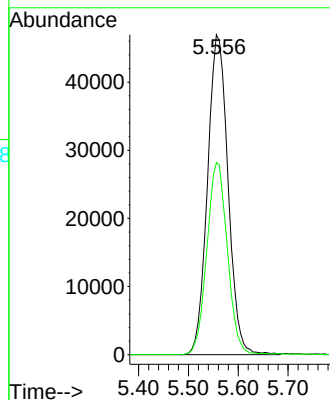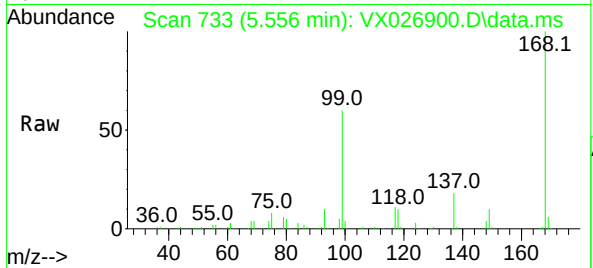

#16
Acetone
Concen: 2.762 ug/l
RT: 2.386 min Scan# 213
Delta R.T. 0.000 min
Lab File: VX026900.D
Acq: 10 Feb 2022 04:29

Tgt Ion: 43 Resp: 1955
Ion Ratio Lower Upper
43 100
58 28.8 23.0 34.6


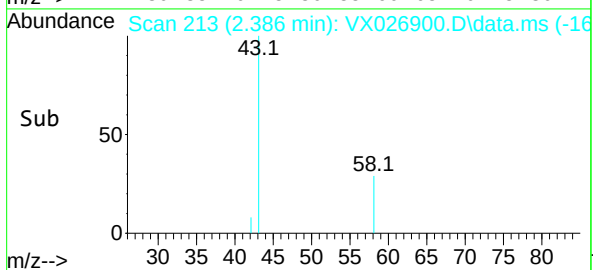
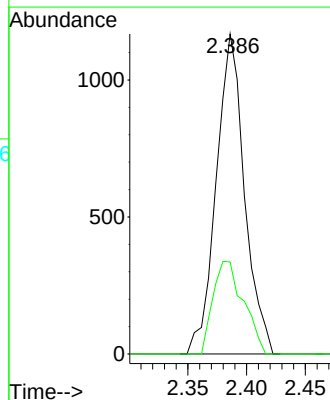
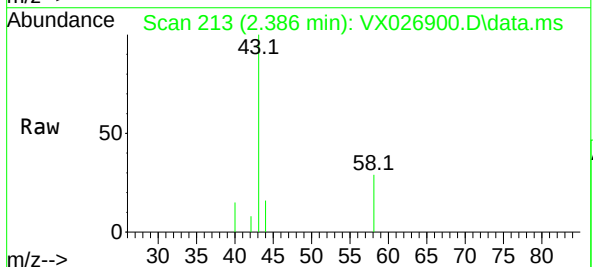


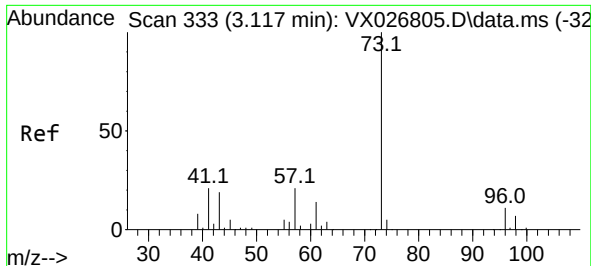

#19
Methyl tert-butyl Ether
Concen: 106.908 ug/l
RT: 3.117 min Scan# 31
Delta R.T. 0.000 min
Lab File: VX026900.D
Acq: 10 Feb 2022 04:29




Instrument :
MSVOA_X
ClientSampleId :
MW-138A


Tgt Ion: 73 Resp: 519921
Ion Ratio Lower Upper
73 100
57 22.6 17.4 26.2

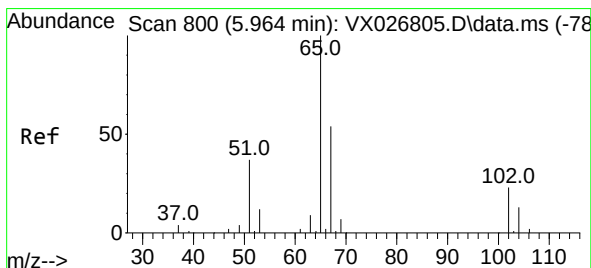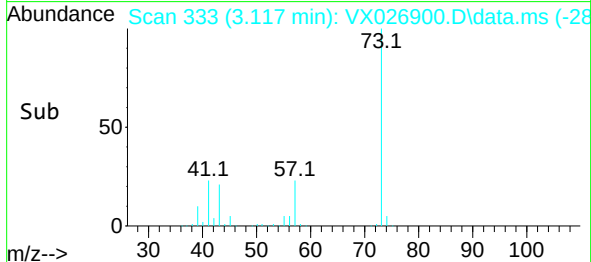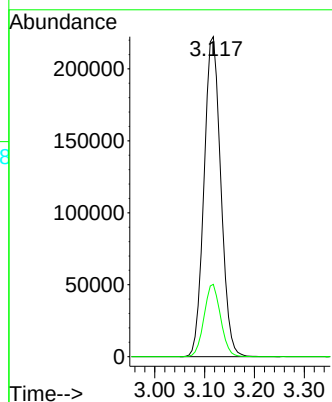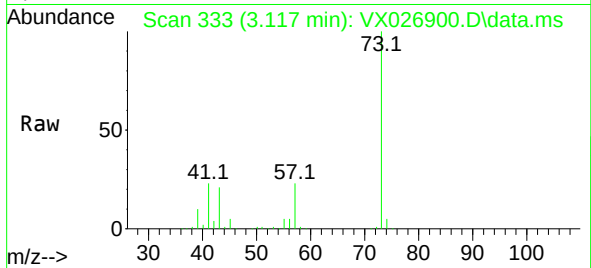

#33
1,2-Dichloroethane-d4
Concen: 53.757 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.006 min
Lab File: VX026900.D
Acq: 10 Feb 2022 04:29

Tgt Ion: 65 Resp: 86633
Ion Ratio Lower Upper
65 100
67 51.2 0.0 100.8


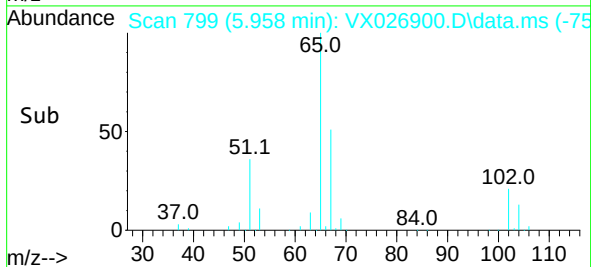
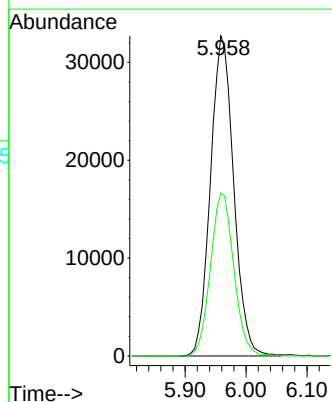
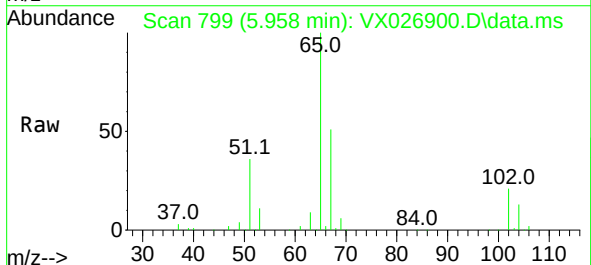


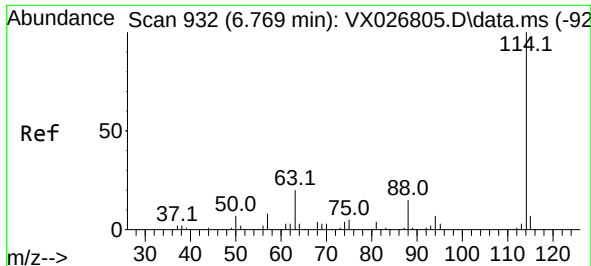

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX026900.D
Acq: 10 Feb 2022 04:29




Instrument :
MSVOA_X
ClientSampleId :
MW-138A


Tgt Ion:114 Resp: 224843
Ion Ratio Lower Upper
114 100
63 20.2 0.0 42.8
88 16.2 0.0 33.0

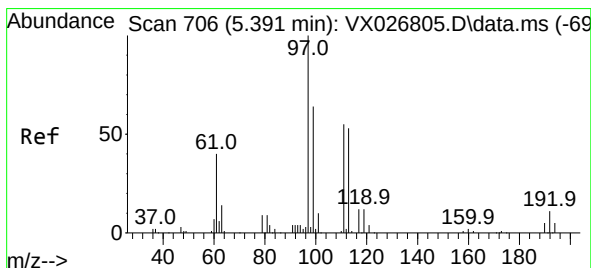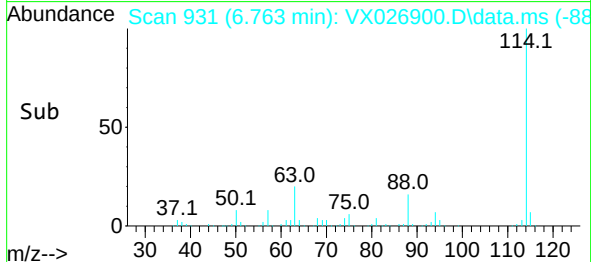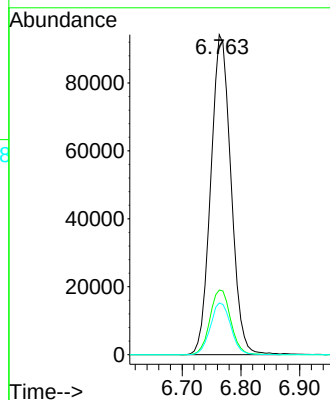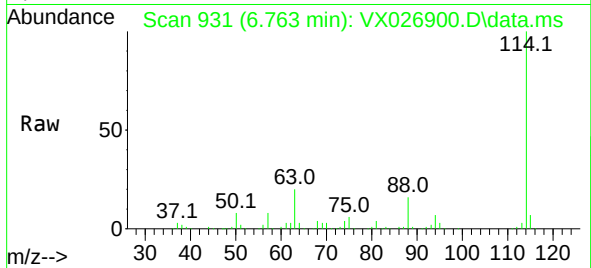

#35
Dibromofluoromethane
Concen: 52.292 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX026900.D
Acq: 10 Feb 2022 04:29

Tgt Ion:113 Resp: 70048
Ion Ratio Lower Upper
113 100
111 102.2 81.2 121.8
192 19.5 15.0 22.4


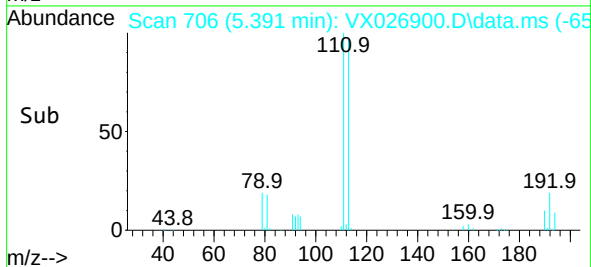
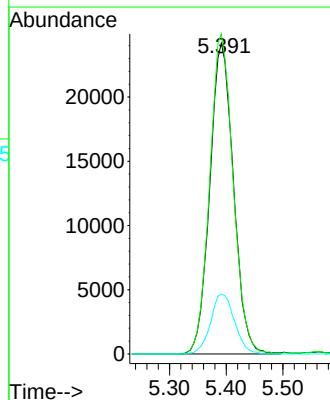
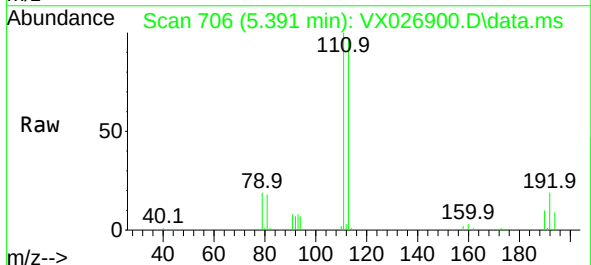


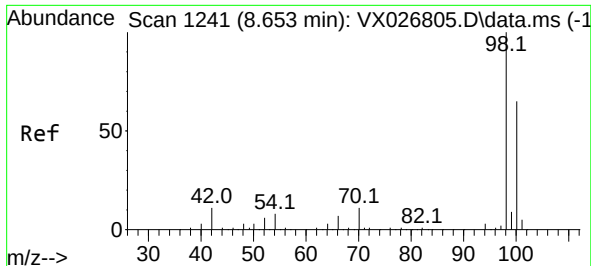

#50
Toluene-d8
Concen: 53.049 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX026900.D
Acq: 10 Feb 2022 04:29




Instrument :
MSVOA_X
ClientSampleId :
MW-138A


Tgt Ion: 98 Resp: 260851
Ion Ratio Lower Upper
98 100
100 66.9 53.2 79.8

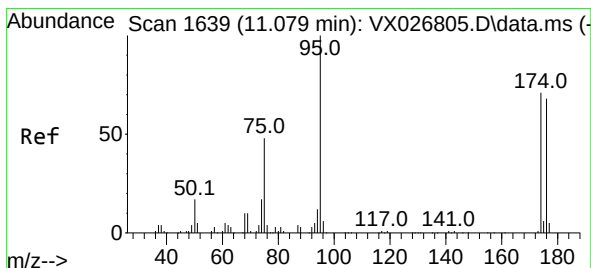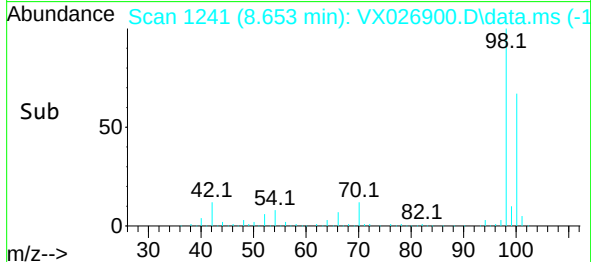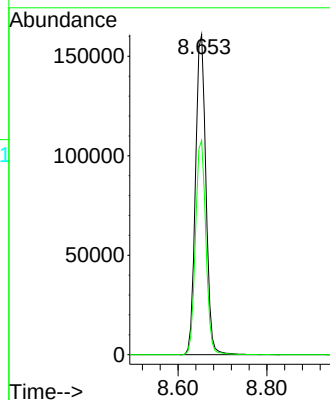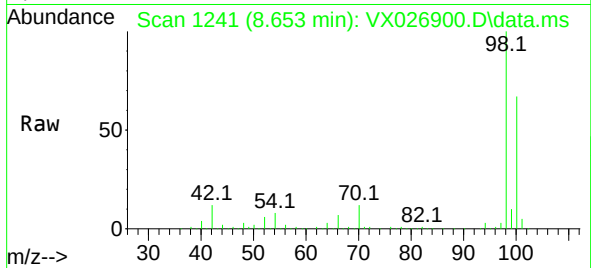

#62
4-Bromofluorobenzene
Concen: 54.882 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX026900.D
Acq: 10 Feb 2022 04:29

Tgt Ion: 95 Resp: 95010
Ion Ratio Lower Upper
95 100
174 75.0 0.0 148.6
176 72.5 0.0 141.4


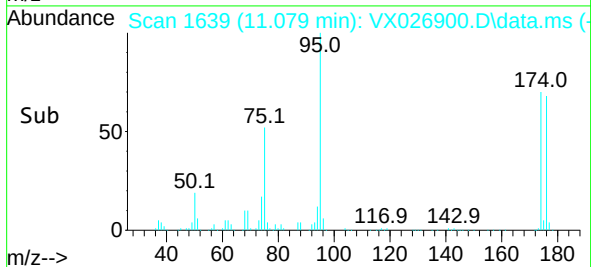
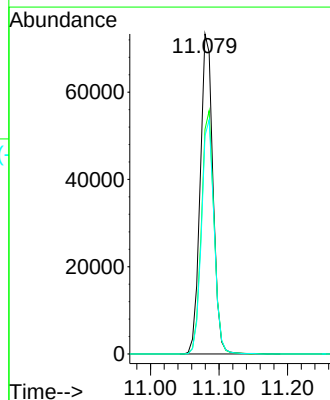
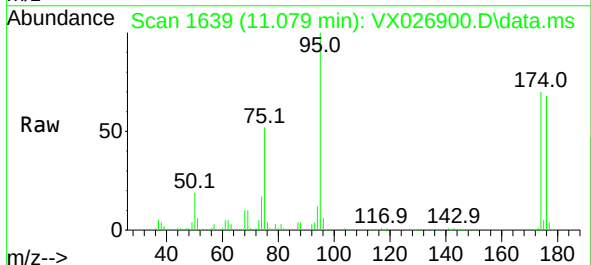


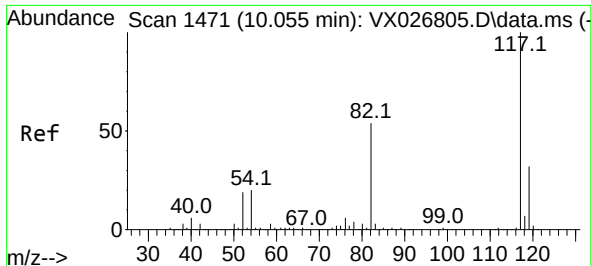

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX026900.D
Acq: 10 Feb 2022 04:29

Instrument :
MSVOA_X
ClientSampleId :
MW-138A

Tgt Ion:117 Resp: 202691
Ion Ratio Lower Upper
117 100
82 56.5 45.2 67.8
119 32.4 26.2 39.2

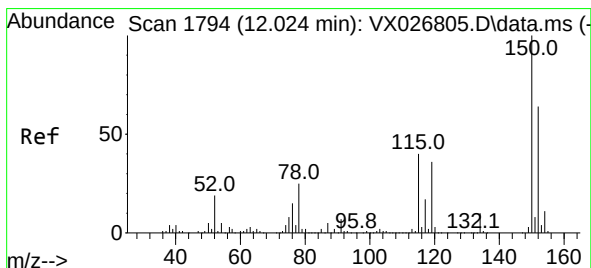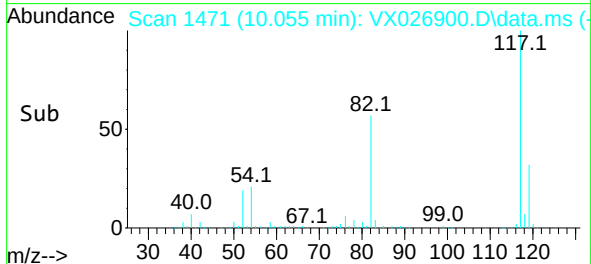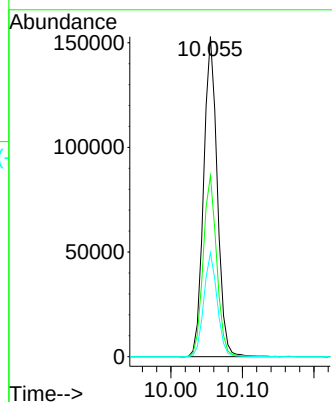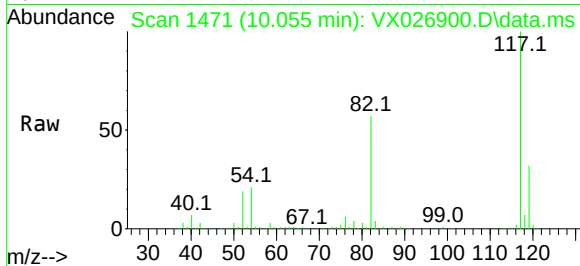

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX026900.D
Acq: 10 Feb 2022 04:29

Tgt Ion:152 Resp: 84666
Ion Ratio Lower Upper
152 100
115 61.0 44.2 132.6
150 158.0 0.0 348.2

