

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020922\
 Data File : VX026902.D
 Acq On : 10 Feb 2022 05:15
 Operator : JC/MD
 Sample : N1447-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-139A

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M

Title : SW846 8260

Signal : TIC: VX026902.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.562	231	242	257	rBV	3233	11066	1.63%	0.306%
2	3.117	325	333	342	rVB2	5157	11785	1.74%	0.325%
3	5.391	695	706	721	rBV2	78554	225013	33.22%	6.213%
4	5.556	721	733	750	rVV	135665	381530	56.33%	10.534%
5	5.958	787	799	808	rBV	85843	229449	33.88%	6.335%
6	6.044	810	813	821	rVB3	4130	9180	1.36%	0.253%
7	6.763	920	931	949	rBV	213115	505277	74.60%	13.951%
8	8.653	1234	1241	1258	rBV	421944	677291	100.00%	18.700%
9	10.055	1465	1471	1486	rBV	444957	594591	87.79%	16.417%
10	11.079	1634	1639	1654	rBV	342826	447744	66.11%	12.362%
11	12.024	1788	1794	1804	rBV	436518	528902	78.09%	14.603%




Sum of corrected areas: 3621828

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020922\
Data File : VX026902.D
Acq On : 10 Feb 2022 05:15
Operator : JC/MD
Sample : N1447-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-139A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

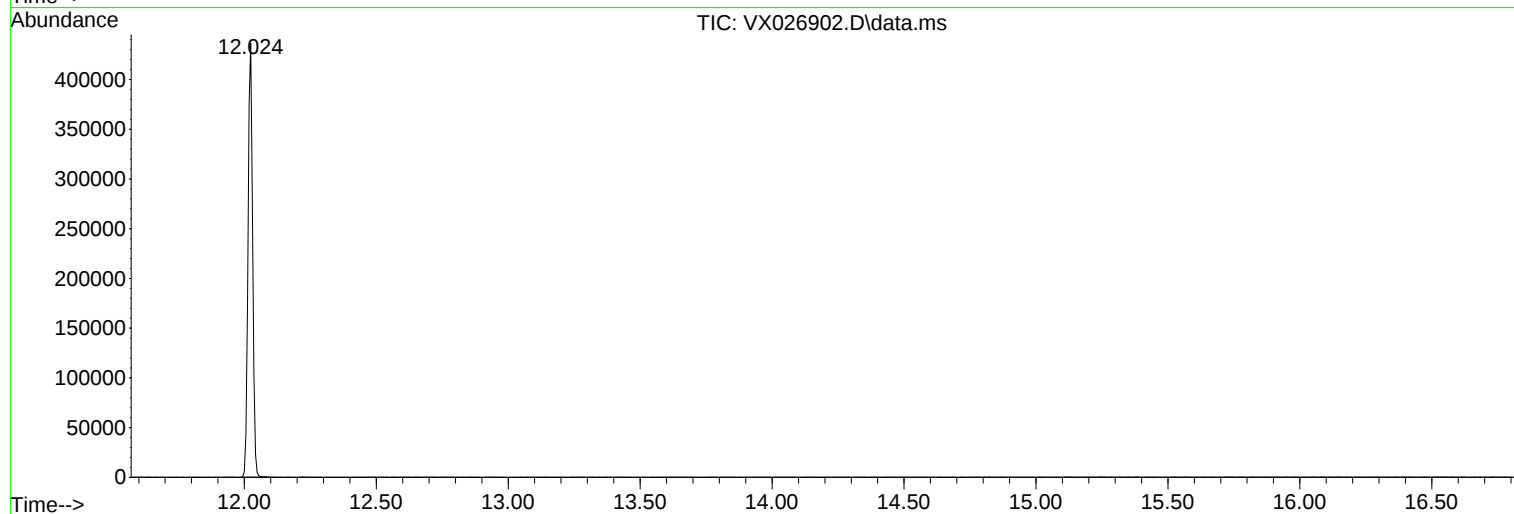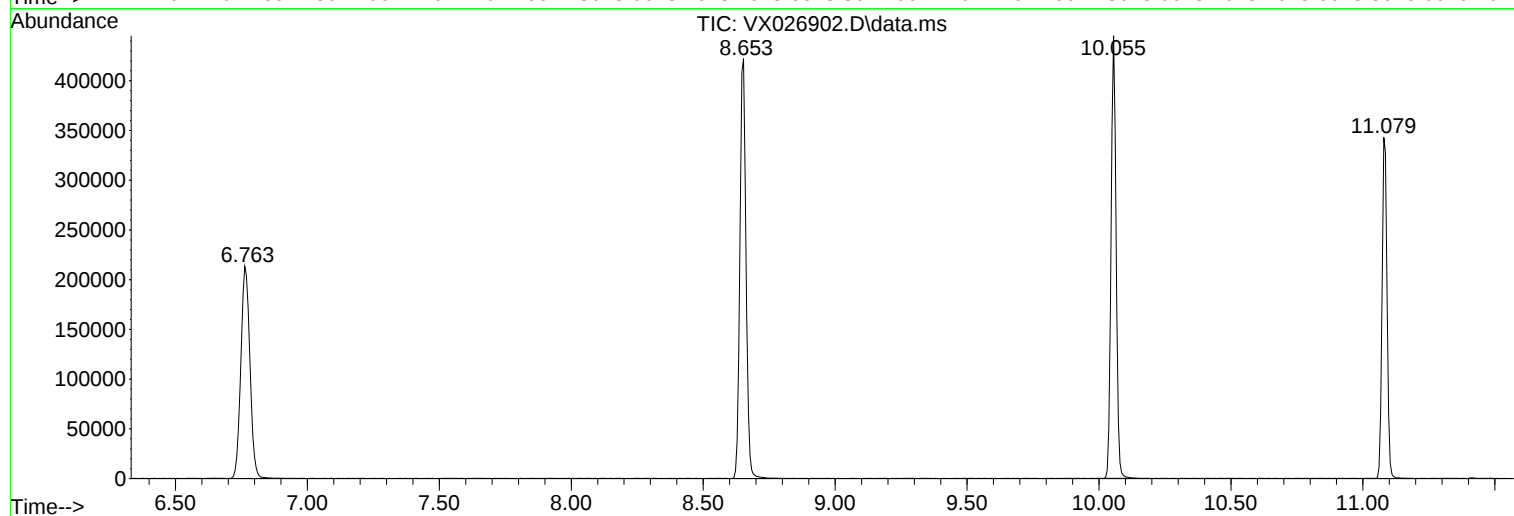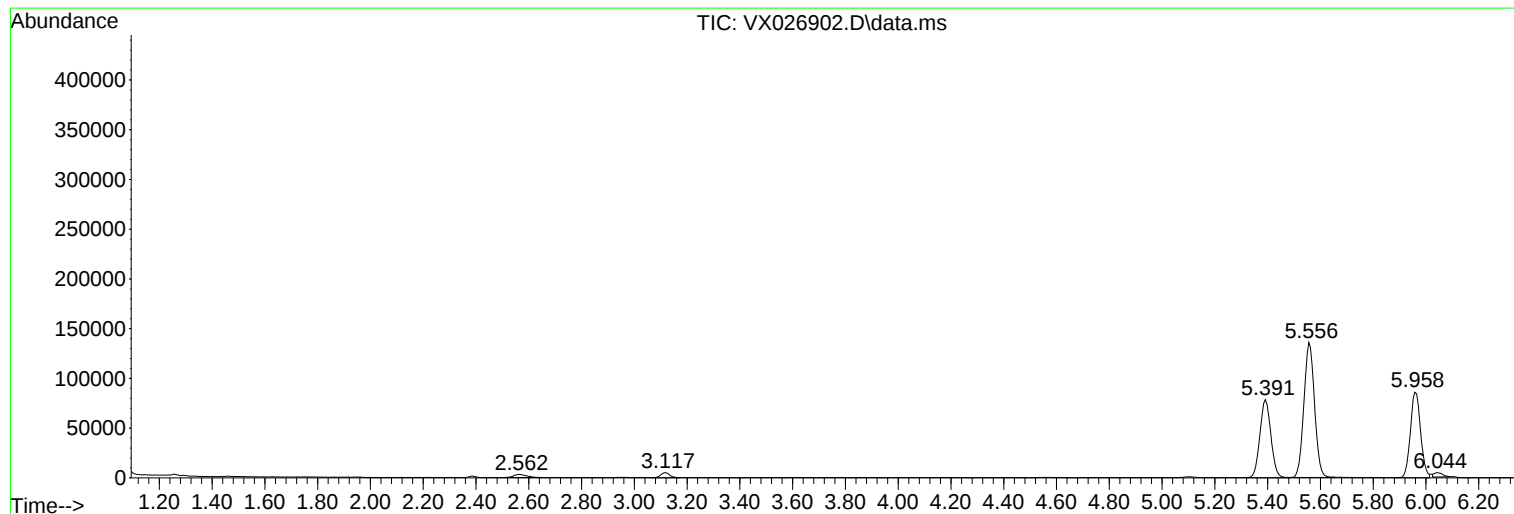

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020922\
Data File : VX026902.D
Acq On : 10 Feb 2022 05:15
Operator : JC/MD
Sample : N1447-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-139A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020922\
Data File : VX026902.D
Acq On : 10 Feb 2022 05:15
Operator : JC/MD
Sample : N1447-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-139A

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
