

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020923\
 Data File : VX034069.D
 Acq On : 07 Feb 2023 18:24
 Operator : JC/MD
 Sample : 01467-01 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 33906

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
 Title : SW846 8260

Signal : TIC: VX034069.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	692	705	721	rBV	64843	190127	35.51%	6.190%
2	5.550	721	732	747	rVV	119003	337618	63.05%	10.992%
3	5.952	787	798	811	rBV	63757	172301	32.18%	5.610%
4	6.763	920	931	945	rBV	165741	395774	73.91%	12.885%
5	8.647	1234	1240	1248	rBV	339853	535459	100.00%	17.433%
6	8.720	1248	1252	1262	rVB	13094	21618	4.04%	0.704%
7	10.055	1465	1471	1485	rBV	339536	457369	85.42%	14.891%
8	10.305	1506	1512	1518	rBV	13249	19519	3.65%	0.635%
9	10.640	1562	1567	1574	rBV	9423	13024	2.43%	0.424%
10	11.079	1634	1639	1652	rBV	293468	374750	69.99%	12.201%
11	11.378	1684	1688	1696	rBV	7483	14136	2.64%	0.460%
12	11.616	1722	1727	1734	rBV	4143	5479	1.02%	0.178%
13	11.756	1745	1750	1757	rVB	12662	16632	3.11%	0.541%
14	12.024	1788	1794	1801	rBV	349213	446879	83.46%	14.549%
15	12.085	1801	1804	1812	rVB	6367	8556	1.60%	0.279%
16	12.244	1826	1830	1833	rBV2	5478	7387	1.38%	0.241%
17	12.317	1838	1842	1851	rVB5	4116	6347	1.19%	0.207%
18	13.170	1973	1982	1986	rBV3	3817	5539	1.03%	0.180%
19	13.292	1999	2002	2007	rVB2	9851	11960	2.23%	0.389%
20	13.420	2019	2023	2030	rVB2	7460	9233	1.72%	0.301%
21	14.231	2147	2156	2162	rBV	8790	14792	2.76%	0.482%
22	14.481	2193	2197	2204	rBV2	5424	6975	1.30%	0.227%




Sum of corrected areas: 3071474

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020923\
Data File : VX034069.D
Acq On : 07 Feb 2023 18:24
Operator : JC/MD
Sample : 01467-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
33906

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

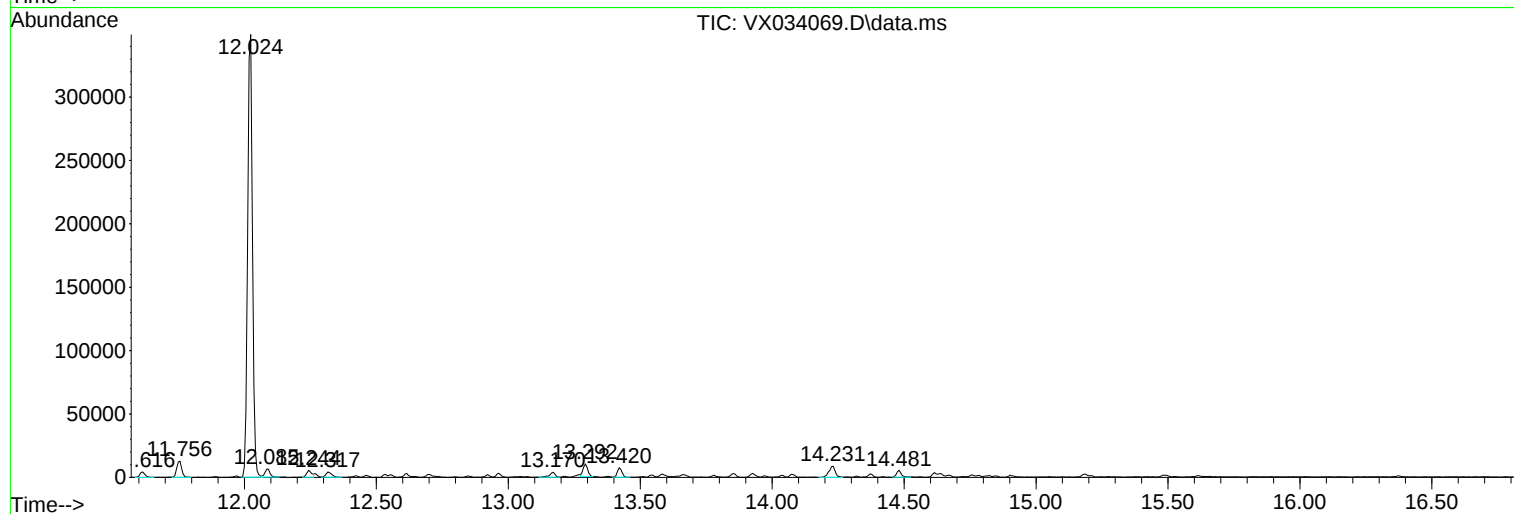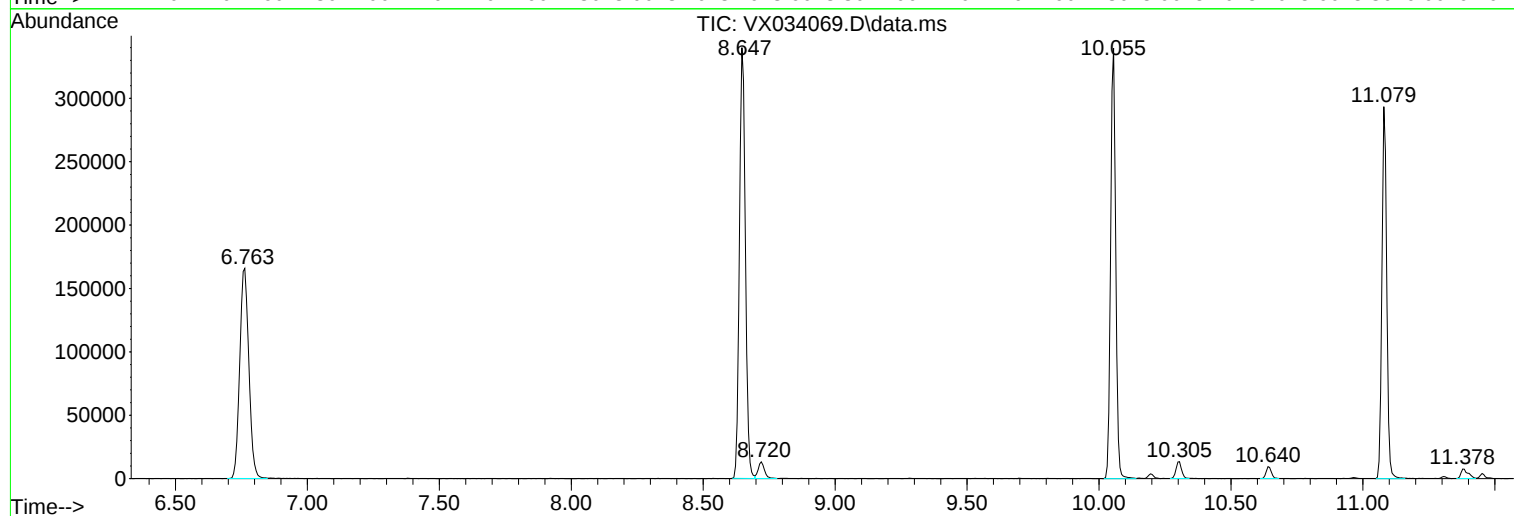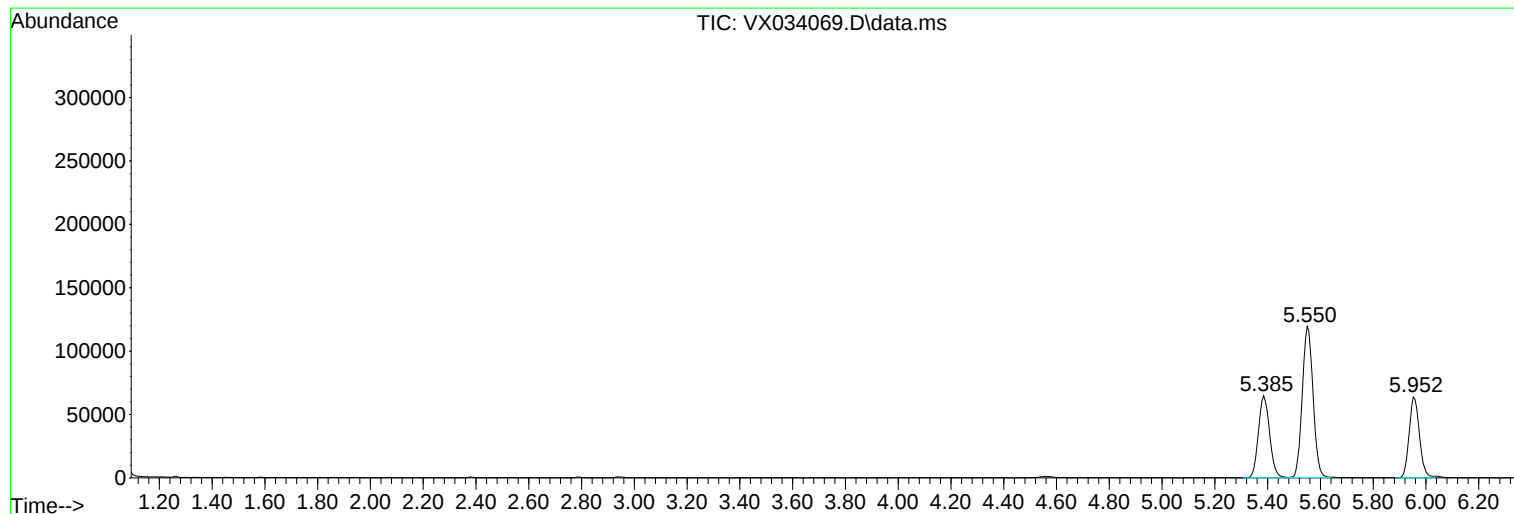

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020923\
Data File : VX034069.D
Acq On : 07 Feb 2023 18:24
Operator : JC/MD
Sample : 01467-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
33906

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX020923\
Data File : VX034069.D
Acq On : 07 Feb 2023 18:24
Operator : JC/MD
Sample : 01467-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
33906

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------