

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX021020\
 Data File : VX014884.D
 Acq On : 10 Feb 2020 13:24
 Operator : JC/SP
 Sample : VX0210MBL01
 Misc : 5.00µL/100µL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0210MBL01

Quant Time: Feb 11 06:43:01 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X021020W.M
 Quant Title : SW846 8260
 QLast Update : Mon Feb 10 12:09:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	454850	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	700818	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	656561	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	331394	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.06	65	258828	50.42	ug/l	0.00
Spiked Amount						
35) Dibromofluoromethane	5.49	113	216142	50.17	ug/l	0.00
Spiked Amount						
50) Toluene-d8	8.71	98	838549	50.99	ug/l	0.00
Spiked Amount						
62) 4-Bromofluorobenzene	11.13	95	308252	52.03	ug/l	0.00
Spiked Amount						


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
4) Vinyl Chloride	1.43	62	1135	0.216	ug/l #	42
5) Bromomethane	1.66	94	2384	0.700	ug/l	93
9) 1,1,2-Trichlorotrifluoroet	2.39	101	979	0.229	ug/l #	44
10) Methyl Iodide	2.51	142	1228	4.604	ug/l #	77
11) Tert butyl alcohol	3.04	59	1098	1.211	ug/l #	72
13) Acrolein	2.30	56	728	1.054	ug/l #	64
15) Acrylonitrile	3.14	53	827	0.360	ug/l #	55
16) Acetone	2.43	43	6665	Below Cal		91
17) Carbon Disulfide	2.57	76	5738	0.493	ug/l #	93
20) Methylene Chloride	2.85	84	1388	0.281	ug/l #	66
21) trans-1,2-Dichloroethene	3.16	96	1066	0.232	ug/l #	59
25) 2-Butanone	4.67	43	1662	0.476	ug/l #	49
29) Tetrahydrofuran	4.98	42	429	0.216	ug/l	92
36) 1,1-Dichloropropene	5.65	75	31186	4.975	ug/l #	51
38) Carbon Tetrachloride	5.65	117	40679	6.658	ug/l #	15
44) Trichloroethene	7.22	130	1228	0.226	ug/l	80
49) 1,4-Dioxane	7.73	88	504	5.078	ug/l #	42
51) 4-Methyl-2-Pentanone	8.64	43	1361	0.209	ug/l #	35
58) 2-Chloroethyl Vinyl ether	8.47	63	833	0.220	ug/l	96
64) Tetrachloroethene	9.32	164	1406	0.229	ug/l #	44
68) m/p-Xylenes	10.35	106	1749	0.200	ug/l #	69
76) 1,2,3-Trichloropropane	11.13	75	152484	25.445	ug/l #	41
77) Bromobenzene	11.26	156	1229	0.212	ug/l	61
81) trans-1,4-Dichloro-2-buten	11.13	75	152484	65.132	ug/l #	12
93) 1,2,4-Trichlorobenzene	13.64	180	2195	0.291	ug/l #	90
94) Hexachlorobutadiene	13.78	225	1017	0.279	ug/l	88
96) 1,2,3-Trichlorobenzene	14.02	180	1642	0.226	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX021020\
Data File : VX014884.D
Acq On : 10 Feb 2020 13:24
Operator : JC/SP
Sample : VX0210MBL01
Misc : 5.0µL/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0210MBL01

Quant Time: Feb 11 06:43:01 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X021020W.M
Quant Title : SW846 8260
QLast Update : Mon Feb 10 12:09:20 2020
Response via : Initial Calibration

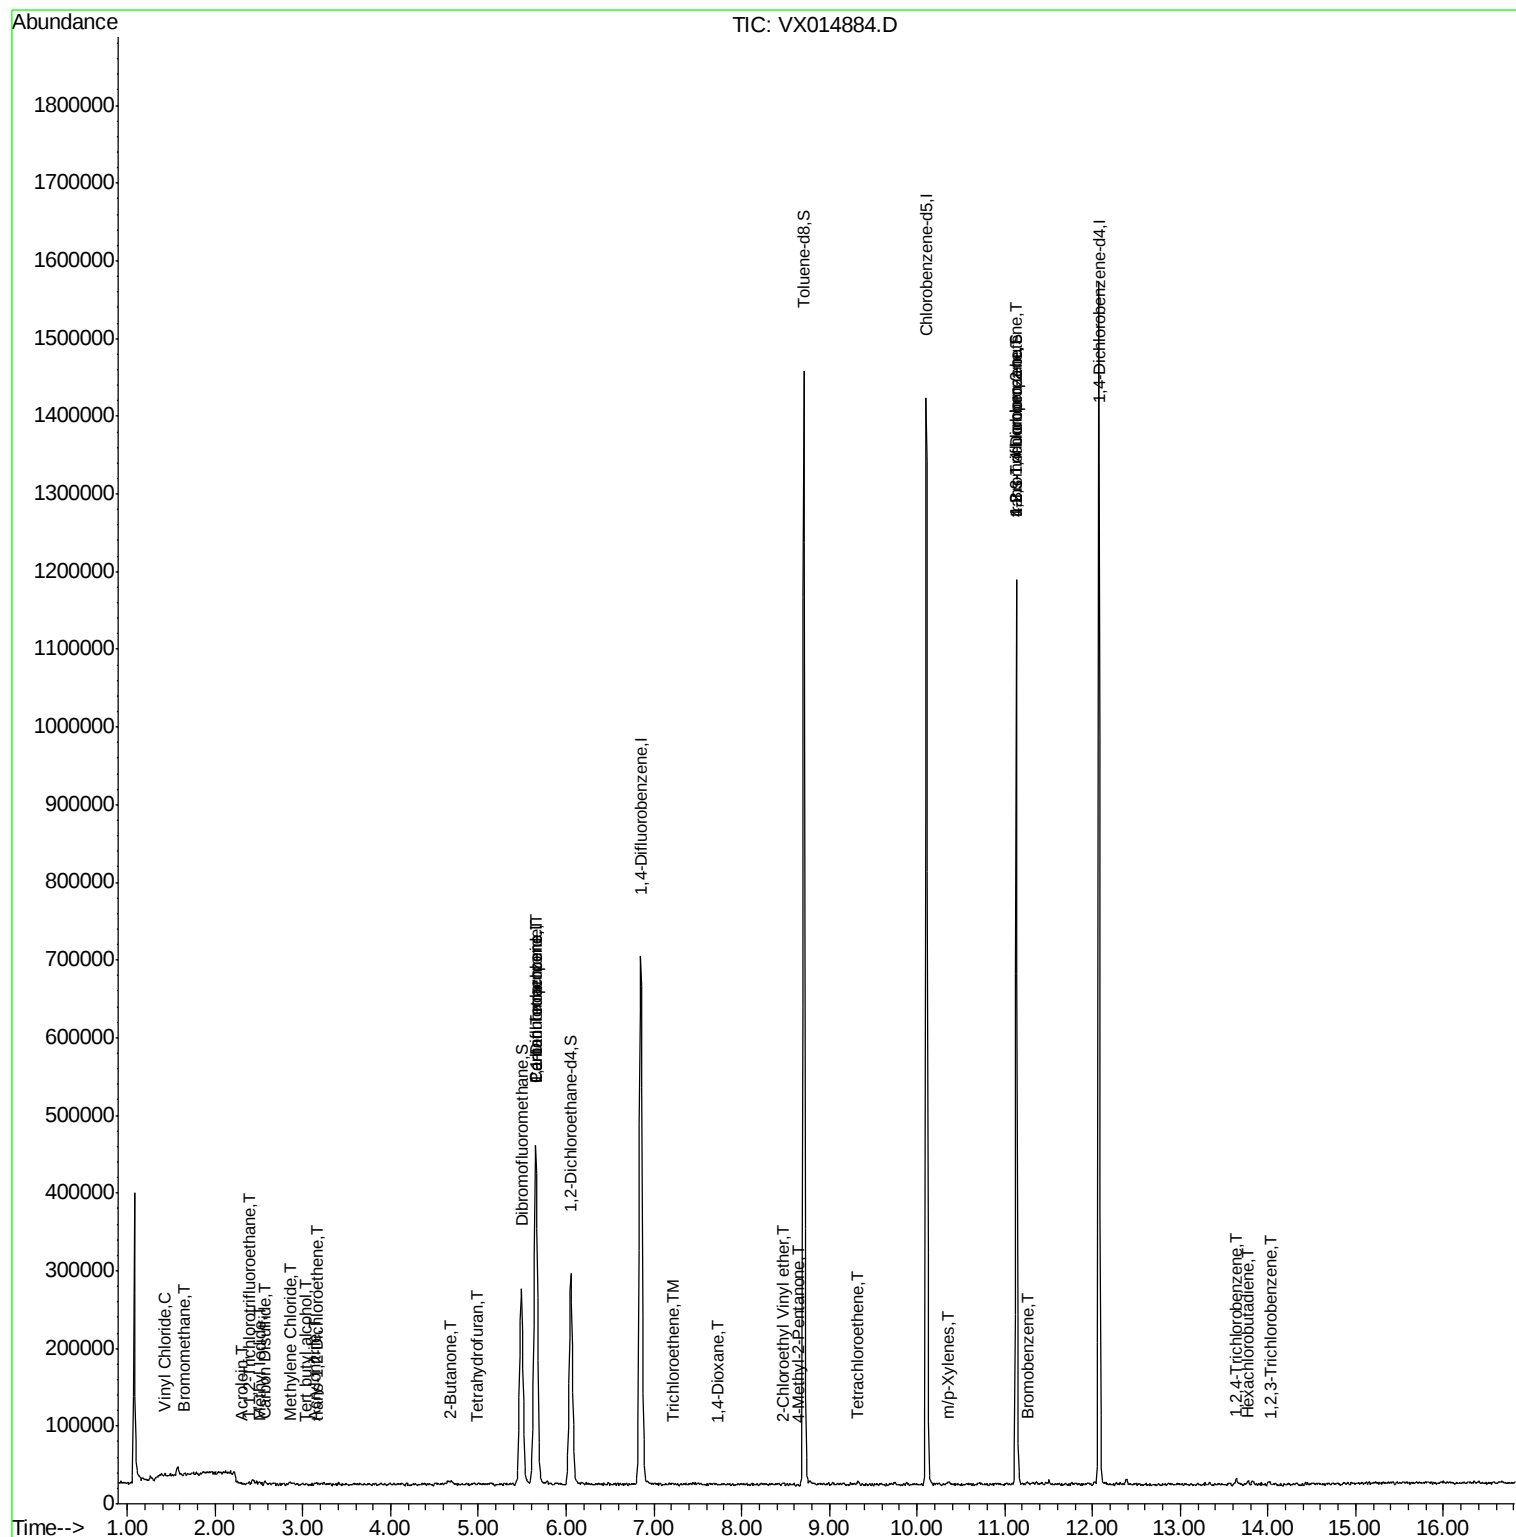

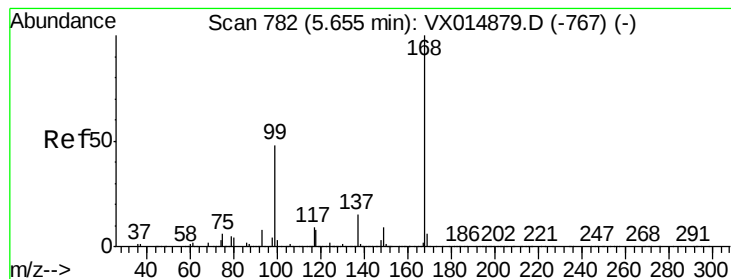

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 782

Delta R.T. -0.00 min

Lab File: VX014884.D

Acq: 10 Feb 2020 13:24

Instrument :

MSVOA_X

ClientSampleId :


VX0210MBL01

Tot Ion:168 Resp: 454850

Ion Ratio Lower Upper

168 100

99 49.1 38.7 58.1



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.65



150000

100000

50000

0

Time-->



#4

Vinyl Chloride

Concen: 0.216 ug/l

RT: 1.43 min Scan# 89

Delta R.T. 0.02 min

Lab File: VX014884.D


Acq: 10 Feb 2020 13:24

Tgt Ion: 62 Resp: 1135

Ion Ratio Lower Upper

62 100

64 62.7 24.8 37.2#



Abundance Ion 61.90 (61.60 to 62.60): VX0

Ion 63.90 (63.60 to 64.60): VX0

800


600


400

200

0

Time-->



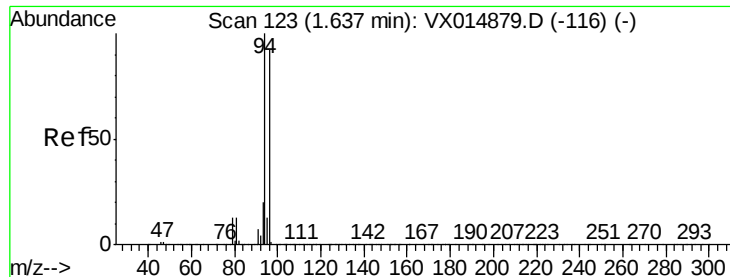

#5

Bromomethane

Concen: 0.700 ug/l

RT: 1.66 min Scan# 126

Delta R.T. 0.02 min

Lab File: VX014884.D

Acq: 10 Feb 2020 13:24

Instrument :

MSVOA_X

ClientSampleId :


VX0210MBL01

Tot Ion: 94 Resp: 2384

Ion Ratio Lower Upper




94 100

96 99.2 73.7 110.5

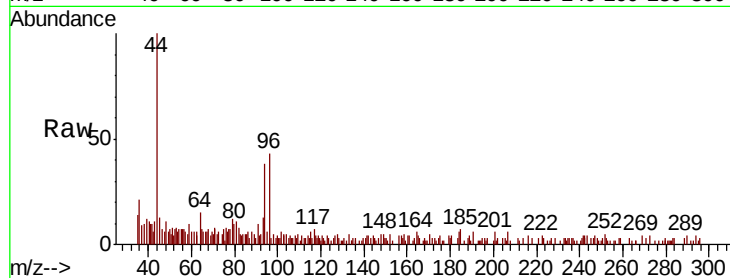

Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

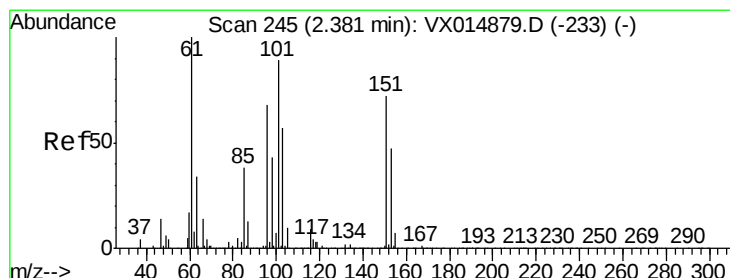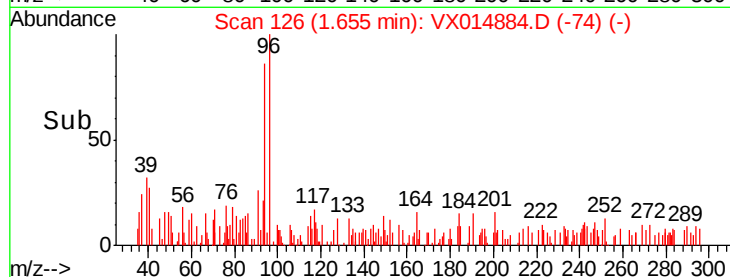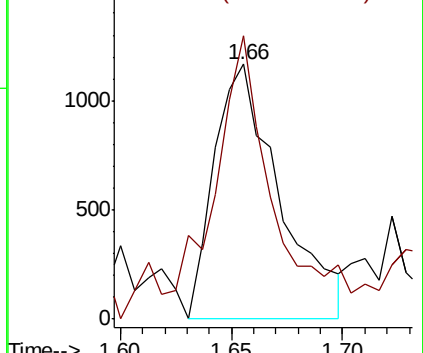

#9

1,1,2-Trichlorotrifluoroethane

Concen: 0.229 ug/l

RT: 2.39 min Scan# 246

Delta R.T. 0.01 min

Lab File: VX014884.D

Acq: 10 Feb 2020 13:24


Tgt Ion: 101 Resp: 979

Ion Ratio Lower Upper

101 100

85 19.9 34.1 51.1#



151 143.8 67.3 100.9#

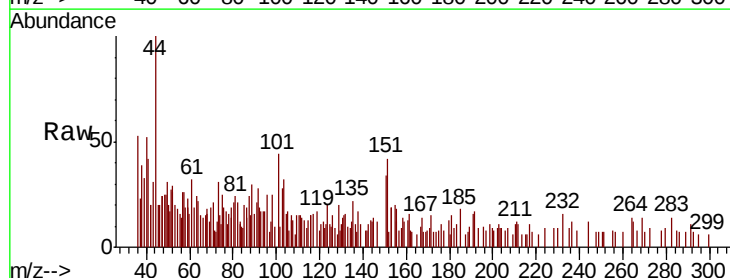


Abundance Ion 100.90 (100.60 to 101.60): V

Ion 84.90 (84.60 to 85.60): VX0

Ion 150.80 (150.50 to 151.50): V

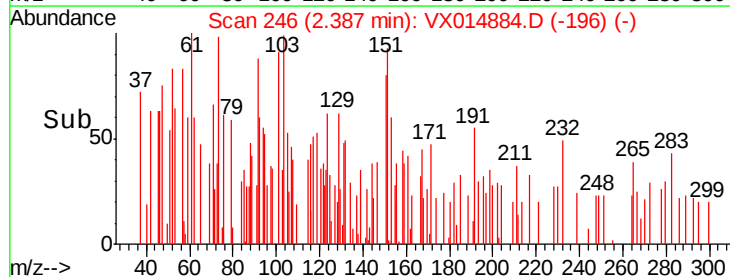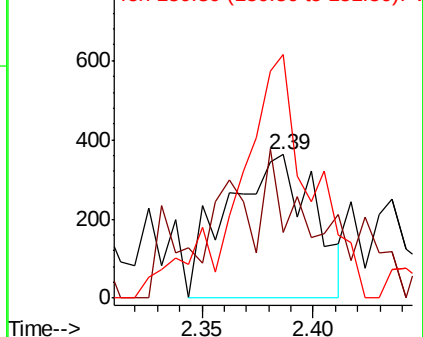

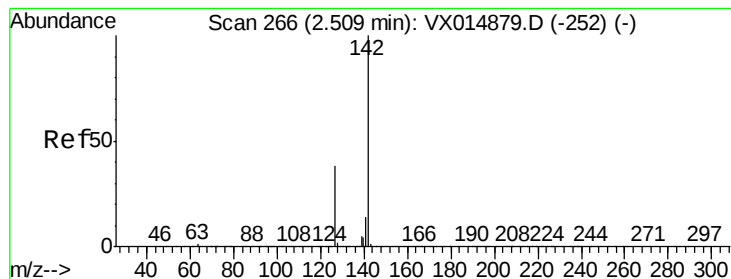

#10

Methvl Iodide

Concen: 4.604 ug/l

RT: 2.51 min Scan# 266

Delta R.T. 0.00 min

Lab File: VX014884.D

Acq: 10 Feb 2020 13:24

Instrument :

MSVOA_X

ClientSampleId :

VX0210MBL01





Tot Ion:142 Resp: 1228

Ion Ratio Lower Upper

142 100

127 57.0 31.1 46.7#

141 12.9 11.3 16.9

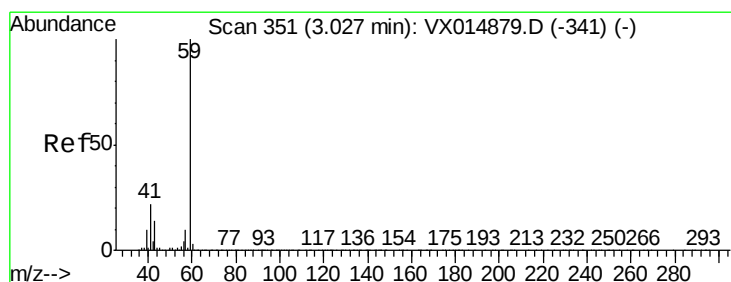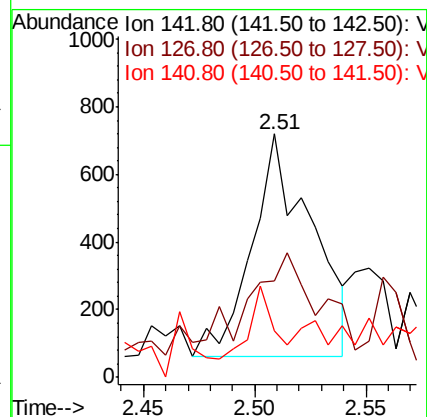

#11

Tert butyl alcohol

Concen: 1.211 ug/l

RT: 3.04 min Scan# 353

Delta R.T. 0.01 min

Lab File: VX014884.D




Acq: 10 Feb 2020 13:24


Tgt Ion: 59 Resp: 1098

Ion Ratio Lower Upper

59 100

57 0.0 8.2 12.4#

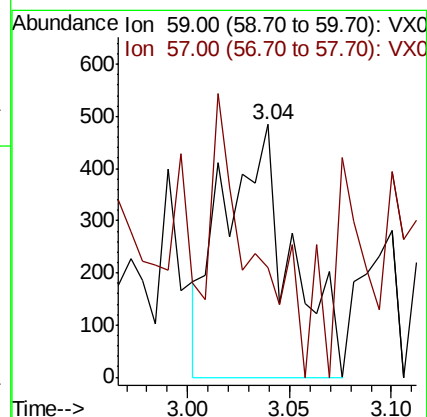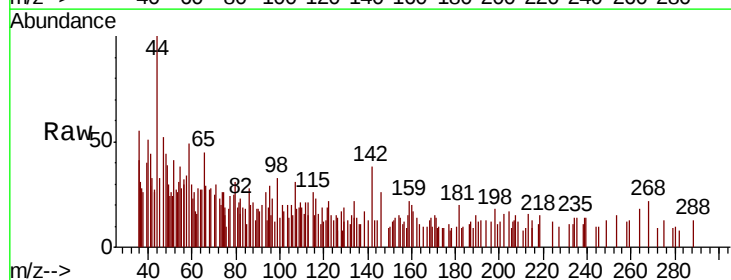

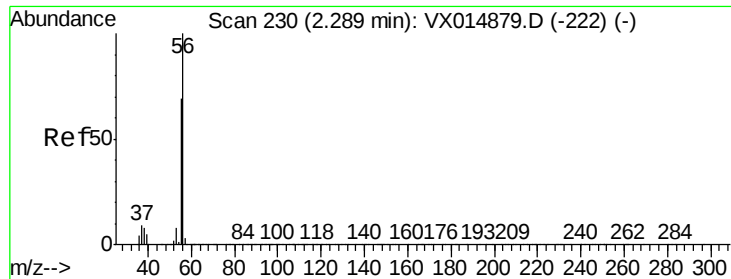

#13

Acrolein

Concen: 1.054 ug/l

RT: 2.30 min Scan# 231

Delta R.T. 0.01 min

Lab File: VX014884.D

Acq: 10 Feb 2020 13:24

Instrument :

MSVOA_X

ClientSampled :





VX0210MBL01

Tot Ion: 56 Resp: 728

Ion Ratio Lower Upper

56 100

55 39.8 55.0 82.4#

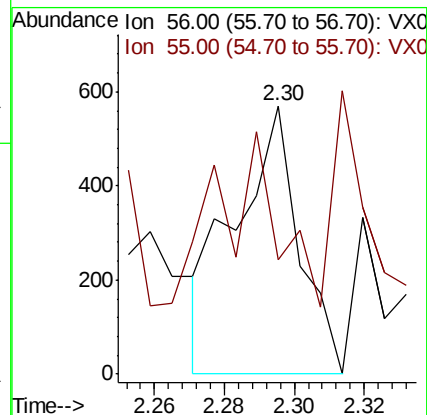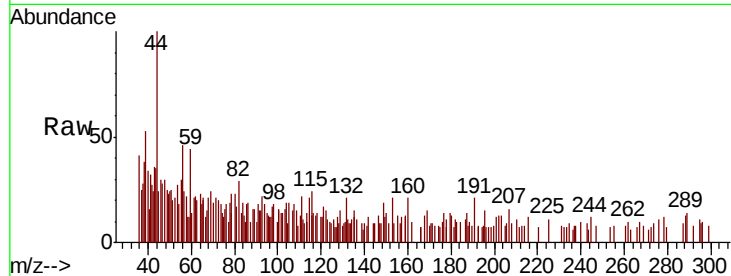

#15

Acrylonitrile

Concen: 0.360 ug/l

RT: 3.14 min Scan# 369

Delta R.T. 0.01 min

Lab File: VX014884.D

Acq: 10 Feb 2020 13:24




Tgt Ion: 53 Resp: 827


Ion Ratio Lower Upper

53 100

52 38.8 65.8 98.6#

51 59.0 29.1 43.7#

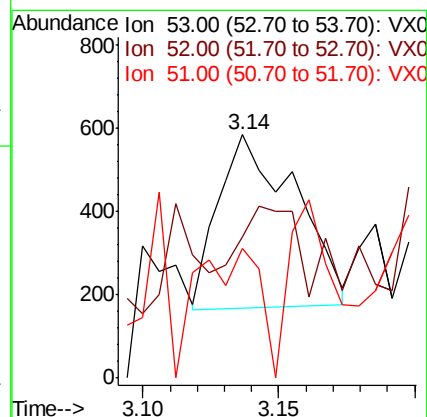



#16

Acetone

Concen: Below Cal

RT: 2.43 min Scan# 253

Delta R.T. 0.00 min

Lab File: VX014884.D

Acq: 10 Feb 2020 13:24

Instrument :

MSVOA_X

ClientSampleId :





VX0210MBL01

Tot Ion: 43 Resp: 6665

Ion Ratio Lower Upper

43 100

58 25.2 24.1 36.1

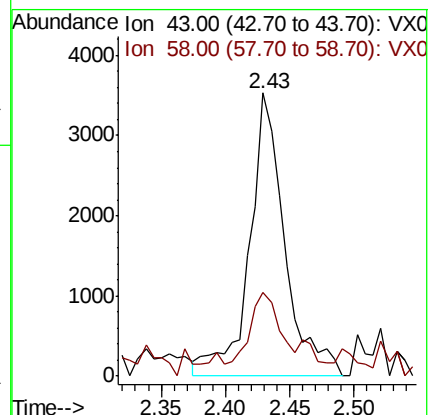

#17

Carbon Disulfide

Concen: 0.493 ug/l

RT: 2.57 min Scan# 276

Delta R.T. -0.00 min

Lab File: VX014884.D




Acq: 10 Feb 2020 13:24


Tgt Ion: 76 Resp: 5738

Ion Ratio Lower Upper

76 100

78 6.6 7.4 11.0#


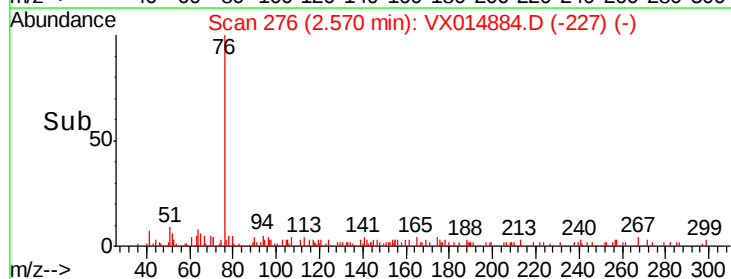
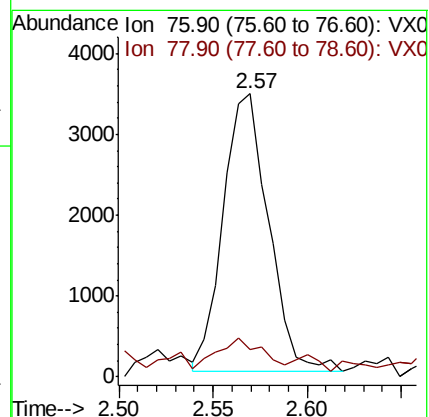



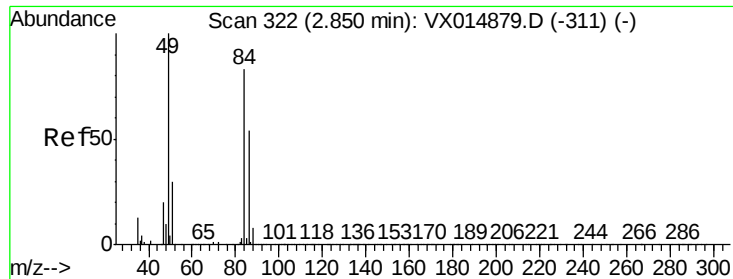

#20
Methvlene Chloride
Concen: 0.281 ug/l
RT: 2.85 min Scan# 322
Delta R.T. -0.00 min
Lab File: VX014884.D
Acq: 10 Feb 2020 13:24




Instrument :
MSVOA_X
ClientSampled :
VX0210MBL01


Tot Ion: 84 Resp: 1388
Ion Ratio Lower Upper
84 100
49 83.7 95.6 143.4#
51 63.2 29.0 43.6#
86 87.2 51.4 77.0#

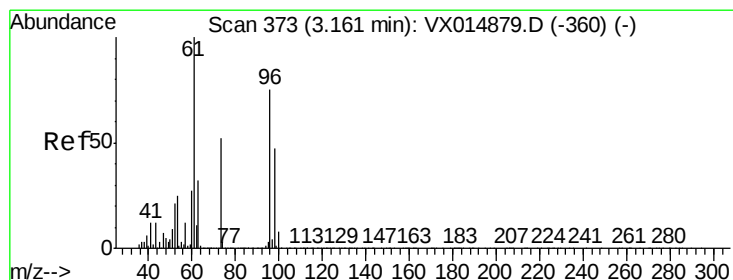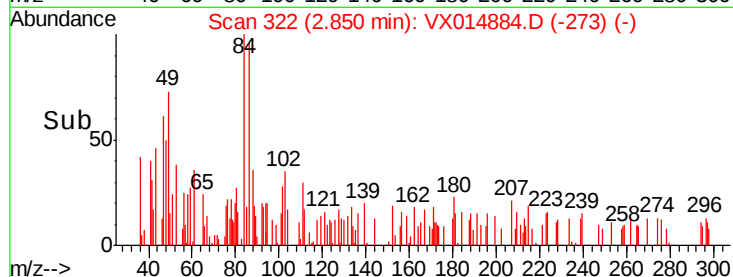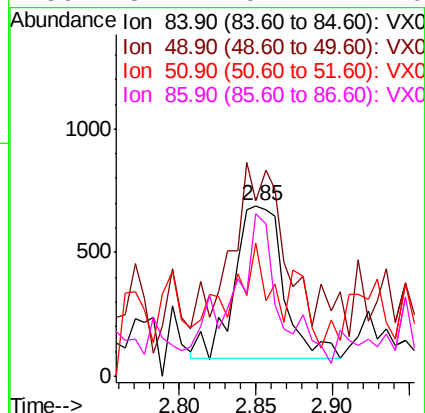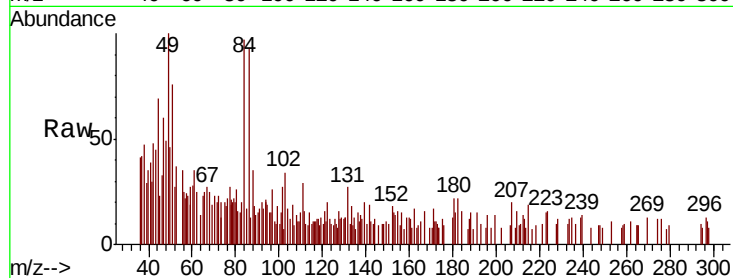

#21
trans-1,2-Dichloroethene
Concen: 0.232 ug/l
RT: 3.16 min Scan# 373
Delta R.T. -0.00 min
Lab File: VX014884.D
Acq: 10 Feb 2020 13:24

Tgt Ion: 96 Resp: 1066
Ion Ratio Lower Upper
96 100
61 75.8 106.9 160.3#
98 44.3 50.7 76.1#

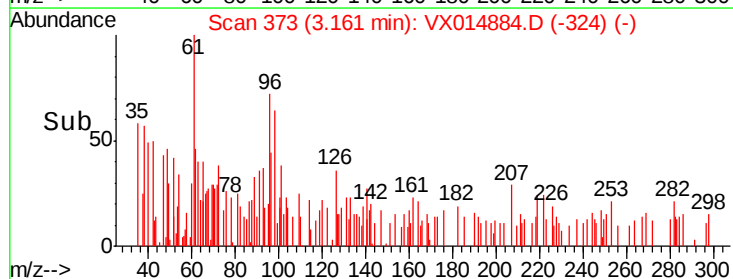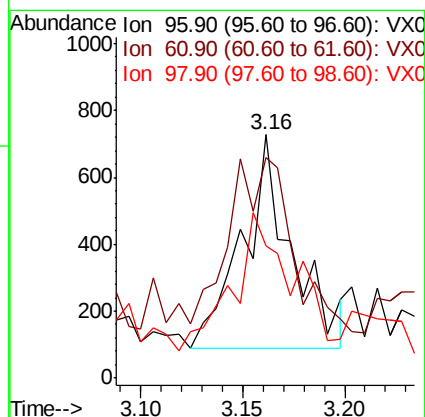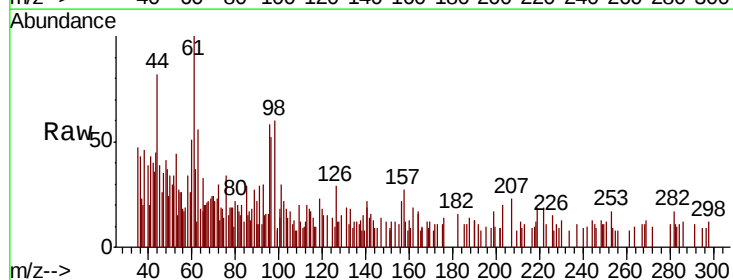

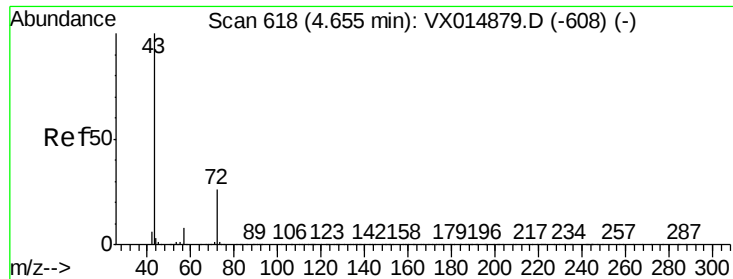

#25

2-Butanone

Concen: 0.476 ug/l

RT: 4.67 min Scan# 621

Delta R.T. 0.02 min

Lab File: VX014884.D

Acq: 10 Feb 2020 13:24

Instrument :

MSVOA_X

ClientSampled :





VX0210MBL01

Tot Ion: 43 Resp: 1662

Ion Ratio Lower Upper

43 100

72 0.0 21.0 31.6#

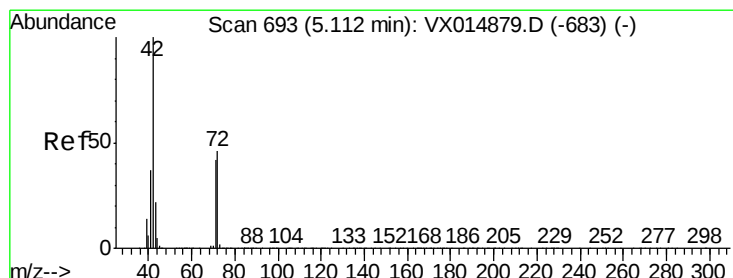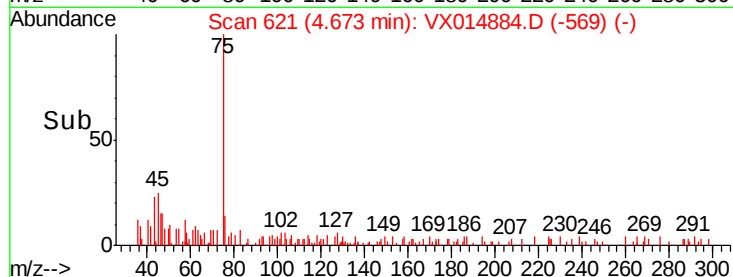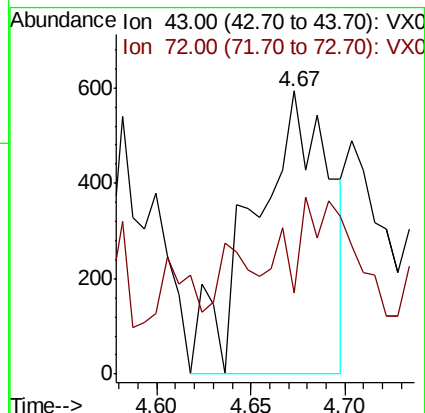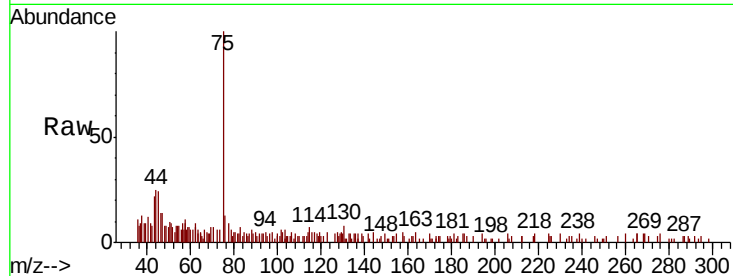

#29

Tetrahydrofuran

Concen: 0.216 ug/l

RT: 4.98 min Scan# 672

Delta R.T. -0.13 min

Lab File: VX014884.D

Acq: 10 Feb 2020 13:24




Tgt Ion: 42 Resp: 429


Ion Ratio Lower Upper

42 100

72 49.4 36.9 55.3

71 50.1 34.1 51.1

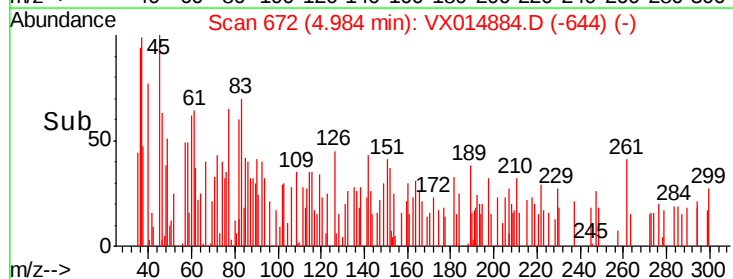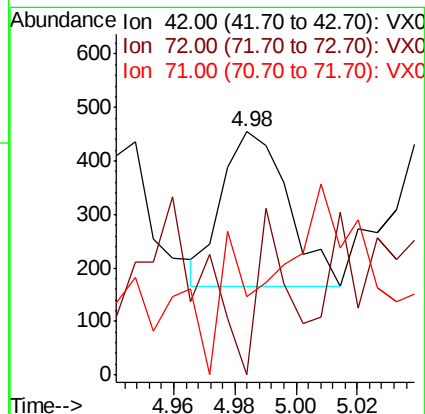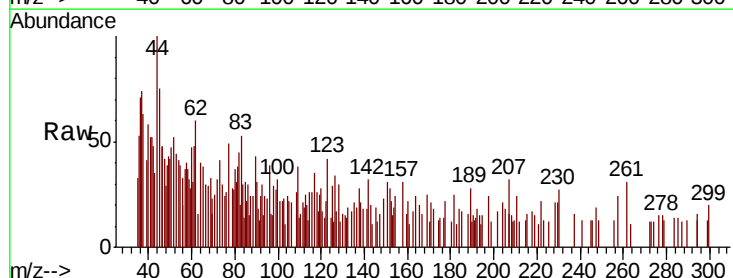



#33

1,2-Dichloroethane-d4

Concen: 50.421 ug/l

RT: 6.06 min Scan# 848

Delta R.T. -0.00 min

Lab File: VX014884.D

Acq: 10 Feb 2020 13:24

Instrument :

MSVOA_X

ClientSampleId :





VX0210MBL01

Tot Ion: 65 Resp: 258828

Ion Ratio Lower Upper

65 100

67 51.7 0.0 103.0

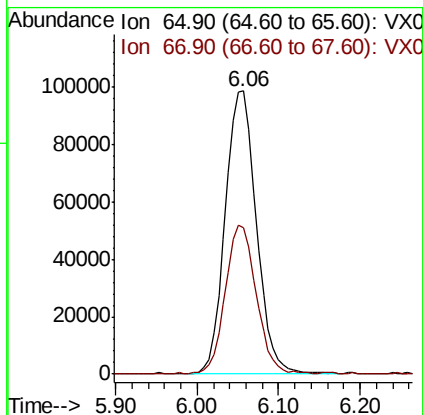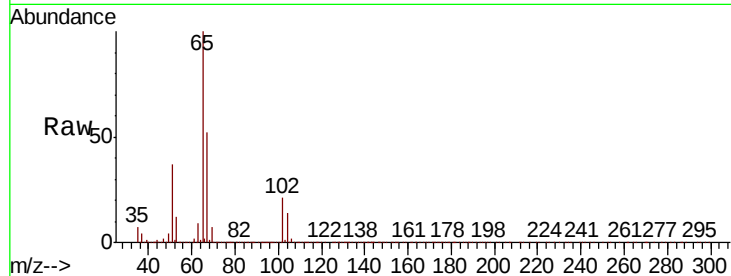

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 978

Delta R.T. -0.00 min

Lab File: VX014884.D

Acq: 10 Feb 2020 13:24




Tgt Ion: 114 Resp: 700818


Ion Ratio Lower Upper

114 100

63 19.5 0.0 39.2

88 15.4 0.0 32.0


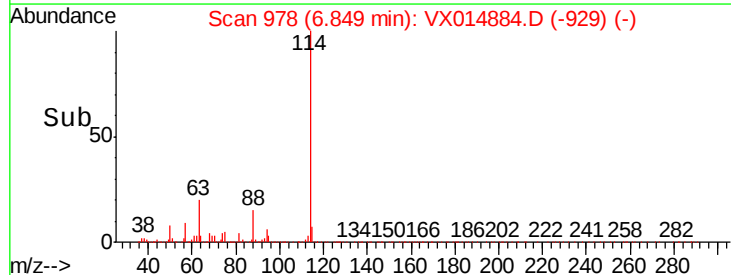
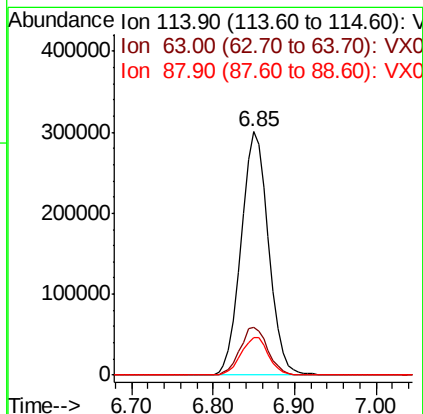





#35
 Dibromofluoromethane
 Concen: 50.167 ug/l
 RT: 5.49 min Scan# 755
 Delta R.T. -0.00 min
 Lab File: VX014884.D
 Acq: 10 Feb 2020 13:24




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0210MBL01


Tot Ion	Ratio	Lower	Upper
113	100		
111	102.4	82.4	123.6
192	24.4	19.1	28.7

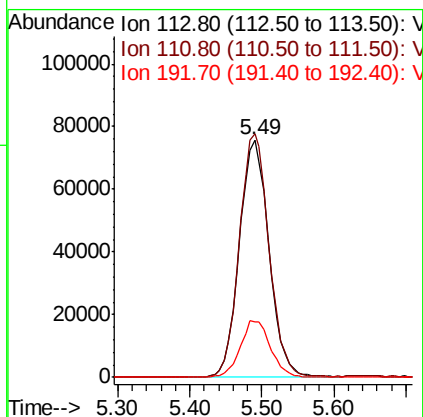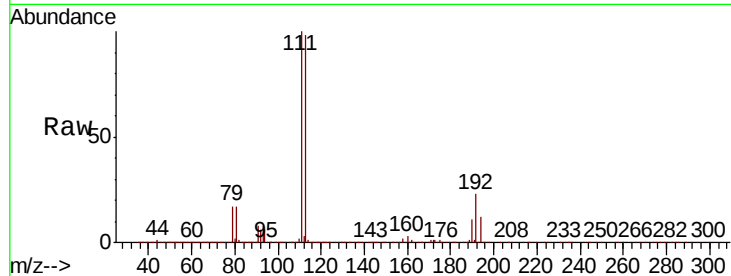

#36
 1,1-Dichloropropene
 Concen: 4.975 ug/l
 RT: 5.65 min Scan# 782
 Delta R.T. -0.14 min
 Lab File: VX014884.D
 Acq: 10 Feb 2020 13:24

Tgt Ion	Ratio	Lower	Upper
75	100		
110	11.2	18.3	54.8#
77	0.0	24.6	36.8#

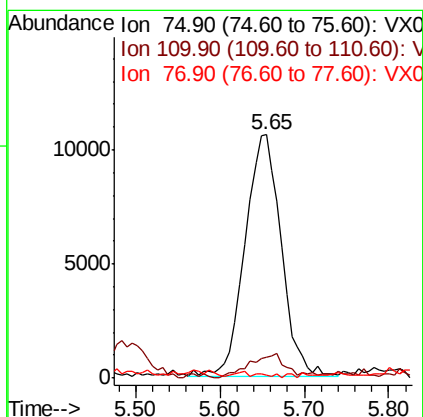

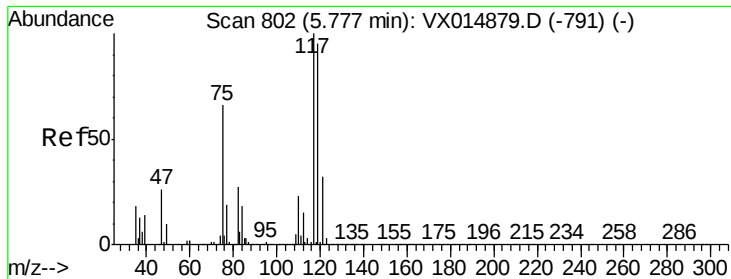

#38

Carbon Tetrachloride

Concen: 6.658 ug/l

RT: 5.65 min Scan# 782

Delta R.T. -0.12 min

Lab File: VX014884.D

Acq: 10 Feb 2020 13:24

Instrument :





MSVOA_X

ClientSampleId :

VX0210MBL01

Tot Ion:117 Resp: 40679

Ion	Ratio	Lower	Upper
117	100		
119	3.6	76.0	114.0#
121	0.0	25.4	38.2#

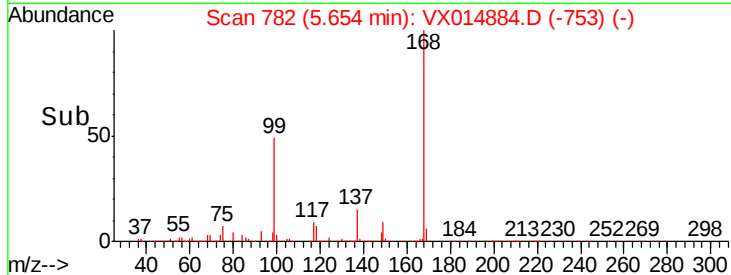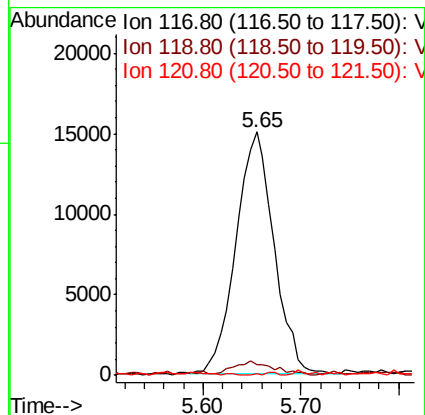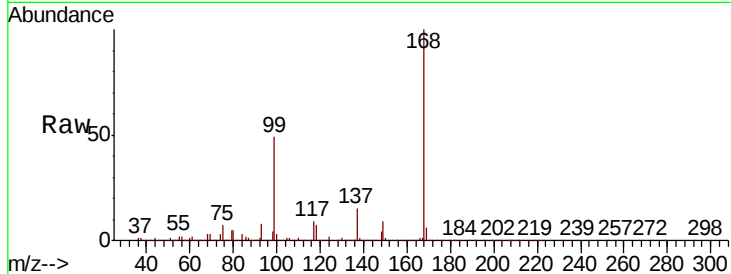

#44

Trichloroethene

Concen: 0.226 ug/l

RT: 7.22 min Scan# 1038




Delta R.T. 0.01 min


Lab File: VX014884.D

Acq: 10 Feb 2020 13:24

Tgt Ion:130 Resp: 1228

Ion	Ratio	Lower	Upper
130	100		
95	72.7	0.0	182.6


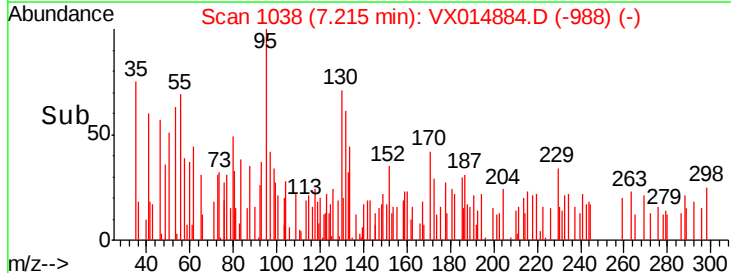
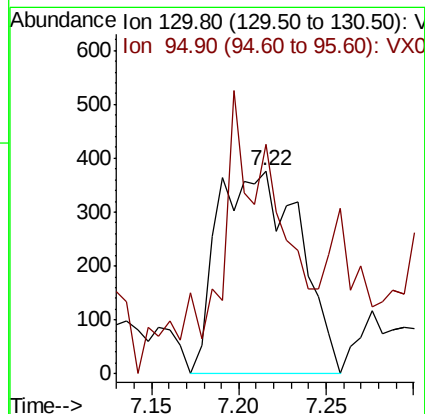





#49
1,4-Dioxane
Concen: 5.078 ug/l
RT: 7.73 min Scan# 1123
Delta R.T. -0.00 min
Lab File: VX014884.D
Acq: 10 Feb 2020 13:24




Instrument :
MSVOA_X
ClientSampleId :
VX0210MBL01


Tot Ion: 88 Resp: 504
Ion Ratio Lower Upper
88 100
43 67.5 27.0 40.4#
58 20.2 53.2 79.8#

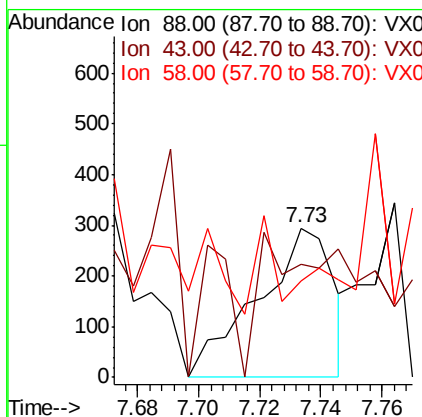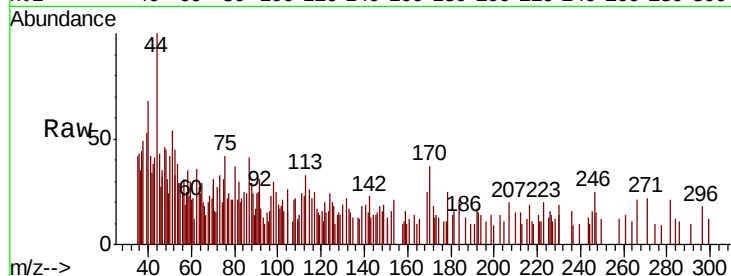

#50
Toluene-d8
Concen: 50.989 ug/l
RT: 8.71 min Scan# 1283
Delta R.T. -0.00 min
Lab File: VX014884.D
Acq: 10 Feb 2020 13:24

Tgt Ion: 98 Resp: 838549
Ion Ratio Lower Upper
98 100
100 65.7 52.4 78.6



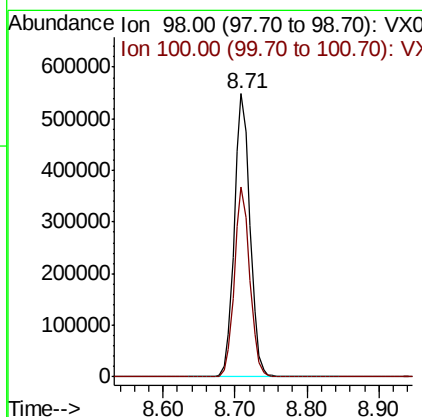



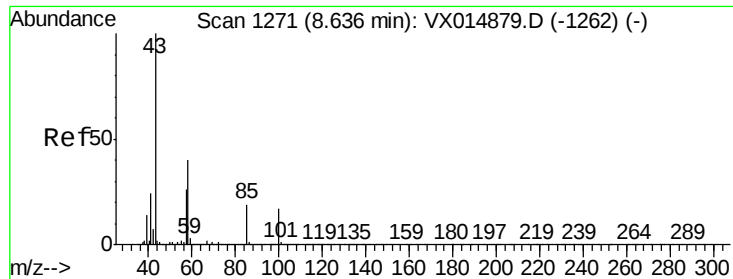

#51
4-Methyl-2-Pentanone
Concen: 0.209 ug/l
RT: 8.64 min Scan# 1271
Delta R.T. -0.00 min
Lab File: VX014884.D
Acq: 10 Feb 2020 13:24




Instrument :
MSVOA_X
ClientSampleId :
VX0210MBL01


Tot Ion: 43 Resp: 1361
Ion Ratio Lower Upper
43 100
58 0.0 31.9 47.9#

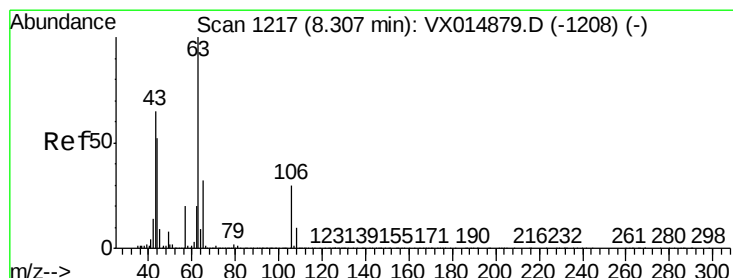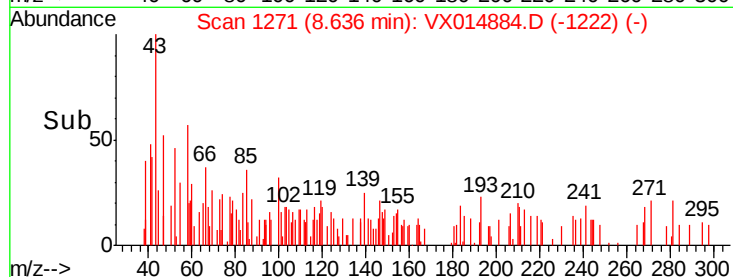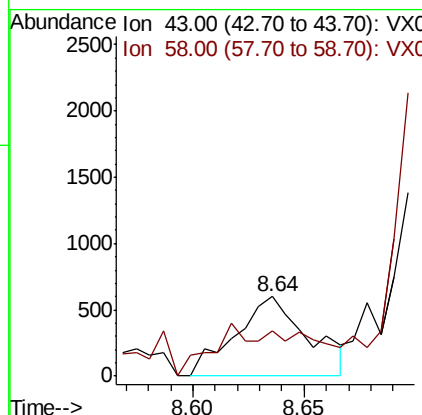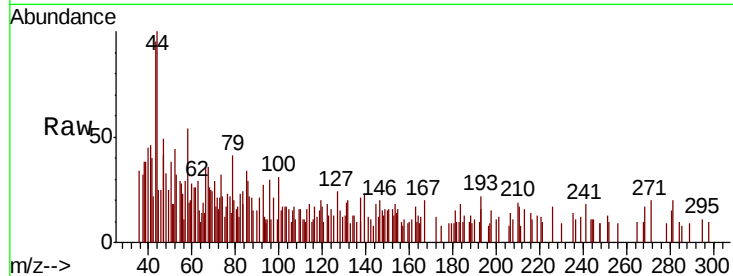

#58
2-Chloroethyl Vinyl ether
Concen: 0.220 ug/l
RT: 8.47 min Scan# 1244
Delta R.T. 0.16 min
Lab File: VX014884.D
Acq: 10 Feb 2020 13:24

Tgt Ion: 63 Resp: 833
Ion Ratio Lower Upper
63 100
106 31.8 23.8 35.8


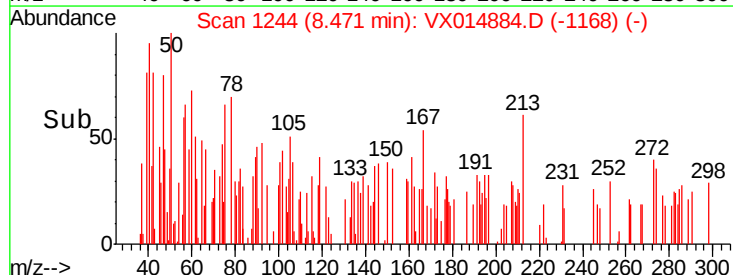
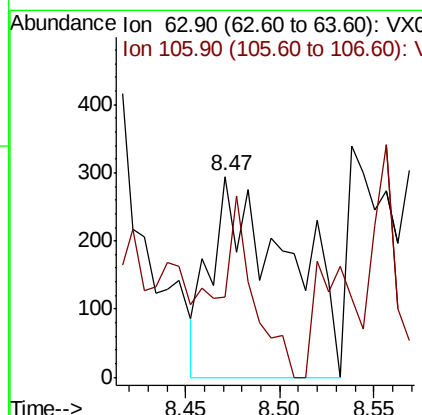
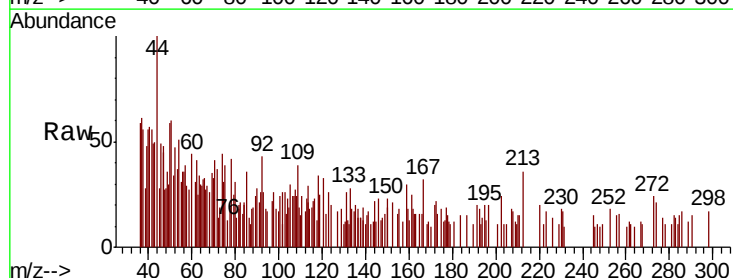


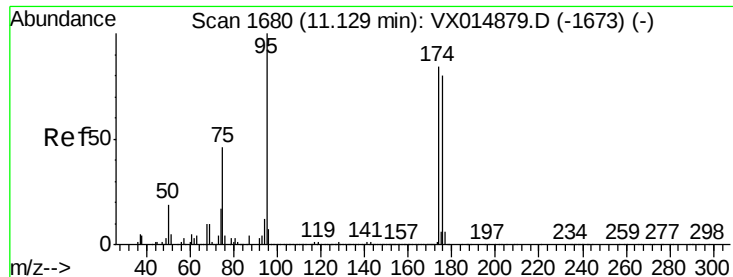

#62
4-Bromofluorobenzene
Concen: 52.032 ug/l
RT: 11.13 min Scan# 1680
Delta R.T. -0.00 min
Lab File: VX014884.D
Acq: 10 Feb 2020 13:24




Instrument :
MSVOA_X
ClientSampleId :
VX0210MBL01


Tot Ion: 95 Resp: 308252
Ion Ratio Lower Upper
95 100
174 91.2 0.0 183.0
176 87.9 0.0 178.0

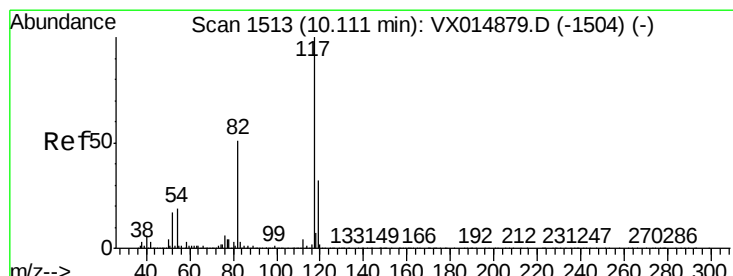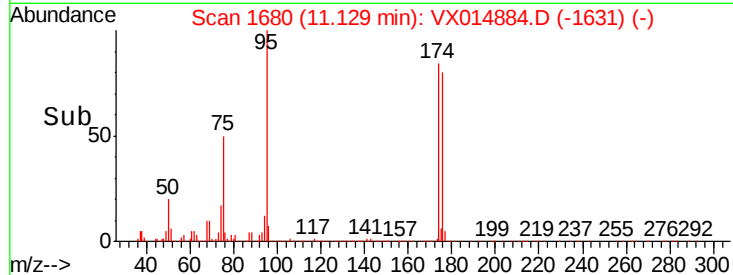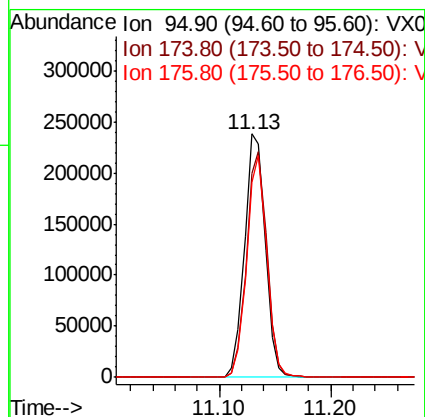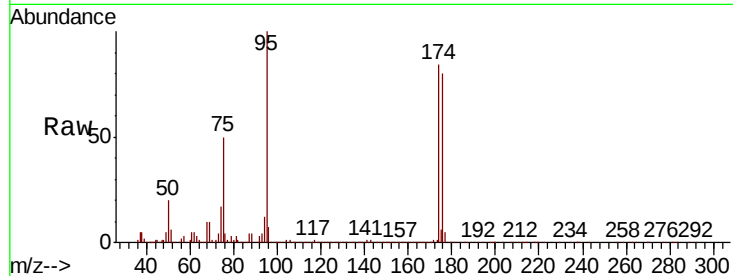

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1512
Delta R.T. -0.01 min
Lab File: VX014884.D
Acq: 10 Feb 2020 13:24

Tgt Ion: 117 Resp: 656561
Ion Ratio Lower Upper
117 100
82 54.4 40.5 60.7
119 31.5 25.8 38.6

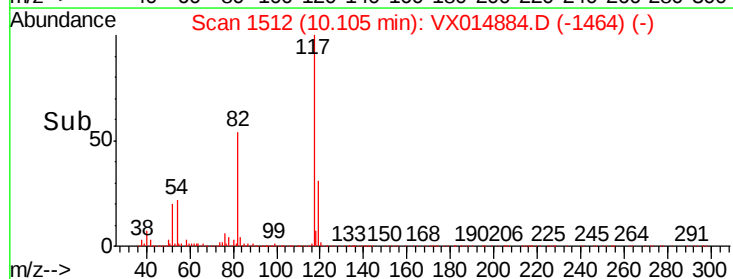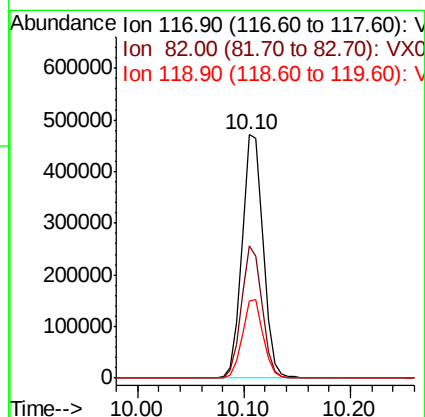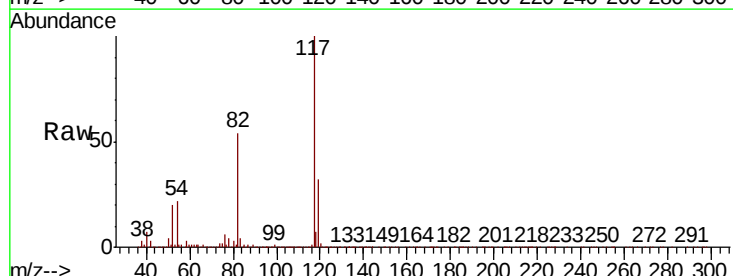

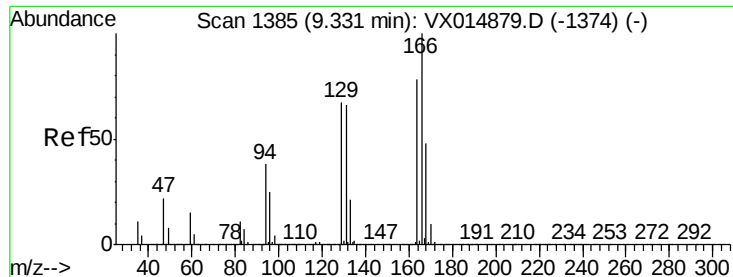

#64

Tetrachloroethene

Concen: 0.229 ug/l

RT: 9.32 min Scan# 1384

Delta R.T. -0.01 min

Lab File: VX014884.D

Acq: 10 Feb 2020 13:24

Instrument :

MSVOA_X

ClientSampleId :

VX0210MBL01

Tot Ion:164 Resp: 1406


Ion Ratio Lower Upper

164 100

166 68.1 102.6 153.8#

129 37.8 68.3 102.5#

131 25.2 67.4 101.2#



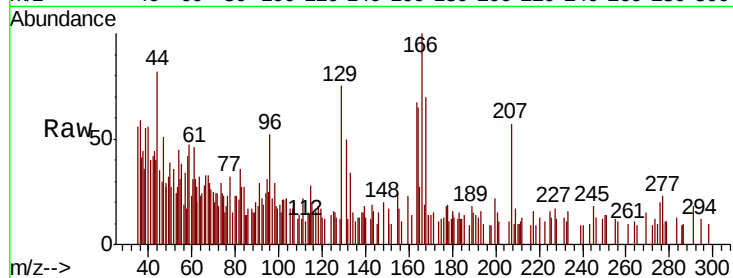


Abundance Ion 163.80 (163.50 to 164.50): V

Ion 165.80 (165.50 to 166.50): V

Ion 128.80 (128.50 to 129.50): V

Ion 130.80 (130.50 to 131.50): V

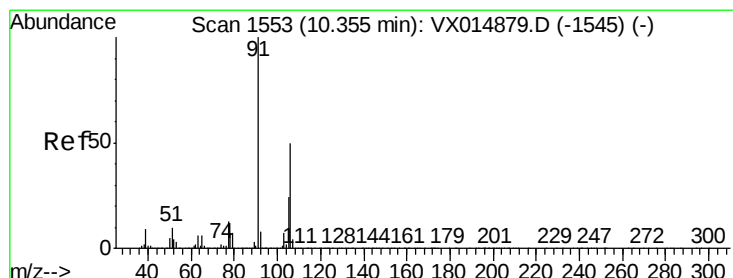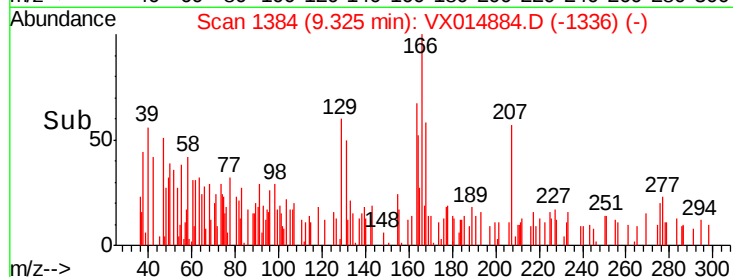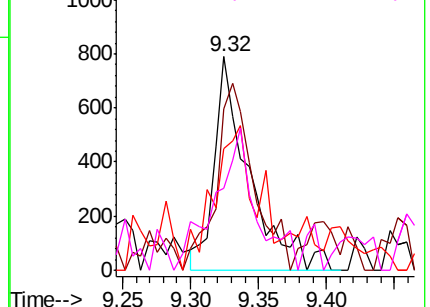

#68

m/p-Xylenes

Concen: 0.200 ug/l

RT: 10.35 min Scan# 1553

Delta R.T. -0.00 min

Lab File: VX014884.D


Acq: 10 Feb 2020 13:24

Tgt Ion:106 Resp: 1749

Ion Ratio Lower Upper



106 100


91 154.1 160.6 240.8#

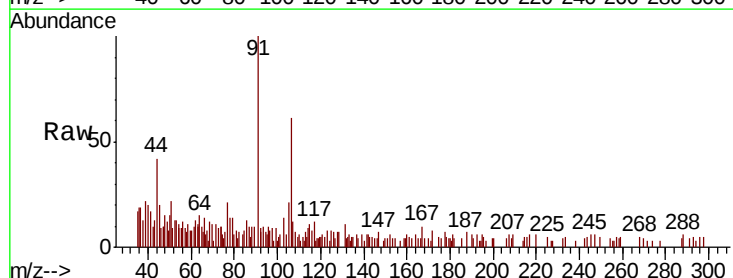

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VX0

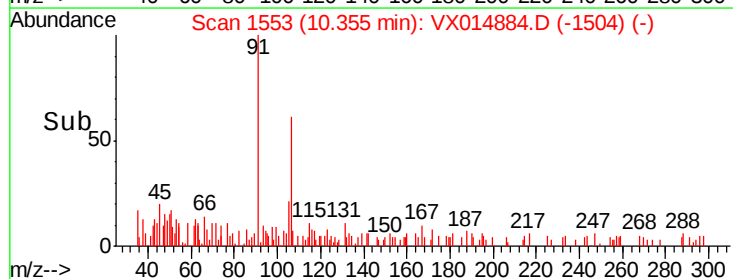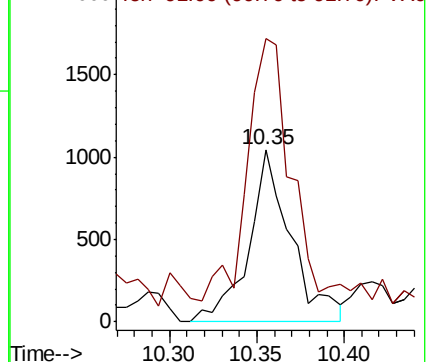

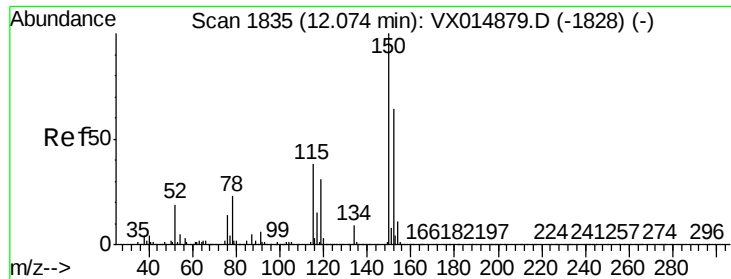

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.07 min Scan# 1835

Delta R.T. -0.00 min

Lab File: VX014884.D

Acq: 10 Feb 2020 13:24

Instrument :

MSVOA_X

ClientSampleId :

VX0210MBL01


Tot Ion:152 Resp: 331394

Ion Ratio Lower Upper

152 100

115 54.4 38.6 116.0




150 156.4 0.0 349.0

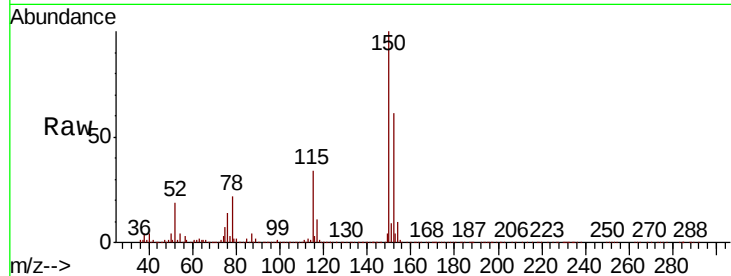

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

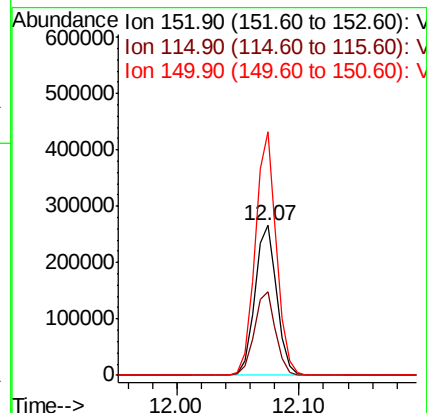

#76

1,2,3-Trichloropropane

Concen: 25.445 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. -0.16 min

Lab File: VX014884.D


Acq: 10 Feb 2020 13:24

Tgt Ion: 75 Resp: 152484

Ion Ratio Lower Upper



75 100


77 1.5 18.4 55.0#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

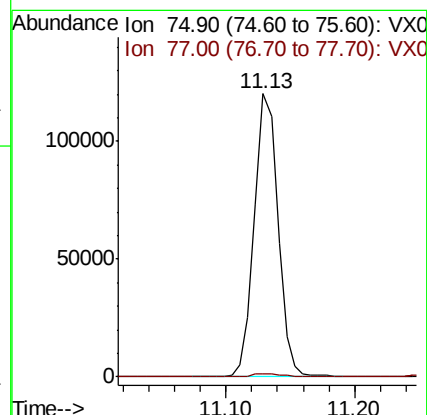

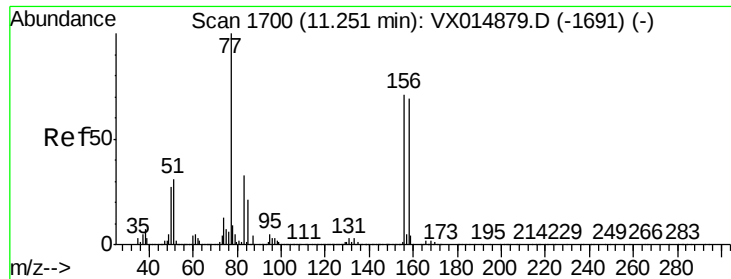

#77

Bromobenzene

Concen: 0.212 ug/l

RT: 11.26 min Scan# 1701

Delta R.T. 0.01 min

Lab File: VX014884.D

Acq: 10 Feb 2020 13:24

Instrument :

MSVOA_X

ClientSampleId :

VX0210MBL01


Tot Ion:156 Resp: 1229

Ion Ratio Lower Upper

156 100

77 95.3 74.0 222.0




158 64.3 48.9 146.6

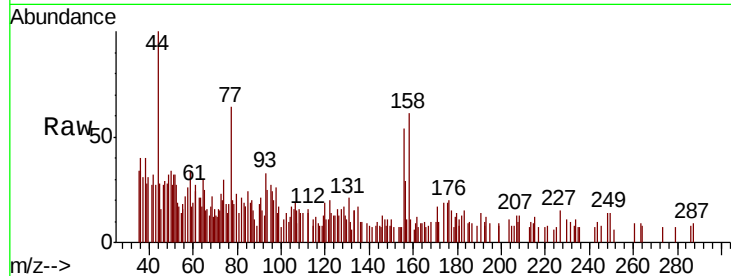

Abundance Ion 155.80 (155.50 to 156.50): V

Ion 77.00 (76.70 to 77.70): VX0

Ion 157.80 (157.50 to 158.50): V

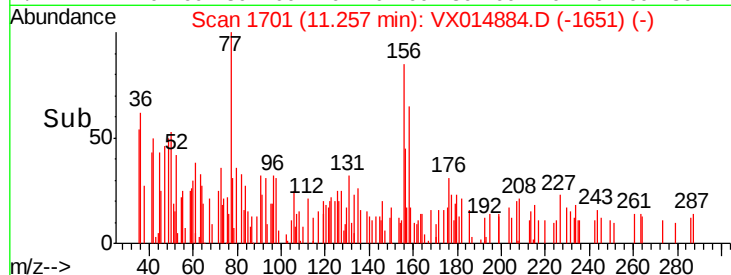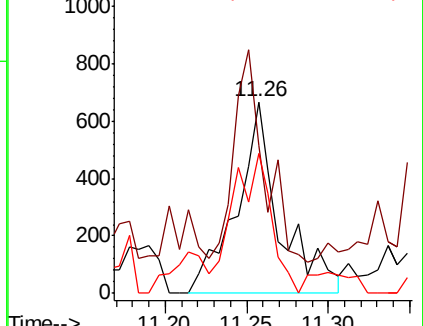

#81

trans-1,4-Dichloro-2-butene

Concen: 65.132 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. 0.06 min

Lab File: VX014884.D

Acq: 10 Feb 2020 13:24


Tgt Ion: 75 Resp: 152484

Ion Ratio Lower Upper

75 100

53 0.2 76.2 114.2#



89 0.1 35.8 53.6#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0




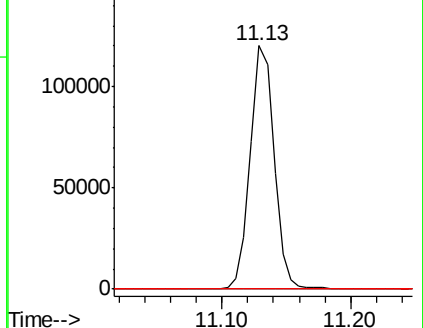




#93
 1,2,4-Trichlorobenzene
 Concen: 0.291 ug/l
 RT: 13.64 min Scan# 2092
 Delta R.T. -0.00 min
 Lab File: VX014884.D
 Acq: 10 Feb 2020 13:24




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0210MBL01


Tot Ion	Ratio	Lower	Upper
180	100		
182	99.1	48.4	145.3
145	48.1	14.1	42.4

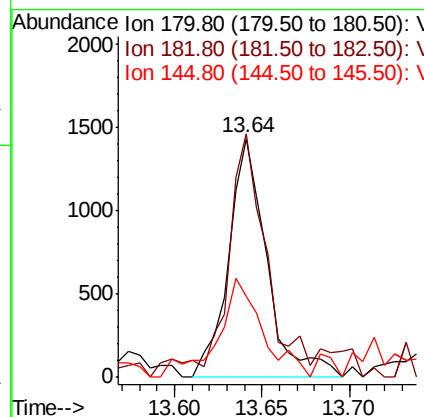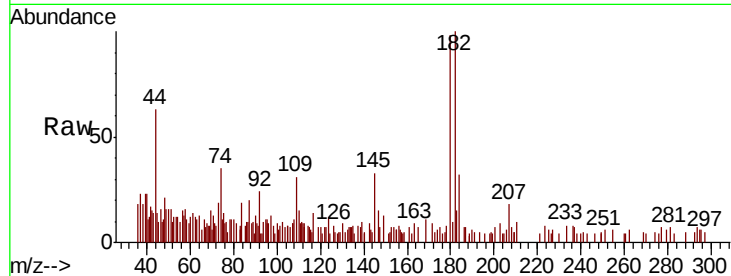

#94
 Hexachlorobutadiene
 Concen: 0.279 ug/l
 RT: 13.78 min Scan# 2115
 Delta R.T. 0.01 min
 Lab File: VX014884.D
 Acq: 10 Feb 2020 13:24

Tgt Ion	Ratio	Lower	Upper
225	100		
223	53.9	31.1	93.2
227	51.5	30.9	92.5

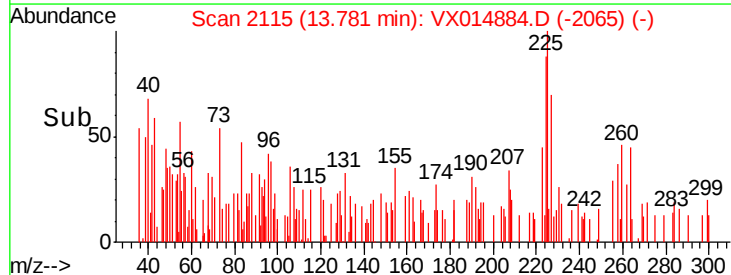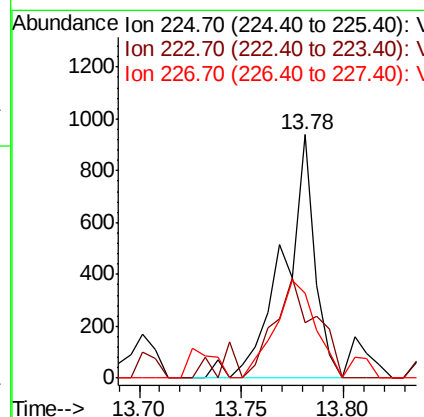


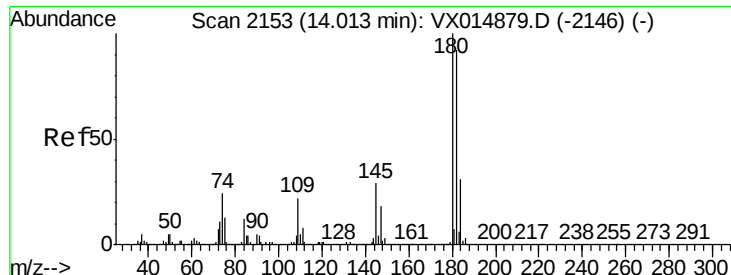

#96
 1,2,3-Trichlorobenzene
 Concen: 0.226 ug/l
 RT: 14.02 min Scan# 2154
 Delta R.T. 0.01 min
 Lab File: VX014884.D
 Acq: 10 Feb 2020 13:24

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0210MBL01

Tot Ion	Ratio	Lower	Upper
180	100		
182	97.0	47.5	142.6
145	37.8	14.5	43.5



Abundance Ion 179.80 (179.50 to 180.50): V
 Ion 181.80 (181.50 to 182.50): V
 Ion 144.90 (144.60 to 145.60): V

