


Instrument :  
MSVOA\_X  
ClientSampleId :

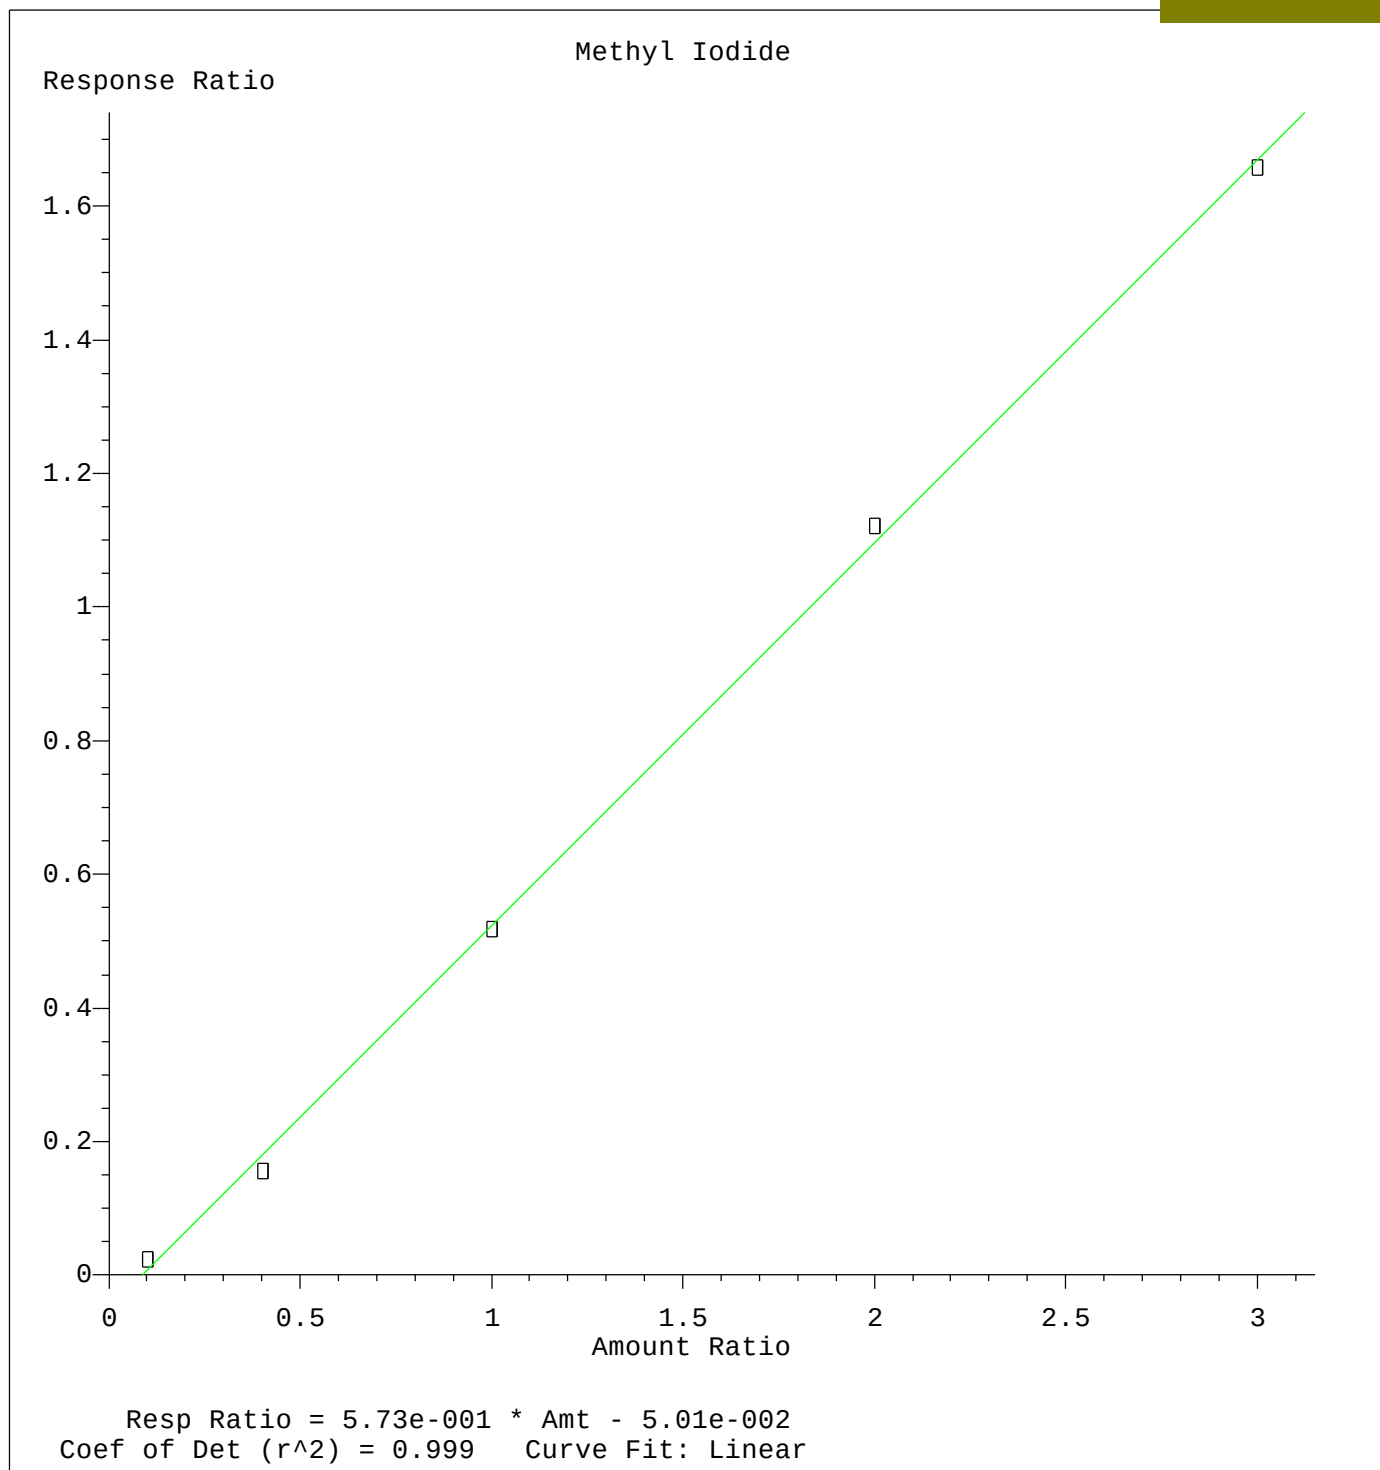


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X021020W.M  
Calibration Table Last Updated: Mon Feb 10 12:09:20 2020

Instrument :  
MSVOA\_X  
ClientSampleId :

# Acetone

Response Ratio

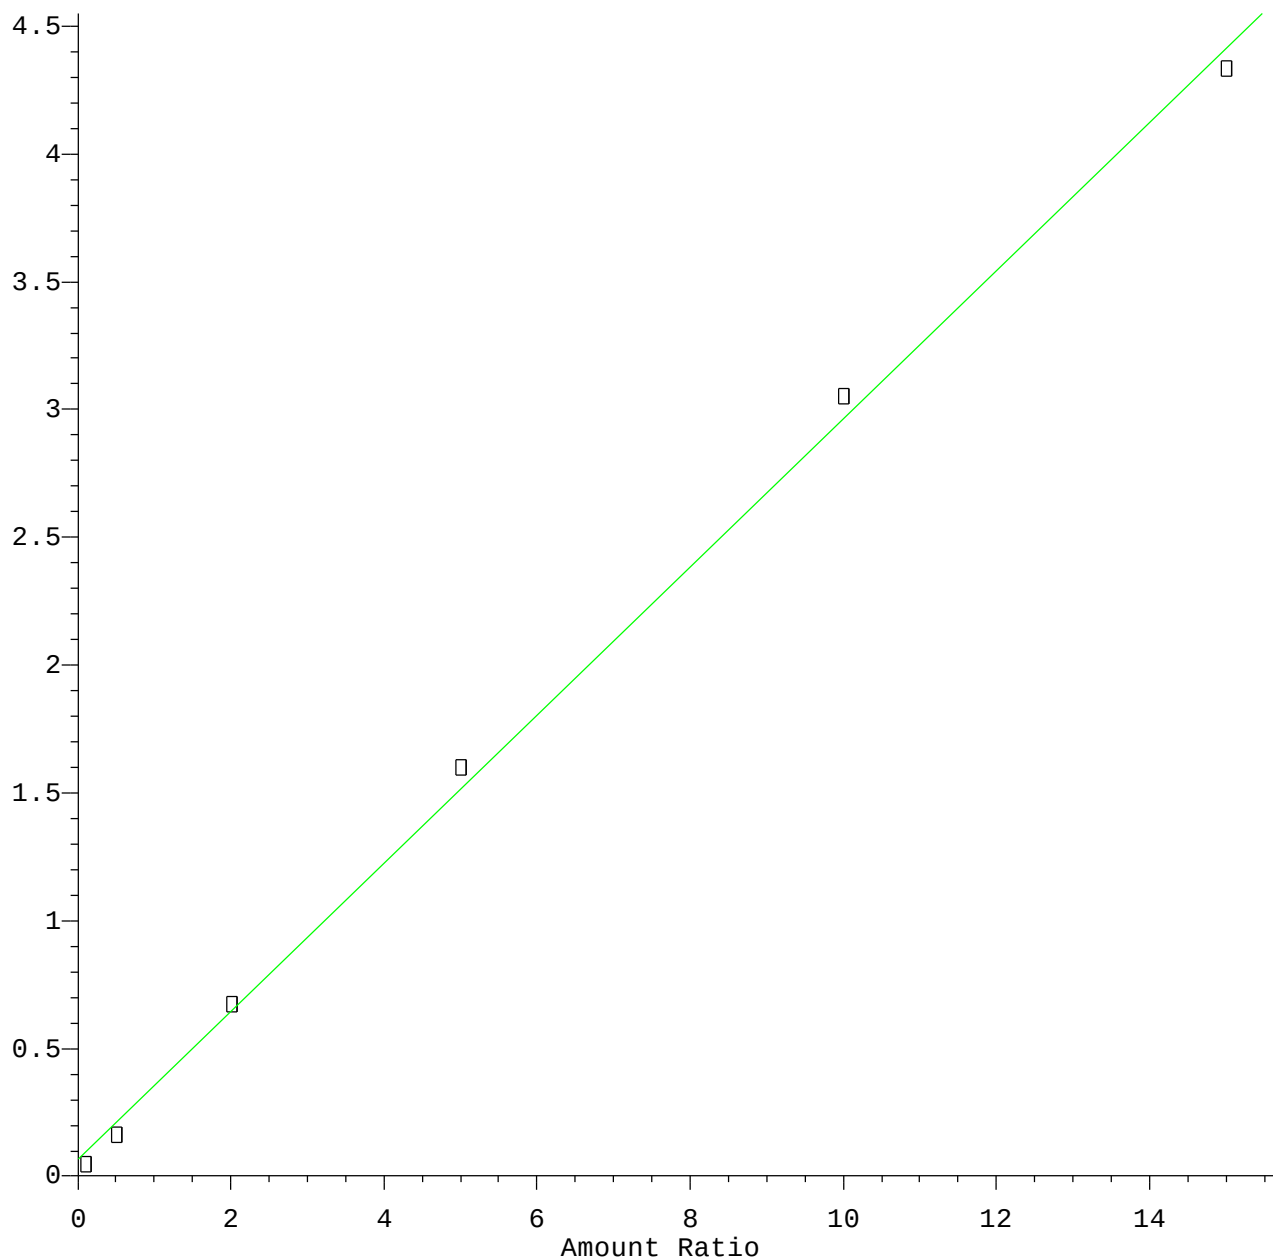

Resp Ratio =  $2.90 \times 10^{-1} \times \text{Amt} + 6.62 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.998    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X021020W.M  
Calibration Table Last Updated: Mon Feb 10 12:09:20 2020