


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX021020\
Data File : VX014875.D
Acq On : 10 Feb 2020 09:21
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X021020W.M
Title : SW846 8260
Last Update : Mon Feb 10 12:09:20 2020

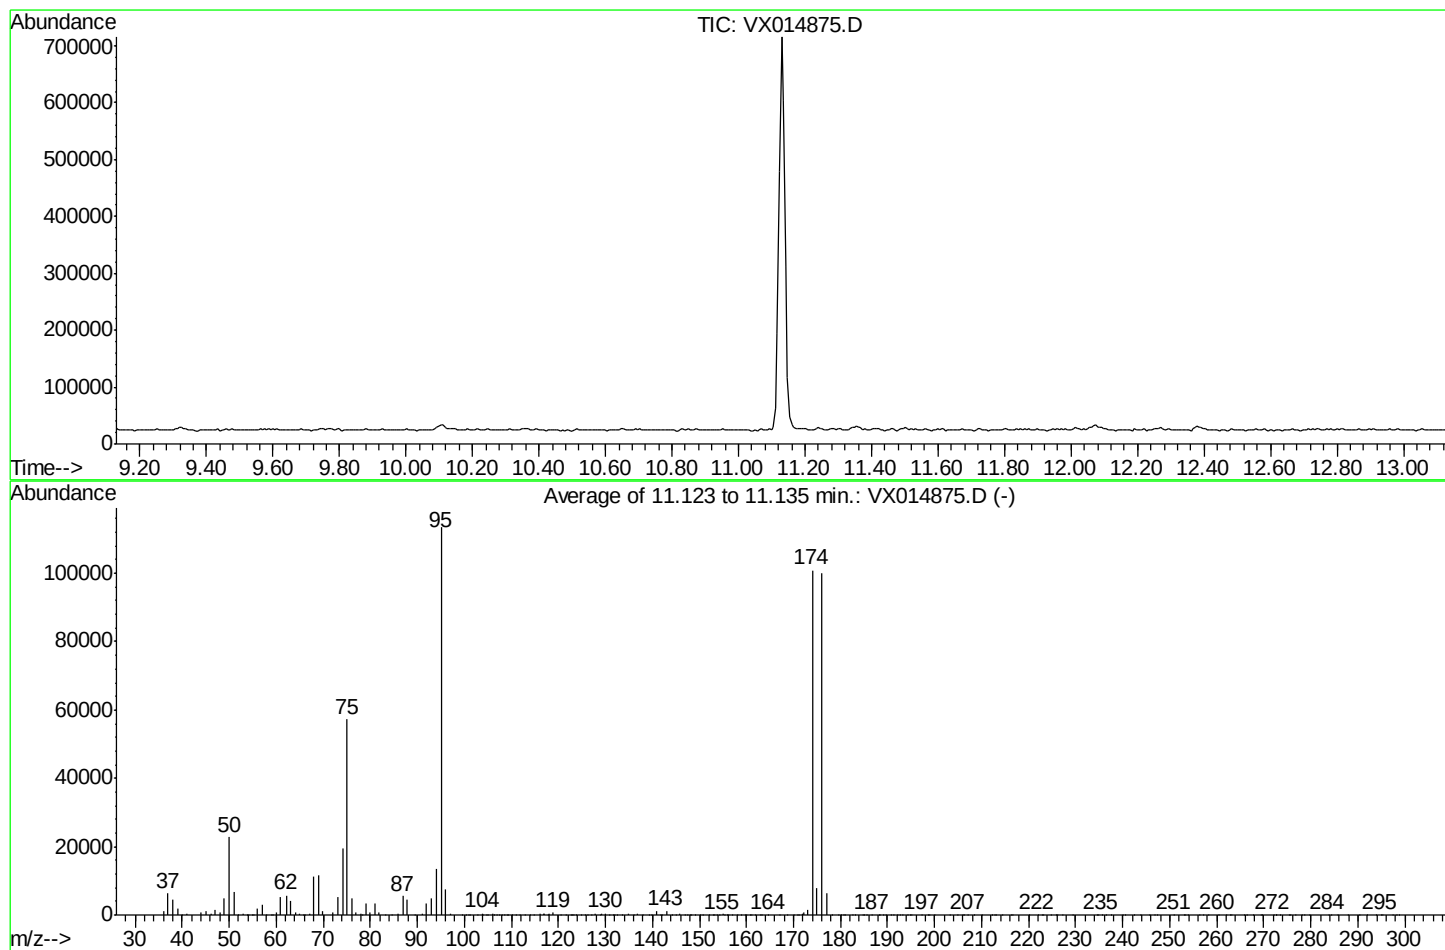

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1672

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	22695	PASS
75	95	30	60	50.4	57192	PASS
95	95	100	100	100.0	113456	PASS
96	95	5	9	6.8	7673	PASS
173	174	0.00	2	1.3	1359	PASS
174	95	50	100	88.9	100813	PASS
175	174	5	9	7.7	7792	PASS
176	174	95	101	99.1	99895	PASS
177	176	5	9	6.5	6456	PASS