

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
 Data File : VX026933.D
 Acq On : 10 Feb 2022 20:13
 Operator : JC/MD
 Sample : N1425-04 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 20422DL

Quant Time: Feb 11 04:03:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 08 07:07:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	115802	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	195253	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	180836	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	78948	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	75064	54.000	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 108.000%			
35) Dibromofluoromethane	5.391	113	61191	52.602	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 105.200%			
50) Toluene-d8	8.653	98	230320	53.938	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 107.880%			
62) 4-Bromofluorobenzene	11.079	95	86507	57.543	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 115.080%			
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	2.959	59	4441	17.684	ug/l	99
16) Acetone	2.386	43	8052	13.188	ug/l #	88
18) Methyl Acetate	2.703	43	613	0.349	ug/l	91
25) 2-Butanone	4.568	43	4220	4.290	ug/l	95
31) Cyclohexane	5.556	56	2353	1.065	ug/l #	1
36) 1,1-Dichloropropene	5.556	75	8975	4.891	ug/l #	51
37) Ethyl Acetate	4.568	43	4220	2.023	ug/l #	69
38) Carbon Tetrachloride	5.556	117	12275	6.379	ug/l #	16
40) Benzene	6.044	78	132016	24.683	ug/l	100
51) 4-Methyl-2-Pentanone	8.580	43	541	0.278	ug/l	94
52) Toluene	8.720	92	67742	20.005	ug/l	99
53) t-1,3-Dichloropropene	8.720	75	763	1.732	ug/l #	1
67) Ethyl Benzene	10.195	91	14550	2.198	ug/l	96
68) m/p-Xylenes	10.299	106	27473	10.788	ug/l	100
69) o-Xylene	10.646	106	23097	9.256	ug/l	99
70) Styrene	10.659	104	13151	3.249	ug/l #	82
73) Isopropylbenzene	10.963	105	2150	0.346	ug/l	98
76) 1,2,3-Trichloropropane	11.079	75	42720	24.719	ug/l #	40
78) n-propylbenzene	11.305	91	7074	1.026	ug/l	97
79) 2-Chlorotoluene	11.384	91	3620	0.850	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.451	105	10833	2.117	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.079	75	42720	75.437	ug/l #	3
82) 4-Chlorotoluene	11.451	91	1194	0.250	ug/l #	46
83) tert-Butylbenzene	11.756	119	5127	1.051	ug/l #	64
84) 1,2,4-Trimethylbenzene	11.756	105	42345	8.203	ug/l	98
85) sec-Butylbenzene	11.890	105	2403	0.389	ug/l	88
86) p-Isopropyltoluene	11.969	119	3079	0.588	ug/l	97
89) n-Butylbenzene	12.335	91	4360	1.017	ug/l #	43
90) Hexachloroethane	12.530	117	619	0.818	ug/l #	14
95) Naphthalene	13.780	128	95034	16.449	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
Data File : VX026933.D
Acq On : 10 Feb 2022 20:13
Operator : JC/MD
Sample : N1425-04 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
20422DL


Quant Time: Feb 11 04:03:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 08 07:07:46 2022
Response via : Initial Calibration

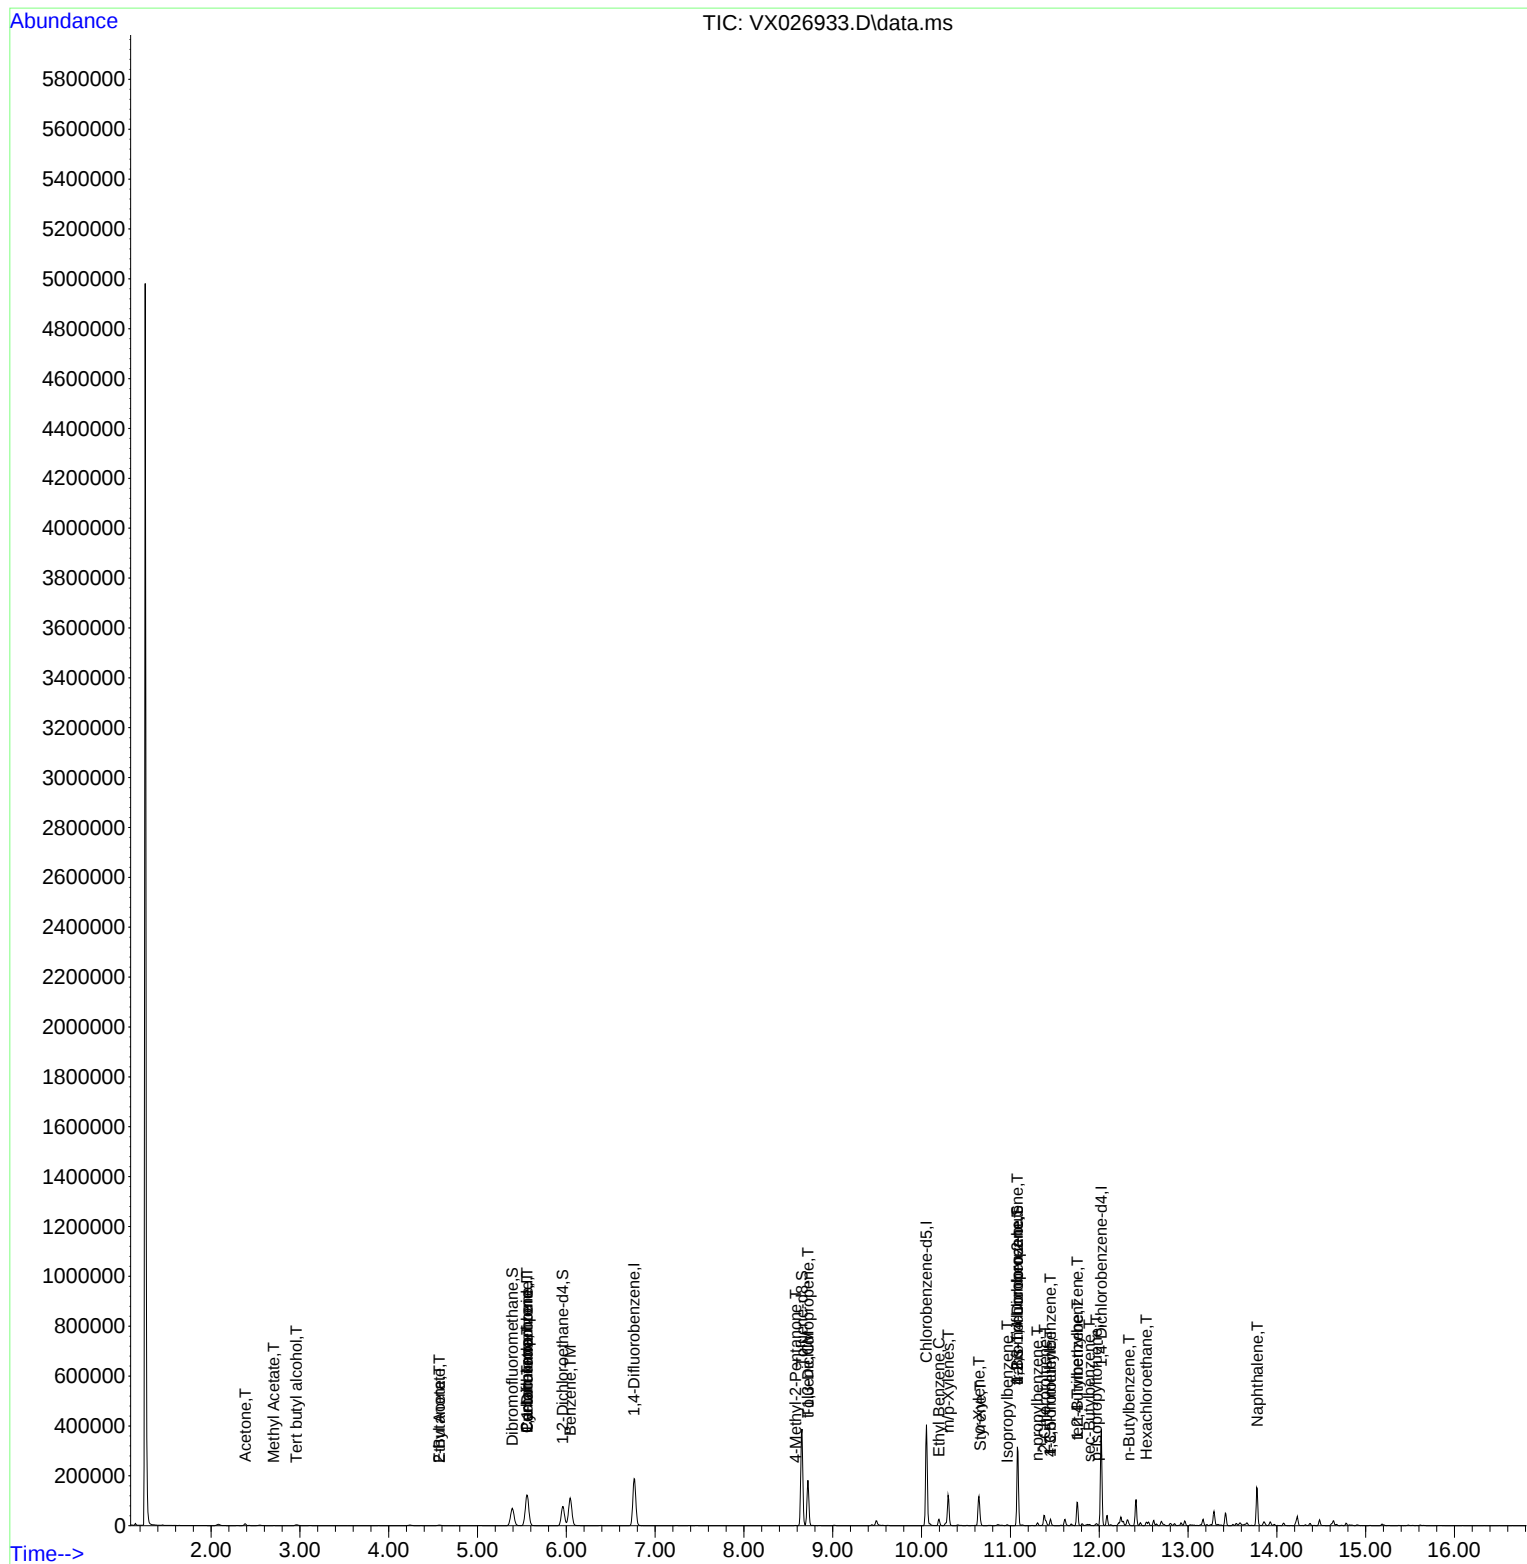



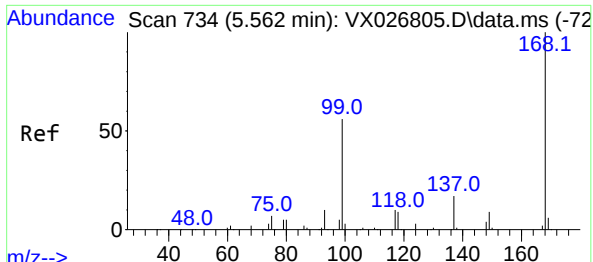


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13

Instrument :
MSVOA_X
ClientSampleId :
20422DL



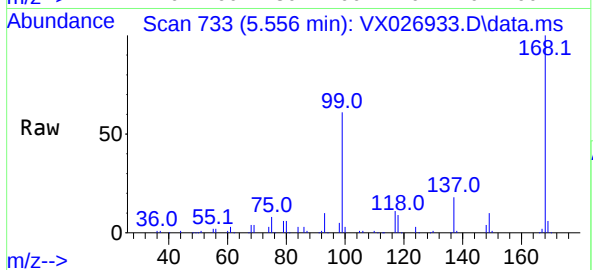



Tgt Ion:168 Resp: 115802
Ion Ratio Lower Upper
168 100
99 61.2 50.3 75.5

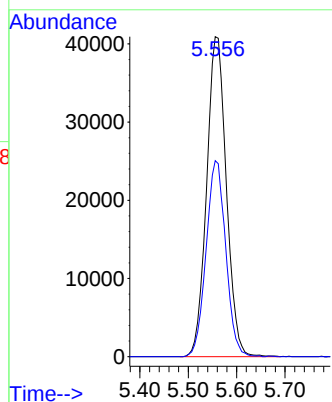

#11
Tert butyl alcohol
Concen: 17.684 ug/l
RT: 2.959 min Scan# 307
Delta R.T. -0.042 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13

Tgt Ion: 59 Resp: 4441
Ion Ratio Lower Upper
59 100
57 9.2 7.2 10.8


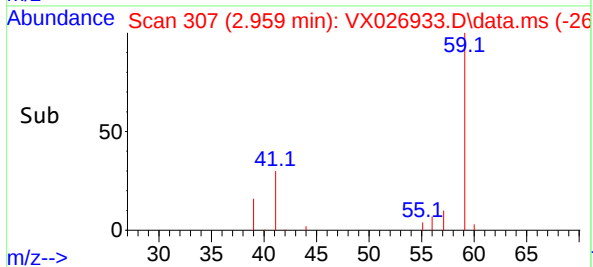
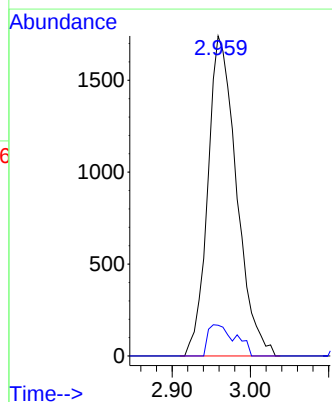
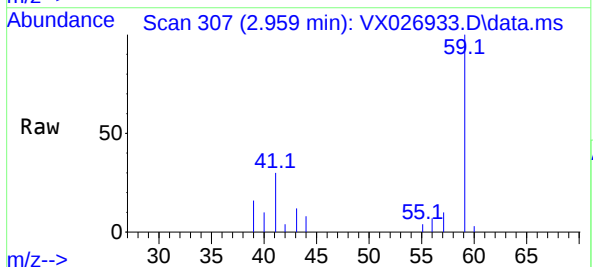




#16
Acetone
Concen: 13.188 ug/l
RT: 2.386 min Scan# 213
Delta R.T. 0.000 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13




Instrument :
MSVOA_X
ClientSampleId :
20422DL


Tgt Ion: 43 Resp: 8052
Ion Ratio Lower Upper
43 100
58 35.1 23.0 34.6#



#18
Methyl Acetate
Concen: 0.349 ug/l
RT: 2.703 min Scan# 265
Delta R.T. -0.006 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13

Tgt Ion: 43 Resp: 613
Ion Ratio Lower Upper
43 100
74 18.4 18.3 27.5


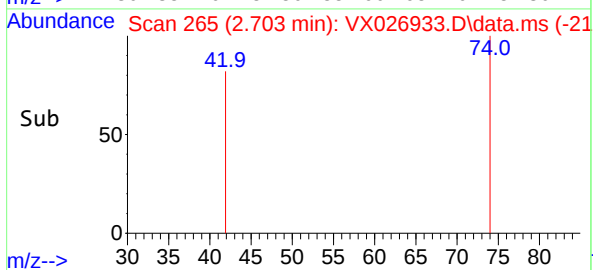






#25
2-Butanone
Concen: 4.290 ug/l
RT: 4.568 min Scan# 51
Delta R.T. 0.006 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13




Instrument :
MSVOA_X
ClientSampleId :
20422DL


Tgt Ion: 43 Resp: 4220
Ion Ratio Lower Upper
43 100
72 28.2 20.4 30.6

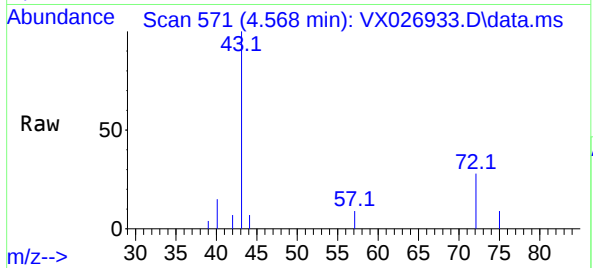

#31
Cyclohexane
Concen: 1.065 ug/l
RT: 5.556 min Scan# 733
Delta R.T. 0.079 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13

Tgt Ion: 56 Resp: 2353
Ion Ratio Lower Upper
56 100
69 199.9 25.8 38.6#
84 142.7 68.9 103.3#

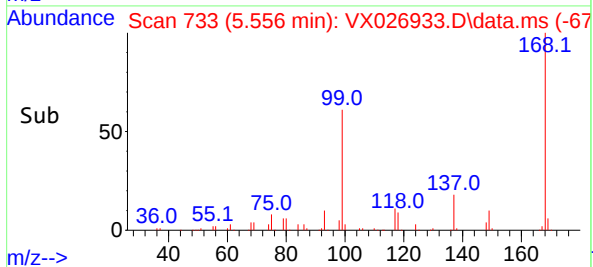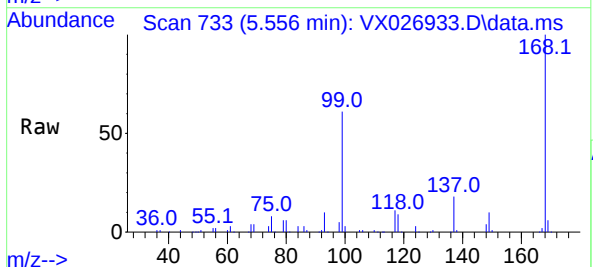



#33

1,2-Dichloroethane-d4

Concen: 54.000 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX026933.D

Acq: 10 Feb 2022 20:13

Instrument :

MSVOA_X

ClientSampleId :





20422DL

Tgt Ion: 65 Resp: 75064

Ion Ratio Lower Upper

65 100

67 52.3 0.0 100.8

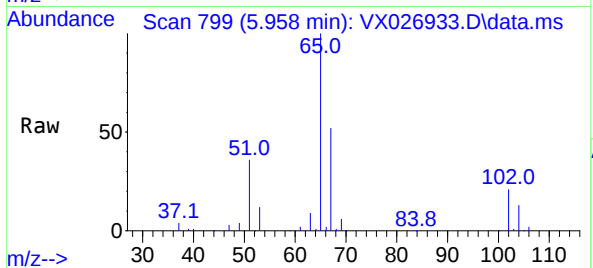

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.006 min

Lab File: VX026933.D

Acq: 10 Feb 2022 20:13




Tgt Ion: 114 Resp: 195253


Ion Ratio Lower Upper

114 100

63 21.1 0.0 42.8

88 16.5 0.0 33.0


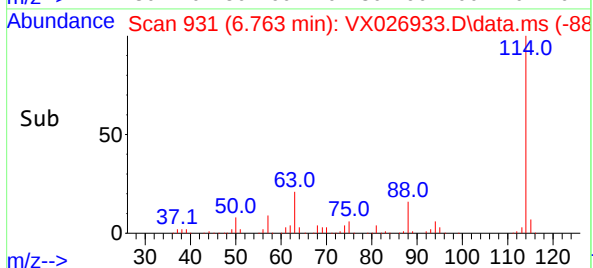
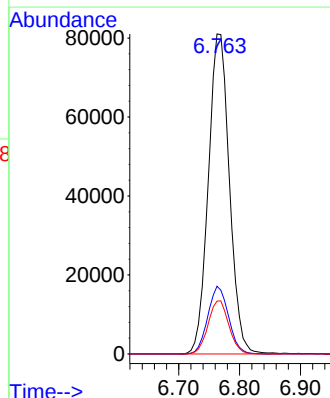



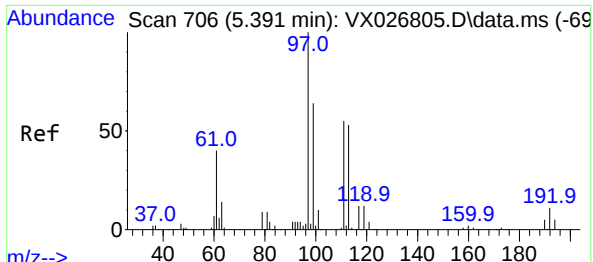

#35
Dibromofluoromethane
Concen: 52.602 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13




Instrument :
MSVOA_X
ClientSampleId :
20422DL


Tgt Ion:	113	Resp:	61191
Ion	Ratio	Lower	Upper
113	100		
111	101.3	81.2	121.8
192	19.1	15.0	22.4

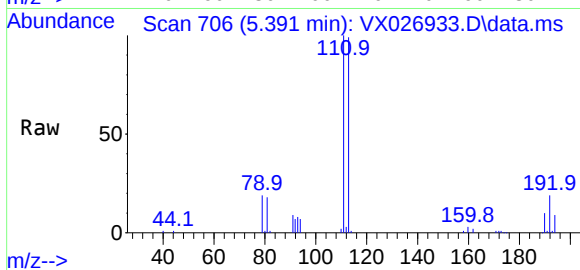

#36
1,1-Dichloropropene
Concen: 4.891 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.140 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13

Tgt Ion:	75	Resp:	8975
Ion	Ratio	Lower	Upper
75	100		
110	9.3	17.2	51.6#
77	0.0	24.6	36.8#

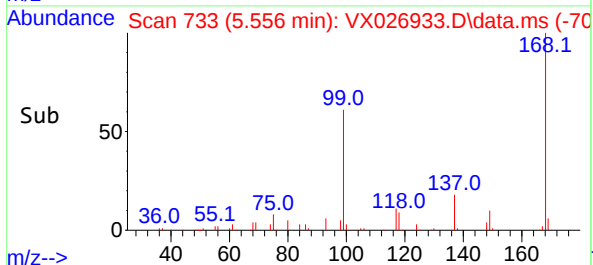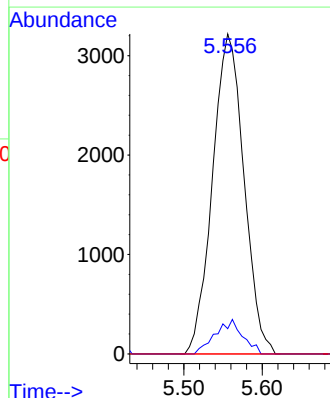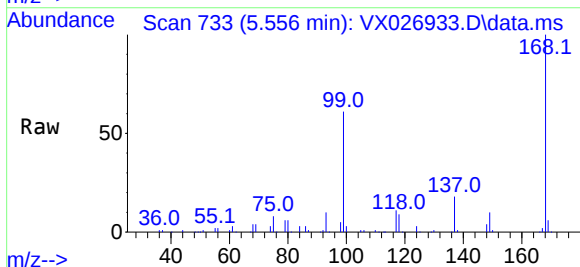



#37

Ethyl Acetate

Concen: 2.023 ug/l

RT: 4.568 min Scan# 51

Delta R.T. -0.146 min

Lab File: VX026933.D

Acq: 10 Feb 2022 20:13

Instrument :

MSVOA_X

ClientSampleId :

20422DL





Tgt Ion: 43 Resp: 4220

Ion Ratio Lower Upper

43 100

61 0.0 10.6 16.0#

70 0.0 8.5 12.7#

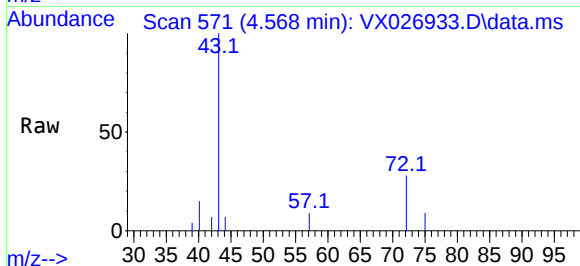

#38

Carbon Tetrachloride

Concen: 6.379 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.128 min

Lab File: VX026933.D

Acq: 10 Feb 2022 20:13




Tgt Ion: 117 Resp: 12275


Ion Ratio Lower Upper

117 100

119 4.0 74.7 112.1#


121 0.0 25.4 38.0#

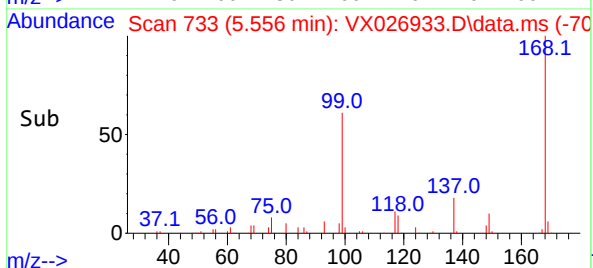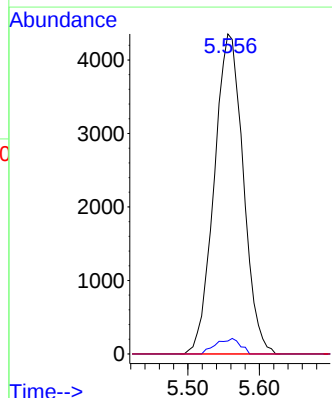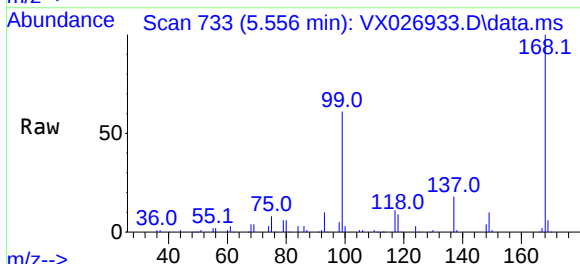






#40
Benzene
Concen: 24.683 ug/l
RT: 6.044 min Scan# 813
Delta R.T. 0.000 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13

Instrument :
MSVOA_X
ClientSampleId :
20422DL



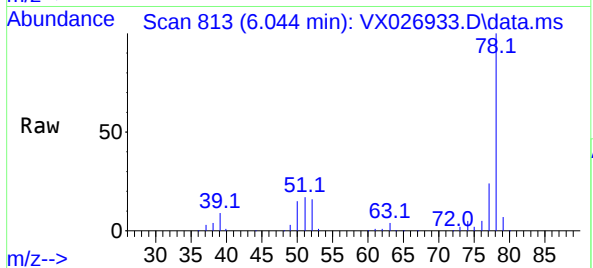



Tgt Ion: 78 Resp: 132016
Ion Ratio Lower Upper
78 100
77 23.8 18.9 28.3

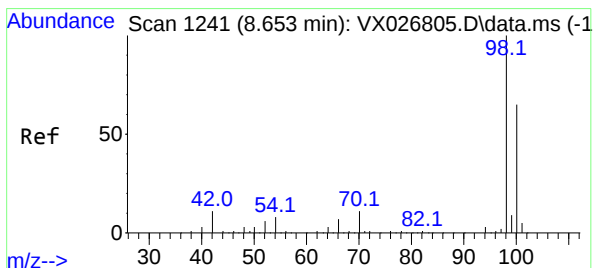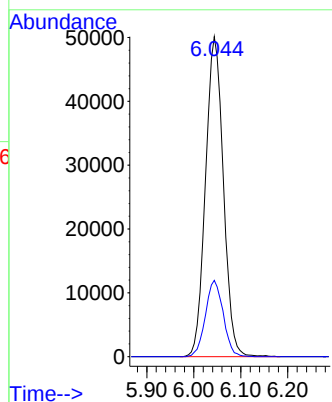

#50
Toluene-d8
Concen: 53.938 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13

Tgt Ion: 98 Resp: 230320
Ion Ratio Lower Upper
98 100
100 66.2 53.2 79.8

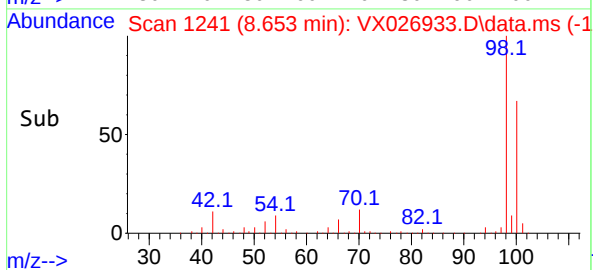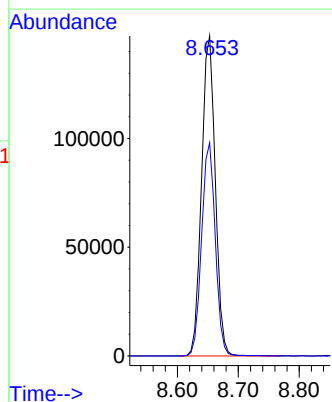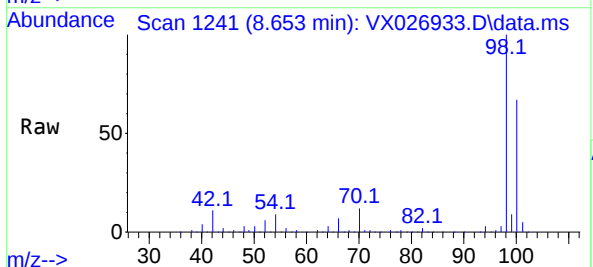



#51

4-Methyl-2-Pentanone

Concen: 0.278 ug/l

RT: 8.580 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX026933.D

Acq: 10 Feb 2022 20:13

Instrument :

MSVOA_X

ClientSampleId :





20422DL

Tgt Ion: 43 Resp: 541

Ion Ratio Lower Upper

43 100

58 34.2 30.5 45.7

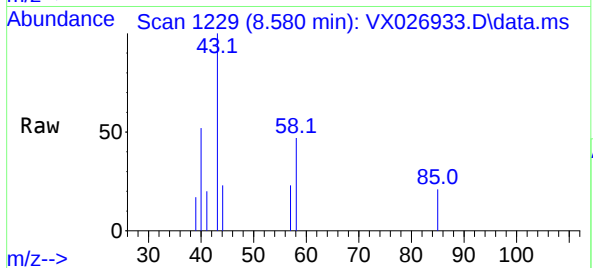

#52

Toluene

Concen: 20.005 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. 0.000 min

Lab File: VX026933.D




Acq: 10 Feb 2022 20:13


Tgt Ion: 92 Resp: 67742

Ion Ratio Lower Upper

92 100

91 170.3 135.7 203.5

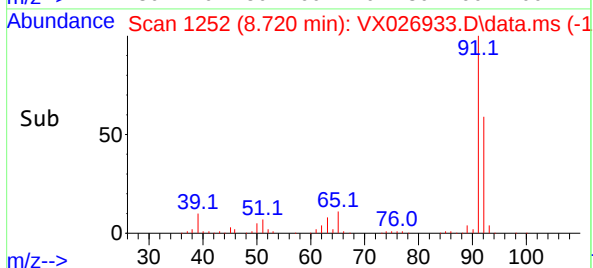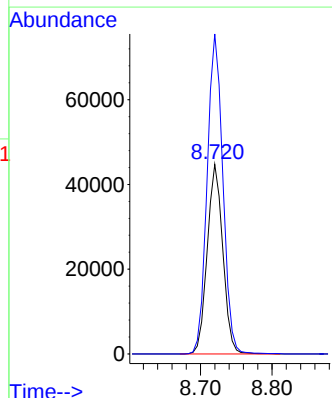



#53

t-1,3-Dichloropropene

Concen: 1.732 ug/l

RT: 8.720 min Scan# 11

Delta R.T. -0.262 min

Lab File: VX026933.D

Acq: 10 Feb 2022 20:13

Instrument :

MSVOA_X

ClientSampleId :





20422DL

Tgt Ion: 75 Resp: 763

Ion Ratio Lower Upper

75 100

77 150.2 25.7 38.5#

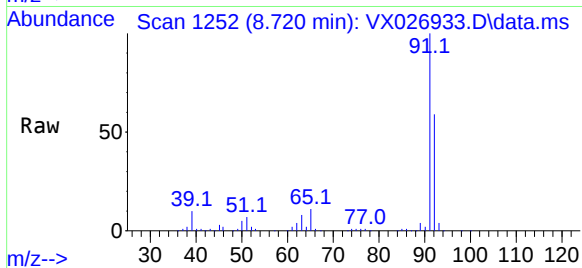

#62

4-Bromofluorobenzene

Concen: 57.543 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX026933.D

Acq: 10 Feb 2022 20:13




Tgt Ion: 95 Resp: 86507


Ion Ratio Lower Upper

95 100

174 74.8 0.0 148.6

176 72.8 0.0 141.4


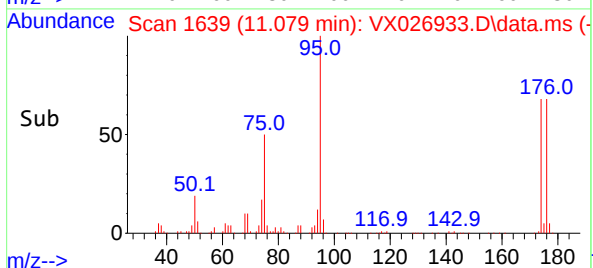
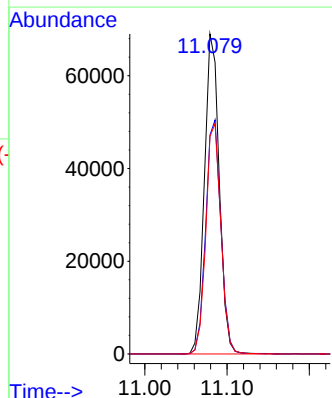
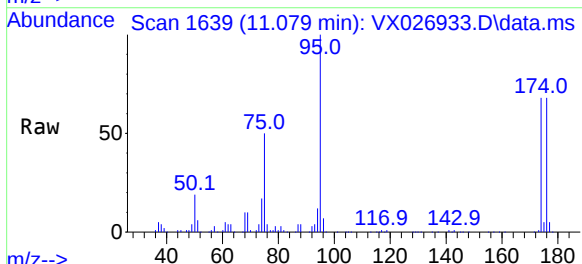




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13




Instrument :
MSVOA_X
ClientSampleId :
20422DL


Tgt Ion:117 Resp: 180836
Ion Ratio Lower Upper
117 100
82 55.8 45.2 67.8
119 31.8 26.2 39.2

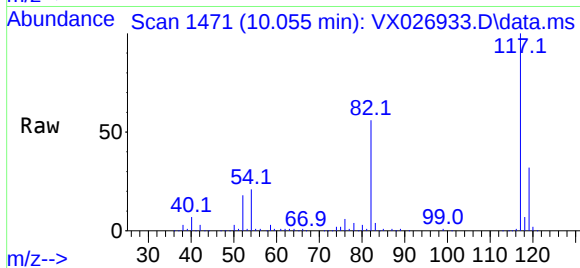

#67
Ethyl Benzene
Concen: 2.198 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13

Tgt Ion: 91 Resp: 14550
Ion Ratio Lower Upper
91 100
106 28.7 24.7 37.1


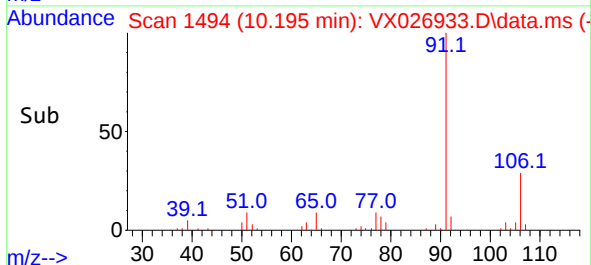
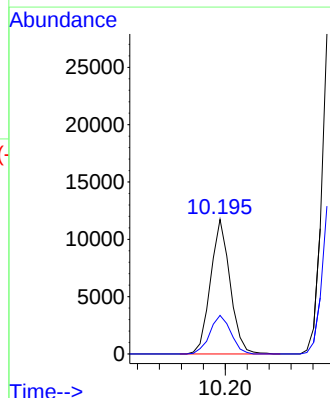
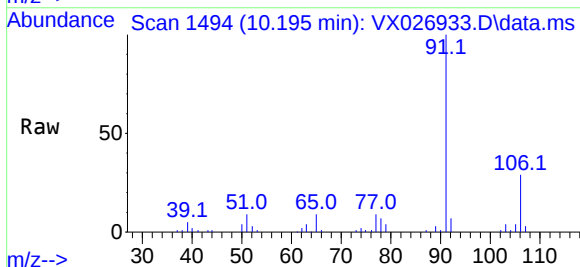




#68
m/p-Xylenes
Concen: 10.788 ug/l
RT: 10.299 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13




Instrument :
MSVOA_X
ClientSampleId :
20422DL


Tgt Ion:106 Resp: 27473
Ion Ratio Lower Upper
106 100
91 206.2 165.3 247.9

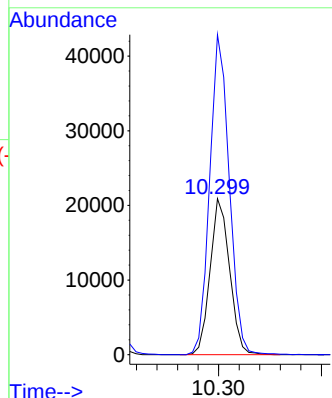

#69
o-Xylene
Concen: 9.256 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.006 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13

Tgt Ion:106 Resp: 23097
Ion Ratio Lower Upper
106 100
91 218.2 109.7 329.0


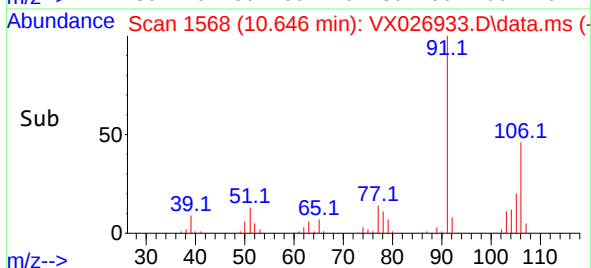






#70
Styrene
Concen: 3.249 ug/l
RT: 10.659 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13




Instrument :
MSVOA_X
ClientSampleId :
20422DL


Tgt Ion:104 Resp: 13151
Ion Ratio Lower Upper
104 100
78 65.4 42.5 63.7#
103 67.3 43.3 64.9#

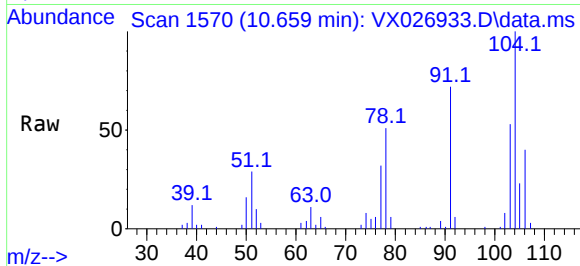

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13

Tgt Ion:152 Resp: 78948
Ion Ratio Lower Upper
152 100
115 60.6 44.2 132.6
150 156.1 0.0 348.2


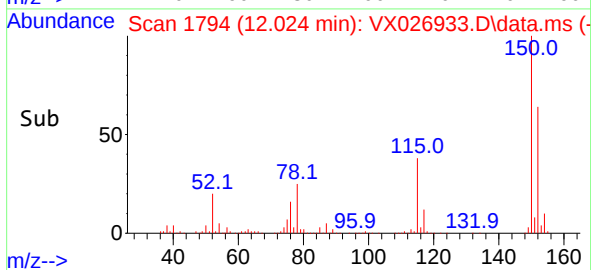

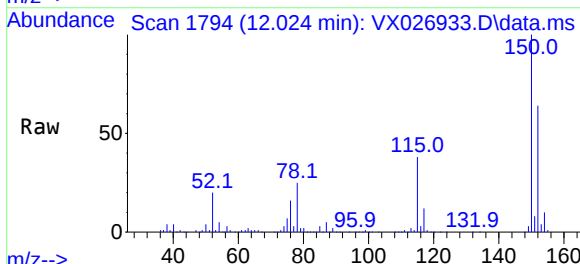




#73
Isopropylbenzene
Concen: 0.346 ug/l
RT: 10.963 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13




Instrument :
MSVOA_X
ClientSampleId :
20422DL


Tgt Ion:105 Resp: 2150
Ion Ratio Lower Upper
105 100
120 25.0 13.1 39.1

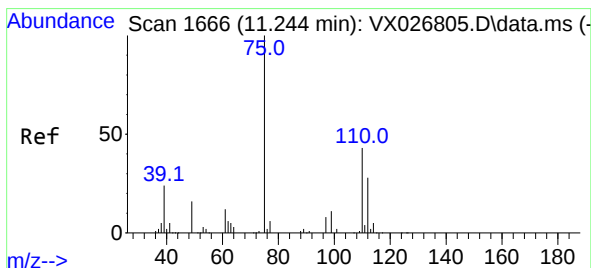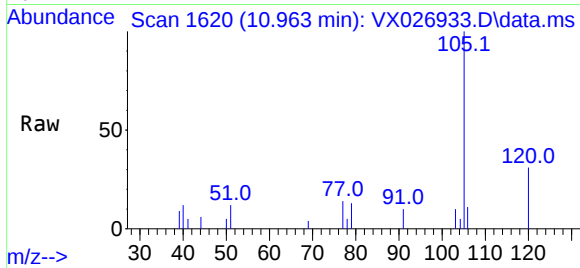

#76
1,2,3-Trichloropropane
Concen: 24.719 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13

Tgt Ion: 75 Resp: 42720
Ion Ratio Lower Upper
75 100
77 1.2 18.3 54.8#


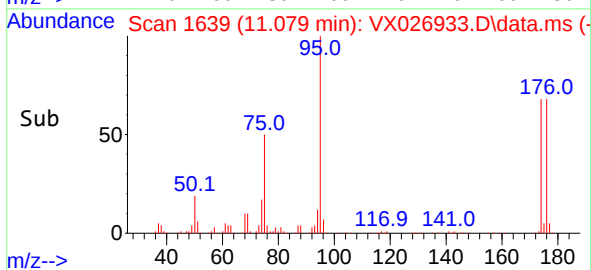

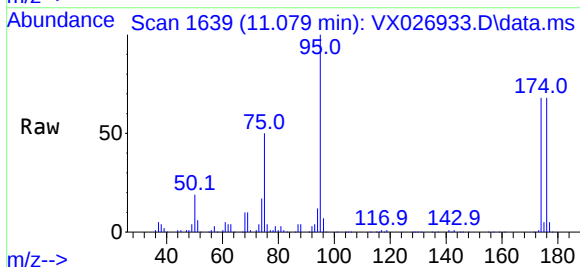




#78
n-propylbenzene
Concen: 1.026 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.000 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13




Instrument :
MSVOA_X
ClientSampleId :
20422DL


Tgt Ion: 91 Resp: 7074
Ion Ratio Lower Upper
91 100
120 21.4 11.6 34.7

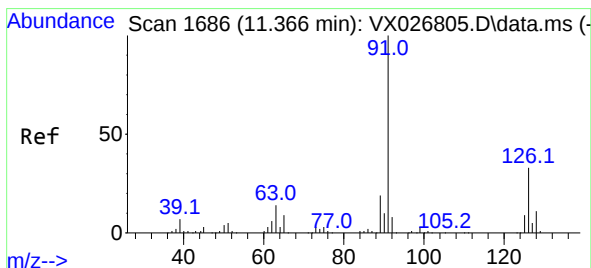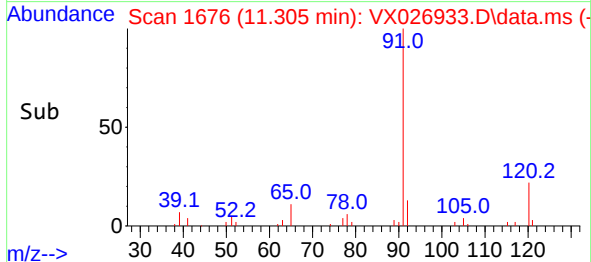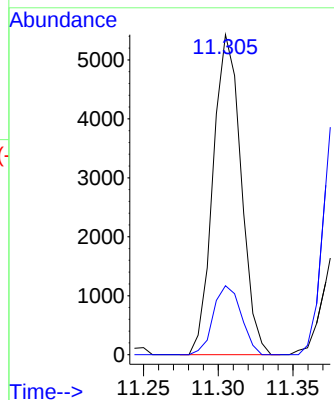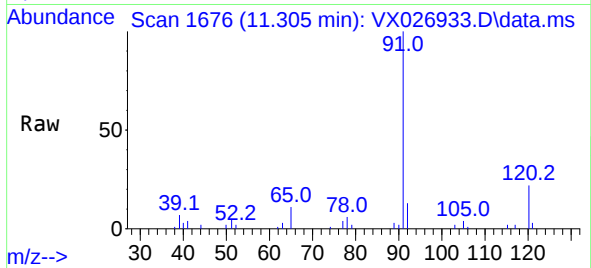

#79
2-Chlorotoluene
Concen: 0.850 ug/l
RT: 11.384 min Scan# 1689
Delta R.T. 0.018 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13

Tgt Ion: 91 Resp: 3620
Ion Ratio Lower Upper
91 100
126 0.0 16.4 49.2#


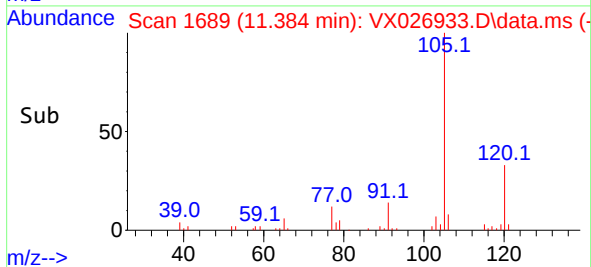
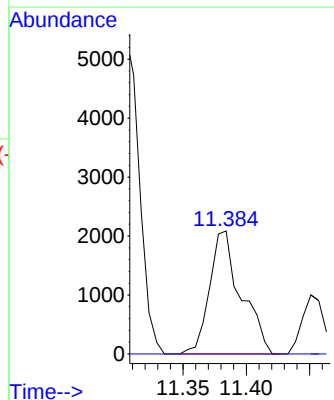
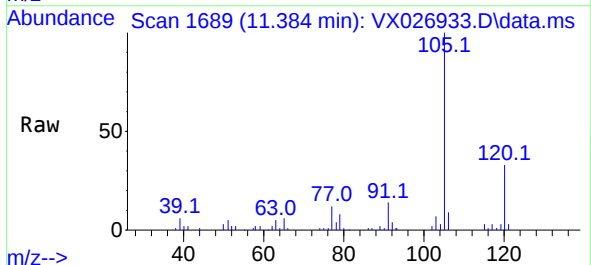




#80
1,3,5-Trimethylbenzene
Concen: 2.117 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13




Instrument :
MSVOA_X
ClientSampleId :
20422DL


Tgt Ion:105 Resp: 10833
Ion Ratio Lower Upper
105 100
120 49.7 24.0 72.0

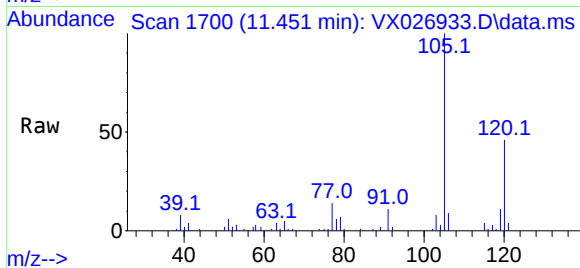

#81
trans-1,4-Dichloro-2-butene
Concen: 75.437 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13

Tgt Ion: 75 Resp: 42720
Ion Ratio Lower Upper
75 100
53 0.0 94.0 141.0#
89 0.0 37.0 55.4#


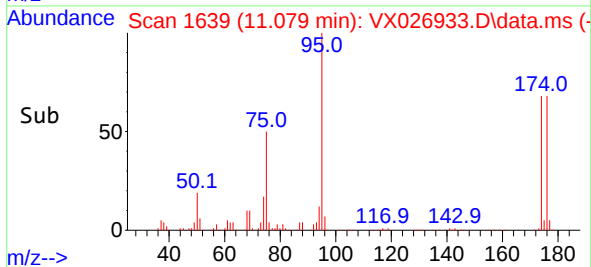

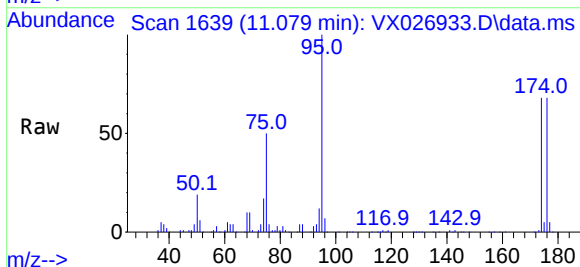




#82
4-Chlorotoluene
Concen: 0.250 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13




Instrument :
MSVOA_X
ClientSampleId :
20422DL


Tgt Ion: 91 Resp: 1194
Ion Ratio Lower Upper
91 100
126 0.0 14.1 42.4#

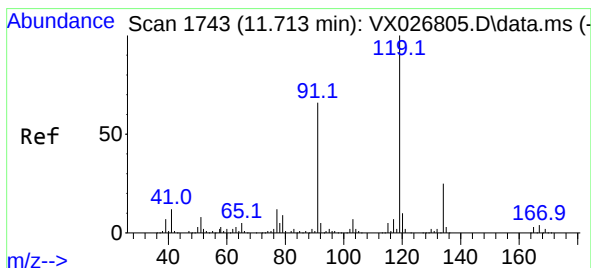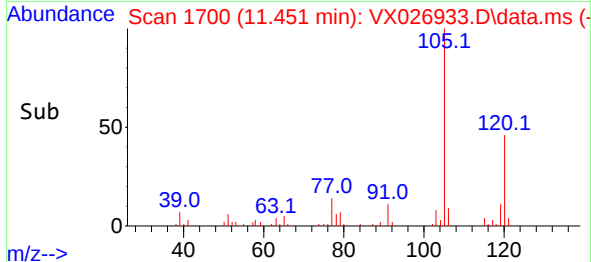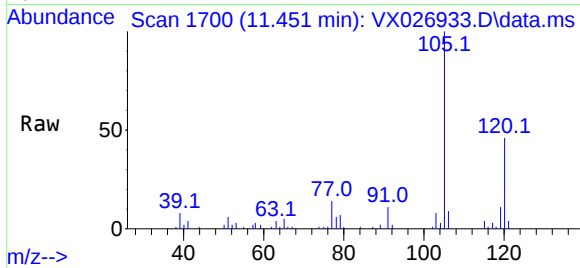

#83
tert-Butylbenzene
Concen: 1.051 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.043 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13

Tgt Ion: 119 Resp: 5127
Ion Ratio Lower Upper
119 100
91 87.3 31.4 94.0
134 0.0 11.8 35.3#


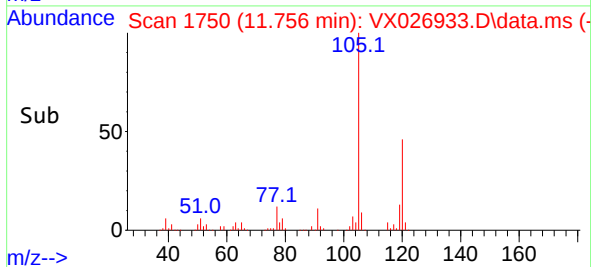

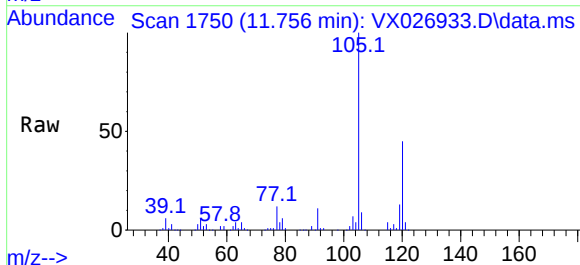




#84
1,2,4-Trimethylbenzene
Concen: 8.203 ug/l
RT: 11.756 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13




Instrument :
MSVOA_X
ClientSampleId :
20422DL


Tgt Ion:105 Resp: 42345
Ion Ratio Lower Upper
105 100
120 44.7 21.9 65.5

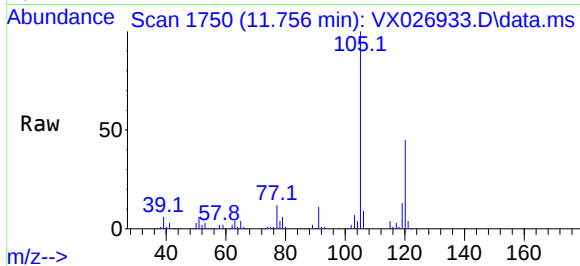

#85
sec-Butylbenzene
Concen: 0.389 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. 0.000 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13

Tgt Ion:105 Resp: 2403
Ion Ratio Lower Upper
105 100
134 25.5 10.1 30.1

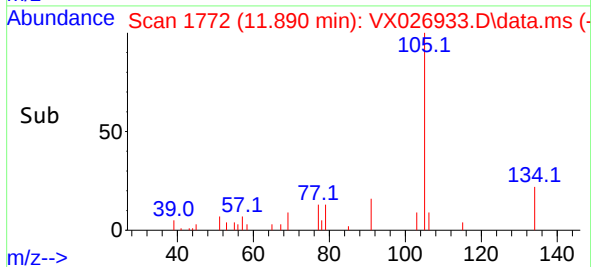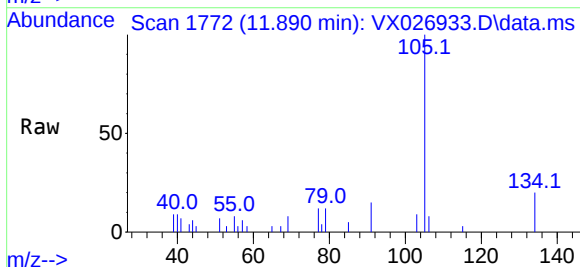







#86
p-Isopropyltoluene
Concen: 0.588 ug/l
RT: 11.969 min Scan# 11
Delta R.T. -0.043 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13

Instrument :
MSVOA_X
ClientSampleId :
20422DL

Tgt Ion:119 Resp: 3079




Ion	Ratio	Lower	Upper
119	100		
134	27.0	13.0	39.0
91	26.6	12.6	37.6

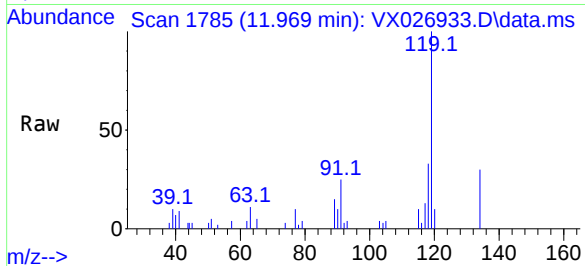


#89
n-Butylbenzene
Concen: 1.017 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13

Tgt Ion: 91 Resp: 4360

Ion	Ratio	Lower	Upper
91	100		
92	37.6	27.2	81.6
134	90.8	13.1	39.1#


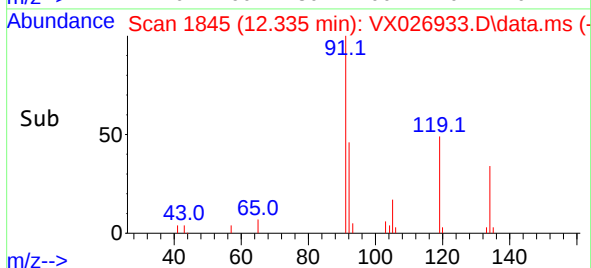
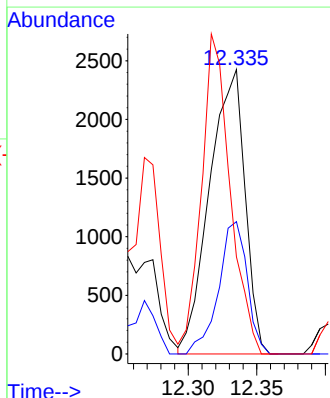
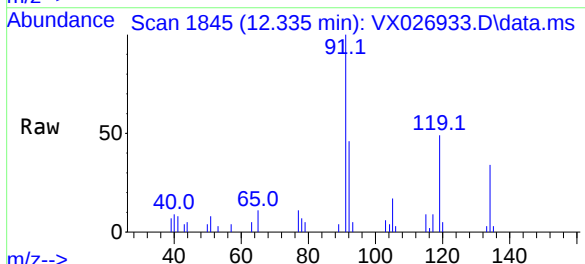




#90
Hexachloroethane
Concen: 0.818 ug/l
RT: 12.530 min Scan# 117
Delta R.T. -0.012 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13

Instrument :
MSVOA_X
ClientSampleId :
20422DL

Tgt Ion:117 Resp: 619
Ion Ratio Lower Upper
117 100
201 0.0 35.6 106.8#

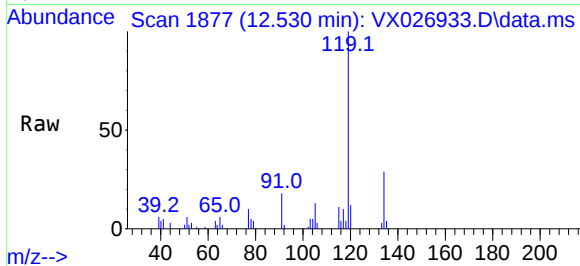

#95
Naphthalene
Concen: 16.449 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX026933.D
Acq: 10 Feb 2022 20:13

Tgt Ion:128 Resp: 95034
Ion Ratio Lower Upper
128 100
127 12.8 10.3 15.5
129 10.7 8.7 13.1

