

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
 Data File : VX026934.D
 Acq On : 10 Feb 2022 20:36
 Operator : JC/MD
 Sample : N1425-03 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 31377

Quant Time: Feb 11 04:03:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 08 07:07:46 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	121359	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	206805	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	185907	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	81554	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	80538	55.284	ug/l	0.00
Spiked Amount 50.000	Range	78 - 117	Recovery	=	110.560%	
35) Dibromofluoromethane	5.391	113	64339	52.219	ug/l	0.00
Spiked Amount 50.000	Range	75 - 124	Recovery	=	104.440%	
50) Toluene-d8	8.653	98	241562	53.411	ug/l	0.00
Spiked Amount 50.000	Range	92 - 112	Recovery	=	106.820%	
62) 4-Bromofluorobenzene	11.079	95	88382	55.506	ug/l	0.00
Spiked Amount 50.000	Range	83 - 123	Recovery	=	111.020%	
Target Compounds						Qvalue
11) Tert butyl alcohol	2.959	59	69	0.262	ug/l #	75
16) Acetone	2.386	43	16126	25.203	ug/l	96
18) Methyl Acetate	2.703	43	503	0.273	ug/l #	53
25) 2-Butanone	4.574	43	1076	1.044	ug/l	92
29) Tetrahydrofuran	5.025	42	234	0.334	ug/l #	56
31) Cyclohexane	5.489	56	823	0.356	ug/l #	85
36) 1,1-Dichloropropene	5.562	75	9437	4.855	ug/l #	51
37) Ethyl Acetate	4.574	43	1076	0.487	ug/l #	69
38) Carbon Tetrachloride	5.556	117	12596	6.180	ug/l #	18
39) Methylcyclohexane	7.379	83	3968	1.665	ug/l	89
40) Benzene	6.050	78	5526	0.975	ug/l	95
48) Methyl methacrylate	7.659	41	461	0.274	ug/l #	63
51) 4-Methyl-2-Pentanone	8.580	43	524	0.254	ug/l #	64
52) Toluene	8.720	92	32534	9.071	ug/l	100
53) t-1,3-Dichloropropene	8.720	75	323	1.503	ug/l #	1
55) 1,1,2-Trichloroethane	9.104	97	1602	1.180	ug/l #	19
59) 2-Hexanone	9.384	43	307	0.204	ug/l #	25
67) Ethyl Benzene	10.195	91	28292	4.158	ug/l	97
68) m/p-Xylenes	10.305	106	34622	13.224	ug/l	100
69) o-Xylene	10.640	106	19710	7.683	ug/l	97
70) Styrene	10.646	104	1171	0.281	ug/l #	1
73) Isopropylbenzene	10.963	105	6154	0.958	ug/l	98
76) 1,2,3-Trichloropropane	11.079	75	43601	24.423	ug/l #	40
78) n-propylbenzene	11.305	91	19550	2.745	ug/l	99
79) 2-Chlorotoluene	11.378	91	8846	2.010	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.451	105	20655	3.907	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.079	75	43601	74.574	ug/l #	3
82) 4-Chlorotoluene	11.451	91	2309	0.468	ug/l #	46
83) tert-Butylbenzene	11.756	119	9519	1.889	ug/l #	62
84) 1,2,4-Trimethylbenzene	11.756	105	80356	15.068	ug/l	98
85) sec-Butylbenzene	11.890	105	6623	1.037	ug/l	87
86) p-Isopropyltoluene	12.012	119	3719	0.687	ug/l	92
89) n-Butylbenzene	12.329	91	12223	2.761	ug/l #	50
90) Hexachloroethane	12.530	117	1236	1.580	ug/l #	14
92) 1,2-Dibromo-3-Chloropr...	12.963	75	101	0.236	ug/l #	3
95) Naphthalene	13.780	128	9683	1.622	ug/l #	94

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
Data File : VX026934.D
Acq On : 10 Feb 2022 20:36
Operator : JC/MD
Sample : N1425-03 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
31377

Quant Time: Feb 11 04:03:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 08 07:07:46 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
Data File : VX026934.D
Acq On : 10 Feb 2022 20:36
Operator : JC/MD
Sample : N1425-03 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
31377

Quant Time: Feb 11 04:03:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 08 07:07:46 2022
Response via : Initial Calibration




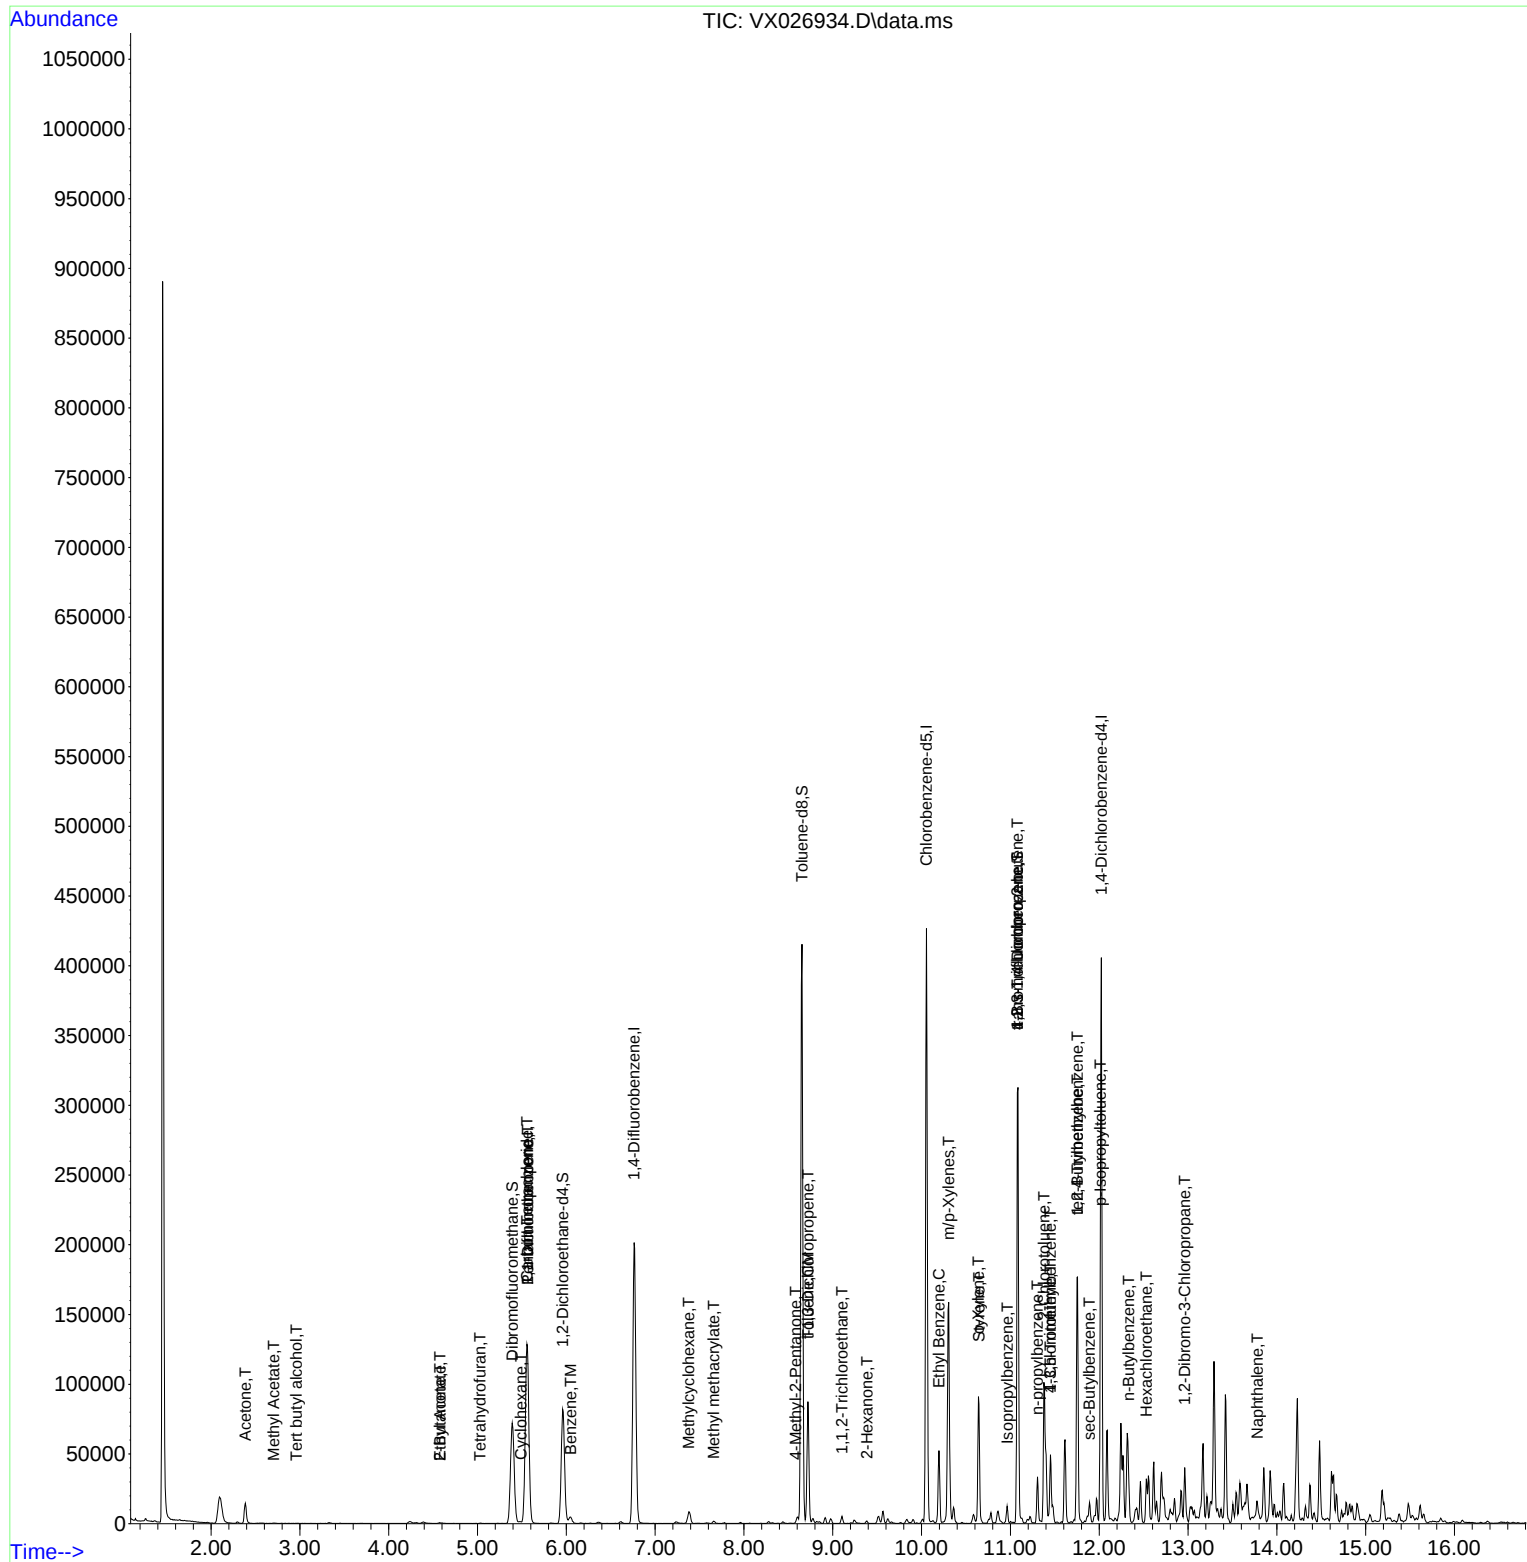


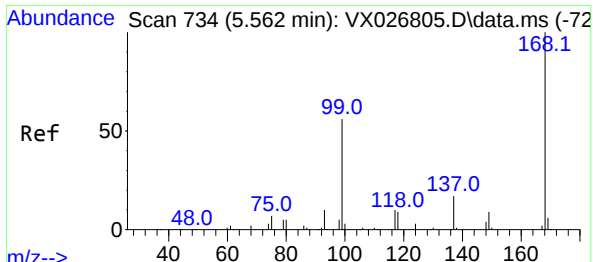

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36




Instrument :
MSVOA_X
ClientSampleId :
31377


Tgt Ion:168 Resp: 121359
Ion Ratio Lower Upper
168 100
99 59.8 50.3 75.5

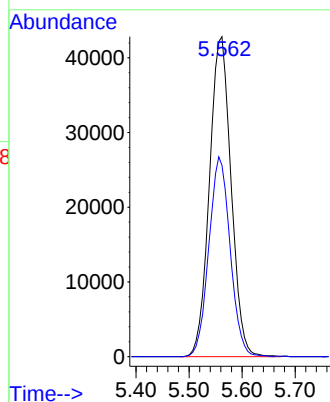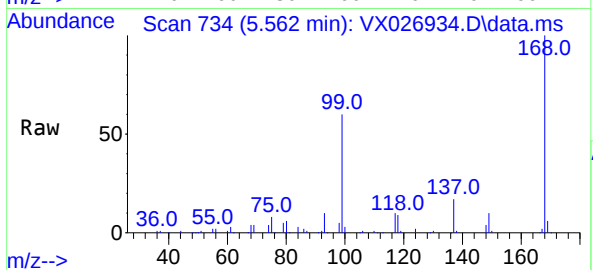

#11
Tert butyl alcohol
Concen: 0.262 ug/l
RT: 2.959 min Scan# 307
Delta R.T. -0.042 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Tgt Ion: 59 Resp: 69
Ion Ratio Lower Upper
59 100
57 0.0 7.2 10.8#

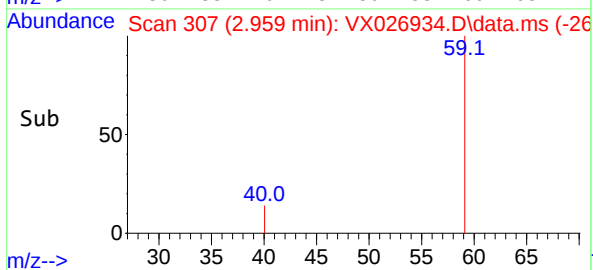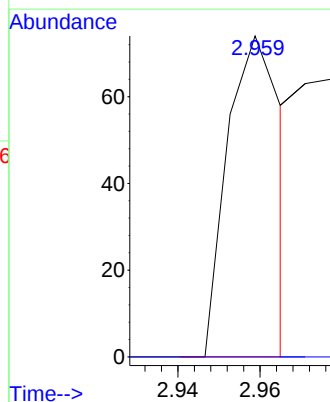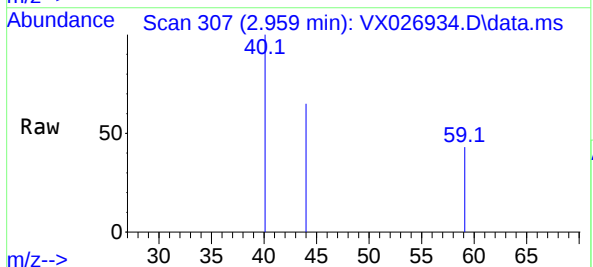



#16

Acetone

Concen: 25.203 ug/l

RT: 2.386 min Scan# 21

Delta R.T. 0.000 min

Lab File: VX026934.D

Acq: 10 Feb 2022 20:36

Instrument :

MSVOA_X

ClientSampleId :





31377

Tgt Ion: 43 Resp: 16126

Ion Ratio Lower Upper

43 100

58 30.7 23.0 34.6

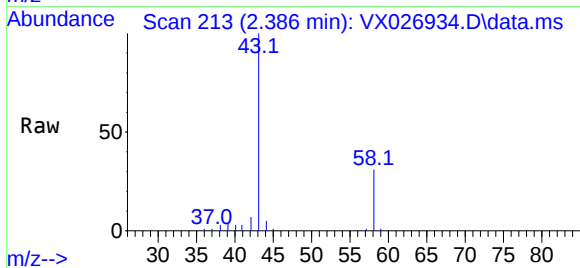

#18

Methyl Acetate

Concen: 0.273 ug/l

RT: 2.703 min Scan# 265

Delta R.T. -0.006 min

Lab File: VX026934.D




Acq: 10 Feb 2022 20:36


Tgt Ion: 43 Resp: 503

Ion Ratio Lower Upper

43 100

74 0.0 18.3 27.5#

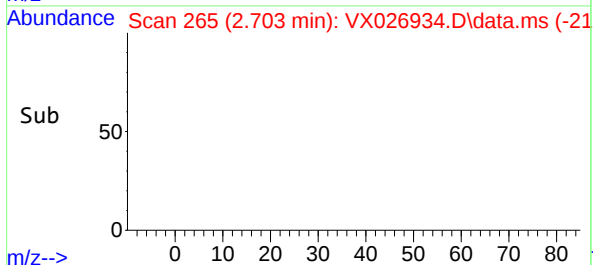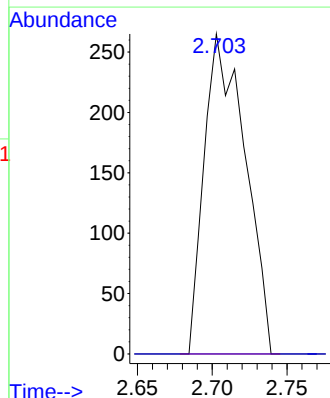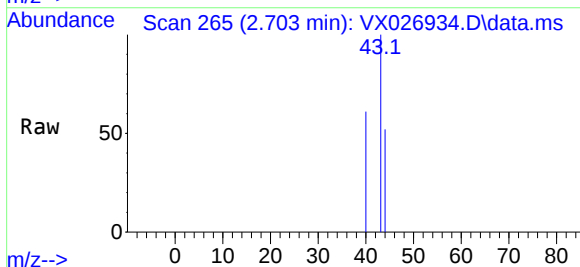



#25

2-Butanone

Concen: 1.044 ug/l

RT: 4.574 min Scan# 51

Delta R.T. 0.012 min

Lab File: VX026934.D

Acq: 10 Feb 2022 20:36

Instrument :

MSVOA_X

ClientSampleId :





31377

Tgt Ion: 43 Resp: 1076

Ion Ratio Lower Upper

43 100

72 29.5 20.4 30.6



#29

Tetrahydrofuran

Concen: 0.334 ug/l

RT: 5.025 min Scan# 646

Delta R.T. 0.018 min

Lab File: VX026934.D

Acq: 10 Feb 2022 20:36




Tgt Ion: 42 Resp: 234


Ion Ratio Lower Upper

42 100

72 19.2 34.6 52.0#


71 8.5 31.8 47.8#

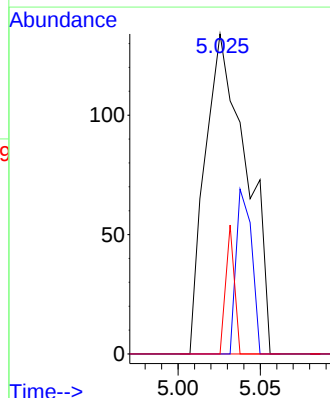






#31
Cyclohexane
Concen: 0.356 ug/l
RT: 5.489 min Scan# 713
Delta R.T. 0.012 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Instrument :
MSVOA_X
ClientSampleId :
31377



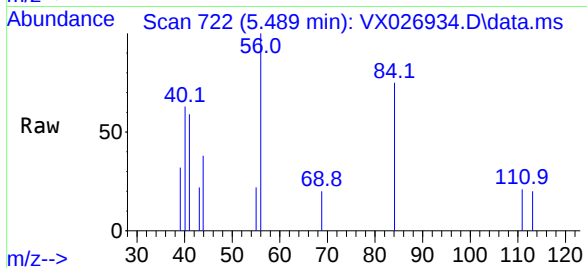



Tgt Ion: 56 Resp: 823
Ion Ratio Lower Upper
56 100
69 20.2 25.8 38.6#
84 75.0 68.9 103.3

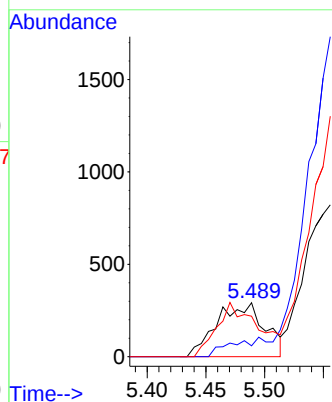

#33
1,2-Dichloroethane-d4
Concen: 55.284 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.006 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Tgt Ion: 65 Resp: 80538
Ion Ratio Lower Upper
65 100
67 50.7 0.0 100.8


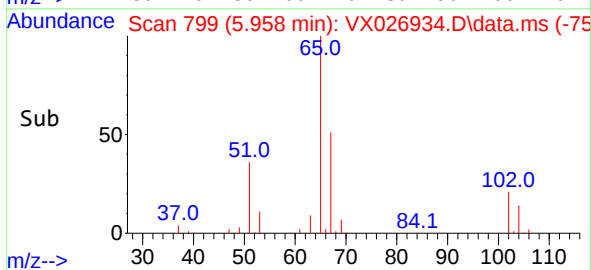
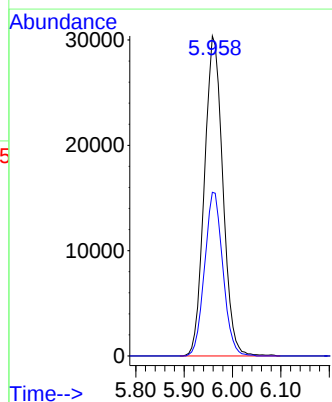
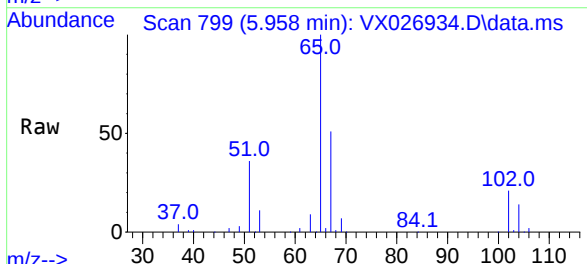




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36




Instrument :
MSVOA_X
ClientSampleId :
31377


Tgt Ion:114 Resp: 206805
Ion Ratio Lower Upper
114 100
63 21.6 0.0 42.8
88 16.2 0.0 33.0

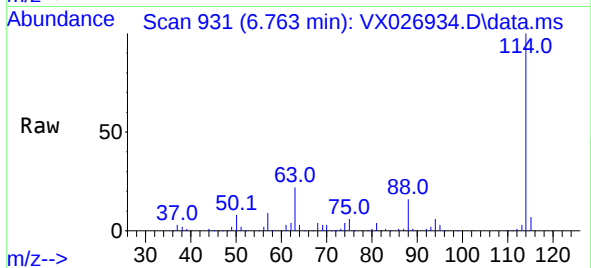

#35
Dibromofluoromethane
Concen: 52.219 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36


Tgt Ion:113 Resp: 64339
Ion Ratio Lower Upper
113 100
111 102.2 81.2 121.8
192 19.1 15.0 22.4

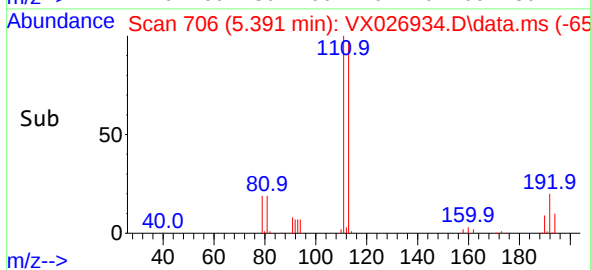






#36
1,1-Dichloropropene
Concen: 4.855 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Instrument :
MSVOA_X
ClientSampleId :
31377



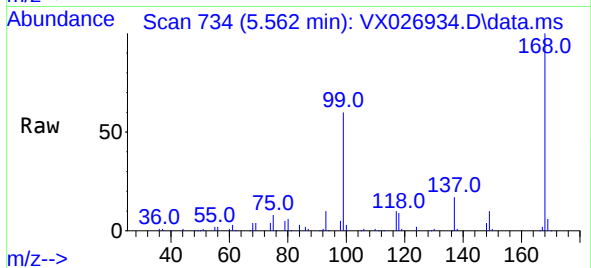



Tgt Ion: 75 Resp: 9437
Ion Ratio Lower Upper
75 100
110 9.4 17.2 51.6#
77 0.0 24.6 36.8#



#37
Ethyl Acetate
Concen: 0.487 ug/l
RT: 4.574 min Scan# 572
Delta R.T. -0.140 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Tgt Ion: 43 Resp: 1076
Ion Ratio Lower Upper
43 100
61 0.0 10.6 16.0#
70 0.0 8.5 12.7#


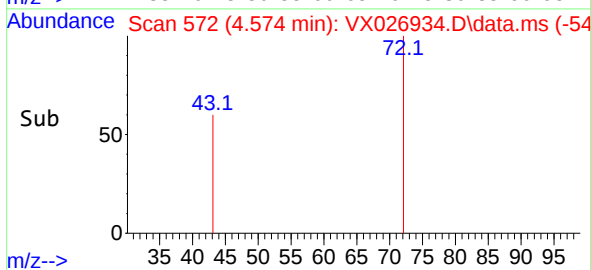




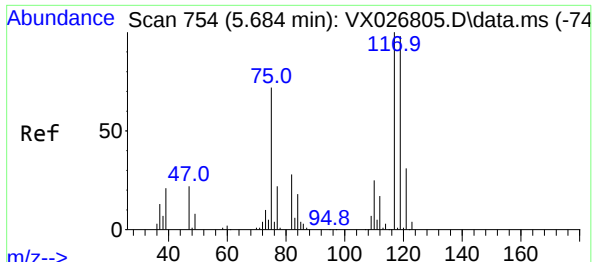

#38
Carbon Tetrachloride
Concen: 6.180 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36




Instrument :
MSVOA_X
ClientSampleId :
31377


Tgt Ion:117 Resp: 12596
Ion Ratio Lower Upper
117 100
119 5.8 74.7 112.1#
121 0.0 25.4 38.0#

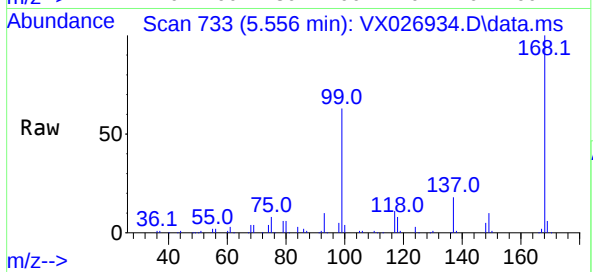

#39
Methylcyclohexane
Concen: 1.665 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. -0.006 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Tgt Ion: 83 Resp: 3968
Ion Ratio Lower Upper
83 100
55 66.6 63.6 95.4
98 45.3 38.4 57.6


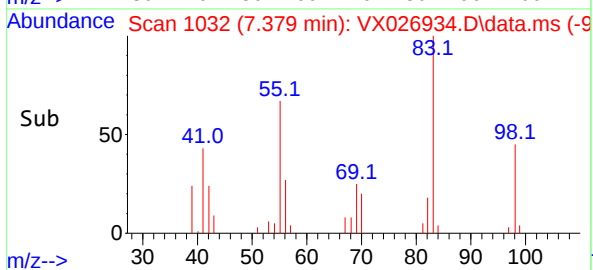

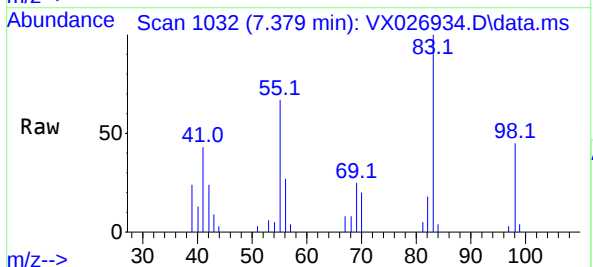




#40
Benzene
Concen: 0.975 ug/l
RT: 6.050 min Scan# 813
Delta R.T. 0.006 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36




Instrument :
MSVOA_X
ClientSampleId :
31377


Tgt Ion: 78 Resp: 5526
Ion Ratio Lower Upper
78 100
77 21.3 18.9 28.3

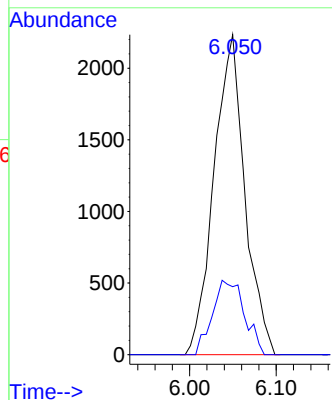

#48
Methyl methacrylate
Concen: 0.274 ug/l
RT: 7.659 min Scan# 1078
Delta R.T. -0.036 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Tgt Ion: 41 Resp: 461
Ion Ratio Lower Upper
41 100
69 118.4 62.2 93.4#
39 39.9 45.4 68.0#


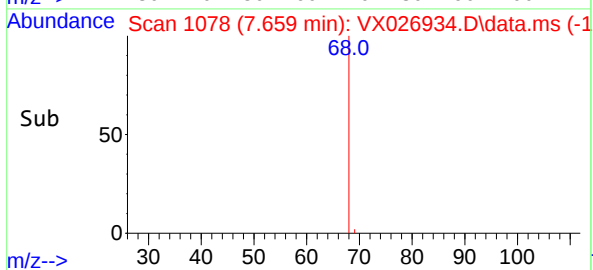
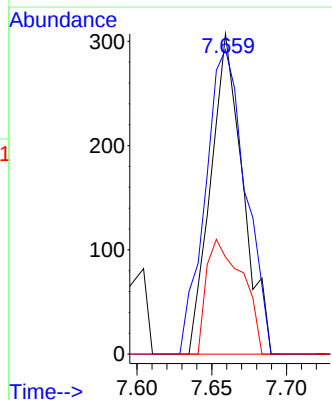





#50
Toluene-d8
Concen: 53.411 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36




Instrument :
MSVOA_X
ClientSampleId :
31377


Tgt Ion: 98 Resp: 241562
Ion Ratio Lower Upper
98 100
100 66.1 53.2 79.8

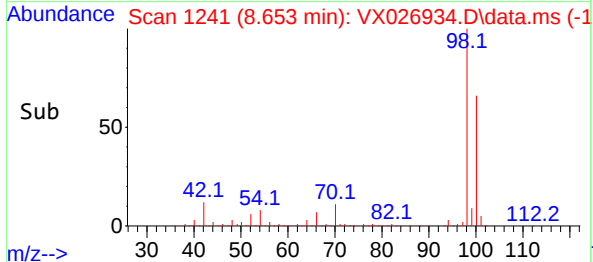

#51
4-Methyl-2-Pentanone
Concen: 0.254 ug/l
RT: 8.580 min Scan# 1229
Delta R.T. 0.006 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Tgt Ion: 43 Resp: 524
Ion Ratio Lower Upper
43 100
58 16.6 30.5 45.7#


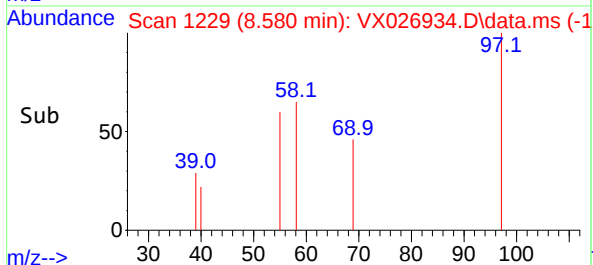

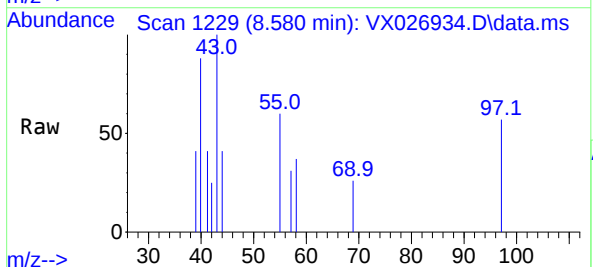




#52
Toluene
Concen: 9.071 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36




Instrument :
MSVOA_X
ClientSampleId :
31377


Tgt Ion: 92 Resp: 32534
Ion Ratio Lower Upper
92 100
91 169.2 135.7 203.5



#53
t-1,3-Dichloropropene
Concen: 1.503 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.262 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Tgt Ion: 75 Resp: 323
Ion Ratio Lower Upper
75 100
77 176.7 25.7 38.5#

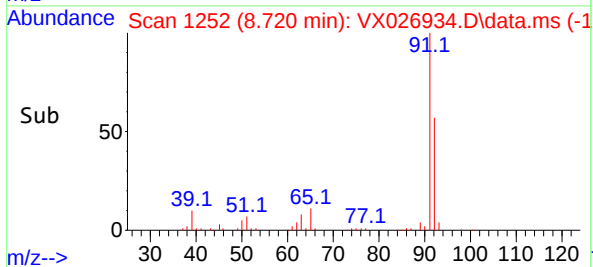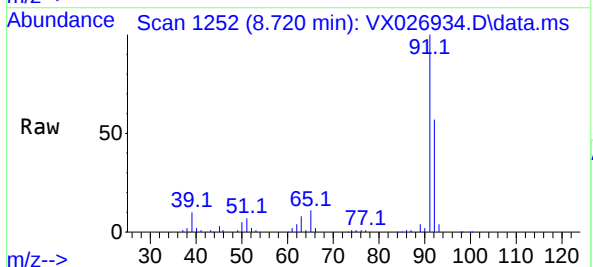







#55
1,1,2-Trichloroethane
Concen: 1.180 ug/l
RT: 9.104 min Scan# 11
Delta R.T. -0.049 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Instrument :
MSVOA_X
ClientSampleId :
31377

Tgt Ion: 97 Resp: 1602




Ion	Ratio	Lower	Upper
97	100		
83	8.7	68.4	102.6#
85	0.0	44.0	66.0#
99	0.0	49.8	74.6#




#59
2-Hexanone
Concen: 0.204 ug/l
RT: 9.384 min Scan# 1361
Delta R.T. -0.049 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Tgt Ion: 43 Resp: 307

Ion	Ratio	Lower	Upper
43	100		
58	0.0	26.4	79.2#



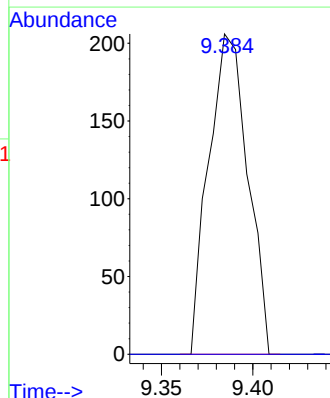





#62
4-Bromofluorobenzene
Concen: 55.506 ug/l
RT: 11.079 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36




Instrument :
MSVOA_X
ClientSampleId :
31377


Tgt Ion: 95 Resp: 88382
Ion Ratio Lower Upper
95 100
174 74.3 0.0 148.6
176 71.4 0.0 141.4

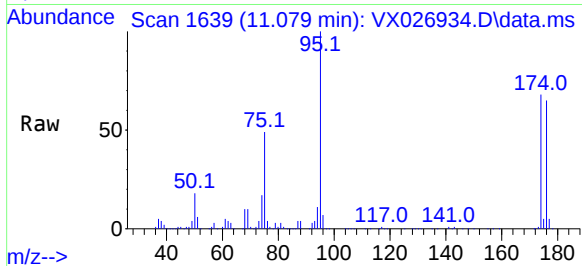

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Tgt Ion: 117 Resp: 185907
Ion Ratio Lower Upper
117 100
82 56.4 45.2 67.8
119 32.5 26.2 39.2

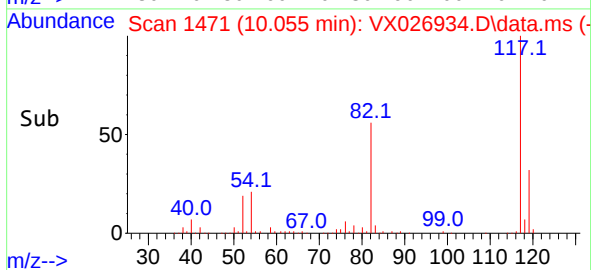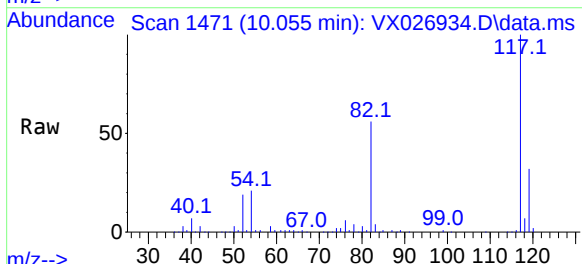



#67

Ethyl Benzene

Concen: 4.158 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX026934.D

Acq: 10 Feb 2022 20:36

Instrument :

MSVOA_X

ClientSampleId :





31377

Tgt Ion: 91 Resp: 28292

Ion Ratio Lower Upper

91 100

106 32.8 24.7 37.1

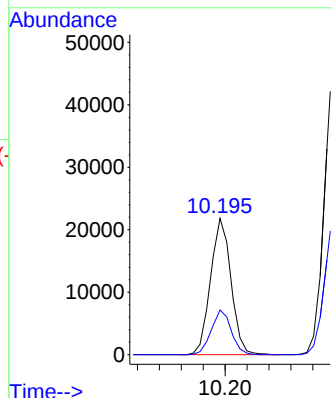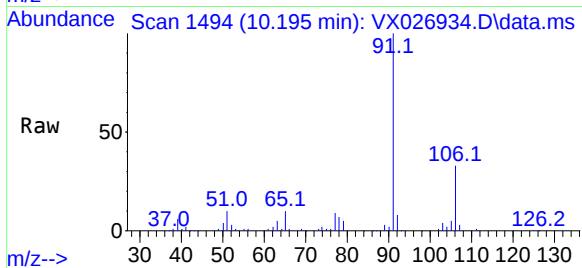

#68

m/p-Xylenes

Concen: 13.224 ug/l

RT: 10.305 min Scan# 1512

Delta R.T. 0.000 min

Lab File: VX026934.D




Acq: 10 Feb 2022 20:36


Tgt Ion: 106 Resp: 34622

Ion Ratio Lower Upper

106 100

91 206.4 165.3 247.9


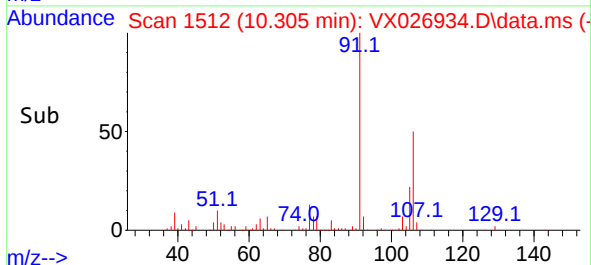
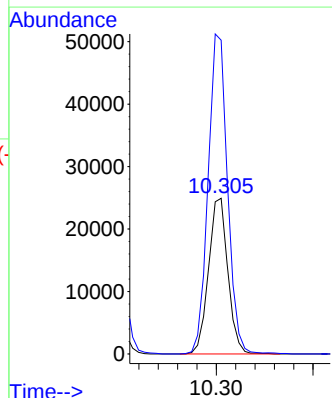
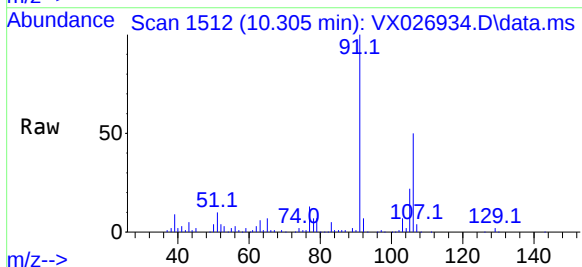




#69
o-Xylene
Concen: 7.683 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36




Instrument :
MSVOA_X
ClientSampleId :
31377


Tgt Ion:106 Resp: 19710
Ion Ratio Lower Upper
106 100
91 214.6 109.7 329.0



#70
Styrene
Concen: 0.281 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.012 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Tgt Ion:104 Resp: 1171
Ion Ratio Lower Upper
104 100
78 259.1 42.5 63.7#
103 229.5 43.3 64.9#


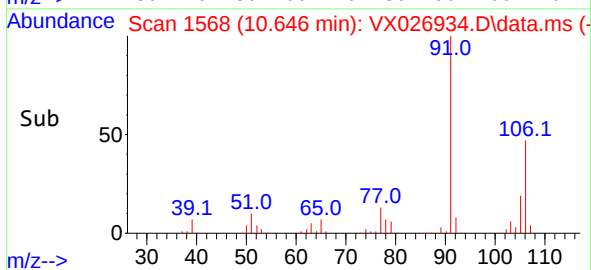






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36




Instrument :
MSVOA_X
ClientSampleId :
31377


Tgt Ion:152 Resp: 81554
Ion Ratio Lower Upper
152 100
115 59.8 44.2 132.6
150 156.6 0.0 348.2

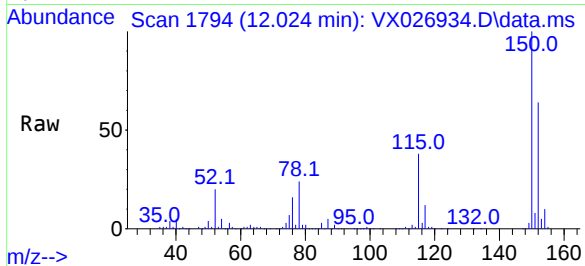

#73
Isopropylbenzene
Concen: 0.958 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Tgt Ion:105 Resp: 6154
Ion Ratio Lower Upper
105 100
120 27.3 13.1 39.1


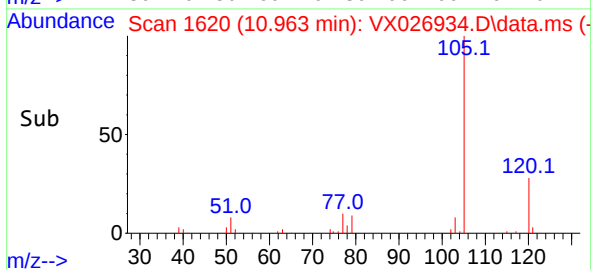

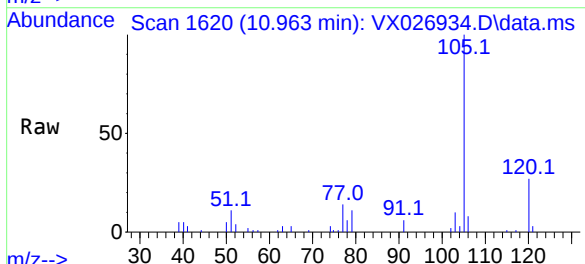




#76
1,2,3-Trichloropropane
Concen: 24.423 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.164 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36




Instrument :
MSVOA_X
ClientSampleId :
31377


Tgt Ion: 75 Resp: 43601
Ion Ratio Lower Upper
75 100
77 1.2 18.3 54.8#

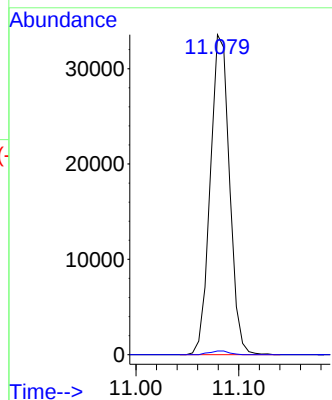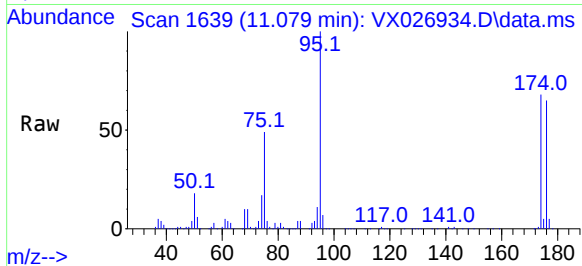

#78
n-propylbenzene
Concen: 2.745 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.000 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Tgt Ion: 91 Resp: 19550
Ion Ratio Lower Upper
91 100
120 22.7 11.6 34.7


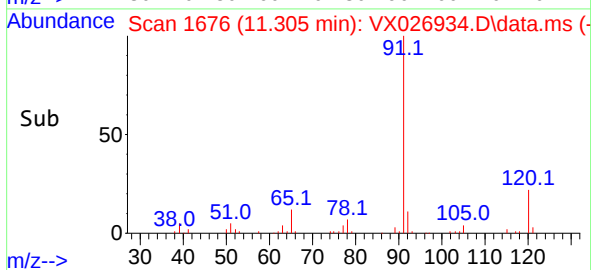
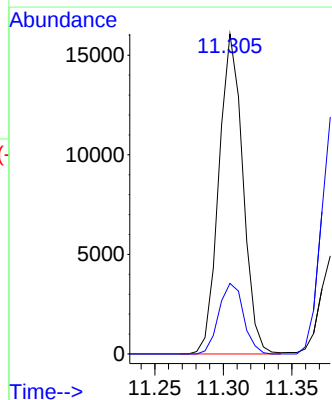
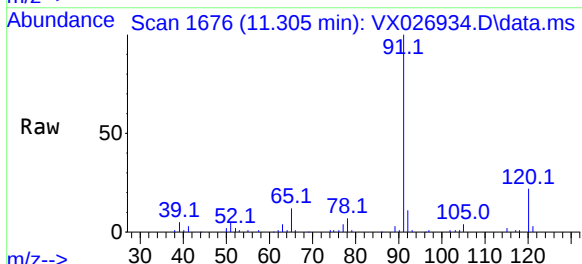




#79
2-Chlorotoluene
Concen: 2.010 ug/l
RT: 11.378 min Scan# 11377
Delta R.T. 0.012 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36




Instrument :
MSVOA_X
ClientSampleId :
31377


Tgt Ion: 91 Resp: 8846
Ion Ratio Lower Upper
91 100
126 0.0 16.4 49.2#

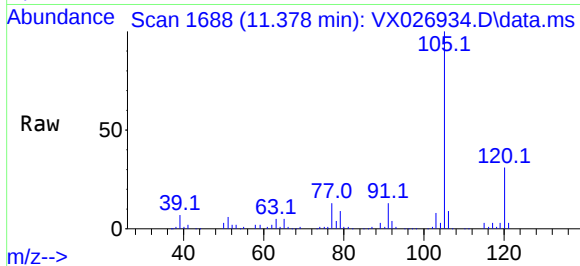

#80
1,3,5-Trimethylbenzene
Concen: 3.907 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Tgt Ion:105 Resp: 20655
Ion Ratio Lower Upper
105 100
120 46.1 24.0 72.0


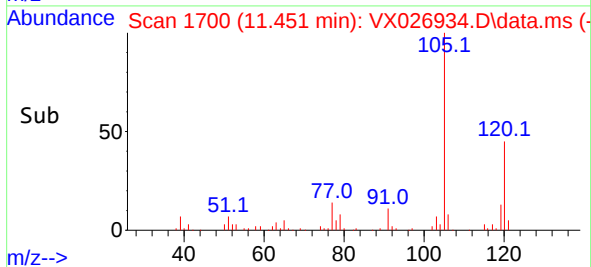

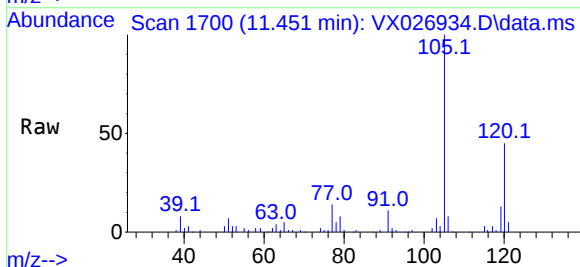




#81
trans-1,4-Dichloro-2-butene
Concen: 74.574 ug/l
RT: 11.079 min Scan# 11
Delta R.T. 0.061 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36




Instrument :
MSVOA_X
ClientSampleId :
31377


Tgt Ion: 75 Resp: 43601
Ion Ratio Lower Upper
75 100
53 0.0 94.0 141.0#
89 0.0 37.0 55.4#

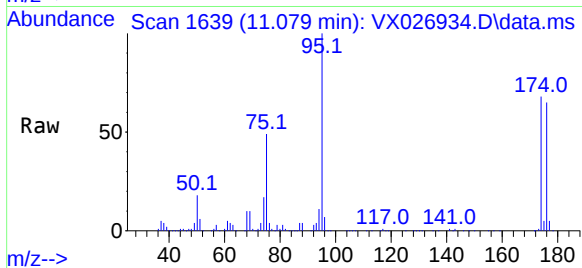

#82
4-Chlorotoluene
Concen: 0.468 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Tgt Ion: 91 Resp: 2309
Ion Ratio Lower Upper
91 100
126 0.0 14.1 42.4#


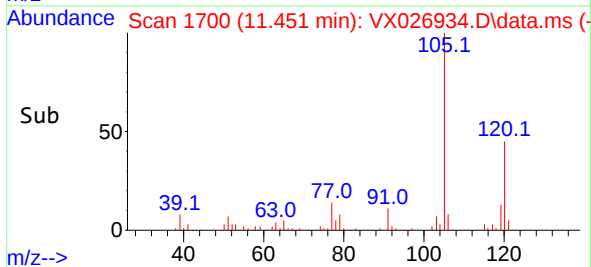

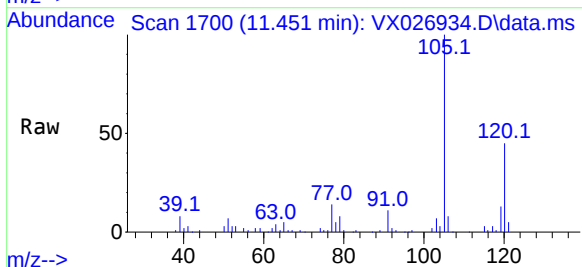




#83
tert-Butylbenzene
Concen: 1.889 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.043 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36




Instrument :
MSVOA_X
ClientSampleId :
31377


Tgt Ion:119 Resp: 9519
Ion Ratio Lower Upper
119 100
91 89.4 31.4 94.0
134 0.0 11.8 35.3#

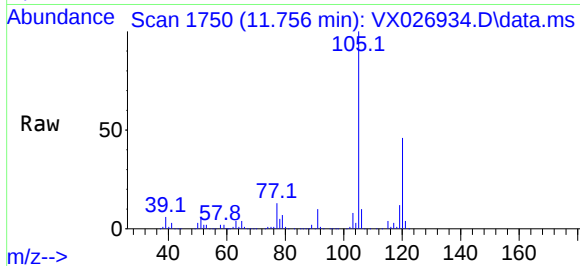

#84
1,2,4-Trimethylbenzene
Concen: 15.068 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Tgt Ion:105 Resp: 80356
Ion Ratio Lower Upper
105 100
120 44.9 21.9 65.5


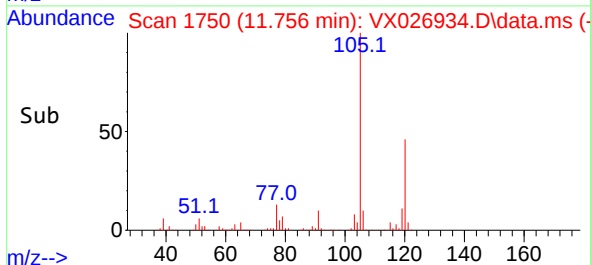
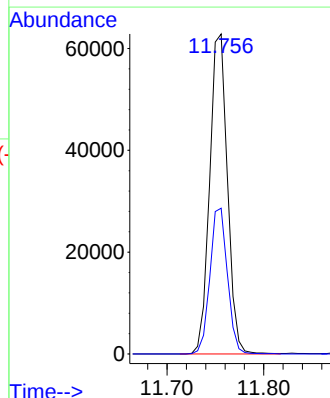
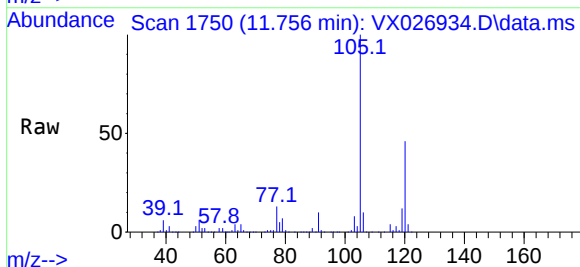




#85
sec-Butylbenzene
Concen: 1.037 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. 0.000 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36




Instrument :
MSVOA_X
ClientSampleId :
31377


Tgt Ion:105 Resp: 6623
Ion Ratio Lower Upper
105 100
134 26.2 10.1 30.1

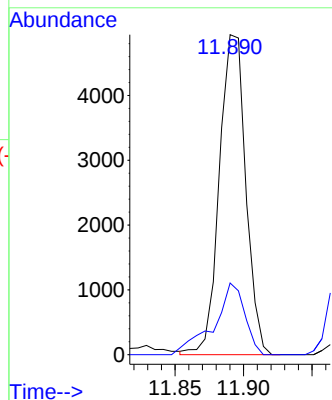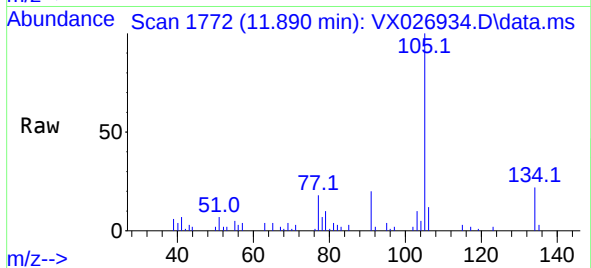

#86
p-Isopropyltoluene
Concen: 0.687 ug/l
RT: 12.012 min Scan# 1792
Delta R.T. 0.000 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Tgt Ion:119 Resp: 3719
Ion Ratio Lower Upper
119 100
134 27.1 13.0 39.0
91 32.2 12.6 37.6

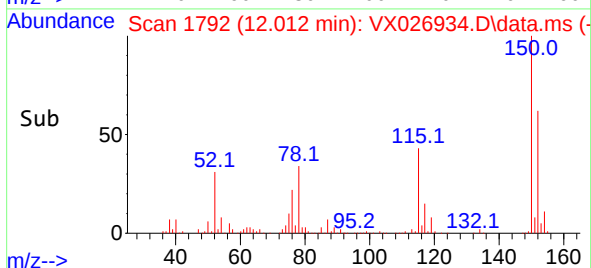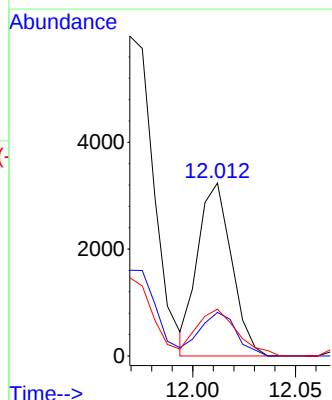



#89

n-Butylbenzene

Concen: 2.761 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. -0.006 min

Lab File: VX026934.D

Acq: 10 Feb 2022 20:36

Instrument :

MSVOA_X

ClientSampleId :

31377





Tgt Ion: 91 Resp: 12223

Ion Ratio Lower Upper

91 100

92 39.8 27.2 81.6

134 83.6 13.1 39.1#

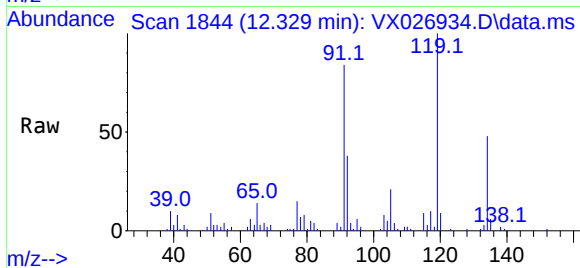

#90

Hexachloroethane

Concen: 1.580 ug/l

RT: 12.530 min Scan# 1877

Delta R.T. -0.012 min

Lab File: VX026934.D




Acq: 10 Feb 2022 20:36


Tgt Ion: 117 Resp: 1236

Ion Ratio Lower Upper

117 100

201 0.0 35.6 106.8#


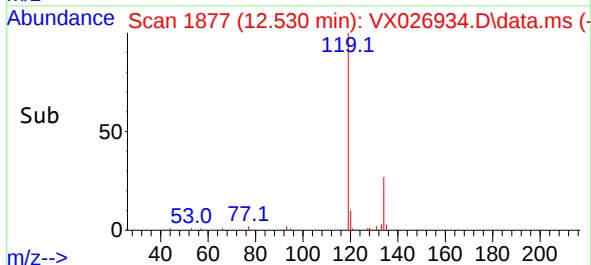
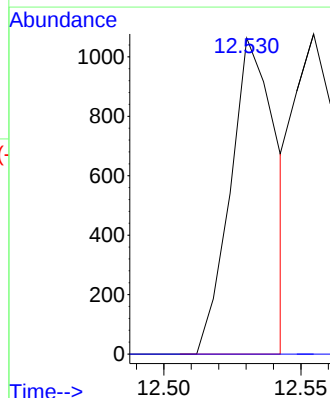
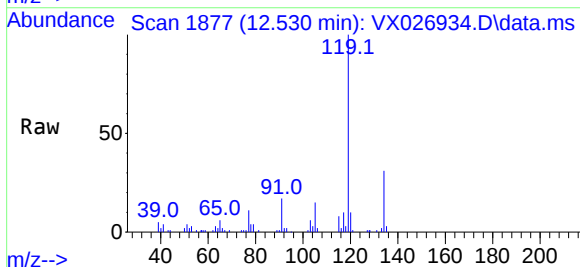




#92
1,2-Dibromo-3-Chloropropane
Concen: 0.236 ug/l
RT: 12.963 min Scan# 1945
Delta R.T. 0.018 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Instrument :
MSVOA_X
ClientSampleId :
31377

Tgt Ion: 75 Resp: 101
Ion Ratio Lower Upper
75 100
155 0.0 40.0 119.9#
157 0.0 51.6 154.8#

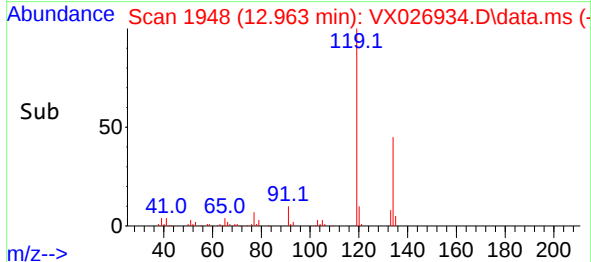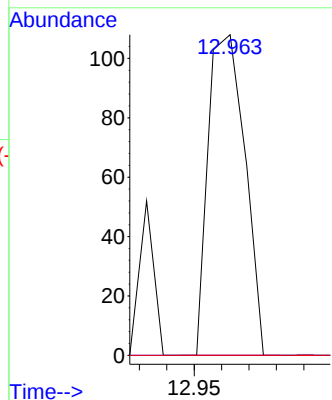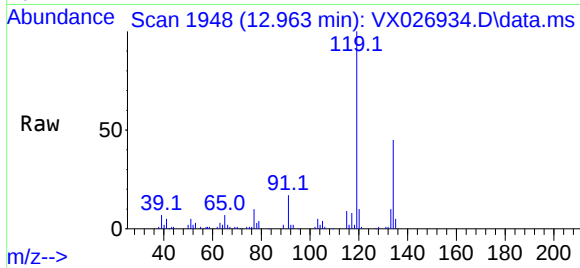

#95
Naphthalene
Concen: 1.622 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX026934.D
Acq: 10 Feb 2022 20:36

Tgt Ion: 128 Resp: 9683
Ion Ratio Lower Upper
128 100
127 14.1 10.3 15.5
129 14.3 8.7 13.1#

