

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
 Data File : VX026927.D
 Acq On : 10 Feb 2022 17:55
 Operator : JC/MD
 Sample : N1446-03DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-118DDL

Quant Time: Feb 11 04:01:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 08 07:07:46 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	121494	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	207658	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	183679	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	77091	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	80974	55.522	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	111.040%
35) Dibromofluoromethane	5.391	113	64485	52.122	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	104.240%
50) Toluene-d8	8.653	98	241940	53.275	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	106.540%
62) 4-Bromofluorobenzene	11.079	95	86227	53.930	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	107.860%
Target Compounds						Qvalue
11) Tert butyl alcohol	2.971	59	10032	38.077	ug/l	# 75
19) Methyl tert-butyl Ether	3.117	73	193591	43.987	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
Data File : VX026927.D
Acq On : 10 Feb 2022 17:55
Operator : JC/MD
Sample : N1446-03DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-118DDL

Quant Time: Feb 11 04:01:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 08 07:07:46 2022
Response via : Initial Calibration




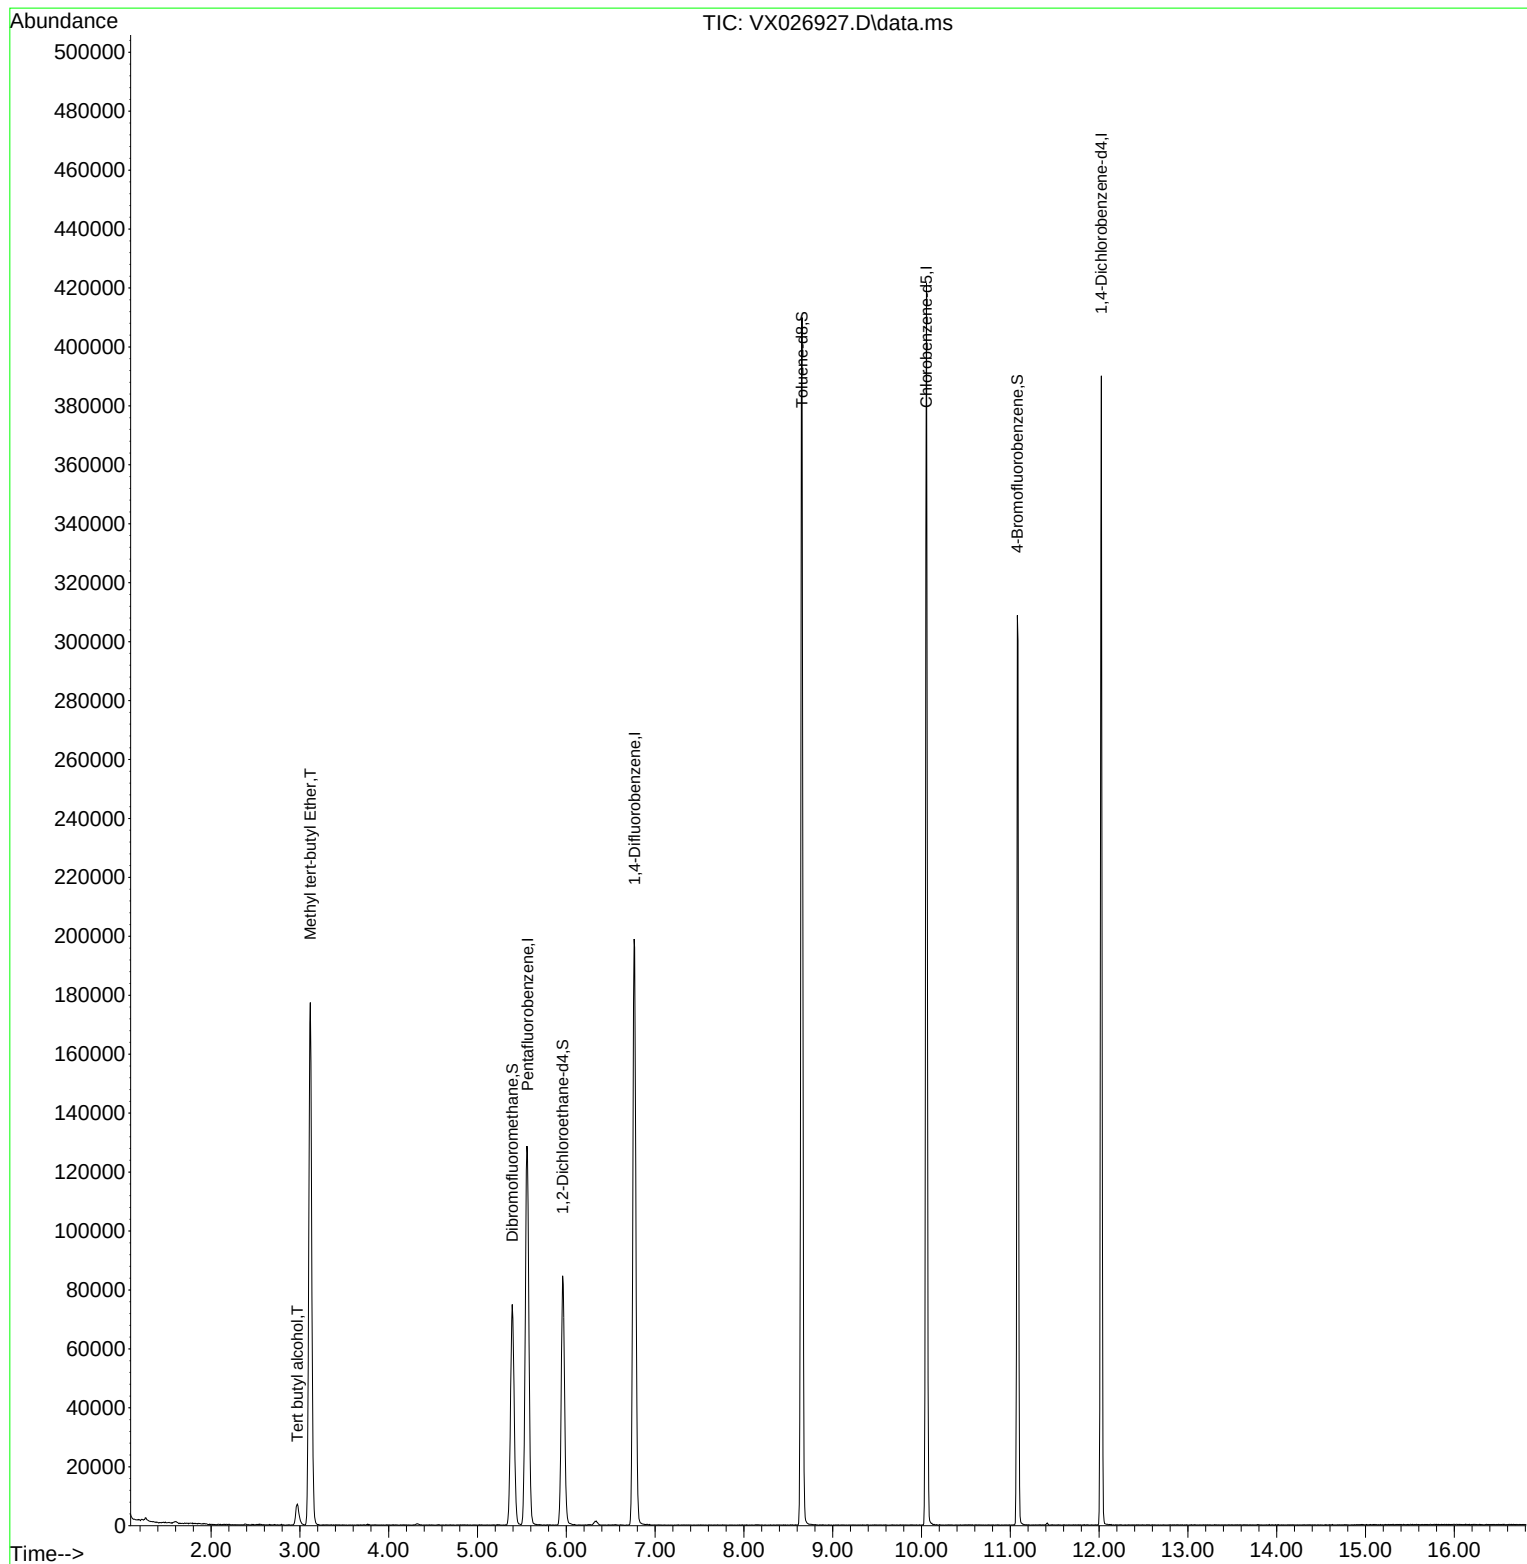


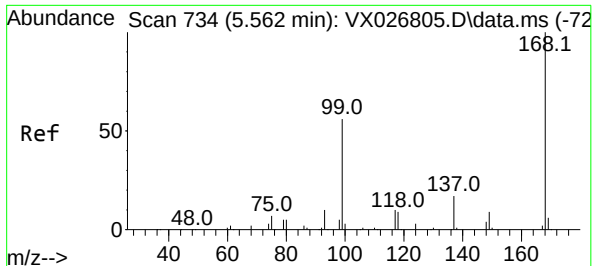

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.000 min
Lab File: VX026927.D
Acq: 10 Feb 2022 17:55




Instrument :
MSVOA_X
ClientSampleId :
MW-118DDL


Tgt Ion:168 Resp: 121494
Ion Ratio Lower Upper
168 100
99 58.9 50.3 75.5

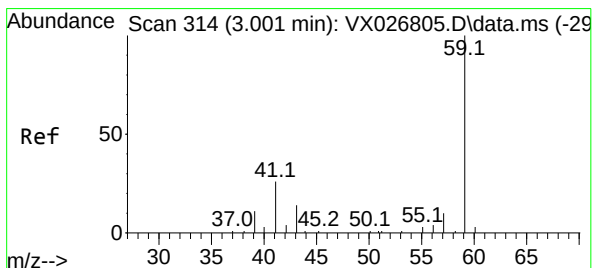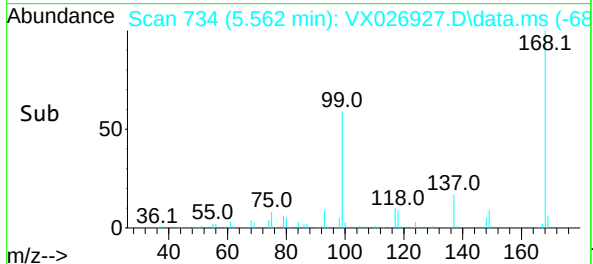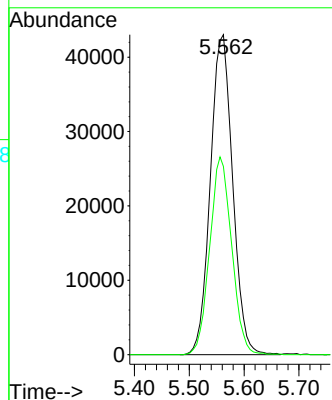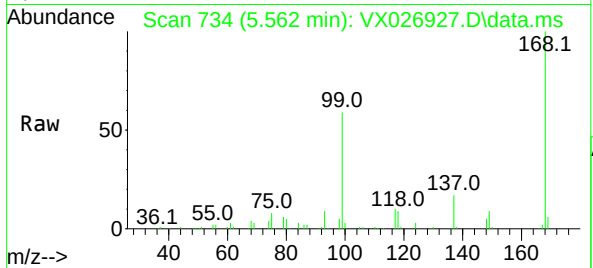

#11
Tert butyl alcohol
Concen: 38.077 ug/l
RT: 2.971 min Scan# 309
Delta R.T. -0.030 min
Lab File: VX026927.D
Acq: 10 Feb 2022 17:55

Tgt Ion: 59 Resp: 10032
Ion Ratio Lower Upper
59 100
57 0.0 7.2 10.8#


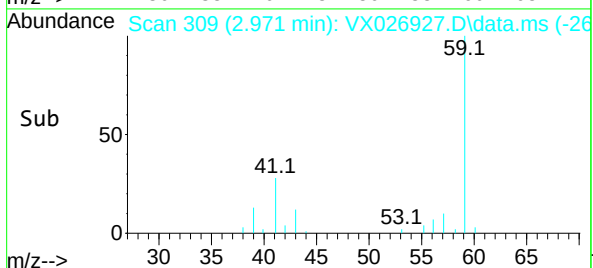
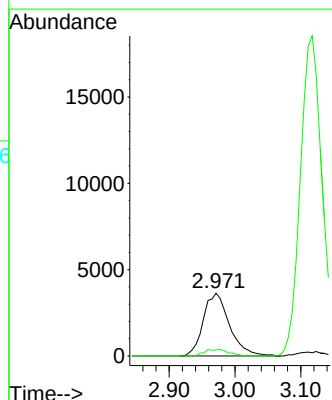
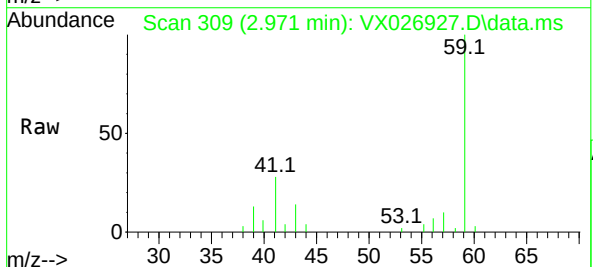


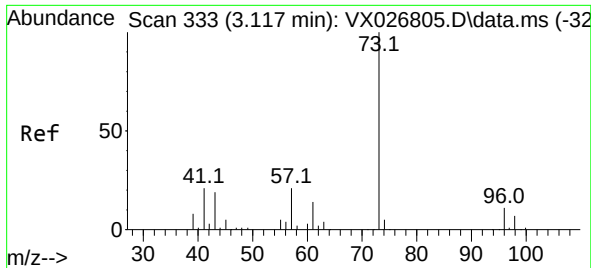

#19
Methyl tert-butyl Ether
Concen: 43.987 ug/l
RT: 3.117 min Scan# 31
Delta R.T. 0.000 min
Lab File: VX026927.D
Acq: 10 Feb 2022 17:55




Instrument :
MSVOA_X
ClientSampleId :
MW-118DDL


Tgt Ion: 73 Resp: 193591
Ion Ratio Lower Upper
73 100
57 22.1 17.4 26.2

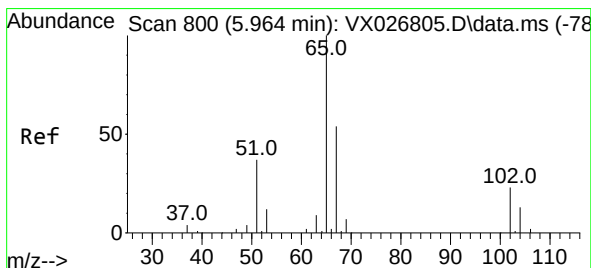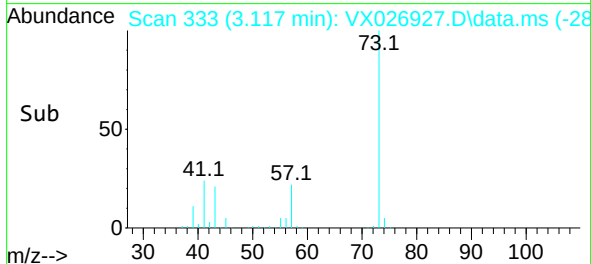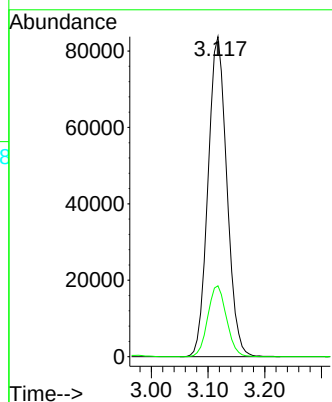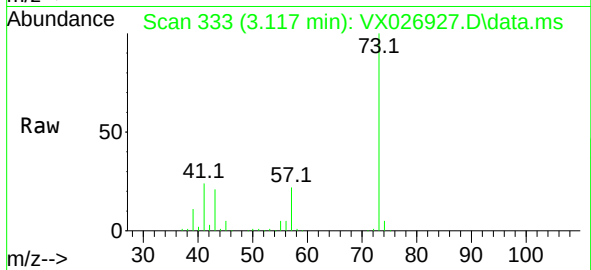

#33
1,2-Dichloroethane-d4
Concen: 55.522 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.006 min
Lab File: VX026927.D
Acq: 10 Feb 2022 17:55

Tgt Ion: 65 Resp: 80974
Ion Ratio Lower Upper
65 100
67 51.5 0.0 100.8


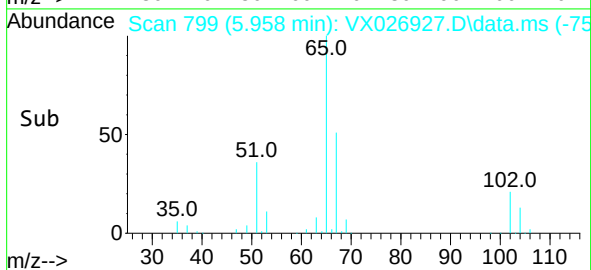
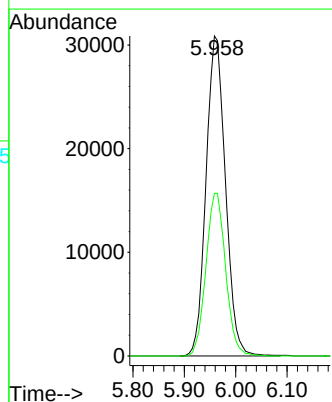
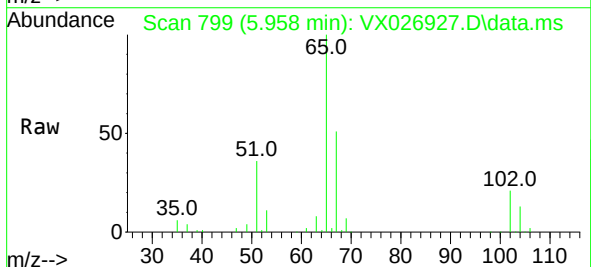


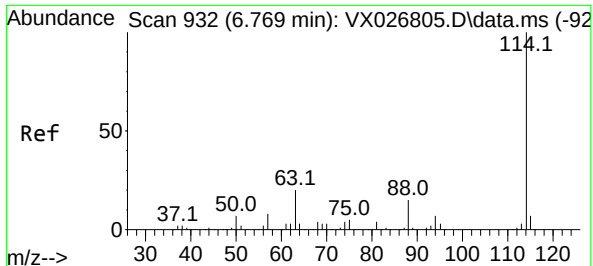

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX026927.D
Acq: 10 Feb 2022 17:55




Instrument :
MSVOA_X
ClientSampleId :
MW-118DDL


Tgt Ion:114 Resp: 207658
Ion Ratio Lower Upper
114 100
63 20.7 0.0 42.8
88 16.2 0.0 33.0

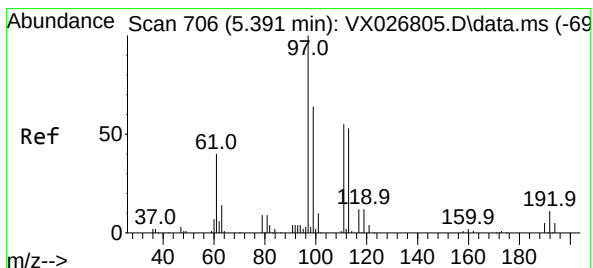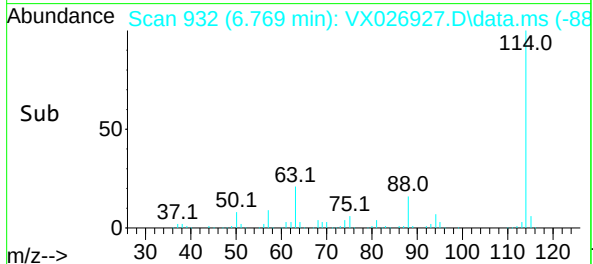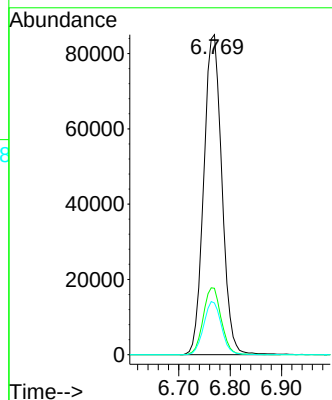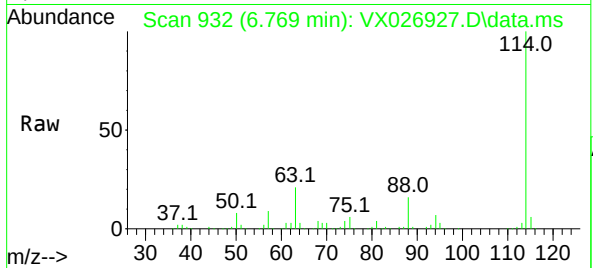

#35
Dibromofluoromethane
Concen: 52.122 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX026927.D
Acq: 10 Feb 2022 17:55

Tgt Ion:113 Resp: 64485
Ion Ratio Lower Upper
113 100
111 103.2 81.2 121.8
192 19.3 15.0 22.4


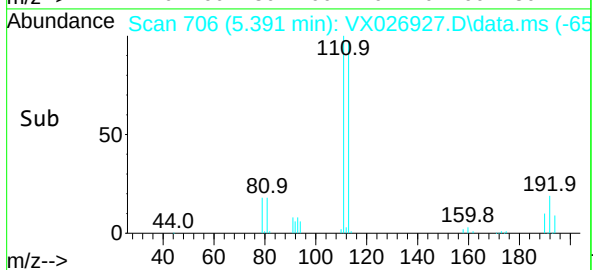
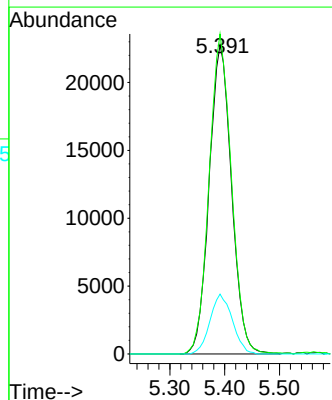
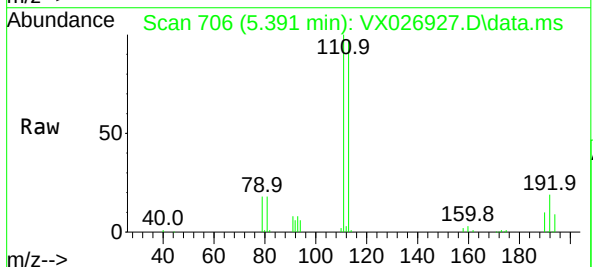


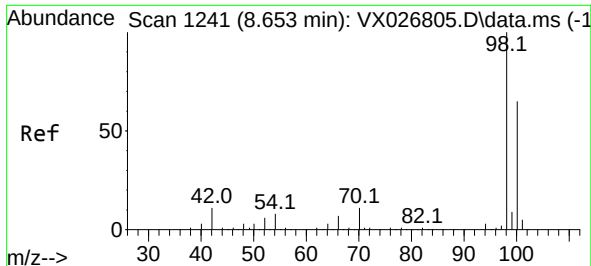

#50
Toluene-d8
Concen: 53.275 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX026927.D
Acq: 10 Feb 2022 17:55




Instrument :
MSVOA_X
ClientSampleId :
MW-118DDL


Tgt Ion: 98 Resp: 241940
Ion Ratio Lower Upper
98 100
100 65.8 53.2 79.8

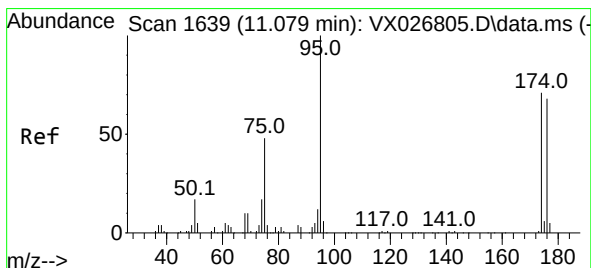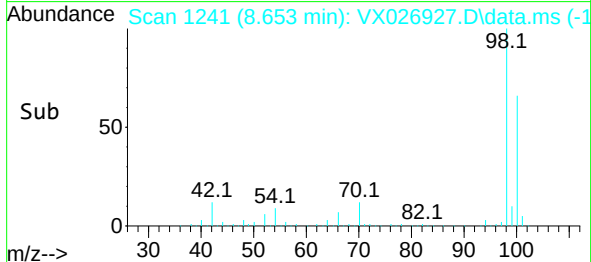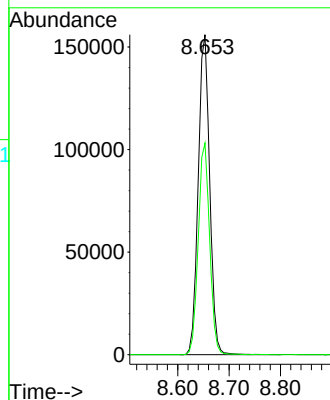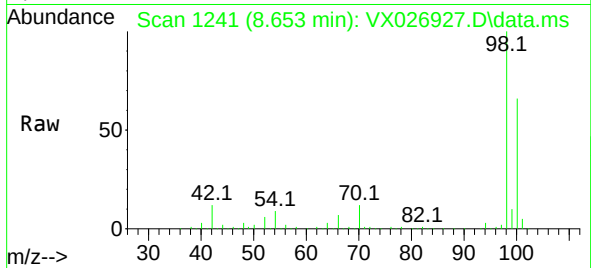

#62
4-Bromofluorobenzene
Concen: 53.930 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX026927.D
Acq: 10 Feb 2022 17:55

Tgt Ion: 95 Resp: 86227
Ion Ratio Lower Upper
95 100
174 75.3 0.0 148.6
176 72.3 0.0 141.4


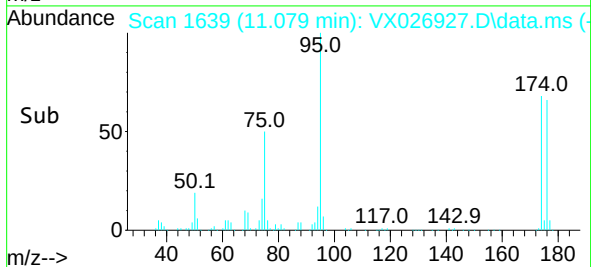
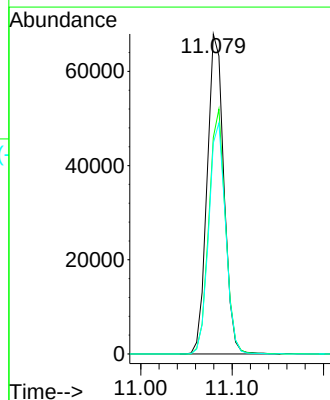
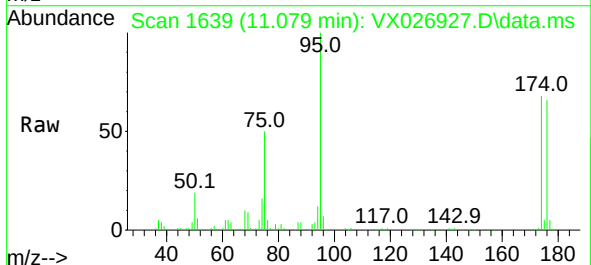


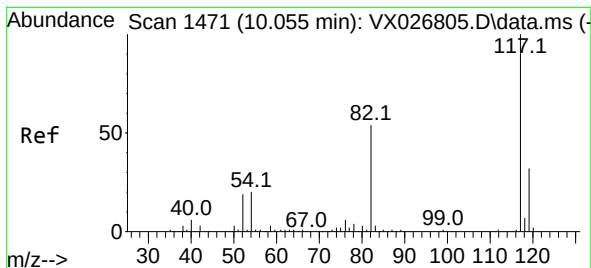

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX026927.D
Acq: 10 Feb 2022 17:55

Instrument :
MSVOA_X
ClientSampleId :
MW-118DDL

Tgt Ion:117 Resp: 183679
Ion Ratio Lower Upper
117 100
82 56.1 45.2 67.8
119 32.3 26.2 39.2

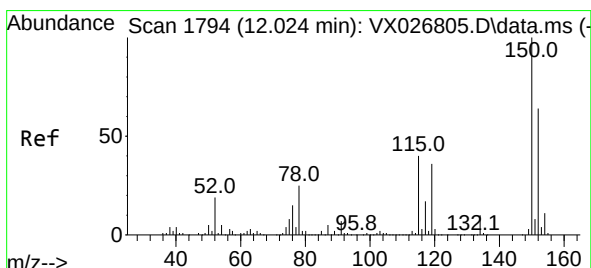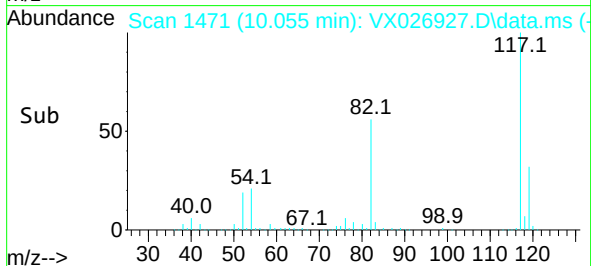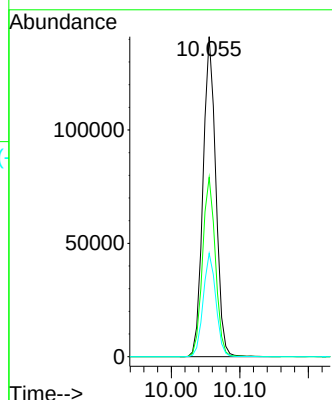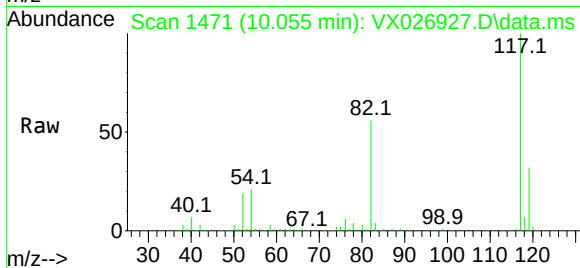

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX026927.D
Acq: 10 Feb 2022 17:55

Tgt Ion:152 Resp: 77091
Ion Ratio Lower Upper
152 100
115 61.8 44.2 132.6
150 159.4 0.0 348.2

