

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
 Data File : VX026932.D
 Acq On : 10 Feb 2022 19:50
 Operator : JC/MD
 Sample : N1446-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-107

Quant Time: Feb 11 04:03:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 08 07:07:46 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	116142	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	196660	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	176871	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	74565	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	76801	55.087	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	110.180%
35) Dibromofluoromethane	5.391	113	61476	52.469	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	104.940%
50) Toluene-d8	8.653	98	229097	53.268	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	106.540%
62) 4-Bromofluorobenzene	11.079	95	82327	54.371	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	108.740%
Target Compounds						Qvalue
19) Methyl tert-butyl Ether	3.117	73	3379	0.803	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
Data File : VX026932.D
Acq On : 10 Feb 2022 19:50
Operator : JC/MD
Sample : N1446-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-107

Quant Time: Feb 11 04:03:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 08 07:07:46 2022
Response via : Initial Calibration




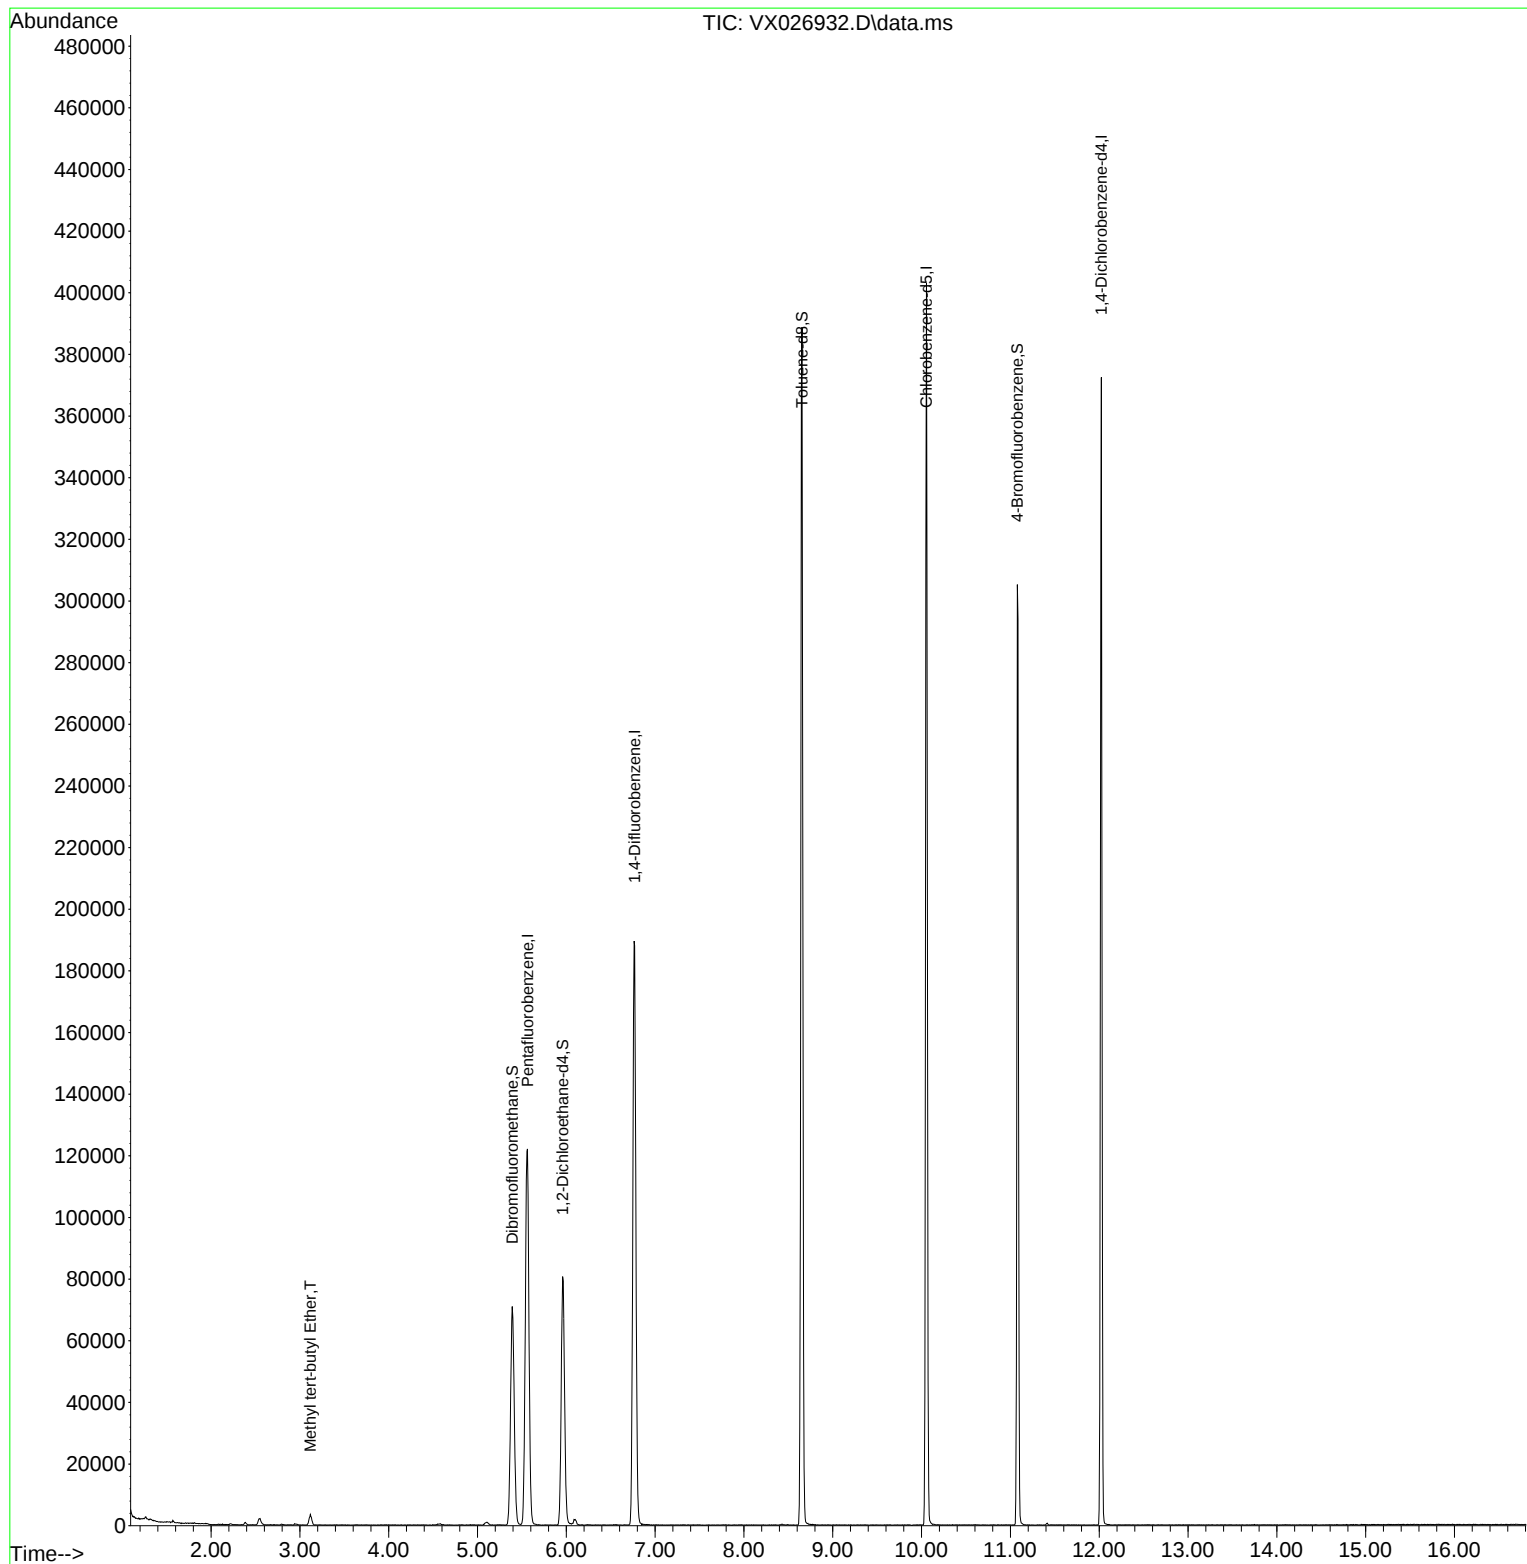




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.000 min
Lab File: VX026932.D
Acq: 10 Feb 2022 19:50




Instrument :
MSVOA_X
ClientSampleId :
MW-107


Tgt Ion:168 Resp: 116142
Ion Ratio Lower Upper
168 100
99 60.7 50.3 75.5

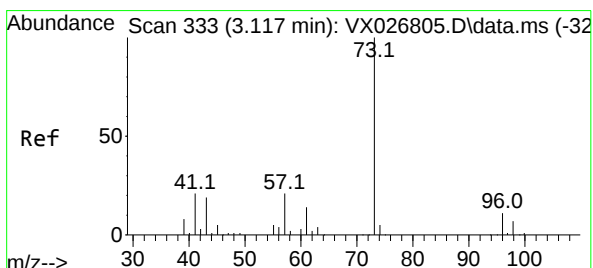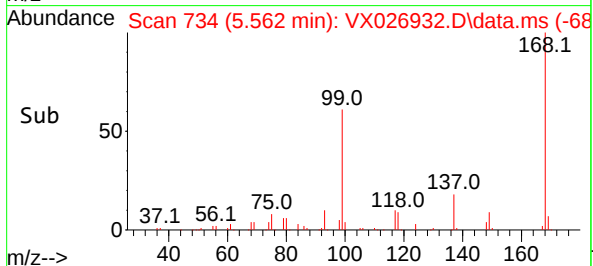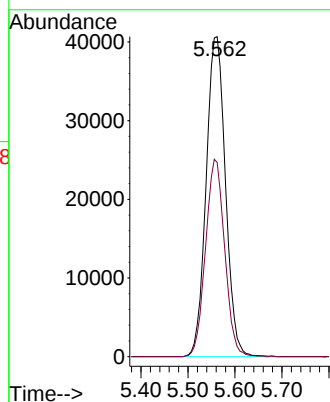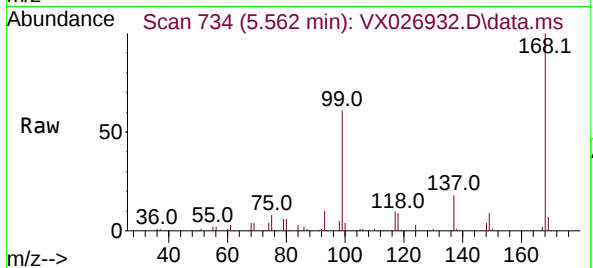

#19
Methyl tert-butyl Ether
Concen: 0.803 ug/l
RT: 3.117 min Scan# 333
Delta R.T. 0.000 min
Lab File: VX026932.D
Acq: 10 Feb 2022 19:50

Tgt Ion: 73 Resp: 3379
Ion Ratio Lower Upper
73 100
57 22.4 17.4 26.2

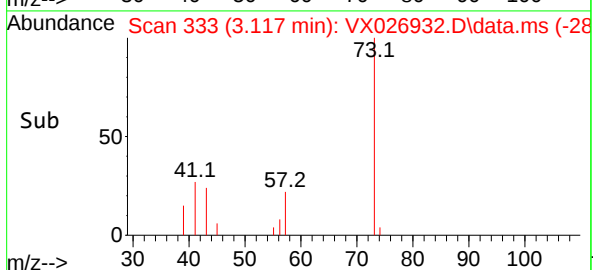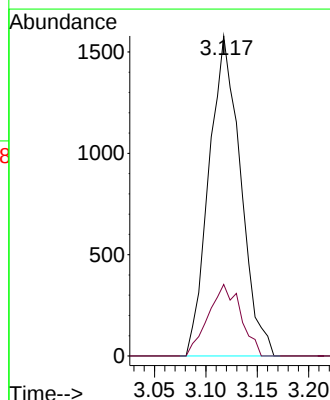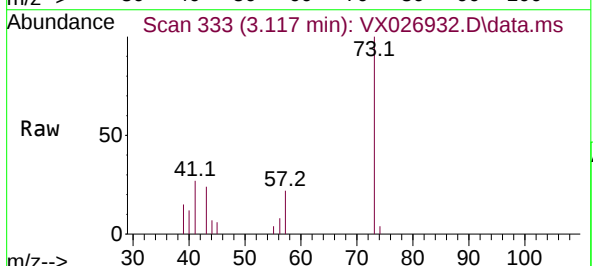

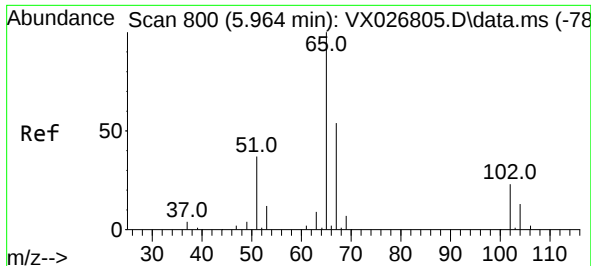

#33

1,2-Dichloroethane-d4

Concen: 55.087 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX026932.D

Acq: 10 Feb 2022 19:50

Instrument :

MSVOA_X

ClientSampleId :





MW-107

Tgt Ion: 65 Resp: 76801

Ion Ratio Lower Upper

65 100

67 52.5 0.0 100.8

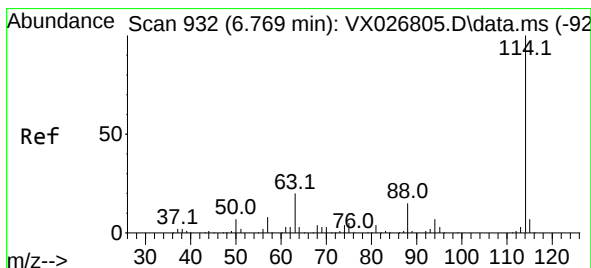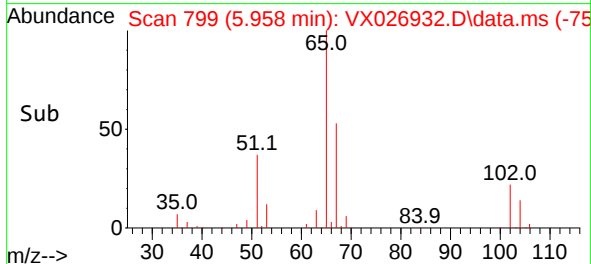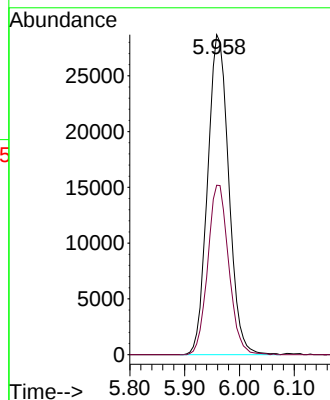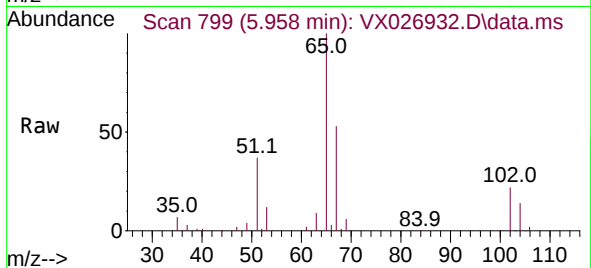

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.000 min

Lab File: VX026932.D

Acq: 10 Feb 2022 19:50




Tgt Ion: 114 Resp: 196660


Ion Ratio Lower Upper

114 100

63 20.9 0.0 42.8

88 16.0 0.0 33.0

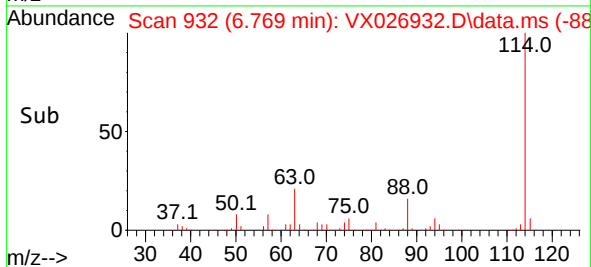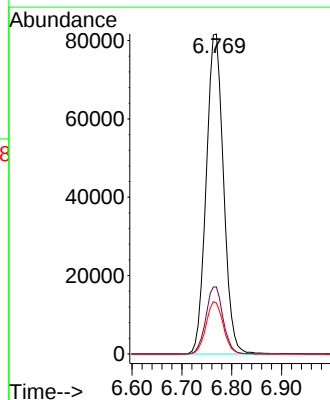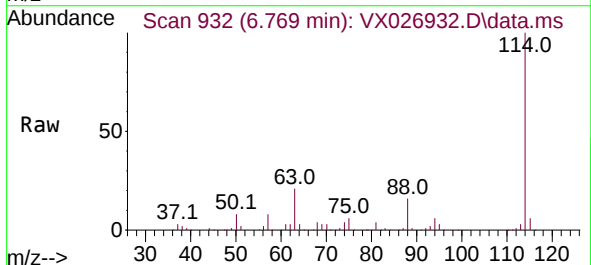

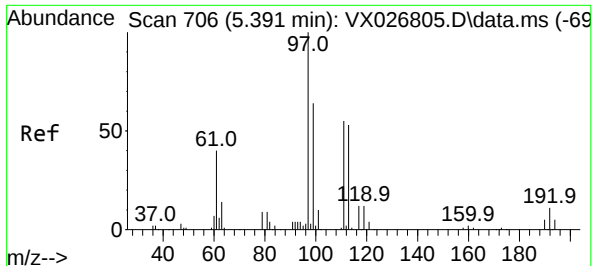

#35

Dibromofluoromethane

Concen: 52.469 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX026932.D

Acq: 10 Feb 2022 19:50

Instrument :

MSVOA_X

ClientSampleId :

MW-107





Tgt Ion:113 Resp: 61476

Ion Ratio Lower Upper

113 100

111 103.5 81.2 121.8

192 19.2 15.0 22.4

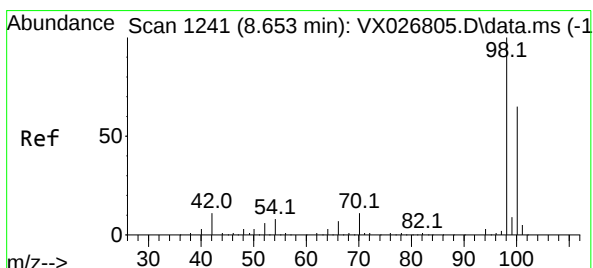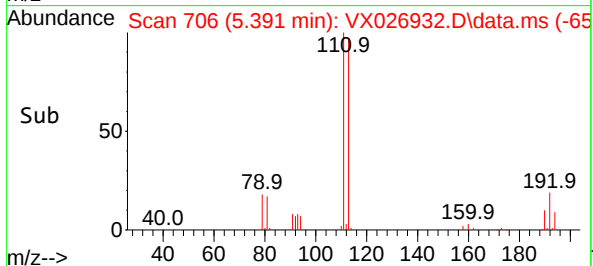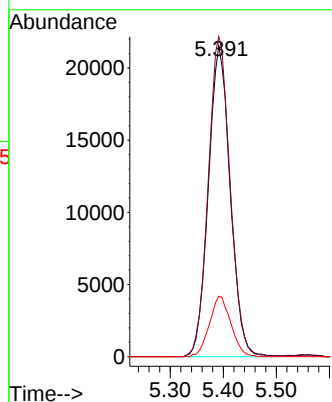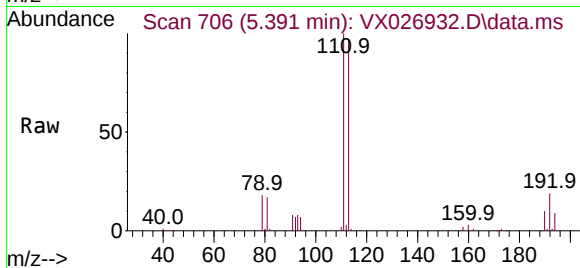

#50

Toluene-d8

Concen: 53.268 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. 0.000 min

Lab File: VX026932.D




Acq: 10 Feb 2022 19:50


Tgt Ion: 98 Resp: 229097

Ion Ratio Lower Upper

98 100

100 66.6 53.2 79.8


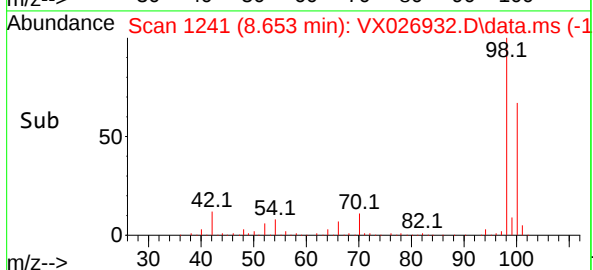
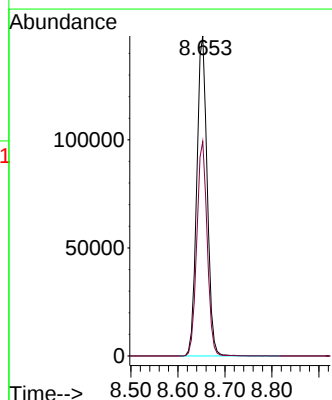
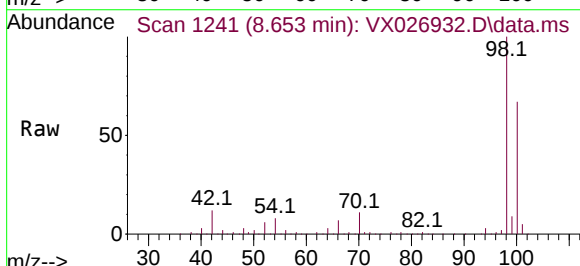


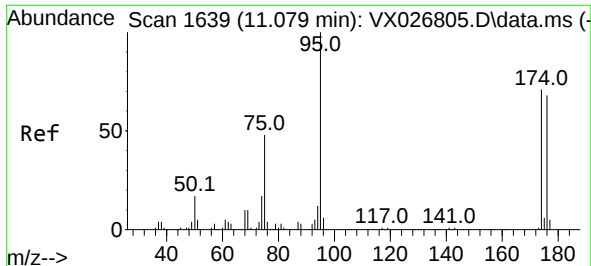

#62
4-Bromofluorobenzene
Concen: 54.371 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX026932.D
Acq: 10 Feb 2022 19:50




Instrument :
MSVOA_X
ClientSampleId :
MW-107


Tgt Ion: 95 Resp: 82327
Ion Ratio Lower Upper
95 100
174 76.0 0.0 148.6
176 72.0 0.0 141.4

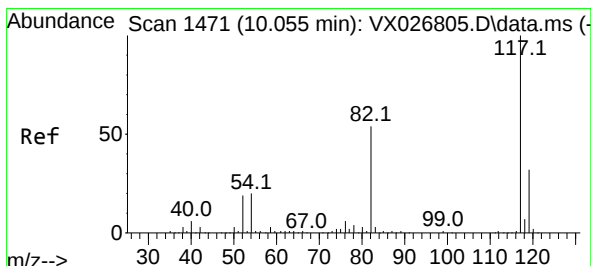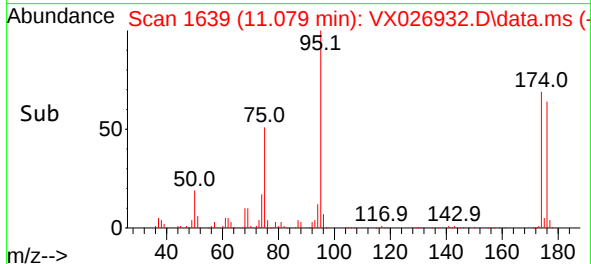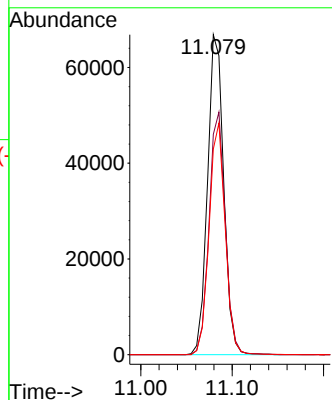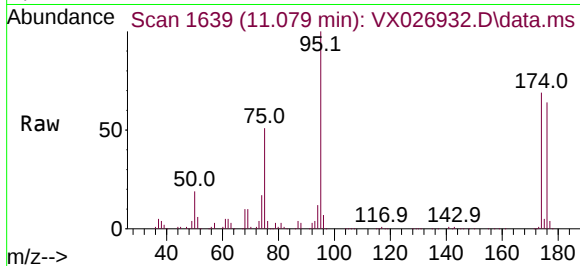

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX026932.D
Acq: 10 Feb 2022 19:50


Tgt Ion: 117 Resp: 176871
Ion Ratio Lower Upper
117 100
82 57.1 45.2 67.8
119 32.9 26.2 39.2

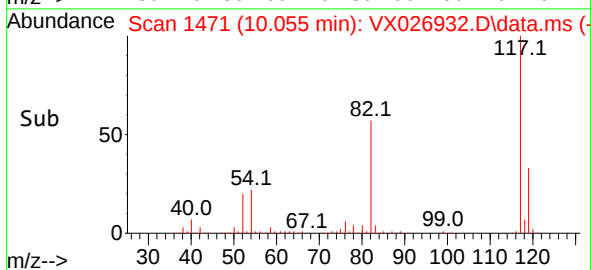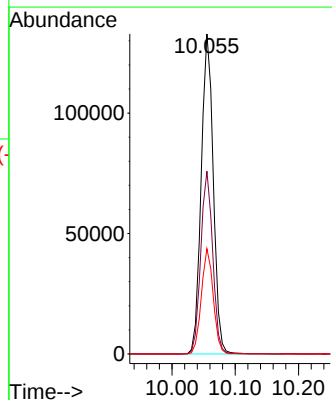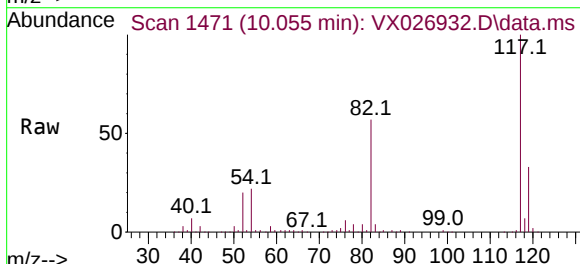

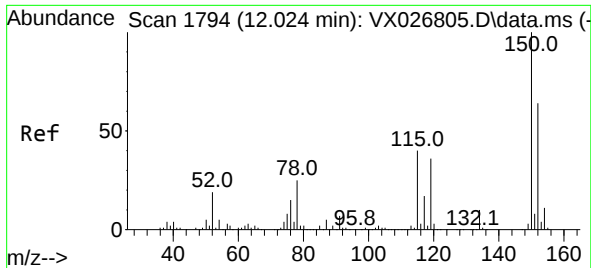

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX026932.D
 Acq: 10 Feb 2022 19:50

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-107

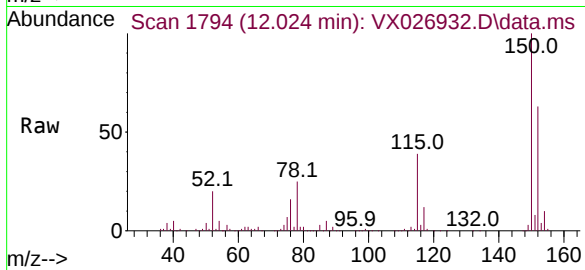

Tgt Ion:152 Resp: 74565
 Ion Ratio Lower Upper
 152 100
 115 61.2 44.2 132.6
 150 157.6 0.0 348.2

