

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
Data File : VX026945.D
Acq On : 11 Feb 2022 01:59
Operator : JC/MD
Sample : N1467-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-30D

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M

Title : SW846 8260

Signal : TIC: VX026945.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.495	546	559	584	rBV	2105838	5698493	100.00%	41.477%
2	5.391	695	706	719	rBV	73118	210267	3.69%	1.530%
3	5.562	722	734	750	rVB	130370	368671	6.47%	2.683%
4	5.958	789	799	813	rBV	81659	216492	3.80%	1.576%
5	6.763	921	931	944	rBV	198447	475997	8.35%	3.465%
6	7.129	981	991	1010	rBV	1063183	2266137	39.77%	16.494%
7	8.653	1234	1241	1250	rBV	407258	642572	11.28%	4.677%
8	9.275	1336	1343	1356	rBV	1636937	2368872	41.57%	17.242%
9	10.055	1465	1471	1481	rBV	430845	568990	9.98%	4.141%
10	11.079	1634	1639	1645	rBV	332835	420140	7.37%	3.058%
11	12.024	1788	1794	1801	rBV	409547	502340	8.82%	3.656%




Sum of corrected areas: 13738971

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
Data File : VX026945.D
Acq On : 11 Feb 2022 01:59
Operator : JC/MD
Sample : N1467-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-30D

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

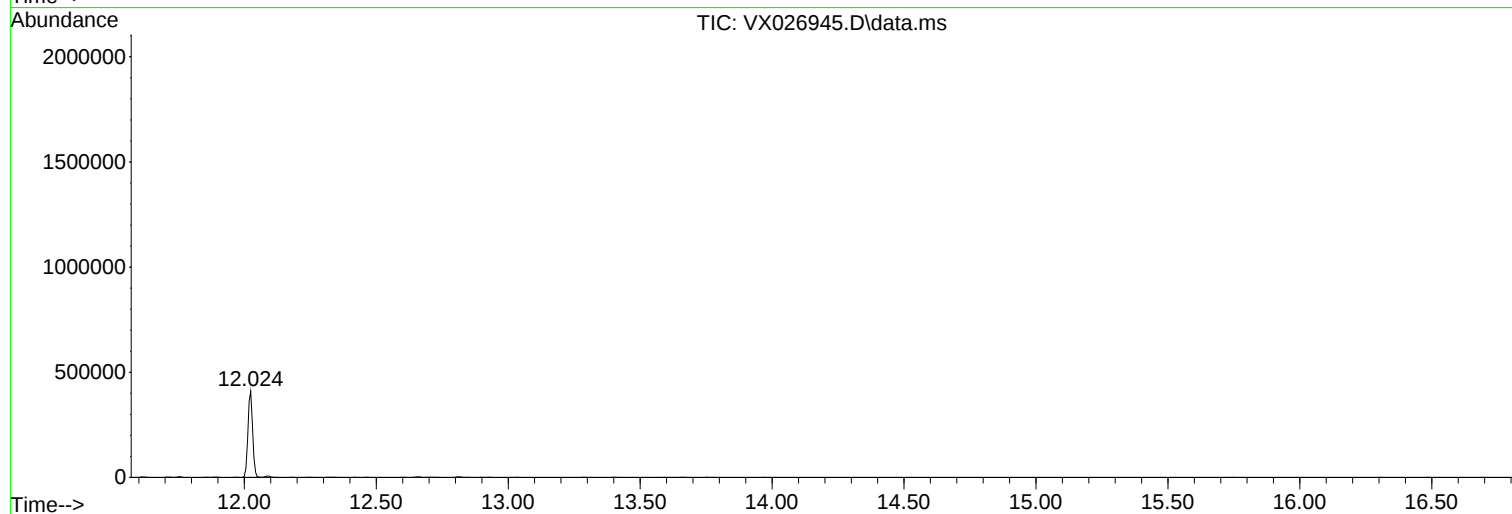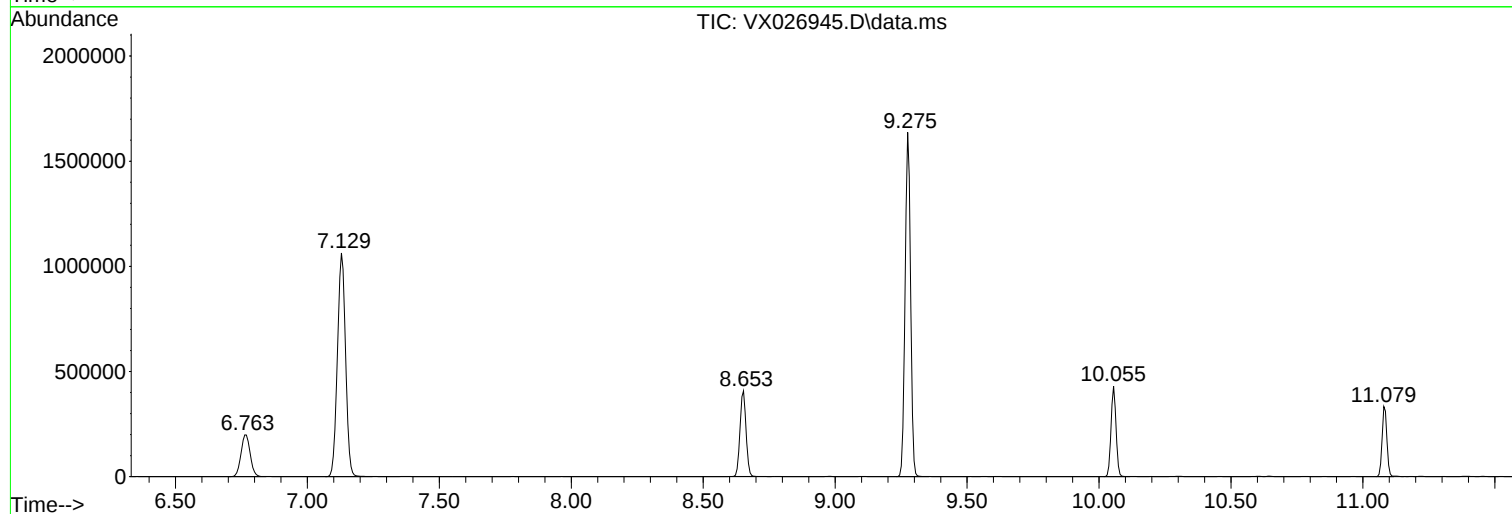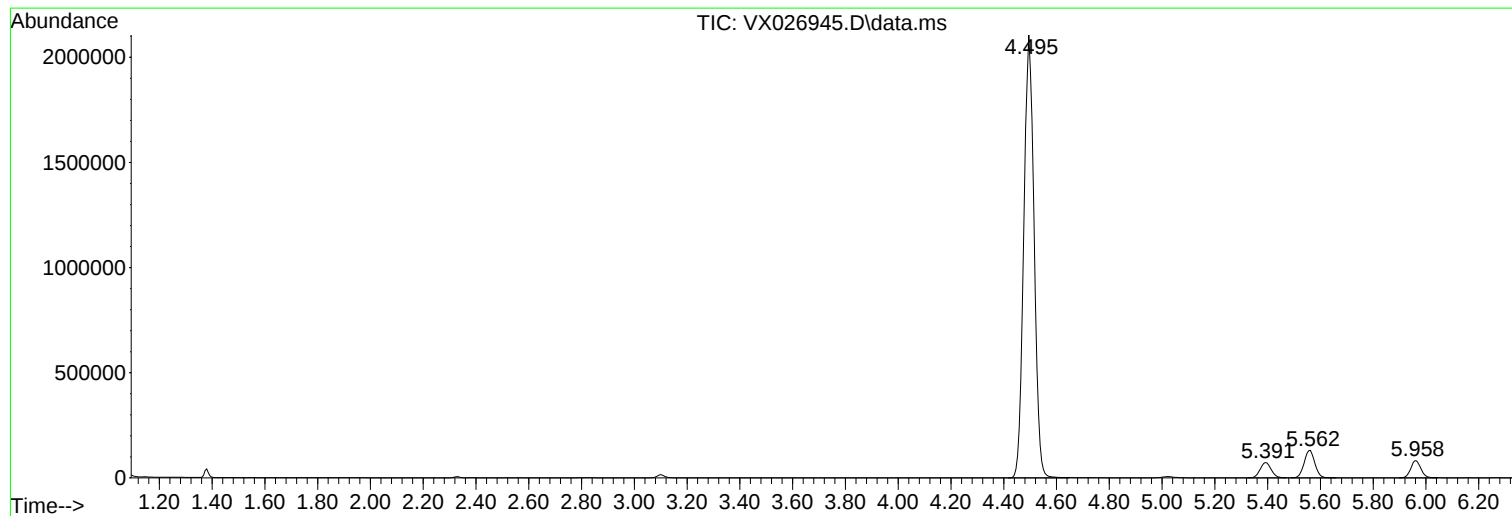

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
Data File : VX026945.D
Acq On : 11 Feb 2022 01:59
Operator : JC/MD
Sample : N1467-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-30D

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
Data File : VX026945.D
Acq On : 11 Feb 2022 01:59
Operator : JC/MD
Sample : N1467-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-30D

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------