

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
 Data File : VX026950.D
 Acq On : 11 Feb 2022 03:54
 Operator : JC/MD
 Sample : N1467-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-23D

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
 Title : SW846 8260

Signal : TIC: VX026950.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.495	546	559	581	rBV	2168110	5820829	93.54%	29.529%
2	5.391	694	706	721	rBV	71841	205939	3.31%	1.045%
3	5.556	721	733	749	rVB	125723	354337	5.69%	1.798%
4	5.958	788	799	812	rBV	76521	208364	3.35%	1.057%
5	6.763	920	931	948	rBV	192279	459438	7.38%	2.331%
6	7.129	980	991	1017	rBV	1997751	4341103	69.76%	22.022%
7	8.653	1234	1241	1251	rBV	390553	621259	9.98%	3.152%
8	9.281	1336	1344	1361	rBV	4086928	6223104	100.00%	31.570%
9	10.055	1465	1471	1486	rBV	424422	555288	8.92%	2.817%
10	11.079	1634	1639	1645	rBV	321598	418001	6.72%	2.120%
11	12.024	1788	1794	1801	rBV	402917	504728	8.11%	2.560%




Sum of corrected areas: 19712390

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
Data File : VX026950.D
Acq On : 11 Feb 2022 03:54
Operator : JC/MD
Sample : N1467-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-23D

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

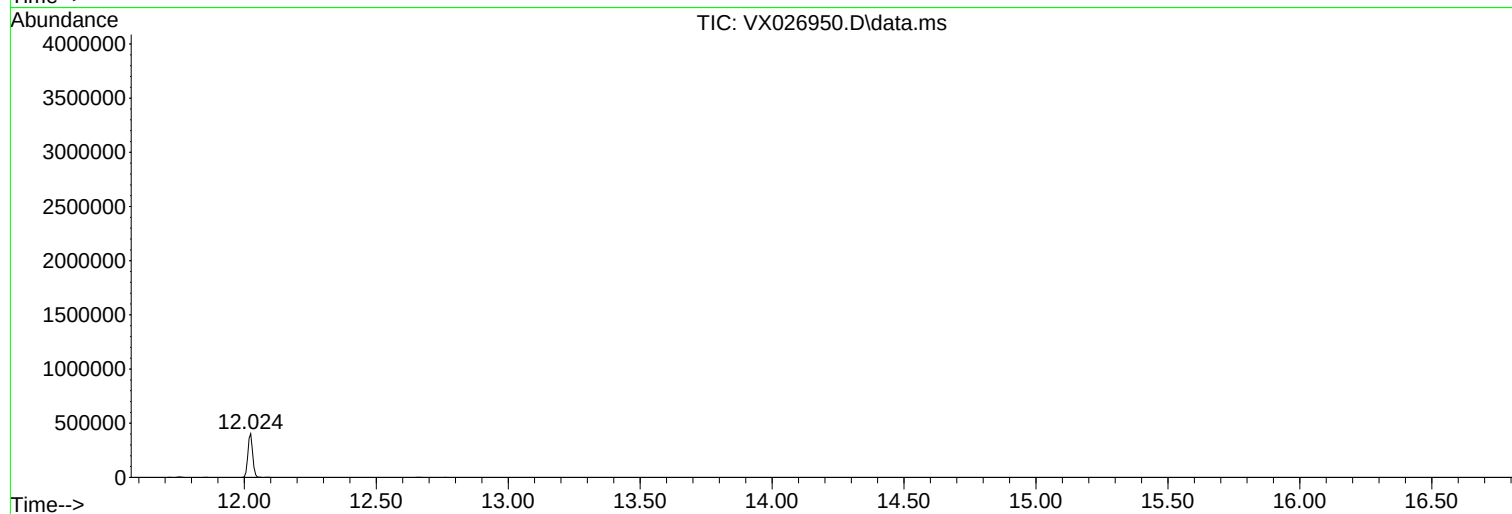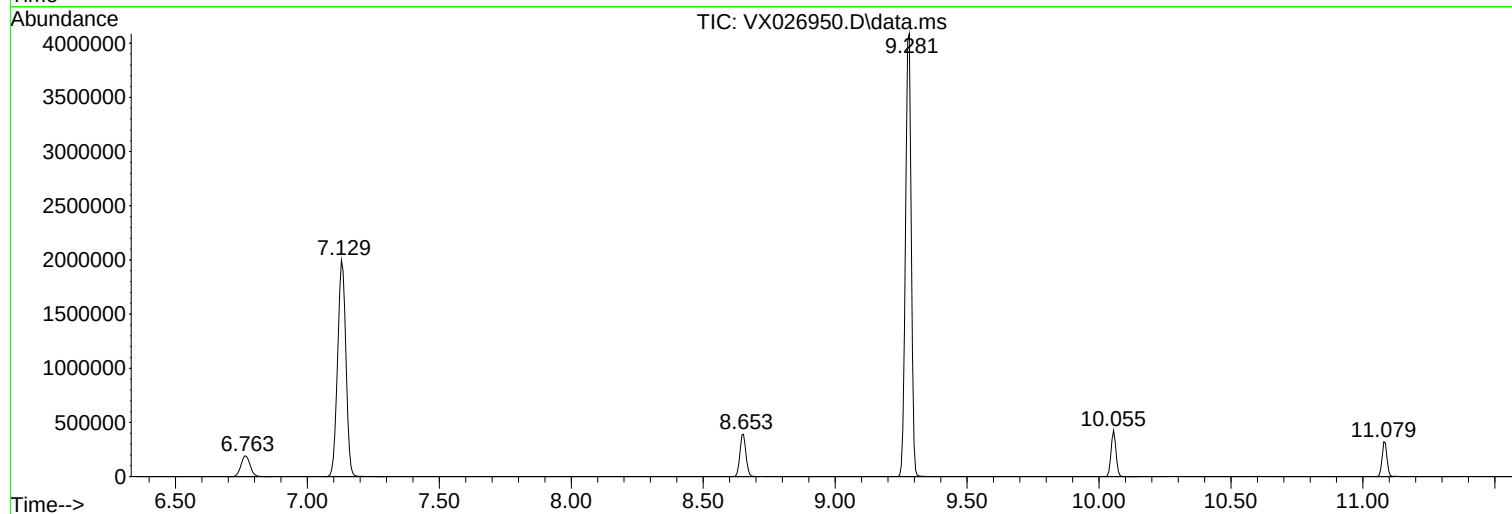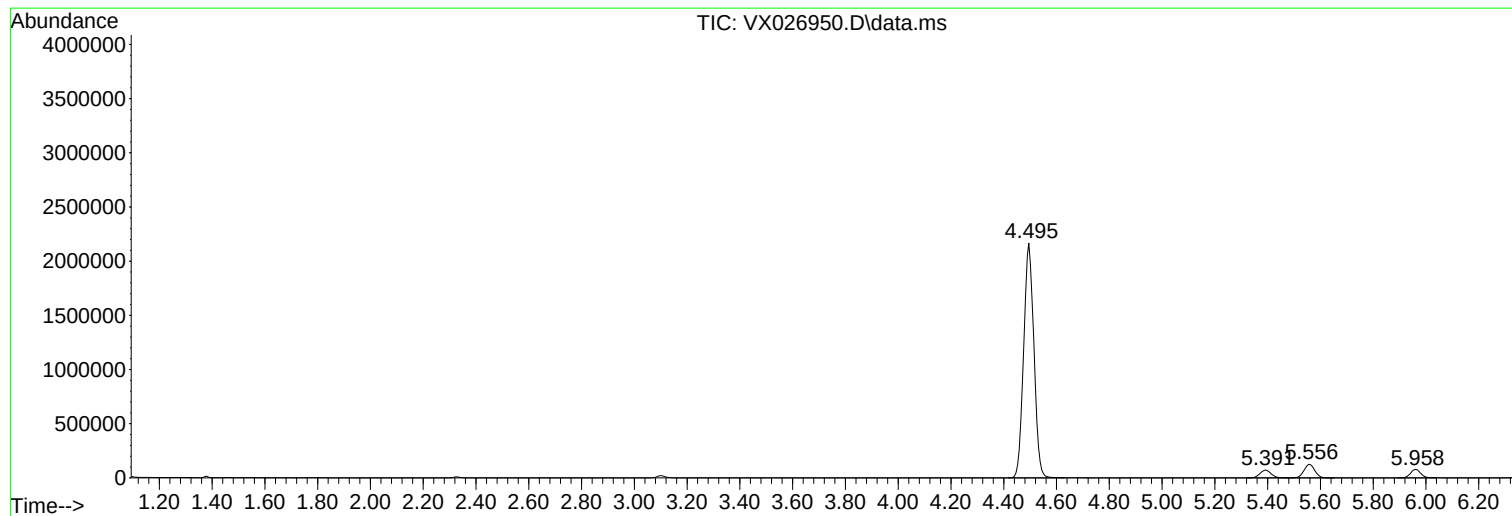

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
Data File : VX026950.D
Acq On : 11 Feb 2022 03:54
Operator : JC/MD
Sample : N1467-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-23D

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
Data File : VX026950.D
Acq On : 11 Feb 2022 03:54
Operator : JC/MD
Sample : N1467-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-23D

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------