

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
Data File : VX026956.D
Acq On : 11 Feb 2022 06:12
Operator : JC/MD
Sample : N1497-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-BLIND-DUPLICATE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M

Title : SW846 8260

Signal : TIC: VX026956.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.391	695	706	722	rBV3	72706	209534	32.94%	6.201%
2	5.556	722	733	749	rVB	127788	358887	56.42%	10.622%
3	5.958	787	799	819	rBV	82903	216598	34.05%	6.410%
4	6.763	922	931	946	rBV	197157	468850	73.71%	13.876%
5	8.653	1234	1241	1254	rBV	405104	636060	100.00%	18.825%
6	10.055	1465	1471	1490	rVB	433687	565481	88.90%	16.736%
7	11.079	1634	1639	1650	rBV	325255	424384	66.72%	12.560%
8	12.024	1788	1794	1804	rBV	402588	499030	78.46%	14.769%




Sum of corrected areas: 3378824

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
Data File : VX026956.D
Acq On : 11 Feb 2022 06:12
Operator : JC/MD
Sample : N1497-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-BLIND-DUPLICATE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

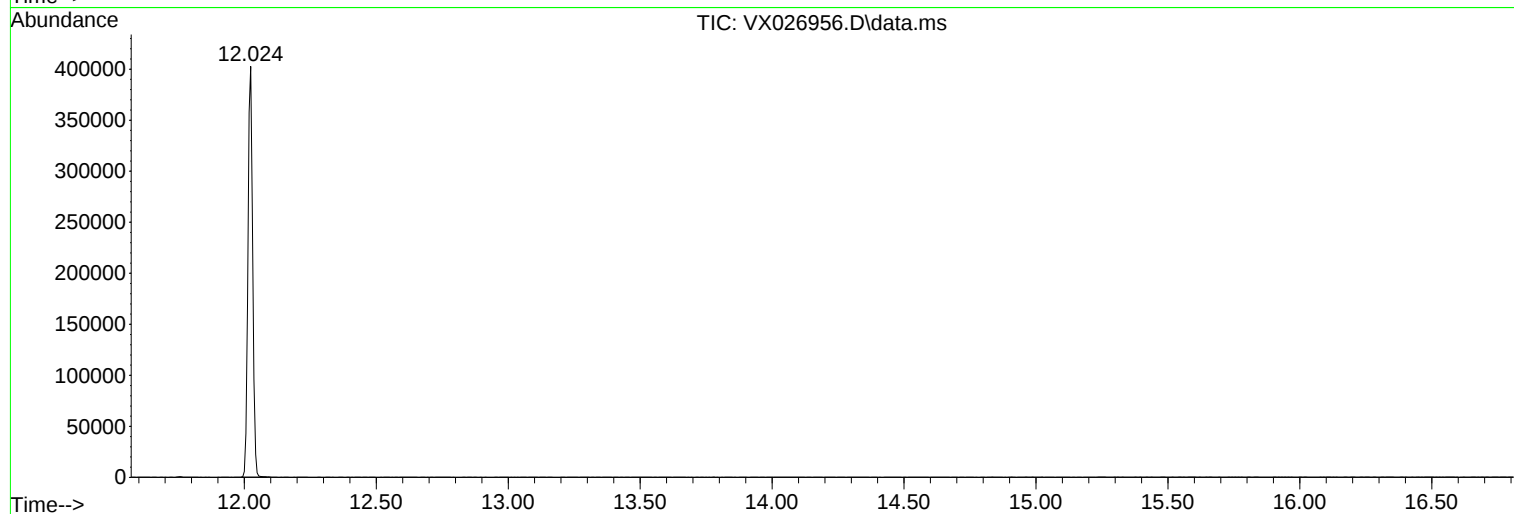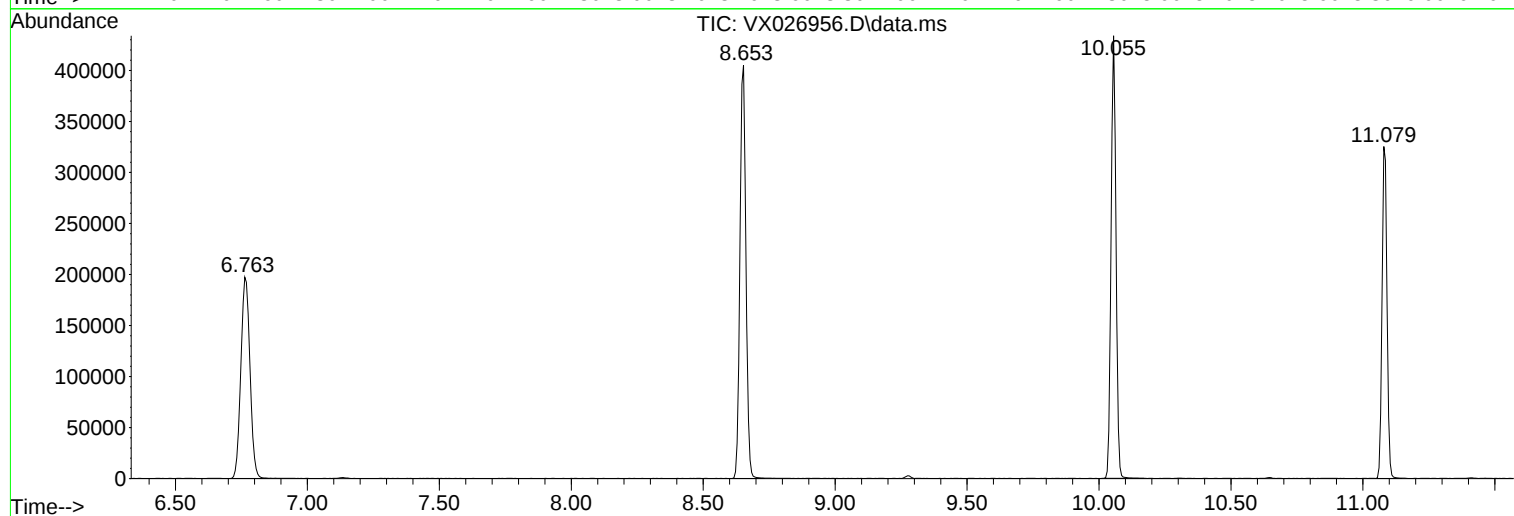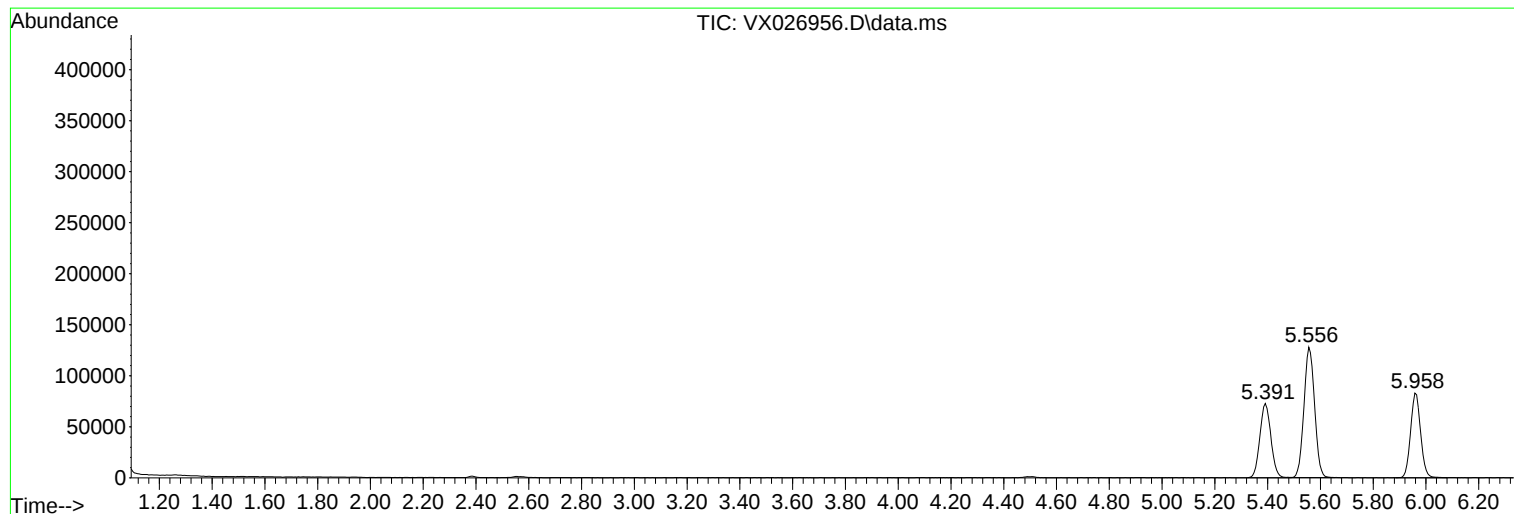

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
Data File : VX026956.D
Acq On : 11 Feb 2022 06:12
Operator : JC/MD
Sample : N1497-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-BLIND-DUPLICATE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021022\
Data File : VX026956.D
Acq On : 11 Feb 2022 06:12
Operator : JC/MD
Sample : N1497-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-BLIND-DUPLICATE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------