

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021023\
 Data File : VX034079.D
 Acq On : 08 Feb 2023 12:46
 Operator : JC/MD
 Sample : 01419-01 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DRUM-COMP

Quant Time: Feb 08 13:29:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 03 23:25:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	126571	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	174828	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	157683	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	81801	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	59853	49.052	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	98.100%
35) Dibromofluoromethane	5.379	113	55053	49.479	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.960%
50) Toluene-d8	8.647	98	198706	49.567	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.140%
62) 4-Bromofluorobenzene	11.079	95	71554	49.976	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.960%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021023\
Data File : VX034079.D
Acq On : 08 Feb 2023 12:46
Operator : JC/MD
Sample : 01419-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DRUM-COMP

Quant Time: Feb 08 13:29:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 03 23:25:45 2023
Response via : Initial Calibration




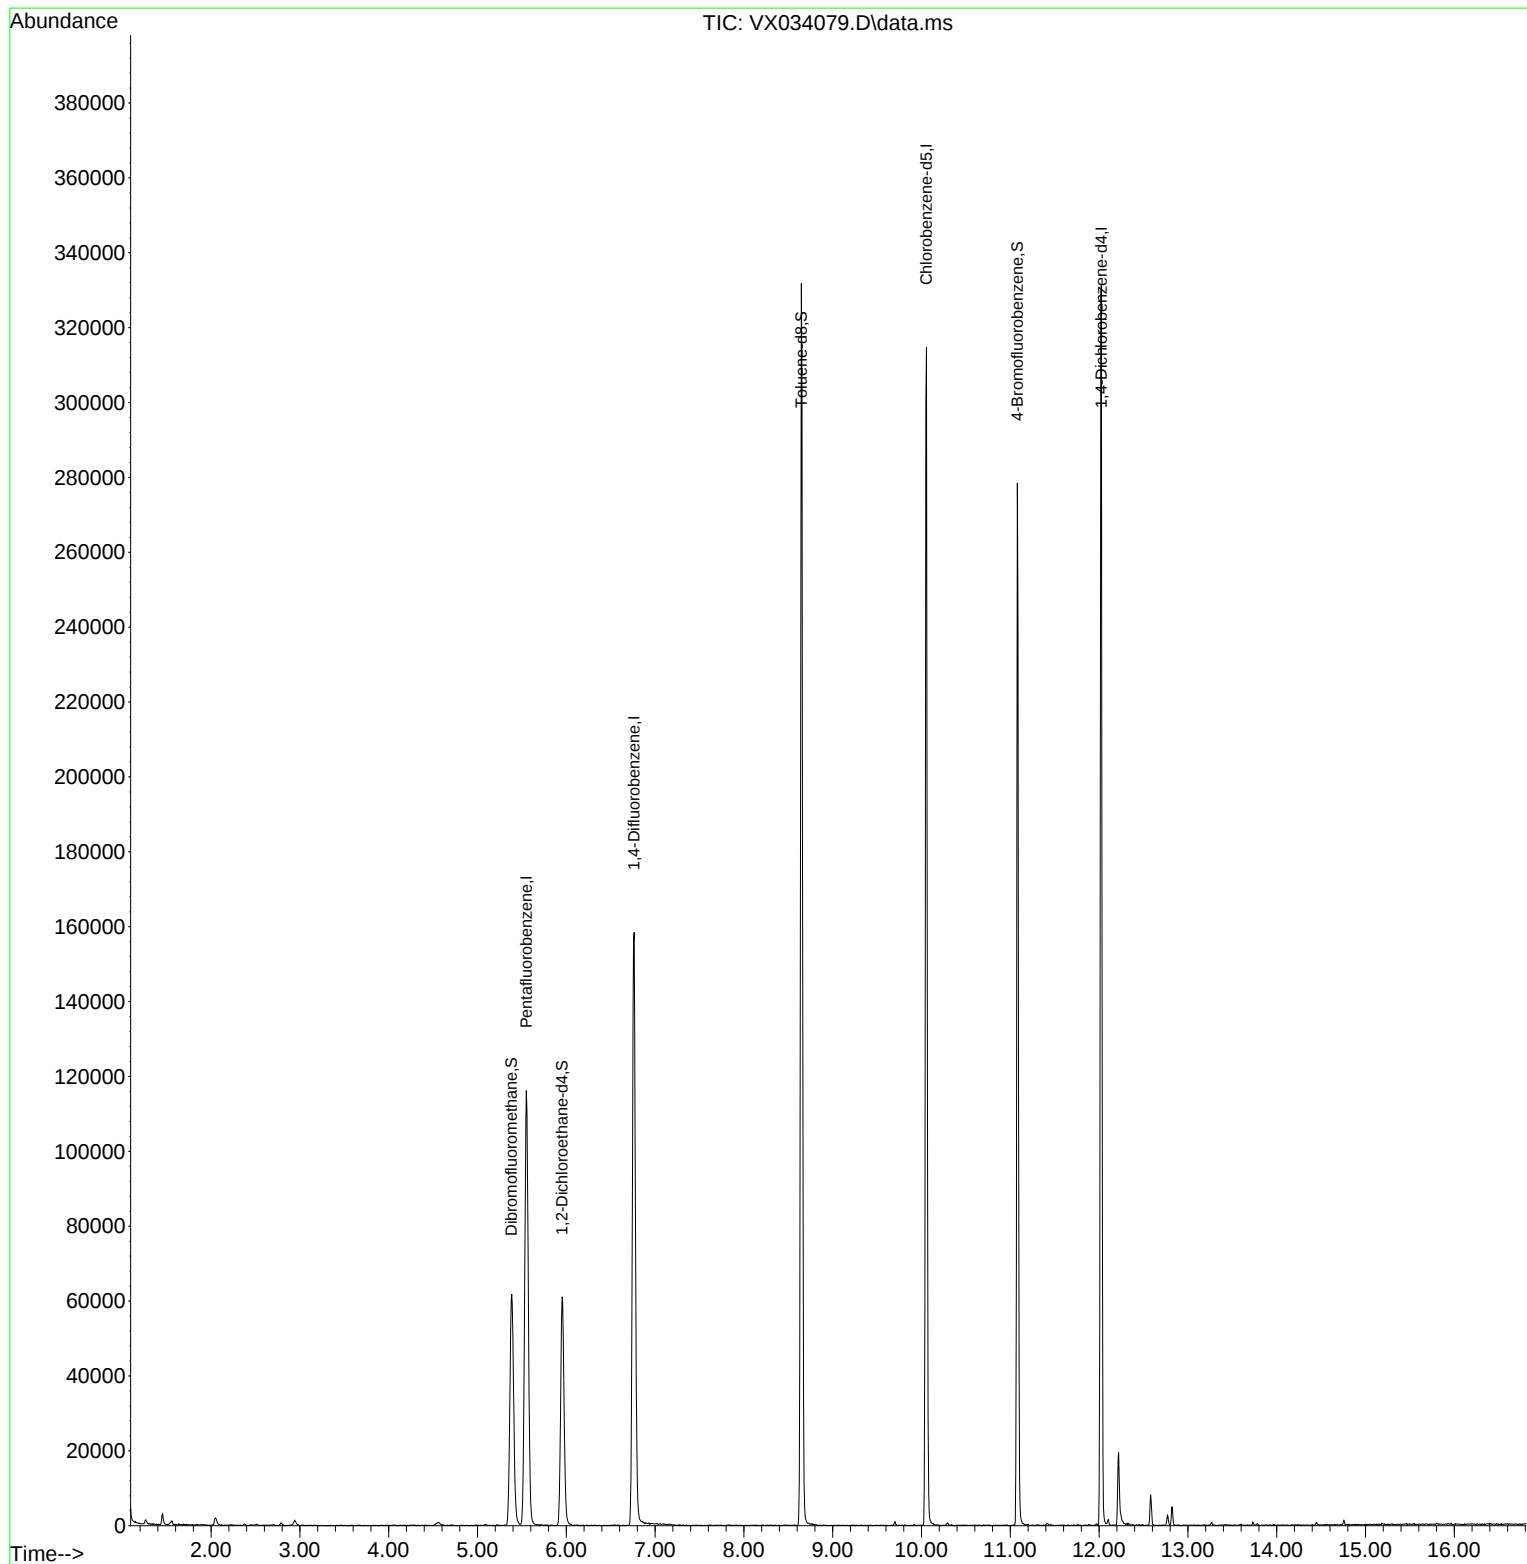


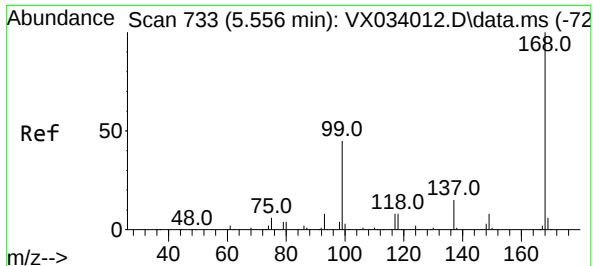

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX034079.D
Acq: 08 Feb 2023 12:46




Instrument :
MSVOA_X
ClientSampleId :
DRUM-COMP


Tgt Ion:168 Resp: 126571
Ion Ratio Lower Upper
168 100
99 48.9 39.6 59.4

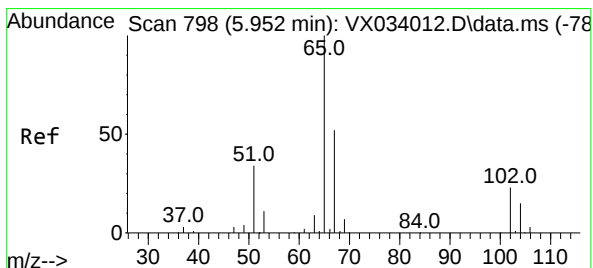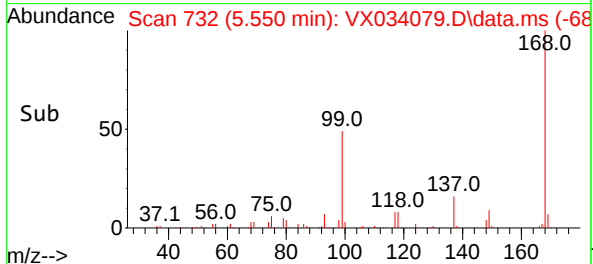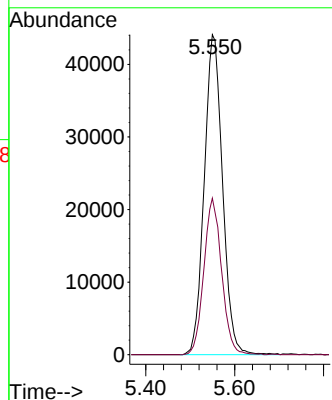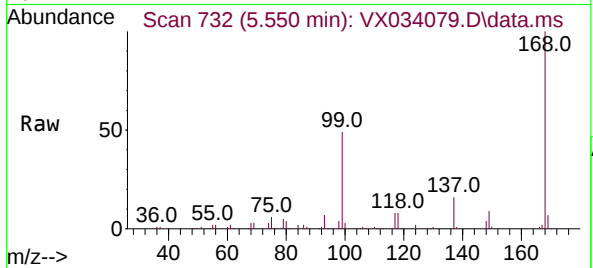

#33
1,2-Dichloroethane-d4
Concen: 49.052 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX034079.D
Acq: 08 Feb 2023 12:46

Tgt Ion: 65 Resp: 59853
Ion Ratio Lower Upper
65 100
67 51.8 0.0 104.8

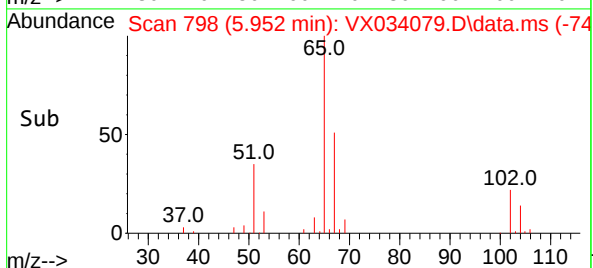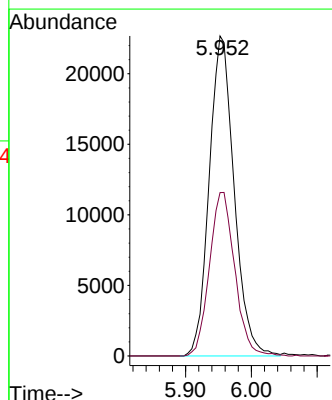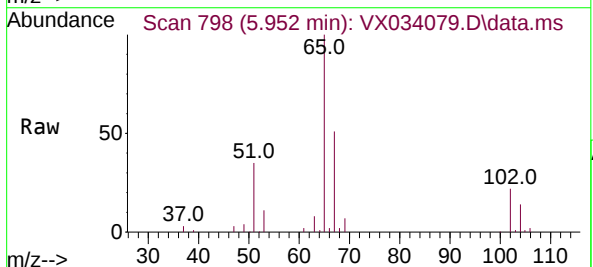

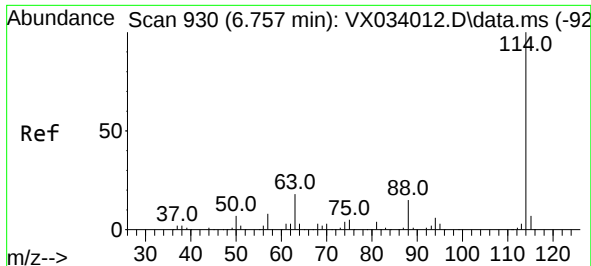

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 91

Delta R.T. 0.006 min

Lab File: VX034079.D

Acq: 08 Feb 2023 12:46

Instrument :

MSVOA_X

ClientSampleId :

DRUM-COMP





Tgt Ion:114 Resp: 174828

Ion Ratio Lower Upper

114 100

63 17.4 0.0 37.4

88 14.9 0.0 30.6

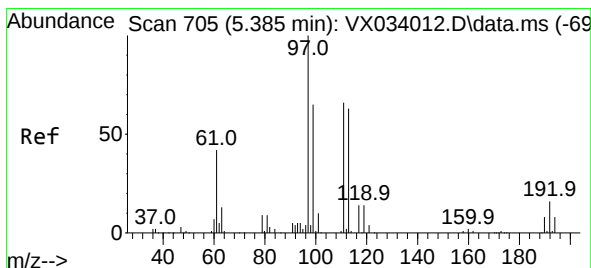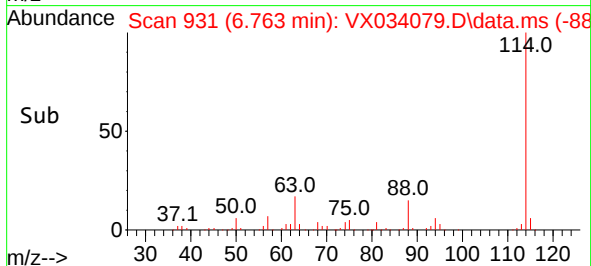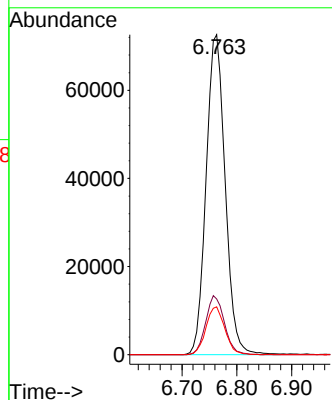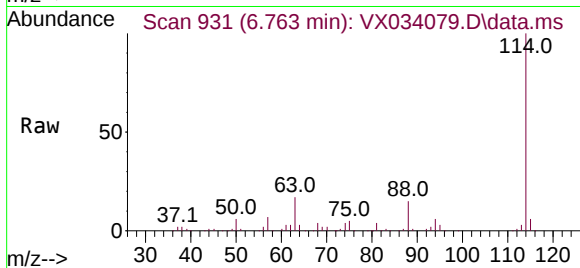

#35

Dibromofluoromethane

Concen: 49.479 ug/l

RT: 5.379 min Scan# 704

Delta R.T. -0.006 min

Lab File: VX034079.D

Acq: 08 Feb 2023 12:46




Tgt Ion:113 Resp: 55053


Ion Ratio Lower Upper

113 100

111 103.0 83.0 124.6

192 25.8 19.0 28.4


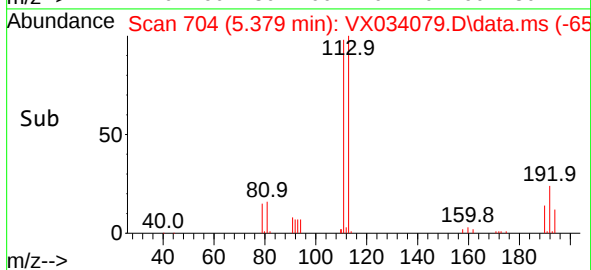
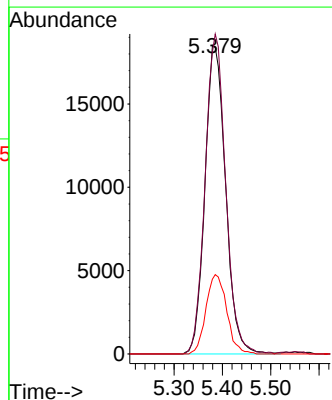
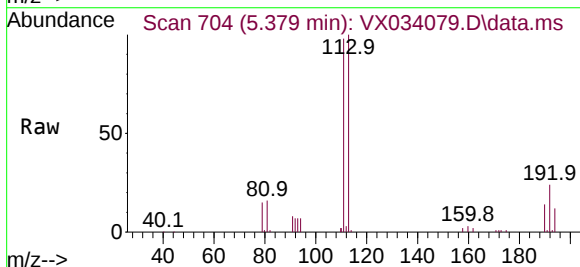


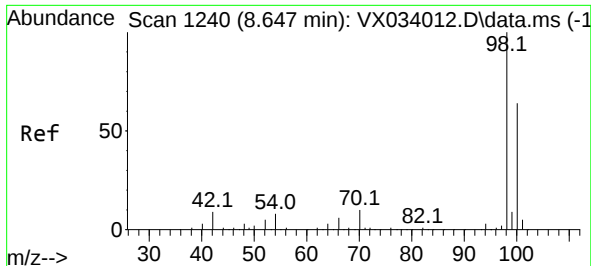

#50
Toluene-d8
Concen: 49.567 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX034079.D
Acq: 08 Feb 2023 12:46




Instrument :
MSVOA_X
ClientSampleId :
DRUM-COMP


Tgt Ion: 98 Resp: 198706
Ion Ratio Lower Upper
98 100
100 67.1 53.6 80.4

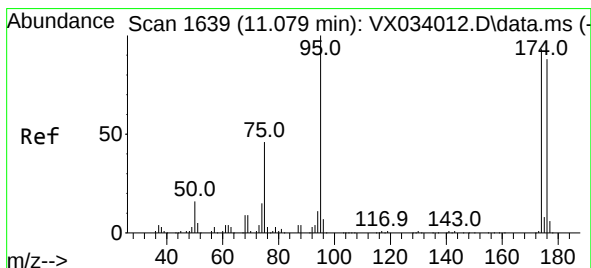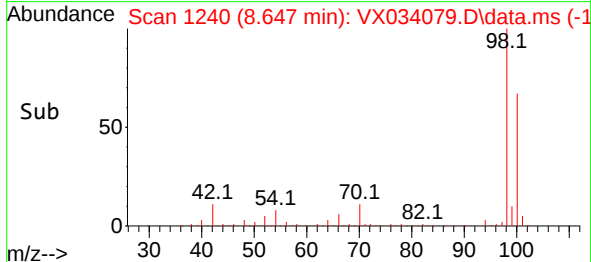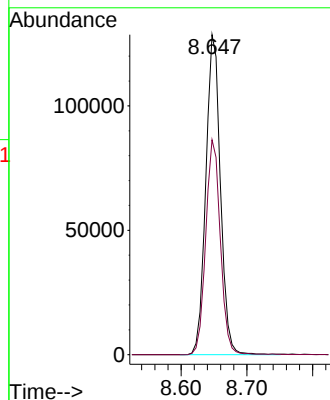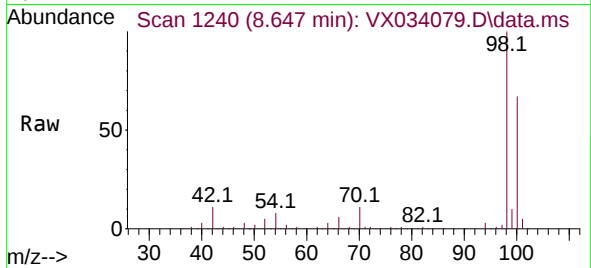

#62
4-Bromofluorobenzene
Concen: 49.976 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX034079.D
Acq: 08 Feb 2023 12:46

Tgt Ion: 95 Resp: 71554
Ion Ratio Lower Upper
95 100
174 98.2 0.0 184.4
176 96.1 0.0 178.8


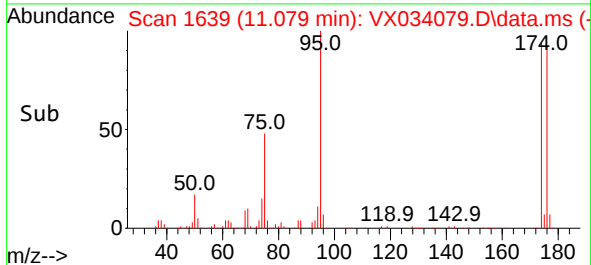
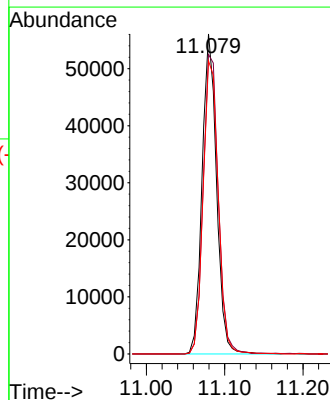
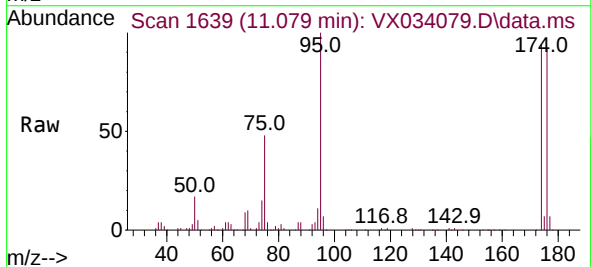


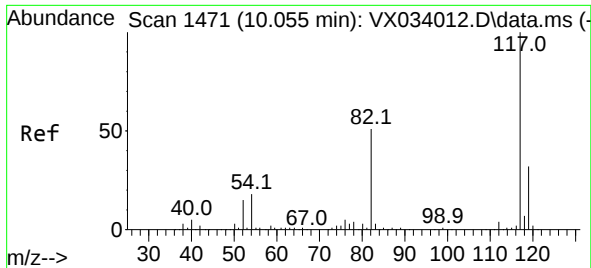

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX034079.D
Acq: 08 Feb 2023 12:46

Instrument :
MSVOA_X
ClientSampleId :
DRUM-COMP

Tgt Ion:117 Resp: 157683
Ion Ratio Lower Upper
117 100
82 50.5 40.6 60.8
119 32.4 25.6 38.4

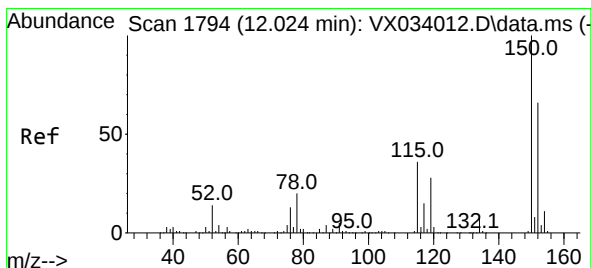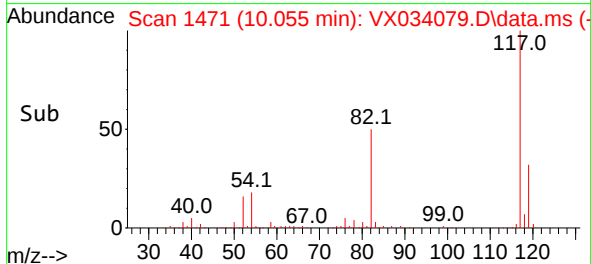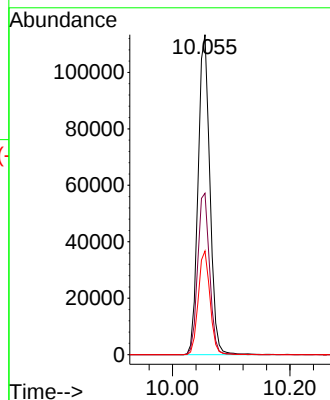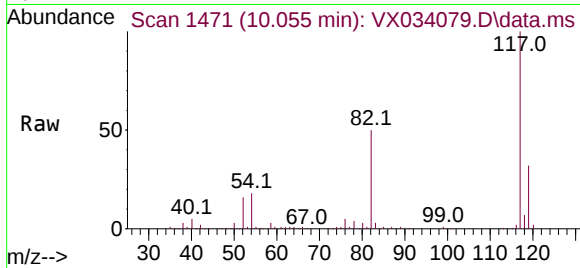

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX034079.D
Acq: 08 Feb 2023 12:46

Tgt Ion:152 Resp: 81801
Ion Ratio Lower Upper
152 100
115 53.3 38.7 116.1
150 154.4 0.0 348.2

