
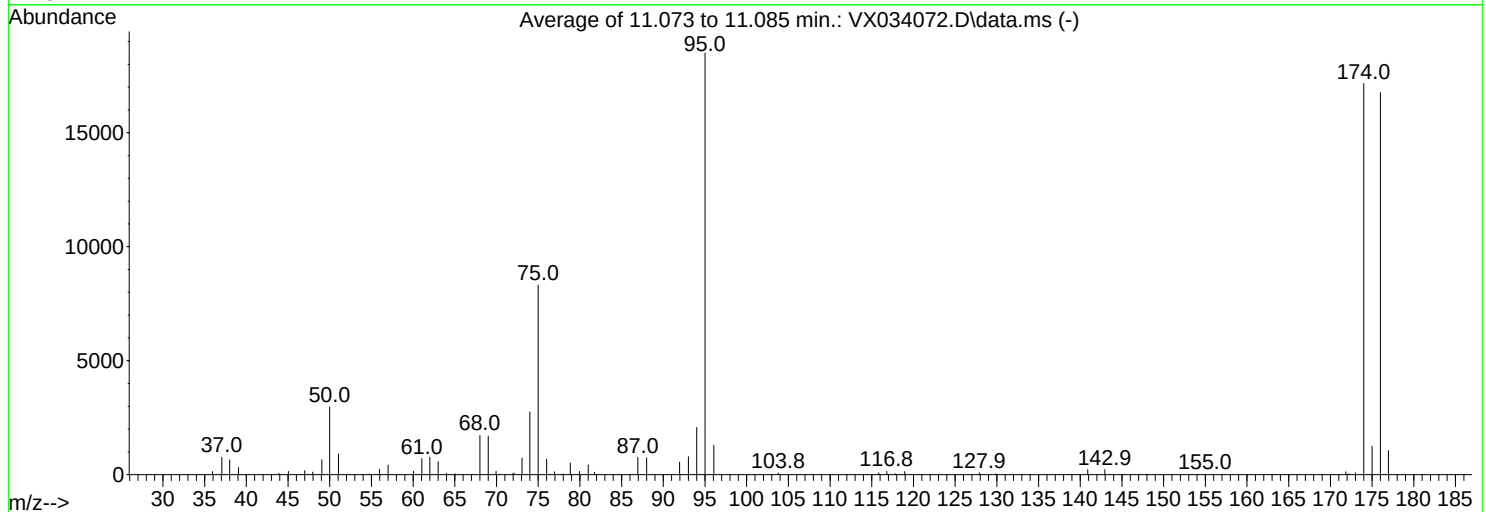


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021023\
Data File : VX034072.D
Acq On : 08 Feb 2023 09:43
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
Title : SW846 8260
Last Update : Fri Feb 03 23:25:45 2023

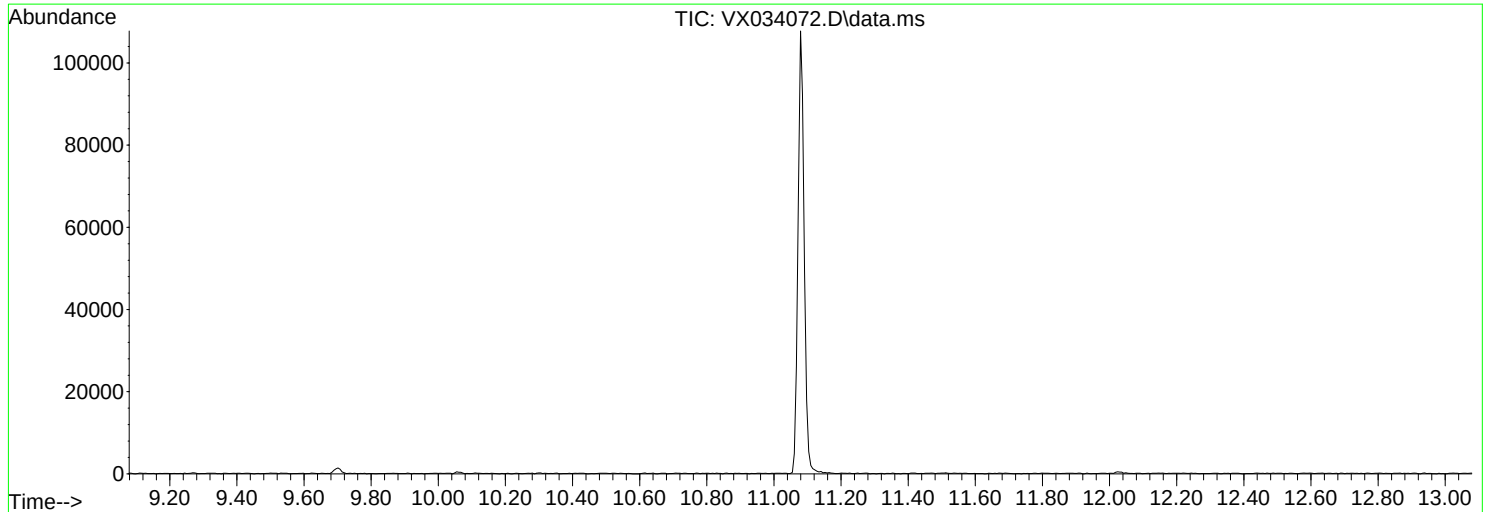

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	2968	PASS
75	95	30	60	44.9	8315	PASS
95	95	100	100	100.0	18505	PASS
96	95	5	9	7.0	1292	PASS
173	174	0.00	2	0.5	84	PASS
174	95	50	100	92.7	17160	PASS
175	174	5	9	7.2	1244	PASS
176	174	95	101	97.7	16763	PASS
177	176	5	9	6.3	1052	PASS