

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021025\
 Data File : VX044881.D
 Acq On : 10 Feb 2025 15:41
 Operator : JC/MD
 Sample : Q1250-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-192-TB-20250127

Quant Time: Feb 11 06:06:36 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021025W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 11 03:41:08 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	92731	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	189692	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	170630	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	69234	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	71967	53.018	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 106.040%	
35) Dibromofluoromethane	5.379	113	61025	49.481	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 98.960%	
50) Toluene-d8	8.647	98	234221	50.223	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 100.440%	
62) 4-Bromofluorobenzene	11.079	95	79575	50.613	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 101.220%	
Target Compounds						
16) Acetone	2.386	43	1601	2.934	ug/l	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021025\
Data File : VX044881.D
Acq On : 10 Feb 2025 15:41
Operator : JC/MD
Sample : Q1250-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-192-TB-20250127

Quant Time: Feb 11 06:06:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021025W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 11 03:41:08 2025
Response via : Initial Calibration




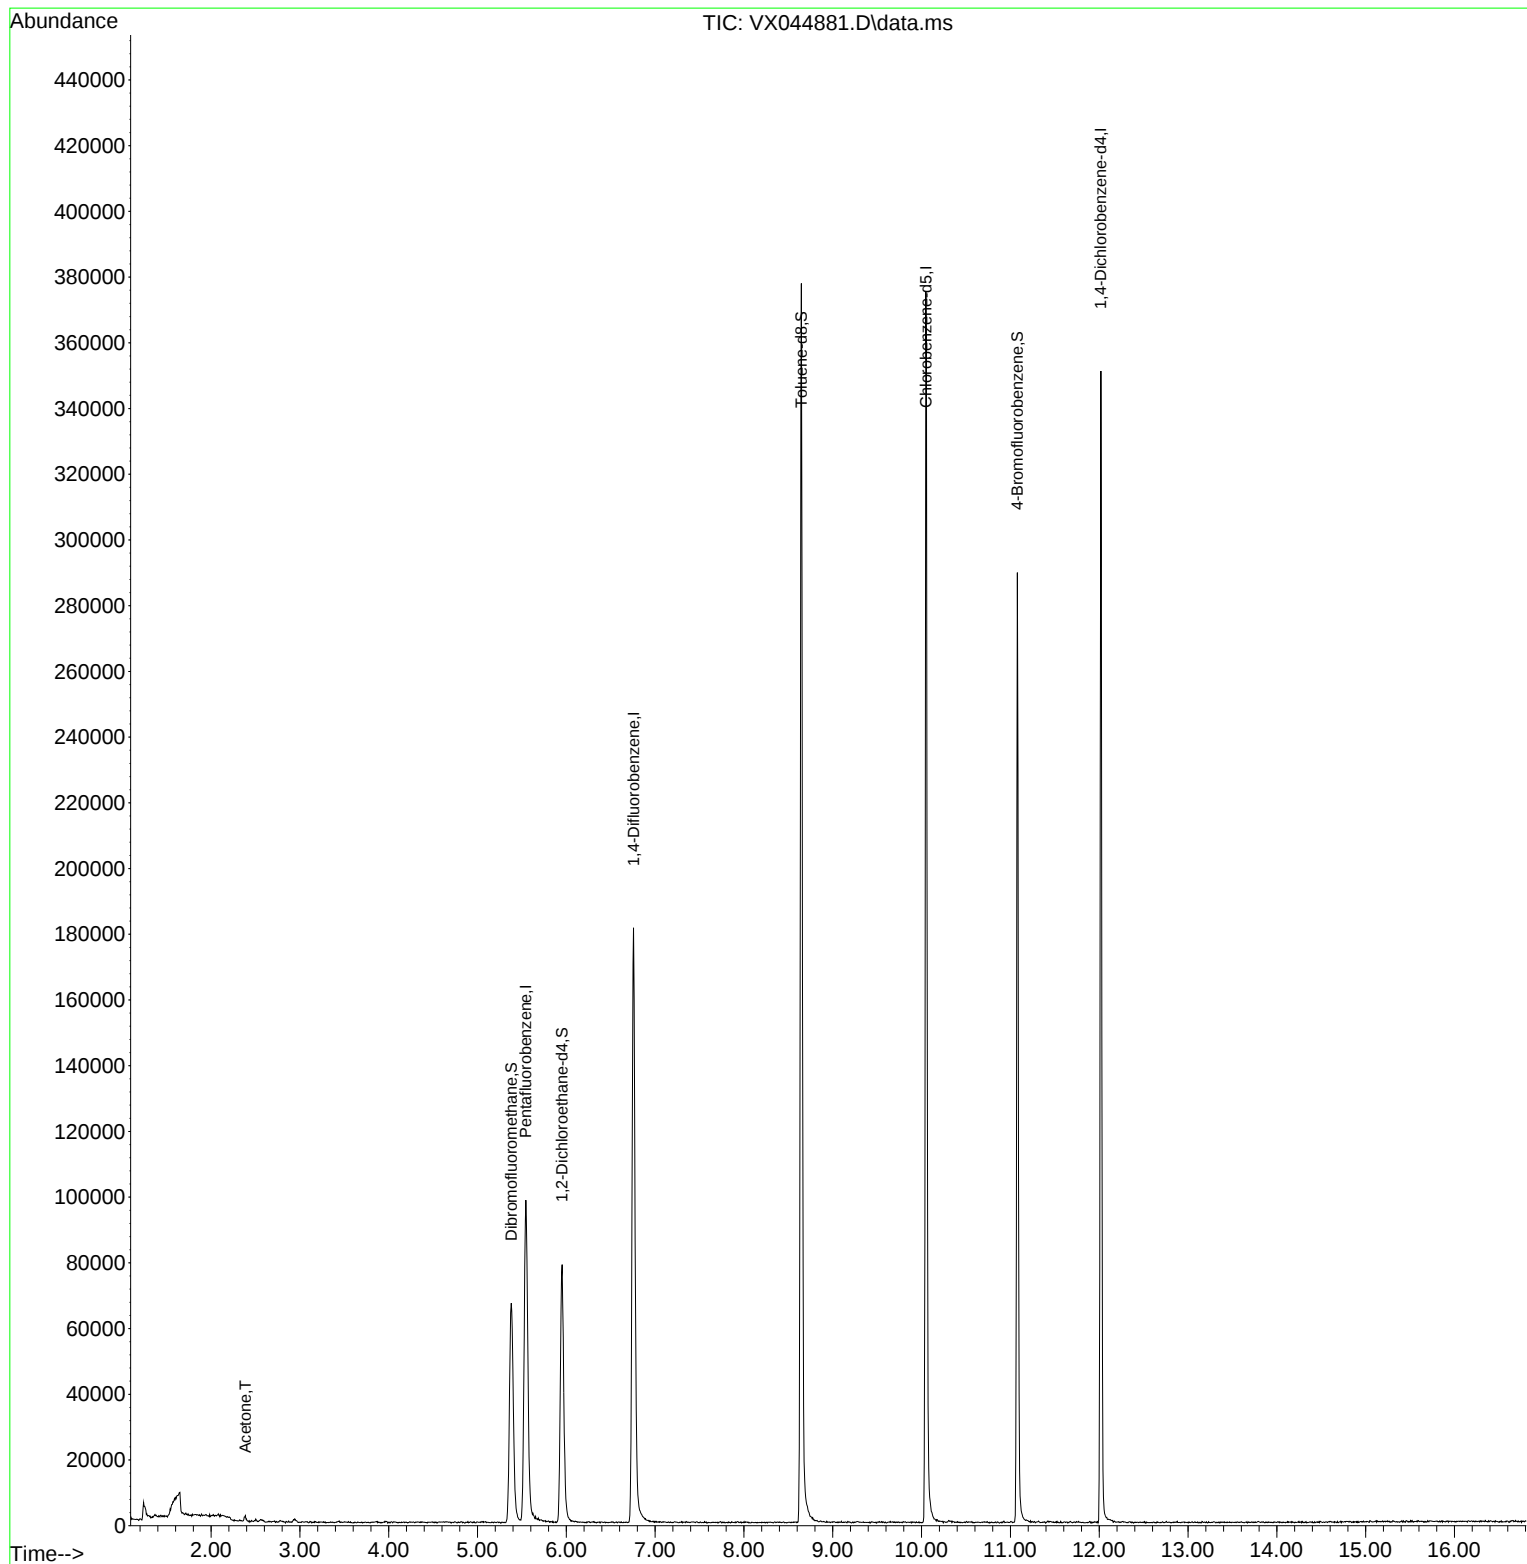


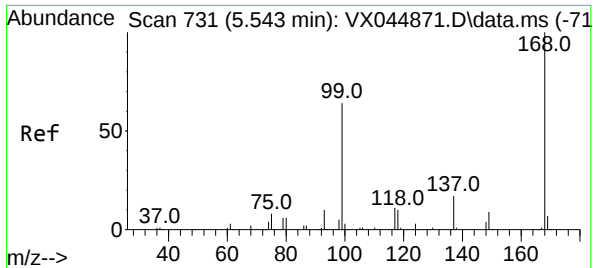

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. 0.001 min
Lab File: VX044881.D
Acq: 10 Feb 2025 15:41




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-192-TB-20250127


Tgt Ion:168 Resp: 92731
Ion Ratio Lower Upper
168 100
99 65.0 51.2 76.8

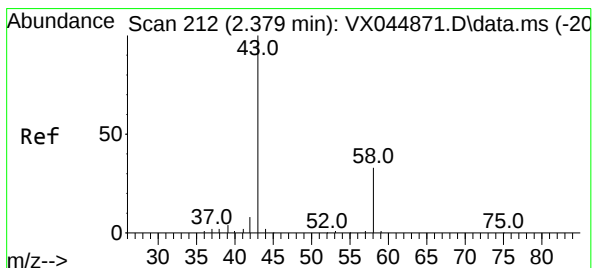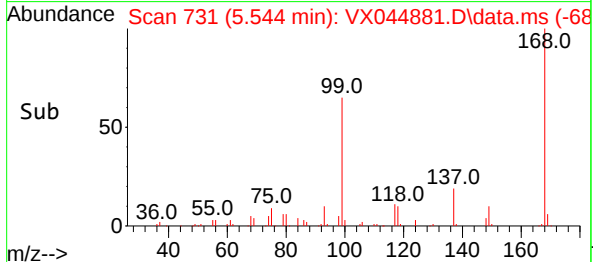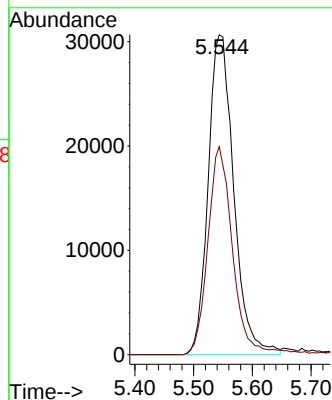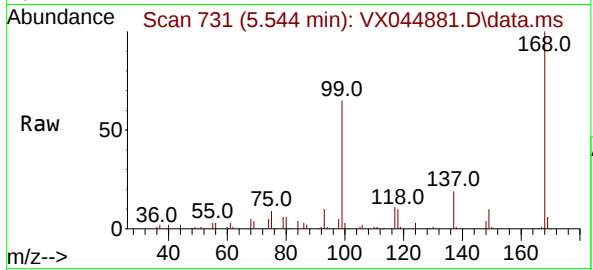

#16
Acetone
Concen: 2.934 ug/l
RT: 2.386 min Scan# 213
Delta R.T. 0.006 min
Lab File: VX044881.D
Acq: 10 Feb 2025 15:41

Tgt Ion: 43 Resp: 1601
Ion Ratio Lower Upper
43 100
58 36.7 26.5 39.7


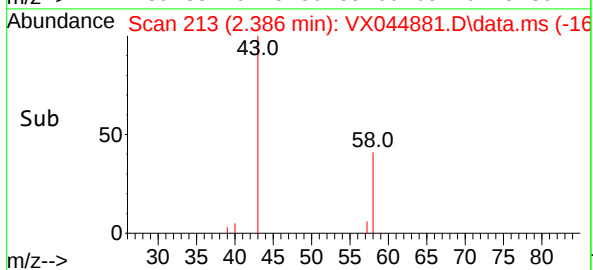
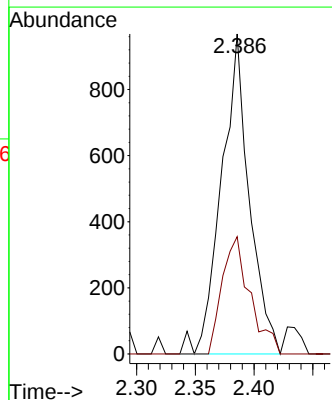
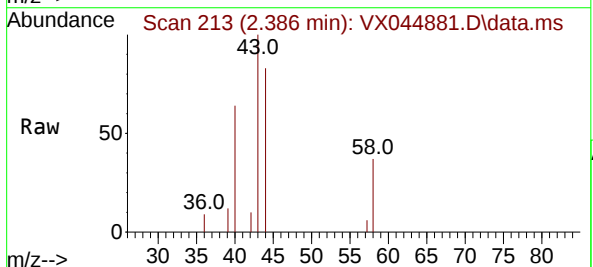


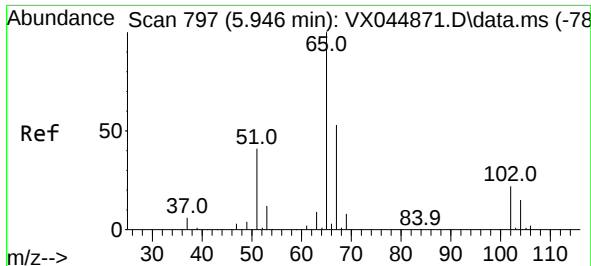

#33
 1,2-Dichloroethane-d4
 Concen: 53.018 ug/l
 RT: 5.952 min Scan# 797
 Delta R.T. 0.006 min
 Lab File: VX044881.D
 Acq: 10 Feb 2025 15:41




Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-192-TB-20250127


Tgt Ion: 65 Resp: 71967
 Ion Ratio Lower Upper
 65 100
 67 54.1 0.0 108.2

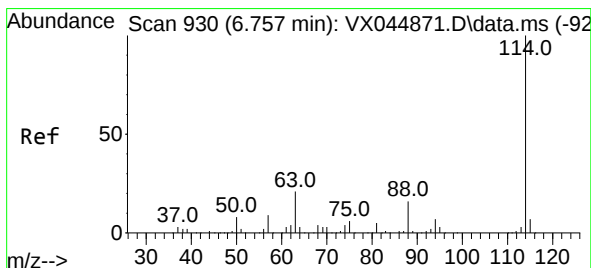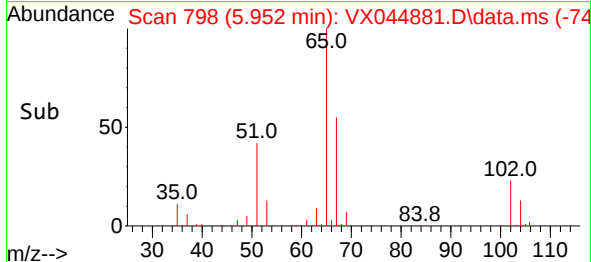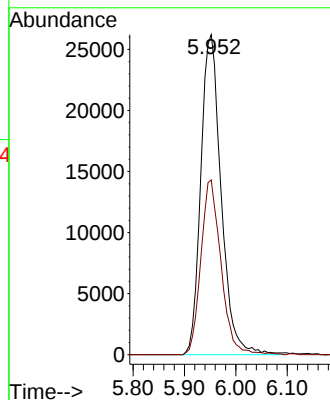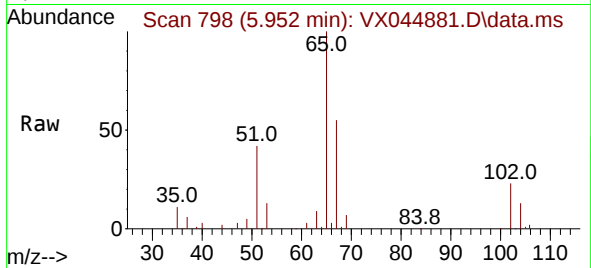

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.757 min Scan# 930
 Delta R.T. 0.000 min
 Lab File: VX044881.D
 Acq: 10 Feb 2025 15:41

Tgt Ion: 114 Resp: 189692
 Ion Ratio Lower Upper
 114 100
 63 20.7 0.0 42.4
 88 15.5 0.0 31.4


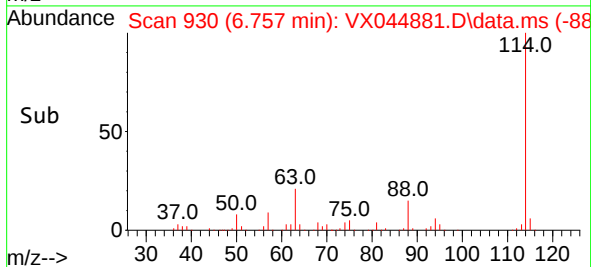
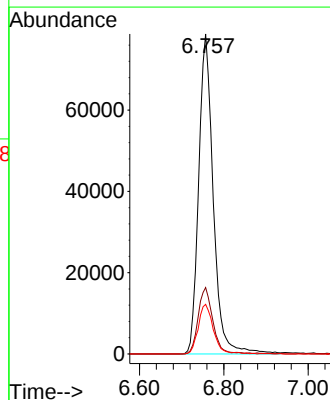
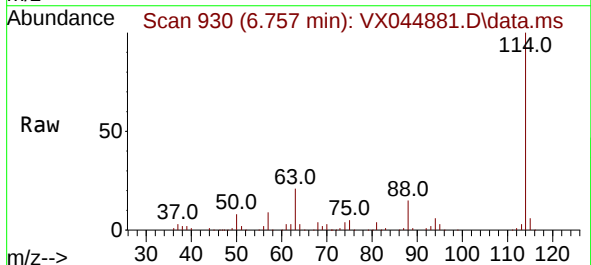


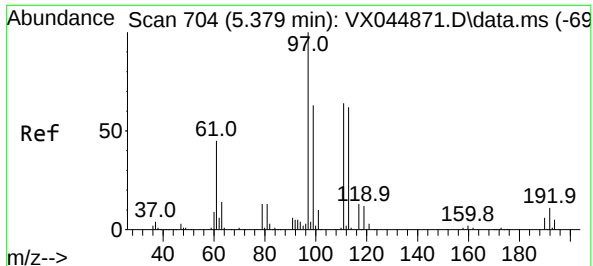

#35
Dibromofluoromethane
Concen: 49.481 ug/l
RT: 5.379 min Scan# 704
Delta R.T. 0.000 min
Lab File: VX044881.D
Acq: 10 Feb 2025 15:41




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-192-TB-20250127


Tgt Ion:113 Resp: 61025
Ion Ratio Lower Upper
113 100
111 104.7 83.5 125.3
192 18.4 14.4 21.6

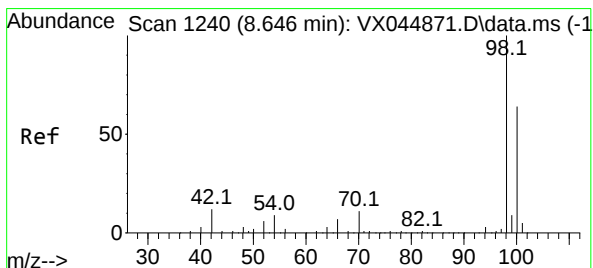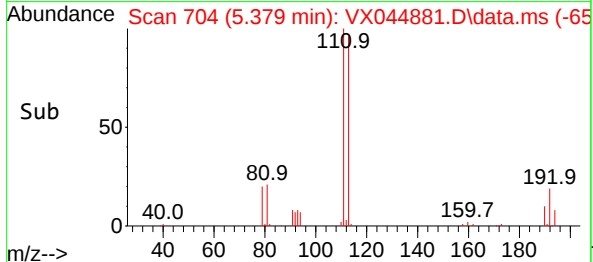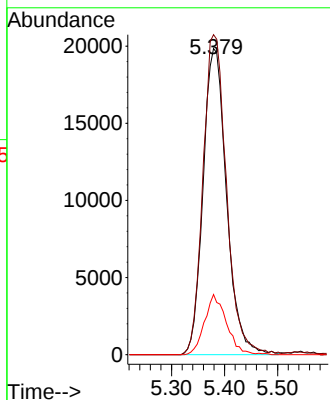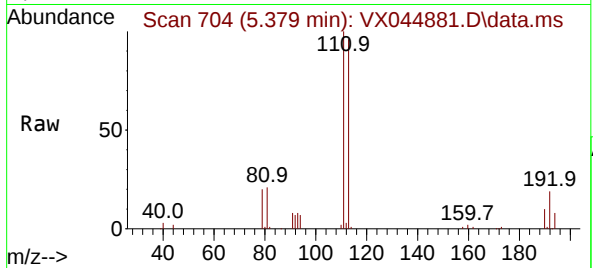

#50
Toluene-d8
Concen: 50.223 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX044881.D
Acq: 10 Feb 2025 15:41

Tgt Ion: 98 Resp: 234221
Ion Ratio Lower Upper
98 100
100 65.3 52.7 79.1


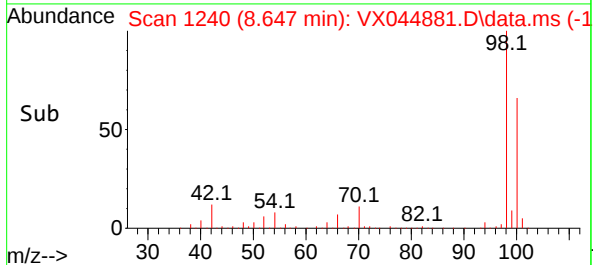
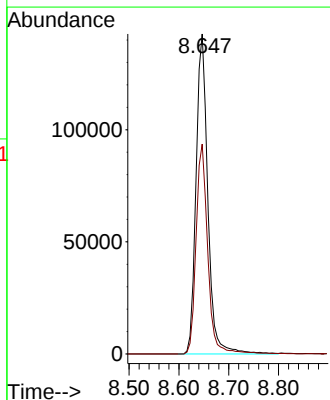
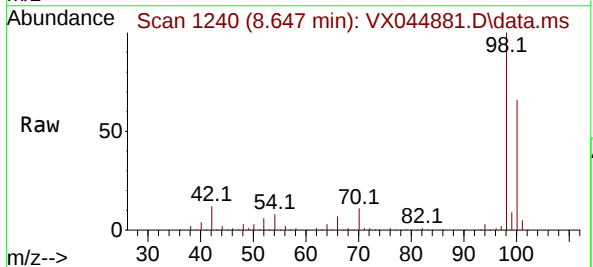


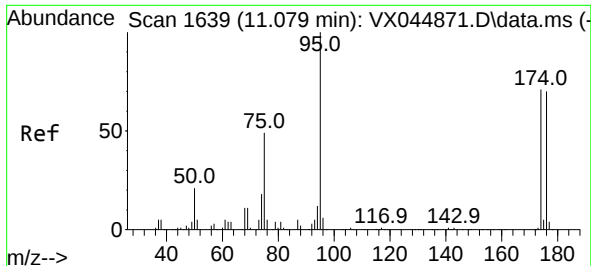

#62
4-Bromofluorobenzene
Concen: 50.613 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX044881.D
Acq: 10 Feb 2025 15:41




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-192-TB-20250127


Tgt Ion: 95 Resp: 79575
Ion Ratio Lower Upper
95 100
174 72.0 0.0 142.6
176 71.3 0.0 141.6

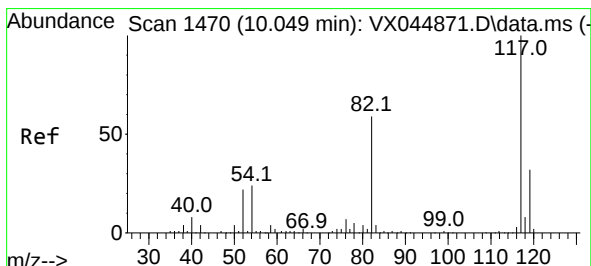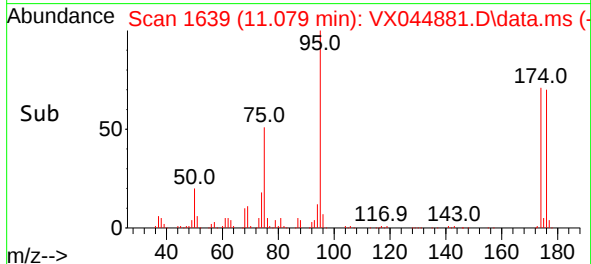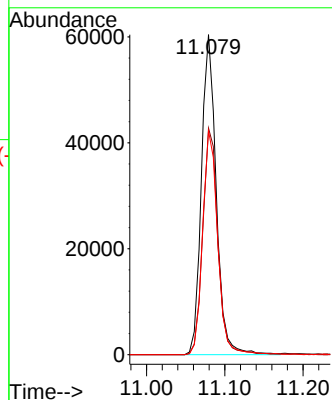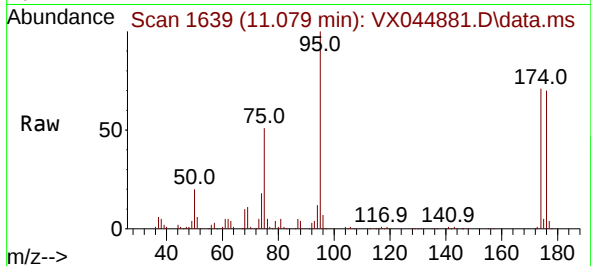

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX044881.D
Acq: 10 Feb 2025 15:41


Tgt Ion: 117 Resp: 170630
Ion Ratio Lower Upper
117 100
82 58.6 47.5 71.3
119 31.4 25.4 38.0

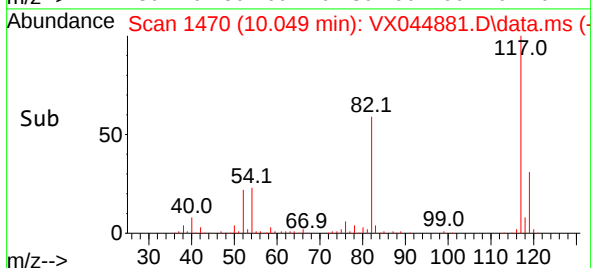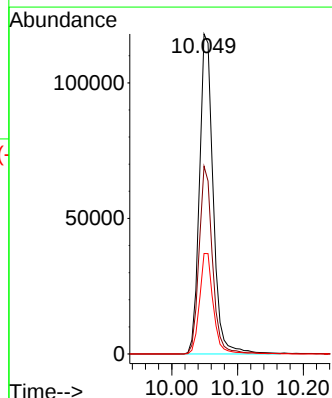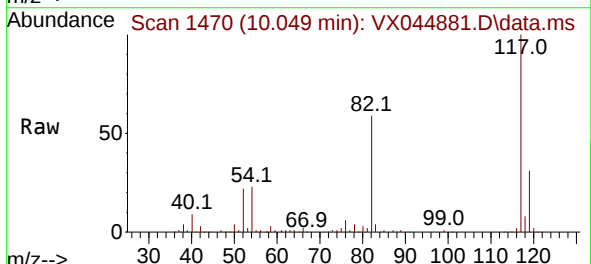

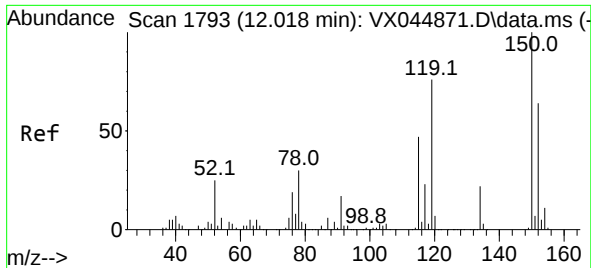

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.018 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX044881.D
 Acq: 10 Feb 2025 15:41

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-192-TB-20250127

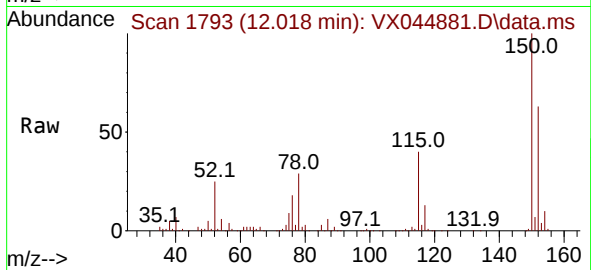

Tgt Ion:152 Resp: 69234
 Ion Ratio Lower Upper
 152 100
 115 62.0 43.4 130.1
 150 156.9 0.0 350.4

