

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX021119\
 Data File : VX007465.D
 Acq On : 11 Feb 2019 14:00
 Operator : JC/SP
 Sample : K1433-07
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 KY001IW064-190207

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.288	17	22	27	rBV2	25819	31431	1.27%	0.217%
2	1.611	67	75	83	rBV3	25809	57820	2.34%	0.399%
3	3.068	308	314	322	rVB	13768	34670	1.40%	0.239%
4	3.208	328	337	347	rVB	262873	622044	25.14%	4.293%
5	5.501	701	713	727	rBV2	305279	877392	35.46%	6.055%
6	5.665	729	740	758	rVB	515647	1434834	57.99%	9.902%
7	6.068	794	806	815	rBV	309802	790362	31.94%	5.455%
8	6.366	844	855	863	rBV6	15362	62271	2.52%	0.430%
9	6.860	925	936	949	rBV	762839	1785712	72.17%	12.324%
10	8.713	1232	1240	1250	rBV	1591591	2474322	100.00%	17.076%
11	8.915	1266	1273	1280	rVB	22328	38557	1.56%	0.266%
12	9.628	1386	1390	1396	rBV3	18595	27135	1.10%	0.187%
13	10.110	1464	1469	1475	rVV	1563819	2152395	86.99%	14.854%
14	11.024	1612	1619	1623	rVB4	13256	24835	1.00%	0.171%
15	11.134	1632	1637	1644	rBV	1319104	1746966	70.60%	12.056%
16	11.359	1669	1674	1684	rVB2	17199	27343	1.11%	0.189%
17	12.079	1786	1792	1799	rBV	1696147	2109398	85.25%	14.558%
18	12.298	1822	1828	1832	rBV	30551	41539	1.68%	0.287%
19	12.755	1900	1903	1910	rVB2	19800	35069	1.42%	0.242%
20	13.834	2072	2080	2089	rBV	59170	90609	3.66%	0.625%
21	14.694	2218	2221	2230	rVB	17006	25180	1.02%	0.174%


Sum of corrected areas: 14489884

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX021119\
Data File : VX007465.D
Acq On : 11 Feb 2019 14:00
Operator : JC/SP
Sample : K1433-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KY001IW064-190207

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

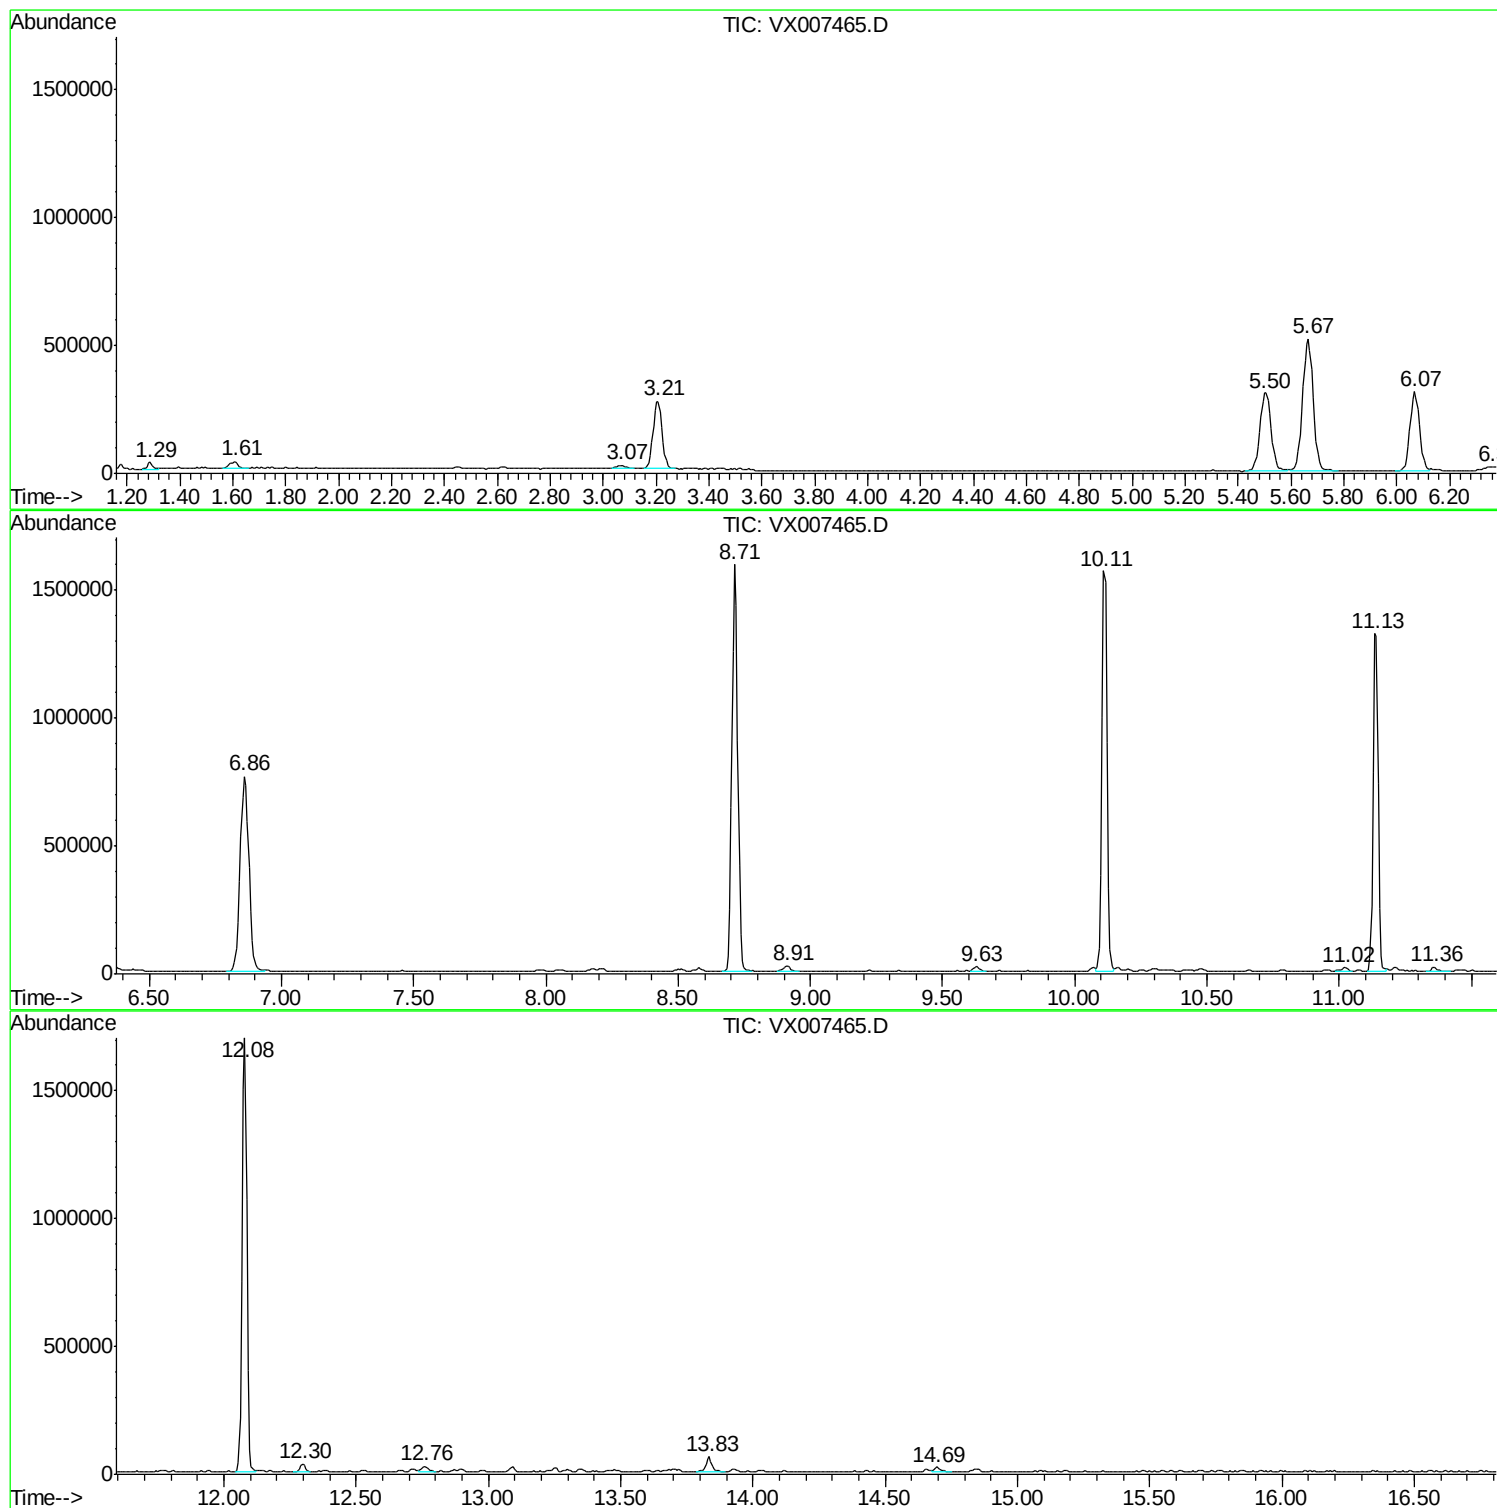

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX021119\
Data File : VX007465.D
Acq On : 11 Feb 2019 14:00
Operator : JC/SP
Sample : K1433-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KY001IW064-190207

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX021119\
Data File : VX007465.D
Acq On : 11 Feb 2019 14:00
Operator : JC/SP
Sample : K1433-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KY001IW064-190207

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc