

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX021119\
 Data File : VX007479.D
 Acq On : 11 Feb 2019 20:12
 Operator : JC/SP
 Sample : K1449-05
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 B-11-OW

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	16	20	23	rBV	206087	235083	9.38%	1.391%
2	1.324	23	28	43	rVV	265996	930063	37.10%	5.504%
3	1.593	68	72	73	rBV2	47503	56495	2.25%	0.334%
4	2.617	235	240	245	rVB	29508	51142	2.04%	0.303%
5	5.153	644	656	672	rBV	673525	2013266	80.32%	11.914%
6	5.507	699	714	725	rBV	317396	908800	36.26%	5.378%
7	5.665	730	740	754	rVB	526243	1457396	58.14%	8.625%
8	6.067	797	806	819	rVB	313989	796257	31.77%	4.712%
9	6.860	925	936	950	rBV	775199	1821486	72.67%	10.780%
10	8.713	1233	1240	1249	rBV	1638277	2506683	100.00%	14.835%
11	10.109	1463	1469	1478	rBV	1595568	2201963	87.84%	13.031%
12	11.134	1632	1637	1649	rVB	1354009	1763594	70.36%	10.437%
13	12.079	1786	1792	1799	rBV	1666882	2155402	85.99%	12.756%


Sum of corrected areas: 16897630

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX021119\
Data File : VX007479.D
Acq On : 11 Feb 2019 20:12
Operator : JC/SP
Sample : K1449-05
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
B-11-OW

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

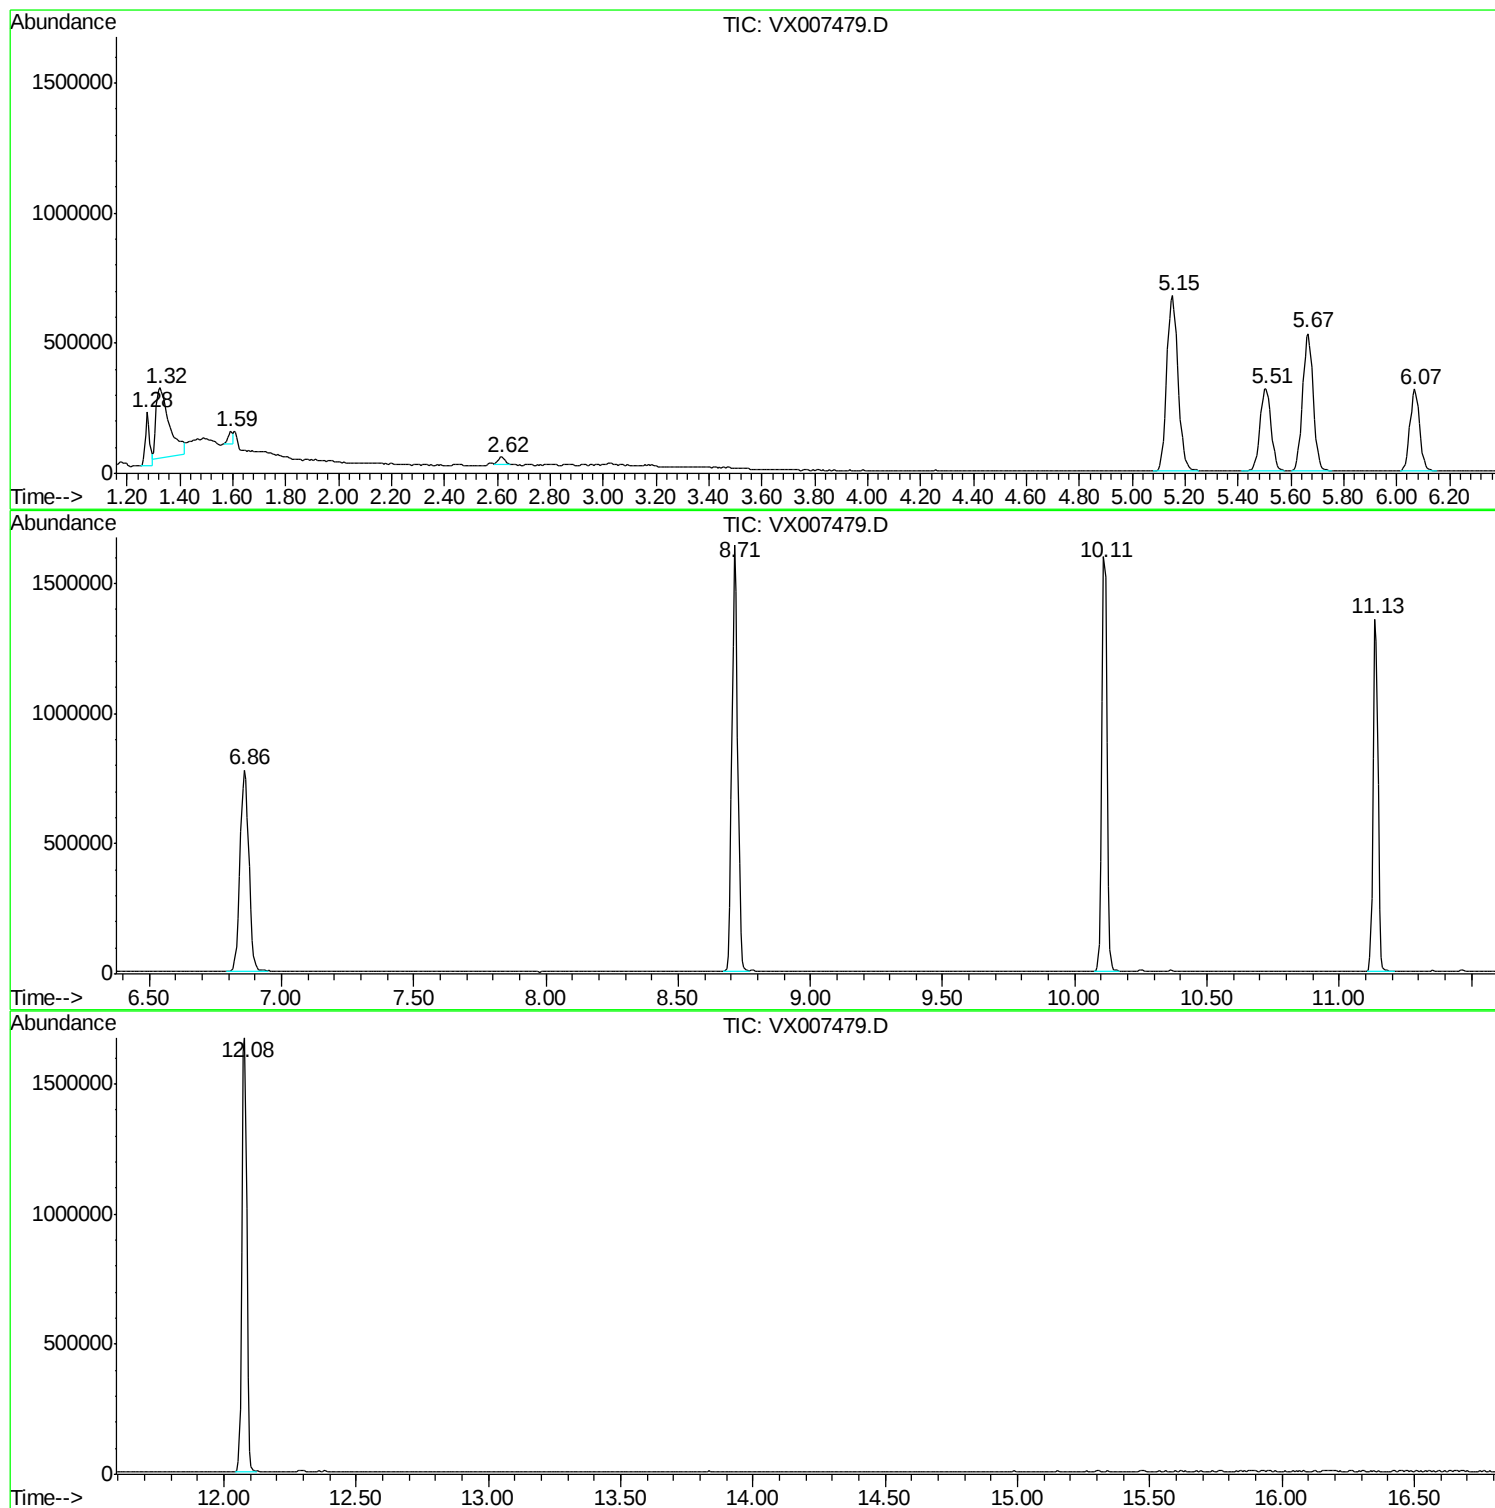

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX021119\
Data File : VX007479.D
Acq On : 11 Feb 2019 20:12
Operator : JC/SP
Sample : K1449-05
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 24 Sample Multiplier: 1










Instrument :
MSVOA_X
ClientSampleId :
B-11-OW

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.		
1.28	8.07 ug/l	235083	Pentafluorobenzene	5.67		
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Sulfur dioxide		64	O2S	007446-09-5	90
2	Aminomethanesulfonic acid		111	CH5NO3S	013881-91-9	74
3	L-Alanine, 3-sulfo-		169	C3H7NO5S	000498-40-8	9
4	Ethene, 1,1-difluoro-		64	C2H2F2	000075-38-7	4
5	Ethyl Chloride		64	C2H5Cl	000075-00-3	3

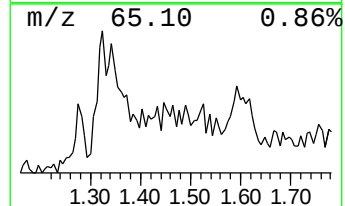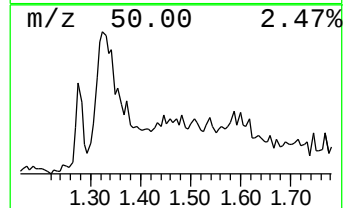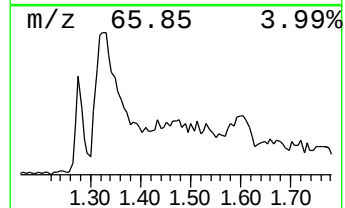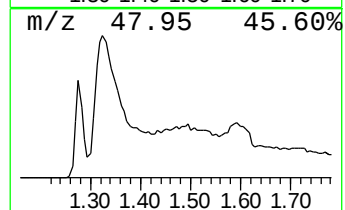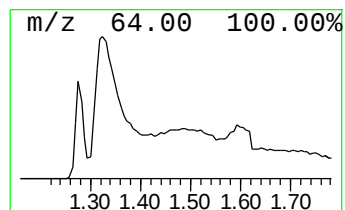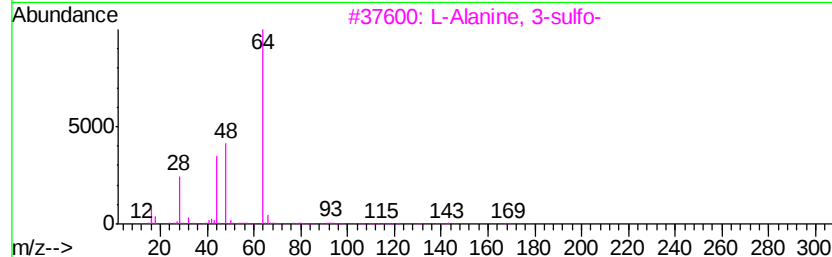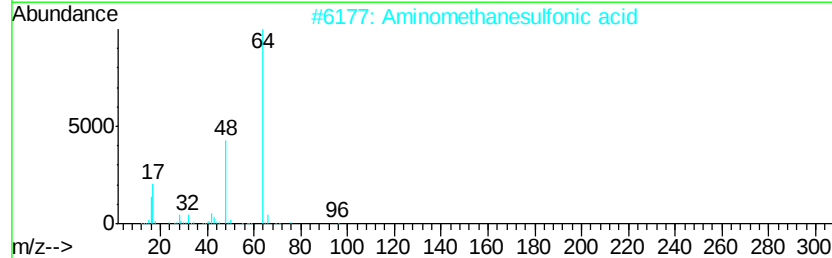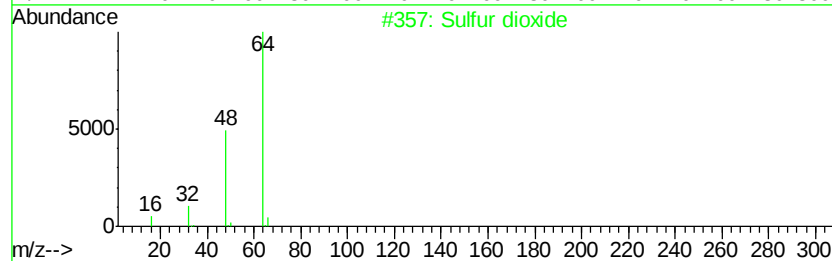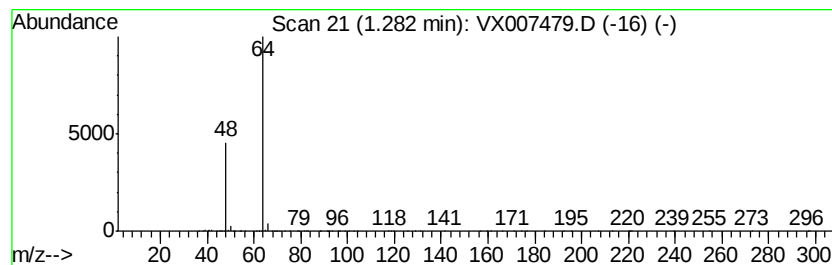

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX021119\
Data File : VX007479.D
Acq On : 11 Feb 2019 20:12
Operator : JC/SP
Sample : K1449-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
B-11-OW

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.28	8.1	ug/l	235083	1	5.67	1457400	50.0