


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX021119\
Data File : VX007456.D
Acq On : 11 Feb 2019 09:31
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Title : SW846 8260
Last Update : Sat Feb 02 01:32:36 2019

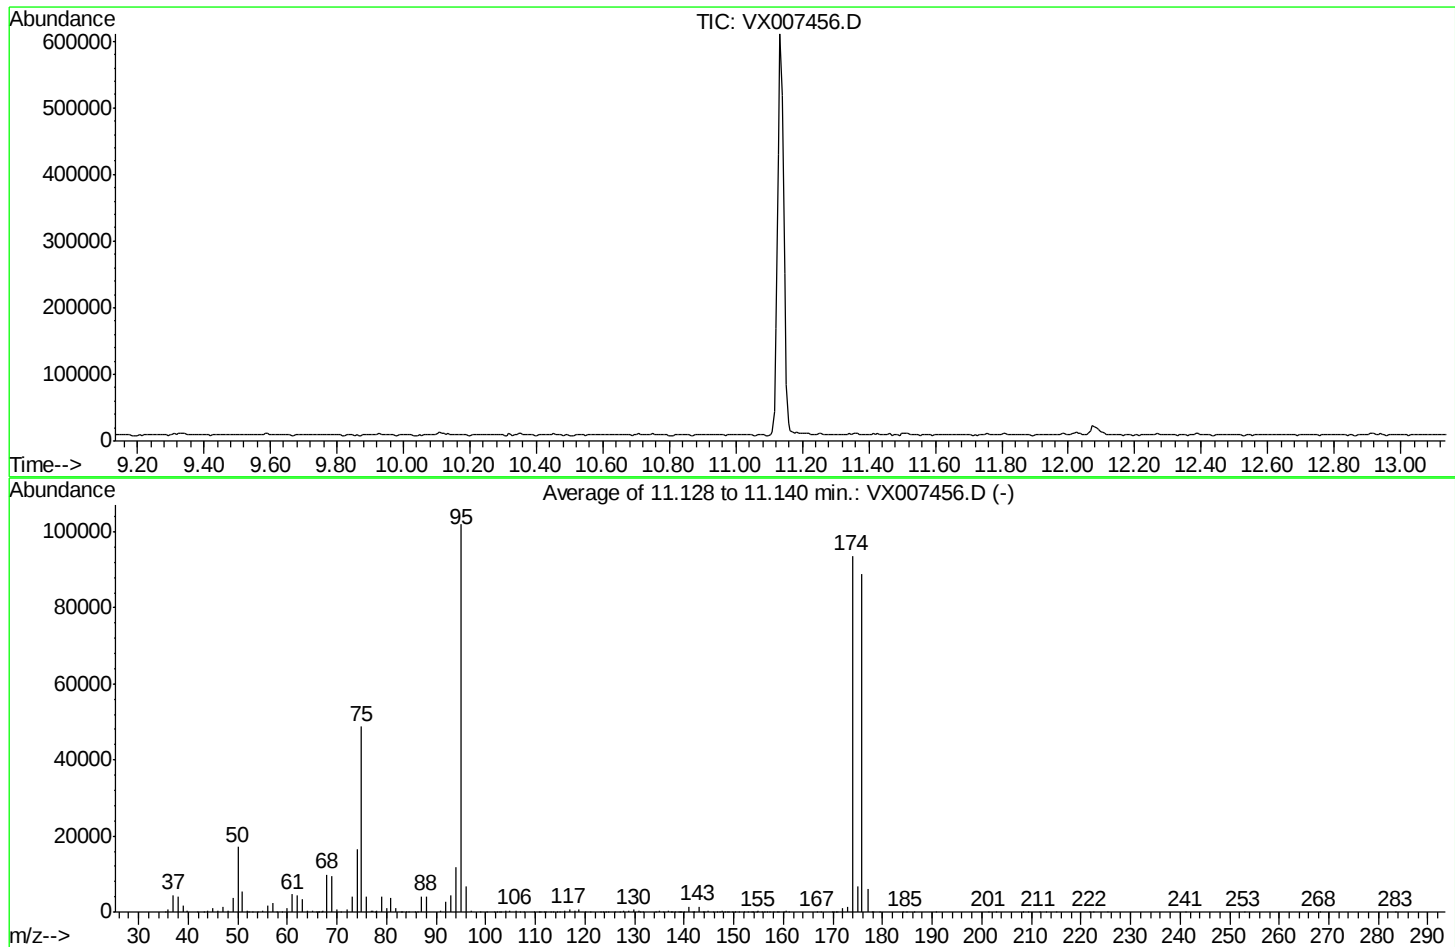

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	17087	PASS
75	95	30	60	47.8	48784	PASS
95	95	100	100	100.0	101992	PASS
96	95	5	9	6.5	6591	PASS
173	174	0.00	2	1.4	1337	PASS
174	95	50	100	91.9	93736	PASS
175	174	5	9	7.2	6742	PASS
176	174	95	101	95.0	89050	PASS
177	176	5	9	6.6	5904	PASS