

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX021120\  
 Data File : VX014913.D  
 Acq On : 11 Feb 2020 13:54  
 Operator : JC/SP  
 Sample : L1015-01  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 PR-MANHOLE

Integration Parameters: RTEINT.P

Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X021020W.M  
 Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.070       | 26            | 30          | 43           | rBV      | 1604238        | 1937314       | 90.83%          | 14.174%       |
| 2         | 5.490       | 743           | 755         | 767          | rBV      | 244615         | 705982        | 33.10%          | 5.165%        |
| 3         | 5.654       | 771           | 782         | 794          | rVV      | 426876         | 1171879       | 54.94%          | 8.574%        |
| 4         | 6.057       | 836           | 848         | 860          | rBV2     | 268864         | 703696        | 32.99%          | 5.148%        |
| 5         | 6.856       | 969           | 979         | 992          | rBV      | 649833         | 1517850       | 71.16%          | 11.105%       |
| 6         | 8.709       | 1276          | 1283        | 1292         | rBV      | 1433425        | 2132897       | 100.00%         | 15.605%       |
| 7         | 10.111      | 1507          | 1513        | 1522         | rBV      | 1374288        | 1911011       | 89.60%          | 13.981%       |
| 8         | 11.135      | 1675          | 1681        | 1691         | rBV      | 1191115        | 1558237       | 73.06%          | 11.400%       |
| 9         | 12.074      | 1829          | 1835        | 1843         | rVB      | 1672914        | 2029571       | 95.16%          | 14.849%       |


Sum of corrected areas: 13668437

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX021120\  
Data File : VX014913.D  
Acq On : 11 Feb 2020 13:54  
Operator : JC/SP  
Sample : L1015-01  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
PR-MANHOLE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X021020W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

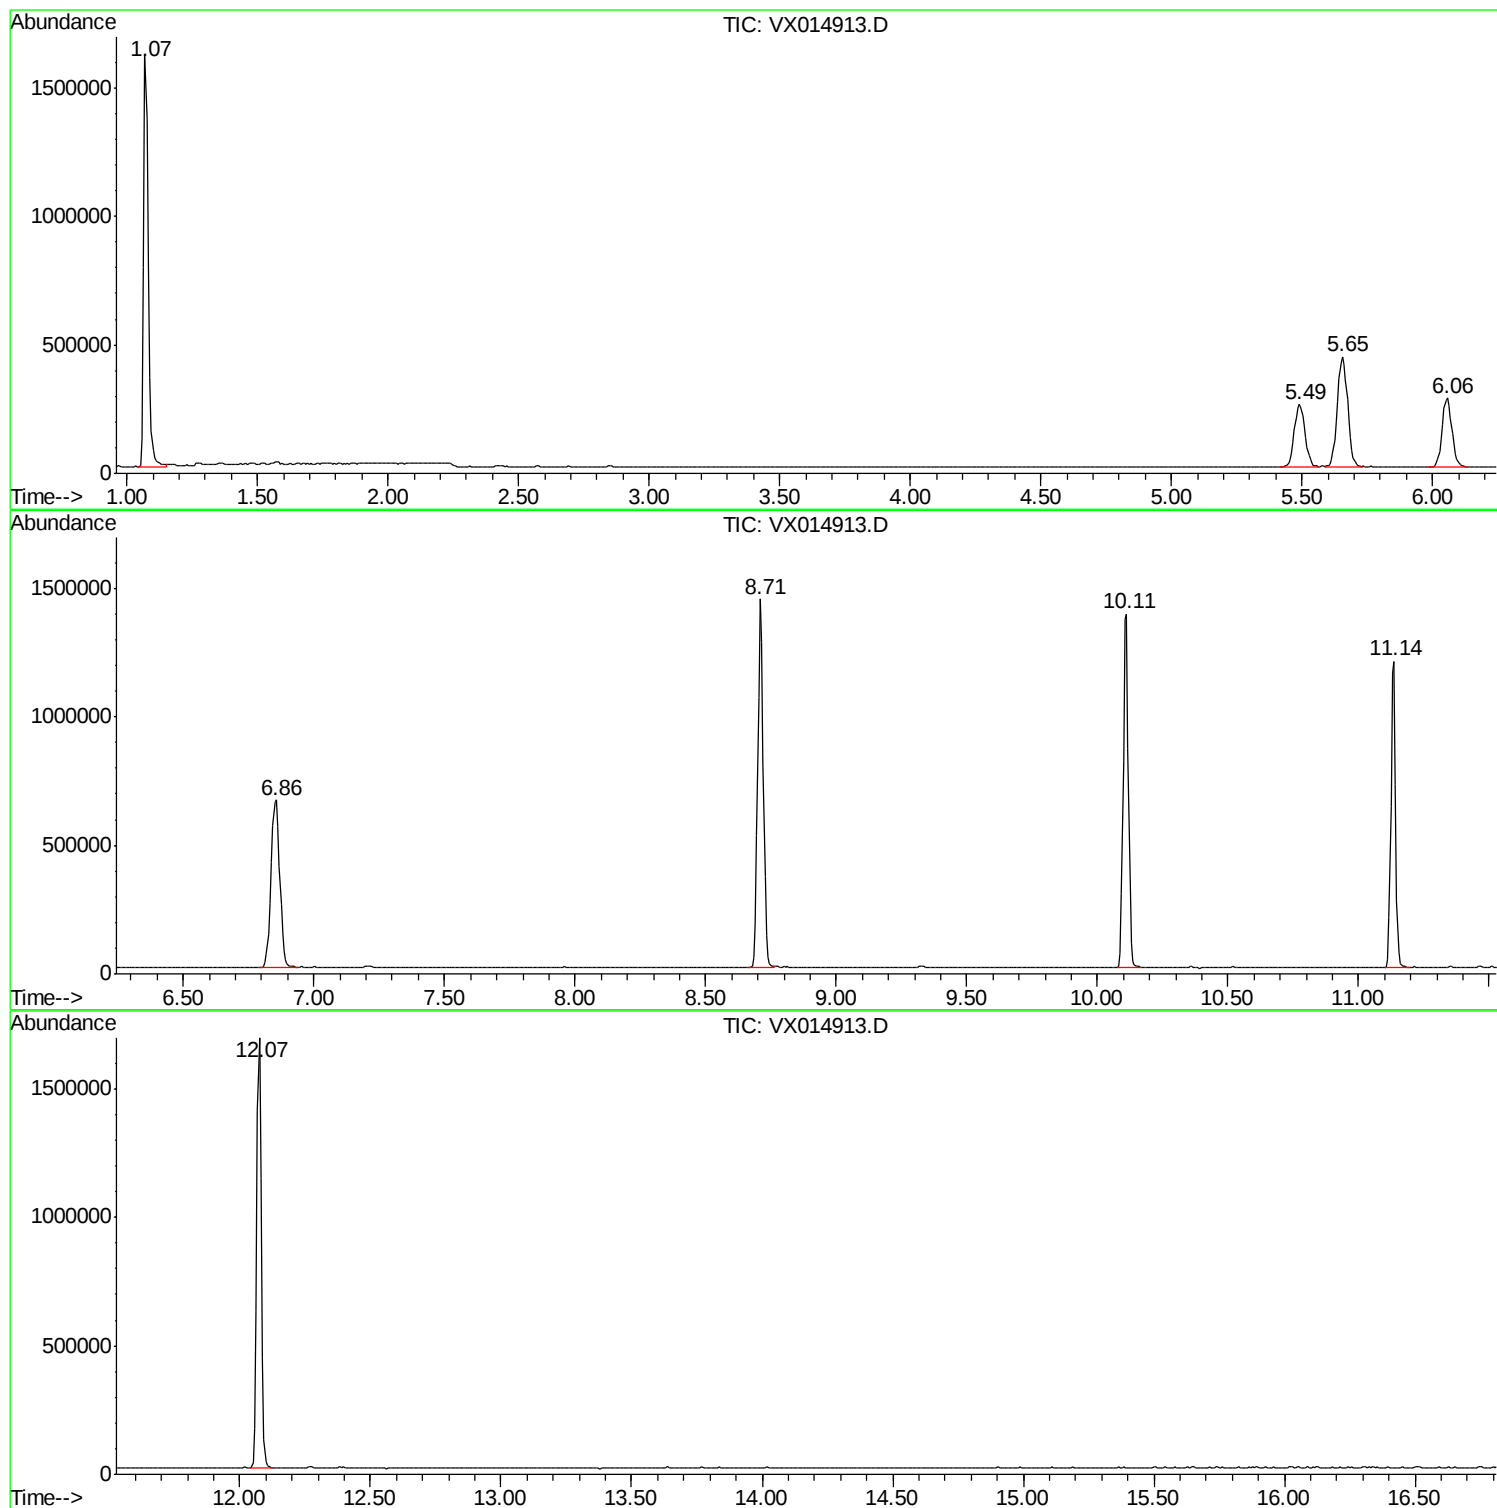

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_X\DATA\VX021120\  
Data File : VX014913.D  
Acq On : 11 Feb 2020 13:54  
Operator : JC/SP  
Sample : L1015-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
PR-MANHOLE

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X021020W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_X\DATA\VX021120\  
Data File : VX014913.D  
Acq On : 11 Feb 2020 13:54  
Operator : JC/SP  
Sample : L1015-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
PR-MANHOLE

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X021020W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |