

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021122\
 Data File : VX026978.D
 Acq On : 11 Feb 2022 19:34
 Operator : JC/MD
 Sample : N1519-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Quant Time: Feb 12 04:34:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 08 07:07:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	107945	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	180668	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	164136	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	68216	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	70347	54.290	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 108.580%	
35) Dibromofluoromethane	5.391	113	57176	53.119	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 106.240%	
50) Toluene-d8	8.653	98	213911	54.140	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 108.280%	
62) 4-Bromofluorobenzene	11.079	95	75782	54.478	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 108.960%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021122\
Data File : VX026978.D
Acq On : 11 Feb 2022 19:34
Operator : JC/MD
Sample : N1519-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Time: Feb 12 04:34:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 08 07:07:46 2022
Response via : Initial Calibration




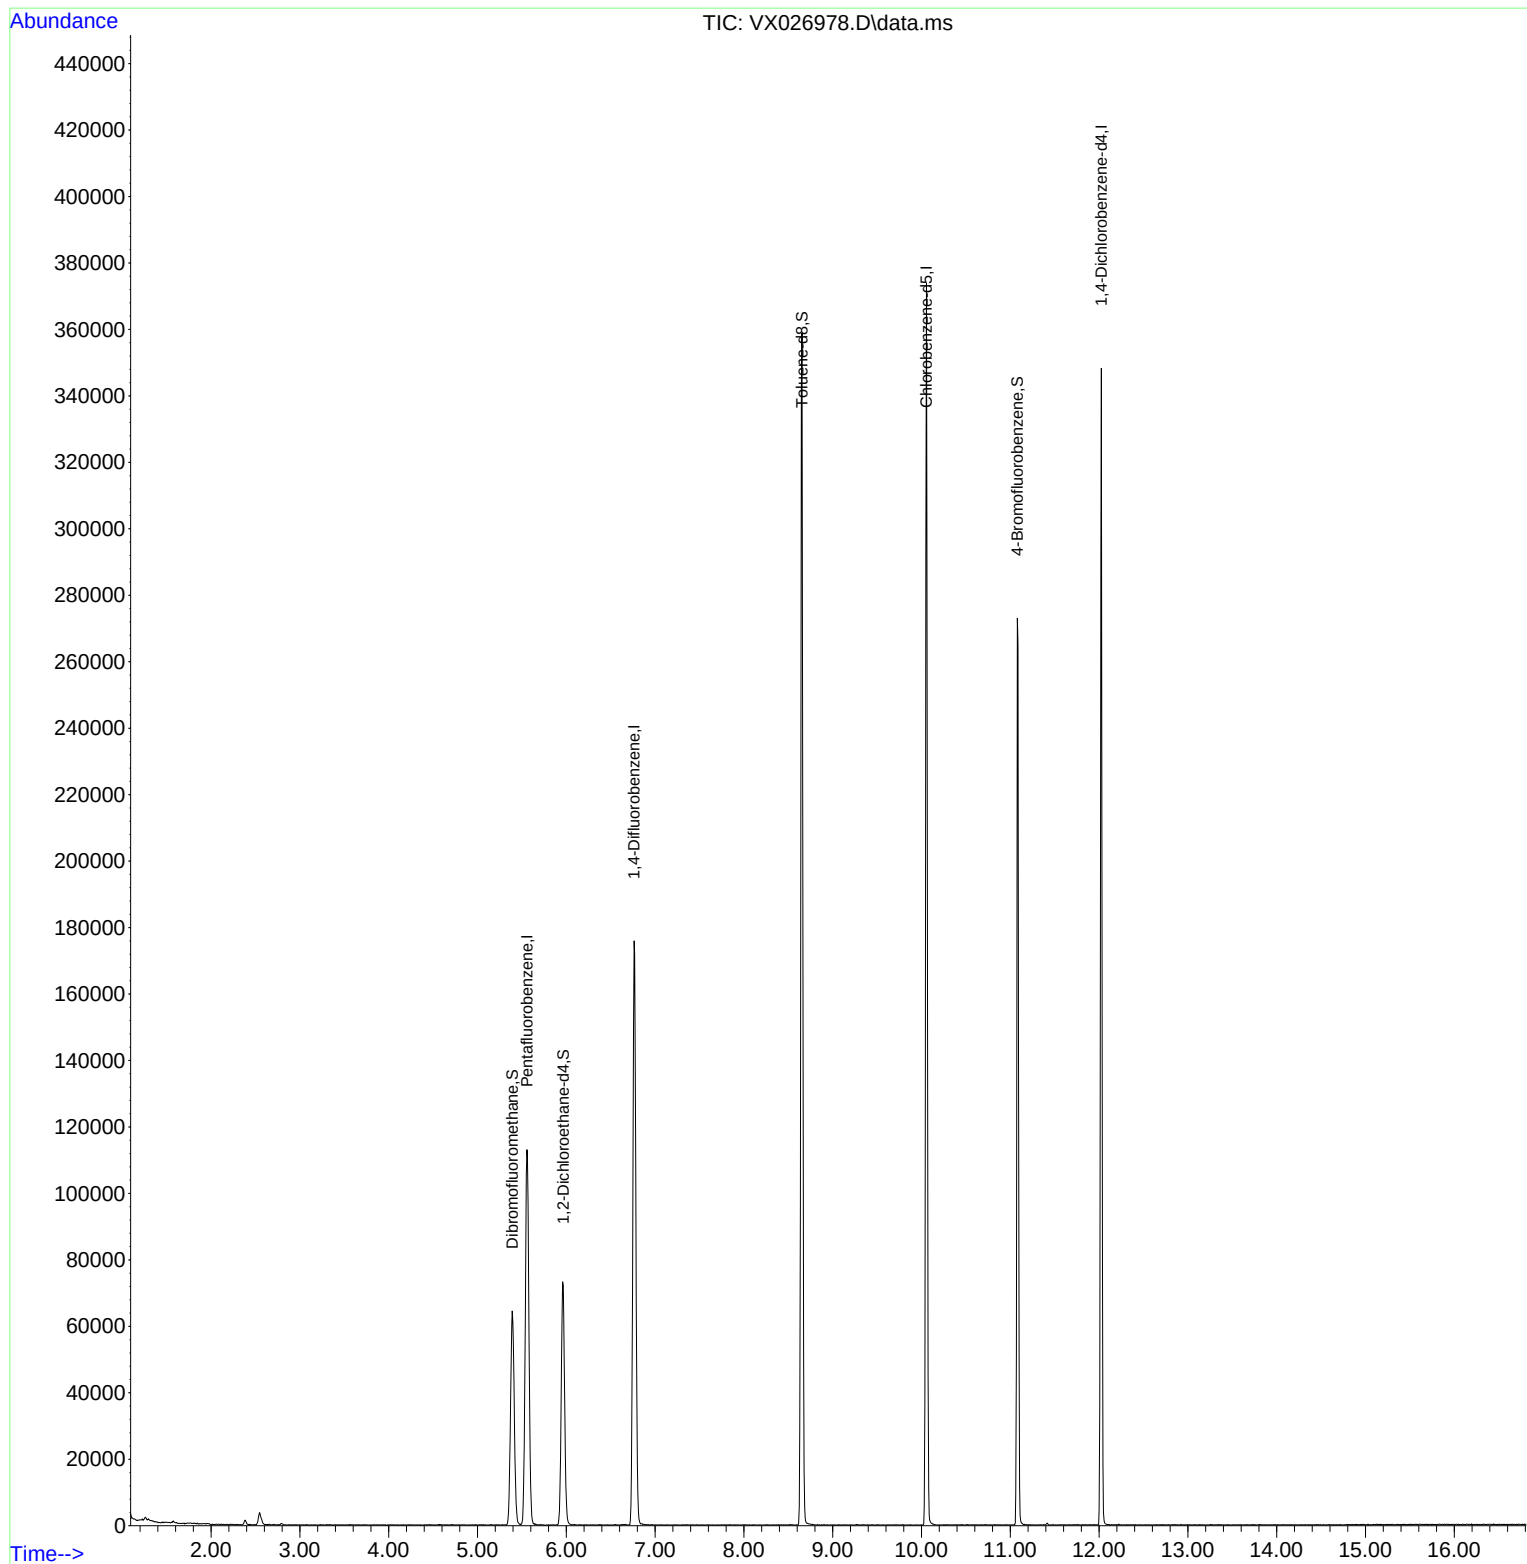


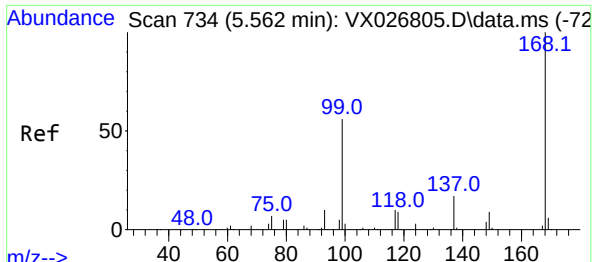

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX026978.D
Acq: 11 Feb 2022 19:34




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:168 Resp: 107945
Ion Ratio Lower Upper
168 100
99 60.9 50.3 75.5

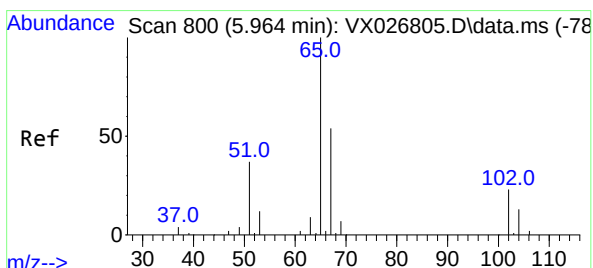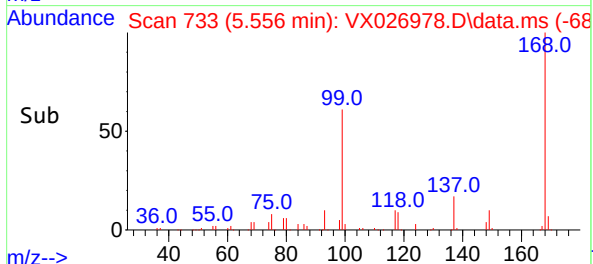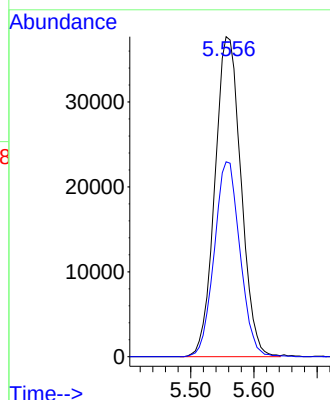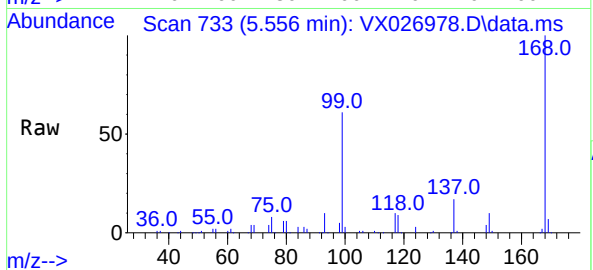

#33
1,2-Dichloroethane-d4
Concen: 54.290 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX026978.D
Acq: 11 Feb 2022 19:34

Tgt Ion: 65 Resp: 70347
Ion Ratio Lower Upper
65 100
67 50.9 0.0 100.8


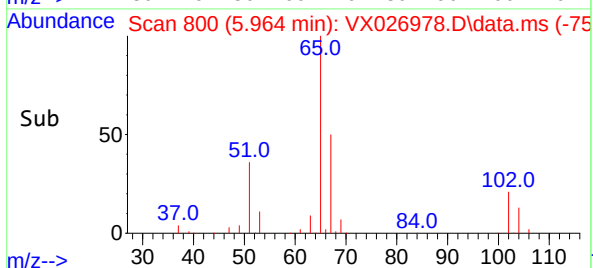
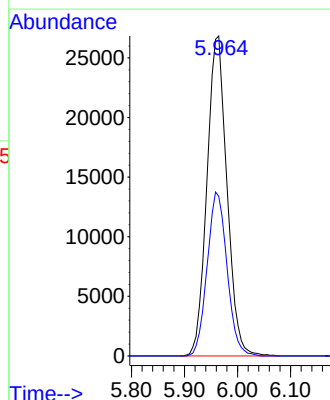
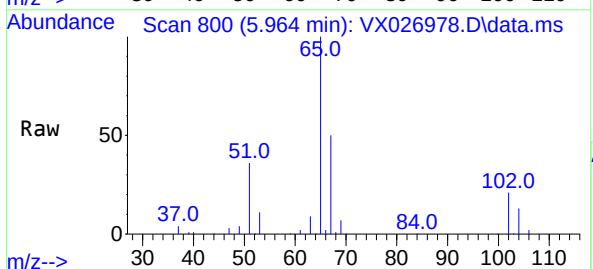


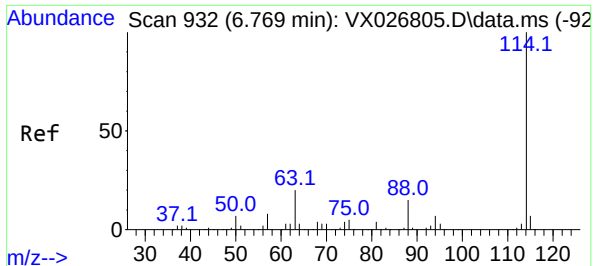

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX026978.D
Acq: 11 Feb 2022 19:34




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:114 Resp: 180668
Ion Ratio Lower Upper
114 100
63 20.9 0.0 42.8
88 16.1 0.0 33.0

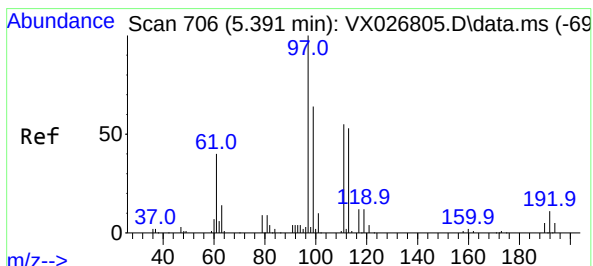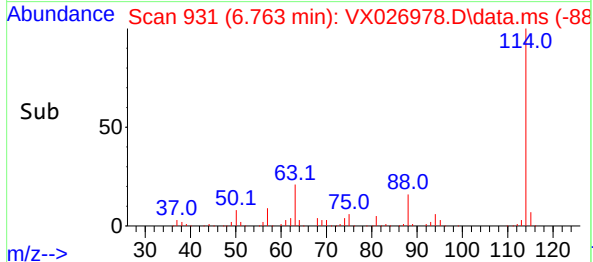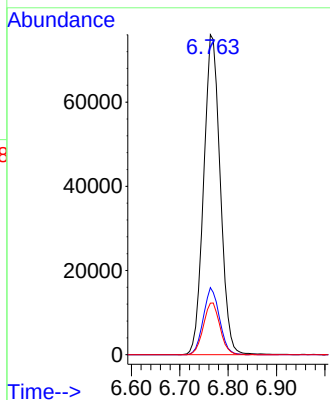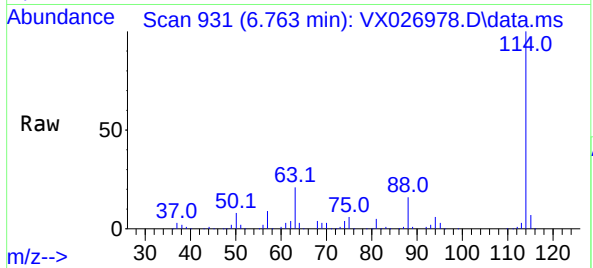

#35
Dibromofluoromethane
Concen: 53.119 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX026978.D
Acq: 11 Feb 2022 19:34

Tgt Ion:113 Resp: 57176
Ion Ratio Lower Upper
113 100
111 101.7 81.2 121.8
192 19.0 15.0 22.4

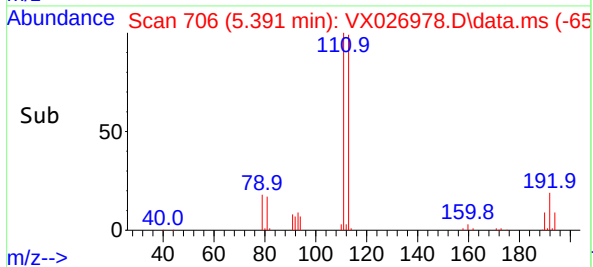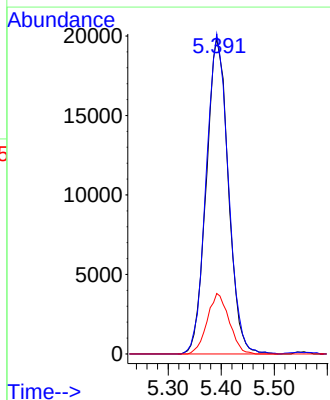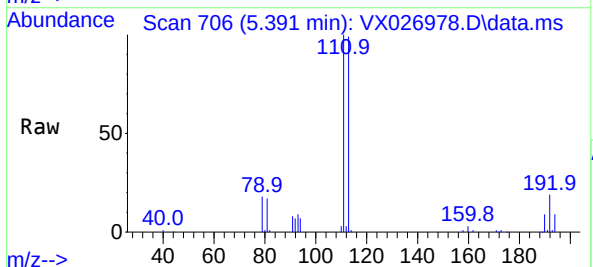

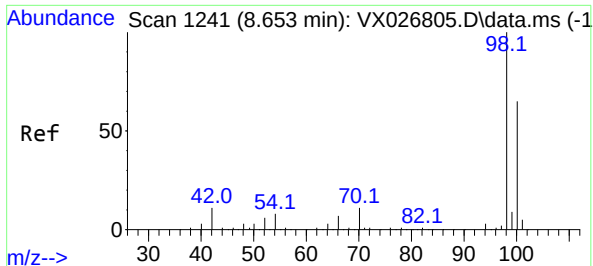

#50

Toluene-d8

Concen: 54.140 ug/l

RT: 8.653 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX026978.D

Acq: 11 Feb 2022 19:34

Instrument :

MSVOA_X

ClientSampleId :





STORAGE-BLANK-WATER-REF-4

Tgt Ion: 98 Resp: 213911

Ion Ratio Lower Upper

98 100

100 65.9 53.2 79.8

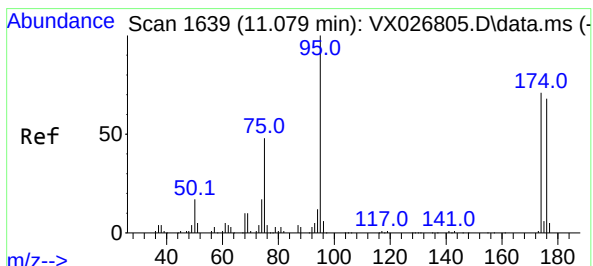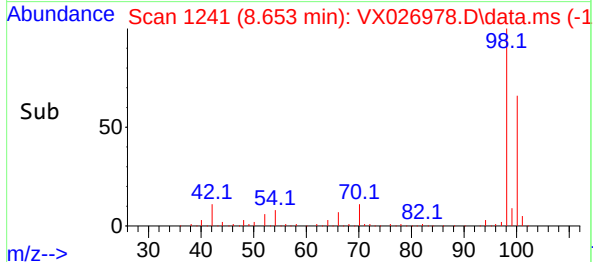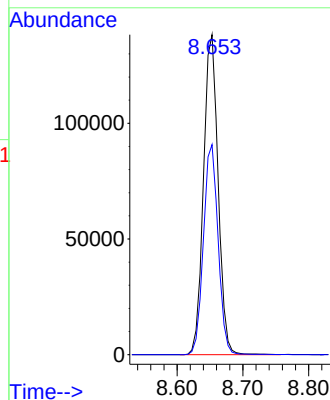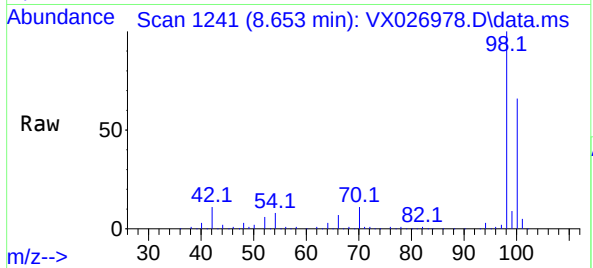

#62

4-Bromofluorobenzene

Concen: 54.478 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX026978.D

Acq: 11 Feb 2022 19:34




Tgt Ion: 95 Resp: 75782


Ion Ratio Lower Upper

95 100

174 76.4 0.0 148.6

176 73.8 0.0 141.4


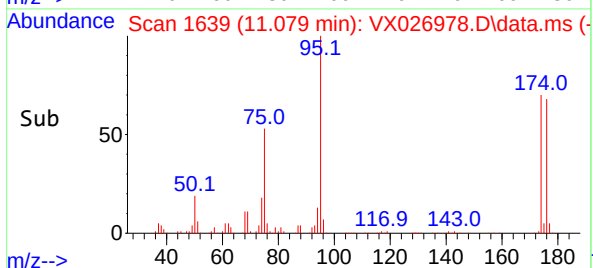
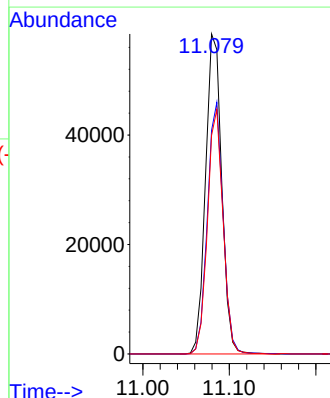
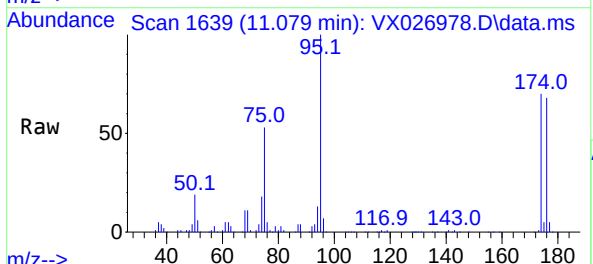


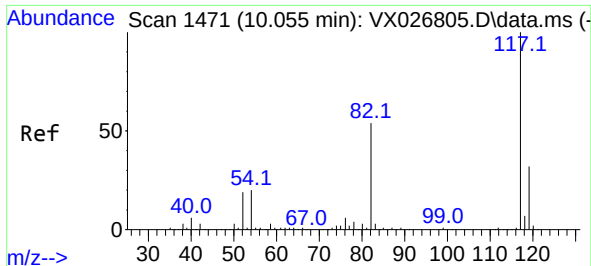

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX026978.D
Acq: 11 Feb 2022 19:34

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Tgt Ion:117 Resp: 164136
Ion Ratio Lower Upper
117 100
82 55.4 45.2 67.8
119 32.3 26.2 39.2

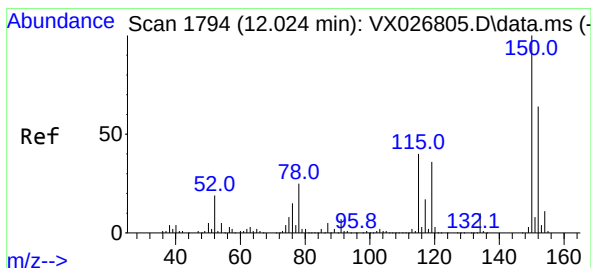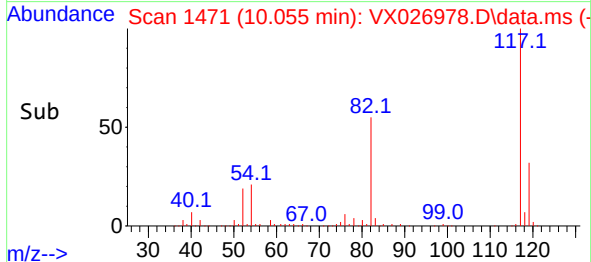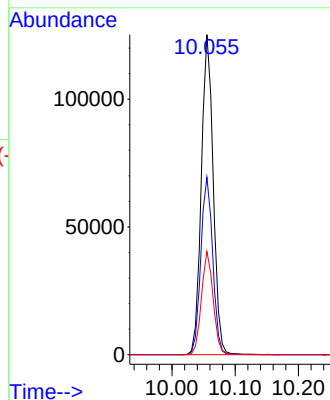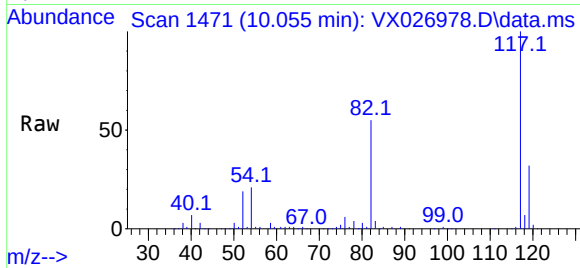

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX026978.D
Acq: 11 Feb 2022 19:34

Tgt Ion:152 Resp: 68216
Ion Ratio Lower Upper
152 100
115 60.8 44.2 132.6
150 157.3 0.0 348.2

