

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021123\
 Data File : VX034097.D
 Acq On : 09 Feb 2023 11:40
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Feb 10 01:06:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 03 23:25:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	126391	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	173813	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	156726	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	79001	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	61148	50.184	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 100.360%	
35) Dibromofluoromethane	5.385	113	55462	50.137	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 100.280%	
50) Toluene-d8	8.647	98	199962	50.171	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 100.340%	
62) 4-Bromofluorobenzene	11.079	95	70886	49.798	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 99.600%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021123\
Data File : VX034097.D
Acq On : 09 Feb 2023 11:40
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Feb 10 01:06:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 03 23:25:45 2023
Response via : Initial Calibration




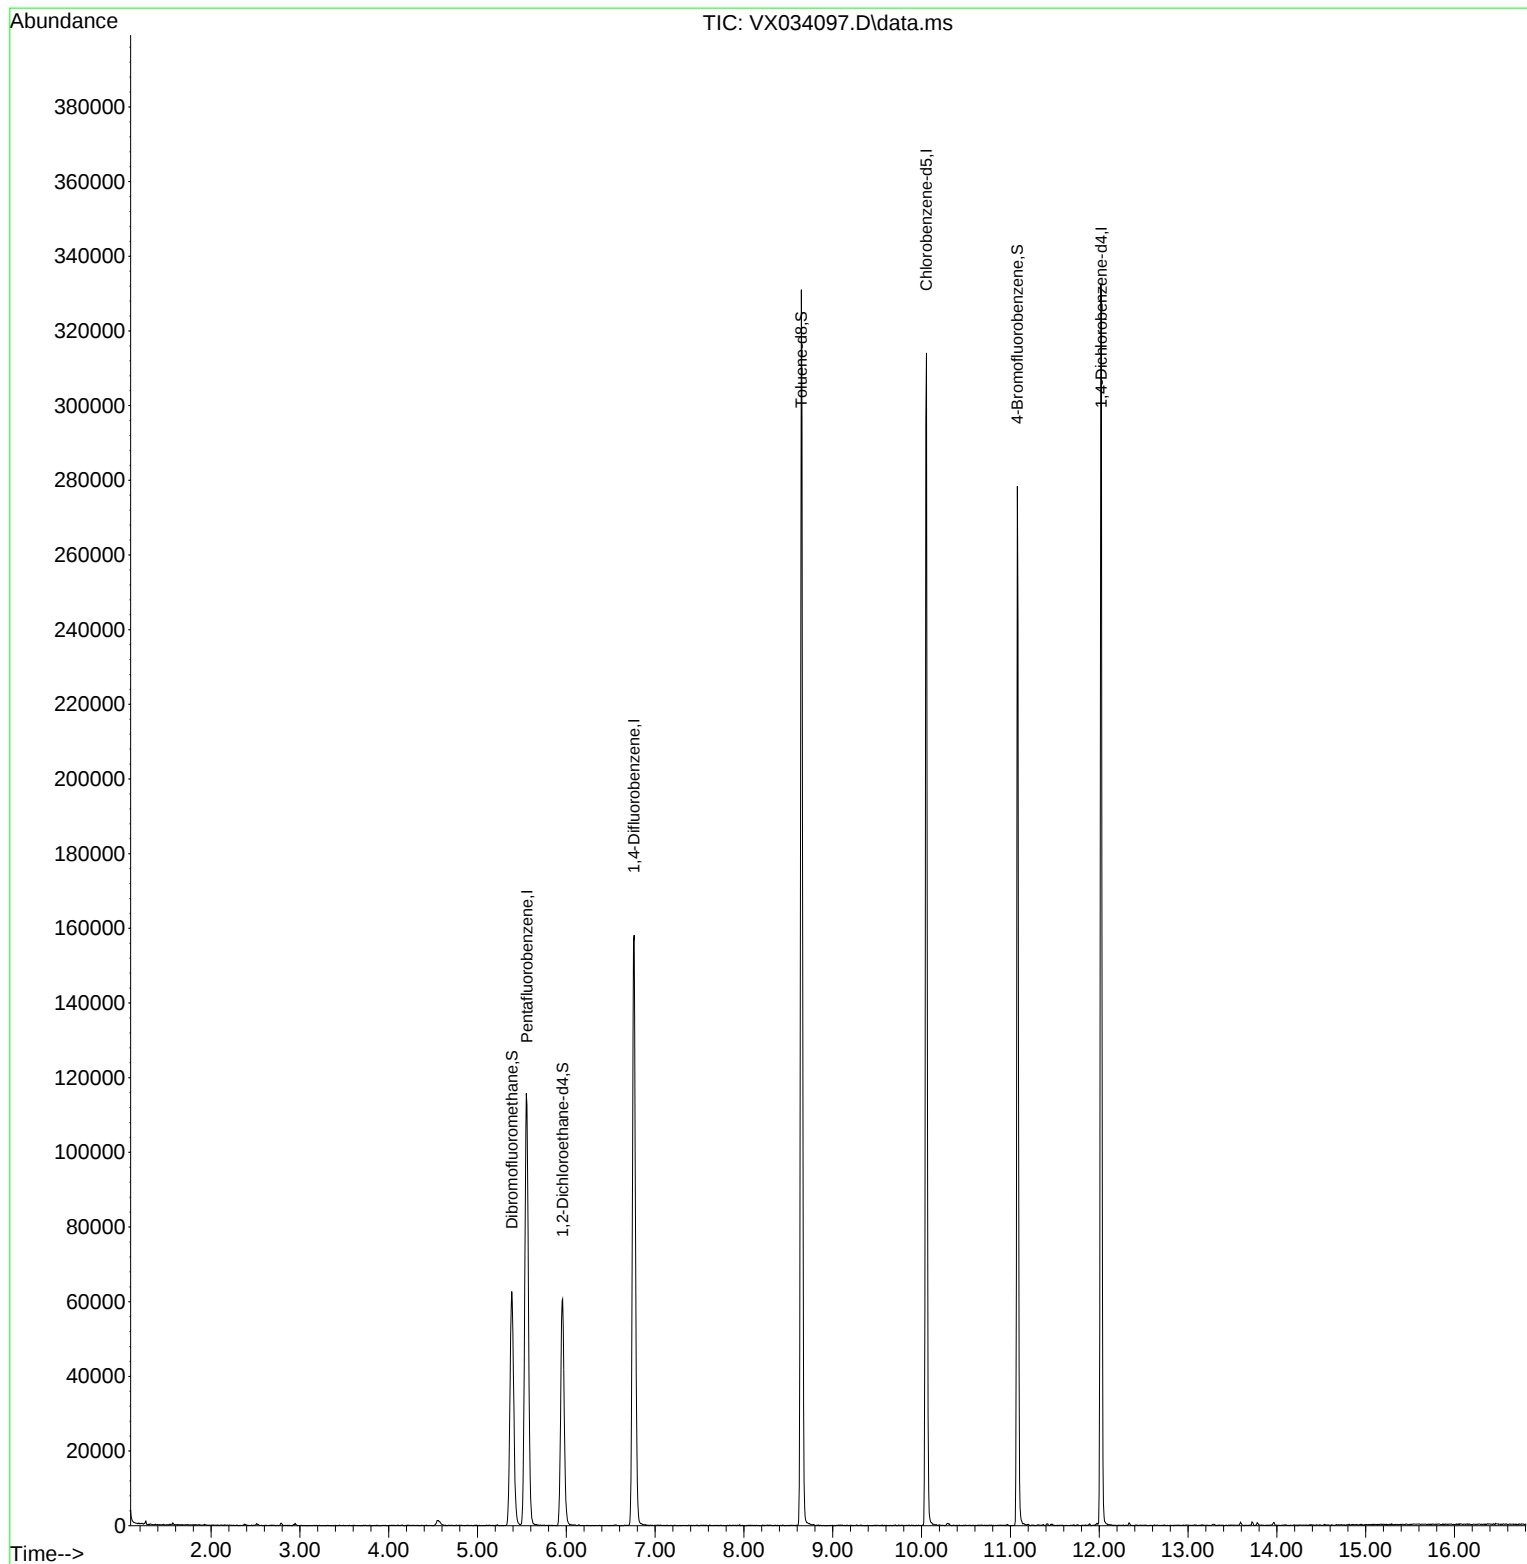


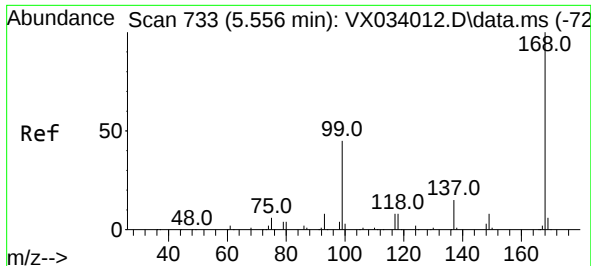

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.000 min
Lab File: VX034097.D
Acq: 09 Feb 2023 11:40




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 126391
Ion Ratio Lower Upper
168 100
99 46.9 39.6 59.4

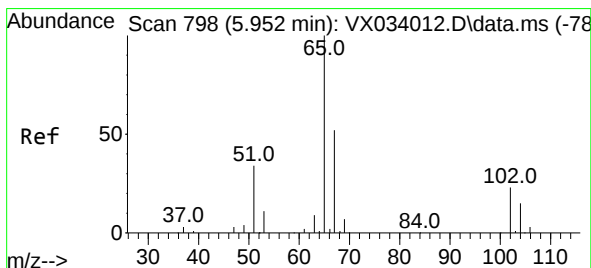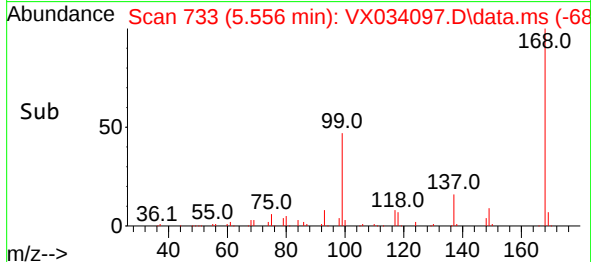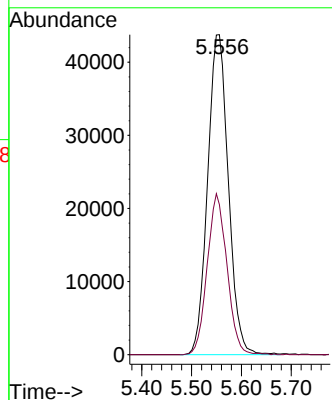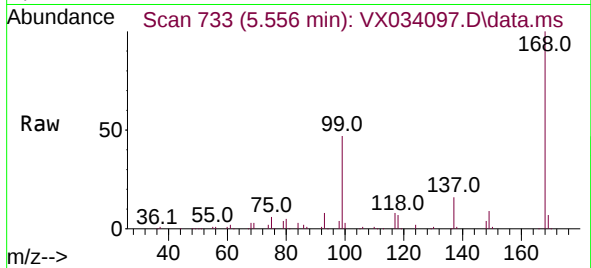

#33
1,2-Dichloroethane-d4
Concen: 50.184 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.006 min
Lab File: VX034097.D
Acq: 09 Feb 2023 11:40

Tgt Ion: 65 Resp: 61148
Ion Ratio Lower Upper
65 100
67 51.7 0.0 104.8


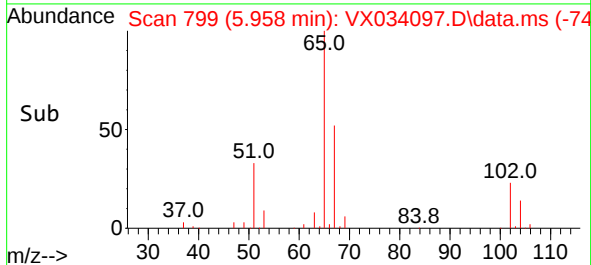
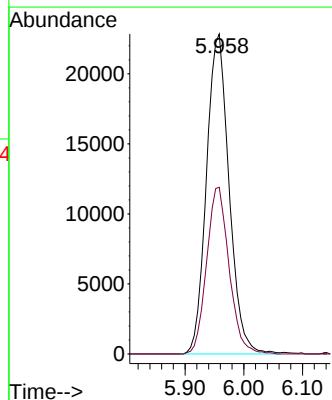
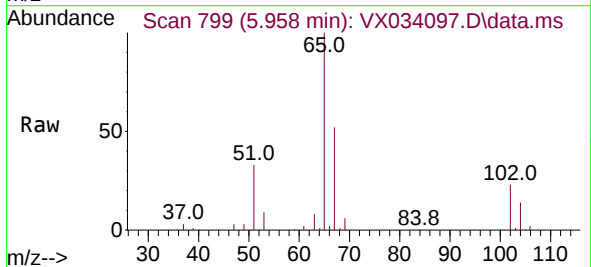


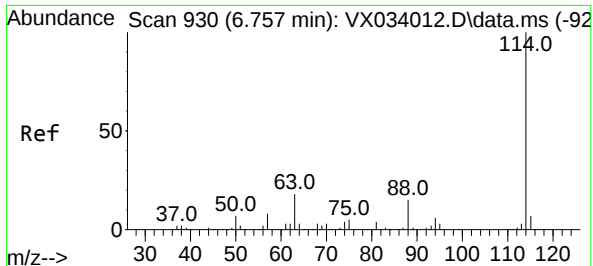

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX034097.D
Acq: 09 Feb 2023 11:40




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:114 Resp: 173813
Ion Ratio Lower Upper
114 100
63 17.8 0.0 37.4
88 15.0 0.0 30.6

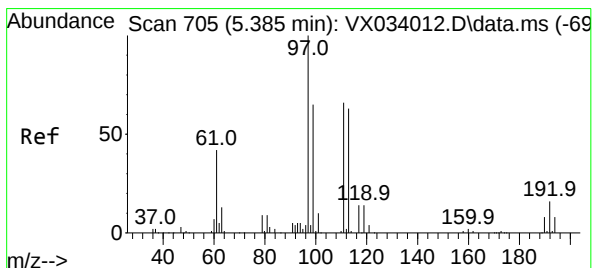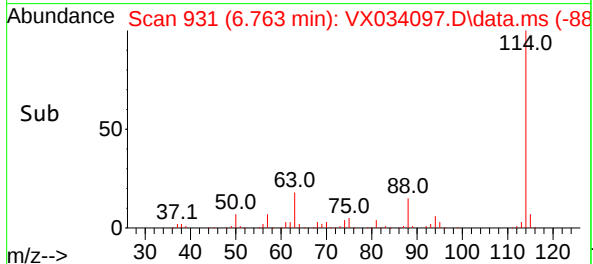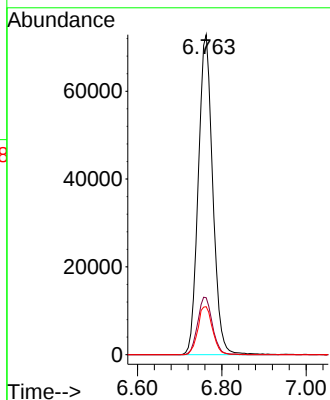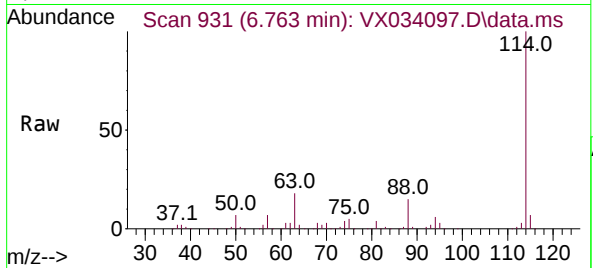

#35
Dibromofluoromethane
Concen: 50.137 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX034097.D
Acq: 09 Feb 2023 11:40

Tgt Ion:113 Resp: 55462
Ion Ratio Lower Upper
113 100
111 102.1 83.0 124.6
192 25.7 19.0 28.4


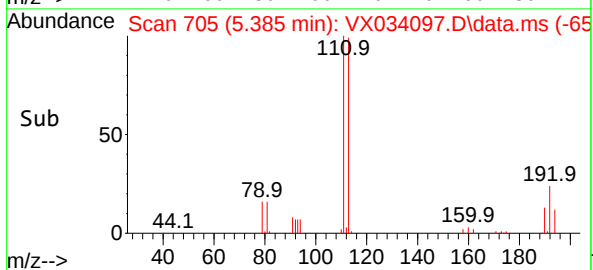
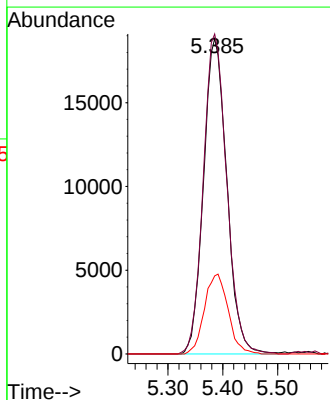
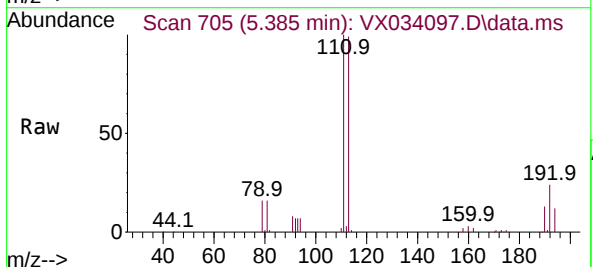


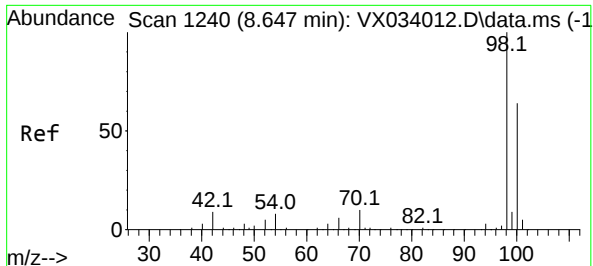

#50
Toluene-d8
Concen: 50.171 ug/l
RT: 8.647 min Scan# 1133
Delta R.T. -0.000 min
Lab File: VX034097.D
Acq: 09 Feb 2023 11:40




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 199962
Ion Ratio Lower Upper
98 100
100 66.3 53.6 80.4

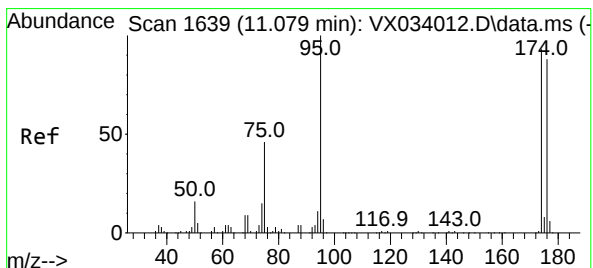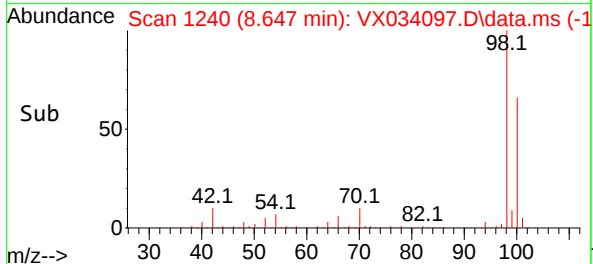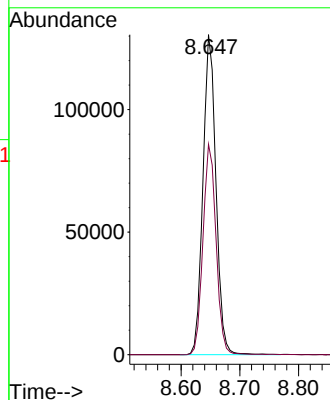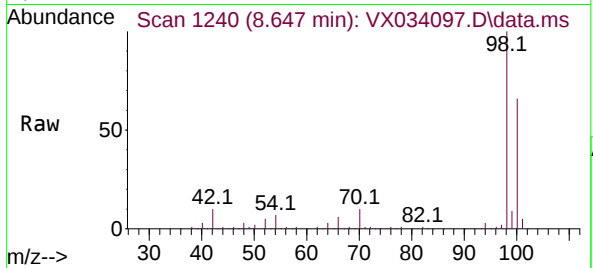

#62
4-Bromofluorobenzene
Concen: 49.798 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX034097.D
Acq: 09 Feb 2023 11:40

Tgt Ion: 95 Resp: 70886
Ion Ratio Lower Upper
95 100
174 99.8 0.0 184.4
176 96.0 0.0 178.8


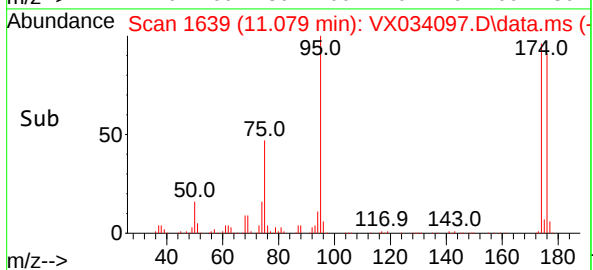
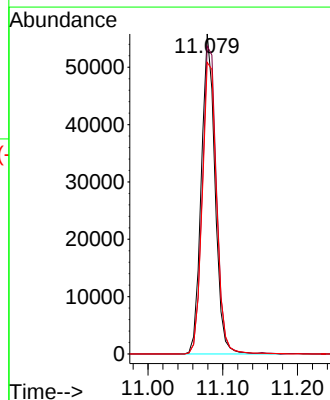
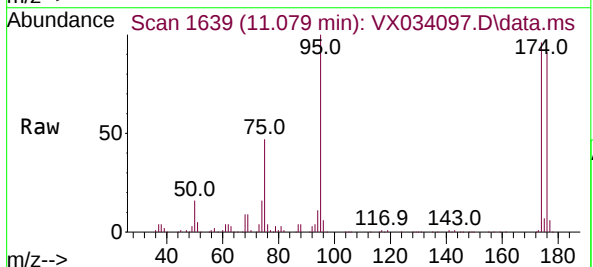


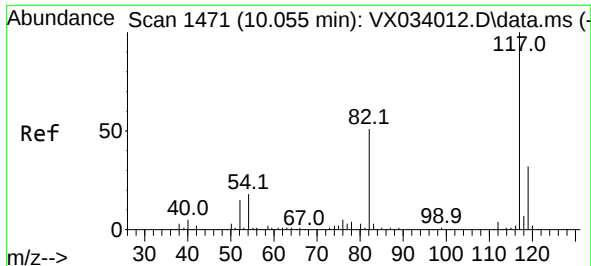

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX034097.D
Acq: 09 Feb 2023 11:40

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion:117 Resp: 156726
Ion Ratio Lower Upper
117 100
82 49.4 40.6 60.8
119 32.2 25.6 38.4

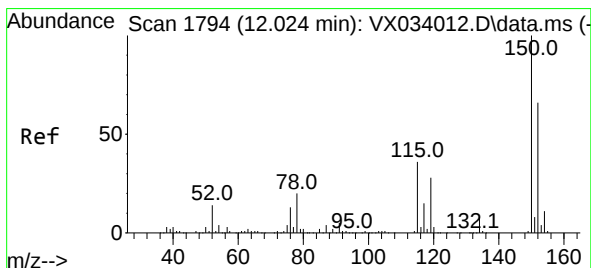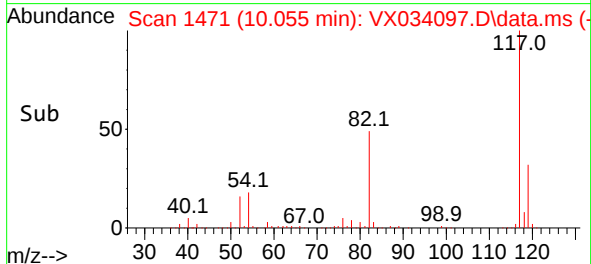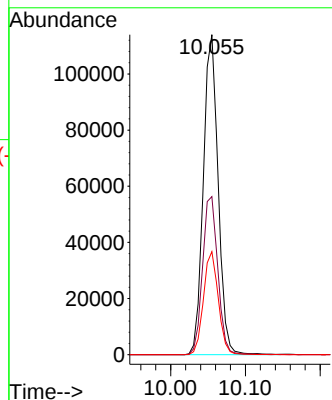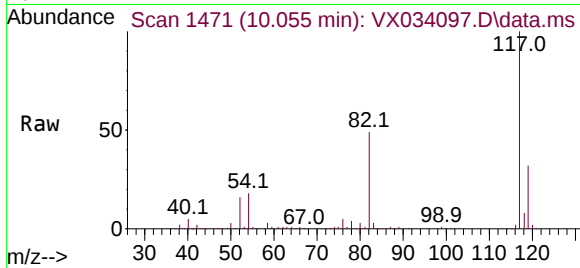

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX034097.D
Acq: 09 Feb 2023 11:40

Tgt Ion:152 Resp: 79001
Ion Ratio Lower Upper
152 100
115 53.8 38.7 116.1
150 155.2 0.0 348.2

