

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX021220\
 Data File : VX014927.D
 Acq On : 12 Feb 2020 15:46
 Operator : JC/SP
 Sample : L1503-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-2

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X021020W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	42	rBV	621535	812827	39.20%	6.271%
2	1.485	95	98	102	rVB	20889	20819	1.00%	0.161%
3	2.381	238	245	251	rBV2	23463	46983	2.27%	0.362%
4	5.490	743	755	766	rBV2	235224	678183	32.71%	5.232%
5	5.655	772	782	798	rVB	417501	1137983	54.89%	8.779%
6	6.057	837	848	863	rVB	261295	679714	32.78%	5.244%
7	6.849	968	978	989	rBV	637125	1489116	71.82%	11.488%
8	7.209	1027	1037	1045	rBV2	111811	246641	11.90%	1.903%
9	8.709	1277	1283	1292	rBV	1378229	2073333	100.00%	15.995%
10	9.331	1379	1385	1395	rVB	275102	401592	19.37%	3.098%
11	10.111	1507	1513	1526	rVB	1358764	1870755	90.23%	14.432%
12	11.135	1675	1681	1692	rBV	1185586	1527519	73.67%	11.784%
13	12.074	1830	1835	1842	rVB	1613039	1976944	95.35%	15.251%


Sum of corrected areas: 12962409

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX021220\
Data File : VX014927.D
Acq On : 12 Feb 2020 15:46
Operator : JC/SP
Sample : L1503-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X021020W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

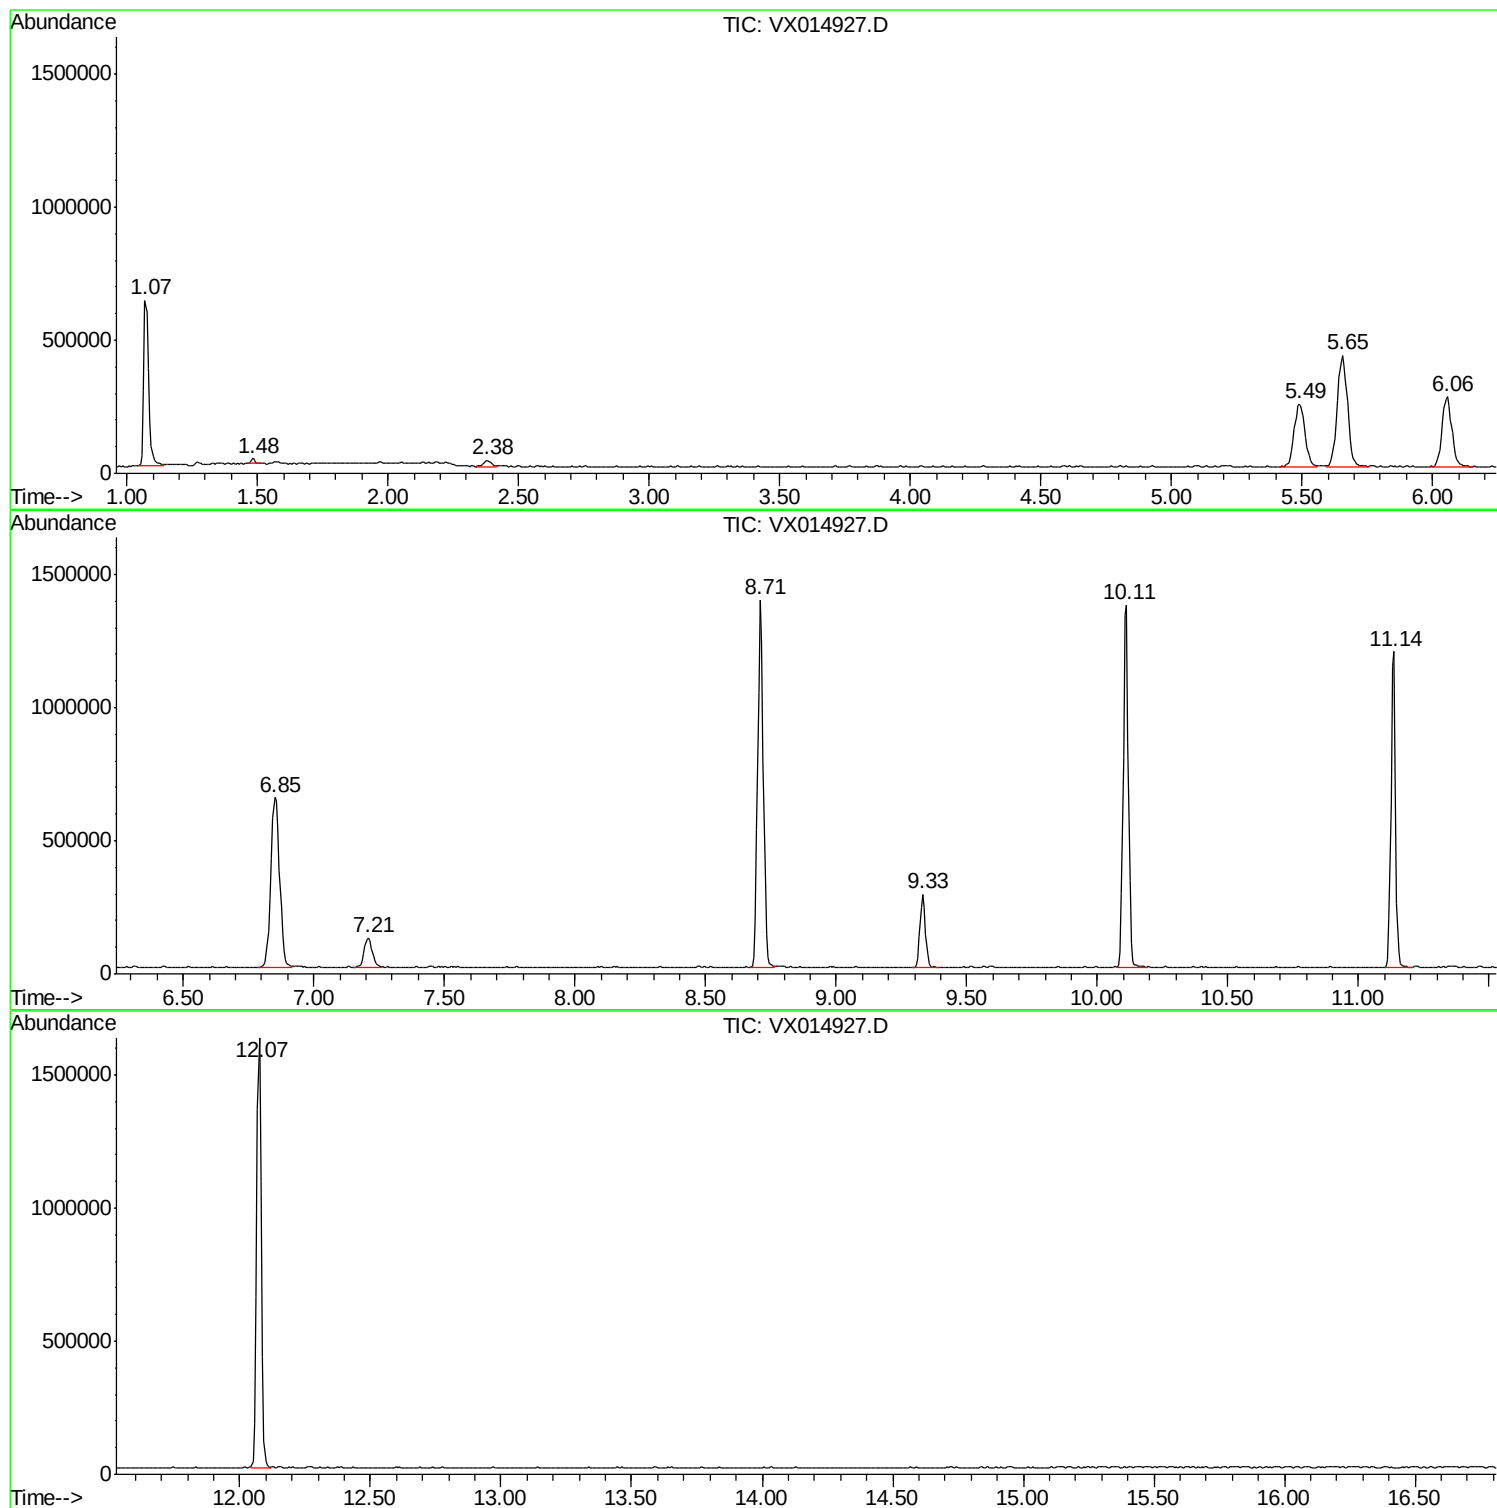

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX021220\
Data File : VX014927.D
Acq On : 12 Feb 2020 15:46
Operator : JC/SP
Sample : L1503-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X021020W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX021220\
Data File : VX014927.D
Acq On : 12 Feb 2020 15:46
Operator : JC/SP
Sample : L1503-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X021020W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc
