

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021223\
 Data File : VX034127.D
 Acq On : 10 Feb 2023 20:08
 Operator : JC/MD
 Sample : 01485-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EA-FILTERBAGS-0208

Quant Time: Feb 11 00:40:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 03 23:25:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	112510	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	155216	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	138361	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	70283	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	56500	52.091	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 104.180%			
35) Dibromofluoromethane	5.385	113	50005	50.620	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 101.240%			
50) Toluene-d8	8.647	98	176184	49.502	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 99.000%			
62) 4-Bromofluorobenzene	11.079	95	62996	49.558	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 99.120%			
Target Compounds					Qvalue	
11) Tert butyl alcohol	2.947	59	1602	10.542	ug/l #	86
15) Acrylonitrile	3.081	53	200	0.410	ug/l #	59
16) Acetone	2.374	43	25110	54.812	ug/l	99
17) Carbon Disulfide	2.514	76	1244	0.532	ug/l	97
18) Methyl Acetate	2.697	43	956	0.671	ug/l	98
20) Methylene Chloride	2.788	84	7574	7.227	ug/l	94
21) trans-1,2-Dichloroethene	3.099	96	259	0.258	ug/l #	57
25) 2-Butanone	4.562	43	3227	4.838	ug/l	97
29) Tetrahydrofuran	5.032	42	263	0.620	ug/l #	34
36) 1,1-Dichloropropene	5.556	75	6678	4.931	ug/l #	48
37) Ethyl Acetate	4.721	43	11826	9.373	ug/l	99
38) Carbon Tetrachloride	5.550	117	9724	6.732	ug/l #	15
43) Isopropyl Acetate	6.336	43	48666	24.733	ug/l	97
48) Methyl methacrylate	7.793	41	35475	34.919	ug/l #	46
51) 4-Methyl-2-Pentanone	8.549	43	42024	34.049	ug/l #	52
54) cis-1,3-Dichloropropene	8.549	75	19180	12.767	ug/l #	59
56) Ethyl methacrylate	9.244	69	313	0.221	ug/l #	1
57) 1,3-Dichloropropane	9.482	76	1656	0.999	ug/l #	43
59) 2-Hexanone	9.482	43	23071	25.543	ug/l #	49
76) 1,2,3-Trichloropropane	11.079	75	29898	24.774	ug/l #	34
81) trans-1,4-Dichloro-2-b...	11.079	75	29898	76.296	ug/l #	8
87) 1,3-Dichlorobenzene	11.975	146	609	0.255	ug/l	95
88) 1,4-Dichlorobenzene	11.975	146	609	0.251	ug/l	97
89) n-Butylbenzene	12.335	91	930	0.280	ug/l	98
93) 1,2,4-Trichlorobenzene	13.591	180	811	0.492	ug/l	96
94) Hexachlorobutadiene	13.725	225	756	0.927	ug/l	89
95) Naphthalene	13.780	128	2132	0.471	ug/l	96
96) 1,2,3-Trichlorobenzene	13.963	180	968	0.585	ug/l	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021223\
Data File : VX034127.D
Acq On : 10 Feb 2023 20:08
Operator : JC/MD
Sample : 01485-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EA-FILTERBAGS-0208

Quant Time: Feb 11 00:40:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 03 23:25:45 2023
Response via : Initial Calibration




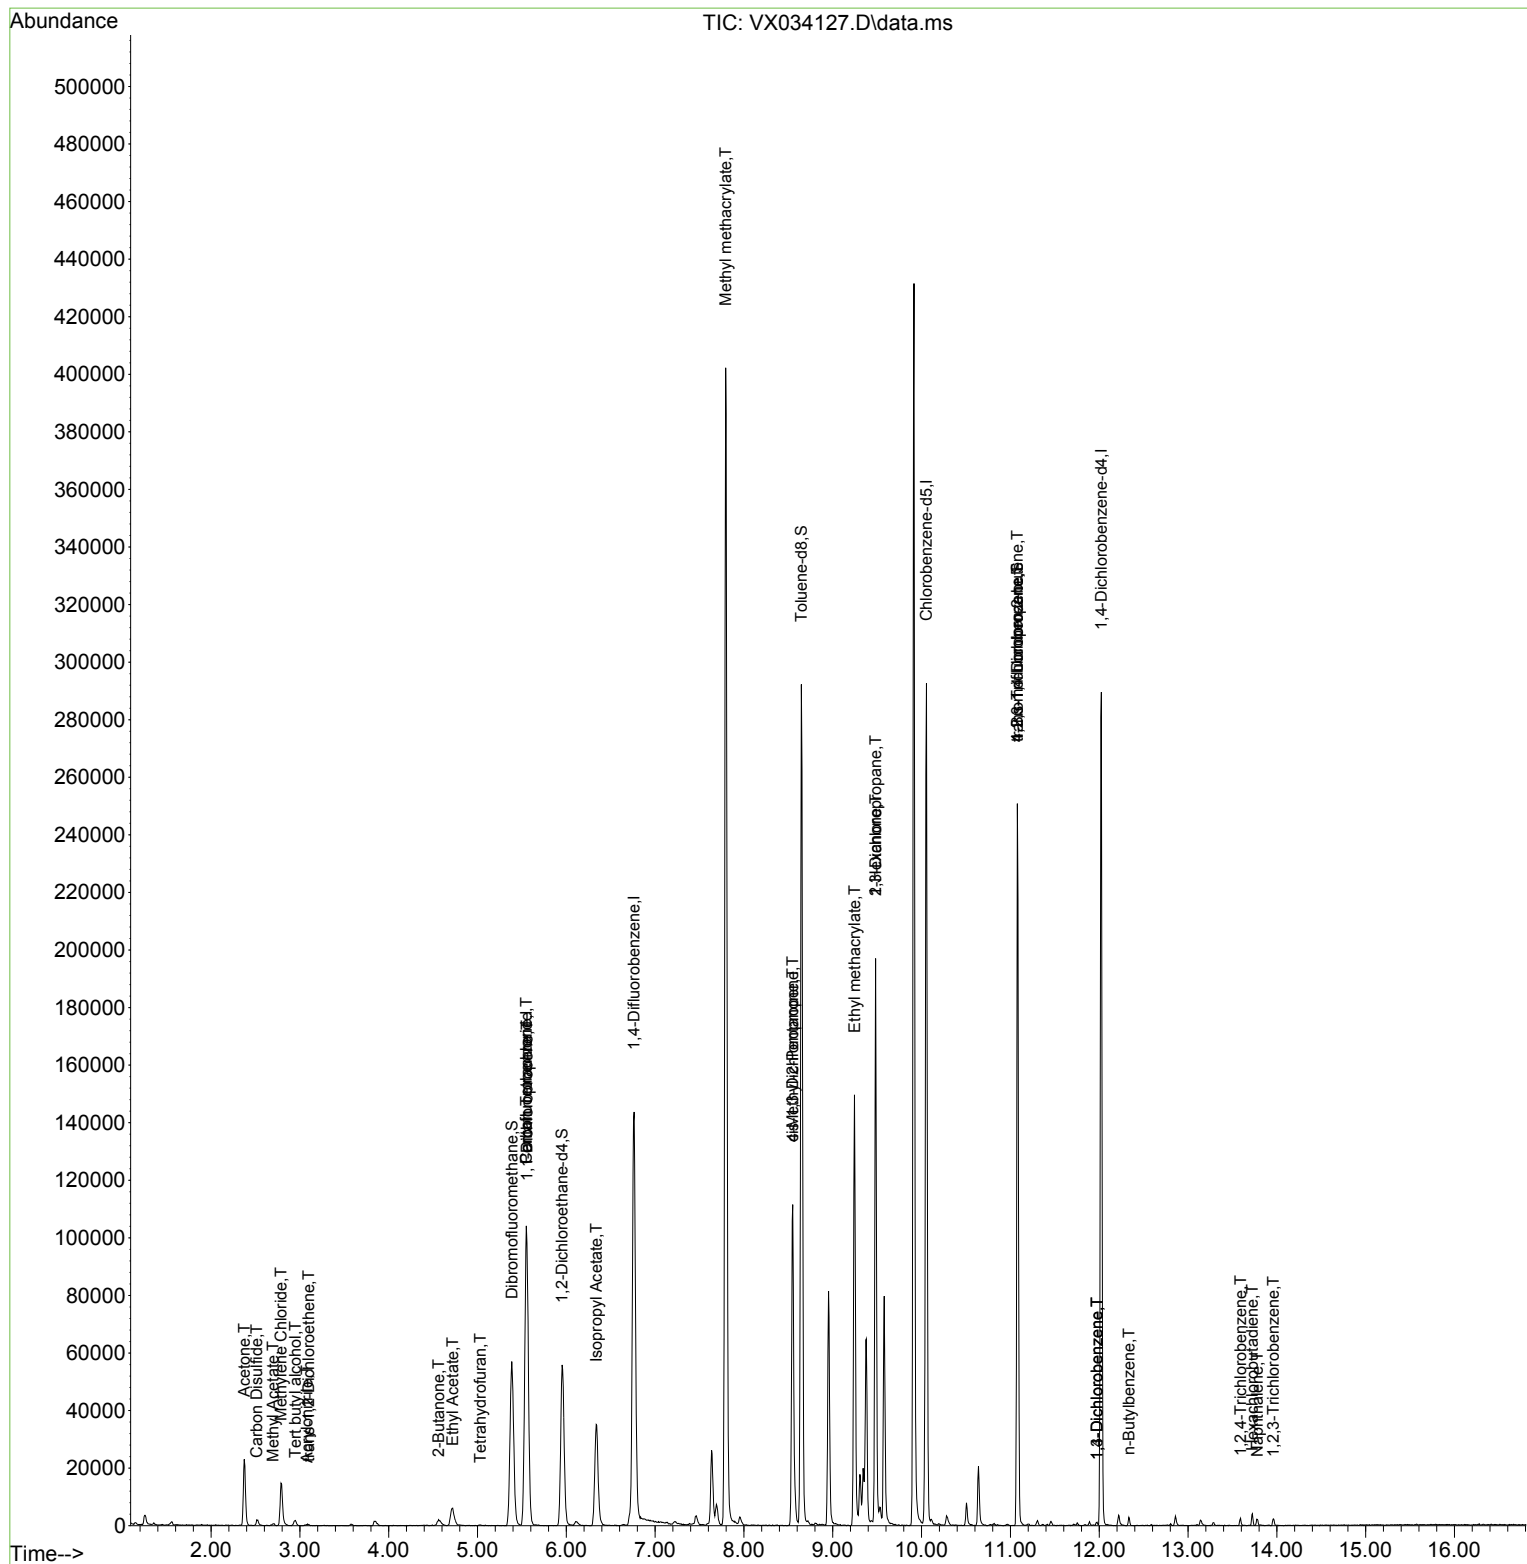


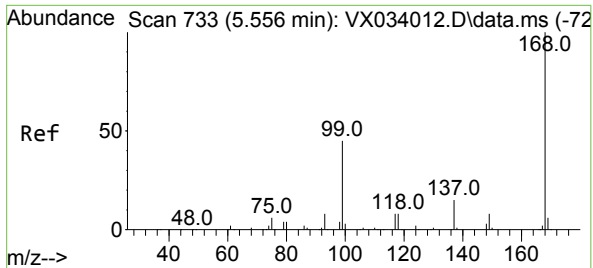

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX034127.D
Acq: 10 Feb 2023 20:08




Instrument :
MSVOA_X
ClientSampleId :
EA-FILTERBAGS-0208


Tgt Ion:168 Resp: 112510
Ion Ratio Lower Upper
168 100
99 47.8 39.6 59.4

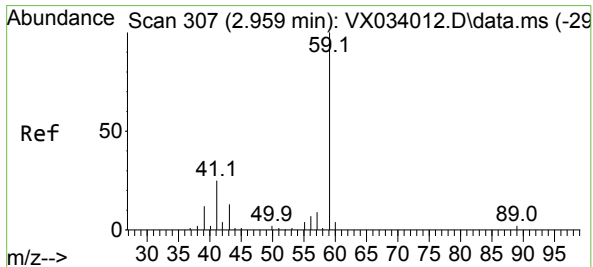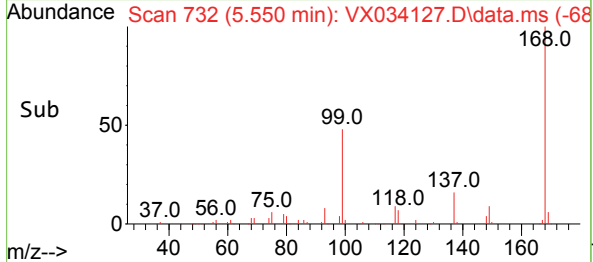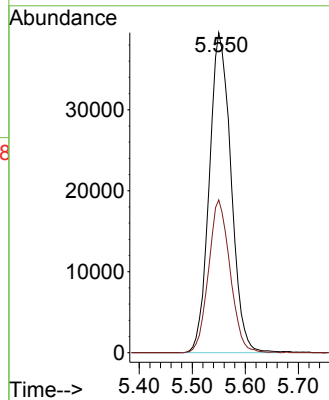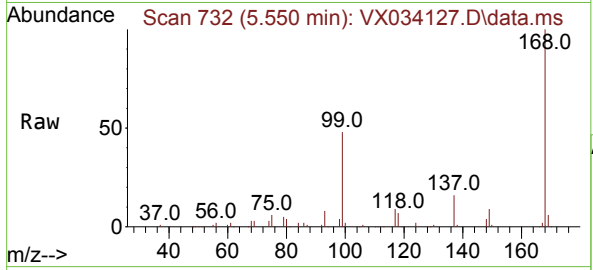

#11
Tert butyl alcohol
Concen: 10.542 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.012 min
Lab File: VX034127.D
Acq: 10 Feb 2023 20:08

Tgt Ion: 59 Resp: 1602
Ion Ratio Lower Upper
59 100
57 0.0 3.7 5.5#

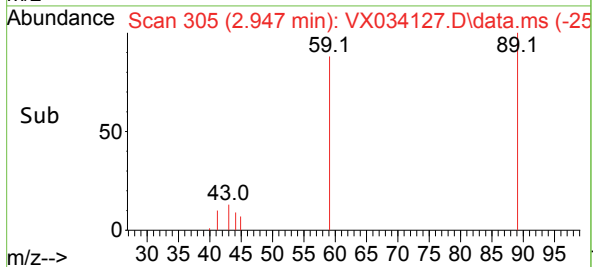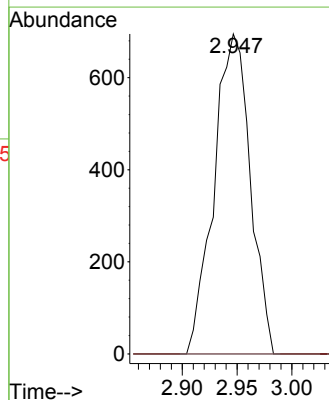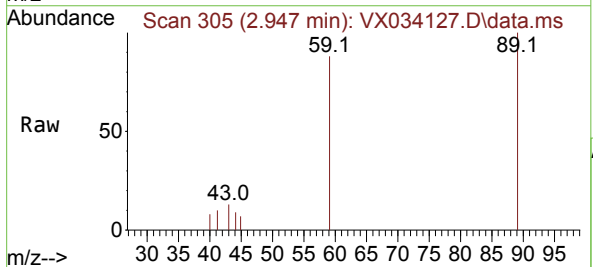



#15

Acrylonitrile

Concen: 0.410 ug/l

RT: 3.081 min Scan# 31

Delta R.T. 0.024 min

Lab File: VX034127.D

Acq: 10 Feb 2023 20:08

Instrument :

MSVOA_X

ClientSampleId :

EA-FILTERBAGS-0208





Tgt Ion: 53 Resp: 200

Ion Ratio Lower Upper

53 100

52 53.5 65.7 98.5#

51 0.0 29.0 43.4#

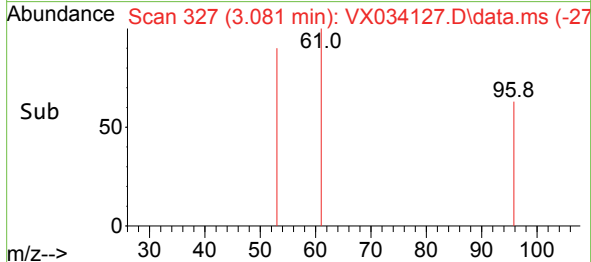

#16

Acetone

Concen: 54.812 ug/l

RT: 2.374 min Scan# 211

Delta R.T. -0.000 min

Lab File: VX034127.D




Acq: 10 Feb 2023 20:08


Tgt Ion: 43 Resp: 25110

Ion Ratio Lower Upper

43 100

58 28.9 22.6 33.8

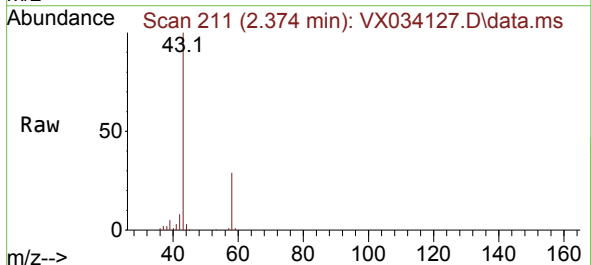



#17

Carbon Disulfide

Concen: 0.532 ug/l

RT: 2.514 min Scan# 21

Delta R.T. -0.000 min

Lab File: VX034127.D


Acq: 10 Feb 2023 20:08

Instrument :

MSVOA_X

ClientSampleId :

EA-FILTERBAGS-0208






Tgt Ion: 76 Resp: 1244

Ion Ratio Lower Upper

76 100

78 7.8 7.0 10.6

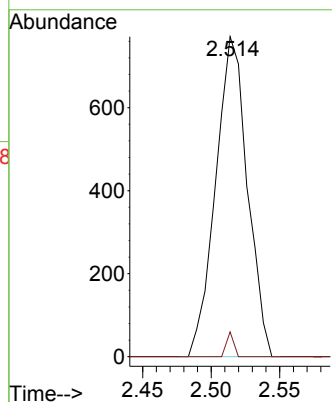

#18

Methyl Acetate

Concen: 0.671 ug/l

RT: 2.697 min Scan# 264

Delta R.T. -0.000 min

Lab File: VX034127.D




Acq: 10 Feb 2023 20:08


Tgt Ion: 43 Resp: 956

Ion Ratio Lower Upper

43 100

74 21.7 18.2 27.4


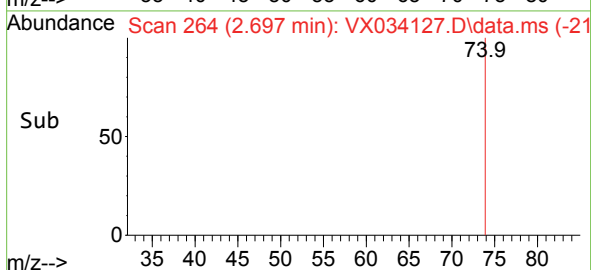






#20
Methylene Chloride
Concen: 7.227 ug/l
RT: 2.788 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX034127.D
Acq: 10 Feb 2023 20:08




Instrument :
MSVOA_X
ClientSampleId :
EA-FILTERBAGS-0208


Tgt Ion: 84	Resp:	7574	
Ion	Ratio	Lower	Upper
84	100		
49	117.9	101.1	151.7
51	32.4	31.0	46.6
86	66.4	52.6	79.0

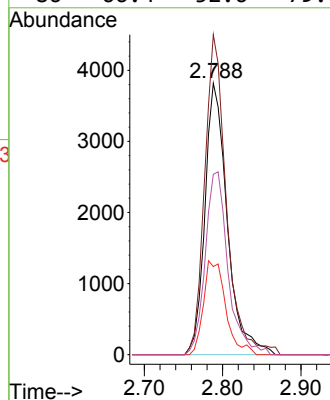

#21
trans-1,2-Dichloroethene
Concen: 0.258 ug/l
RT: 3.099 min Scan# 330
Delta R.T. 0.006 min
Lab File: VX034127.D
Acq: 10 Feb 2023 20:08

Tgt Ion: 96	Resp:	259	
Ion	Ratio	Lower	Upper
96	100		
61	62.5	106.7	160.1#
98	58.1	50.0	75.0

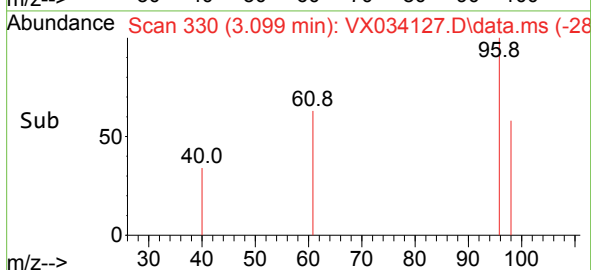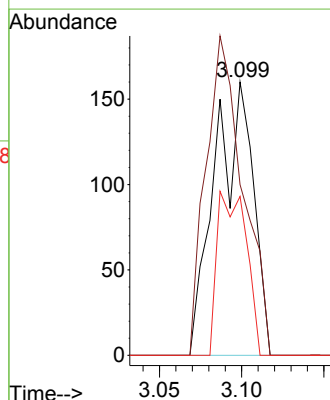



#25

2-Butanone

Concen: 4.838 ug/l

RT: 4.562 min Scan# 51

Delta R.T. 0.012 min

Lab File: VX034127.D

Acq: 10 Feb 2023 20:08

Instrument :

MSVOA_X

ClientSampleId :





EA-FILTERBAGS-0208

Tgt Ion: 43 Resp: 3227

Ion Ratio Lower Upper

43 100

72 23.0 19.4 29.2

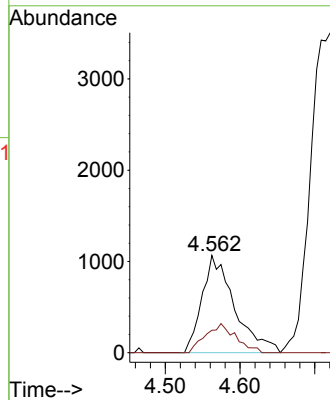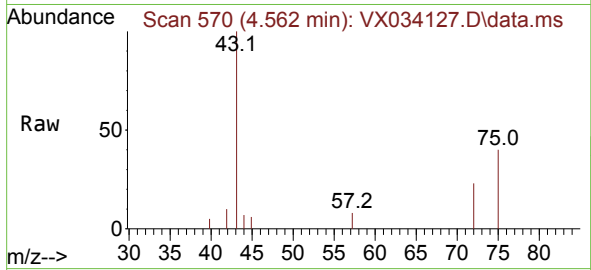

#29

Tetrahydrofuran

Concen: 0.620 ug/l

RT: 5.032 min Scan# 647

Delta R.T. 0.030 min

Lab File: VX034127.D

Acq: 10 Feb 2023 20:08




Tgt Ion: 42 Resp: 263


Ion Ratio Lower Upper

42 100

72 0.0 34.8 52.2#

71 0.0 32.2 48.2#



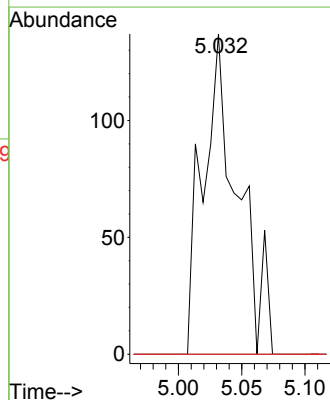





#33
 1,2-Dichloroethane-d4
 Concen: 52.091 ug/l
 RT: 5.952 min Scan# 798
 Delta R.T. -0.000 min
 Lab File: VX034127.D
 Acq: 10 Feb 2023 20:08




Instrument :
 MSVOA_X
 ClientSampleId :
 EA-FILTERBAGS-0208


Tgt Ion: 65 Resp: 56500
 Ion Ratio Lower Upper
 65 100
 67 50.8 0.0 104.8

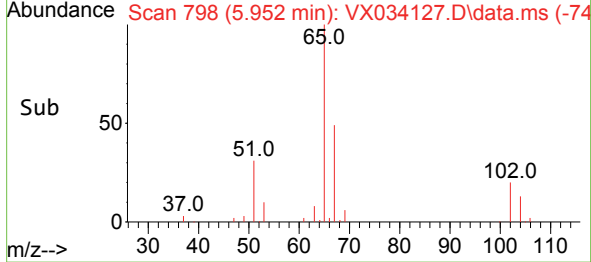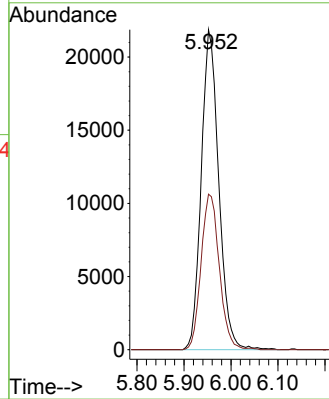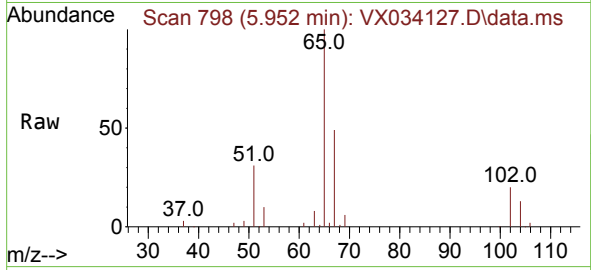

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.763 min Scan# 931
 Delta R.T. 0.006 min
 Lab File: VX034127.D
 Acq: 10 Feb 2023 20:08

Tgt Ion: 114 Resp: 155216
 Ion Ratio Lower Upper
 114 100
 63 16.7 0.0 37.4
 88 16.1 0.0 30.6

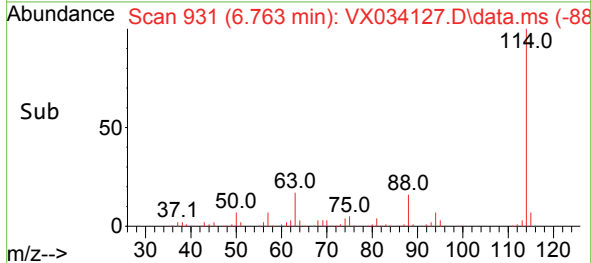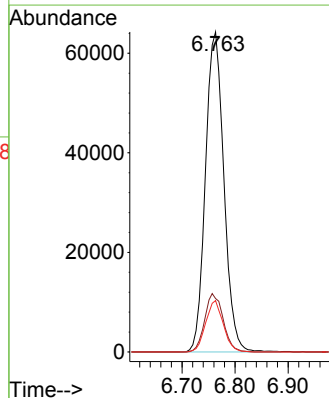

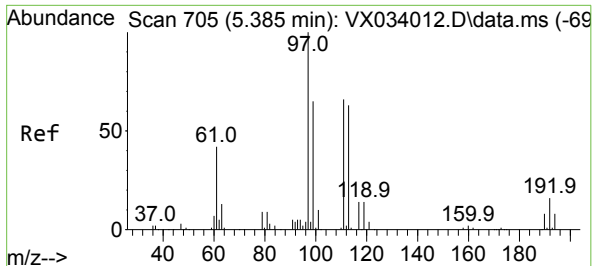

#35

Dibromofluoromethane

Concen: 50.620 ug/l

RT: 5.385 min Scan# 705

Delta R.T. -0.000 min

Lab File: VX034127.D


Acq: 10 Feb 2023 20:08

Instrument :




MSVOA_X

ClientSampleId :

EA-FILTERBAGS-0208

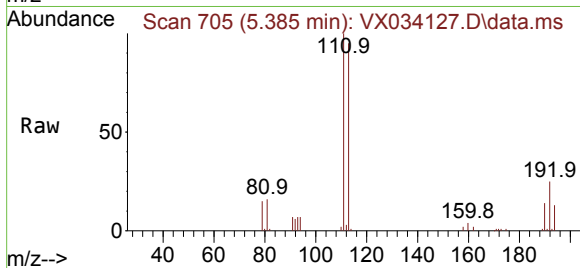

Tgt Ion:	113	Resp:	50005
Ion	Ratio	Lower	Upper
113	100		
111	100.7	83.0	124.6
192	24.5	19.0	28.4

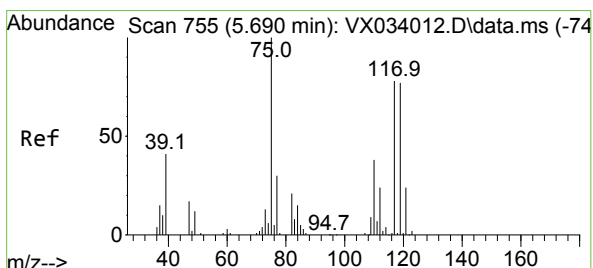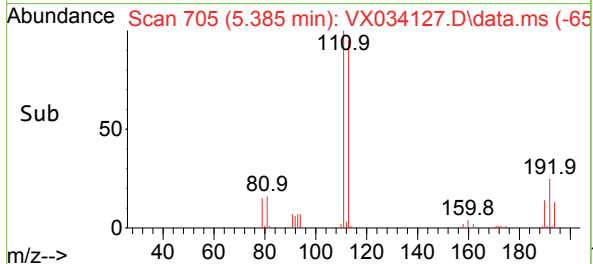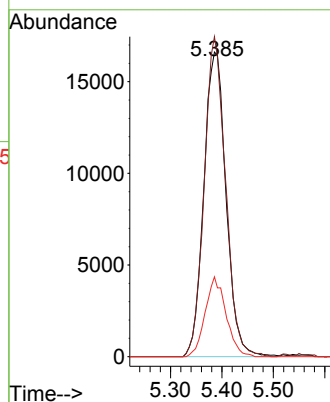

#36

1,1-Dichloropropene

Concen: 4.931 ug/l




RT: 5.556 min Scan# 733


Delta R.T. -0.134 min

Lab File: VX034127.D

Acq: 10 Feb 2023 20:08

Tgt Ion:	75	Resp:	6678
Ion	Ratio	Lower	Upper
75	100		
110	8.5	18.8	56.4#
77	0.0	25.1	37.7#

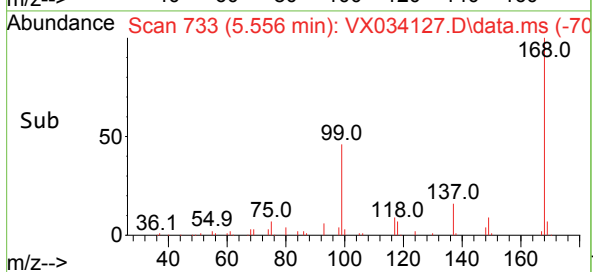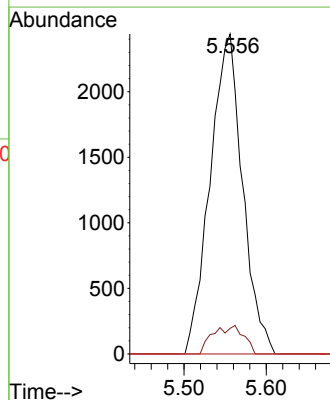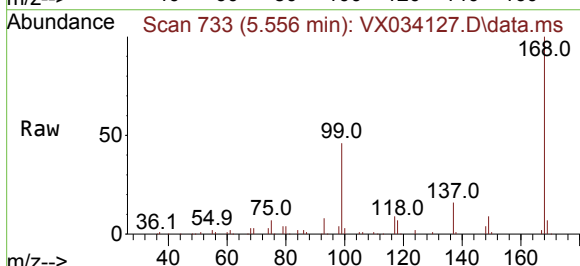



#37

Ethyl Acetate

Concen: 9.373 ug/l

RT: 4.721 min Scan# 596

Delta R.T. 0.012 min

Lab File: VX034127.D

Acq: 10 Feb 2023 20:08





Instrument :

MSVOA_X

ClientSampleId :

EA-FILTERBAGS-0208

Tgt Ion: 43	Resp: 11826
Ion Ratio	Lower Upper
43	100
61	13.4 11.1 16.7
70	11.1 8.5 12.7



#38

Carbon Tetrachloride

Concen: 6.732 ug/l




RT: 5.550 min Scan# 732


Delta R.T. -0.128 min

Lab File: VX034127.D

Acq: 10 Feb 2023 20:08

Tgt Ion: 117	Resp: 9724
Ion Ratio	Lower Upper
117	100
119	4.3 78.0 117.0#
121	0.0 24.4 36.6#



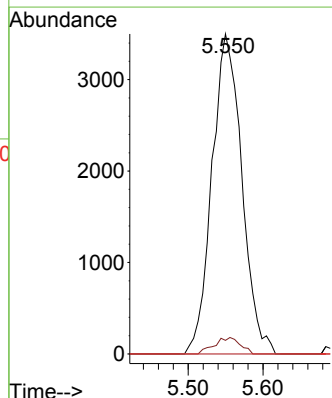





#43
Isopropyl Acetate
Concen: 24.733 ug/l
RT: 6.336 min Scan# 81
Delta R.T. -0.000 min
Lab File: VX034127.D
Acq: 10 Feb 2023 20:08




Instrument :
MSVOA_X
ClientSampleId :
EA-FILTERBAGS-0208


Tgt Ion: 43 Resp: 48666
Ion Ratio Lower Upper
43 100
61 20.7 15.7 23.5
87 14.8 10.6 15.8

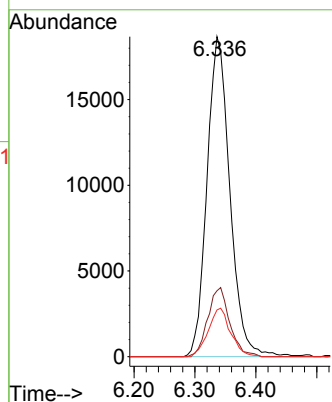

#48
Methyl methacrylate
Concen: 34.919 ug/l
RT: 7.793 min Scan# 1100
Delta R.T. 0.104 min
Lab File: VX034127.D
Acq: 10 Feb 2023 20:08

Tgt Ion: 41 Resp: 35475
Ion Ratio Lower Upper
41 100
69 0.1 63.1 94.7#
39 52.8 43.2 64.8









#50
Toluene-d8
Concen: 49.502 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX034127.D
Acq: 10 Feb 2023 20:08




Instrument :
MSVOA_X
ClientSampleId :
EA-FILTERBAGS-0208


Tgt Ion: 98 Resp: 176184
Ion Ratio Lower Upper
98 100
100 66.9 53.6 80.4

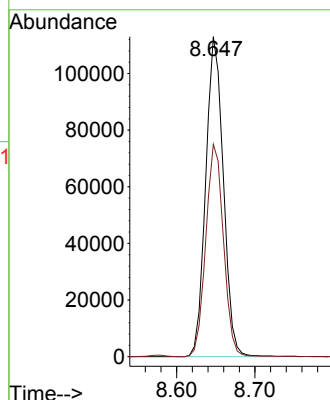

#51
4-Methyl-2-Pentanone
Concen: 34.049 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.024 min
Lab File: VX034127.D
Acq: 10 Feb 2023 20:08

Tgt Ion: 43 Resp: 42024
Ion Ratio Lower Upper
43 100
58 9.5 31.2 46.8#


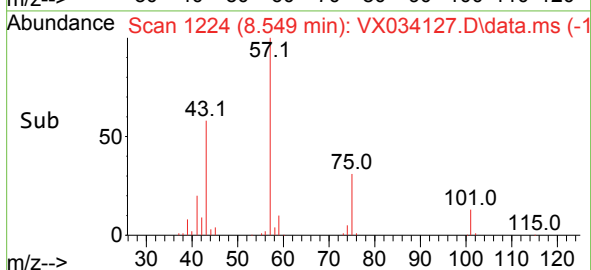
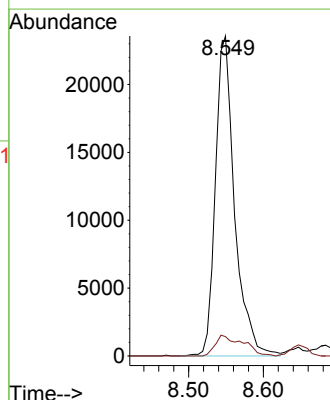





#54
 cis-1,3-Dichloropropene
 Concen: 12.767 ug/l
 RT: 8.549 min Scan# 1194
 Delta R.T. 0.183 min
 Lab File: VX034127.D
 Acq: 10 Feb 2023 20:08




Instrument :
 MSVOA_X
 ClientSampleId :
 EA-FILTERBAGS-0208


Tgt Ion: 75 Resp: 19180
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.0 37.6#
 39 27.1 38.6 58.0#

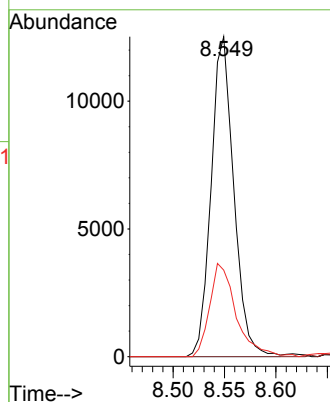

#56
 Ethyl methacrylate
 Concen: 0.221 ug/l
 RT: 9.244 min Scan# 1338
 Delta R.T. 0.128 min
 Lab File: VX034127.D
 Acq: 10 Feb 2023 20:08

Tgt Ion: 69 Resp: 313
 Ion Ratio Lower Upper
 69 100
 41 7336.1 55.1 82.7#
 39 3003.2 28.5 42.7#

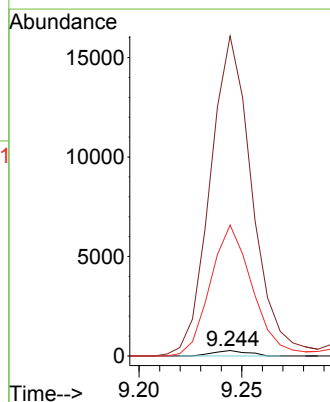



#57

1,3-Dichloropropane

Concen: 0.999 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.177 min

Lab File: VX034127.D

Acq: 10 Feb 2023 20:08

Instrument :

MSVOA_X

ClientSampleId :





EA-FILTERBAGS-0208

Tgt Ion: 76 Resp: 1656

Ion Ratio Lower Upper

76 100

78 0.0 25.6 38.4#

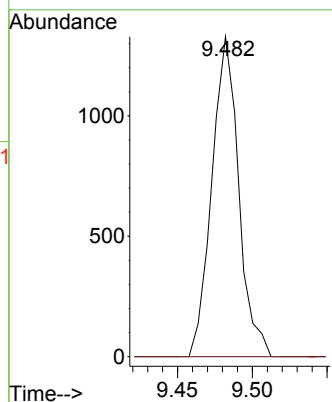

#59

2-Hexanone

Concen: 25.543 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.055 min

Lab File: VX034127.D




Acq: 10 Feb 2023 20:08


Tgt Ion: 43 Resp: 23071

Ion Ratio Lower Upper

43 100

58 18.2 27.4 82.0#


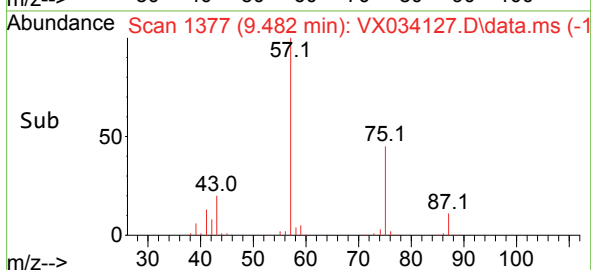






#62
4-Bromofluorobenzene
Concen: 49.558 ug/l
RT: 11.079 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX034127.D
Acq: 10 Feb 2023 20:08




Instrument :
MSVOA_X
ClientSampleId :
EA-FILTERBAGS-0208


Tgt Ion: 95 Resp: 62996
Ion Ratio Lower Upper
95 100
174 98.6 0.0 184.4
176 96.2 0.0 178.8

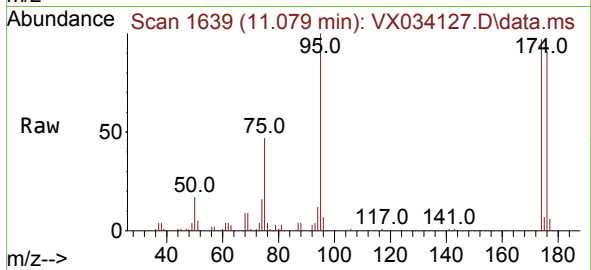

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX034127.D
Acq: 10 Feb 2023 20:08

Tgt Ion: 117 Resp: 138361
Ion Ratio Lower Upper
117 100
82 49.7 40.6 60.8
119 31.2 25.6 38.4


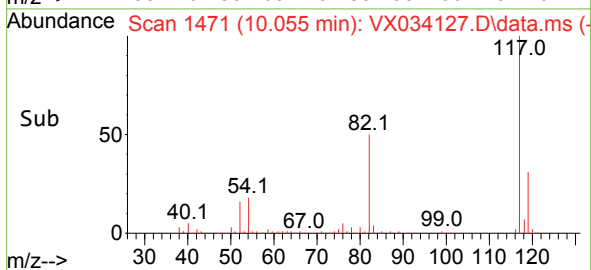






#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX034127.D
 Acq: 10 Feb 2023 20:08




Instrument :
 MSVOA_X
 ClientSampleId :
 EA-FILTERBAGS-0208


Tgt Ion:152 Resp: 70283
 Ion Ratio Lower Upper
 152 100
 115 54.7 38.7 116.1
 150 154.8 0.0 348.2

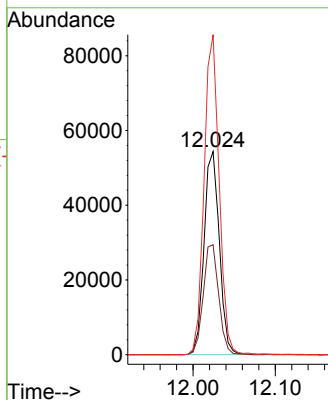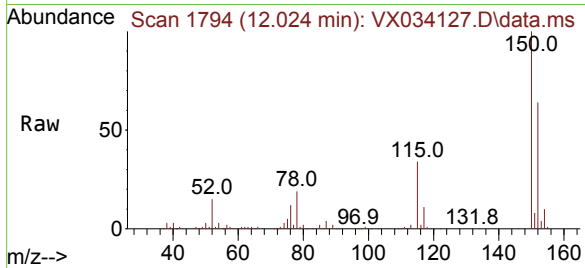

#76
 1,2,3-Trichloropropane
 Concen: 24.774 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. -0.159 min
 Lab File: VX034127.D
 Acq: 10 Feb 2023 20:08

Tgt Ion: 75 Resp: 29898
 Ion Ratio Lower Upper
 75 100
 77 1.1 21.8 65.4#



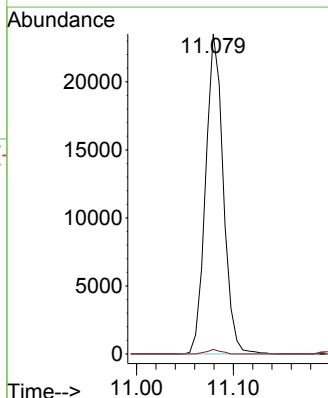
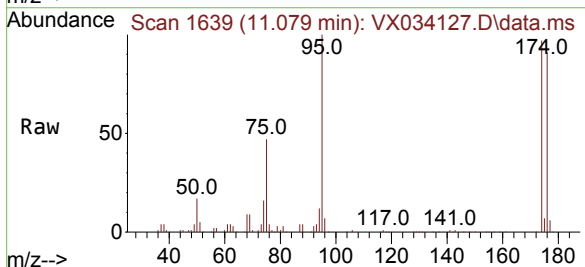




#81
trans-1,4-Dichloro-2-butene
Concen: 76.296 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX034127.D
Acq: 10 Feb 2023 20:08




Instrument :
MSVOA_X
ClientSampleId :
EA-FILTERBAGS-0208


Tgt Ion: 75 Resp: 29898
Ion Ratio Lower Upper
75 100
53 0.0 83.0 124.6#
89 0.0 37.7 56.5#

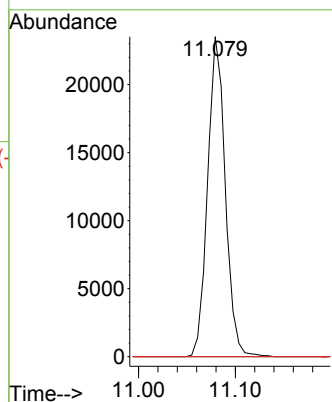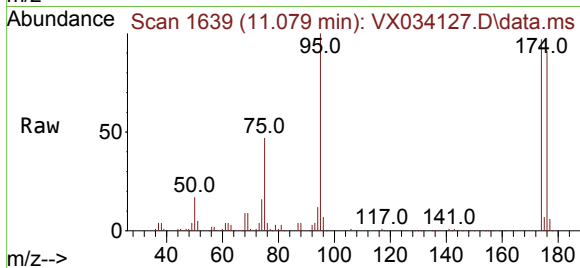

#87
1,3-Dichlorobenzene
Concen: 0.255 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. 0.006 min
Lab File: VX034127.D
Acq: 10 Feb 2023 20:08

Tgt Ion:146 Resp: 609
Ion Ratio Lower Upper
146 100
111 31.5 18.6 55.6
148 65.0 31.9 95.5


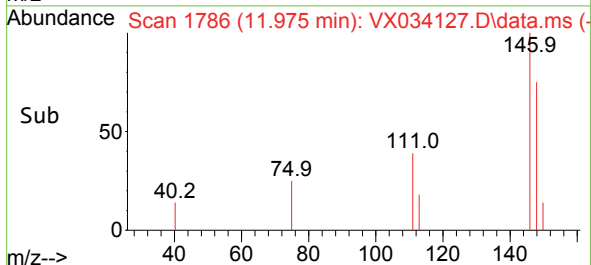

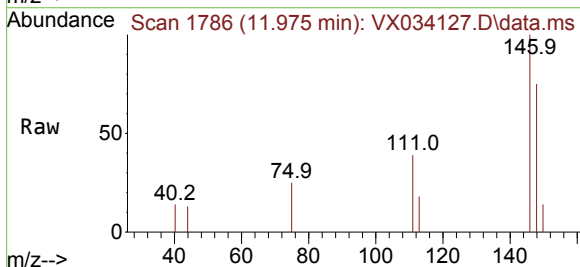




#88
1,4-Dichlorobenzene
Concen: 0.251 ug/l
RT: 11.975 min Scan# 11
Delta R.T. -0.067 min
Lab File: VX034127.D
Acq: 10 Feb 2023 20:08




Instrument :
MSVOA_X
ClientSampleId :
EA-FILTERBAGS-0208


Tgt Ion:146 Resp: 609
Ion Ratio Lower Upper
146 100
111 31.5 17.8 53.4
148 65.0 32.1 96.3

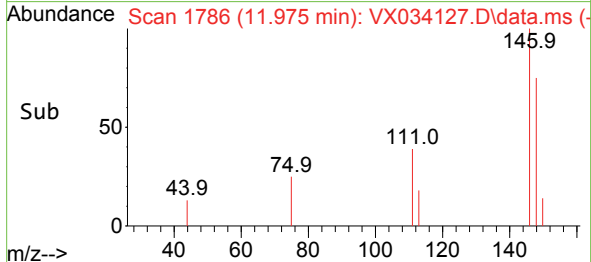

#89
n-Butylbenzene
Concen: 0.280 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.006 min
Lab File: VX034127.D
Acq: 10 Feb 2023 20:08

Tgt Ion: 91 Resp: 930
Ion Ratio Lower Upper
91 100
92 56.8 27.5 82.5
134 29.6 14.3 42.9

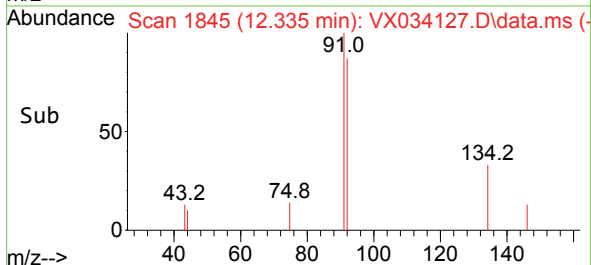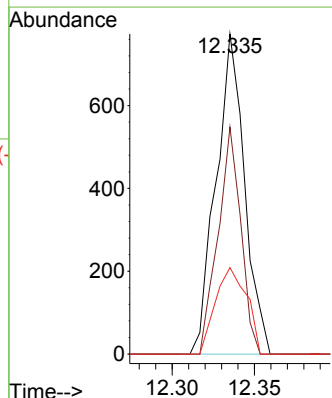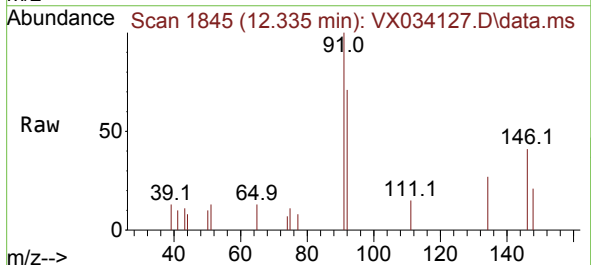



#93

1,2,4-Trichlorobenzene

Concen: 0.492 ug/l

RT: 13.591 min Scan# 2051

Delta R.T. 0.006 min

Lab File: VX034127.D

Acq: 10 Feb 2023 20:08

Instrument :

MSVOA_X

ClientSampleId :

EA-FILTERBAGS-0208





Tgt Ion:180 Resp: 811

Ion Ratio Lower Upper

180 100

182 98.8 47.9 143.6

145 32.8 14.1 42.2

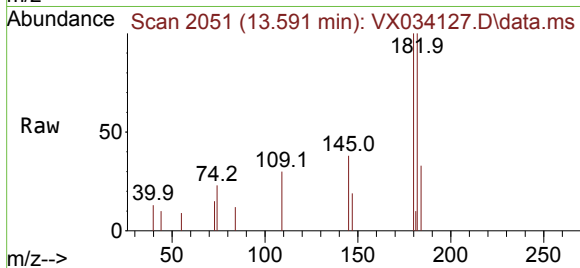

#94

Hexachlorobutadiene

Concen: 0.927 ug/l

RT: 13.725 min Scan# 2073

Delta R.T. -0.000 min

Lab File: VX034127.D

Acq: 10 Feb 2023 20:08




Tgt Ion:225 Resp: 756


Ion Ratio Lower Upper

225 100

223 63.8 31.3 93.9

227 80.8 32.3 96.9


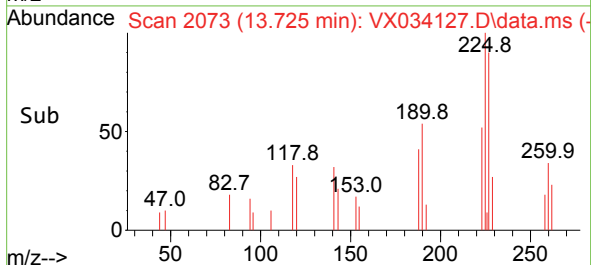
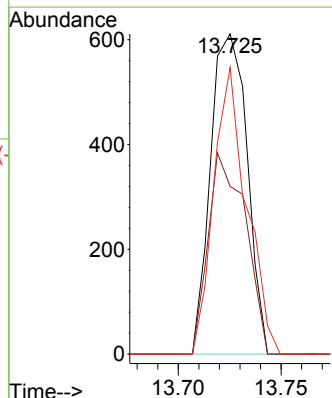
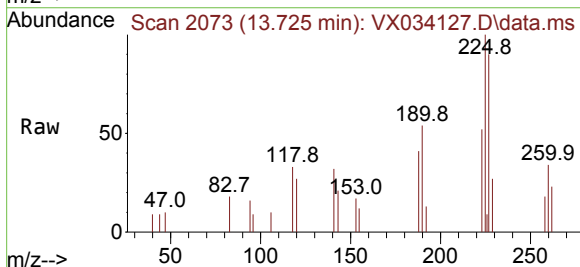




#95
Naphthalene
Concen: 0.471 ug/l
RT: 13.780 min Scan# 2081
Delta R.T. 0.006 min
Lab File: VX034127.D
Acq: 10 Feb 2023 20:08

Instrument :
MSVOA_X
ClientSampleId :
EA-FILTERBAGS-0208

Tgt Ion:128 Resp: 2132
Ion Ratio Lower Upper
128 100
127 11.0 10.3 15.5
129 9.6 8.7 13.1

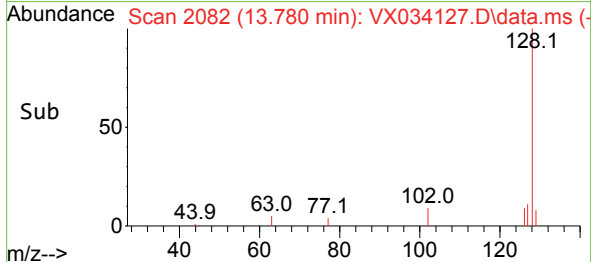

#96
1,2,3-Trichlorobenzene
Concen: 0.585 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. -0.000 min
Lab File: VX034127.D
Acq: 10 Feb 2023 20:08

Tgt Ion:180 Resp: 968
Ion Ratio Lower Upper
180 100
182 87.8 47.6 142.9
145 27.5 15.1 45.3

