

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021223\
 Data File : VX034112.D
 Acq On : 10 Feb 2023 14:18
 Operator : JC/MD
 Sample : 01519-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-RW10-GW-658-660

Quant Time: Feb 11 02:50:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 03 23:25:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	119445	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	161654	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	141312	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	68152	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	58608	50.897	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	101.800%
35) Dibromofluoromethane	5.385	113	51379	49.940	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.880%
50) Toluene-d8	8.647	98	181468	48.956	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	97.920%
62) 4-Bromofluorobenzene	11.079	95	63492	47.959	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	95.920%
Target Compounds						
16) Acetone	2.373	43	1607	3.304	ug/l	Qvalue # 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021223\
Data File : VX034112.D
Acq On : 10 Feb 2023 14:18
Operator : JC/MD
Sample : 01519-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10-GW-658-660

Quant Time: Feb 11 02:50:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 03 23:25:45 2023
Response via : Initial Calibration




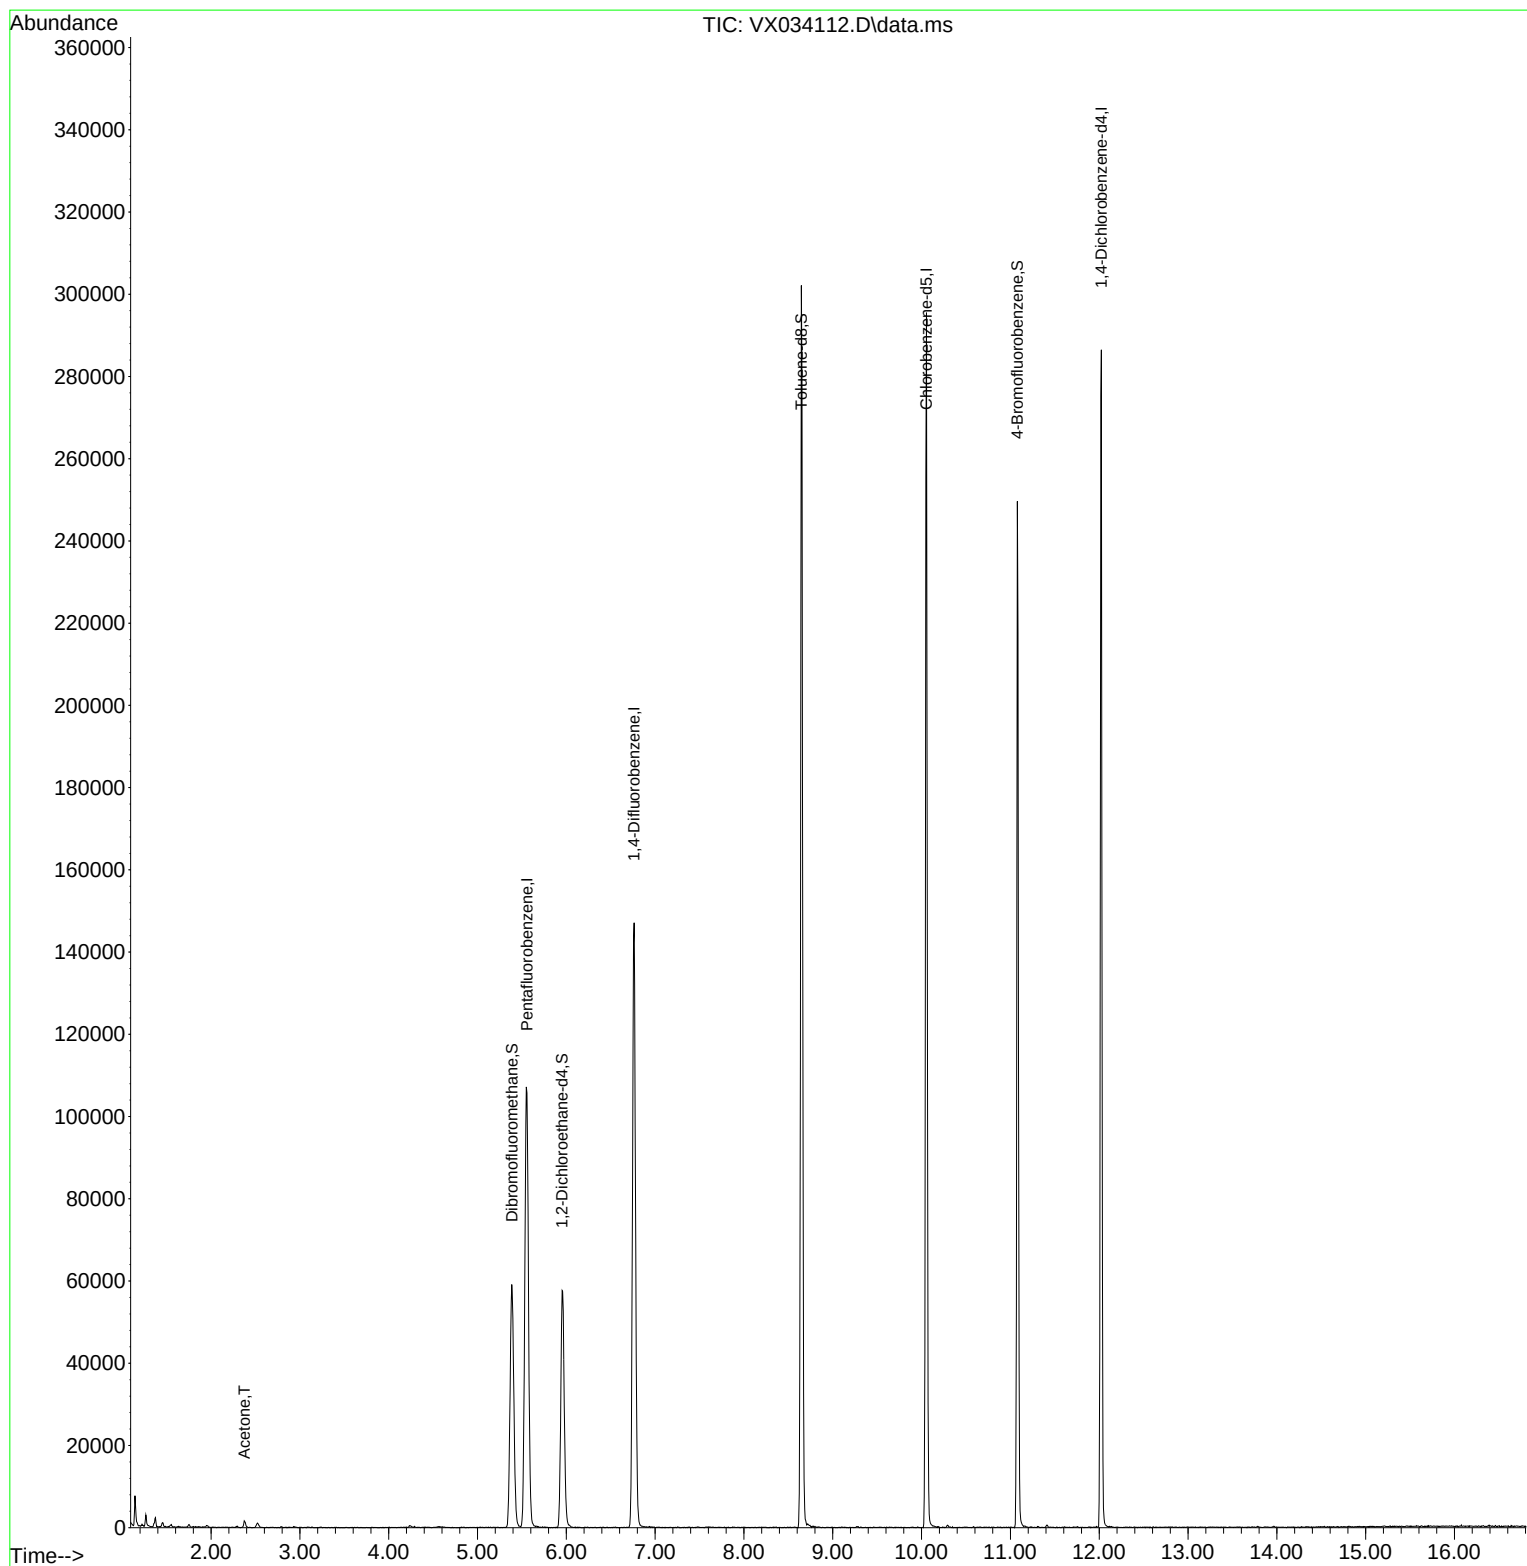


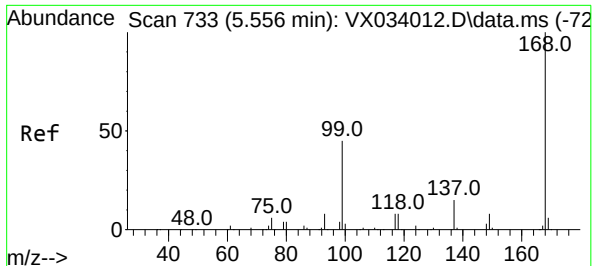

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX034112.D
Acq: 10 Feb 2023 14:18




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10-GW-658-660


Tgt Ion:168 Resp: 119445
Ion Ratio Lower Upper
168 100
99 46.9 39.6 59.4

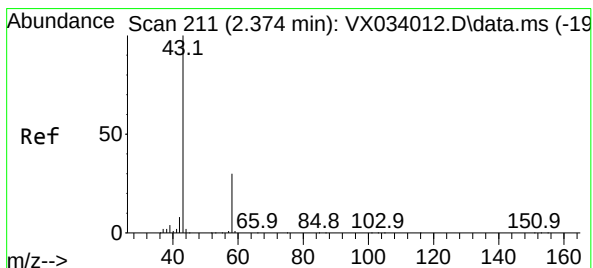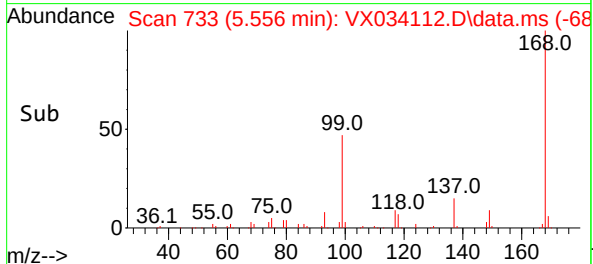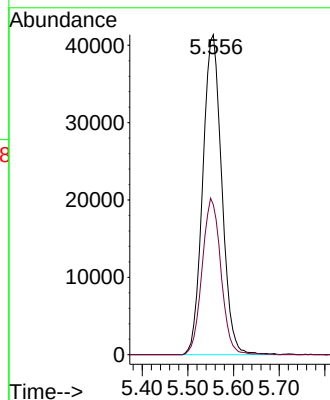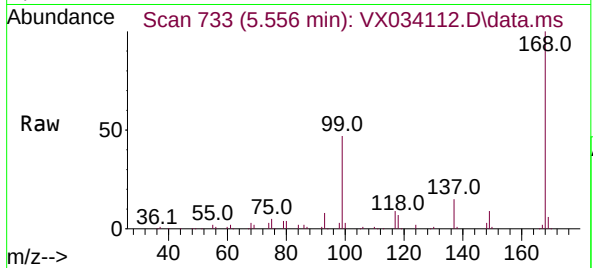

#16
Acetone
Concen: 3.304 ug/l
RT: 2.373 min Scan# 211
Delta R.T. -0.000 min
Lab File: VX034112.D
Acq: 10 Feb 2023 14:18

Tgt Ion: 43 Resp: 1607
Ion Ratio Lower Upper
43 100
58 34.5 22.6 33.8#

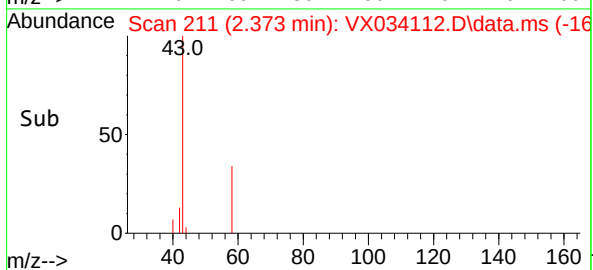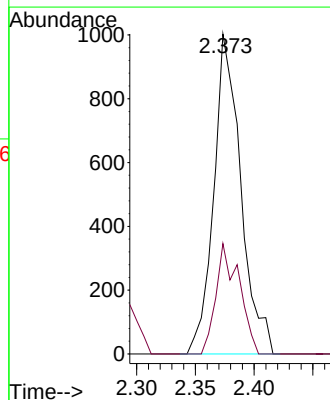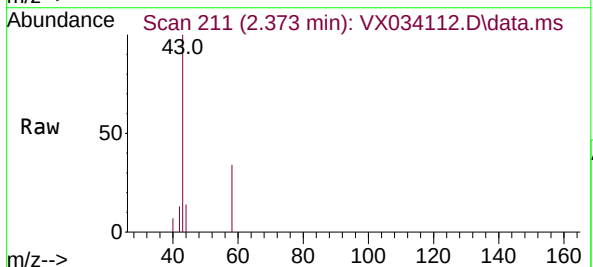

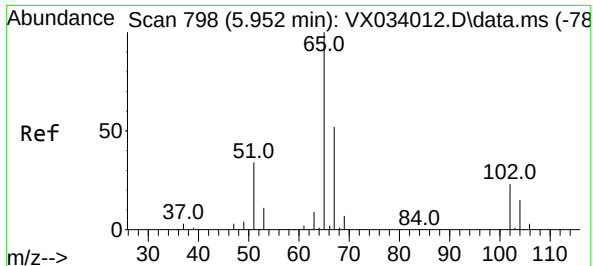

#33

1,2-Dichloroethane-d4

Concen: 50.897 ug/l

RT: 5.952 min Scan# 798

Delta R.T. -0.000 min

Lab File: VX034112.D

Acq: 10 Feb 2023 14:18

Instrument :

MSVOA_X

ClientSampleId :





BP-VPB-RW10-GW-658-660

Tgt Ion: 65 Resp: 58608

Ion Ratio Lower Upper

65 100

67 51.0 0.0 104.8

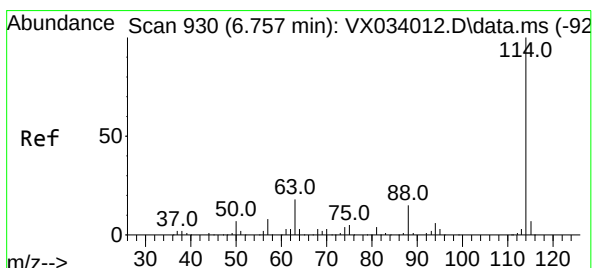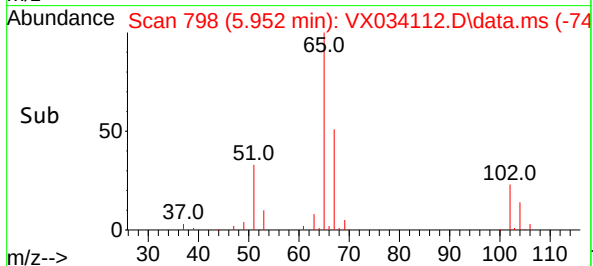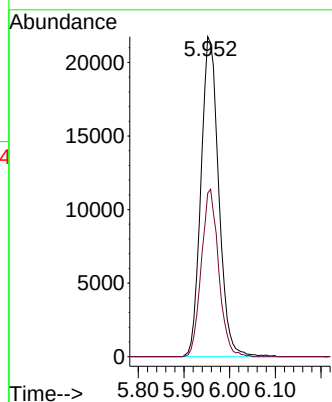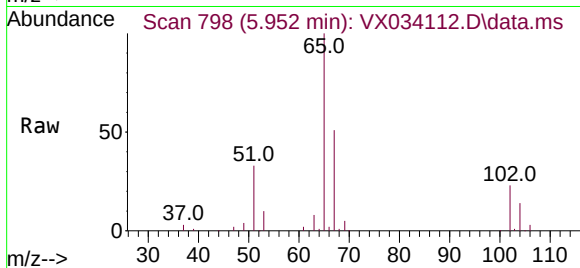

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.006 min

Lab File: VX034112.D

Acq: 10 Feb 2023 14:18




Tgt Ion: 114 Resp: 161654


Ion Ratio Lower Upper

114 100

63 18.4 0.0 37.4

88 14.9 0.0 30.6


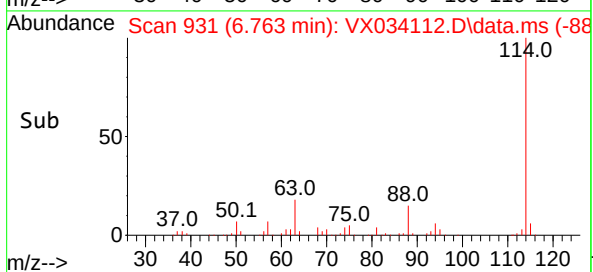
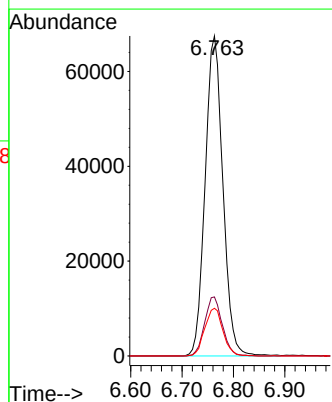
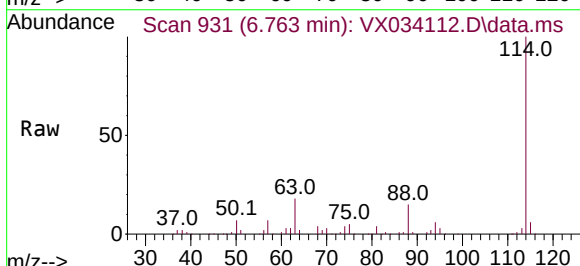


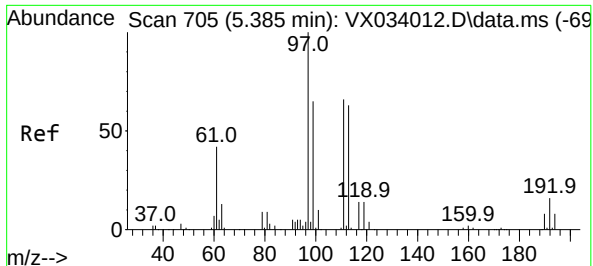

#35
Dibromofluoromethane
Concen: 49.940 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX034112.D
Acq: 10 Feb 2023 14:18




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10-GW-658-660


Tgt Ion:113 Resp: 51379
Ion Ratio Lower Upper
113 100
111 103.9 83.0 124.6
192 25.7 19.0 28.4

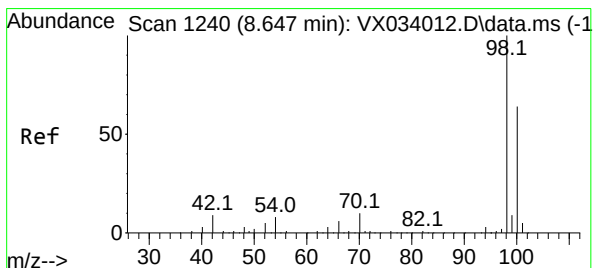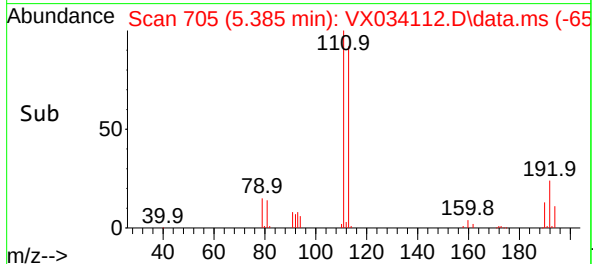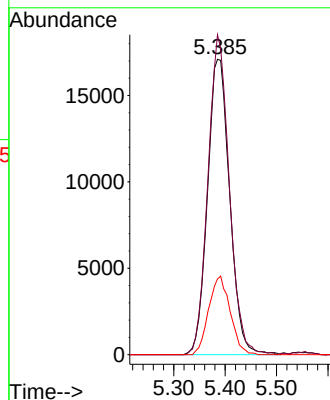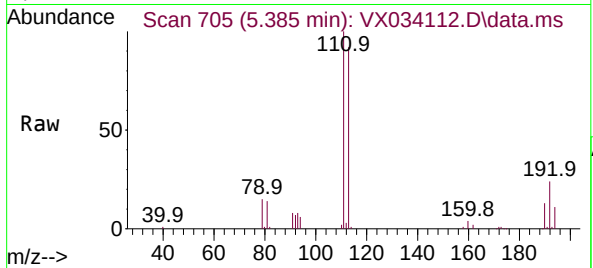

#50
Toluene-d8
Concen: 48.956 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX034112.D
Acq: 10 Feb 2023 14:18

Tgt Ion: 98 Resp: 181468
Ion Ratio Lower Upper
98 100
100 67.7 53.6 80.4


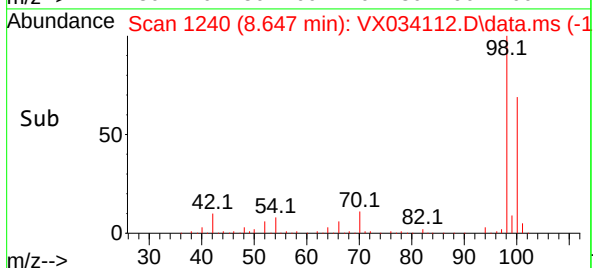
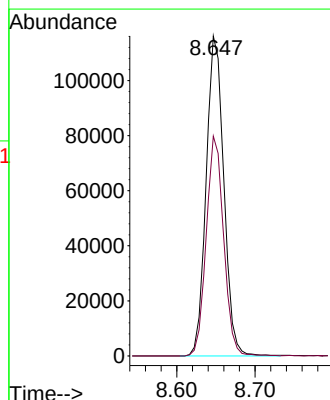
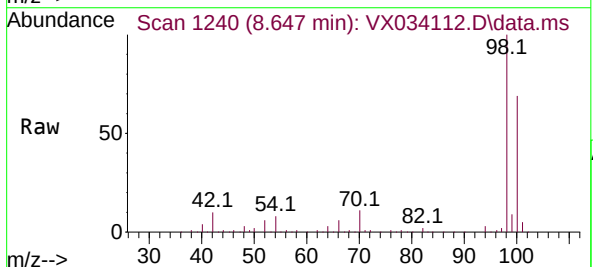


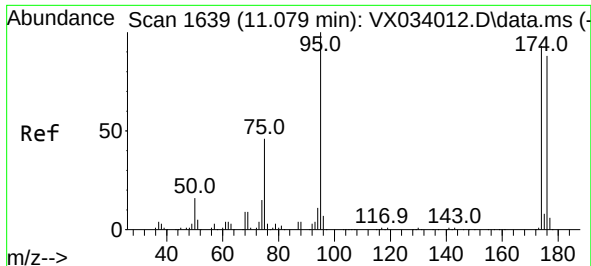

#62
4-Bromofluorobenzene
Concen: 47.959 ug/l
RT: 11.079 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX034112.D
Acq: 10 Feb 2023 14:18




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10-GW-658-660


Tgt Ion: 95 Resp: 63492
Ion Ratio Lower Upper
95 100
174 98.2 0.0 184.4
176 94.7 0.0 178.8

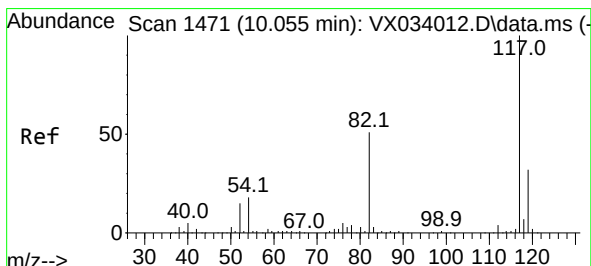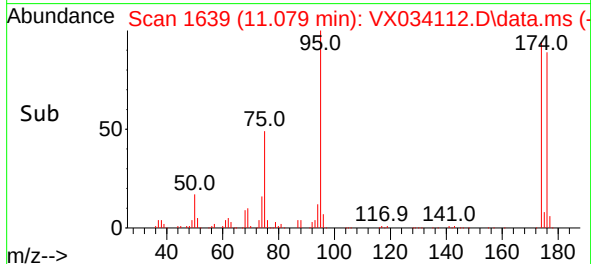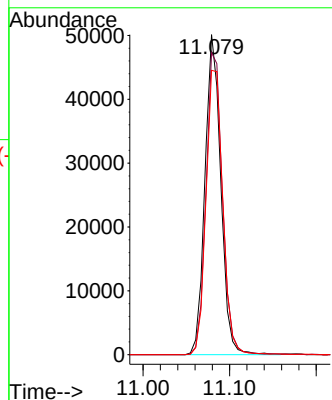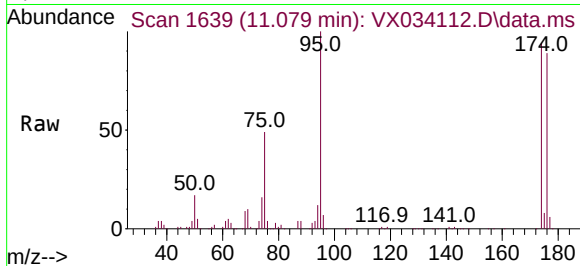

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX034112.D
Acq: 10 Feb 2023 14:18


Tgt Ion: 117 Resp: 141312
Ion Ratio Lower Upper
117 100
82 49.6 40.6 60.8
119 31.9 25.6 38.4

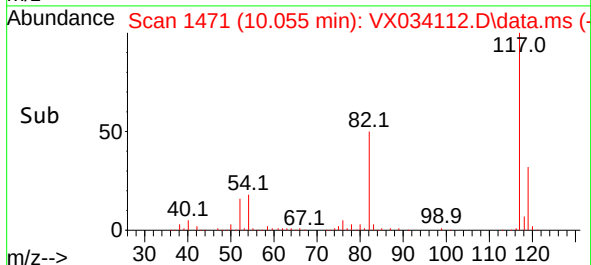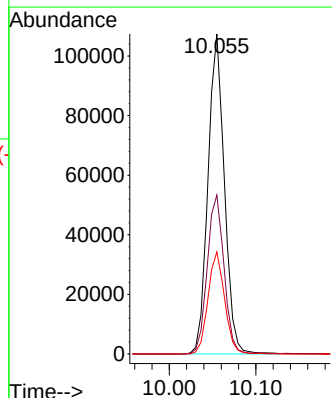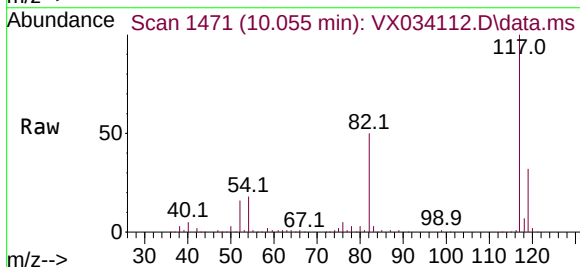

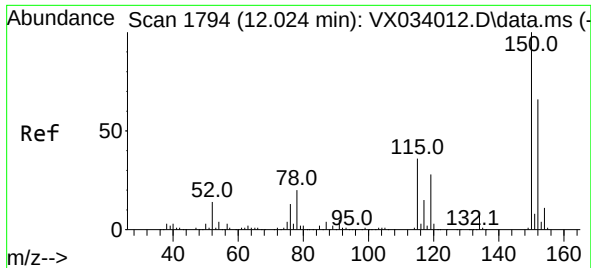

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX034112.D
 Acq: 10 Feb 2023 14:18

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-RW10-GW-658-660

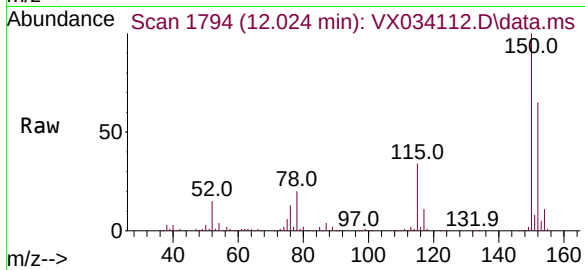

Tgt Ion:152 Resp: 68152
 Ion Ratio Lower Upper
 152 100
 115 53.3 38.7 116.1
 150 155.7 0.0 348.2

