

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021223\
Data File : VX034116.D
Acq On : 10 Feb 2023 15:52
Operator : JC/MD
Sample : 01516-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-15B-35-45-020923

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
Title : SW846 8260

Signal : TIC: VX034116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	15	rVB	6397	6083	1.29%	0.227%
2	4.495	549	559	568	rBV3	3112	8195	1.74%	0.305%
3	5.385	695	705	720	rBV	59403	172535	36.60%	6.426%
4	5.550	722	732	746	rVB	108231	305972	64.91%	11.395%
5	5.952	788	798	814	rBV	57493	154258	32.73%	5.745%
6	6.763	919	931	943	rBV	147708	355357	75.39%	13.235%
7	7.129	983	991	1004	rBV	38323	83847	17.79%	3.123%
8	8.647	1234	1240	1250	rBV	305675	471374	100.00%	17.556%
9	10.055	1465	1471	1487	rBV	300073	404937	85.91%	15.081%
10	11.079	1634	1639	1653	rBV	249522	328668	69.73%	12.241%
11	12.024	1788	1794	1803	rBV	306491	393814	83.55%	14.667%




Sum of corrected areas: 2685040

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021223\
Data File : VX034116.D
Acq On : 10 Feb 2023 15:52
Operator : JC/MD
Sample : 01516-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-15B-35-45-020923

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

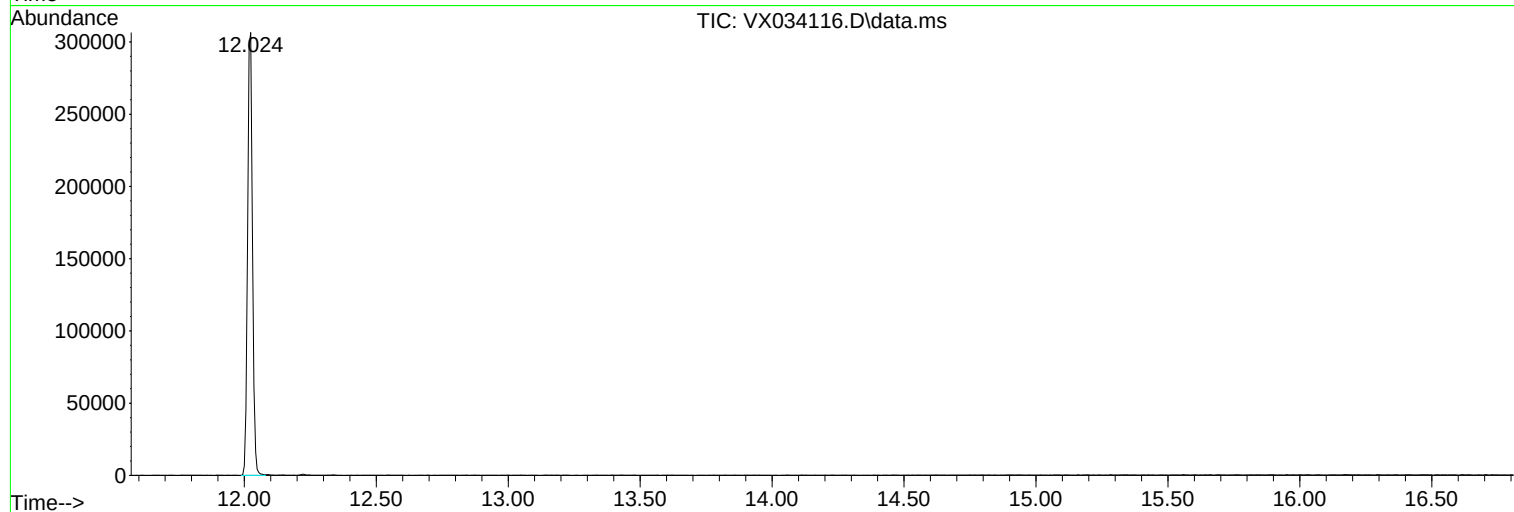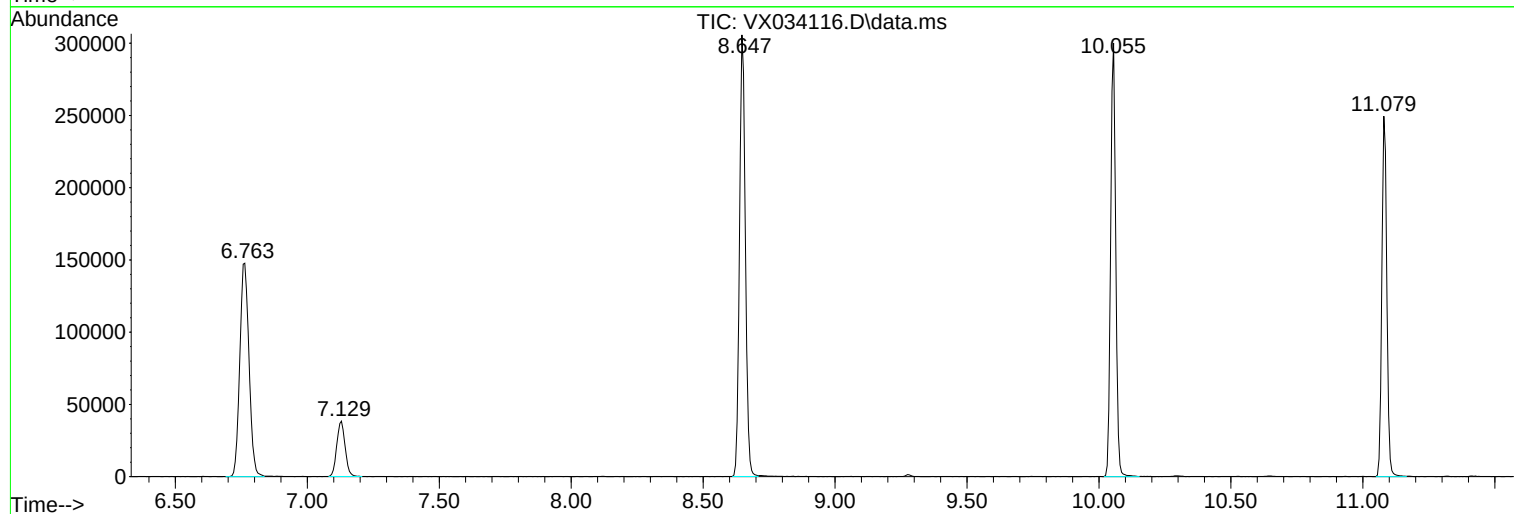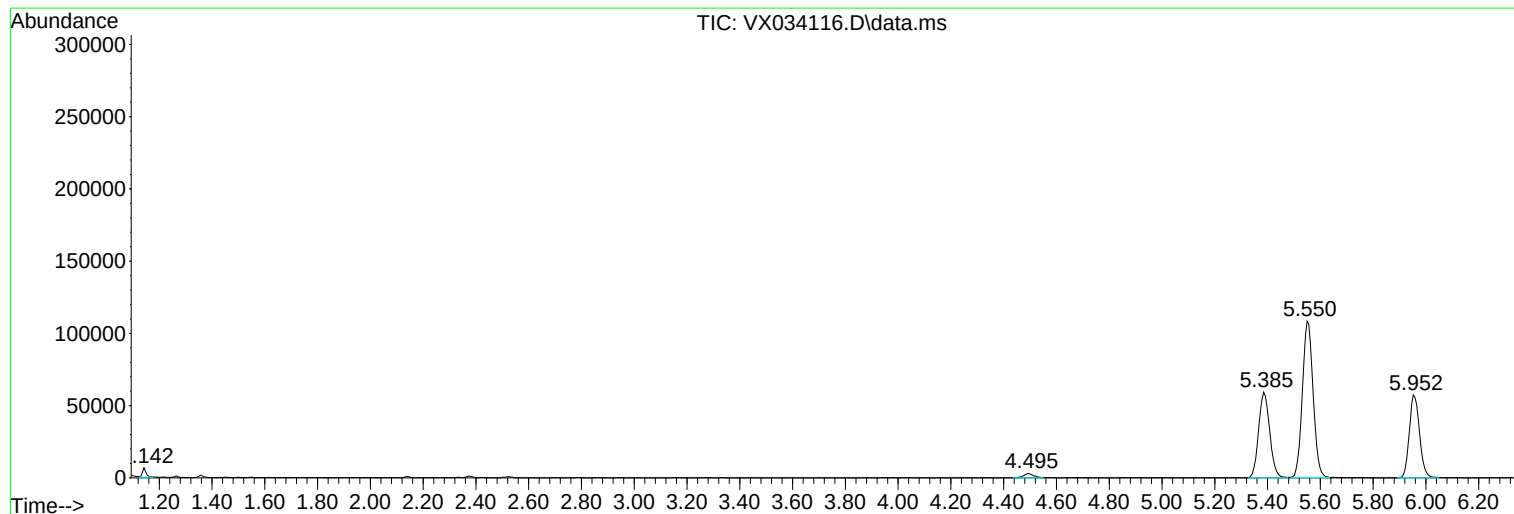

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021223\
Data File : VX034116.D
Acq On : 10 Feb 2023 15:52
Operator : JC/MD
Sample : 01516-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-15B-35-45-020923

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021223\
Data File : VX034116.D
Acq On : 10 Feb 2023 15:52
Operator : JC/MD
Sample : 01516-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-15B-35-45-020923

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------