
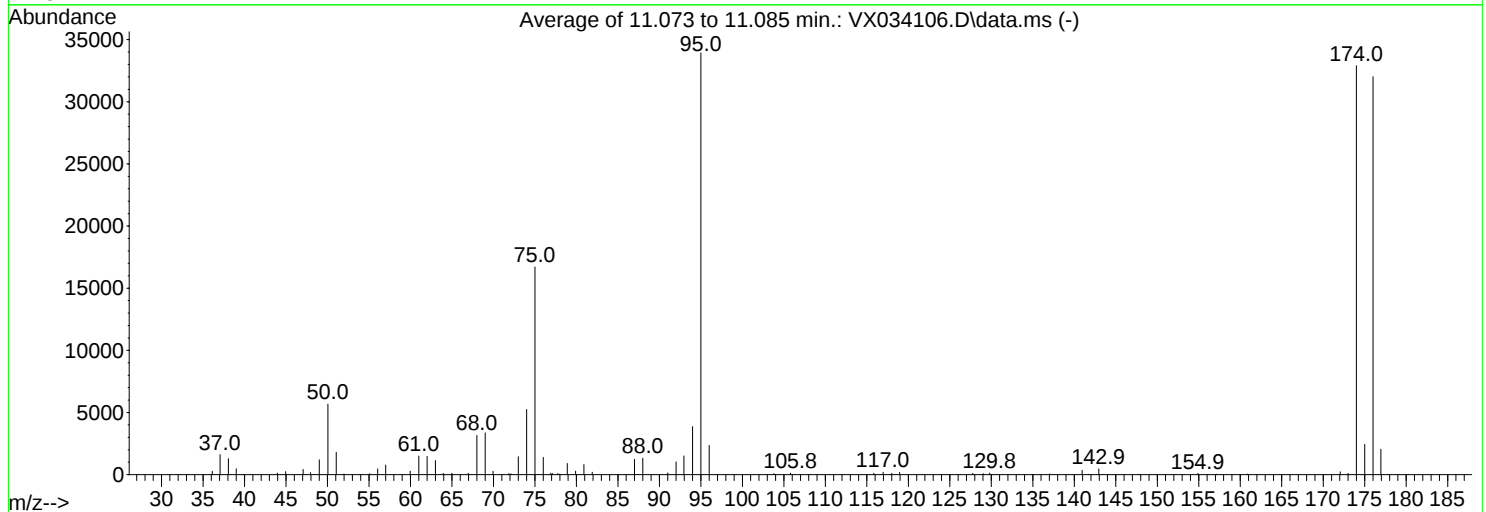


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021223\
Data File : VX034106.D
Acq On : 10 Feb 2023 11:19
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020423W.M
Title : SW846 8260
Last Update : Fri Feb 03 23:25:45 2023

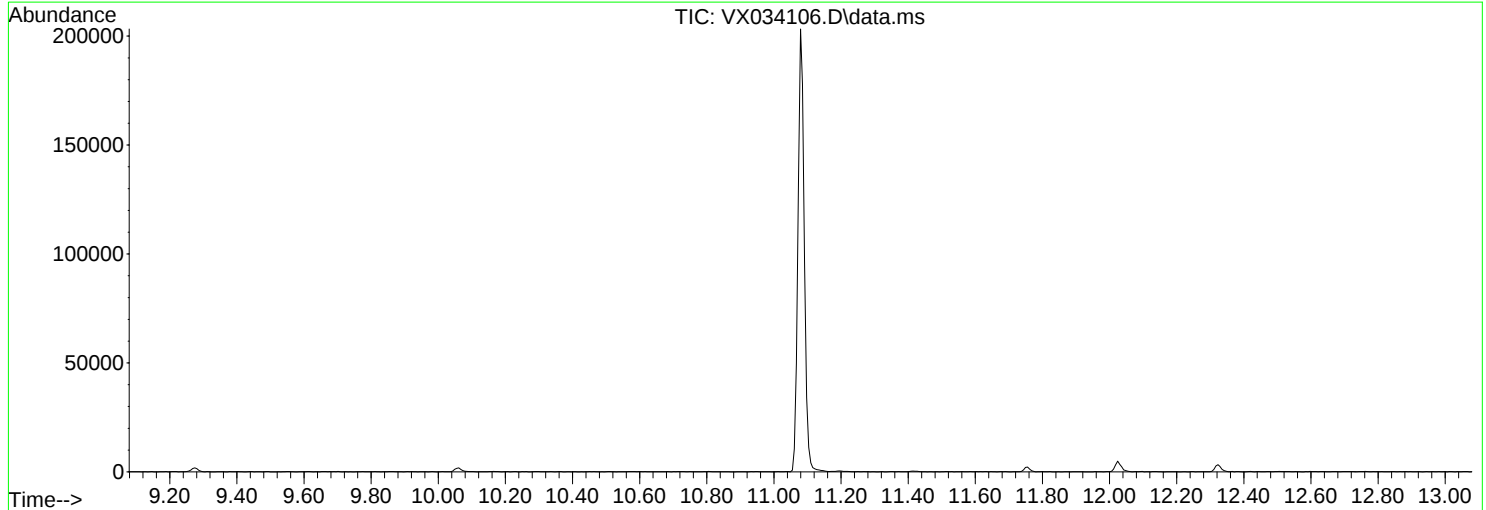

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.7	5678	PASS
75	95	30	60	49.2	16713	PASS
95	95	100	100	100.0	33936	PASS
96	95	5	9	6.9	2357	PASS
173	174	0.00	2	0.3	109	PASS
174	95	50	100	97.0	32907	PASS
175	174	5	9	7.4	2438	PASS
176	174	95	101	97.3	32016	PASS
177	176	5	9	6.4	2048	PASS