

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021425\
 Data File : VX044955.D
 Acq On : 14 Feb 2025 12:48
 Operator : JC/MD
 Sample : Q1168-09 0.2PPB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MDL-WATER-03-QT1-2025

Quant Time: Feb 14 13:15:01 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021025W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 11 03:41:08 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	94172	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	177149	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	154748	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	66049	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	85180	61.79	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 123.58%			
35) Dibromofluoromethane	5.379	113	65011	56.44	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 112.88%			
50) Toluene-d8	8.647	98	241226	55.39	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 110.78%			
62) 4-Bromofluorobenzene	11.079	95	80747	55.00	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 110.00%			
Target Compounds						Qvalue
3) Chloromethane	1.301	50	448	0.28	ug/l #	88
5) Bromomethane	1.593	94	282	0.61	ug/l	91
6) Chloroethane	1.672	64	343	1.80	ug/l	96
7) Trichlorofluoromethane	1.880	101	437	0.22	ug/l	91
11) Tert butyl alcohol	2.934	59	1656	6.48	ug/l #	73
13) Acrolein	2.227	56	388	1.47	ug/l	95
14) Allyl chloride	2.660	41	572	0.26	ug/l #	85
15) Acrylonitrile	3.081	53	717	1.05	ug/l #	80
16) Acetone	2.380	43	767	1.38	ug/l #	79
17) Carbon Disulfide	2.508	76	847	0.25	ug/l #	66
18) Methyl Acetate	2.709	43	457	0.26	ug/l #	52
19) Methyl tert-butyl Ether	3.117	73	801	0.21	ug/l #	85
20) Methylene Chloride	2.776	84	364	0.27	ug/l #	67
23) Vinyl Acetate	3.751	43	2504	0.74	ug/l #	72
29) Tetrahydrofuran	5.019	42	421	0.70	ug/l #	37
31) Cyclohexane	5.470	56	435	0.20	ug/l #	84
36) 1,1-Dichloropropene	5.544	75	8298	4.99	ug/l #	49
42) 1,2-Dichloroethane	6.105	62	416	0.25	ug/l #	74
51) 4-Methyl-2-Pentanone	8.580	43	1370	0.76	ug/l #	87
52) Toluene	8.720	92	640	0.21	ug/l	100
58) 2-Chloroethyl Vinyl ether	8.257	63	1787	1.90	ug/l	99
59) 2-Hexanone	9.470	43	952	0.73	ug/l	63
64) Tetrachloroethene	9.275	164	200	0.20	ug/l #	80
65) Chlorobenzene	10.079	112	705	0.21	ug/l #	79
68) m/p-Xylenes	10.305	106	671	0.31	ug/l	83
71) Bromoform	10.805	173	186	0.23	ug/l #	94
76) 1,2,3-Trichloropropane	11.079	75	42852	29.26	ug/l #	34
77) Bromobenzene	11.201	156	256	0.21	ug/l	96
79) 2-Chlorotoluene	11.372	91	941	0.25	ug/l	75
81) trans-1,4-Dichloro-2-b...	11.079	75	42852	75.27	ug/l #	11
91) 1,2-Dichlorobenzene	12.341	146	448	0.21	ug/l	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021425\
Data File : VX044955.D
Acq On : 14 Feb 2025 12:48
Operator : JC/MD
Sample : Q1168-09 0.2PPB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT1-2025

Quant Time: Feb 14 13:15:01 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021025W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 11 03:41:08 2025
Response via : Initial Calibration




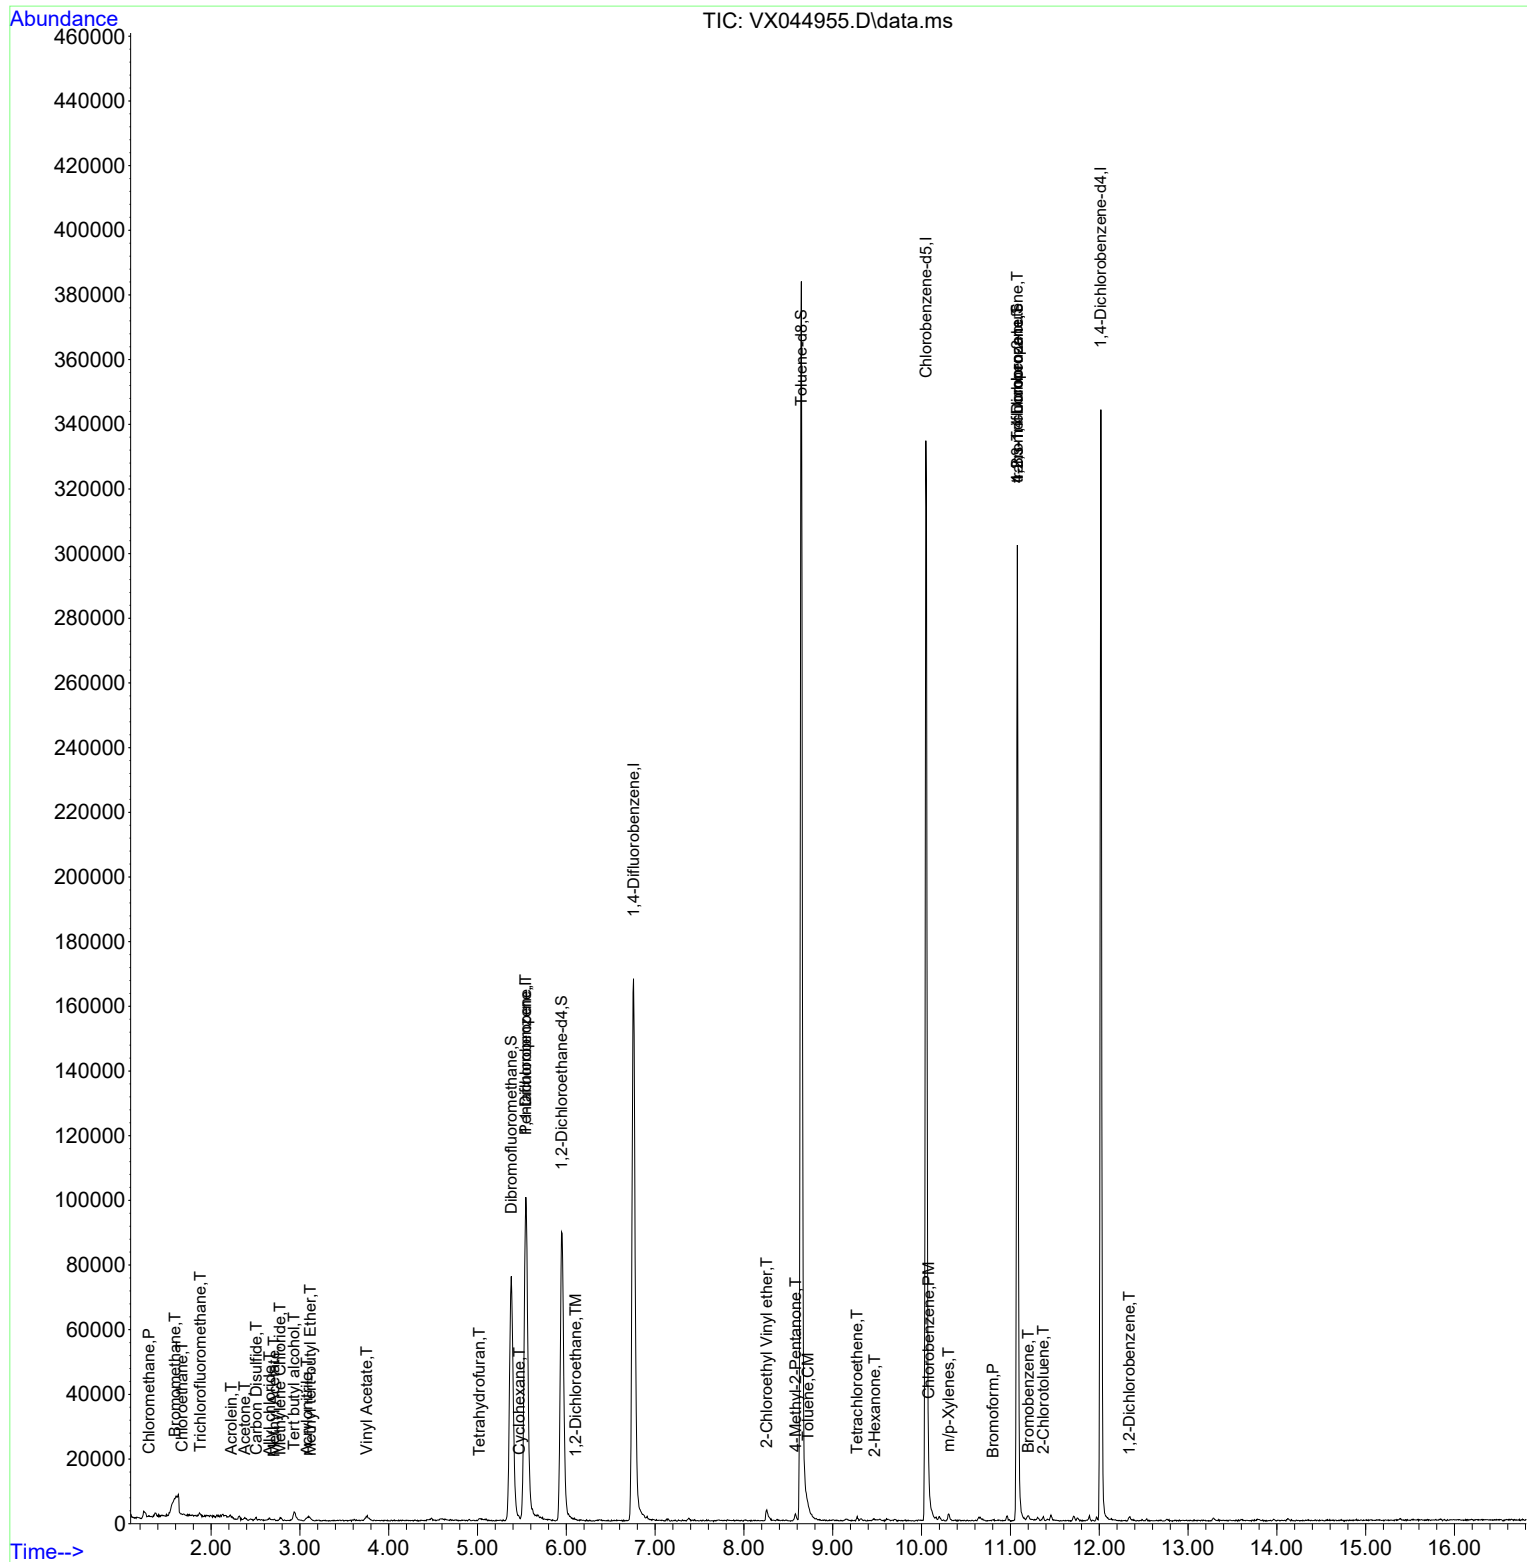




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.544 min Scan# 71
Delta R.T. 0.001 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT1-2025


Tgt Ion:168 Resp: 94172
Ion Ratio Lower Upper
168 100
99 64.9 51.2 76.8

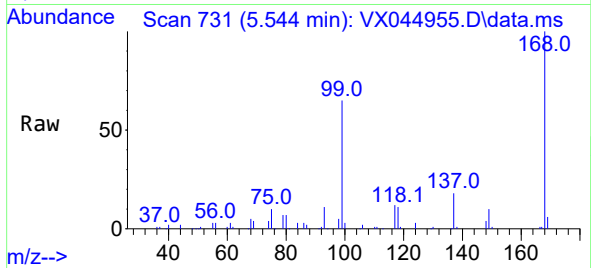

#3
Chloromethane
Concen: 0.28 ug/l
RT: 1.301 min Scan# 35
Delta R.T. 0.000 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48

Tgt Ion: 50 Resp: 448
Ion Ratio Lower Upper
50 100
52 25.5 25.9 38.9#


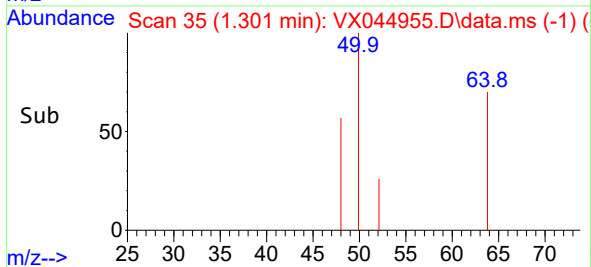

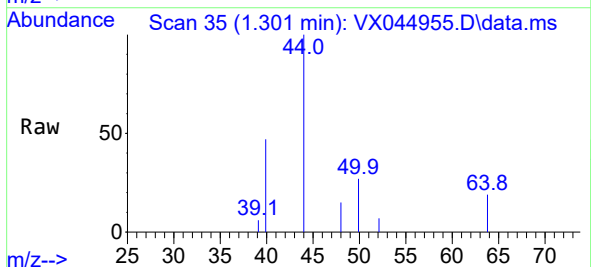


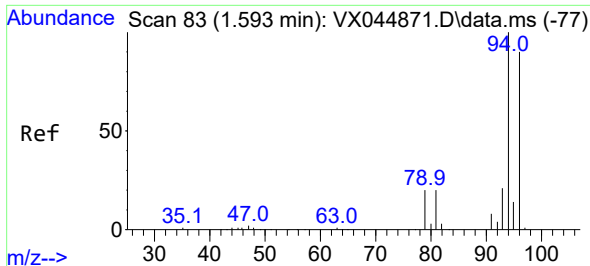

#5
Bromomethane
Concen: 0.61 ug/l
RT: 1.593 min Scan# 81
Delta R.T. 0.000 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT1-2025


Tgt Ion: 94 Resp: 282
Ion Ratio Lower Upper
94 100
96 97.7 71.6 107.4

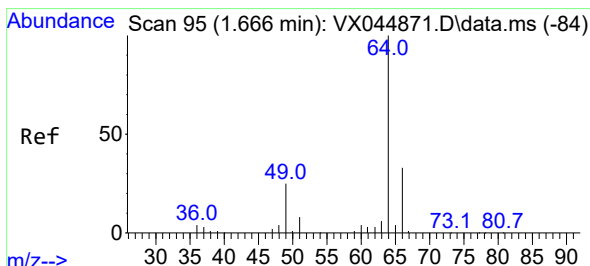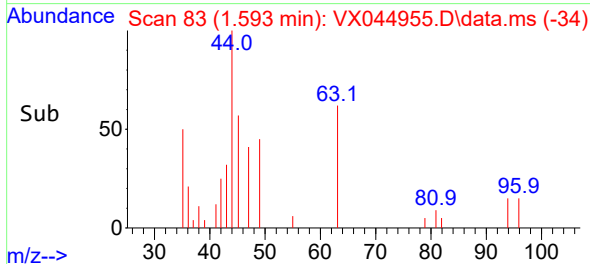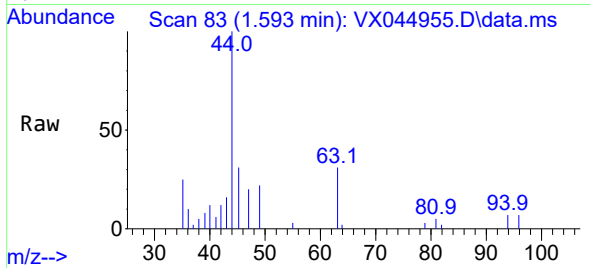

#6
Chloroethane
Concen: 1.80 ug/l
RT: 1.672 min Scan# 96
Delta R.T. 0.006 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48

Tgt Ion: 64 Resp: 343
Ion Ratio Lower Upper
64 100
66 34.5 25.9 38.9


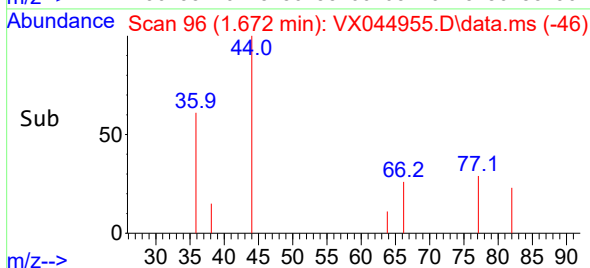
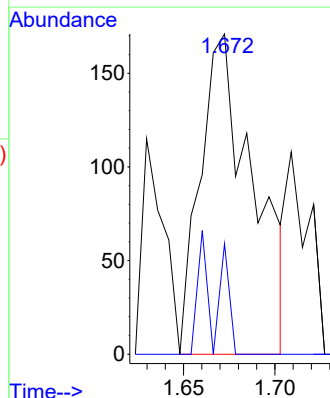
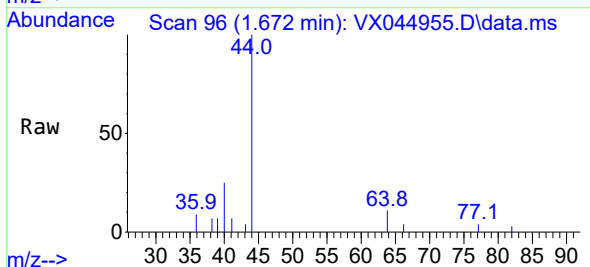




#7
Trichlorofluoromethane
Concen: 0.22 ug/l
RT: 1.880 min Scan# 11
Delta R.T. 0.007 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT1-2025


Tgt Ion:101 Resp: 437
Ion Ratio Lower Upper
101 100
103 72.6 52.4 78.6

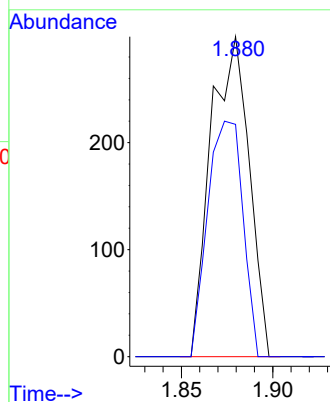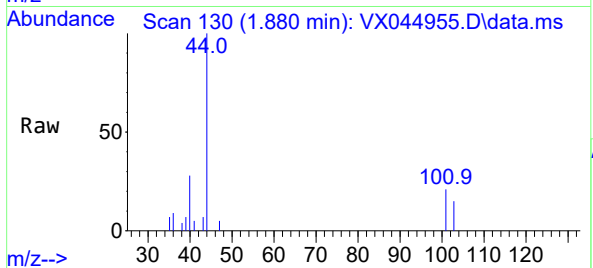

#11
Tert butyl alcohol
Concen: 6.48 ug/l
RT: 2.934 min Scan# 303
Delta R.T. -0.048 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48

Tgt Ion: 59 Resp: 1656
Ion Ratio Lower Upper
59 100
57 0.0 8.1 12.1#

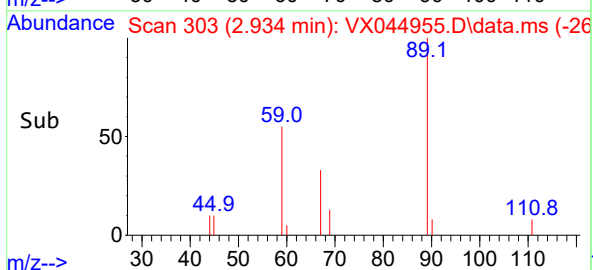



#13

Acrolein

Concen: 1.47 ug/l

RT: 2.227 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX044955.D

Acq: 14 Feb 2025 12:48

Instrument :

MSVOA_X

ClientSampleId :





MDL-WATER-03-QT1-2025

Tgt Ion: 56 Resp: 388

Ion Ratio Lower Upper

56 100

55 73.5 55.7 83.5

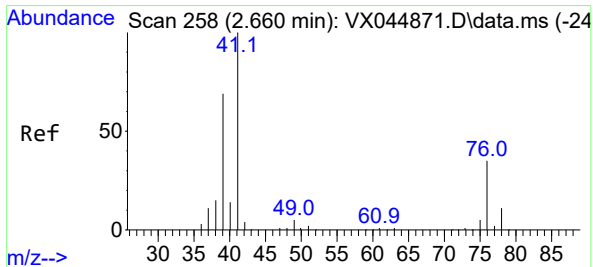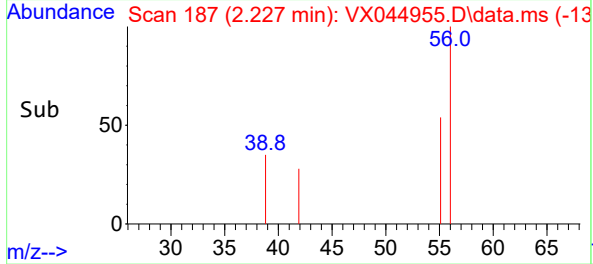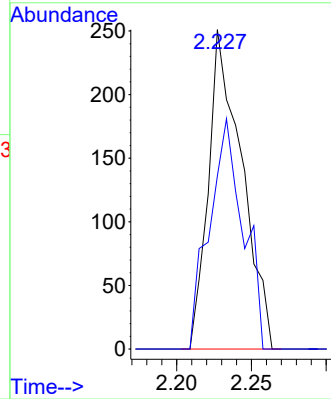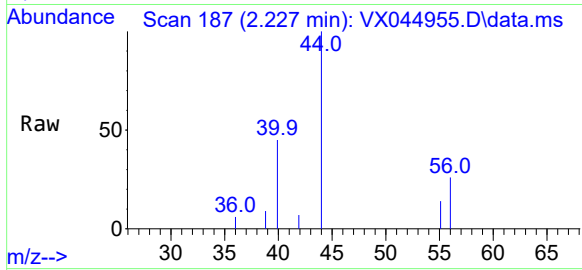

#14

Allyl chloride

Concen: 0.26 ug/l

RT: 2.660 min Scan# 258

Delta R.T. 0.000 min

Lab File: VX044955.D

Acq: 14 Feb 2025 12:48




Tgt Ion: 41 Resp: 572


Ion Ratio Lower Upper

41 100

39 54.9 51.4 77.2

76 22.4 27.0 40.4#


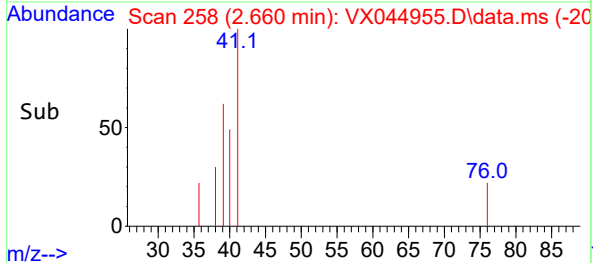
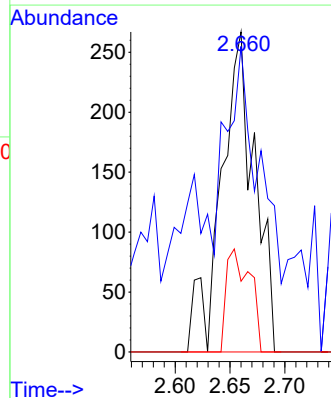
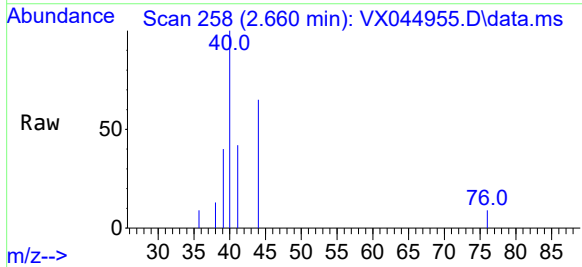




#15
Acrylonitrile
Concen: 1.05 ug/l
RT: 3.081 min Scan# 31
Delta R.T. 0.019 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT1-2025


Tgt Ion: 53	Resp:	717
Ion	Ratio	Lower Upper
53	100	
52	79.2	65.0 97.6
51	0.0	28.0 42.0#

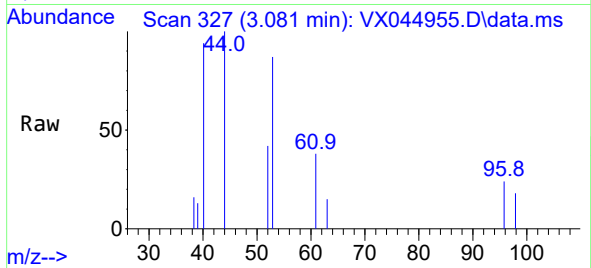

#16
Acetone
Concen: 1.38 ug/l
RT: 2.380 min Scan# 212
Delta R.T. 0.000 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48

Tgt Ion: 43	Resp:	767
Ion	Ratio	Lower Upper
43	100	
58	21.2	26.5 39.7#


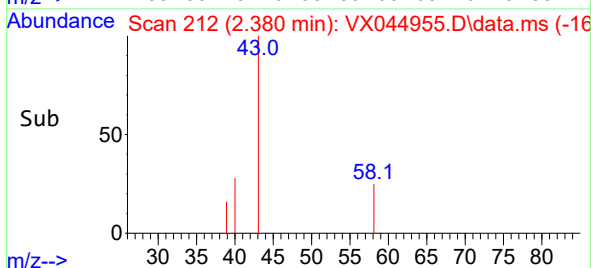
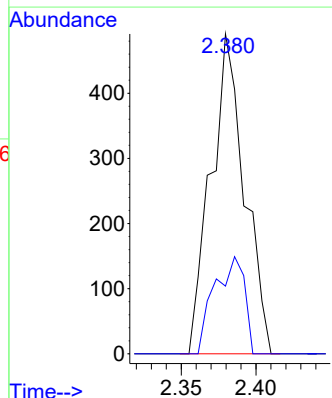



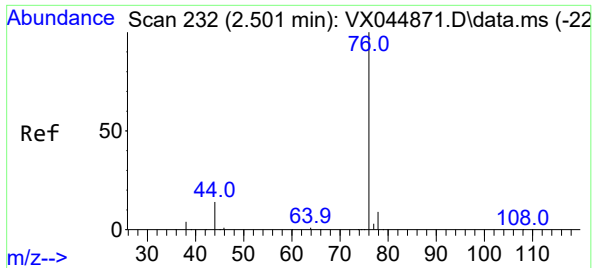

#17
Carbon Disulfide
Concen: 0.25 ug/l
RT: 2.508 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48




Instrument : MSVOA_X
ClientSampleId : MDL-WATER-03-QT1-2025


Tgt Ion: 76 Resp: 847
Ion Ratio Lower Upper
76 100
78 21.0 7.0 10.4#

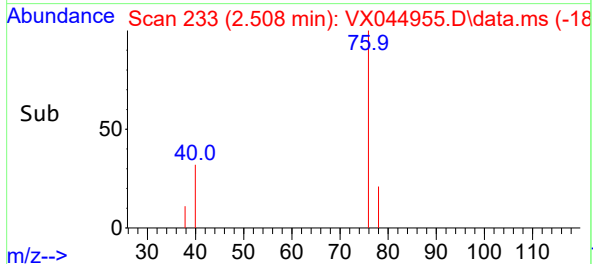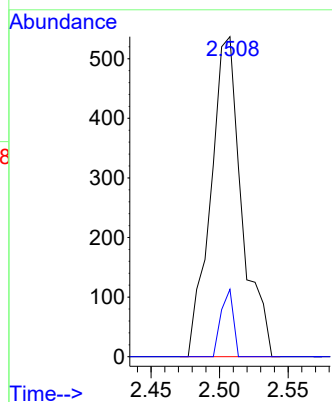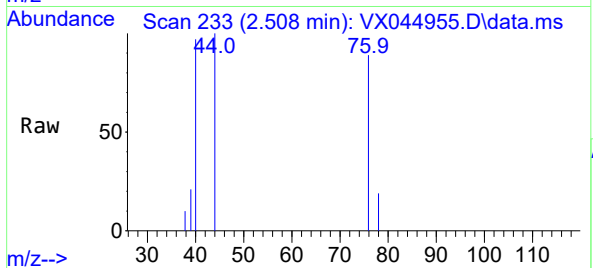

#18
Methyl Acetate
Concen: 0.26 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.006 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48

Tgt Ion: 43 Resp: 457
Ion Ratio Lower Upper
43 100
74 0.0 18.9 28.3#


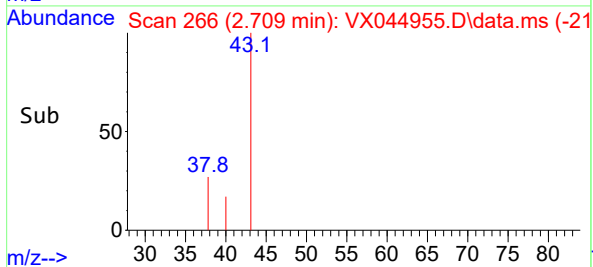
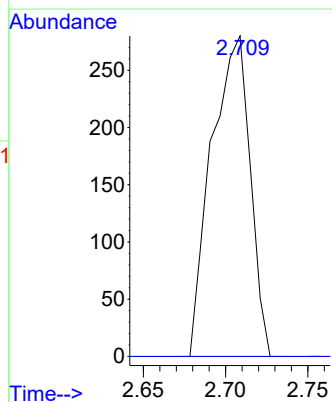
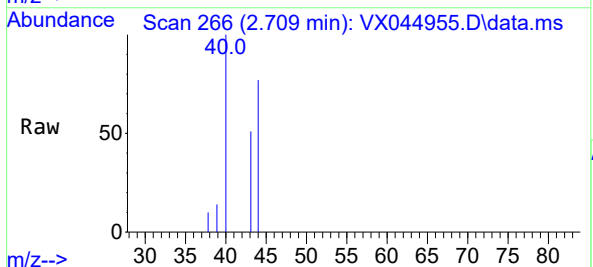




#19
Methyl tert-butyl Ether
Concen: 0.21 ug/l
RT: 3.117 min Scan# 311
Delta R.T. 0.006 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT1-2025


Tgt Ion: 73 Resp: 801
Ion Ratio Lower Upper
73 100
57 15.3 17.9 26.9#

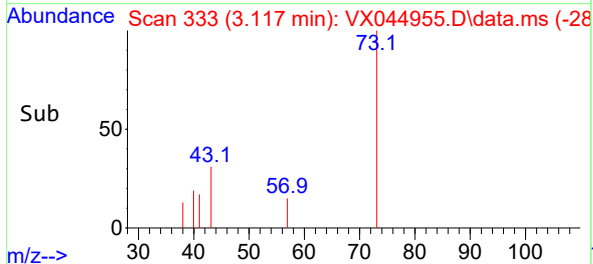

#20
Methylene Chloride
Concen: 0.27 ug/l
RT: 2.776 min Scan# 277
Delta R.T. -0.006 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48

Tgt Ion: 84 Resp: 364
Ion Ratio Lower Upper
84 100
49 75.6 100.1 150.1#
51 32.9 31.7 47.5
86 42.8 50.8 76.2#


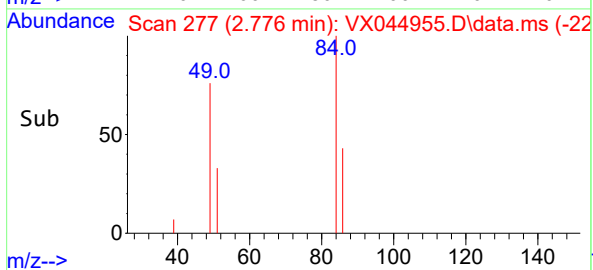

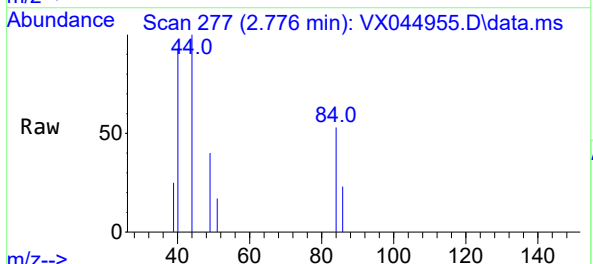




#23
Vinyl Acetate
Concen: 0.74 ug/l
RT: 3.751 min Scan# 41
Delta R.T. 0.037 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT1-2025


Tgt Ion: 43 Resp: 2504
Ion Ratio Lower Upper
43 100
86 0.0 8.3 12.5#

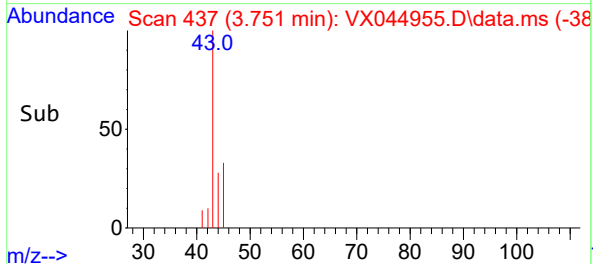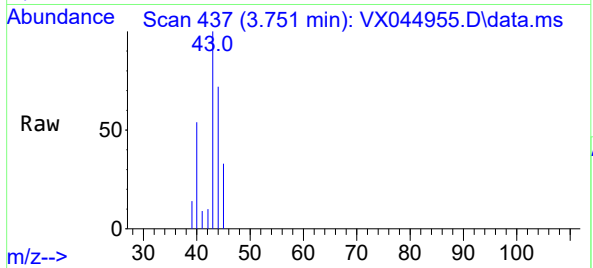

#29
Tetrahydrofuran
Concen: 0.70 ug/l
RT: 5.019 min Scan# 645
Delta R.T. 0.019 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48

Tgt Ion: 42 Resp: 421
Ion Ratio Lower Upper
42 100
72 4.8 35.0 52.4#
71 0.0 32.6 48.8#


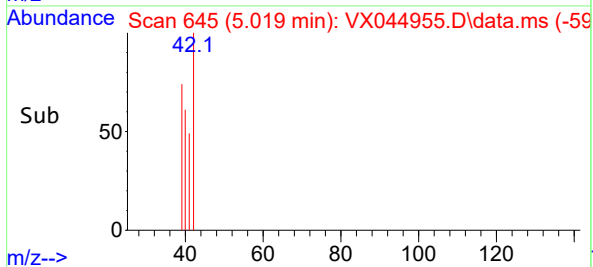

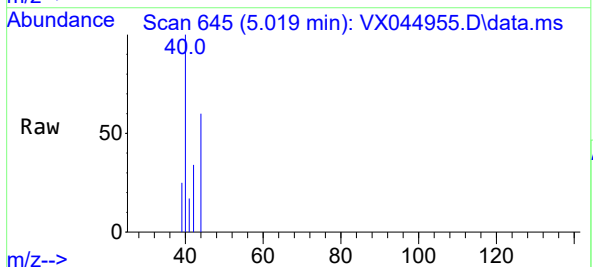




#31
Cyclohexane
Concen: 0.20 ug/l
RT: 5.470 min Scan# 718
Delta R.T. 0.006 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT1-2025


Tgt Ion: 56 Resp: 435
Ion Ratio Lower Upper
56 100
69 0.0 24.4 36.6#
84 84.8 69.0 103.6

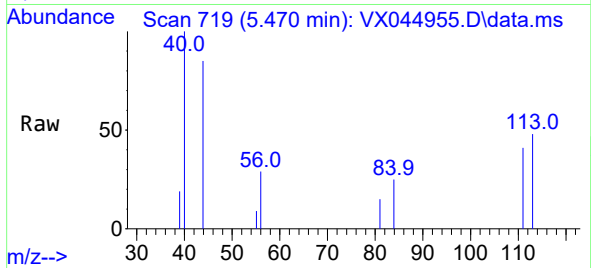

#33
1,2-Dichloroethane-d4
Concen: 61.79 ug/l
RT: 5.946 min Scan# 797
Delta R.T. 0.000 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48

Tgt Ion: 65 Resp: 85180
Ion Ratio Lower Upper
65 100
67 52.9 0.0 108.2


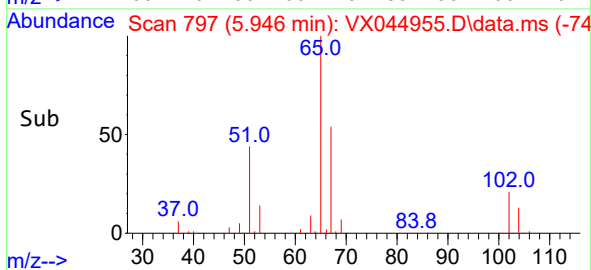






#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.757 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT1-2025


Tgt Ion:	114	Resp:	177149
Ion	Ratio	Lower	Upper
114	100		
63	22.1	0.0	42.4
88	16.0	0.0	31.4

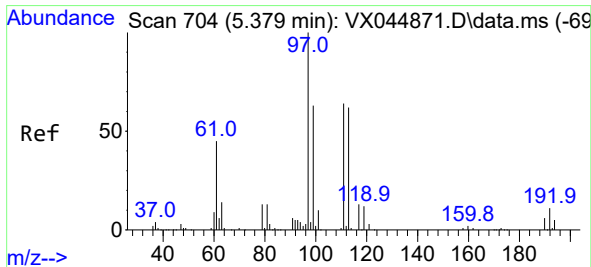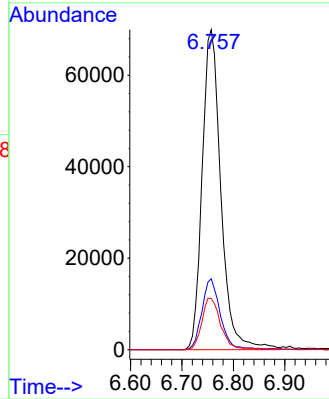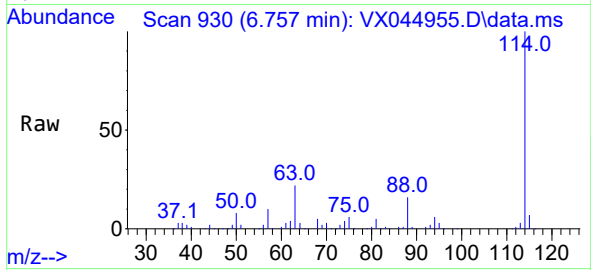

#35
Dibromofluoromethane
Concen: 56.44 ug/l
RT: 5.379 min Scan# 704
Delta R.T. 0.000 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48


Tgt Ion:	113	Resp:	65011
Ion	Ratio	Lower	Upper
113	100		
111	105.3	83.5	125.3
192	18.1	14.4	21.6

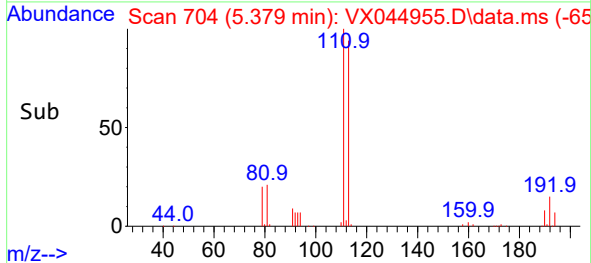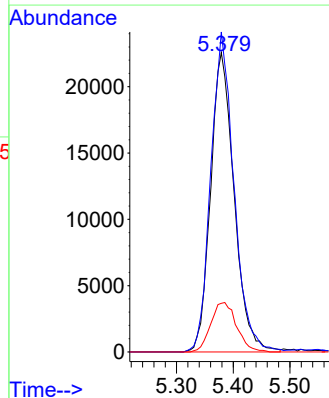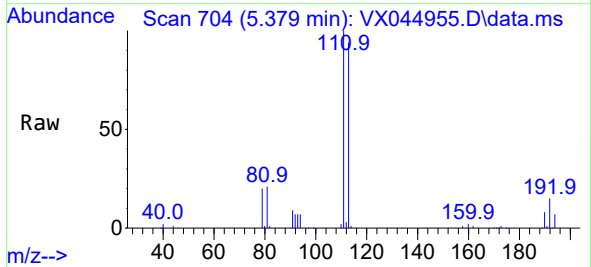



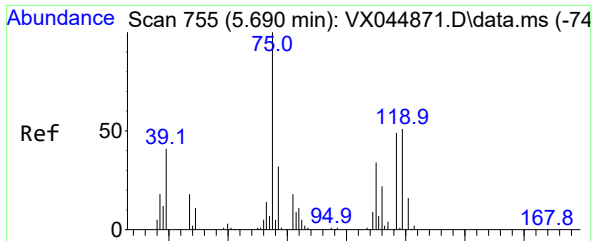


#36
1,1-Dichloropropene
Concen: 4.99 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.146 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48

Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT1-2025



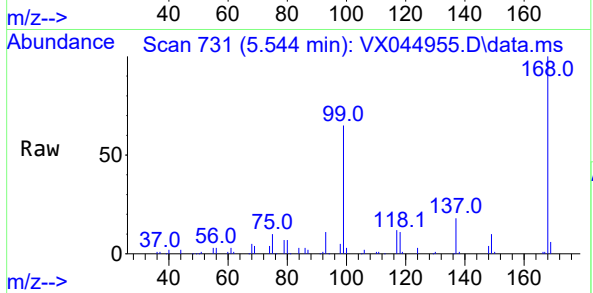



Tgt Ion: 75 Resp: 8298
Ion Ratio Lower Upper
75 100
110 7.8 17.2 51.6#
77 0.0 24.6 37.0#

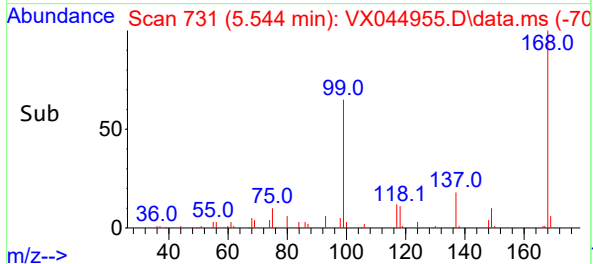

#42
1,2-Dichloroethane
Concen: 0.25 ug/l
RT: 6.105 min Scan# 823
Delta R.T. 0.025 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48

Tgt Ion: 62 Resp: 416
Ion Ratio Lower Upper
62 100
98 0.0 0.0 19.4


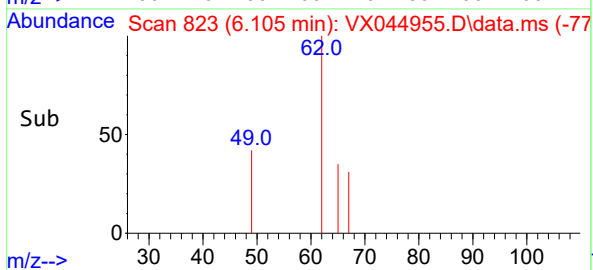

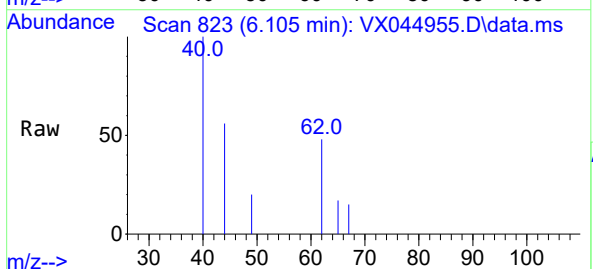




#50
Toluene-d8
Concen: 55.39 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT1-2025


Tgt Ion: 98 Resp: 241226
Ion Ratio Lower Upper
98 100
100 65.4 52.7 79.1

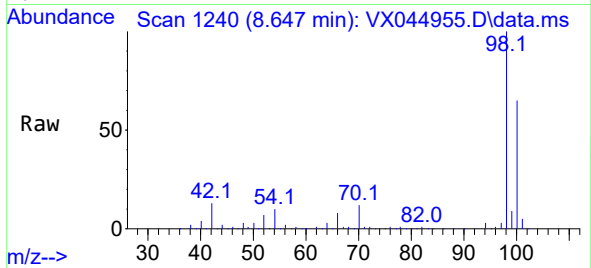

#51
4-Methyl-2-Pentanone
Concen: 0.76 ug/l
RT: 8.580 min Scan# 1229
Delta R.T. 0.006 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48

Tgt Ion: 43 Resp: 1370
Ion Ratio Lower Upper
43 100
58 30.4 30.8 46.2#


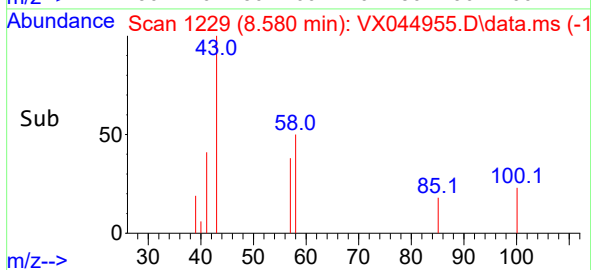

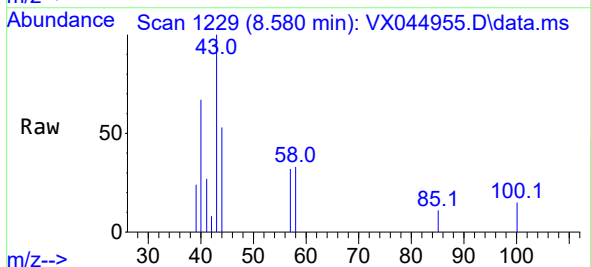




#52
Toluene
Concen: 0.21 ug/l
RT: 8.720 min Scan# 1176
Delta R.T. 0.006 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT1-2025


Tgt Ion: 92 Resp: 640
Ion Ratio Lower Upper
92 100
91 171.6 137.4 206.2

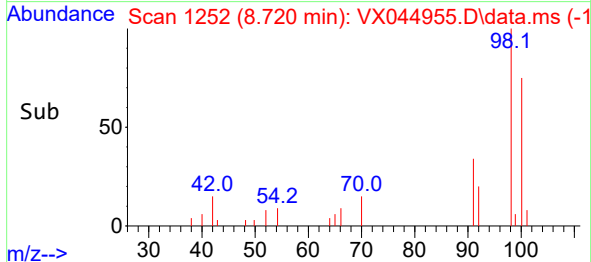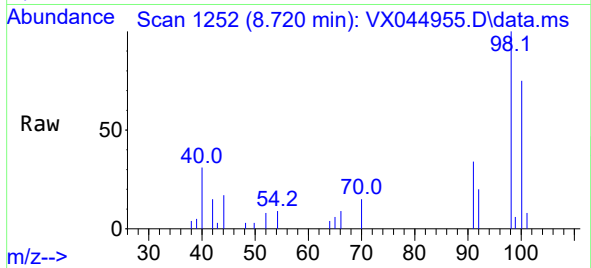

#58
2-Chloroethyl Vinyl ether
Concen: 1.90 ug/l
RT: 8.257 min Scan# 1176
Delta R.T. 0.019 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48

Tgt Ion: 63 Resp: 1787
Ion Ratio Lower Upper
63 100
106 26.2 21.3 31.9


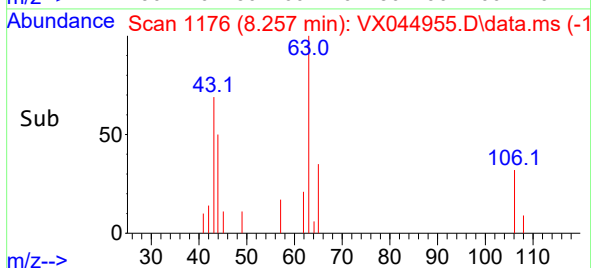
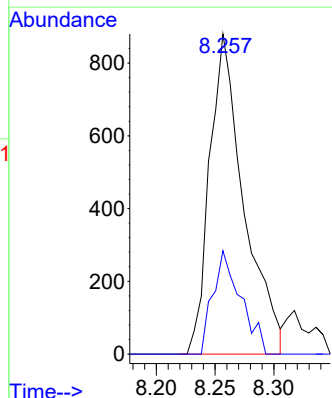





#59
2-Hexanone
Concen: 0.73 ug/l
RT: 9.470 min Scan# 11
Delta R.T. 0.043 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT1-2025


Tgt Ion: 43 Resp: 952
Ion Ratio Lower Upper
43 100
58 28.4 27.5 82.4

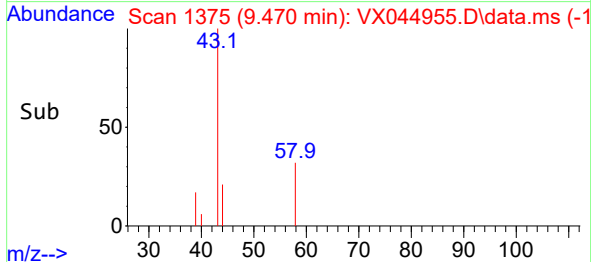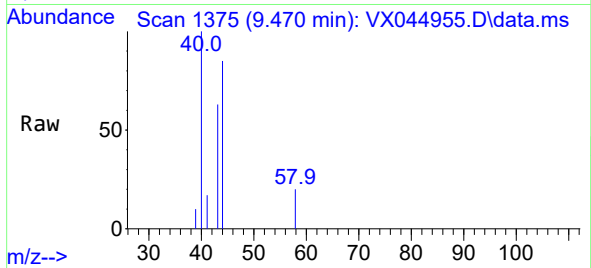

#62
4-Bromofluorobenzene
Concen: 55.00 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48

Tgt Ion: 95 Resp: 80747
Ion Ratio Lower Upper
95 100
174 71.8 0.0 142.6
176 70.3 0.0 141.6


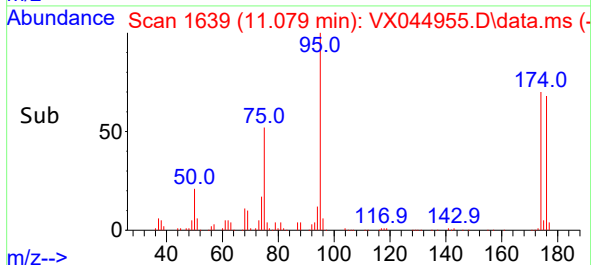
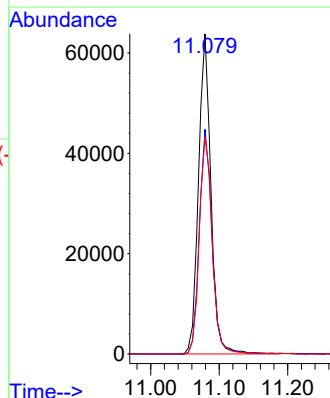
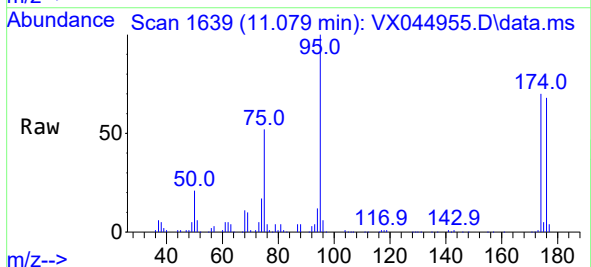




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT1-2025


Tgt Ion:117 Resp: 154748
Ion Ratio Lower Upper
117 100
82 59.5 47.5 71.3
119 32.0 25.4 38.0

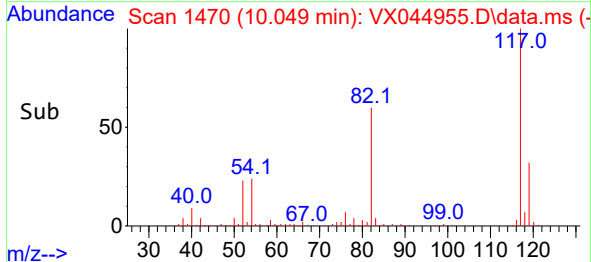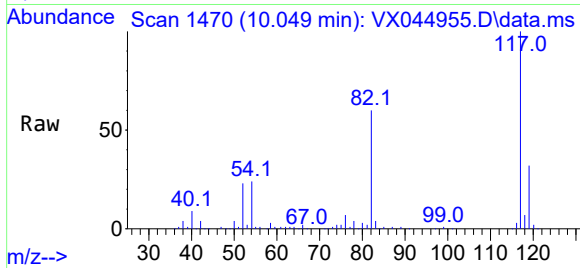

#64
Tetrachloroethene
Concen: 0.20 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. 0.006 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48

Tgt Ion:164 Resp: 200
Ion Ratio Lower Upper
164 100
166 86.4 100.4 150.6#
129 102.3 79.9 119.9
131 75.6 75.9 113.9#


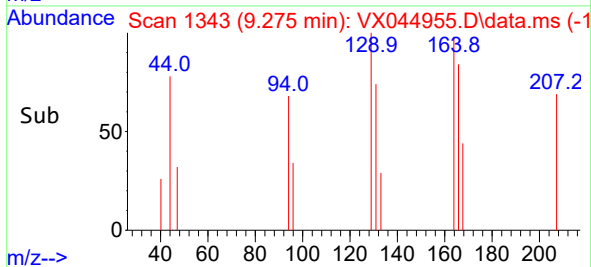

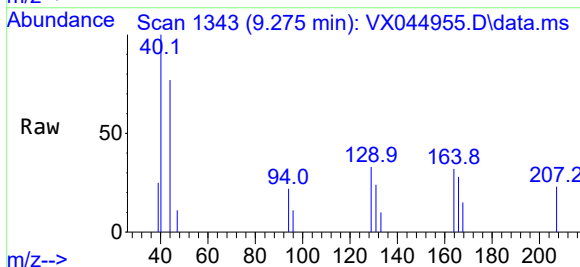




#65
Chlorobenzene
Concen: 0.21 ug/l
RT: 10.079 min Scan# 1475
Delta R.T. 0.000 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT1-2025


Tgt Ion:112 Resp: 705
Ion Ratio Lower Upper
112 100
114 19.5 25.0 37.6#

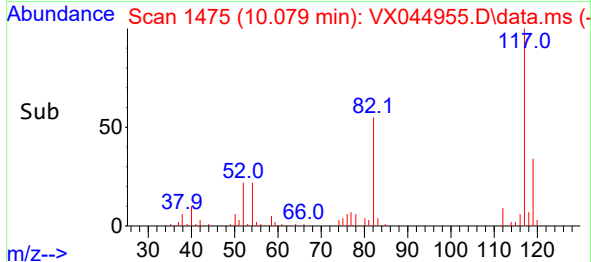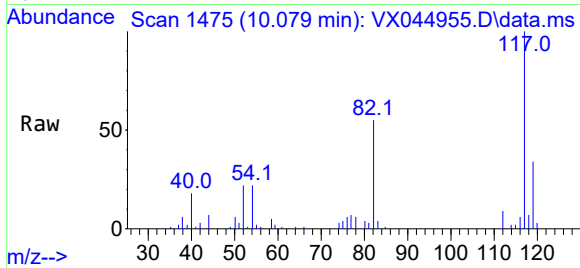

#68
m/p-Xylenes
Concen: 0.31 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48

Tgt Ion:106 Resp: 671
Ion Ratio Lower Upper
106 100
91 231.3 164.3 246.5


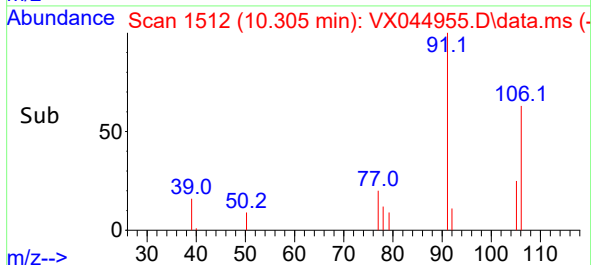
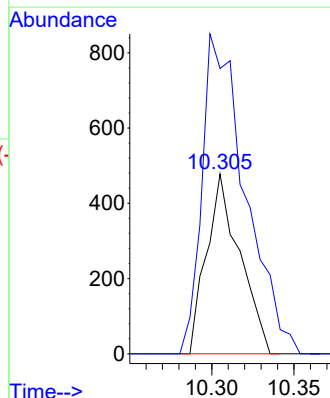
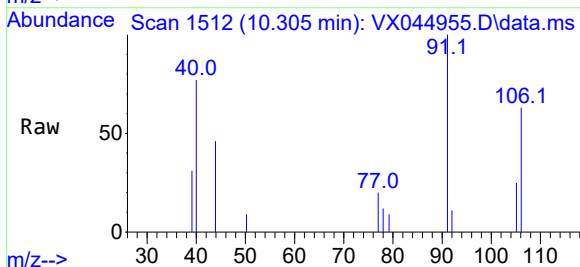




#71
Bromoform
Concen: 0.23 ug/l
RT: 10.805 min Scan# 1594
Delta R.T. 0.006 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT1-2025


Tgt Ion:173 Resp: 186
Ion Ratio Lower Upper
173 100
175 52.7 24.3 72.8
254 0.0 0.0 0.0

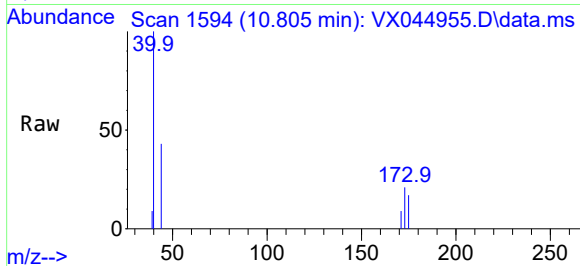

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48

Tgt Ion:152 Resp: 66049
Ion Ratio Lower Upper
152 100
115 61.9 43.4 130.1
150 156.9 0.0 350.4


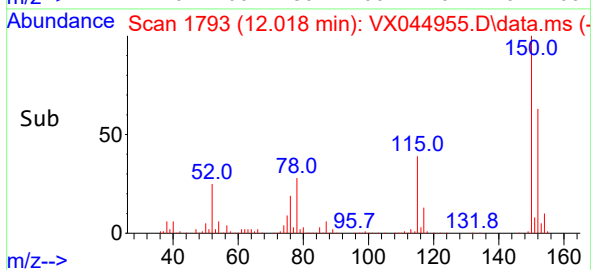

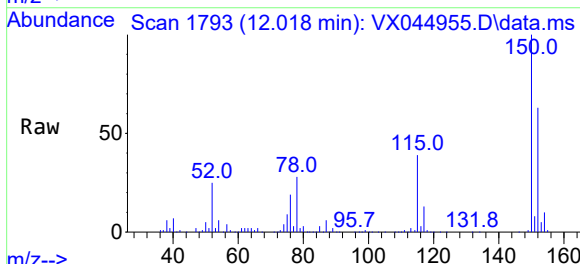




#76
1,2,3-Trichloropropane
Concen: 29.26 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT1-2025


Tgt Ion: 75 Resp: 42852
Ion Ratio Lower Upper
75 100
77 1.0 21.9 65.7#

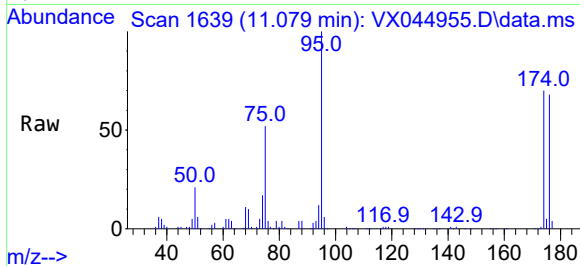

#77
Bromobenzene
Concen: 0.21 ug/l
RT: 11.201 min Scan# 1659
Delta R.T. 0.006 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48

Tgt Ion:156 Resp: 256
Ion Ratio Lower Upper
156 100
77 185.9 88.4 265.3
158 96.9 48.4 145.2


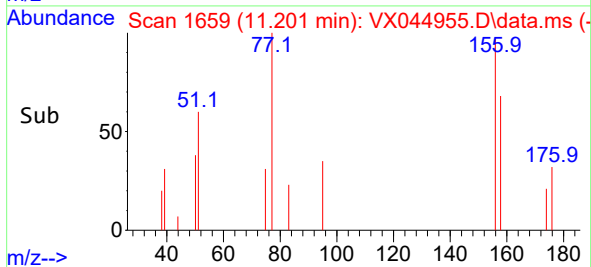

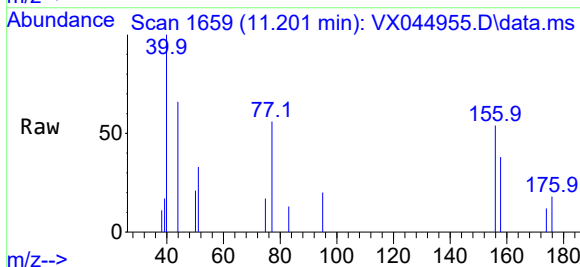




#79
2-Chlorotoluene
Concen: 0.25 ug/l
RT: 11.372 min Scan# 1687
Delta R.T. 0.012 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-03-QT1-2025


Tgt Ion: 91 Resp: 941
Ion Ratio Lower Upper
91 100
126 18.5 16.2 48.6

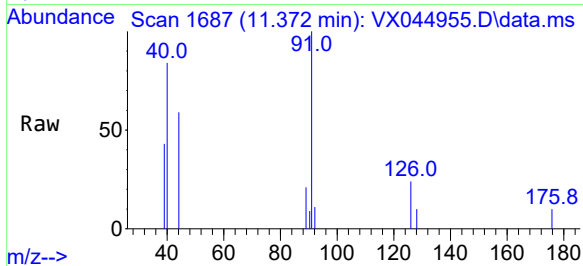

#81
trans-1,4-Dichloro-2-butene
Concen: 75.27 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX044955.D
Acq: 14 Feb 2025 12:48


Tgt Ion: 75 Resp: 42852
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.0 36.6 54.8#

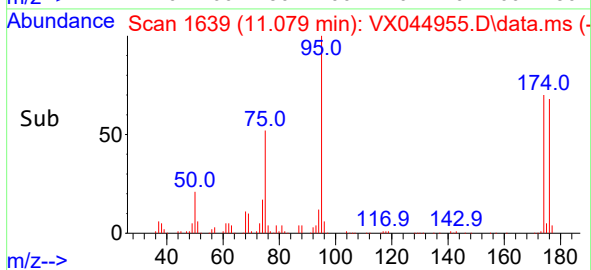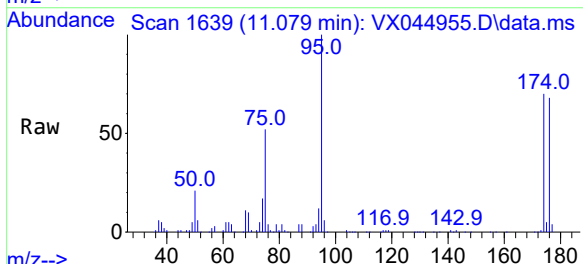

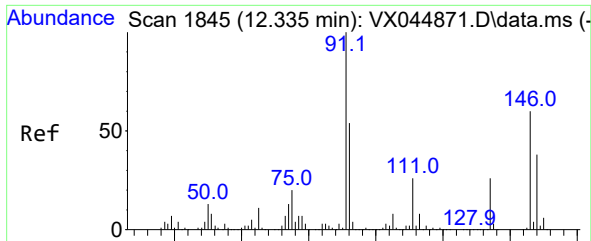

#91
 1,2-Dichlorobenzene
 Concen: 0.21 ug/l
 RT: 12.341 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: VX044955.D
 Acq: 14 Feb 2025 12:48

Instrument :
 MSVOA_X
 ClientSampleId :
 MDL-WATER-03-QT1-2025

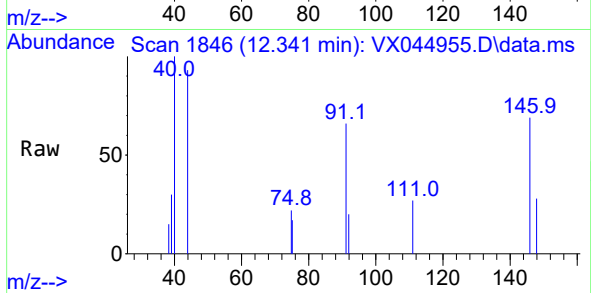

Tgt Ion:146 Resp: 448

Ion	Ratio	Lower	Upper
146	100		
111	36.8	21.8	65.4
148	51.1	31.9	95.9

