

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021225\
 Data File : VX044941.D
 Acq On : 12 Feb 2025 18:16
 Operator : JC/MD
 Sample : Q1356-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CARBON-WATER

Quant Time: Feb 13 00:53:34 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021025W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 11 03:41:08 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	84607	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	171255	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	157249	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	64055	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	67934	54.852	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	109.700%
35) Dibromofluoromethane	5.385	113	57263	51.429	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	102.860%
50) Toluene-d8	8.647	98	215155	51.101	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	102.200%
62) 4-Bromofluorobenzene	11.079	95	72785	51.278	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	102.560%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021225\
Data File : VX044941.D
Acq On : 12 Feb 2025 18:16
Operator : JC/MD
Sample : Q1356-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CARBON-WATER

Quant Time: Feb 13 00:53:34 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021025W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 11 03:41:08 2025
Response via : Initial Calibration




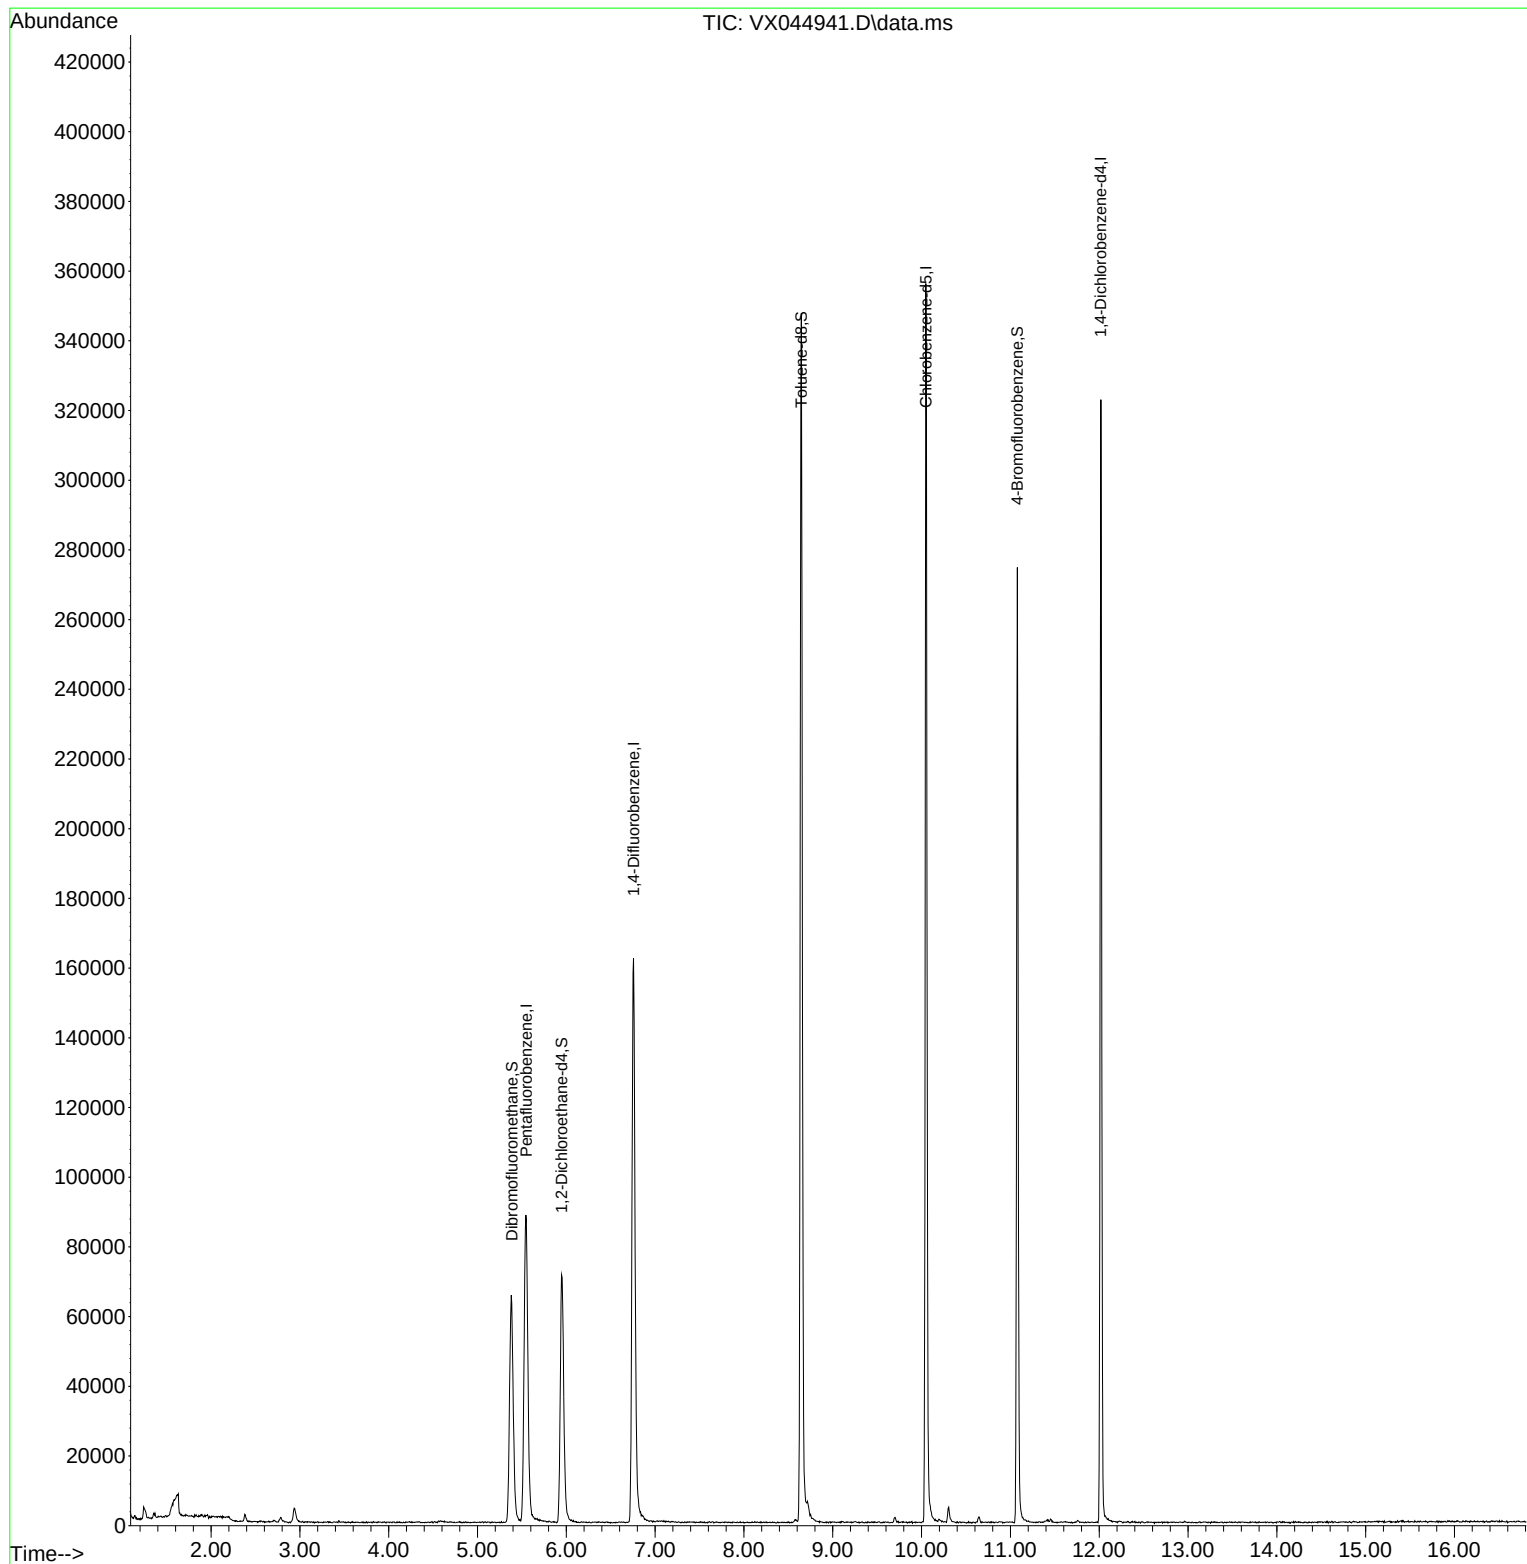


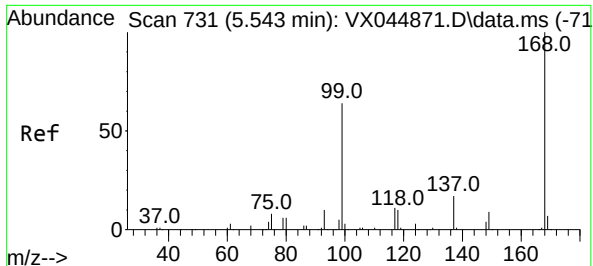

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.007 min
Lab File: VX044941.D
Acq: 12 Feb 2025 18:16




Instrument :
MSVOA_X
ClientSampleId :
CARBON-WATER


Tgt Ion:168 Resp: 84607
Ion Ratio Lower Upper
168 100
99 59.0 51.2 76.8

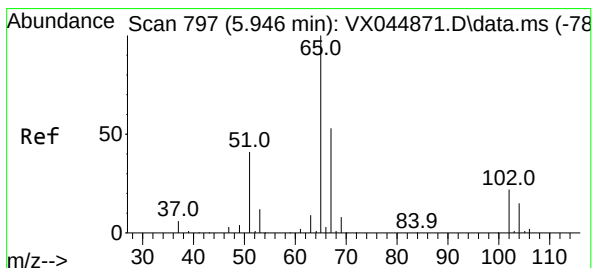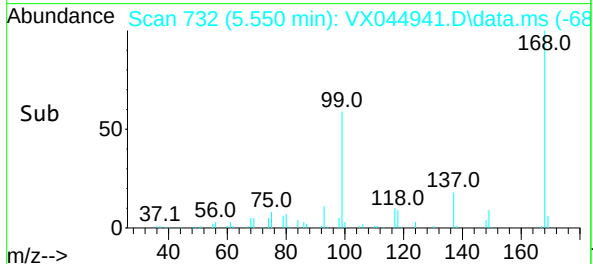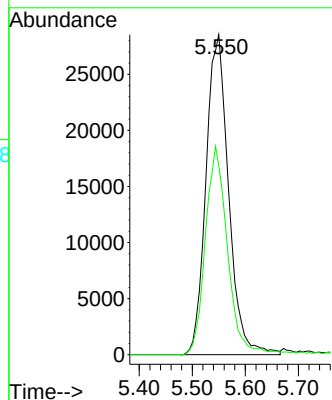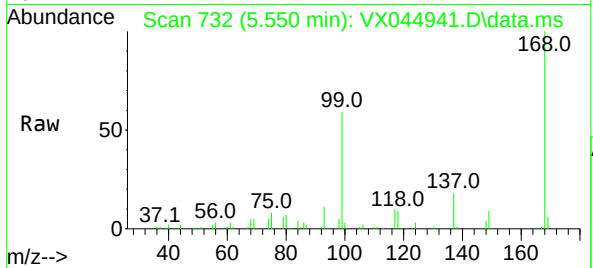

#33
1,2-Dichloroethane-d4
Concen: 54.852 ug/l
RT: 5.946 min Scan# 797
Delta R.T. 0.000 min
Lab File: VX044941.D
Acq: 12 Feb 2025 18:16

Tgt Ion: 65 Resp: 67934
Ion Ratio Lower Upper
65 100
67 53.3 0.0 108.2


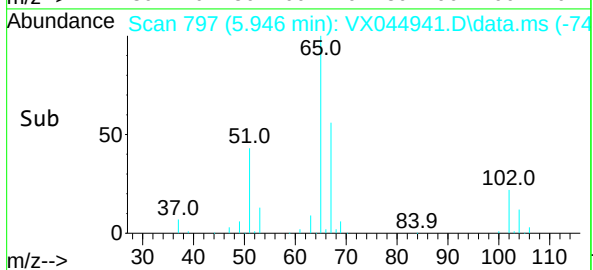
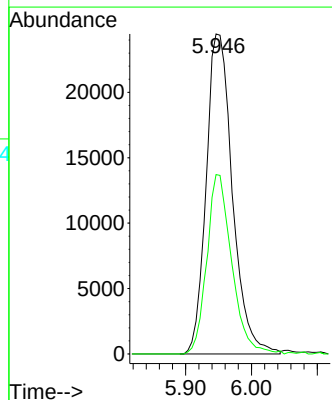
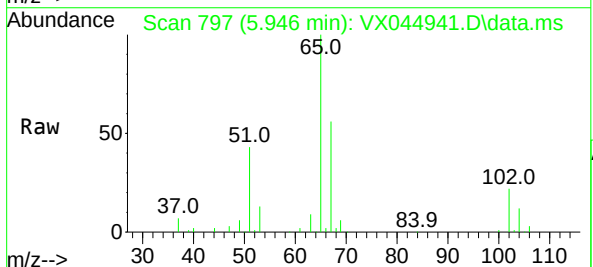


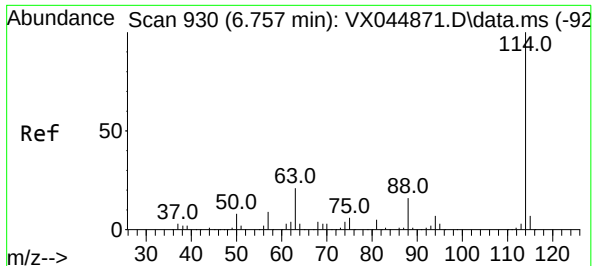

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX044941.D
Acq: 12 Feb 2025 18:16




Instrument :
MSVOA_X
ClientSampleId :
CARBON-WATER


Tgt Ion:114 Resp: 171255
Ion Ratio Lower Upper
114 100
63 20.5 0.0 42.4
88 15.4 0.0 31.4

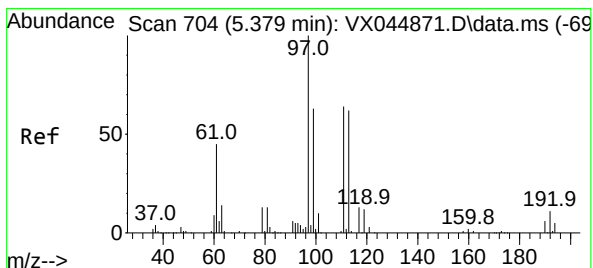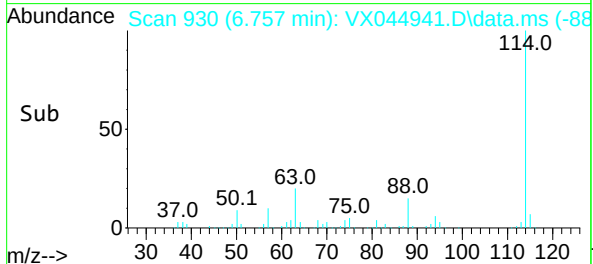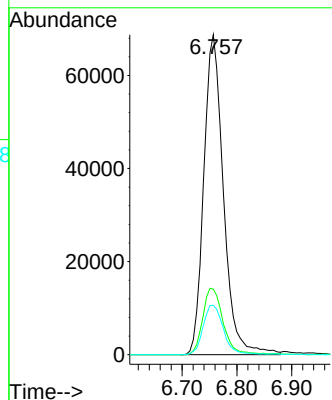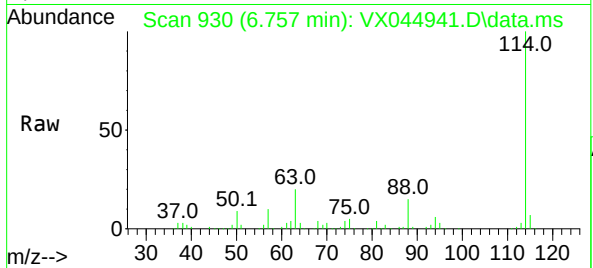

#35
Dibromofluoromethane
Concen: 51.429 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX044941.D
Acq: 12 Feb 2025 18:16

Tgt Ion:113 Resp: 57263
Ion Ratio Lower Upper
113 100
111 102.9 83.5 125.3
192 16.8 14.4 21.6


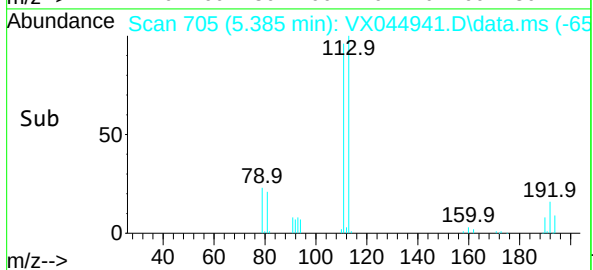
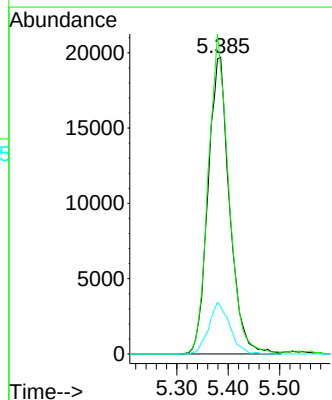
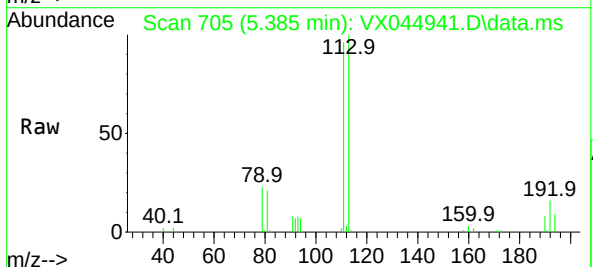


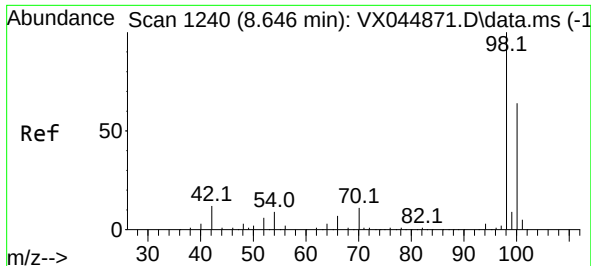

#50
Toluene-d8
Concen: 51.101 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX044941.D
Acq: 12 Feb 2025 18:16




Instrument :
MSVOA_X
ClientSampleId :
CARBON-WATER


Tgt Ion: 98 Resp: 215155
Ion Ratio Lower Upper
98 100
100 65.3 52.7 79.1

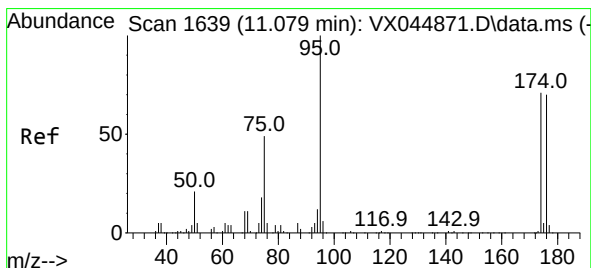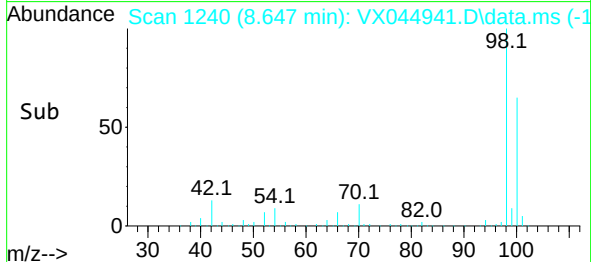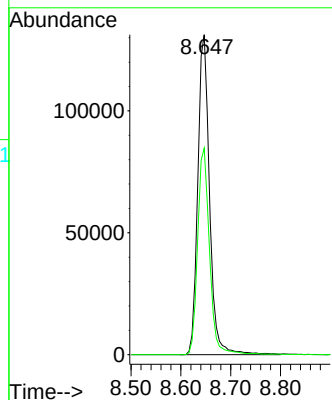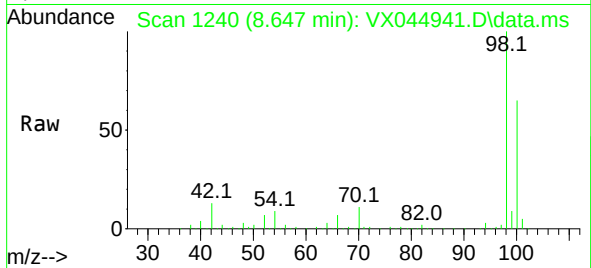

#62
4-Bromofluorobenzene
Concen: 51.278 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX044941.D
Acq: 12 Feb 2025 18:16

Tgt Ion: 95 Resp: 72785
Ion Ratio Lower Upper
95 100
174 72.2 0.0 142.6
176 69.9 0.0 141.6


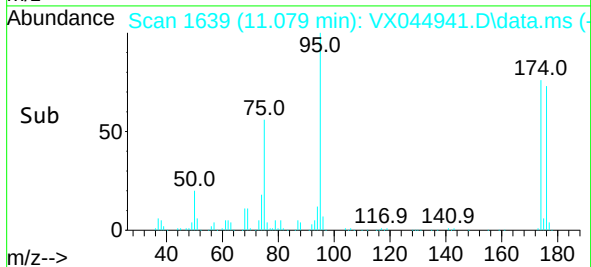
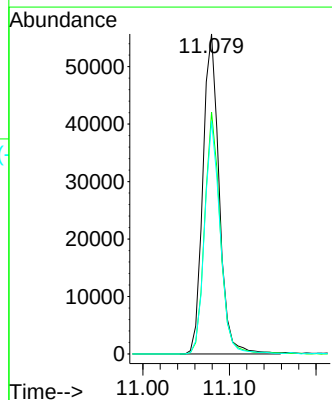
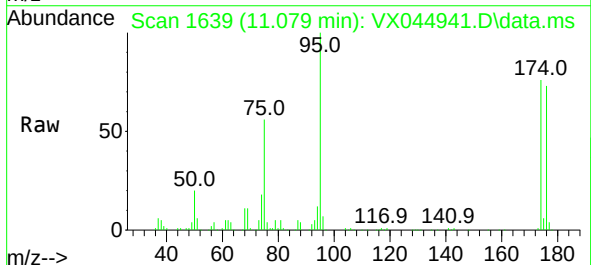


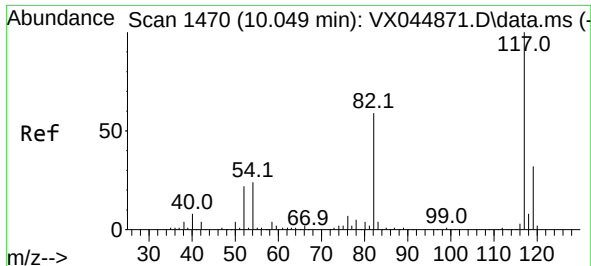

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX044941.D
Acq: 12 Feb 2025 18:16

Instrument :
MSVOA_X
ClientSampleId :
CARBON-WATER

Tgt Ion:117 Resp: 157249
Ion Ratio Lower Upper
117 100
82 57.8 47.5 71.3
119 32.1 25.4 38.0

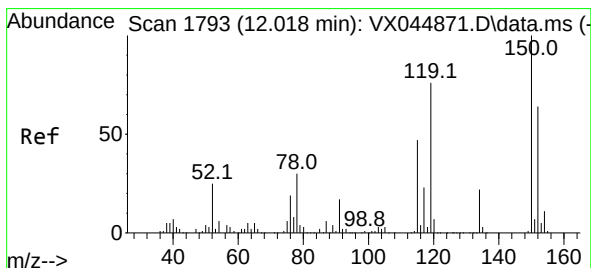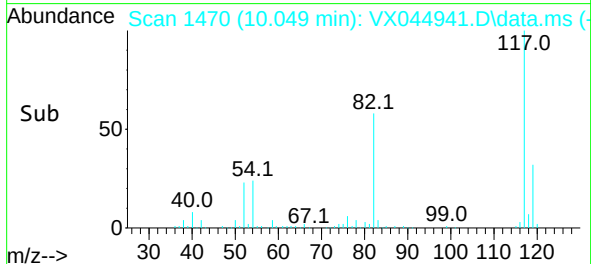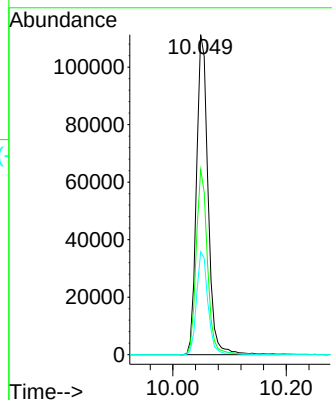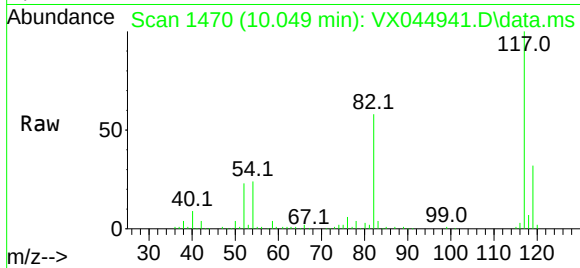

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX044941.D
Acq: 12 Feb 2025 18:16

Tgt Ion:152 Resp: 64055
Ion Ratio Lower Upper
152 100
115 62.0 43.4 130.1
150 158.8 0.0 350.4

