


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX021319\
Data File : VX007498.D
Acq On : 12 Feb 2019 22:09
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Title : SW846 8260
Last Update : Sat Feb 02 01:32:36 2019

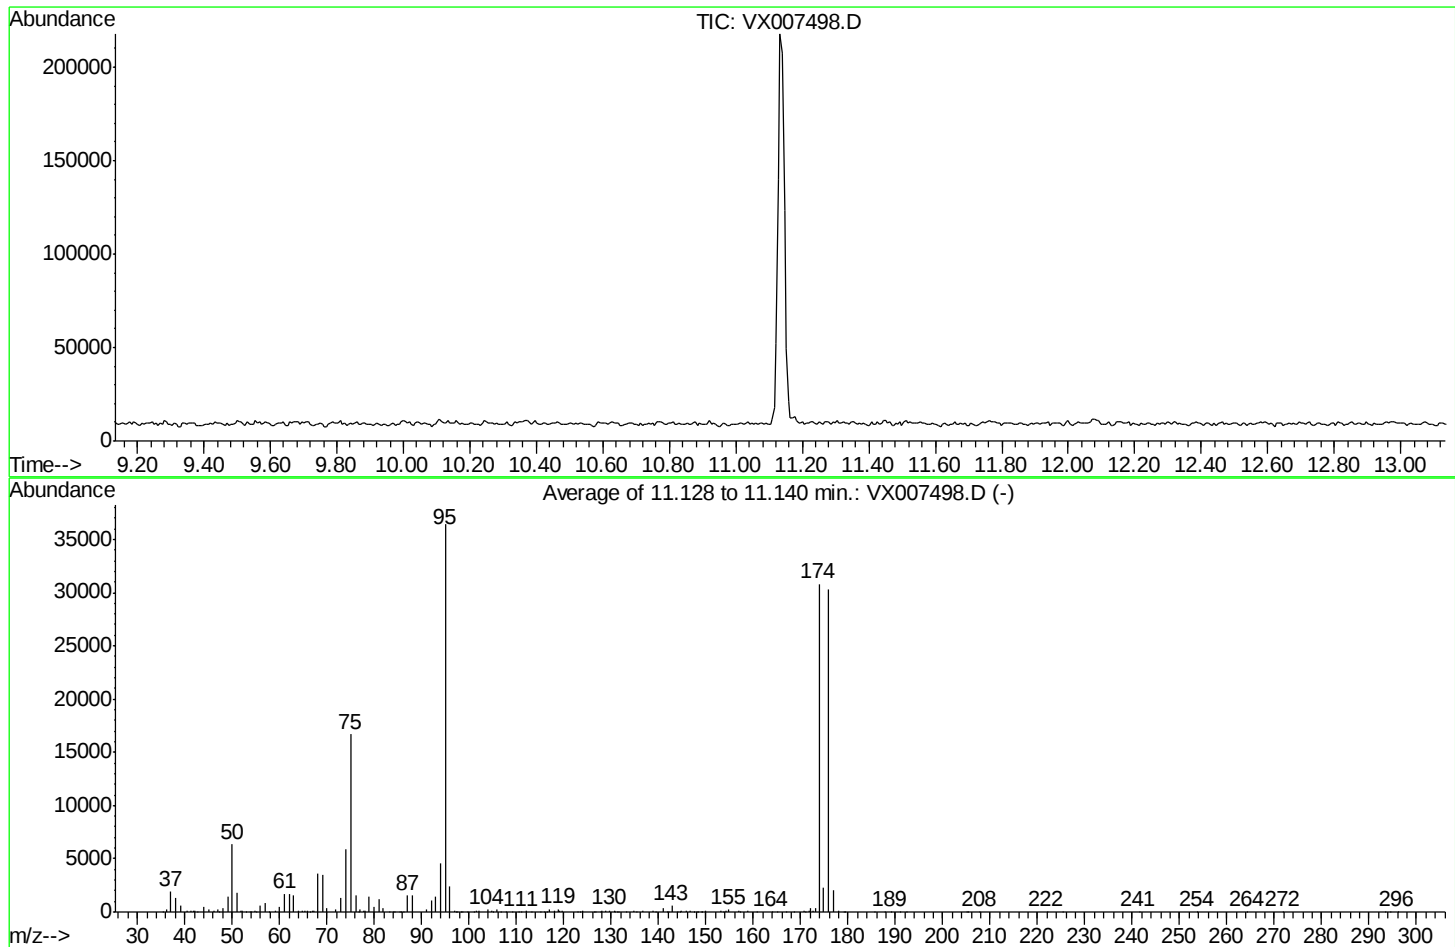

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	6372	PASS
75	95	30	60	45.9	16697	PASS
95	95	100	100	100.0	36413	PASS
96	95	5	9	6.8	2466	PASS
173	174	0.00	2	1.4	416	PASS
174	95	50	100	84.6	30797	PASS
175	174	5	9	7.4	2292	PASS
176	174	95	101	98.4	30296	PASS
177	176	5	9	6.9	2087	PASS