

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021323\
 Data File : VX034143.D
 Acq On : 13 Feb 2023 14:43
 Operator : JC/MD
 Sample : VX0213WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK616

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML021323WMA.M
 Title : VOC Analysis

Signal : TIC: VX034143.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	60	rVB	35840	42238	8.82%	1.143%
2	1.648	88	92	104	rVB	24289	36233	7.56%	0.981%
3	1.807	114	118	122	rVB	97	129	0.03%	0.003%
4	1.874	127	129	137	rVB3	494	746	0.16%	0.020%
5	2.300	193	199	210	rBV	105414	158216	33.03%	4.283%
6	2.373	210	211	214	rVB	171	149	0.03%	0.004%
7	2.508	228	233	237	rBB	803	1195	0.25%	0.032%
8	2.703	260	265	268	rBB	177	257	0.05%	0.007%
9	2.788	274	279	284	rBB2	656	1049	0.22%	0.028%
10	2.934	297	303	311	rBB2	1108	2698	0.56%	0.073%
11	3.093	324	329	330	rBV	512	610	0.13%	0.017%
12	3.599	409	412	414	rBV	146	181	0.04%	0.005%
13	4.446	542	551	564	rBV	26930	72139	15.06%	1.953%
14	5.050	638	650	664	rBV	58134	166215	34.70%	4.499%
15	5.373	699	703	705	rBV	486	529	0.11%	0.014%
16	5.470	713	719	721	rBB2	208	302	0.06%	0.008%
17	5.556	725	733	740	rBB2	727	2033	0.42%	0.055%
18	5.666	748	751	755	rBB	210	322	0.07%	0.009%
19	5.964	788	800	817	rBV2	163324	479008	100.00%	12.966%
20	6.092	819	821	826	rVV2	369	652	0.14%	0.018%
21	6.135	826	828	831	rVB	189	164	0.03%	0.004%
22	6.208	837	840	843	rBB	141	187	0.04%	0.005%
23	6.665	911	915	918	rBV	137	184	0.04%	0.005%
24	6.751	920	929	945	rBV	124475	299921	62.61%	8.119%
25	6.921	954	957	958	rBV	126	130	0.03%	0.004%
26	7.049	975	978	982	rBB	127	129	0.03%	0.003%
27	7.117	983	989	997	rBB5	1333	2839	0.59%	0.077%
28	7.306	1011	1020	1037	rBB	104850	232397	48.52%	6.291%
29	7.415	1037	1038	1040	rBV	181	166	0.03%	0.004%
30	7.476	1044	1048	1051	rBV	297	354	0.07%	0.010%
31	7.812	1100	1103	1110	rVB3	281	513	0.11%	0.014%
32	7.897	1115	1117	1120	rVB	192	155	0.03%	0.004%
33	7.940	1121	1124	1128	rBV	241	306	0.06%	0.008%
34	8.257	1172	1176	1178	rBV	153	189	0.04%	0.005%
35	8.318	1181	1186	1201	rBV	69935	118853	24.81%	3.217%
36	8.470	1208	1211	1214	rBB	133	144	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021323\
 Data File : VX034143.D
 Acq On : 13 Feb 2023 14:43
 Operator : JC/MD
 Sample : VX0213WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK616

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML021323WMA.M
 Title : VOC Analysis

37	8.580	1223	1229	1233	rBV2	567	850	0.18%	0.023%
38	8.647	1233	1240	1250	rBV	275961	439613	91.78%	11.900%
39	8.945	1283	1289	1303	rVB	51102	76267	15.92%	2.064%
40	9.153	1321	1323	1328	rVB2	572	609	0.13%	0.016%
41	9.275	1339	1343	1348	rBB	1018	1481	0.31%	0.040%
42	9.384	1355	1361	1378	rBV	134894	205396	42.88%	5.560%
43	9.573	1389	1392	1394	rBV2	222	247	0.05%	0.007%
44	9.610	1394	1398	1401	rVV3	350	573	0.12%	0.016%
45	9.945	1451	1453	1456	rVB	133	136	0.03%	0.004%
46	10.000	1459	1462	1465	rBV	125	153	0.03%	0.004%
47	10.049	1465	1470	1481	rBV	233442	329565	68.80%	8.921%
48	10.195	1489	1494	1502	rBB	1088	1841	0.38%	0.050%
49	10.305	1507	1512	1516	rBB2	956	1390	0.29%	0.038%
50	10.555	1552	1553	1558	rVB	127	151	0.03%	0.004%
51	10.646	1564	1568	1575	rBB3	1579	2899	0.61%	0.078%
52	10.799	1590	1593	1597	rBB	364	353	0.07%	0.010%
53	10.963	1615	1620	1624	rBV	1233	1773	0.37%	0.048%
54	11.085	1637	1640	1642	rBV	147	186	0.04%	0.005%
55	11.104	1642	1643	1648	rVB2	135	155	0.03%	0.004%
56	11.189	1652	1657	1664	rBV	182081	239917	50.09%	6.494%
57	11.311	1674	1677	1681	rBB	908	1023	0.21%	0.028%
58	11.421	1694	1695	1697	rBV	161	131	0.03%	0.004%
59	11.451	1697	1700	1706	rVV	1258	1446	0.30%	0.039%
60	11.756	1744	1750	1755	rBB2	1247	1559	0.33%	0.042%
61	11.975	1782	1786	1789	rBV2	1300	1748	0.36%	0.047%
62	12.024	1789	1794	1804	rVB	264662	339979	70.98%	9.203%
63	12.317	1837	1842	1850	rBV	305168	403217	84.18%	10.915%
64	12.530	1874	1877	1879	rBV	178	148	0.03%	0.004%
65	12.634	1891	1894	1895	rBV	144	132	0.03%	0.004%
66	12.707	1900	1906	1908	rBB2	174	294	0.06%	0.008%
67	12.762	1908	1915	1919	rBB3	1382	1875	0.39%	0.051%
68	12.835	1924	1927	1929	rBV3	157	159	0.03%	0.004%
69	12.926	1939	1942	1944	rBV3	135	157	0.03%	0.004%
70	12.951	1944	1946	1948	rVB3	238	173	0.04%	0.005%
71	13.073	1963	1966	1969	rBB	124	136	0.03%	0.004%
72	13.115	1970	1973	1980	rBV2	2376	2431	0.51%	0.066%
73	13.237	1988	1993	1994	rBV	153	240	0.05%	0.006%
74	13.591	2048	2051	2056	rBV2	2078	2484	0.52%	0.067%
75	13.676	2061	2065	2067	rVB	139	168	0.04%	0.005%
76	13.780	2076	2082	2087	rBV	2313	2723	0.57%	0.074%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021323\
 Data File : VX034143.D
 Acq On : 13 Feb 2023 14:43
 Operator : JC/MD
 Sample : VX0213WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK616

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML021323WMA.M
 Title : VOC Analysis

77	13.914	2100	2104	2105	rBV	141	142	0.03%	0.004%
78	13.963	2108	2112	2118	rBV	1831	2422	0.51%	0.066%
79	14.127	2134	2139	2144	rVV2	827	1403	0.29%	0.038%
80	14.268	2160	2162	2163	rBV2	189	182	0.04%	0.005%
81	14.329	2170	2172	2175	rBV	178	227	0.05%	0.006%
82	14.408	2183	2185	2187	rVV2	119	154	0.03%	0.004%
83	14.451	2190	2192	2193	rVV	158	138	0.03%	0.004%
84	14.524	2200	2204	2206	rBV	199	201	0.04%	0.005%
85	14.640	2221	2223	2226	rVB	216	210	0.04%	0.006%
86	14.676	2226	2229	2232	rBV3	185	275	0.06%	0.007%
87	14.816	2248	2252	2254	rVB2	205	278	0.06%	0.008%
88	14.847	2254	2257	2258	rBV	167	197	0.04%	0.005%
89	14.865	2258	2260	2262	rVV	206	196	0.04%	0.005%
90	14.920	2265	2269	2270	rBV	131	165	0.03%	0.004%
91	14.944	2271	2273	2276	rVB2	233	210	0.04%	0.006%
92	15.079	2293	2295	2296	rBV2	215	183	0.04%	0.005%
93	15.097	2296	2298	2302	rVB	341	271	0.06%	0.007%
94	15.286	2327	2329	2330	rBV	206	153	0.03%	0.004%
95	15.396	2344	2347	2349	rBV	463	664	0.14%	0.018%
96	15.456	2356	2357	2360	rBV	280	233	0.05%	0.006%
97	15.774	2407	2409	2410	rBV	202	182	0.04%	0.005%
98	16.340	2500	2502	2506	rBV3	217	294	0.06%	0.008%
99	16.487	2522	2526	2528	rBV3	244	356	0.07%	0.010%
100	16.712	2561	2563	2564	rBV	312	181	0.04%	0.005%




Sum of corrected areas: 3694227

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021323\
Data File : VX034143.D
Acq On : 13 Feb 2023 14:43
Operator : JC/MD
Sample : VX0213WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML021323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

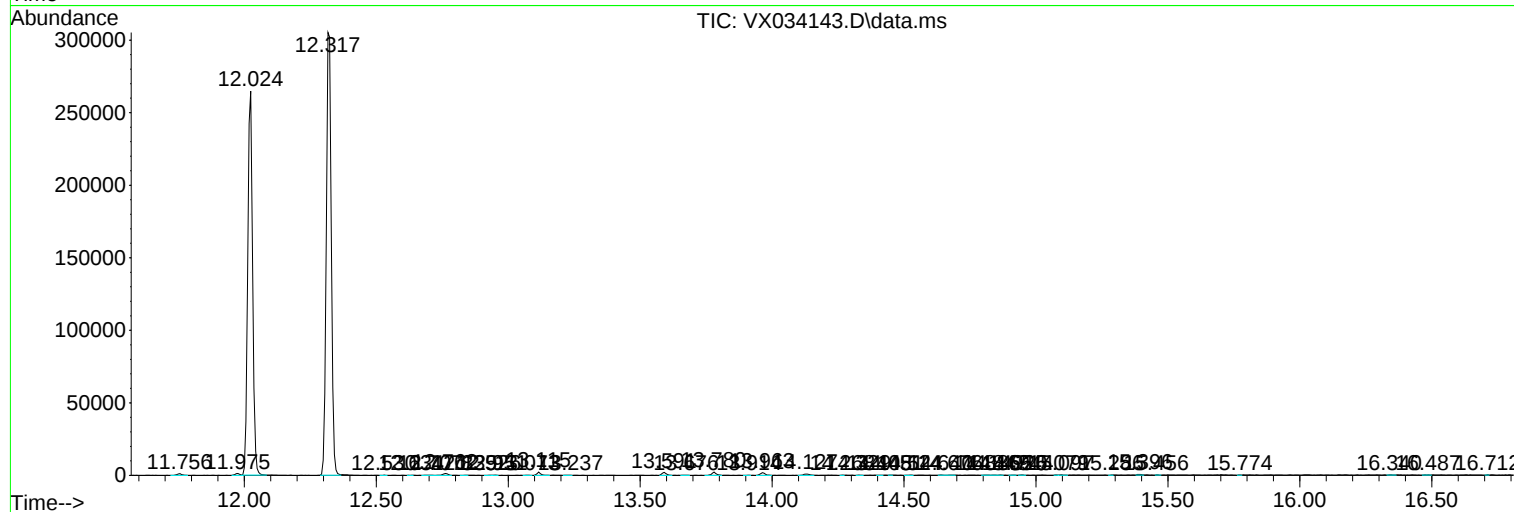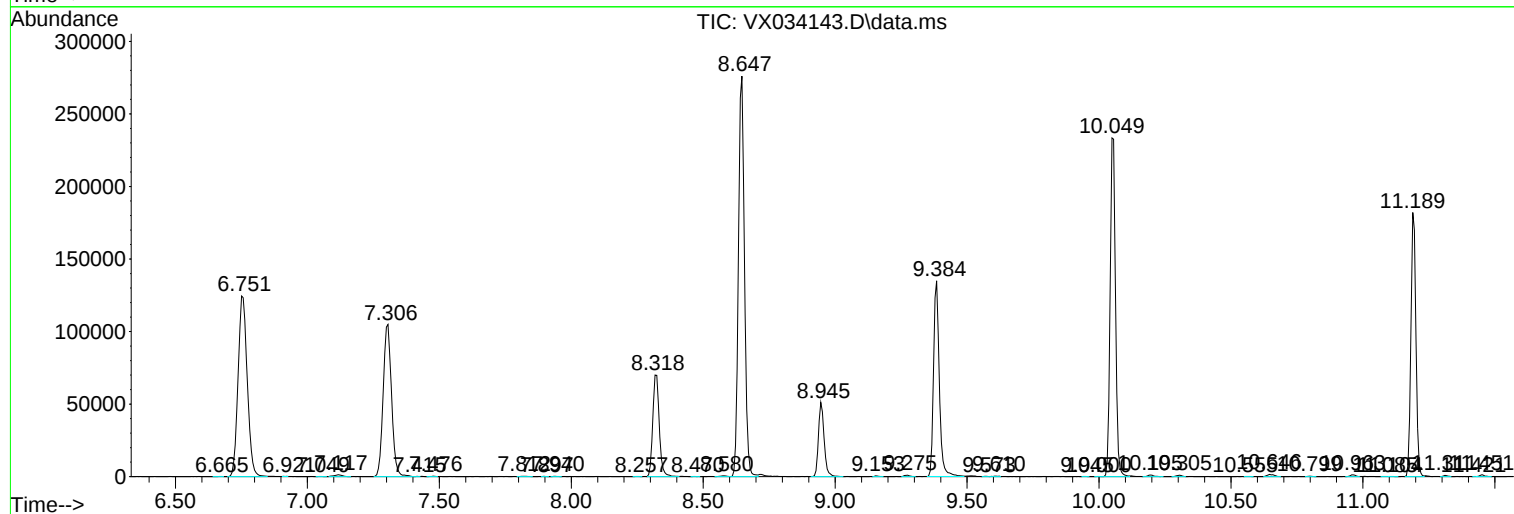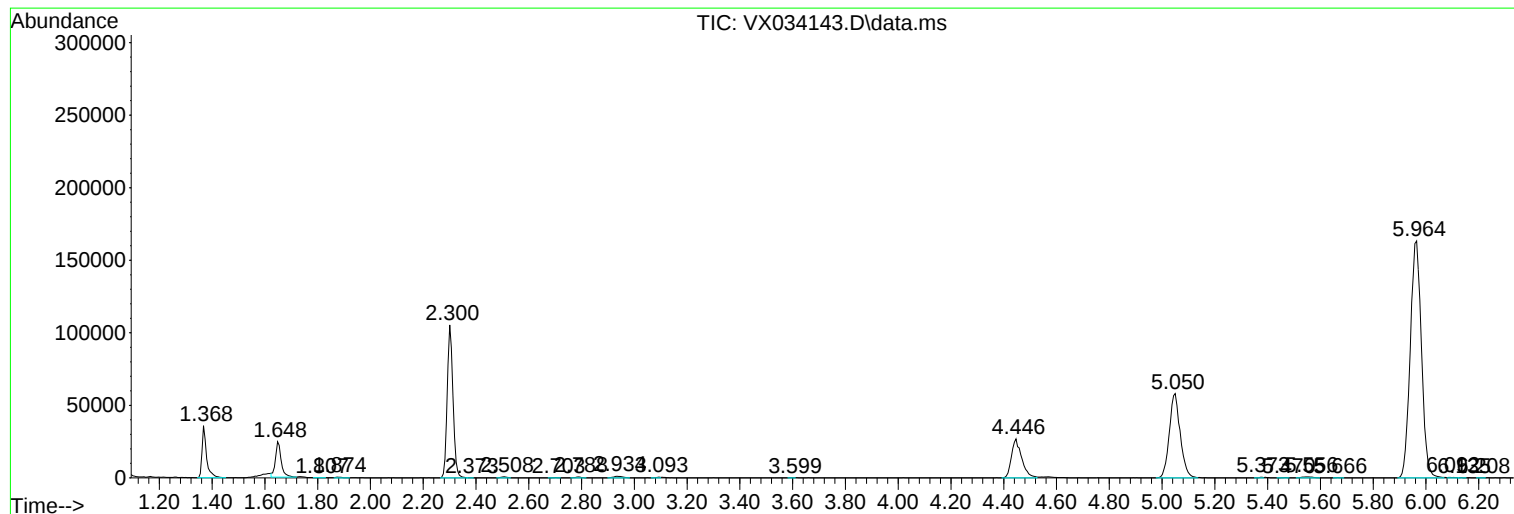

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021323\
Data File : VX034143.D
Acq On : 13 Feb 2023 14:43
Operator : JC/MD
Sample : VX0213WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML021323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021323\
Data File : VX034143.D
Acq On : 13 Feb 2023 14:43
Operator : JC/MD
Sample : VX0213WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML021323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------