
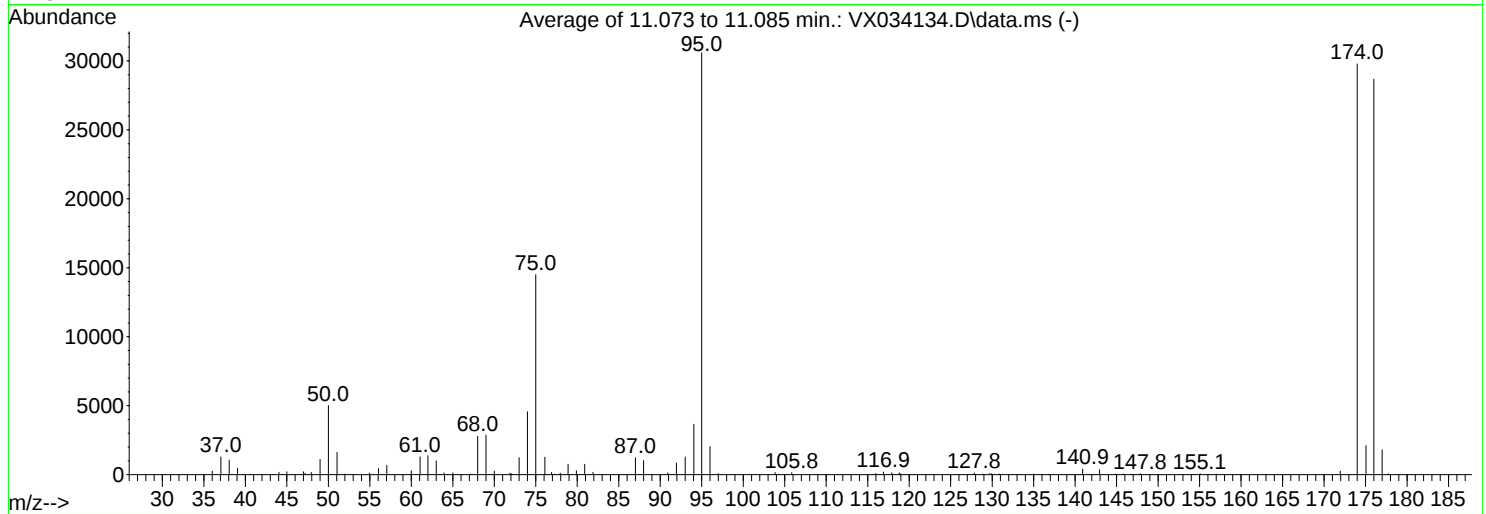


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021323\
Data File : VX034134.D
Acq On : 13 Feb 2023 08:54
Operator : JC/MD
Sample : BFB611
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB611

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM021323WMA.M
Title : VOC Analysis
Last Update : Mon Feb 13 13:44:02 2023

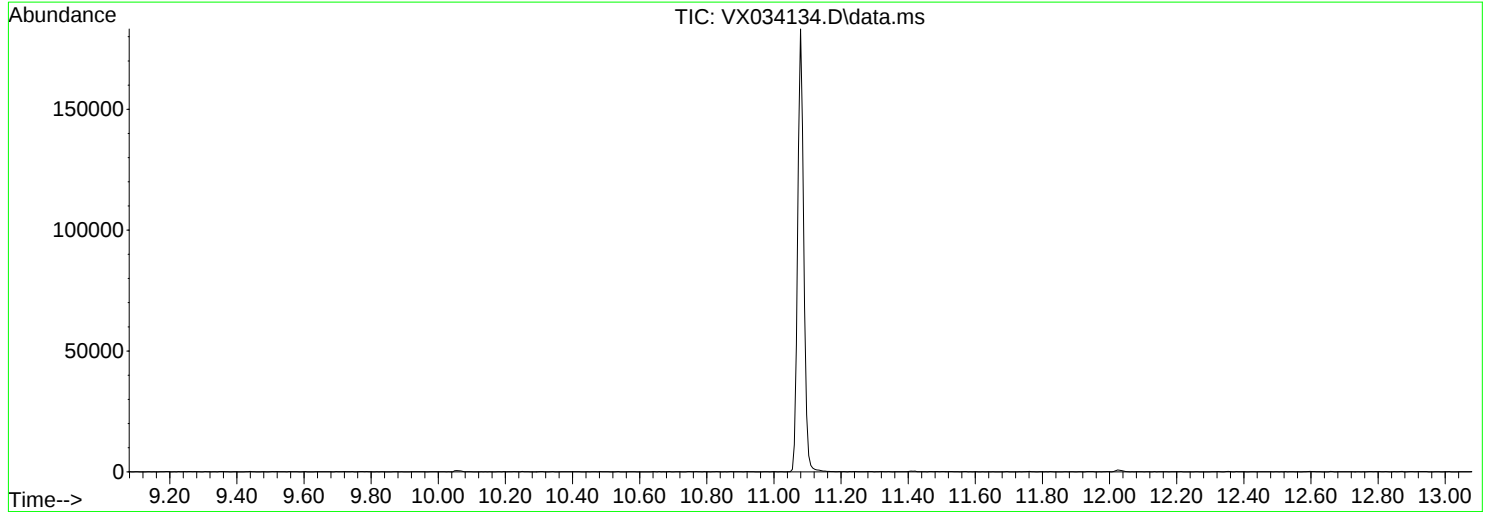

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	5007	PASS
75	95	30	80	47.4	14506	PASS
95	95	100	100	100.0	30587	PASS
96	95	5	9	6.6	2026	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	97.4	29781	PASS
175	174	5	9	7.1	2112	PASS
176	174	95	101	96.3	28683	PASS
177	176	5	9	6.3	1795	PASS

m/z	Abundance
39.90	53.0

Instrument :
MSVOA_X
ClientSampleId :
BFB611

m/z	Abundance
36.00	280.0
37.10	1271.0
38.00	1332.0
39.00	395.0
40.00	107.0
44.00	160.0
45.00	231.0
47.00	384.0
48.10	152.0
49.00	1123.0
50.00	5000.0
51.10	1446.0
52.00	71.0
54.90	119.0
56.00	373.0
57.00	563.0
60.00	272.0
61.00	1166.0
62.00	1360.0
63.00	978.0
64.00	132.0
65.00	125.0
67.10	51.0
68.00	2746.0
69.00	2669.0
70.10	169.0
71.90	120.0
73.00	1037.0
74.00	4217.0
75.00	14353.0
76.10	1237.0
76.90	97.0
77.20	93.0
77.90	97.0
78.90	673.0
79.90	280.0
80.90	750.0
81.90	158.0
87.00	1285.0
88.00	1052.0
90.80	144.0
92.00	727.0
93.00	1231.0
94.00	3189.0
95.00	27528.0
96.00	2046.0
97.00	121.0
103.90	134.0
105.80	188.0
115.80	115.0
116.90	132.0
117.80	115.0
118.80	154.0
127.90	74.0
129.70	76.0
130.00	67.0
130.80	73.0
135.00	66.0
140.90	386.0
143.00	330.0
145.90	57.0
147.10	63.0
147.80	66.0
155.10	55.0
157.00	83.0
172.00	167.0
174.00	23032.0
175.10	1797.0
176.00	21720.0
177.00	1507.0
177.80	63.0

Instrument :
MSVOA_X
ClientSampleId :
BFB611

m/z	Abundance
36.00	307.0
37.10	1543.0
38.10	1012.0
39.10	591.0
40.00	93.0
44.10	203.0
45.00	208.0
47.20	259.0
47.90	215.0
49.00	1354.0
50.00	5819.0
51.00	1942.0
52.00	84.0
55.00	144.0
56.00	606.0
57.00	762.0
60.00	397.0
61.00	1578.0
62.00	1680.0
63.00	1168.0
63.90	163.0
65.00	157.0
67.10	78.0
68.00	3236.0
69.00	3388.0
70.00	367.0
72.10	226.0
73.00	1617.0
74.00	5569.0
75.00	16832.0
76.10	1490.0
76.90	194.0
78.00	124.0
78.90	912.0
80.00	338.0
80.90	905.0
81.90	205.0
87.00	1283.0
88.00	1102.0
90.90	149.0
92.00	1106.0
93.00	1533.0
94.10	4529.0
95.00	36232.0
96.00	2381.0
97.00	121.0
103.80	168.0
104.90	70.0
105.90	139.0
116.00	131.0
116.90	250.0
117.90	189.0
118.80	222.0
127.80	163.0
128.90	75.0
129.90	160.0
130.90	57.0
135.00	94.0
140.90	447.0
141.80	50.0
142.20	53.0
142.90	472.0
144.90	75.0
145.80	83.0
147.90	78.0
155.00	91.0
157.00	72.0
171.90	370.0
174.00	35936.0
175.00	2487.0
176.00	34856.0
177.00	2148.0
177.80	64.0

Instrument :
MSVOA_X
ClientSampleId :
BFB611

m/z	Abundance
36.00	189.0
37.00	1008.0
38.00	824.0
39.10	357.0
40.00	66.0
44.00	139.0
45.00	206.0
47.00	246.0
47.80	116.0
49.00	816.0
50.00	4202.0
51.10	1444.0
55.00	100.0
56.10	331.0
57.10	663.0
59.90	186.0
61.10	1133.0
62.00	1083.0
63.00	861.0
63.90	99.0
65.00	92.0
68.00	2376.0
69.00	2553.0
69.90	224.0
71.90	215.0
73.00	1029.0
74.00	3882.0
75.00	12333.0
76.10	1059.0
76.90	148.0
77.90	116.0
78.90	680.0
79.80	234.0
80.90	566.0
81.80	117.0
87.00	1104.0
88.00	918.0
91.00	86.0
91.90	718.0
93.00	1061.0
94.00	3225.0
95.00	28000.0
96.00	1651.0
103.80	151.0
105.80	137.0
116.00	127.0
116.90	178.0
118.00	101.0
119.00	180.0
127.90	115.0
128.90	59.0
129.70	136.0
136.80	65.0
140.90	393.0
142.90	290.0
144.90	56.0
146.80	64.0
147.90	72.0
155.00	115.0
171.90	228.0
174.00	30376.0
175.00	2052.0
176.00	29472.0
177.00	1731.0
177.80	57.0

Instrument :
MSVOA_X
ClientSampleId :
BFB611