

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX021419\
 Data File : VX007513.D
 Acq On : 13 Feb 2019 11:38
 Operator : JC/SP
 Sample : VX0214WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0214WBL01

Quant Time: Feb 13 14:58:33 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
 Quant Title : SW846 8260
 QLast Update : Sat Feb 02 01:32:36 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	515187	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	808545	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	749874	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	352639	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	280441	51.28	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.56%	
35) Dibromofluoromethane	5.50	113	264466	50.27	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.54%	
50) Toluene-d8	8.71	98	951823	48.76	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.52%	
62) 4-Bromofluorobenzene	11.13	95	333904	46.85	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.70%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX021419\
Data File : VX007513.D
Acq On : 13 Feb 2019 11:38
Operator : JC/SP
Sample : VX0214WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0214WBL01

Quant Time: Feb 13 14:58:33 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Quant Title : SW846 8260
QLast Update : Sat Feb 02 01:32:36 2019
Response via : Initial Calibration

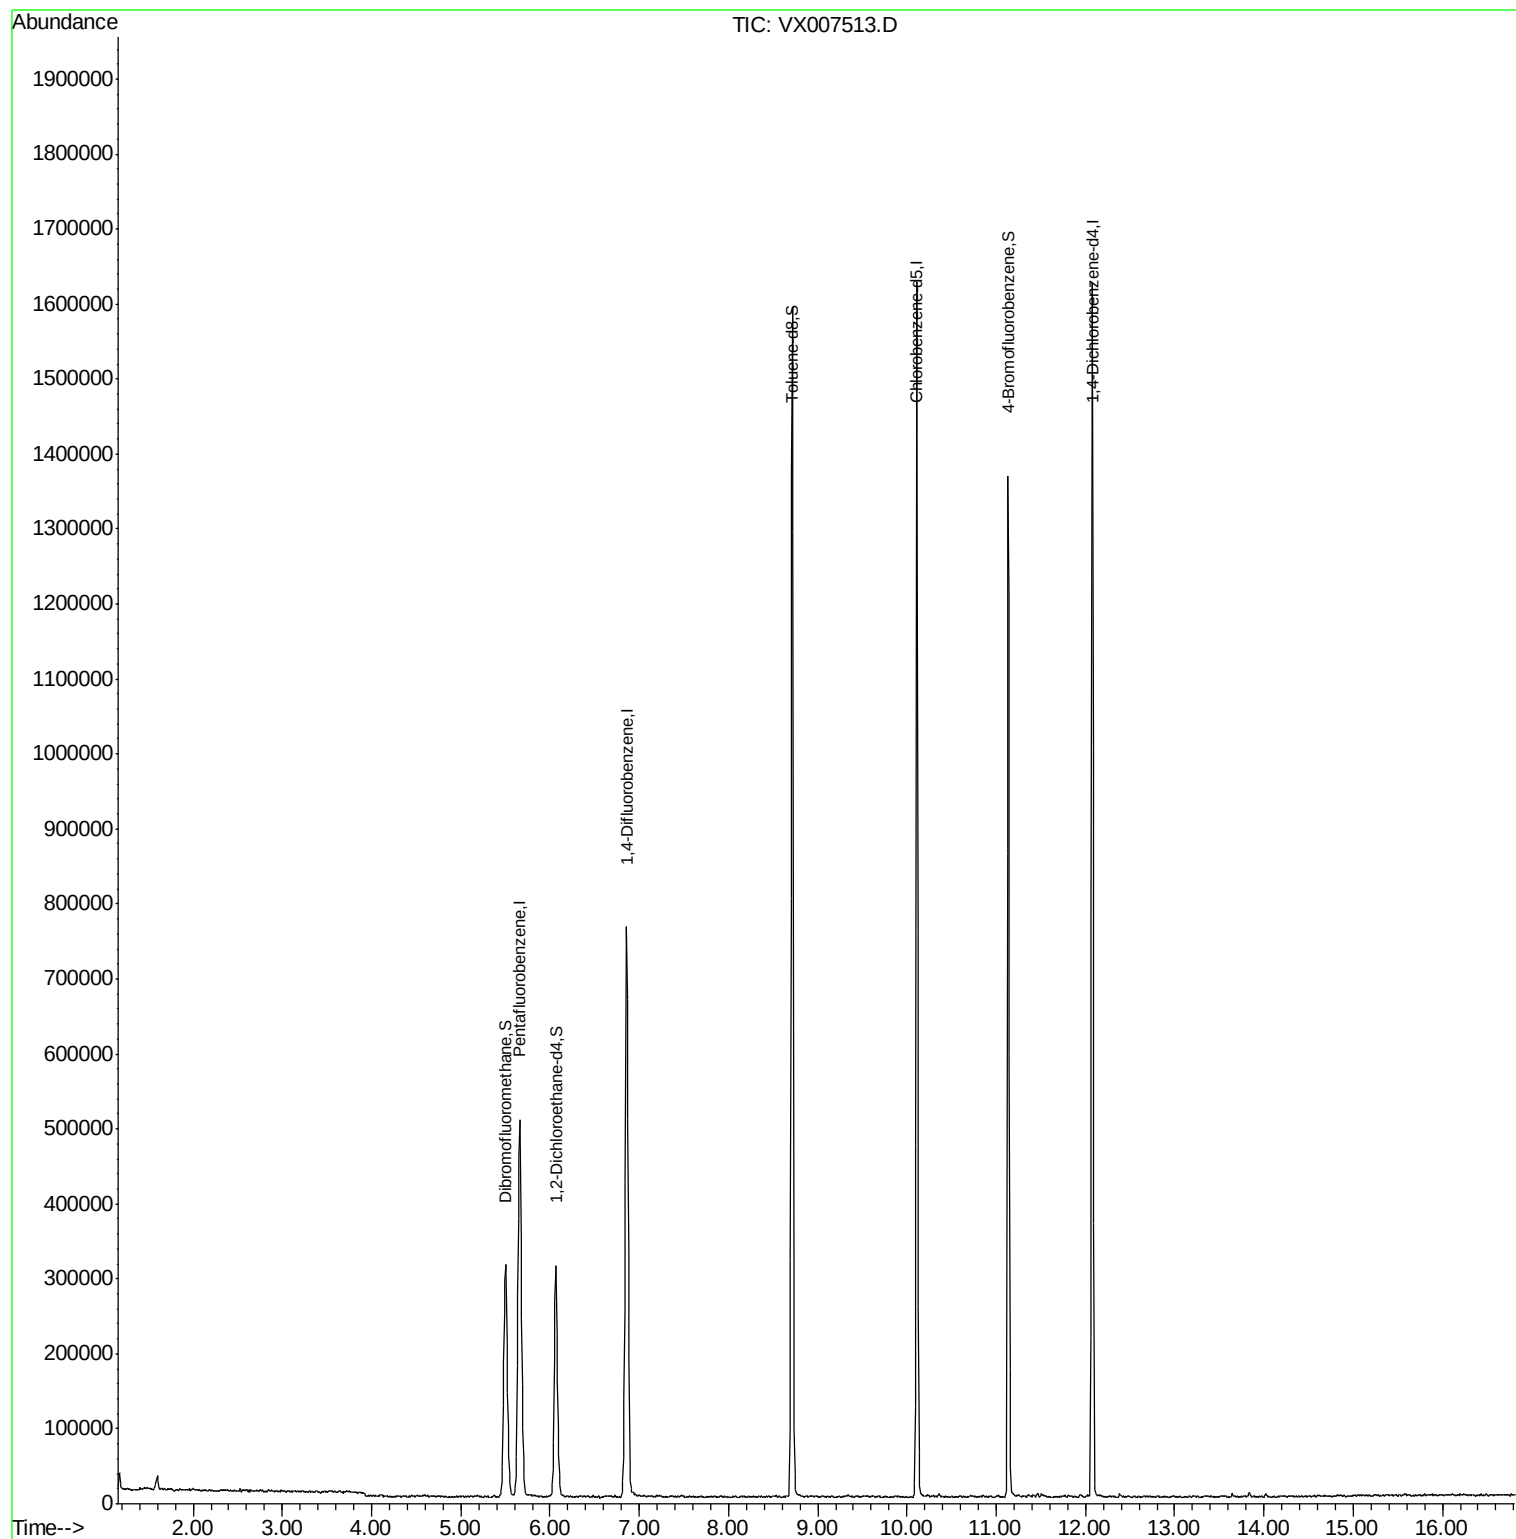

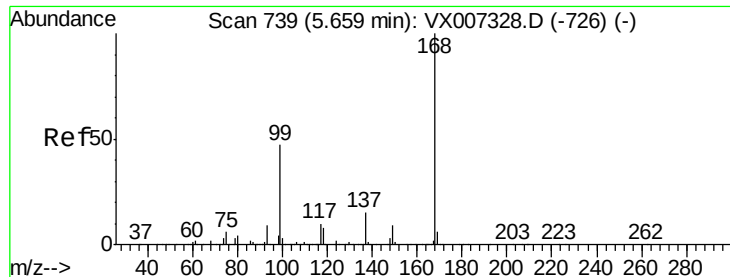

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.01 min

Lab File: VX007513.D

Acq: 13 Feb 2019 11:38

Instrument :

MSVOA_X

ClientSampleId :


VX0214WBL01

Tot Ion:168 Resp: 515187

Ion Ratio Lower Upper

168 100

99 46.7 37.9 56.9

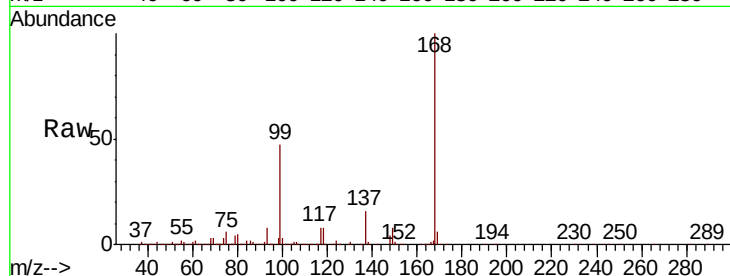

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

200000

150000

100000

50000

0



Time-->

5.50

5.60

5.70

5.80

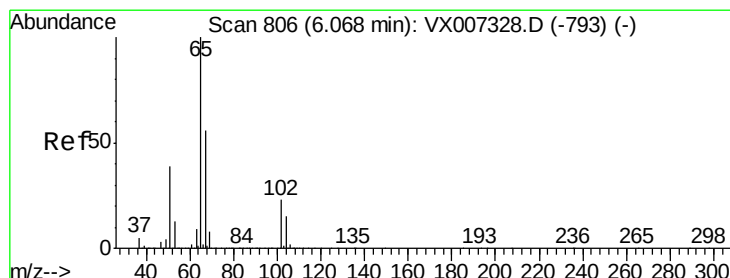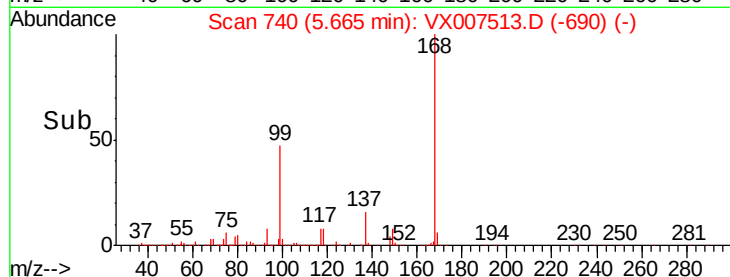

#33

1,2-Dichloroethane-d4

Concen: 51.285 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.00 min

Lab File: VX007513.D


Acq: 13 Feb 2019 11:38

Tgt Ion: 65 Resp: 280441

Ion Ratio Lower Upper

65 100

67 53.9 0.0 108.8

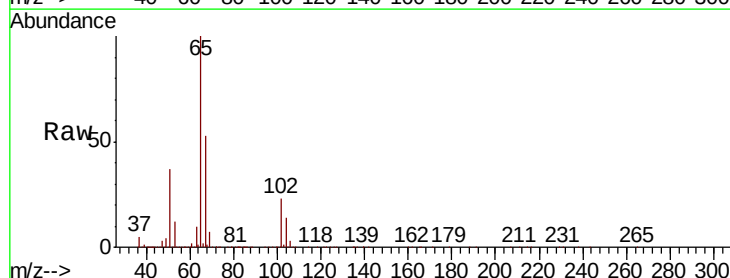

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07

120000

100000

80000

60000

40000

20000


0


Time-->

6.00

6.10

6.20

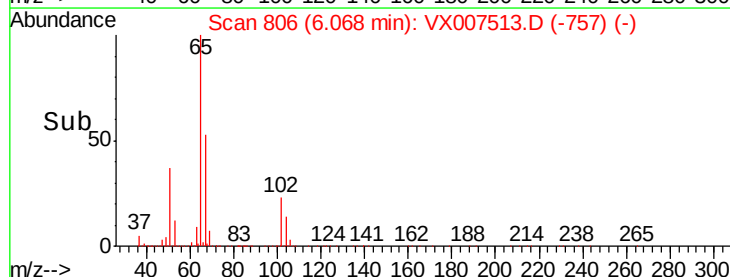

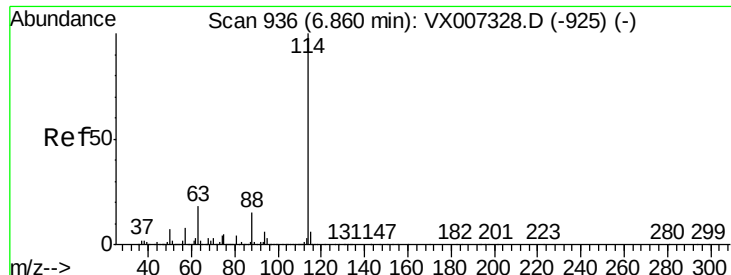

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. 0.00 min

Lab File: VX007513.D

Acq: 13 Feb 2019 11:38

Instrument :

MSVOA_X

ClientSampleId :

VX0214WBL01


Tot Ion:114 Resp: 808545

Ion Ratio Lower Upper

114 100

63 18.1 0.0 35.6




88 14.5 0.0 29.6

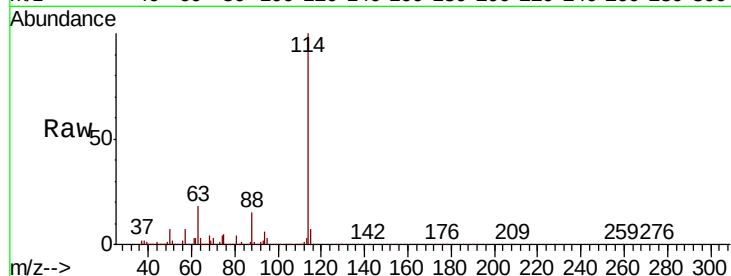

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

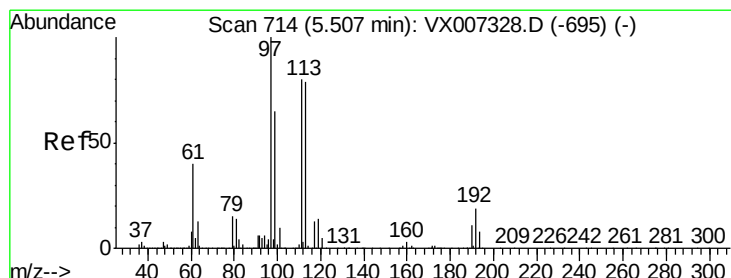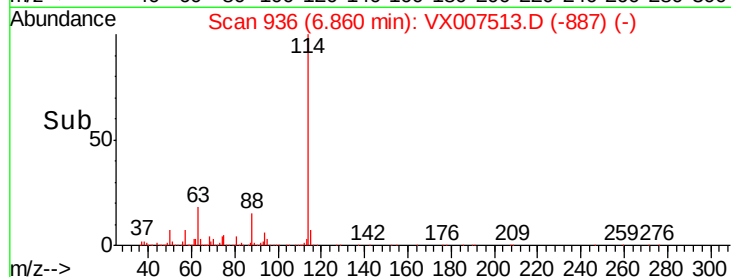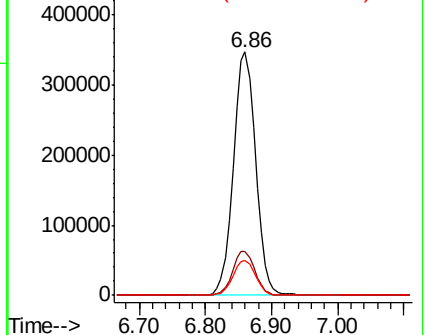

#35

Dibromofluoromethane

Concen: 50.270 ug/l

RT: 5.50 min Scan# 713

Delta R.T. -0.01 min

Lab File: VX007513.D

Acq: 13 Feb 2019 11:38


Tgt Ion:113 Resp: 264466

Ion Ratio Lower Upper

113 100

111 101.9 81.8 122.8



192 21.7 18.5 27.7

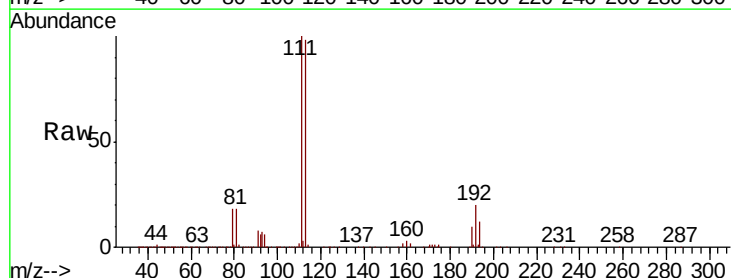


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



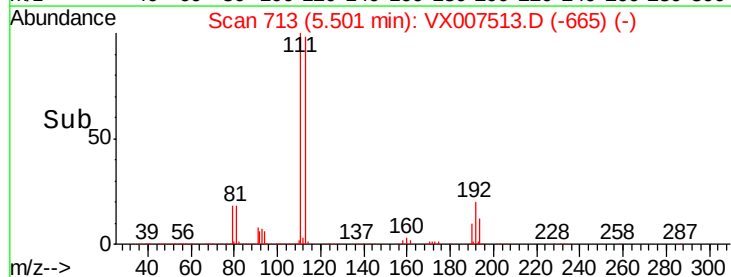
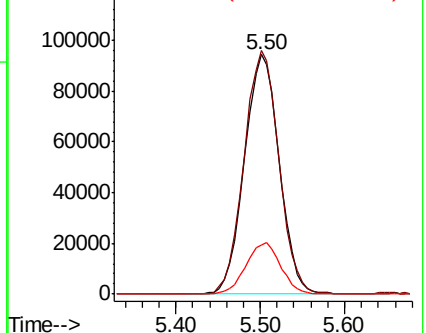


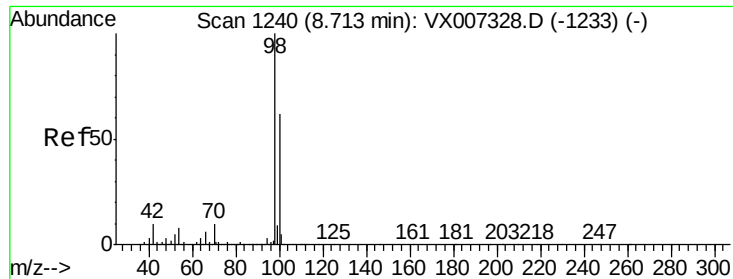

#50
Toluene-d8
Concen: 48.764 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. 0.00 min
Lab File: VX007513.D
Acq: 13 Feb 2019 11:38




Instrument :
MSVOA_X
ClientSampleId :
VX0214WBL01


Tot Ion: 98 Resp: 951823
Ion Ratio Lower Upper
98 100
100 64.6 51.6 77.4

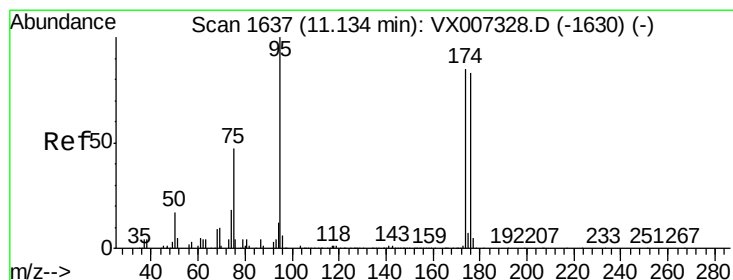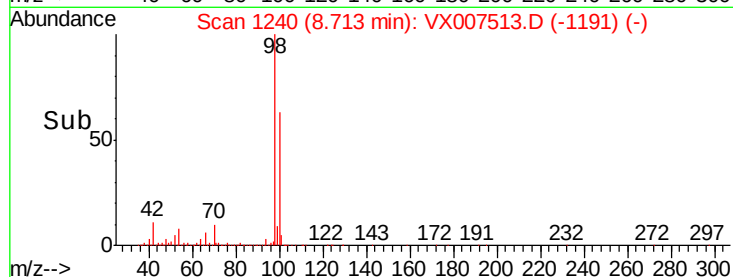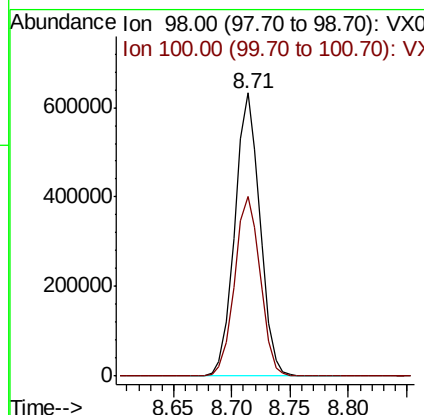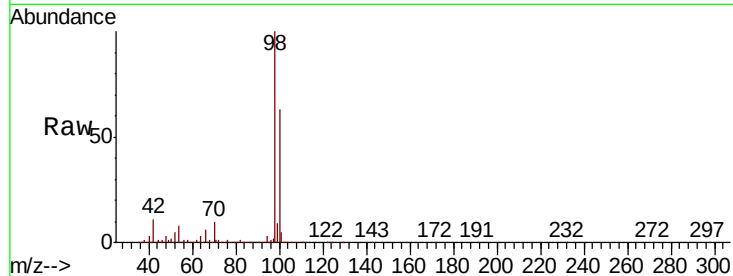

#62
4-Bromofluorobenzene
Concen: 46.855 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. 0.00 min
Lab File: VX007513.D
Acq: 13 Feb 2019 11:38

Tgt Ion: 95 Resp: 333904
Ion Ratio Lower Upper
95 100
174 92.6 0.0 189.2
176 91.0 0.0 186.2

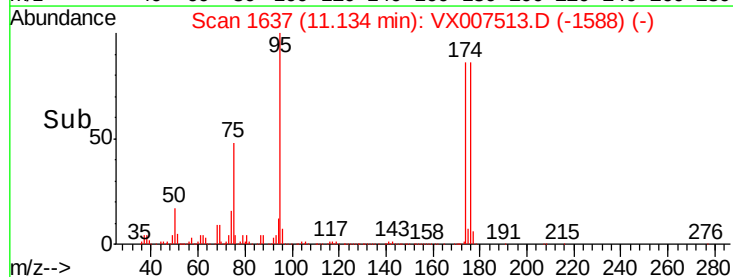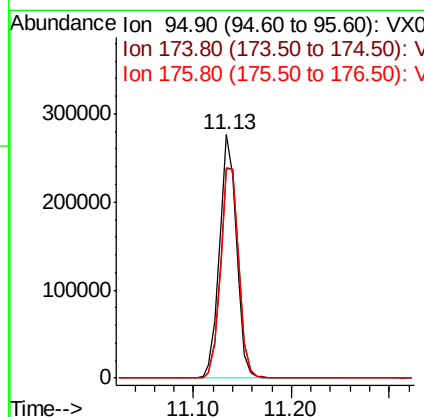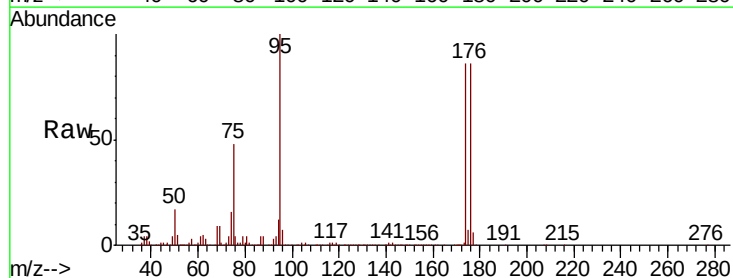

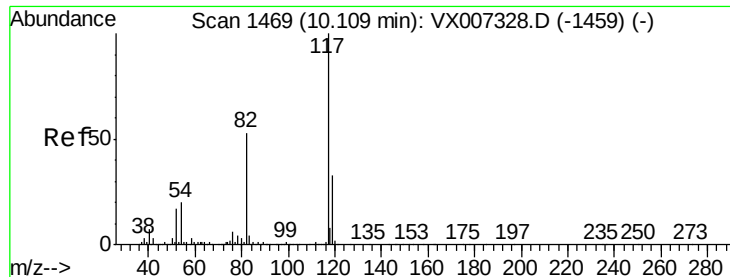

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. 0.00 min

Lab File: VX007513.D

Acq: 13 Feb 2019 11:38

Instrument :

MSVOA_X

ClientSampleId :

VX0214WBL01


Tot Ion:117 Resp: 749874

Ion Ratio Lower Upper

117 100

82 51.8 42.1 63.1




119 32.4 26.5 39.7

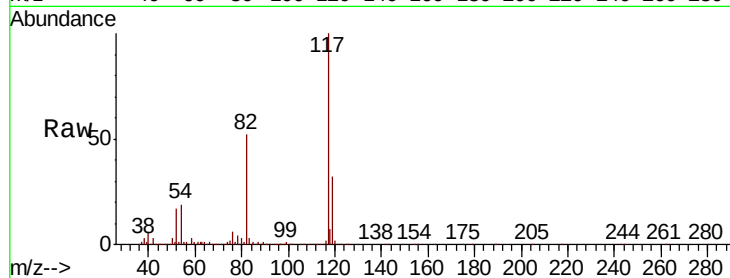

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): V

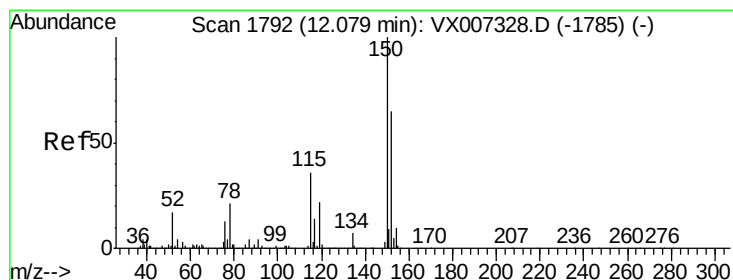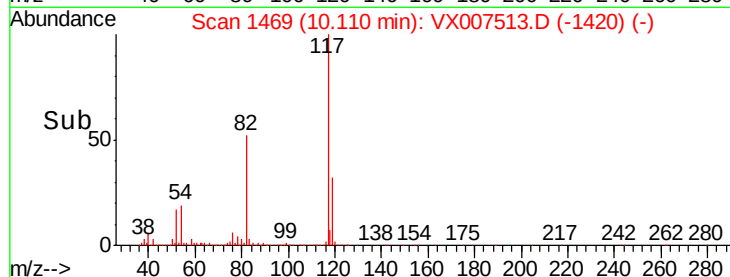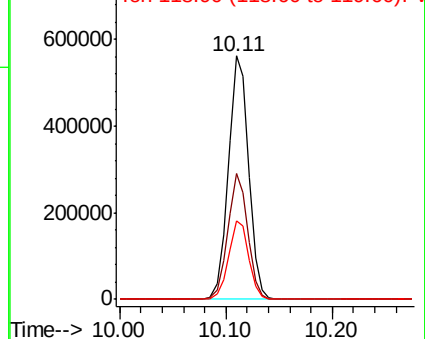

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. 0.00 min

Lab File: VX007513.D

Acq: 13 Feb 2019 11:38


Tgt Ion:152 Resp: 352639

Ion Ratio Lower Upper

152 100

115 54.2 38.0 114.0

150 158.2 0.0 346.4

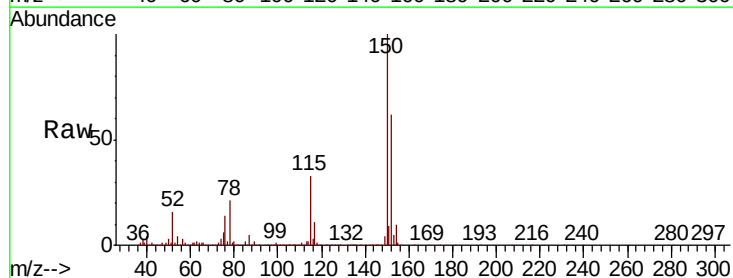

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

