


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX021420\
Data File : VX014936.D
Acq On : 14 Feb 2020 08:56
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X021020W.M
Title : SW846 8260
Last Update : Mon Feb 10 12:09:20 2020

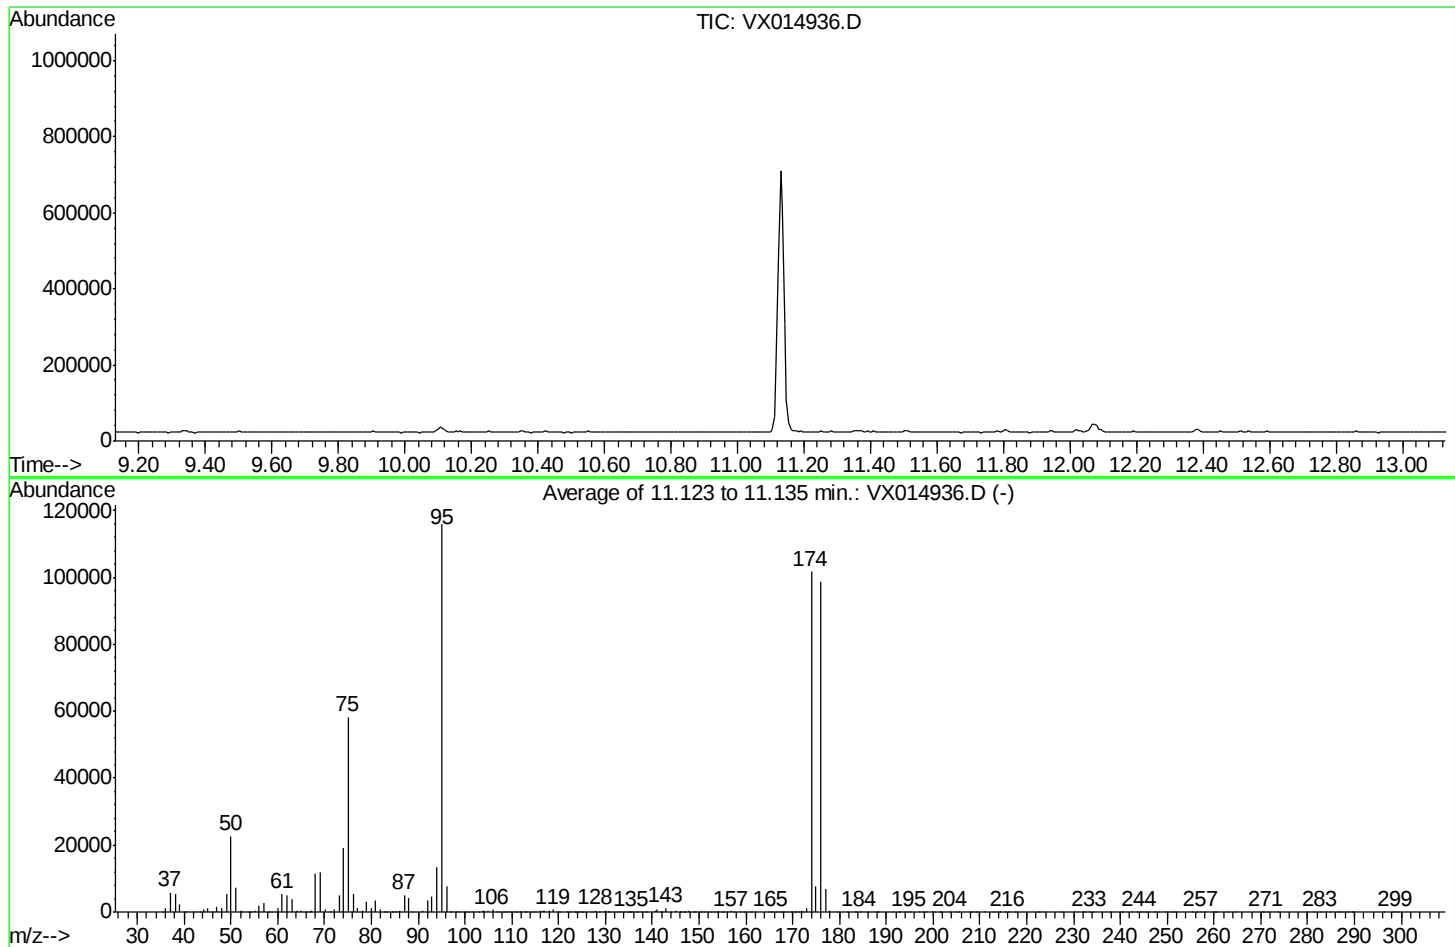

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1668

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	22577	PASS
75	95	30	60	50.3	58242	PASS
95	95	100	100	100.0	115884	PASS
96	95	5	9	6.6	7660	PASS
173	174	0.00	2	1.1	1169	PASS
174	95	50	100	87.8	101733	PASS
175	174	5	9	7.6	7780	PASS
176	174	95	101	97.1	98766	PASS
177	176	5	9	6.8	6763	PASS