

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021422\
 Data File : VX027019.D
 Acq On : 14 Feb 2022 17:37
 Operator : JC/MD
 Sample : VIBLK625
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK625

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML021422WMA.M

Title : VOC Analysis

Signal : TIC: VX027019.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	54	rVB	67178	72073	13.27%	1.764%
2	1.672	91	96	103	rVB	50526	61098	11.25%	1.495%
3	2.087	163	164	166	rBV	220	135	0.02%	0.003%
4	2.313	194	201	211	rBV	123916	199363	36.70%	4.880%
5	2.544	237	239	243	rBV2	126	111	0.02%	0.003%
6	2.642	253	255	256	rBV	134	92	0.02%	0.002%
7	2.715	261	267	270	rVV3	149	311	0.06%	0.008%
8	2.788	275	279	284	rVB4	670	1046	0.19%	0.026%
9	2.831	284	286	288	rBV	118	107	0.02%	0.003%
10	3.032	317	319	321	rVB2	133	141	0.03%	0.003%
11	3.056	321	323	324	rBV	168	139	0.03%	0.003%
12	3.239	349	353	354	rBV	126	177	0.03%	0.004%
13	3.398	377	379	382	rBV	120	135	0.02%	0.003%
14	3.599	408	412	413	rBV	191	222	0.04%	0.005%
15	3.709	429	430	434	rVB	134	148	0.03%	0.004%
16	3.745	434	436	439	rBV2	138	209	0.04%	0.005%
17	3.922	462	465	471	rBV2	141	256	0.05%	0.006%
18	3.977	471	474	475	rVB	143	133	0.02%	0.003%
19	4.007	475	479	482	rBV	176	286	0.05%	0.007%
20	4.099	490	494	497	rBV2	110	229	0.04%	0.006%
21	4.166	502	505	507	rBV2	121	125	0.02%	0.003%
22	4.312	527	529	530	rBV2	129	117	0.02%	0.003%
23	4.330	530	532	536	rVB	179	181	0.03%	0.004%
24	4.391	538	542	543	rBV	122	139	0.03%	0.003%
25	4.452	543	552	570	rBV	40910	119575	22.01%	2.927%
26	4.904	624	626	629	rBV2	159	185	0.03%	0.005%
27	4.977	635	638	639	rBV	95	113	0.02%	0.003%
28	5.062	639	652	666	rVV2	69935	213000	39.21%	5.213%
29	5.184	669	672	673	rBV	135	98	0.02%	0.002%
30	5.379	703	704	705	rBV	217	139	0.03%	0.003%
31	5.495	721	723	724	rBV	157	111	0.02%	0.003%
32	5.544	728	731	732	rBV2	342	330	0.06%	0.008%
33	5.690	753	755	757	rBV	95	93	0.02%	0.002%
34	5.818	772	776	777	rVB	155	151	0.03%	0.004%
35	5.970	788	801	818	rVV2	182719	543291	100.00%	13.298%
36	6.233	842	844	845	rVB	142	100	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021422\
 Data File : VX027019.D
 Acq On : 14 Feb 2022 17:37
 Operator : JC/MD
 Sample : VIBLK625
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK625

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML021422WMA.M
 Title : VOC Analysis

37	6.263	847	849	850	rVB	145	93	0.02%	0.002%
38	6.287	850	853	854	rBV	189	233	0.04%	0.006%
39	6.385	868	869	871	rBV	157	99	0.02%	0.002%
40	6.483	883	885	888	rVB2	124	121	0.02%	0.003%
41	6.623	906	908	911	rVB2	144	137	0.03%	0.003%
42	6.653	911	913	914	rBV2	99	86	0.02%	0.002%
43	6.763	921	931	945	rBV	130128	311145	57.27%	7.616%
44	6.928	956	958	960	rBV	162	184	0.03%	0.005%
45	6.982	965	967	968	rBV	177	128	0.02%	0.003%
46	7.019	970	973	974	rBV2	93	114	0.02%	0.003%
47	7.110	981	988	998	rVB	6408	13932	2.56%	0.341%
48	7.196	1000	1002	1005	rBV2	120	180	0.03%	0.004%
49	7.306	1011	1020	1033	rVB	111682	241279	44.41%	5.906%
50	7.415	1037	1038	1040	rVB	192	126	0.02%	0.003%
51	7.446	1040	1043	1044	rBV	151	158	0.03%	0.004%
52	7.732	1089	1090	1092	rBV	141	94	0.02%	0.002%
53	7.805	1098	1102	1107	rVB3	276	542	0.10%	0.013%
54	7.854	1107	1110	1111	rBV	171	163	0.03%	0.004%
55	7.927	1120	1122	1128	rVB2	424	639	0.12%	0.016%
56	8.037	1136	1140	1142	rBV	139	177	0.03%	0.004%
57	8.177	1160	1163	1165	rBV	136	132	0.02%	0.003%
58	8.251	1173	1175	1177	rVB2	135	108	0.02%	0.003%
59	8.275	1177	1179	1181	rBV	151	119	0.02%	0.003%
60	8.324	1181	1187	1198	rVV	69913	112760	20.75%	2.760%
61	8.476	1209	1212	1215	rBV3	253	366	0.07%	0.009%
62	8.647	1233	1240	1248	rVV	285891	448482	82.55%	10.977%
63	8.720	1248	1252	1261	rVB	3968	6206	1.14%	0.152%
64	8.781	1261	1262	1264	rBV	167	127	0.02%	0.003%
65	8.909	1281	1283	1284	rBV	195	160	0.03%	0.004%
66	8.952	1284	1290	1300	rVB	48921	70036	12.89%	1.714%
67	9.098	1311	1314	1315	rBV	140	105	0.02%	0.003%
68	9.116	1315	1317	1320	rBV	86	92	0.02%	0.002%
69	9.269	1340	1342	1346	rVB	438	573	0.11%	0.014%
70	9.384	1355	1361	1379	rBV	186171	275151	50.65%	6.735%
71	9.866	1439	1440	1442	rBV	155	103	0.02%	0.003%
72	10.055	1465	1471	1485	rBV	283195	381332	70.19%	9.333%
73	10.195	1492	1494	1497	rBV	207	131	0.02%	0.003%
74	10.299	1508	1511	1515	rBV3	645	897	0.17%	0.022%
75	10.409	1526	1529	1530	rBV2	161	154	0.03%	0.004%
76	10.457	1535	1537	1539	rVV2	122	101	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021422\
 Data File : VX027019.D
 Acq On : 14 Feb 2022 17:37
 Operator : JC/MD
 Sample : VIBLK625
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK625

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML021422WMA.M
 Title : VOC Analysis

77	10.659	1566	1570	1575	rVB3	999	1243	0.23%	0.030%
78	10.963	1617	1620	1624	rVB	423	470	0.09%	0.012%
79	11.122	1642	1646	1652	rBV	1627	2112	0.39%	0.052%
80	11.189	1652	1657	1666	rBV	182580	233977	43.07%	5.727%
81	11.274	1668	1671	1675	rBV3	243	389	0.07%	0.010%
82	11.384	1687	1689	1691	rVB2	172	131	0.02%	0.003%
83	11.433	1696	1697	1699	rBV	115	91	0.02%	0.002%
84	11.482	1701	1705	1710	rVB2	977	1171	0.22%	0.029%
85	11.750	1744	1749	1753	rVB2	1282	1732	0.32%	0.042%
86	11.841	1762	1764	1770	rVB	297	310	0.06%	0.008%
87	11.933	1776	1779	1782	rBV	852	929	0.17%	0.023%
88	11.969	1782	1785	1788	rVV	648	700	0.13%	0.017%
89	12.018	1788	1793	1804	rVV	288136	378941	69.75%	9.275%
90	12.317	1837	1842	1849	rBV	284311	375602	69.13%	9.193%
91	12.427	1857	1860	1866	rBV2	400	413	0.08%	0.010%
92	12.481	1867	1869	1872	rVB2	187	163	0.03%	0.004%
93	12.622	1890	1892	1896	rBV2	192	262	0.05%	0.006%
94	12.658	1896	1898	1899	rBV2	162	150	0.03%	0.004%
95	13.115	1967	1973	1977	rBV	2524	3113	0.57%	0.076%
96	13.591	2047	2051	2054	rVB	1775	1913	0.35%	0.047%
97	13.701	2067	2069	2072	rBV	139	101	0.02%	0.002%
98	13.963	2110	2112	2115	rBV2	562	565	0.10%	0.014%
99	14.481	2194	2197	2198	rBV	140	140	0.03%	0.003%
100	14.829	2253	2254	2257	rBV2	115	94	0.02%	0.002%




Sum of corrected areas: 4085636

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021422\
Data File : VX027019.D
Acq On : 14 Feb 2022 17:37
Operator : JC/MD
Sample : VIBLK625
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK625

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML021422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

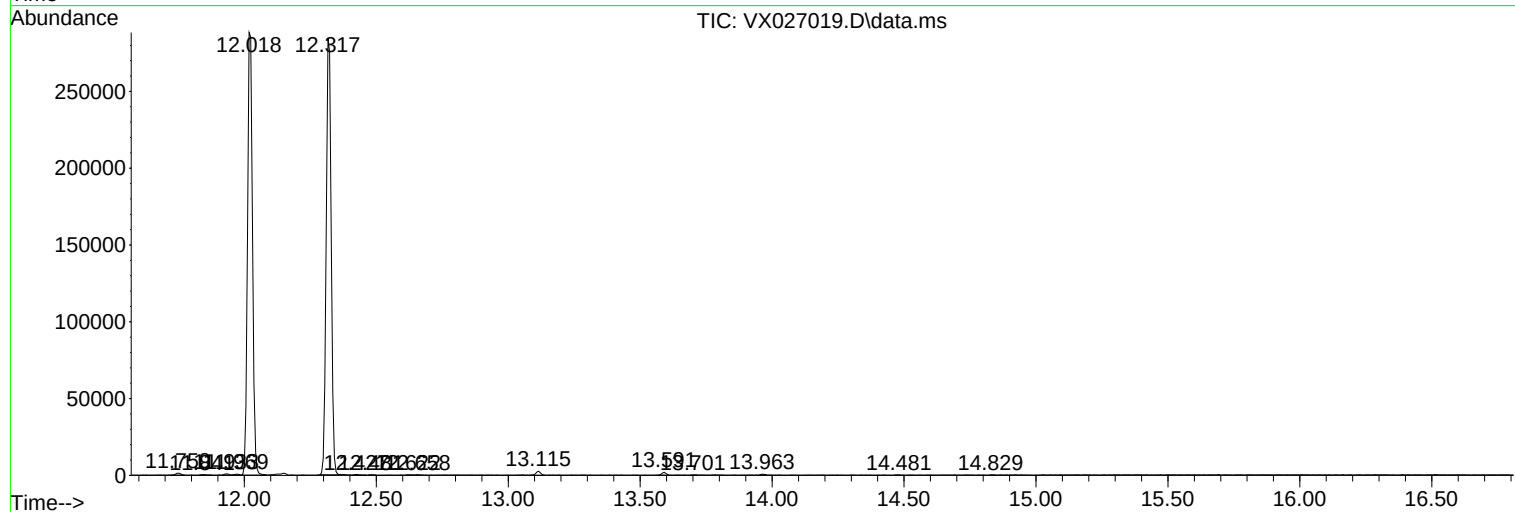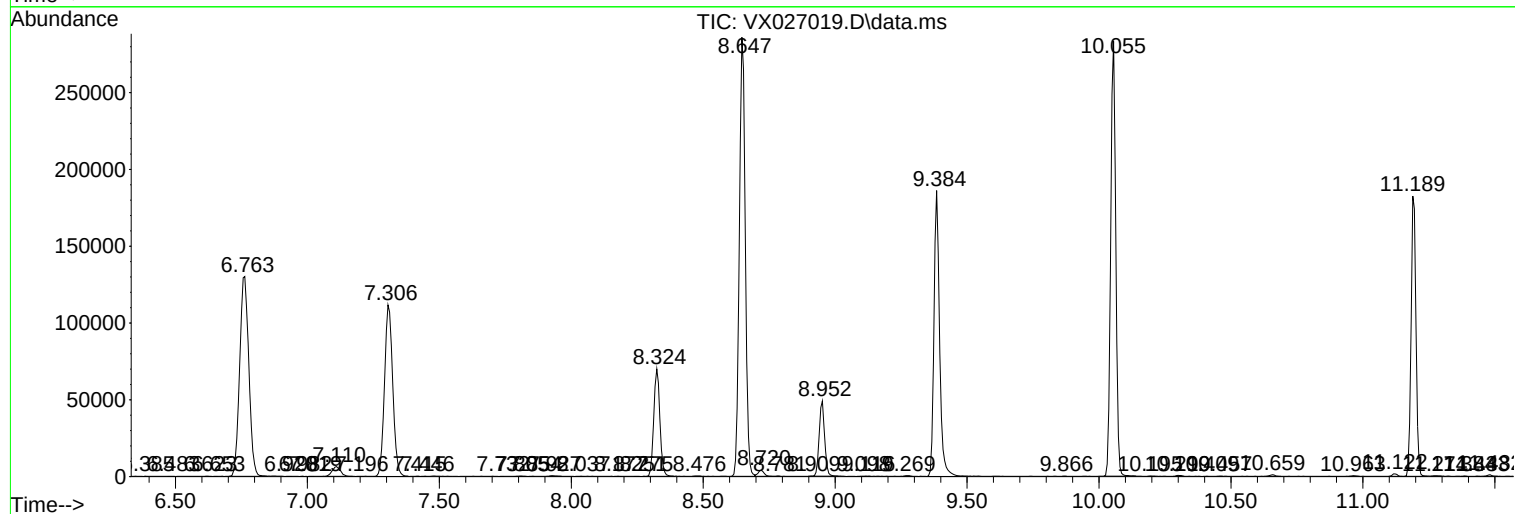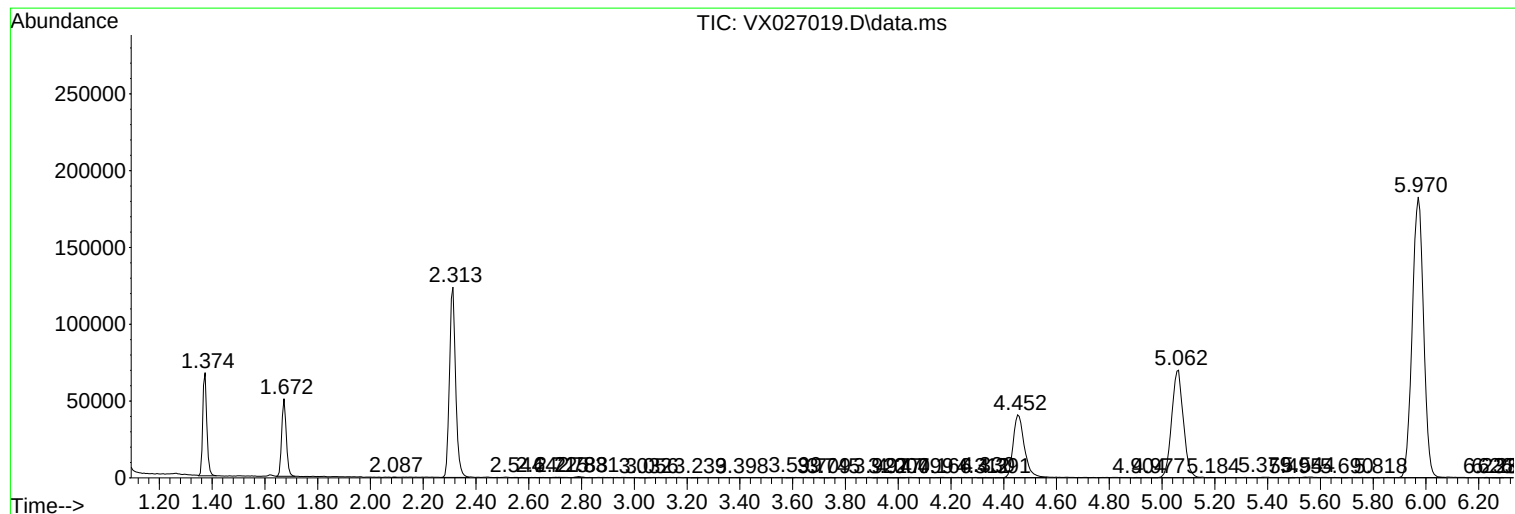

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021422\
Data File : VX027019.D
Acq On : 14 Feb 2022 17:37
Operator : JC/MD
Sample : VIBLK625
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK625

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML021422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021422\
Data File : VX027019.D
Acq On : 14 Feb 2022 17:37
Operator : JC/MD
Sample : VIBLK625
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK625

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML021422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc