
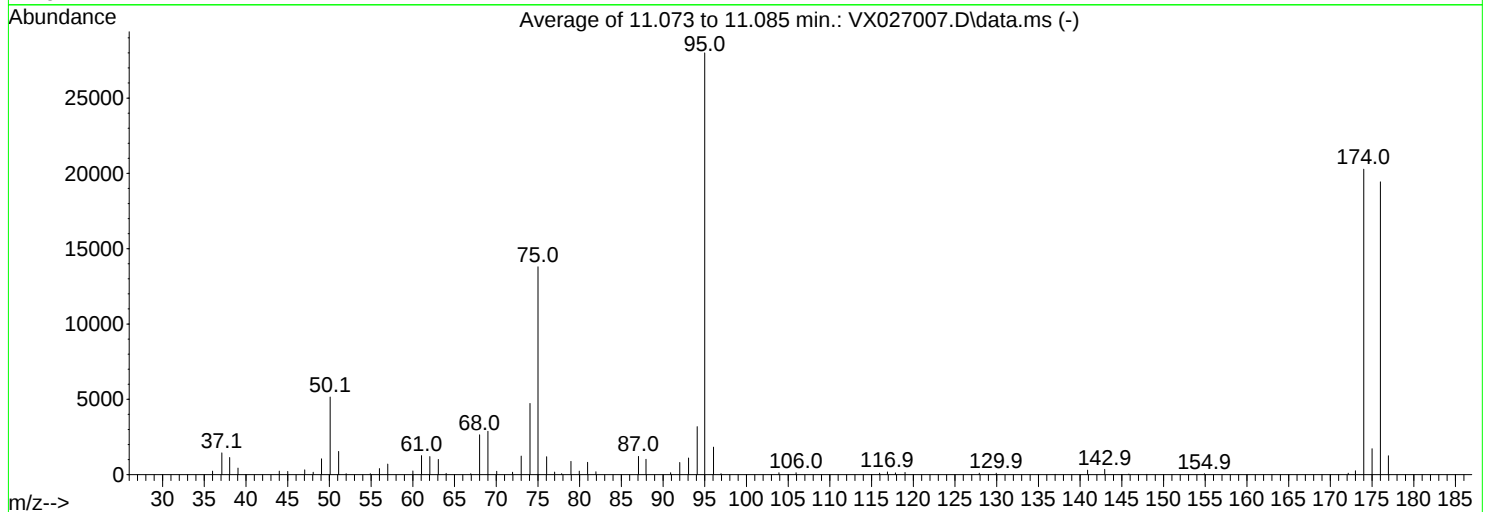


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021422\
Data File : VX027007.D
Acq On : 14 Feb 2022 09:38
Operator : JC/MD
Sample : BFB634
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB634

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM021422WMA.M
Title : VOC Analysis
Last Update : Wed Feb 16 01:34:21 2022

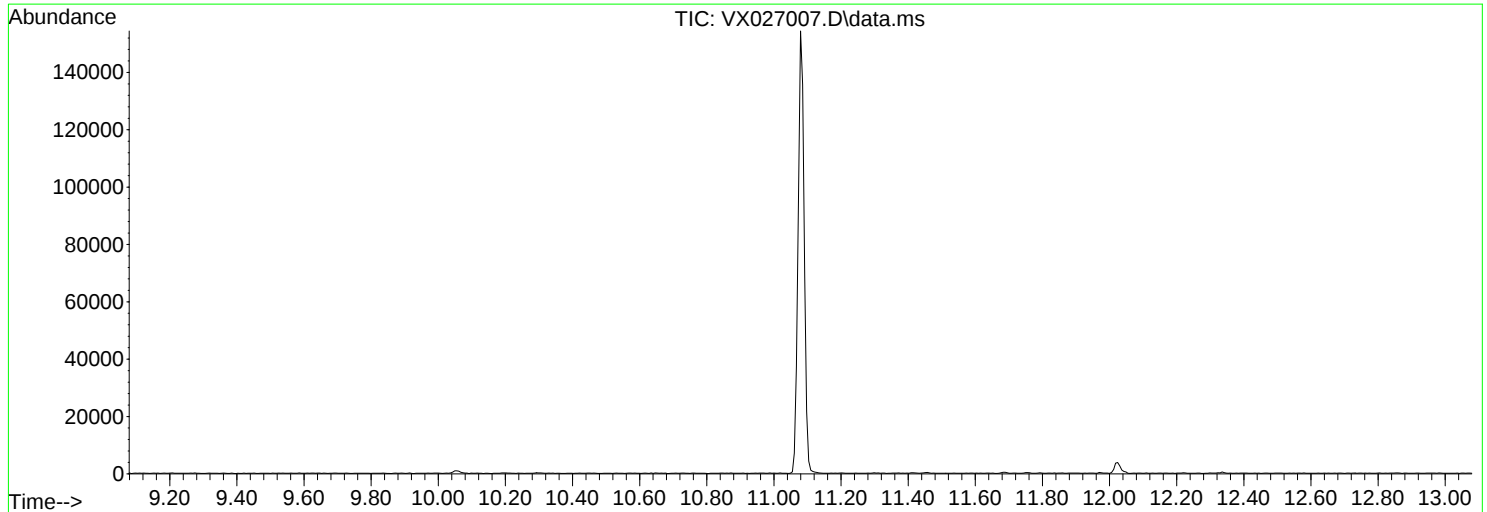

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	5155	PASS
75	95	30	80	49.3	13798	PASS
95	95	100	100	100.0	28003	PASS
96	95	5	9	6.5	1825	PASS
173	174	0.00	2	1.3	259	PASS
174	95	50	120	72.4	20277	PASS
175	174	5	9	8.5	1716	PASS
176	174	95	101	95.9	19442	PASS
177	176	5	9	6.4	1252	PASS

m/z	Abundance
40.00	153.0

Instrument :
MSVOA_X
ClientSampleId :
BFB634

m/z	Abundance
36.00	181.0
37.10	1245.0
38.10	1021.0
39.10	396.0
40.10	150.0
44.00	199.0
45.00	188.0
47.10	307.0
48.00	145.0
49.00	984.0
50.10	4475.0
51.10	1322.0
52.00	78.0
54.90	58.0
56.00	220.0
57.00	586.0
60.00	220.0
61.00	990.0
62.00	1068.0
63.00	932.0
64.00	64.0
68.00	2073.0
69.00	2326.0
70.00	163.0
72.10	165.0
73.00	945.0
74.00	3829.0
75.00	10861.0
76.00	940.0
77.00	117.0
78.90	630.0
80.00	152.0
80.90	553.0
82.00	165.0
87.00	958.0
87.90	772.0
90.90	81.0
92.00	693.0
93.00	861.0
94.10	2267.0
95.00	21240.0
96.00	1532.0
96.90	60.0
103.90	111.0
106.00	93.0
115.90	80.0
116.90	130.0
117.80	82.0
119.00	133.0
127.90	74.0
130.00	65.0
140.90	212.0
142.90	201.0
172.10	100.0
173.00	128.0
174.00	13495.0
175.00	1199.0
176.00	12502.0
176.90	881.0

Instrument :
MSVOA_X
ClientSampleId :
BFB634

m/z	Abundance
36.00	347.0
37.10	1679.0
38.10	1345.0
39.10	495.0
40.10	183.0
44.00	286.0
45.00	272.0
47.10	413.0
48.10	200.0
49.10	1238.0
50.10	6275.0
51.10	1856.0
52.00	100.0
54.90	84.0
56.00	547.0
57.00	877.0
60.00	322.0
61.00	1494.0
62.10	1465.0
63.10	1162.0
64.00	88.0
66.90	80.0
68.00	3198.0
69.00	3419.0
70.10	307.0
71.90	186.0
73.00	1540.0
74.10	5526.0
75.00	16688.0
76.00	1499.0
77.00	226.0
77.90	118.0
79.00	1084.0
79.90	267.0
80.90	1071.0
81.90	221.0
87.10	1513.0
88.00	1161.0
91.00	171.0
92.00	939.0
93.10	1281.0
94.10	3974.0
95.00	34240.0
96.10	2145.0
96.90	61.0
103.90	138.0
106.00	160.0
115.90	99.0
116.90	239.0
117.90	112.0
119.10	159.0
127.90	106.0
130.00	137.0
140.90	355.0
143.00	386.0
145.90	62.0
148.00	69.0
154.90	112.0
172.10	114.0
173.00	340.0
174.00	23712.0
175.00	2013.0
176.00	23000.0
177.00	1464.0

Instrument :
MSVOA_X
ClientSampleId :
BFB634

m/z	Abundance
36.10	171.0
37.10	1404.0
38.00	1036.0
39.00	411.0
40.00	172.0
44.00	229.0
45.00	189.0
47.00	241.0
48.00	122.0
49.00	928.0
50.10	4714.0
51.10	1438.0
54.90	65.0
56.00	442.0
57.00	649.0
60.00	194.0
61.10	1316.0
62.10	1071.0
63.00	938.0
64.00	91.0
67.00	97.0
68.00	2676.0
69.00	2901.0
70.00	210.0
71.90	142.0
73.00	1221.0
74.00	4814.0
75.00	13844.0
76.10	1146.0
77.00	172.0
77.80	76.0
78.90	916.0
80.00	284.0
81.00	818.0
81.90	198.0
87.00	1175.0
88.00	1129.0
90.80	117.0
92.00	802.0
93.10	1185.0
94.10	3316.0
95.00	28528.0
96.00	1797.0
97.00	57.0
103.90	128.0
105.90	145.0
116.00	105.0
116.90	161.0
117.90	166.0
118.90	158.0
127.90	110.0
129.90	91.0
137.00	59.0
140.90	332.0
142.90	453.0
145.80	58.0
154.90	86.0
172.20	75.0
173.00	308.0
174.00	23624.0
175.00	1937.0
176.00	22824.0
177.00	1410.0

Instrument :
MSVOA_X
ClientSampleId :
BFB634