

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021424\
 Data File : VX040225.D
 Acq On : 14 Feb 2024 17:04
 Operator : JC/MD
 Sample : P1395-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-20240205

Quant Time: Feb 15 00:05:18 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020924W.M
 Quant Title : SW846 8260
 QLast Update : Mon Feb 12 00:21:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	74490	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	123181	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	119129	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	61495	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	46827	42.255	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	84.520%
35) Dibromofluoromethane	5.391	113	39261	45.640	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	91.280%
50) Toluene-d8	8.647	98	148057	46.011	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	92.020%
62) 4-Bromofluorobenzene	11.079	95	58217	44.360	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	88.720%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021424\
Data File : VX040225.D
Acq On : 14 Feb 2024 17:04
Operator : JC/MD
Sample : P1395-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-20240205

Quant Time: Feb 15 00:05:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020924W.M
Quant Title : SW846 8260
QLast Update : Mon Feb 12 00:21:14 2024
Response via : Initial Calibration




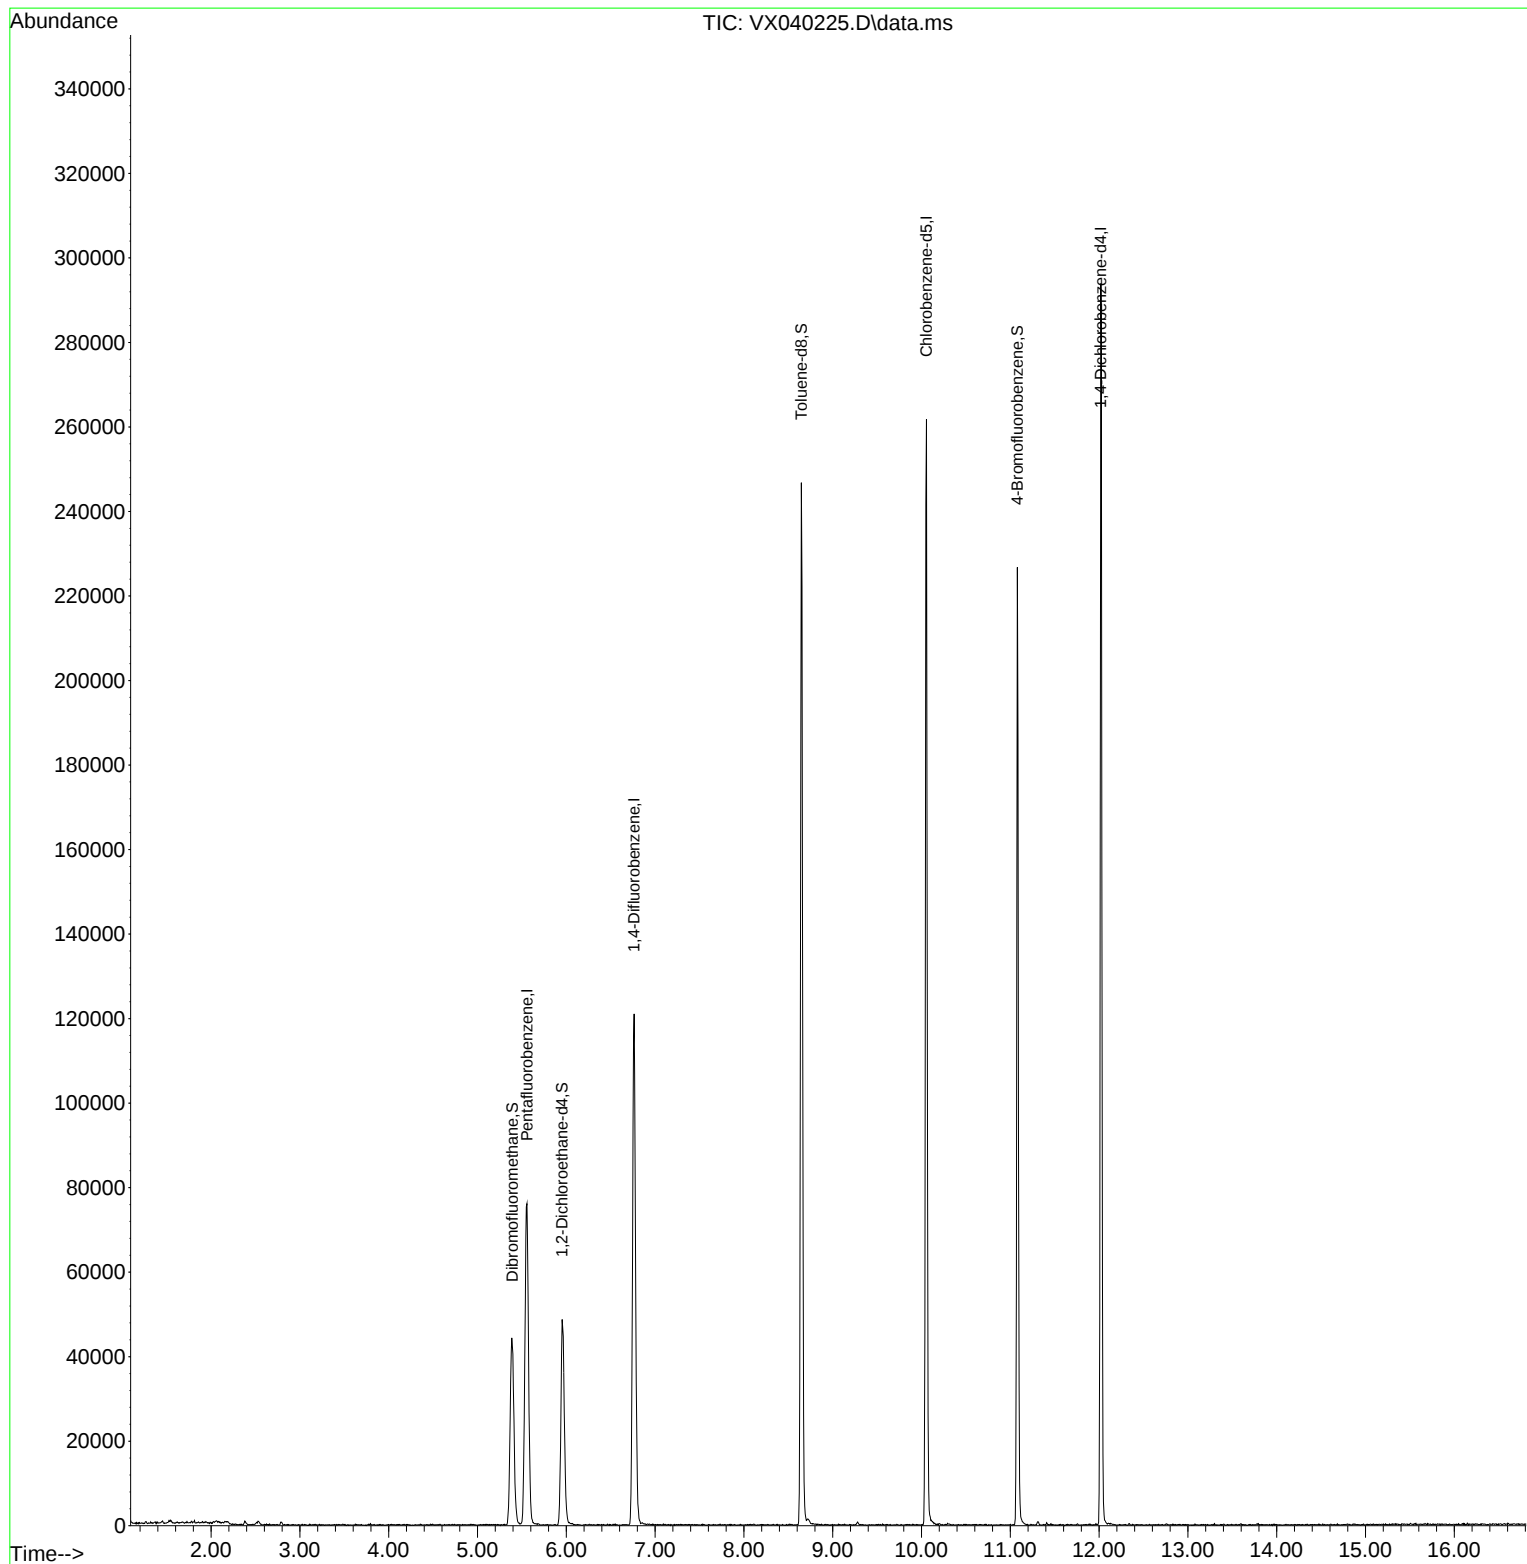


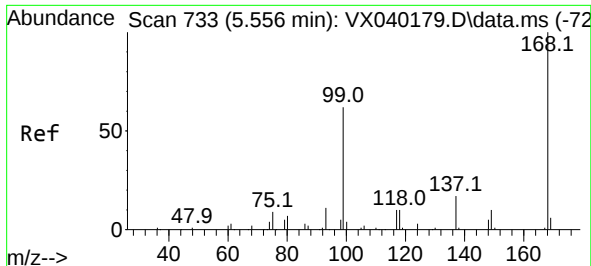

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX040225.D
Acq: 14 Feb 2024 17:04




Instrument :
MSVOA_X
ClientSampleId :
TB-20240205


Tgt Ion:168 Resp: 74490
Ion Ratio Lower Upper
168 100
99 55.2 56.6 85.0#

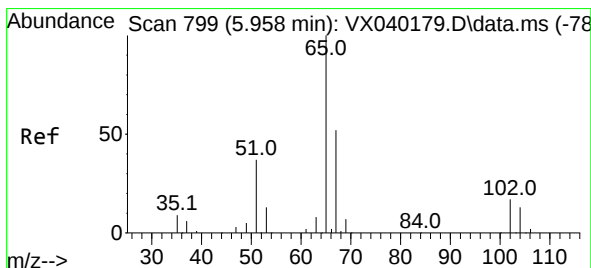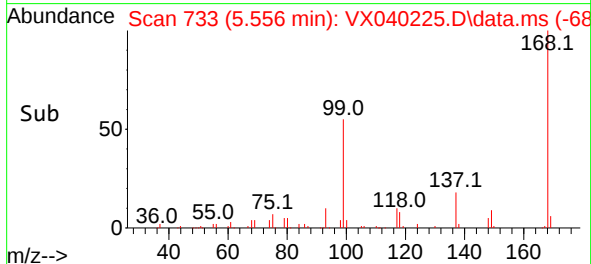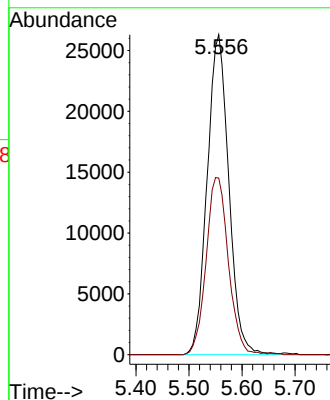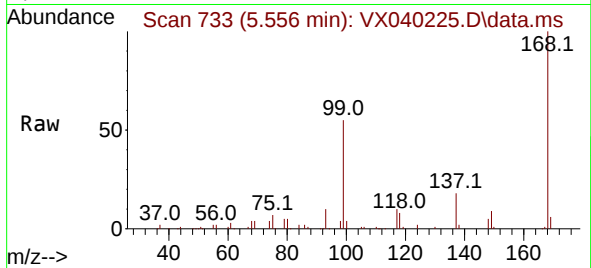

#33
1,2-Dichloroethane-d4
Concen: 42.255 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX040225.D
Acq: 14 Feb 2024 17:04

Tgt Ion: 65 Resp: 46827
Ion Ratio Lower Upper
65 100
67 53.9 0.0 100.2

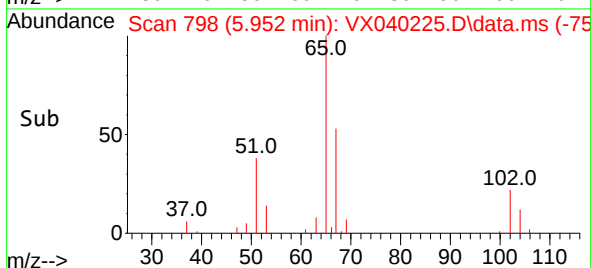
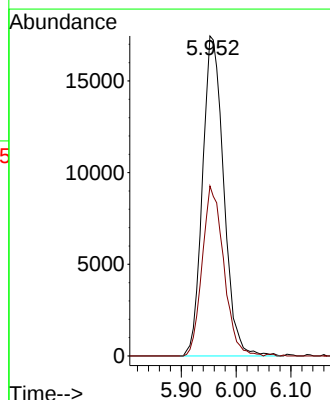
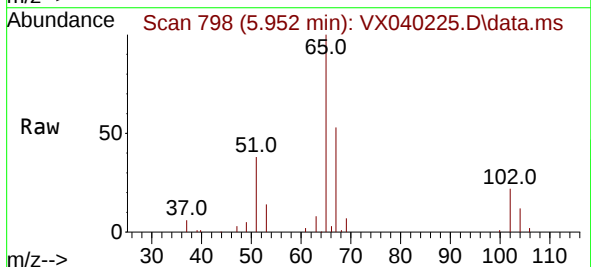


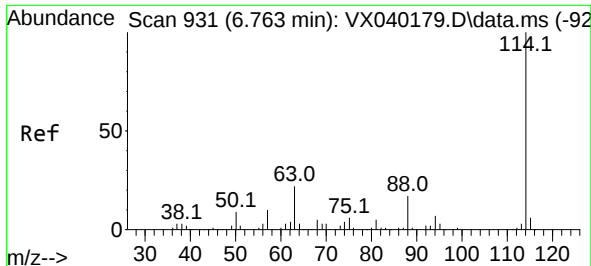

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX040225.D
Acq: 14 Feb 2024 17:04




Instrument :
MSVOA_X
ClientSampleId :
TB-20240205


Tgt Ion:114 Resp: 123181
Ion Ratio Lower Upper
114 100
63 20.5 0.0 45.0
88 16.0 0.0 36.6

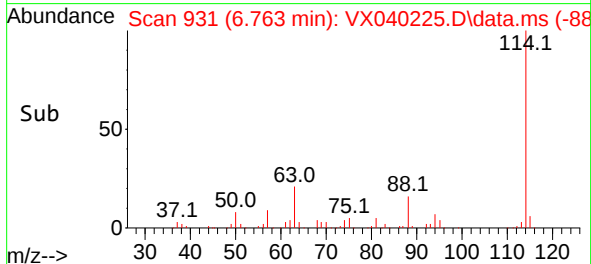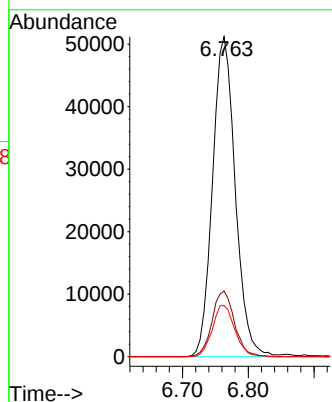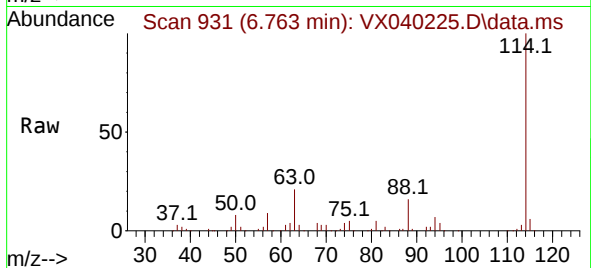

#35
Dibromofluoromethane
Concen: 45.640 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX040225.D
Acq: 14 Feb 2024 17:04

Tgt Ion:113 Resp: 39261
Ion Ratio Lower Upper
113 100
111 102.8 82.9 124.3
192 19.8 13.3 19.9


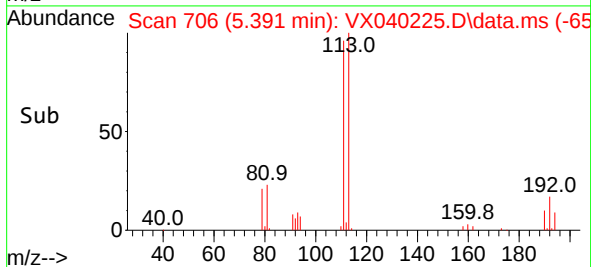
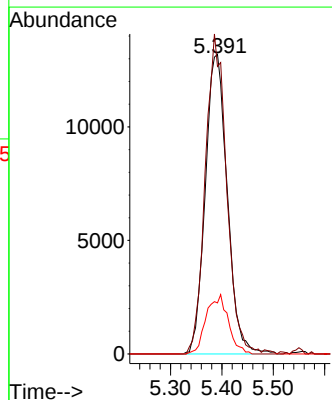
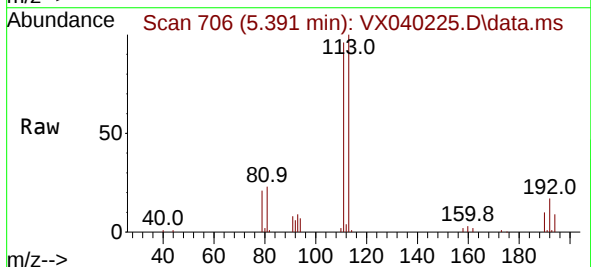


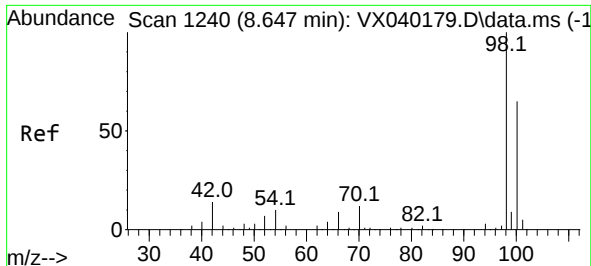

#50
Toluene-d8
Concen: 46.011 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX040225.D
Acq: 14 Feb 2024 17:04




Instrument :
MSVOA_X
ClientSampleId :
TB-20240205


Tgt Ion: 98 Resp: 148057
Ion Ratio Lower Upper
98 100
100 64.0 53.1 79.7

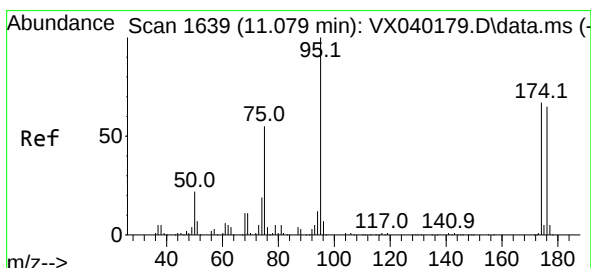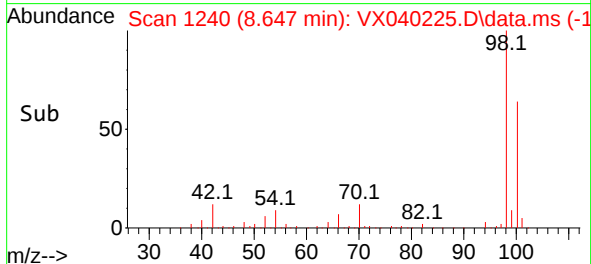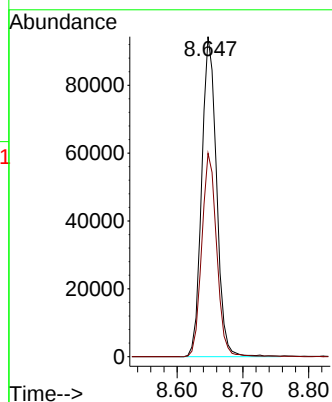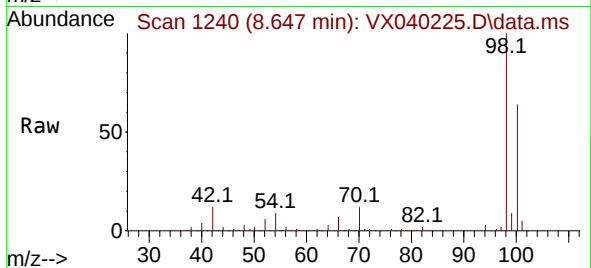

#62
4-Bromofluorobenzene
Concen: 44.360 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX040225.D
Acq: 14 Feb 2024 17:04

Tgt Ion: 95 Resp: 58217
Ion Ratio Lower Upper
95 100
174 80.5 0.0 135.6
176 77.0 0.0 131.0


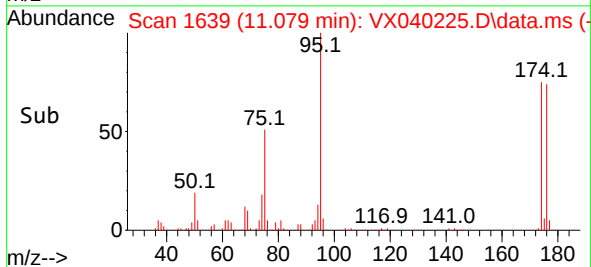
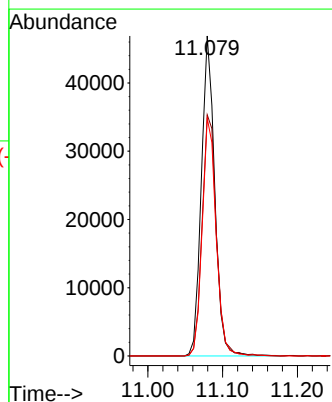
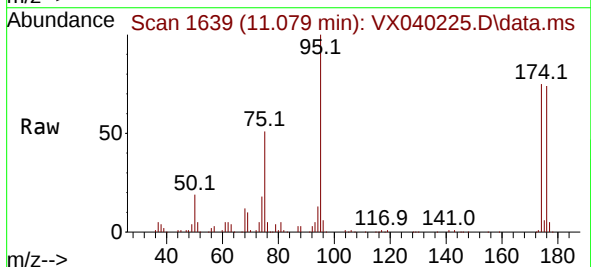


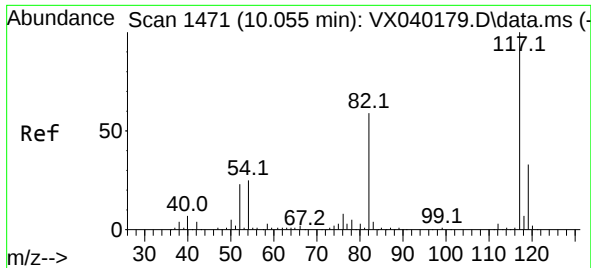

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX040225.D
Acq: 14 Feb 2024 17:04

Instrument :
MSVOA_X
ClientSampleId :
TB-20240205

Tgt Ion:117 Resp: 119129
Ion Ratio Lower Upper
117 100
82 54.8 46.2 69.4
119 32.4 25.5 38.3

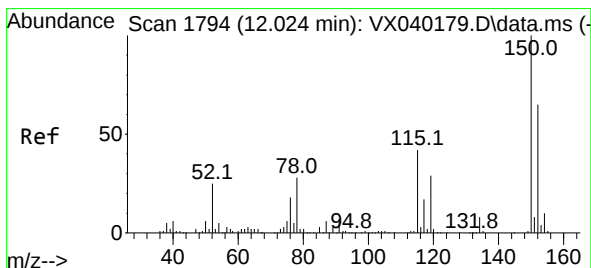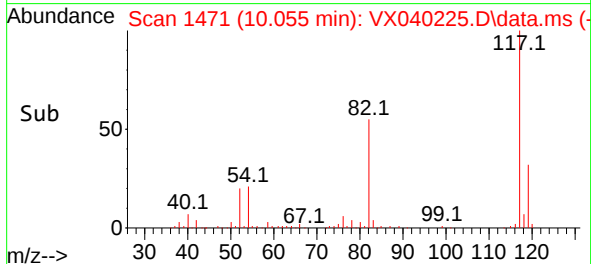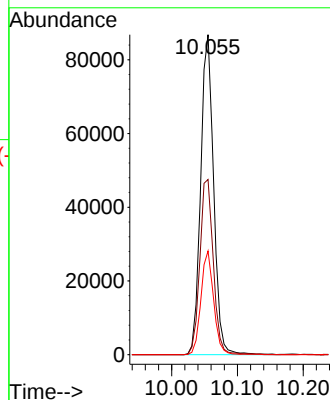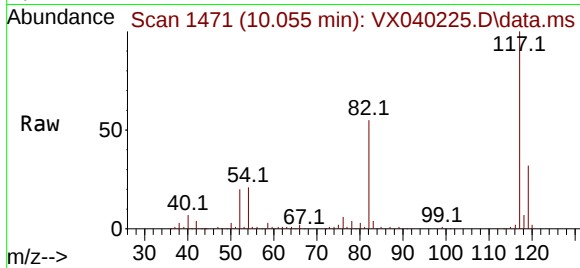

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.006 min
Lab File: VX040225.D
Acq: 14 Feb 2024 17:04

Tgt Ion:152 Resp: 61495
Ion Ratio Lower Upper
152 100
115 61.2 43.3 129.9
150 157.1 0.0 345.0

