

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021424\
 Data File : VX040228.D
 Acq On : 14 Feb 2024 18:13
 Operator : JC/MD
 Sample : P1445-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Quant Time: Feb 15 00:06:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020924W.M
 Quant Title : SW846 8260
 QLast Update : Mon Feb 12 00:21:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	71344	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	118782	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	115532	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	60988	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	45066	42.460	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	84.920%
35) Dibromofluoromethane	5.391	113	38287	46.156	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.320%
50) Toluene-d8	8.647	98	144177	46.465	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	92.920%
62) 4-Bromofluorobenzene	11.079	95	57179	45.183	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	90.360%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021424\
Data File : VX040228.D
Acq On : 14 Feb 2024 18:13
Operator : JC/MD
Sample : P1445-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Time: Feb 15 00:06:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020924W.M
Quant Title : SW846 8260
QLast Update : Mon Feb 12 00:21:14 2024
Response via : Initial Calibration




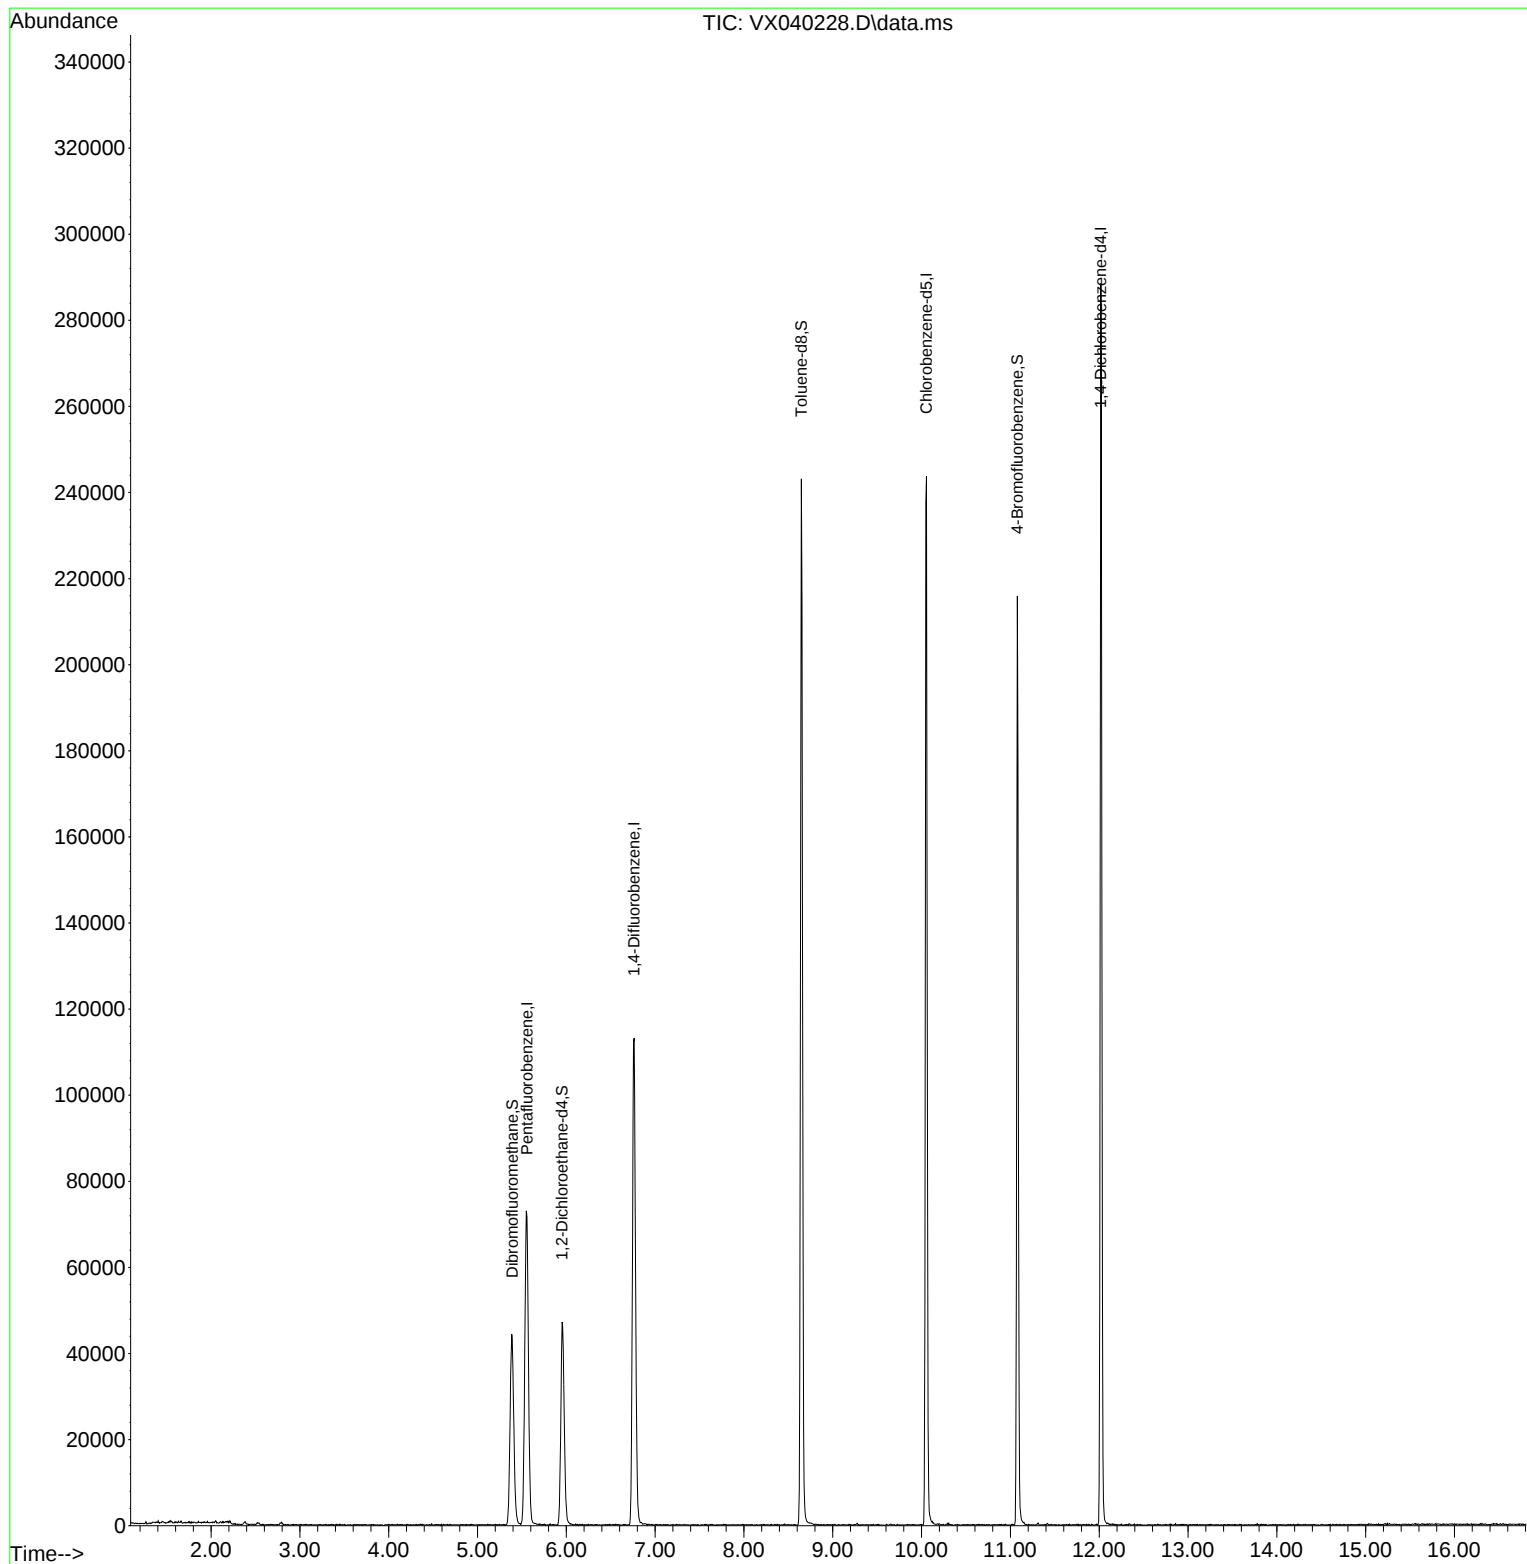


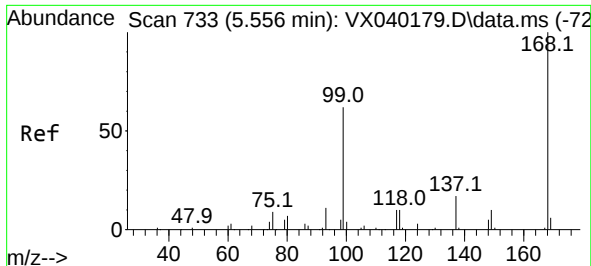

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 713
Delta R.T. 0.006 min
Lab File: VX040228.D
Acq: 14 Feb 2024 18:13




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:168 Resp: 71344
Ion Ratio Lower Upper
168 100
99 52.9 56.6 85.0#

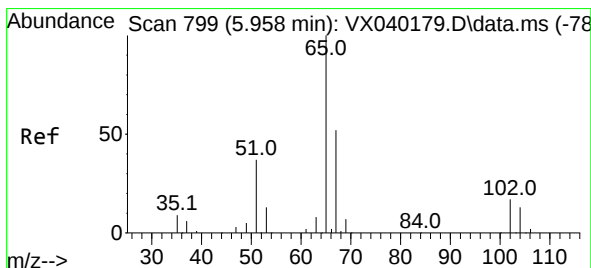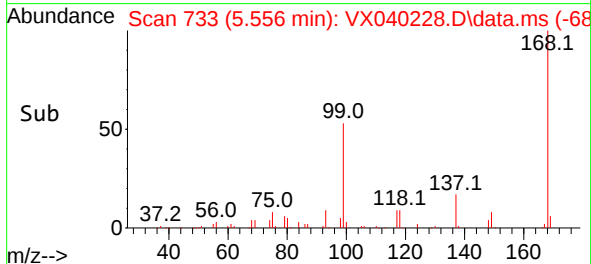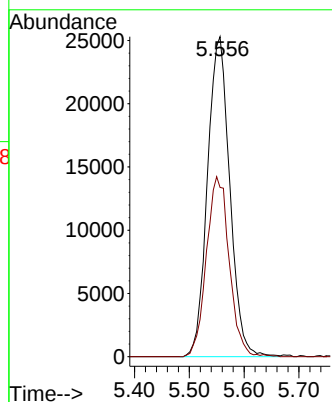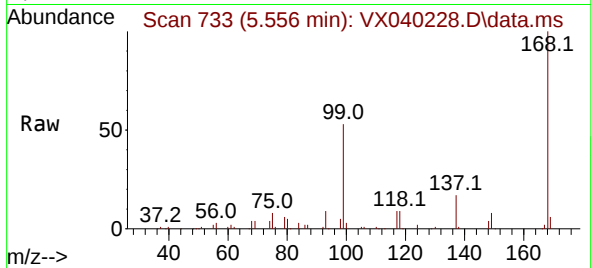

#33
1,2-Dichloroethane-d4
Concen: 42.460 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX040228.D
Acq: 14 Feb 2024 18:13

Tgt Ion: 65 Resp: 45066
Ion Ratio Lower Upper
65 100
67 52.7 0.0 100.2

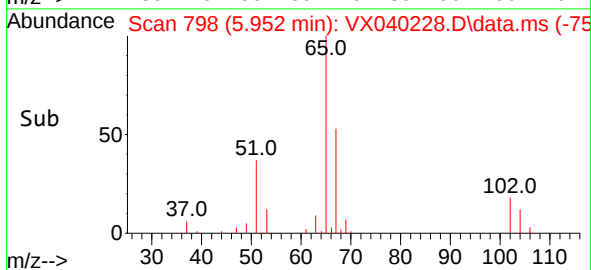
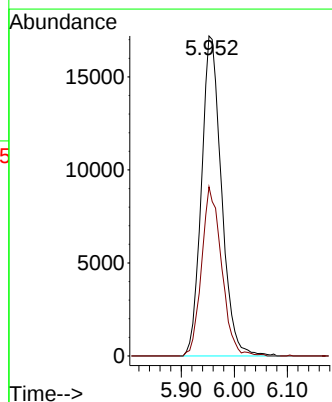
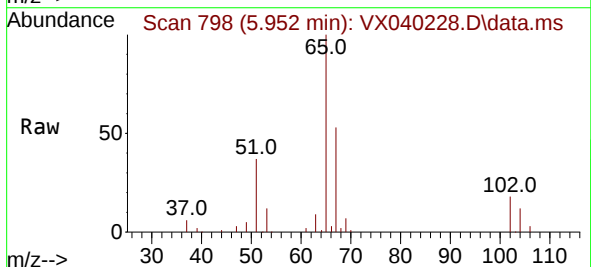


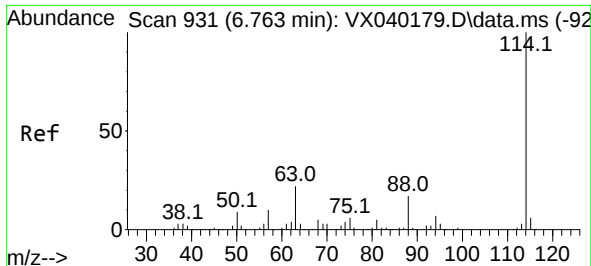

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX040228.D
Acq: 14 Feb 2024 18:13




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:114 Resp: 118782
Ion Ratio Lower Upper
114 100
63 19.7 0.0 45.0
88 15.8 0.0 36.6

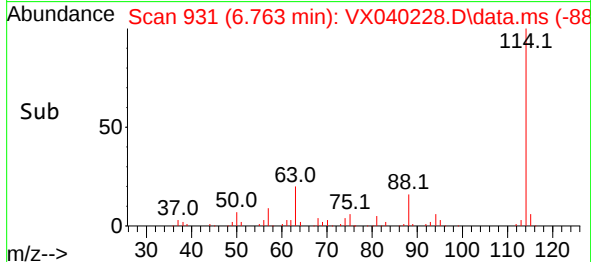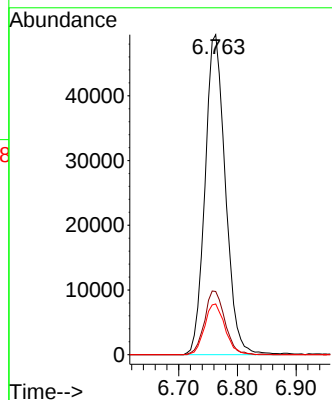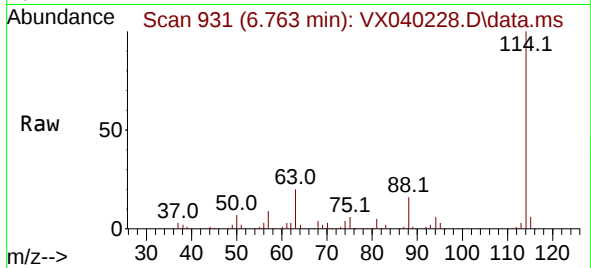

#35
Dibromofluoromethane
Concen: 46.156 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX040228.D
Acq: 14 Feb 2024 18:13

Tgt Ion:113 Resp: 38287
Ion Ratio Lower Upper
113 100
111 102.9 82.9 124.3
192 20.0 13.3 19.9#


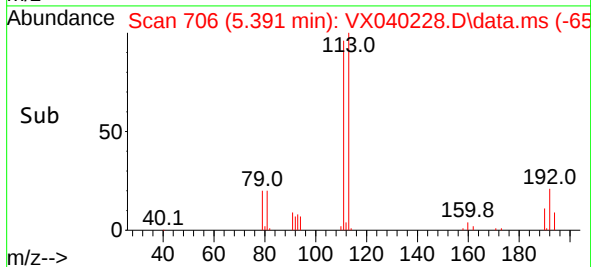
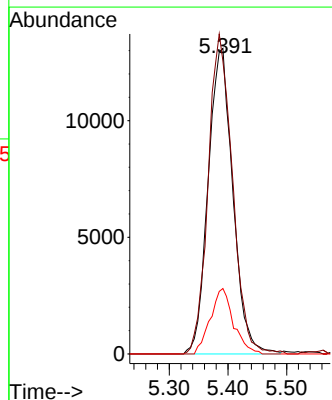
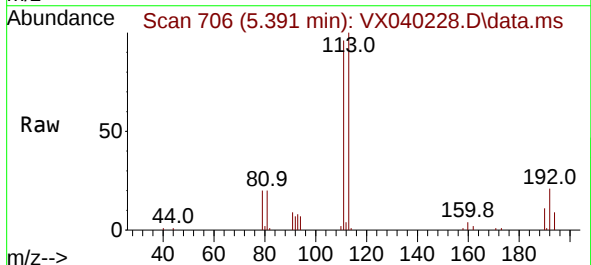


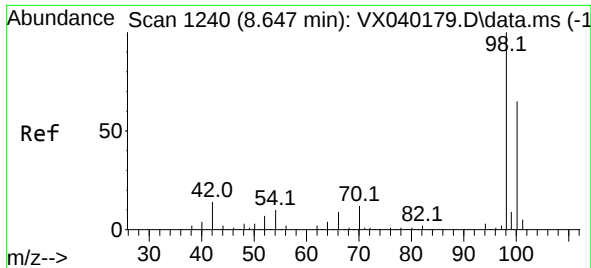

#50
Toluene-d8
Concen: 46.465 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX040228.D
Acq: 14 Feb 2024 18:13




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion: 98 Resp: 144177
Ion Ratio Lower Upper
98 100
100 64.0 53.1 79.7

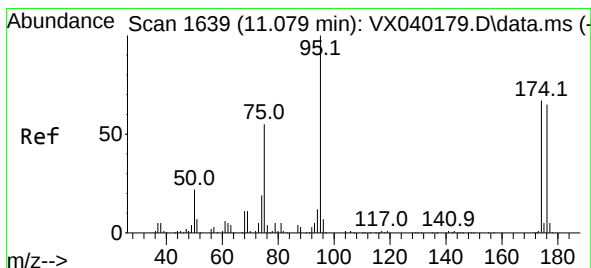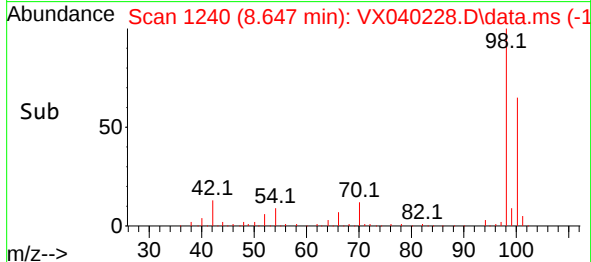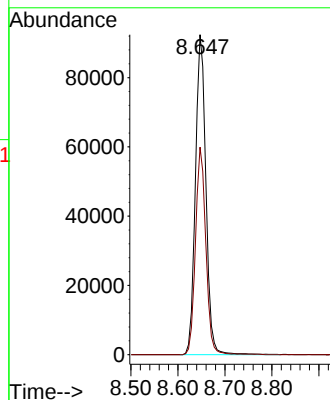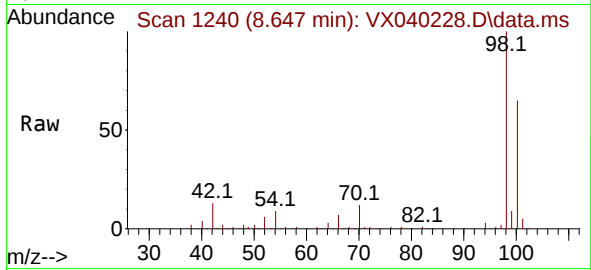

#62
4-Bromofluorobenzene
Concen: 45.183 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX040228.D
Acq: 14 Feb 2024 18:13

Tgt Ion: 95 Resp: 57179
Ion Ratio Lower Upper
95 100
174 77.0 0.0 135.6
176 75.7 0.0 131.0


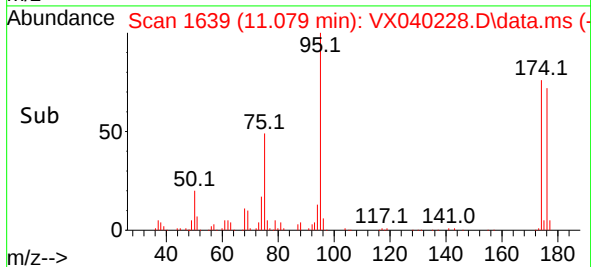
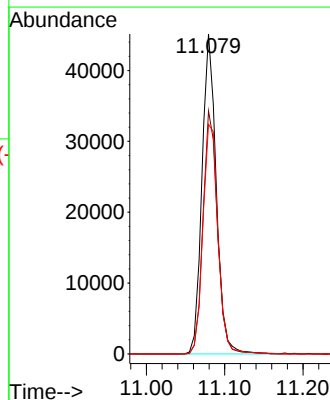
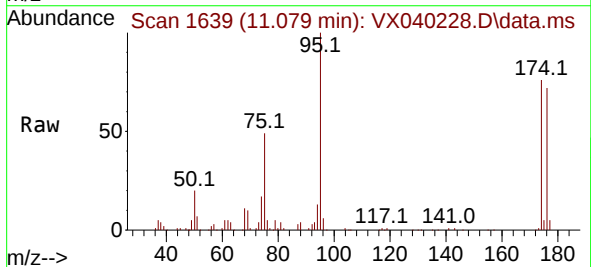


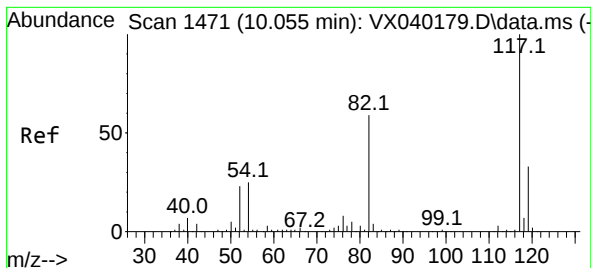

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX040228.D
Acq: 14 Feb 2024 18:13

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Tgt Ion:117 Resp: 115532
Ion Ratio Lower Upper
117 100
82 55.1 46.2 69.4
119 32.8 25.5 38.3

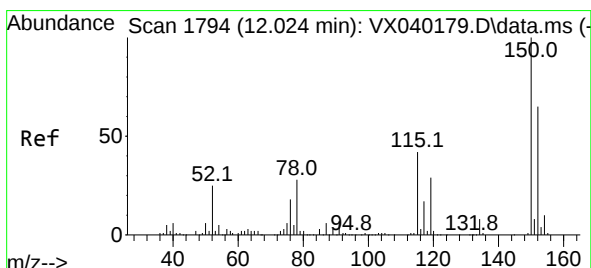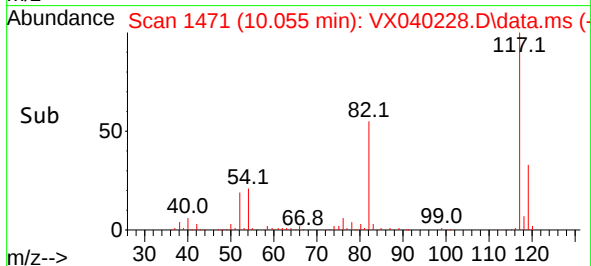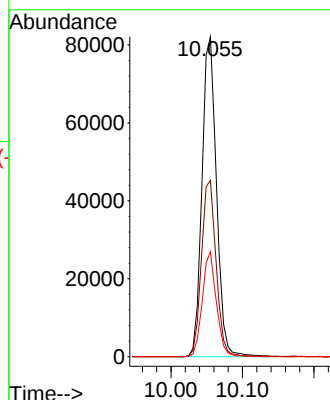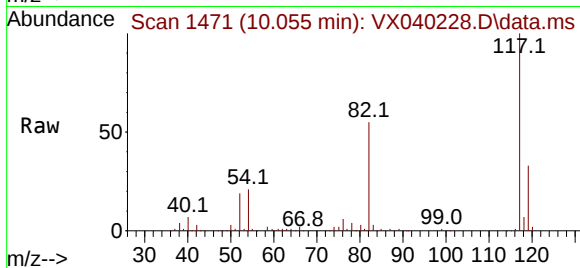

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.006 min
Lab File: VX040228.D
Acq: 14 Feb 2024 18:13

Tgt Ion:152 Resp: 60988
Ion Ratio Lower Upper
152 100
115 57.7 43.3 129.9
150 152.4 0.0 345.0

