


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX021519\
Data File : VX007536.D
Acq On : 14 Feb 2019 10:27
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X020119W.M
Title : SW846 8260
Last Update : Sat Feb 02 01:32:36 2019

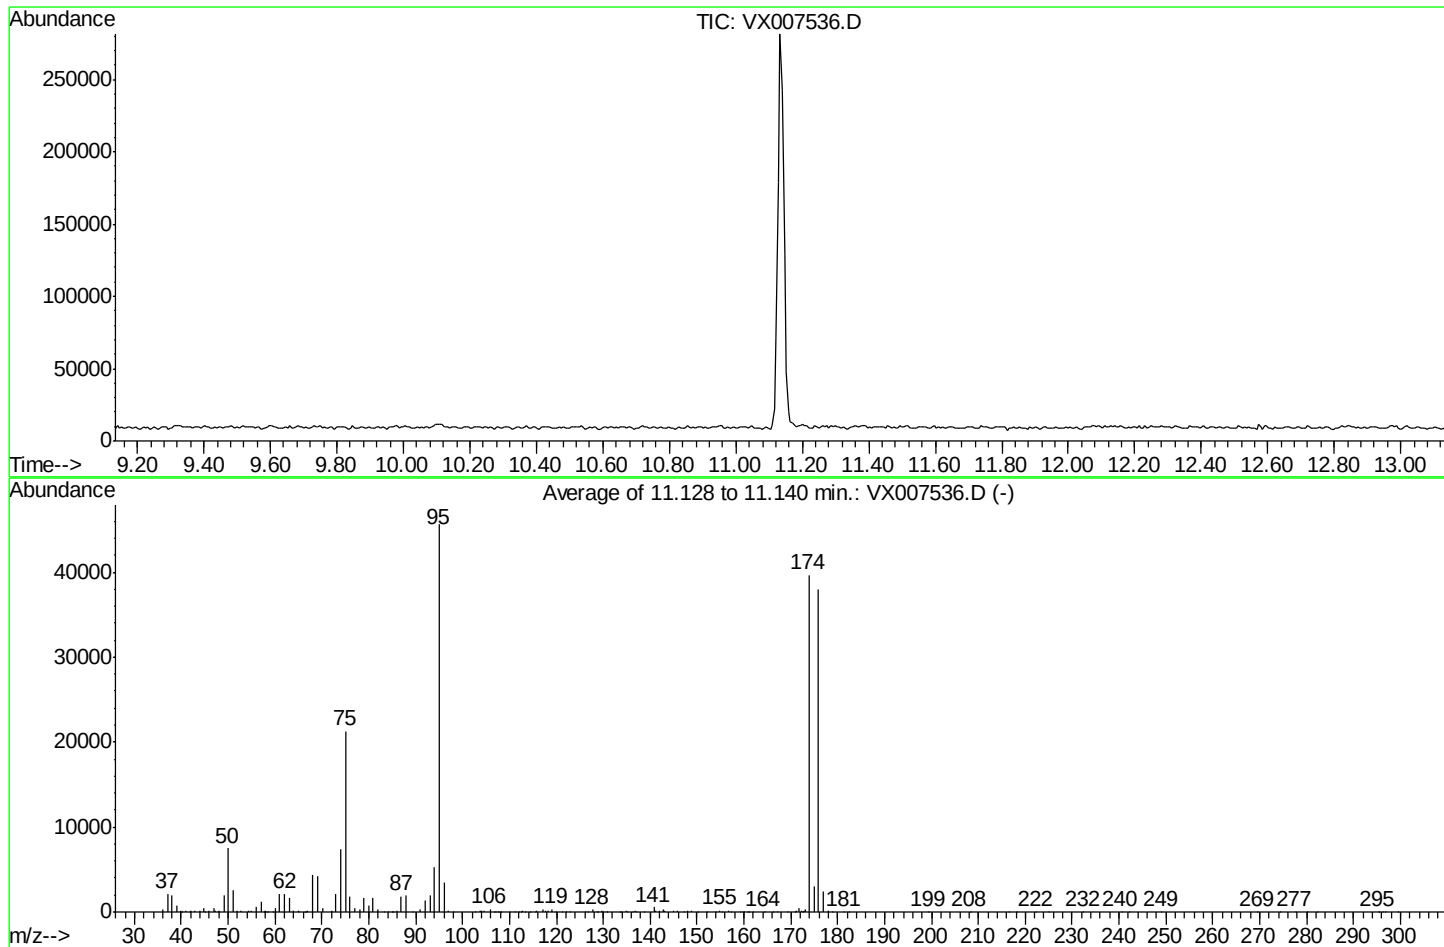

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	7507	PASS
75	95	30	60	46.6	21272	PASS
95	95	100	100	100.0	45632	PASS
96	95	5	9	7.5	3405	PASS
173	174	0.00	2	0.6	236	PASS
174	95	50	100	87.0	39693	PASS
175	174	5	9	7.8	3092	PASS
176	174	95	101	95.8	38008	PASS
177	176	5	9	6.3	2396	PASS