

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021522\
 Data File : VX027025.D
 Acq On : 15 Feb 2022 10:55
 Operator : JC/MD
 Sample : VX0215MBL01
 Misc : 5.00g/5.00mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML021422WMA.M
 Title : VOC Analysis

Signal : TIC: VX027025.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	56	rVB	72061	72836	12.98%	1.746%
2	1.672	92	96	107	rVB	49513	59358	10.58%	1.423%
3	1.989	146	148	150	rBV2	201	146	0.03%	0.003%
4	2.313	194	201	217	rVB	124017	204233	36.41%	4.895%
5	2.441	220	222	228	rVB3	225	215	0.04%	0.005%
6	2.794	278	280	282	rVB	234	204	0.04%	0.005%
7	2.873	292	293	296	rVB	147	134	0.02%	0.003%
8	2.910	296	299	300	rBV	148	153	0.03%	0.004%
9	2.959	305	307	310	rBV2	107	124	0.02%	0.003%
10	3.123	331	334	337	rBV	171	197	0.04%	0.005%
11	3.410	379	381	385	rBV2	125	177	0.03%	0.004%
12	3.672	420	424	425	rBV2	104	129	0.02%	0.003%
13	3.709	428	430	433	rVV2	165	179	0.03%	0.004%
14	3.739	433	435	436	rVB	168	111	0.02%	0.003%
15	3.764	436	439	443	rBV2	165	295	0.05%	0.007%
16	3.855	452	454	456	rBV2	147	184	0.03%	0.004%
17	3.940	465	468	470	rVB2	160	166	0.03%	0.004%
18	4.074	489	490	493	rBV	123	131	0.02%	0.003%
19	4.337	531	533	535	rBV2	106	121	0.02%	0.003%
20	4.459	543	553	567	rBV	37533	112512	20.06%	2.696%
21	4.733	594	598	599	rBV2	154	159	0.03%	0.004%
22	4.824	612	613	618	rBV2	141	161	0.03%	0.004%
23	5.062	639	652	669	rVB	73667	223863	39.91%	5.365%
24	5.269	682	686	691	rBV2	122	232	0.04%	0.006%
25	5.343	695	698	700	rBV	92	119	0.02%	0.003%
26	5.446	713	715	718	rVB	122	104	0.02%	0.002%
27	5.733	760	762	764	rBV	152	148	0.03%	0.004%
28	5.849	779	781	785	rBV2	158	236	0.04%	0.006%
29	5.970	789	801	816	rBV2	185272	560970	100.00%	13.444%
30	6.117	823	825	826	rBV2	136	133	0.02%	0.003%
31	6.208	838	840	843	rBV	134	140	0.02%	0.003%
32	6.294	852	854	857	rBV	109	141	0.03%	0.003%
33	6.422	873	875	878	rBV	137	166	0.03%	0.004%
34	6.562	896	898	901	rBV2	136	125	0.02%	0.003%
35	6.617	905	907	909	rVB	141	116	0.02%	0.003%
36	6.641	909	911	913	rBV	106	116	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021522\
 Data File : VX027025.D
 Acq On : 15 Feb 2022 10:55
 Operator : JC/MD
 Sample : VX0215MBL01
 Misc : 5.00g/5.00mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML021422WMA.M
 Title : VOC Analysis

37	6.763	920	931	945	rBV	138459	331354	59.07%	7.941%
38	7.062	977	980	981	rVV	135	143	0.03%	0.003%
39	7.110	981	988	996	rVB2	6803	14886	2.65%	0.357%
40	7.171	996	998	999	rBV	110	107	0.02%	0.003%
41	7.208	1002	1004	1006	rBV	107	121	0.02%	0.003%
42	7.306	1011	1020	1033	rBV	113316	248331	44.27%	5.951%
43	7.482	1046	1049	1053	rBV	266	399	0.07%	0.010%
44	7.623	1068	1072	1073	rBV	102	127	0.02%	0.003%
45	7.799	1097	1101	1102	rBV	212	261	0.05%	0.006%
46	7.873	1112	1113	1116	rBV2	121	134	0.02%	0.003%
47	7.927	1119	1122	1129	rVB2	570	812	0.14%	0.019%
48	8.007	1134	1135	1137	rBV	125	105	0.02%	0.003%
49	8.074	1142	1146	1148	rBV2	129	219	0.04%	0.005%
50	8.141	1155	1157	1161	rBV2	91	133	0.02%	0.003%
51	8.324	1181	1187	1199	rBV	72796	119960	21.38%	2.875%
52	8.470	1208	1211	1218	rVB3	317	582	0.10%	0.014%
53	8.525	1218	1220	1221	rBV2	123	103	0.02%	0.002%
54	8.647	1233	1240	1248	rBV	295247	454508	81.02%	10.893%
55	8.720	1248	1252	1265	rVB	3718	6398	1.14%	0.153%
56	8.952	1284	1290	1300	rVV	52496	74705	13.32%	1.790%
57	9.384	1355	1361	1380	rBV	177774	262943	46.87%	6.302%
58	9.677	1407	1409	1411	rBV2	90	107	0.02%	0.003%
59	9.811	1428	1431	1432	rBV2	118	147	0.03%	0.004%
60	9.927	1448	1450	1451	rBV	182	152	0.03%	0.004%
61	10.055	1465	1471	1485	rBV	293049	397386	70.84%	9.524%
62	10.195	1491	1494	1499	rVB2	223	371	0.07%	0.009%
63	10.268	1504	1506	1508	rBV	136	163	0.03%	0.004%
64	10.305	1508	1512	1517	rVB2	511	734	0.13%	0.018%
65	10.348	1517	1519	1522	rBV2	99	117	0.02%	0.003%
66	10.598	1556	1560	1561	rBV2	98	128	0.02%	0.003%
67	10.707	1574	1578	1579	rBV2	79	116	0.02%	0.003%
68	10.854	1600	1602	1603	rVB	199	114	0.02%	0.003%
69	10.878	1603	1606	1609	rBV	123	195	0.03%	0.005%
70	10.963	1618	1620	1622	rBV	189	187	0.03%	0.004%
71	11.067	1635	1637	1642	rBB	94	126	0.02%	0.003%
72	11.122	1642	1646	1651	rVB3	1559	2023	0.36%	0.048%
73	11.195	1652	1658	1666	rVV	173180	233429	41.61%	5.594%
74	11.329	1678	1680	1681	rBV2	162	118	0.02%	0.003%
75	11.457	1698	1701	1702	rVB2	160	174	0.03%	0.004%
76	11.482	1702	1705	1708	rBV3	471	706	0.13%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021522\
 Data File : VX027025.D
 Acq On : 15 Feb 2022 10:55
 Operator : JC/MD
 Sample : VX0215MBL01
 Misc : 5.00g/5.00mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML021422WMA.M
 Title : VOC Analysis

77	11.549	1713	1716	1718	rBV2	183	173	0.03%	0.004%
78	11.665	1731	1735	1738	rBV	142	205	0.04%	0.005%
79	11.750	1745	1749	1754	rVB2	1256	1492	0.27%	0.036%
80	11.835	1761	1763	1766	rBV2	274	284	0.05%	0.007%
81	11.933	1776	1779	1783	rBV	795	730	0.13%	0.017%
82	12.024	1788	1794	1805	rVV	317640	393546	70.15%	9.432%
83	12.128	1808	1811	1812	rVV	776	928	0.17%	0.022%
84	12.146	1812	1814	1820	rVV	1218	1387	0.25%	0.033%
85	12.323	1837	1843	1853	rVV	289623	379643	67.68%	9.098%
86	12.433	1857	1861	1862	rBV3	325	378	0.07%	0.009%
87	12.488	1868	1870	1873	rBV2	202	195	0.03%	0.005%
88	13.628	2055	2057	2061	rBV2	85	109	0.02%	0.003%
89	13.780	2079	2082	2087	rVB2	215	359	0.06%	0.009%
90	13.963	2111	2112	2115	rVV2	238	189	0.03%	0.005%
91	14.006	2118	2119	2122	rBV2	136	139	0.02%	0.003%
92	14.128	2137	2139	2142	rBV	156	184	0.03%	0.004%
93	14.554	2204	2209	2211	rBV	133	187	0.03%	0.004%
94	14.652	2224	2225	2230	rVB	155	149	0.03%	0.004%
95	14.743	2238	2240	2242	rBV	163	159	0.03%	0.004%
96	14.768	2242	2244	2247	rBV	148	213	0.04%	0.005%
97	14.883	2261	2263	2265	rBV2	156	143	0.03%	0.003%
98	15.359	2339	2341	2343	rBV	181	136	0.02%	0.003%
99	15.816	2414	2416	2419	rBV2	149	201	0.04%	0.005%
100	16.182	2474	2476	2479	rBV2	129	137	0.02%	0.003%




Sum of corrected areas: 4172624

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021522\
Data File : VX027025.D
Acq On : 15 Feb 2022 10:55
Operator : JC/MD
Sample : VX0215MBL01
Misc : 5.00g/5.00mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK655

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML021422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

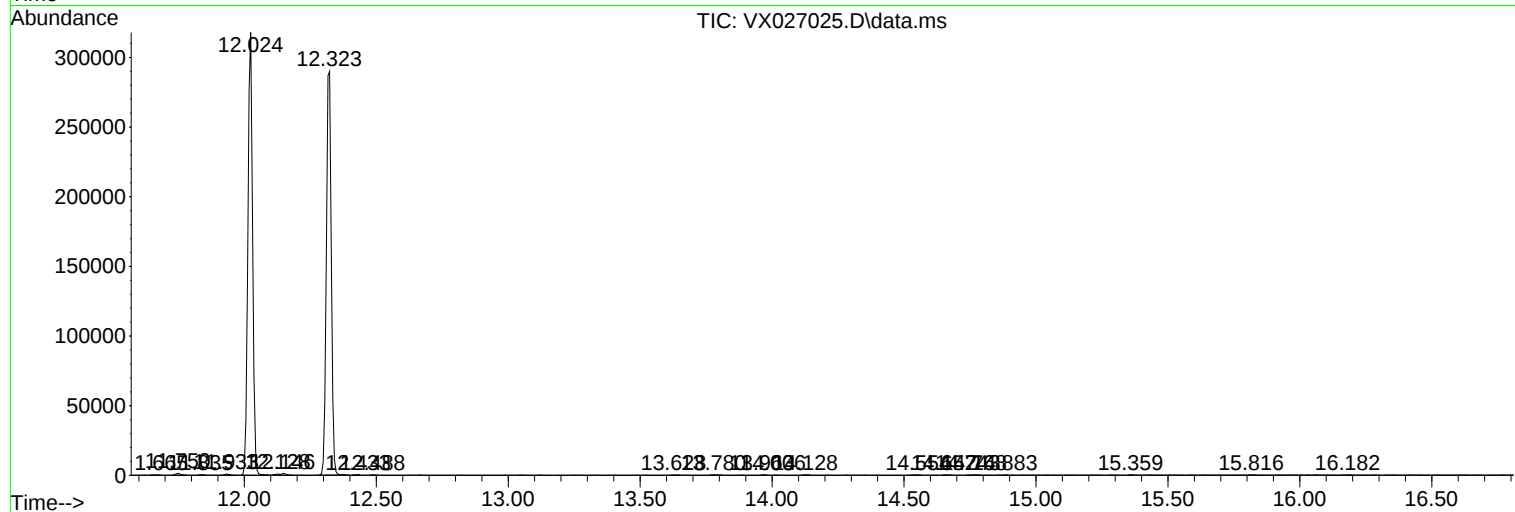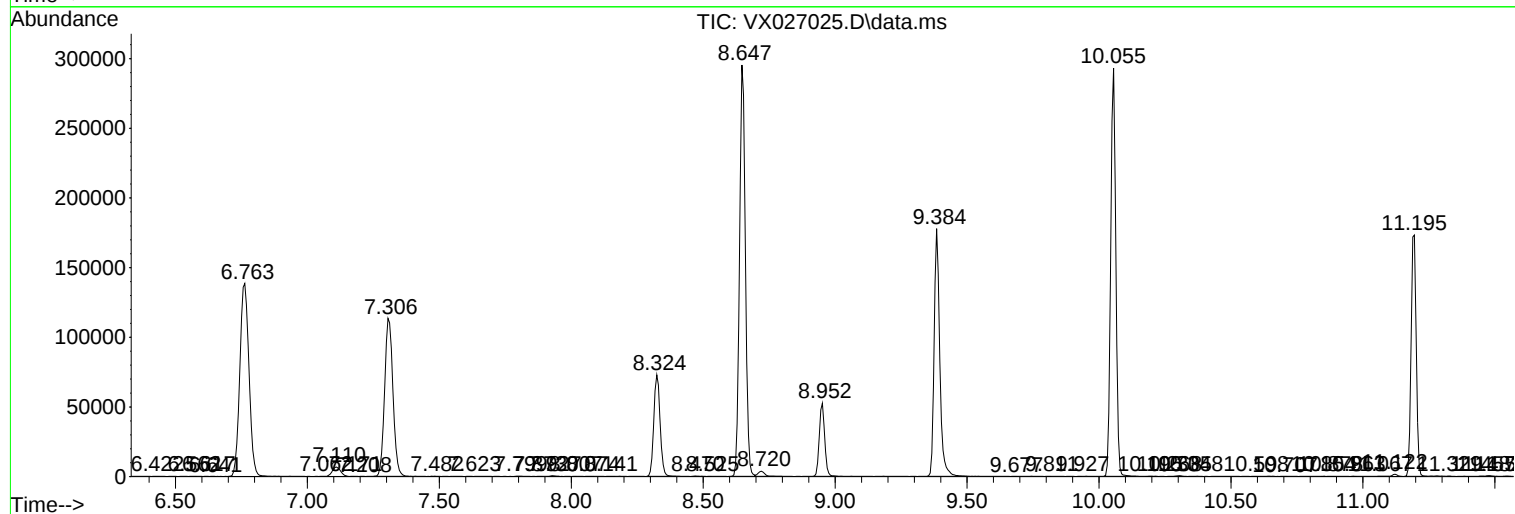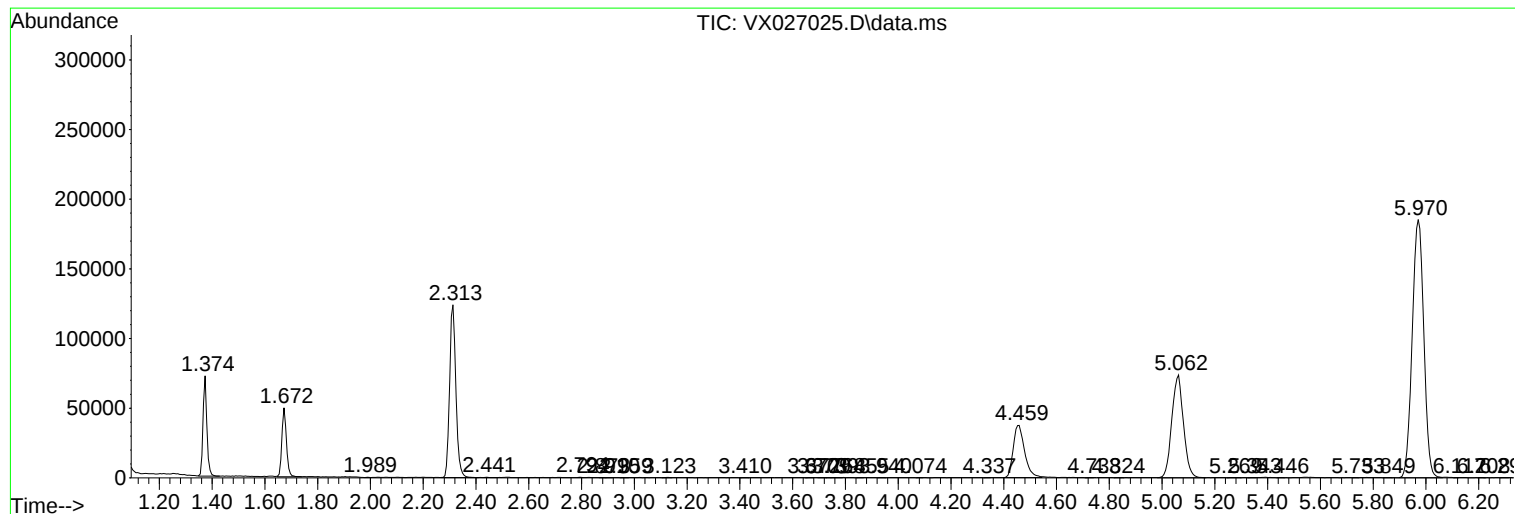

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021522\
Data File : VX027025.D
Acq On : 15 Feb 2022 10:55
Operator : JC/MD
Sample : VX0215MBL01
Misc : 5.00g/5.00mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK655

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML021422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021522\
Data File : VX027025.D
Acq On : 15 Feb 2022 10:55
Operator : JC/MD
Sample : VX0215MBL01
Misc : 5.00g/5.00mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK655

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML021422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
