
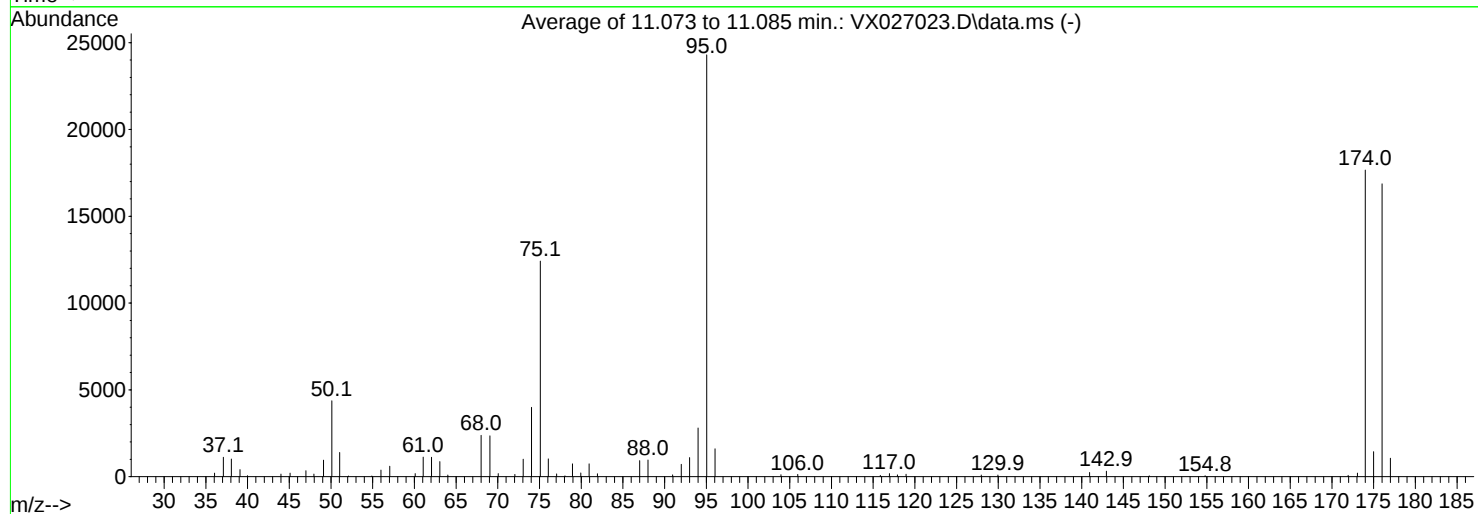


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021522\
Data File : VX027023.D
Acq On : 15 Feb 2022 09:18
Operator :
Sample : BFB635
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB635

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM021422WMA.M
Title : VOC Analysis
Last Update : Wed Feb 16 01:34:21 2022

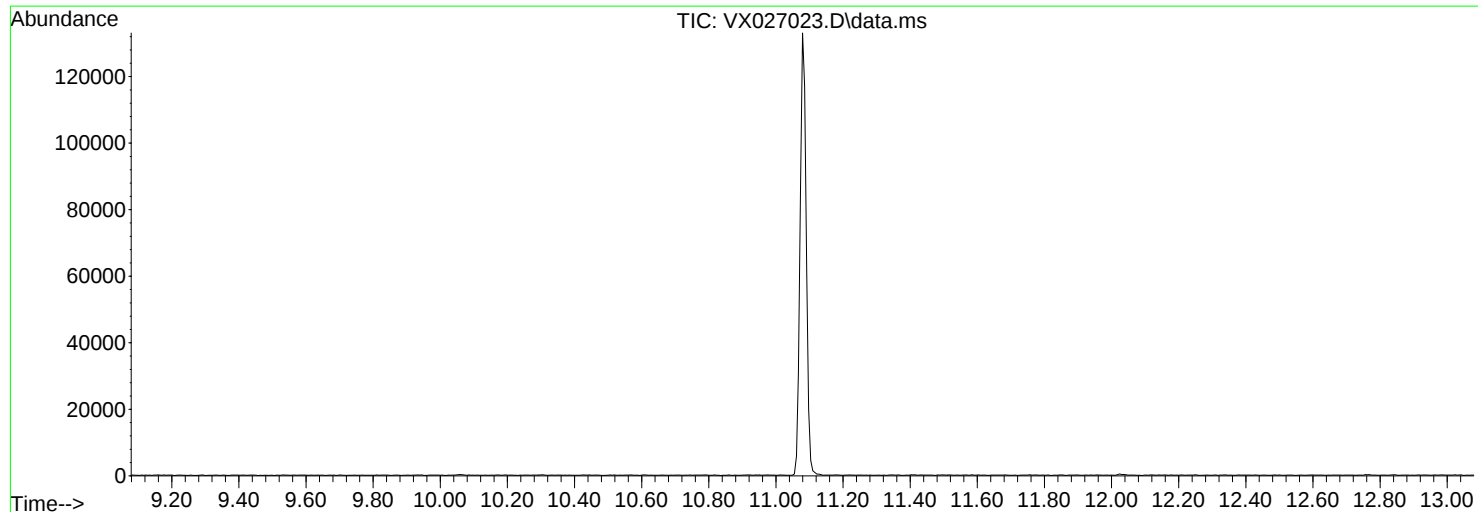

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	4365	PASS
75	95	30	80	51.1	12416	PASS
95	95	100	100	100.0	24299	PASS
96	95	5	9	6.6	1604	PASS
173	174	0.00	2	1.1	202	PASS
174	95	50	120	72.7	17657	PASS
175	174	5	9	8.1	1434	PASS
176	174	95	101	95.5	16865	PASS
177	176	5	9	6.3	1060	PASS

m/z	Abundance
40.00	127.0
44.10	64.0

Instrument :
MSVOA_X
ClientSampleId :
BFB635

m/z	Abundance
36.10	165.0
37.10	988.0
38.00	935.0
39.10	378.0
40.00	198.0
44.10	171.0
45.10	120.0
47.00	244.0
47.90	87.0
49.10	839.0
50.10	3903.0
51.00	1290.0
52.20	57.0
56.00	321.0
57.00	483.0
60.20	163.0
61.10	929.0
62.10	973.0
63.00	786.0
64.00	123.0
68.00	1856.0
69.10	2019.0
70.10	116.0
72.00	94.0
73.00	740.0
74.00	3050.0
75.10	10195.0
76.00	887.0
77.20	125.0
78.10	73.0
79.00	694.0
80.00	162.0
81.00	663.0
81.90	117.0
87.00	760.0
88.00	758.0
91.00	62.0
92.00	538.0
93.00	995.0
94.00	2288.0
95.00	18752.0
96.00	1462.0
104.00	86.0
106.00	81.0
115.80	85.0
117.00	139.0
117.90	61.0
119.00	90.0
127.90	60.0
129.90	75.0
141.00	174.0
142.90	221.0
173.10	96.0
174.00	11828.0
175.00	965.0
176.00	11092.0
177.00	835.0

Instrument :
MSVOA_X
ClientSampleId :
BFB635

m/z	Abundance
36.00	274.0
37.10	1341.0
38.10	1195.0
39.10	492.0
40.00	182.0
44.00	247.0
45.10	283.0
47.00	488.0
47.90	182.0
49.10	1086.0
50.10	5030.0
51.10	1577.0
52.00	59.0
54.90	52.0
56.00	410.0
57.00	681.0
60.00	194.0
61.00	1367.0
62.00	1361.0
63.10	1003.0
63.90	67.0
68.00	2908.0
69.00	2875.0
70.00	232.0
72.10	138.0
73.10	1256.0
74.10	4835.0
75.10	15221.0
76.10	1113.0
77.00	172.0
78.00	56.0
79.00	869.0
79.90	271.0
81.00	858.0
81.90	223.0
87.00	1100.0
88.00	1148.0
91.00	94.0
92.00	847.0
93.00	1292.0
94.00	3311.0
95.00	29256.0
96.00	1886.0
103.90	135.0
106.00	175.0
115.90	142.0
116.90	212.0
117.90	110.0
118.90	154.0
127.90	123.0
130.00	120.0
140.90	292.0
143.00	366.0
148.10	80.0
154.80	55.0
171.90	88.0
173.00	240.0
174.00	20584.0
175.00	1555.0
176.00	19928.0
177.00	1200.0

Instrument :
MSVOA_X
ClientSampleId :
BFB635

m/z	Abundance
36.10	169.0
37.10	1005.0
38.10	922.0
39.10	352.0
40.10	181.0
43.90	212.0
45.10	219.0
47.00	279.0
48.00	181.0
49.10	924.0
50.10	4162.0
51.10	1305.0
54.90	52.0
56.00	399.0
57.10	640.0
60.10	160.0
61.00	1085.0
62.00	998.0
63.00	820.0
64.10	87.0
68.00	2380.0
69.00	2162.0
70.00	181.0
72.00	155.0
73.00	1015.0
74.10	4087.0
75.10	11833.0
76.00	1083.0
77.00	176.0
78.90	659.0
80.00	190.0
80.90	691.0
82.00	157.0
87.00	902.0
88.00	975.0
90.90	140.0
92.00	751.0
93.00	994.0
94.00	2799.0
95.10	24888.0
96.10	1465.0
104.00	116.0
105.90	120.0
116.90	171.0
117.90	123.0
118.90	171.0
128.00	87.0
130.00	78.0
141.00	266.0
142.90	342.0
148.10	54.0
154.80	101.0
172.00	125.0
173.10	271.0
174.00	20560.0
175.00	1782.0
176.00	19576.0
177.00	1145.0

Instrument :
MSVOA_X
ClientSampleId :
BFB635