

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021622\
 Data File : VX027051.D
 Acq On : 16 Feb 2022 15:53
 Operator : JC/MD
 Sample : N1575-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COP-1R

Quant Time: Feb 17 07:12:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 08 07:07:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	110619	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	184093	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	171432	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	77159	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	68792	51.806	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 103.620%			
35) Dibromofluoromethane	5.391	113	56905	51.883	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 103.760%			
50) Toluene-d8	8.653	98	216372	53.744	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 107.480%			
62) 4-Bromofluorobenzene	11.079	95	83169	58.676	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 117.360%			
Target Compounds						Qvalue
5) Bromomethane	1.617	94	209	0.420	ug/l	100
10) Methyl Iodide	2.465	142	448	2.527	ug/l #	88
11) Tert butyl alcohol	2.952	59	334	1.392	ug/l #	75
13) Acrolein	2.221	56	137	0.618	ug/l #	1
16) Acetone	2.379	43	10640	18.244	ug/l #	89
18) Methyl Acetate	2.702	43	555	0.331	ug/l #	53
25) 2-Butanone	4.568	43	1425	1.517	ug/l	94
29) Tetrahydrofuran	5.019	42	238	0.373	ug/l #	34
31) Cyclohexane	5.482	56	1110	0.526	ug/l	99
36) 1,1-Dichloropropene	5.556	75	8207	4.743	ug/l #	51
37) Ethyl Acetate	4.720	43	19988	10.165	ug/l	98
38) Carbon Tetrachloride	5.562	117	11071	6.102	ug/l #	16
39) Methylcyclohexane	7.378	83	620	0.292	ug/l	85
40) Benzene	6.043	78	5395	1.070	ug/l	94
52) Toluene	8.720	92	22886	7.168	ug/l	98
53) t-1,3-Dichloropropene	8.720	75	253	1.484	ug/l #	1
59) 2-Hexanone	9.445	43	383	0.286	ug/l	86
67) Ethyl Benzene	10.195	91	11019	1.756	ug/l	96
68) m/p-Xylenes	10.305	106	18542	7.680	ug/l	98
69) o-Xylene	10.646	106	16487	6.969	ug/l	99
70) Styrene	10.652	104	1369	0.357	ug/l #	1
73) Isopropylbenzene	10.963	105	1280	0.211	ug/l	92
76) 1,2,3-Trichloropropane	11.079	75	40852	24.186	ug/l #	40
78) n-propylbenzene	11.305	91	1604	0.238	ug/l	100
79) 2-Chlorotoluene	11.378	91	2318	0.557	ug/l #	44
80) 1,3,5-Trimethylbenzene	11.451	105	14420	2.883	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.079	75	40852	73.885	ug/l #	3
82) 4-Chlorotoluene	11.451	91	1797	0.385	ug/l #	46
84) 1,2,4-Trimethylbenzene	11.750	105	15408	3.054	ug/l	100
85) sec-Butylbenzene	11.750	105	15408	2.550	ug/l #	56
86) p-Isopropyltoluene	12.012	119	1188	0.232	ug/l	79
89) n-Butylbenzene	12.317	91	1036	0.247	ug/l #	19
95) Naphthalene	13.780	128	9411	1.667	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
COP-1R

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021622\
Data File : VX027051.D
Acq On : 16 Feb 2022 15:53
Operator : JC/MD
Sample : N1575-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COP-1R

Quant Time: Feb 17 07:12:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 08 07:07:46 2022
Response via : Initial Calibration




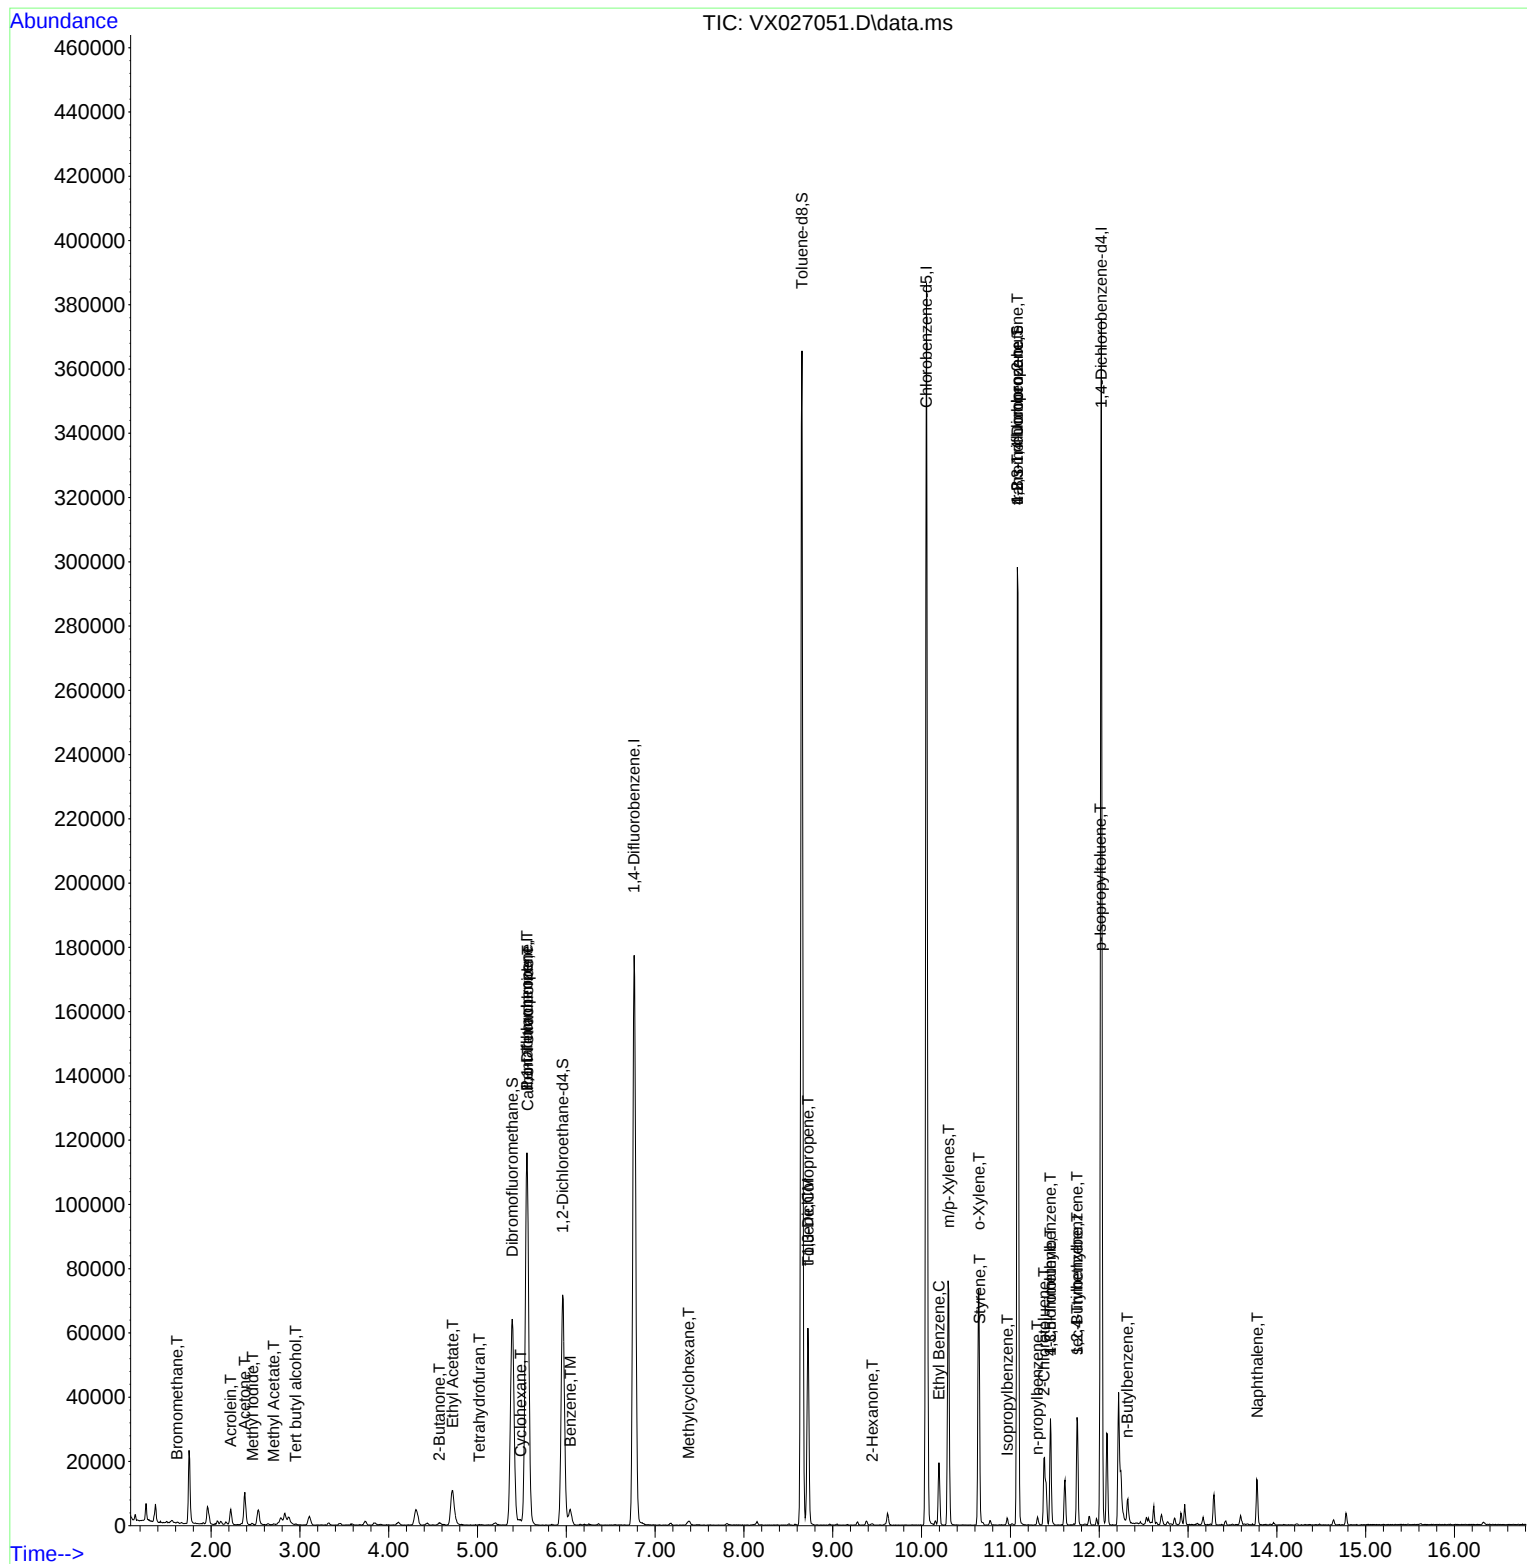




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53




Instrument :
MSVOA_X
ClientSampleId :
COP-1R


Tgt Ion:168 Resp: 110619
Ion Ratio Lower Upper
168 100
99 58.7 50.3 75.5

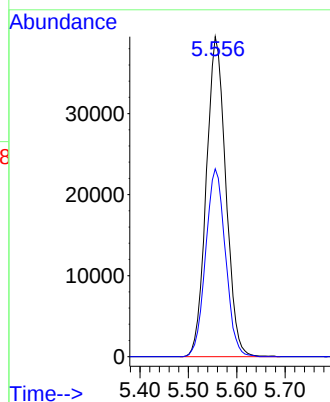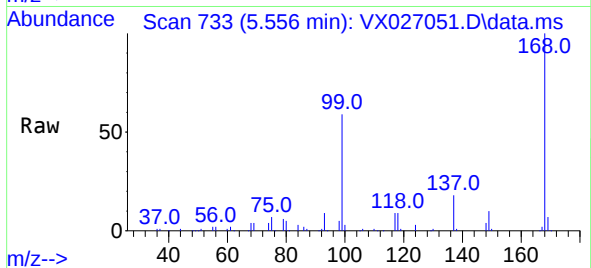

#5
Bromomethane
Concen: 0.420 ug/l
RT: 1.617 min Scan# 87
Delta R.T. 0.006 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53

Tgt Ion: 94 Resp: 209
Ion Ratio Lower Upper
94 100
96 95.2 75.9 113.9


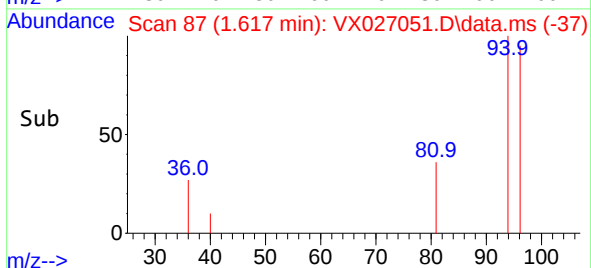






#10
Methyl Iodide
Concen: 2.527 ug/l
RT: 2.465 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53




Instrument :
MSVOA_X
ClientSampleId :
COP-1R


Tgt Ion:142 Resp: 448
Ion Ratio Lower Upper
142 100
127 43.8 38.1 57.1
141 0.0 11.2 16.8#

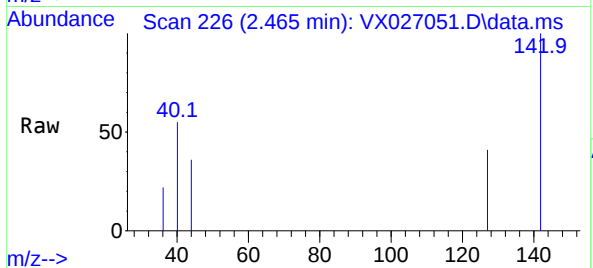

#11
Tert butyl alcohol
Concen: 1.392 ug/l
RT: 2.952 min Scan# 306
Delta R.T. -0.049 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53

Tgt Ion: 59 Resp: 334
Ion Ratio Lower Upper
59 100
57 0.0 7.2 10.8#


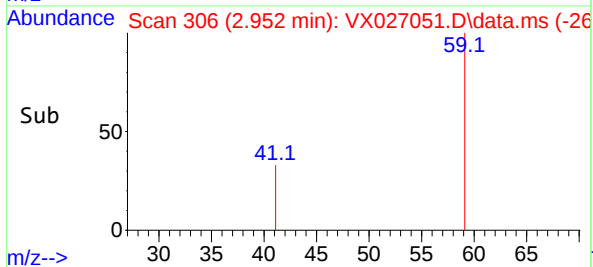

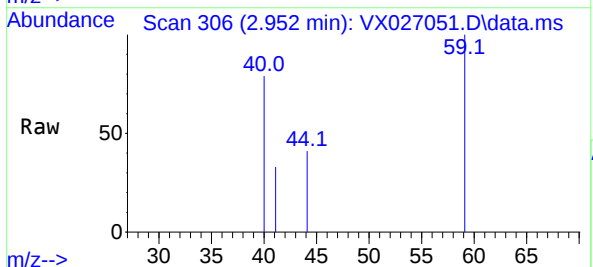




#13
Acrolein
Concen: 0.618 ug/l
RT: 2.221 min Scan# 11
Delta R.T. -0.018 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53




Instrument :
MSVOA_X
ClientSampleId :
COP-1R


Tgt Ion: 56 Resp: 137
Ion Ratio Lower Upper
56 100
55 1859.9 56.9 85.3#



#16
Acetone
Concen: 18.244 ug/l
RT: 2.379 min Scan# 212
Delta R.T. -0.006 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53

Tgt Ion: 43 Resp: 10640
Ion Ratio Lower Upper
43 100
58 34.7 23.0 34.6#

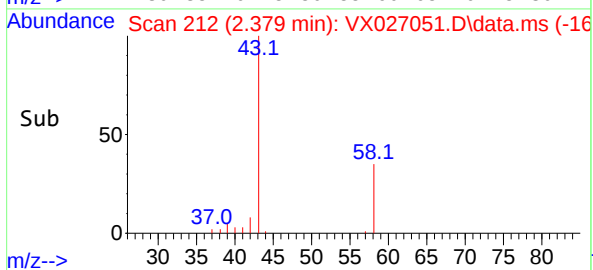



#18

Methyl Acetate

Concen: 0.331 ug/l

RT: 2.702 min Scan# 2

Delta R.T. -0.006 min

Lab File: VX027051.D

Acq: 16 Feb 2022 15:53

Instrument :

MSVOA_X

ClientSampleId :





COP-1R

Tgt Ion: 43 Resp: 555

Ion Ratio Lower Upper

43 100

74 0.0 18.3 27.5#

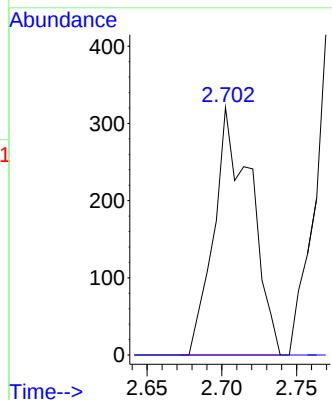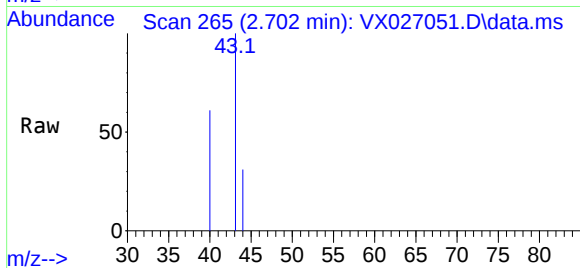

#25

2-Butanone

Concen: 1.517 ug/l

RT: 4.568 min Scan# 571

Delta R.T. 0.006 min

Lab File: VX027051.D




Acq: 16 Feb 2022 15:53


Tgt Ion: 43 Resp: 1425

Ion Ratio Lower Upper

43 100

72 28.3 20.4 30.6

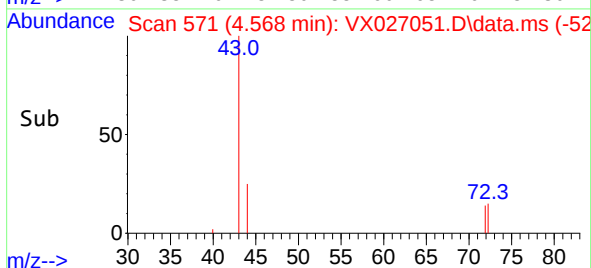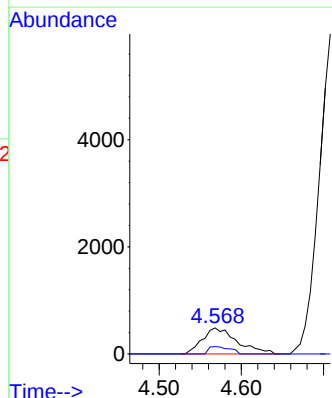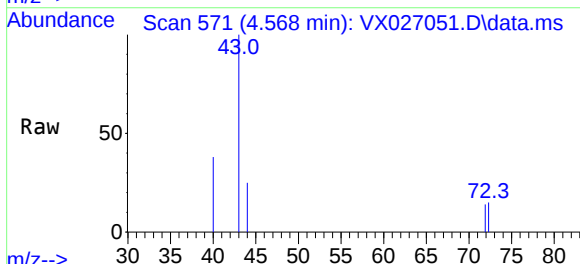



#29

Tetrahydrofuran

Concen: 0.373 ug/l

RT: 5.019 min Scan# 64

Delta R.T. 0.012 min

Lab File: VX027051.D

Acq: 16 Feb 2022 15:53

Instrument :

MSVOA_X

ClientSampleId :

COP-1R





Tgt Ion: 42 Resp: 238

Ion Ratio Lower Upper

42 100

72 0.0 34.6 52.0#

71 0.0 31.8 47.8#

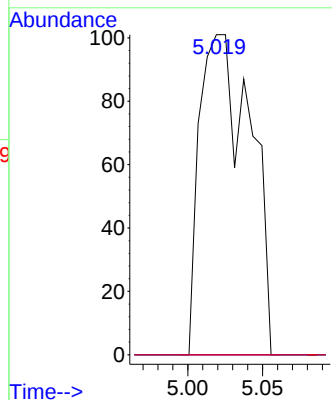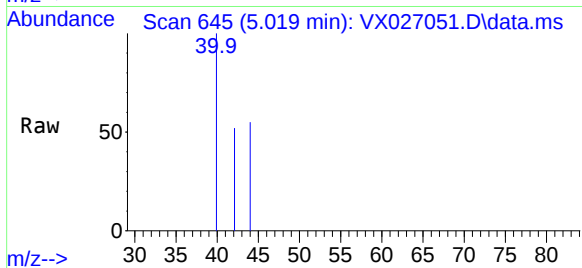

#31

Cyclohexane

Concen: 0.526 ug/l

RT: 5.482 min Scan# 721

Delta R.T. 0.006 min

Lab File: VX027051.D

Acq: 16 Feb 2022 15:53




Tgt Ion: 56 Resp: 1110


Ion Ratio Lower Upper

56 100

69 31.8 25.8 38.6

84 87.1 68.9 103.3

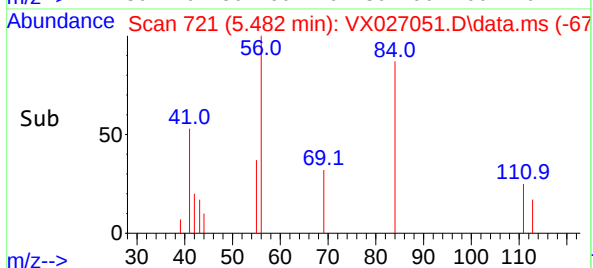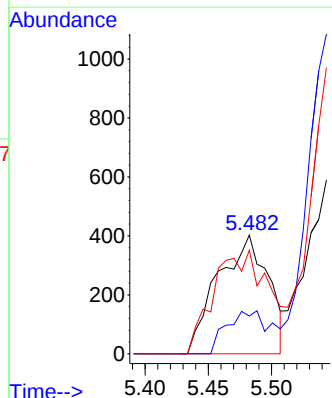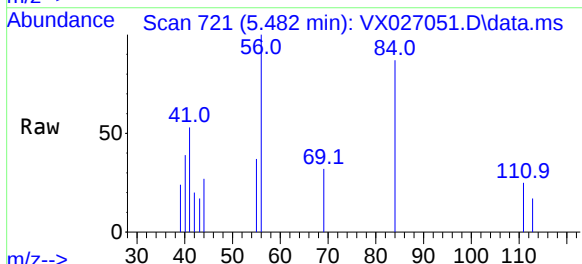



#33

1,2-Dichloroethane-d4

Concen: 51.806 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX027051.D

Acq: 16 Feb 2022 15:53

Instrument :

MSVOA_X

ClientSampleId :





COP-1R

Tgt Ion: 65 Resp: 68792

Ion Ratio Lower Upper

65 100

67 52.0 0.0 100.8

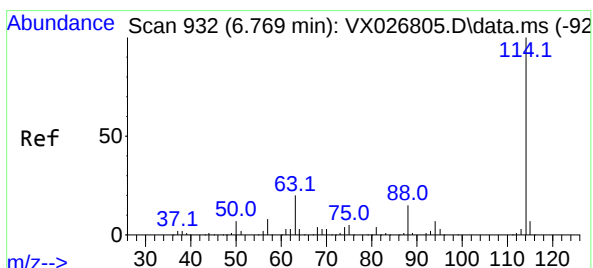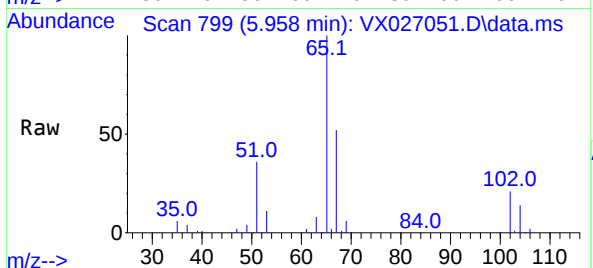

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.006 min

Lab File: VX027051.D

Acq: 16 Feb 2022 15:53




Tgt Ion: 114 Resp: 184093


Ion Ratio Lower Upper

114 100

63 20.2 0.0 42.8

88 16.3 0.0 33.0


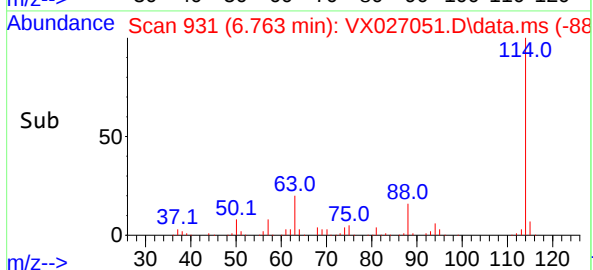




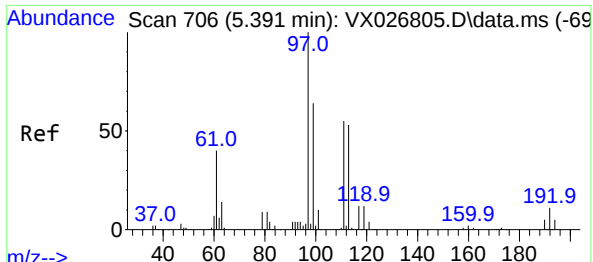

#35
Dibromofluoromethane
Concen: 51.883 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.000 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53




Instrument :
MSVOA_X
ClientSampleId :
COP-1R


Tgt Ion:113 Resp: 56905
Ion Ratio Lower Upper
113 100
111 102.2 81.2 121.8
192 20.0 15.0 22.4

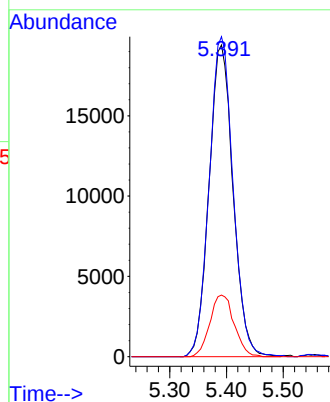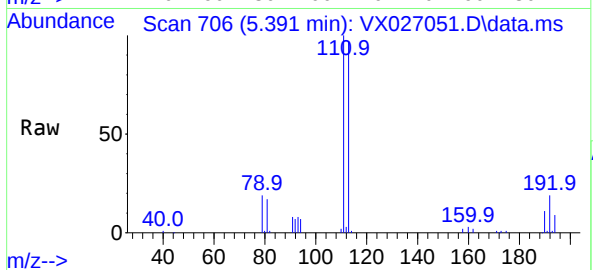

#36
1,1-Dichloropropene
Concen: 4.743 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.140 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53

Tgt Ion: 75 Resp: 8207
Ion Ratio Lower Upper
75 100
110 10.3 17.2 51.6#
77 0.0 24.6 36.8#

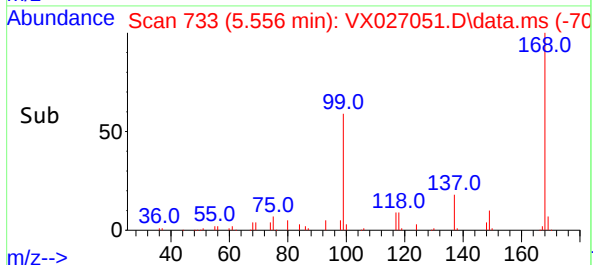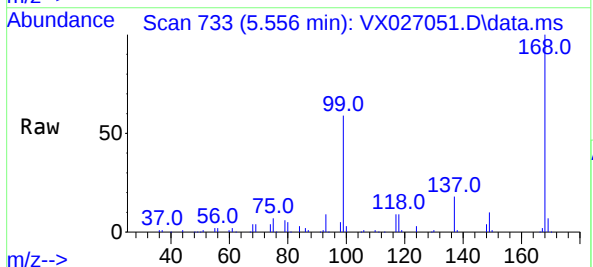



#37

Ethyl Acetate

Concen: 10.165 ug/l

RT: 4.720 min Scan# 596

Delta R.T. 0.006 min

Lab File: VX027051.D

Acq: 16 Feb 2022 15:53

Instrument :

MSVOA_X

ClientSampleId :

COP-1R





Tgt Ion: 43 Resp: 19988

Ion Ratio Lower Upper

43 100

61 14.1 10.6 16.0

70 11.3 8.5 12.7

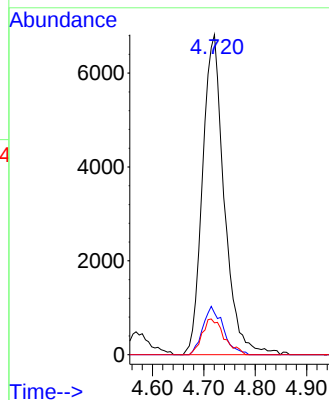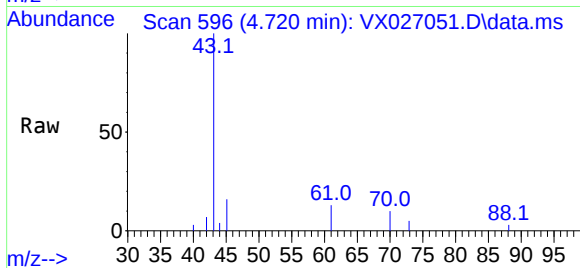

#38

Carbon Tetrachloride

Concen: 6.102 ug/l

RT: 5.562 min Scan# 734

Delta R.T. -0.122 min

Lab File: VX027051.D

Acq: 16 Feb 2022 15:53




Tgt Ion: 117 Resp: 11071


Ion Ratio Lower Upper

117 100

119 3.8 74.7 112.1#

121 0.0 25.4 38.0#

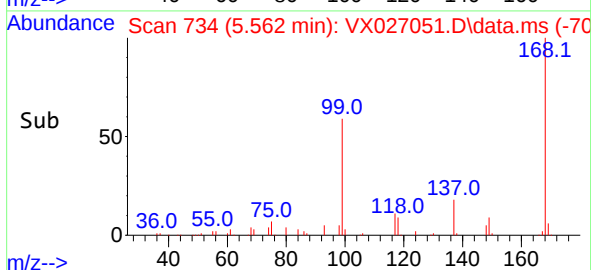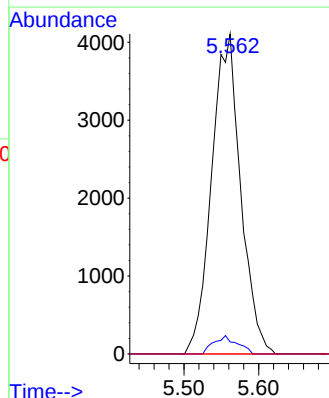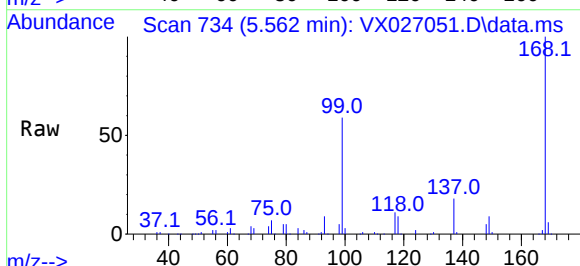



#39

Methylcyclohexane

Concen: 0.292 ug/l

RT: 7.378 min Scan# 1033

Delta R.T. -0.006 min

Lab File: VX027051.D

Acq: 16 Feb 2022 15:53

Instrument :

MSVOA_X

ClientSampleId :

COP-1R





Tgt Ion: 83 Resp: 620

Ion Ratio Lower Upper

83 100

55 93.2 63.6 95.4

98 39.0 38.4 57.6

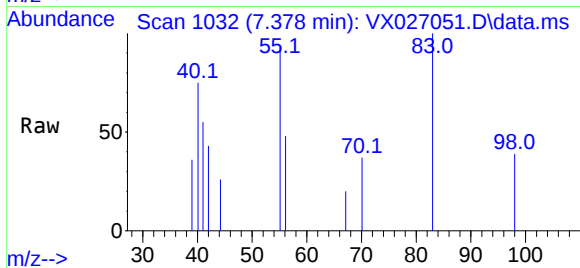

#40

Benzene

Concen: 1.070 ug/l

RT: 6.043 min Scan# 813

Delta R.T. -0.000 min

Lab File: VX027051.D




Acq: 16 Feb 2022 15:53


Tgt Ion: 78 Resp: 5395

Ion Ratio Lower Upper

78 100

77 20.4 18.9 28.3

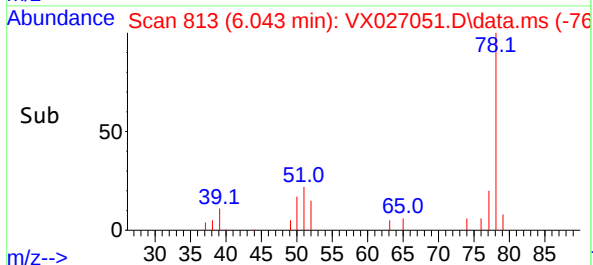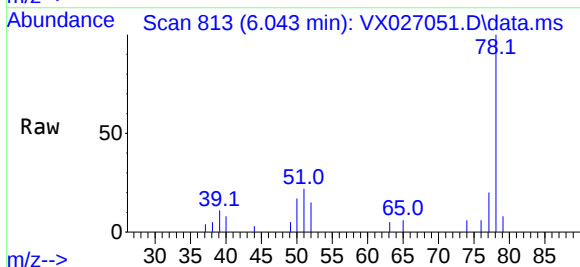



#50

Toluene-d8

Concen: 53.744 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX027051.D

Acq: 16 Feb 2022 15:53

Instrument :

MSVOA_X

ClientSampleId :





COP-1R

Tgt Ion: 98 Resp: 216372

Ion Ratio Lower Upper

98 100

100 66.5 53.2 79.8

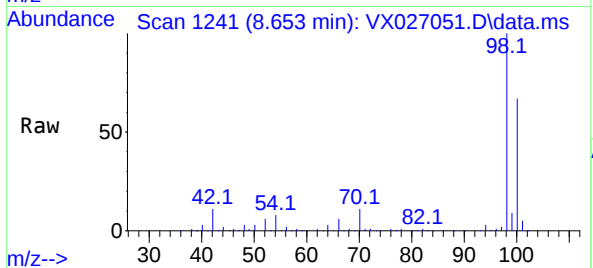

#52

Toluene

Concen: 7.168 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX027051.D




Acq: 16 Feb 2022 15:53


Tgt Ion: 92 Resp: 22886

Ion Ratio Lower Upper

92 100

91 172.7 135.7 203.5

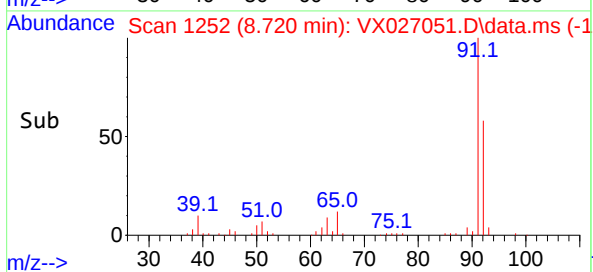



#53

t-1,3-Dichloropropene

Concen: 1.484 ug/l

RT: 8.720 min Scan# 11

Delta R.T. -0.262 min

Lab File: VX027051.D

Acq: 16 Feb 2022 15:53

Instrument :

MSVOA_X

ClientSampleId :





COP-1R

Tgt Ion: 75 Resp: 253

Ion Ratio Lower Upper

75 100

77 134.3 25.7 38.5#

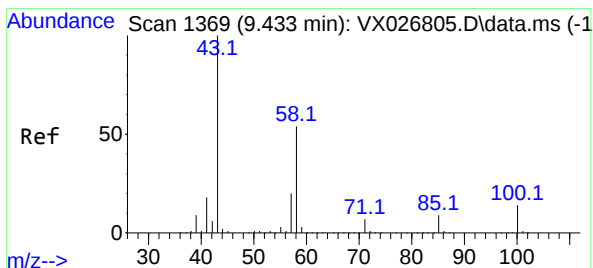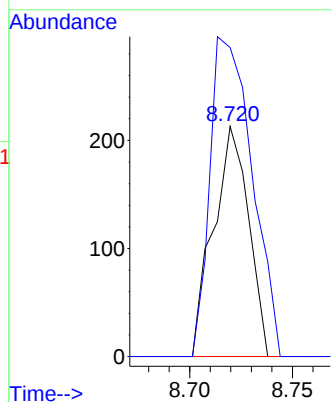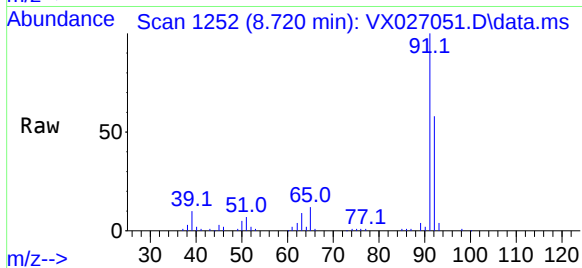

#59

2-Hexanone

Concen: 0.286 ug/l

RT: 9.445 min Scan# 1371

Delta R.T. 0.012 min

Lab File: VX027051.D




Acq: 16 Feb 2022 15:53


Tgt Ion: 43 Resp: 383

Ion Ratio Lower Upper

43 100

58 43.1 26.4 79.2


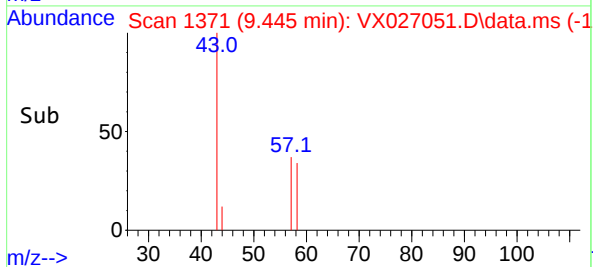
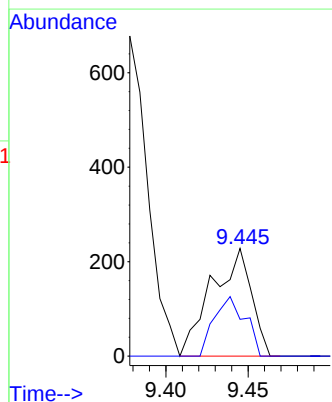
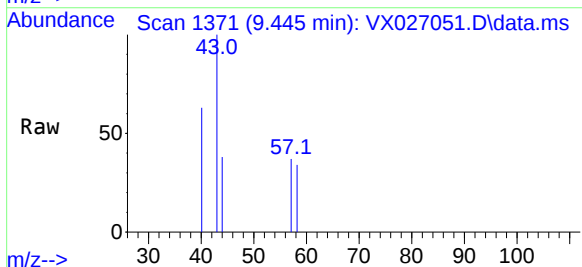




#62
4-Bromofluorobenzene
Concen: 58.676 ug/l
RT: 11.079 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53




Instrument :
MSVOA_X
ClientSampleId :
COP-1R


Tgt Ion: 95 Resp: 83169
Ion Ratio Lower Upper
95 100
174 76.6 0.0 148.6
176 74.3 0.0 141.4

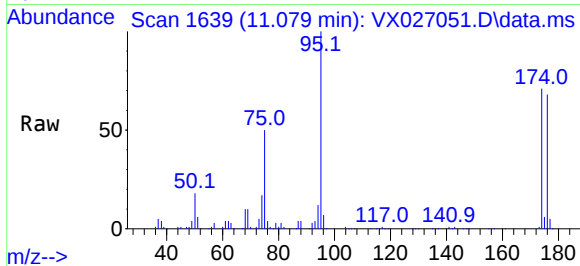

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53

Tgt Ion: 117 Resp: 171432
Ion Ratio Lower Upper
117 100
82 55.4 45.2 67.8
119 31.9 26.2 39.2

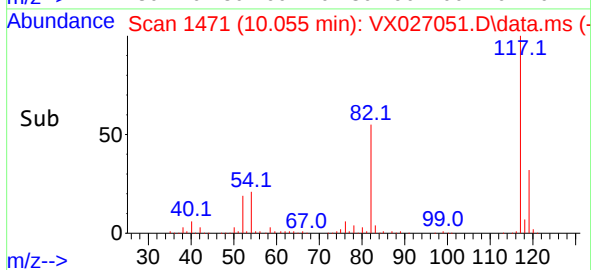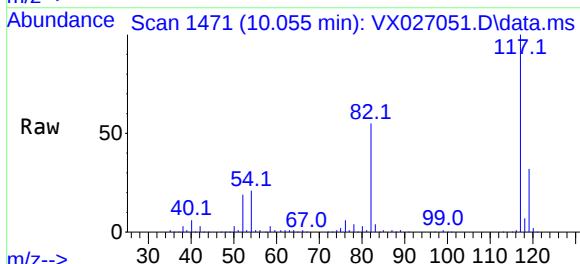



#67

Ethyl Benzene

Concen: 1.756 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. -0.000 min

Lab File: VX027051.D

Acq: 16 Feb 2022 15:53

Instrument :

MSVOA_X

ClientSampleId :





COP-1R

Tgt Ion: 91 Resp: 11019

Ion Ratio Lower Upper

91 100

106 33.2 24.7 37.1

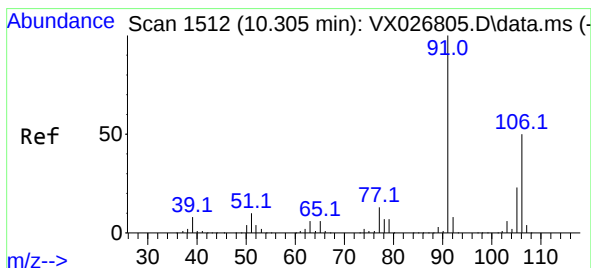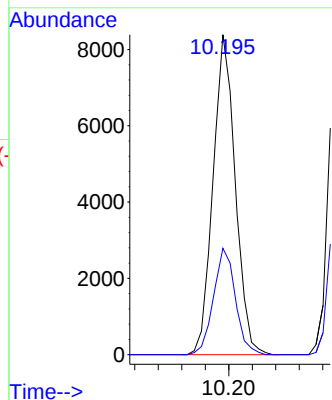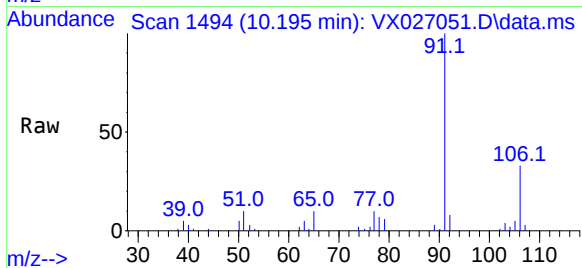

#68

m/p-Xylenes

Concen: 7.680 ug/l

RT: 10.305 min Scan# 1512

Delta R.T. -0.000 min

Lab File: VX027051.D




Acq: 16 Feb 2022 15:53


Tgt Ion: 106 Resp: 18542

Ion Ratio Lower Upper

106 100

91 202.8 165.3 247.9


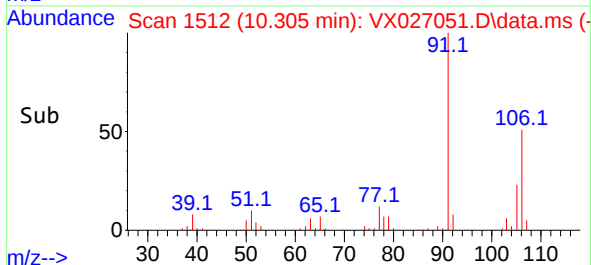
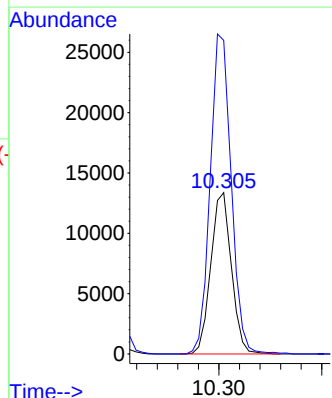
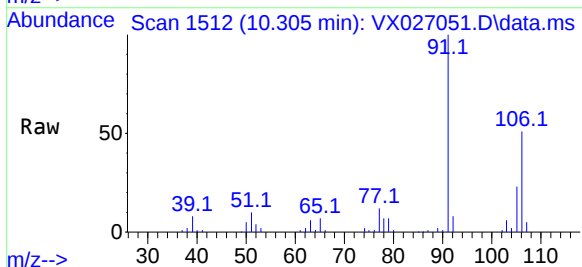




#69
o-Xylene
Concen: 6.969 ug/l
RT: 10.646 min Scan# 1567
Delta R.T. 0.006 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53




Instrument :
MSVOA_X
ClientSampleId :
COP-1R


Tgt Ion:106 Resp: 16487
Ion Ratio Lower Upper
106 100
91 220.6 109.7 329.0

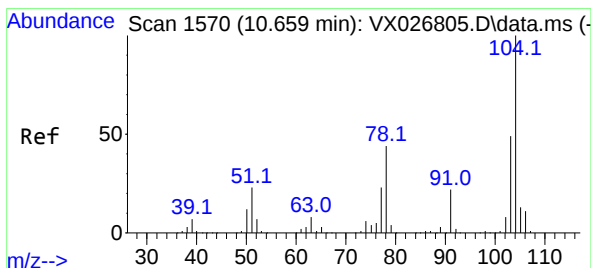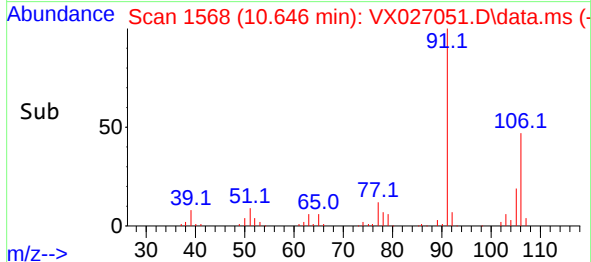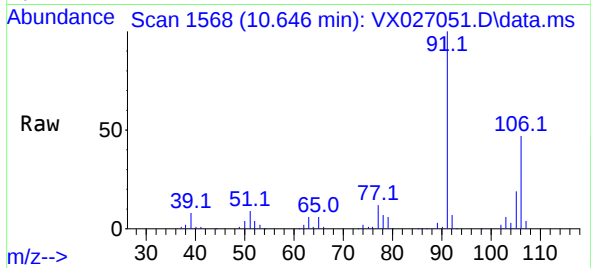

#70
Styrene
Concen: 0.357 ug/l
RT: 10.652 min Scan# 1569
Delta R.T. -0.006 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53

Tgt Ion:104 Resp: 1369
Ion Ratio Lower Upper
104 100
78 192.9 42.5 63.7#
103 179.2 43.3 64.9#


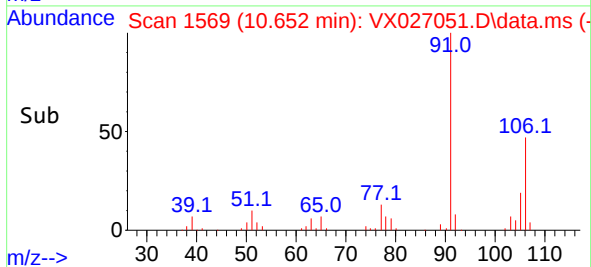

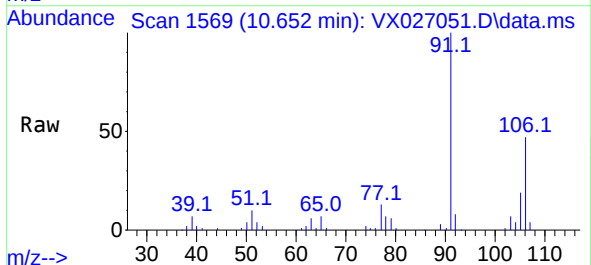




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53




Instrument :
MSVOA_X
ClientSampleId :
COP-1R


Tgt Ion:152 Resp: 77159
Ion Ratio Lower Upper
152 100
115 59.8 44.2 132.6
150 157.4 0.0 348.2

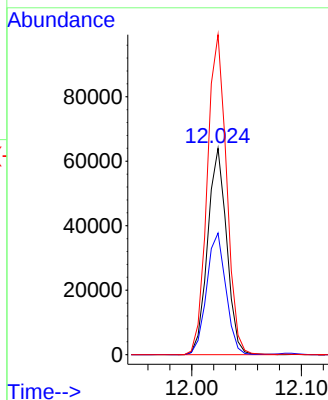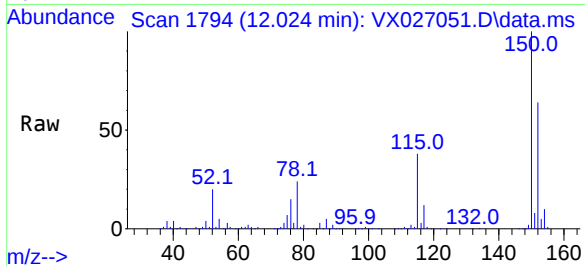

#73
Isopropylbenzene
Concen: 0.211 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. -0.000 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53

Tgt Ion:105 Resp: 1280
Ion Ratio Lower Upper
105 100
120 30.2 13.1 39.1


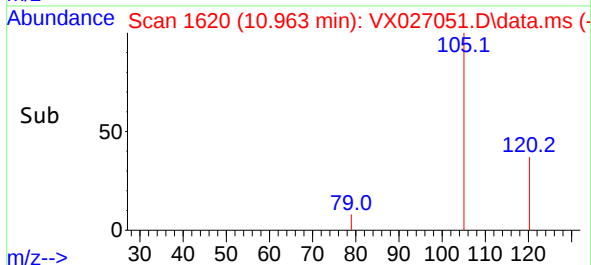
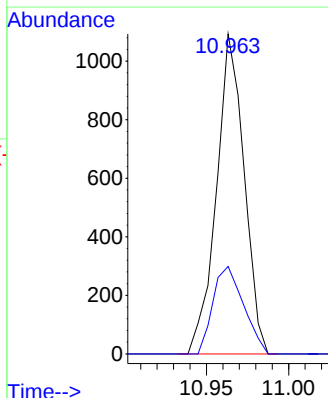
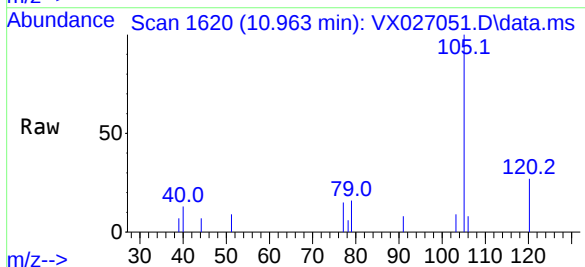




#76
1,2,3-Trichloropropane
Concen: 24.186 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53




Instrument :
MSVOA_X
ClientSampleId :
COP-1R


Tgt Ion: 75 Resp: 40852
Ion Ratio Lower Upper
75 100
77 1.1 18.3 54.8#

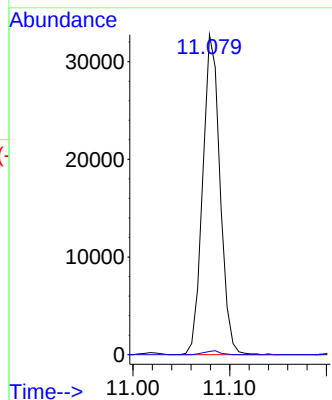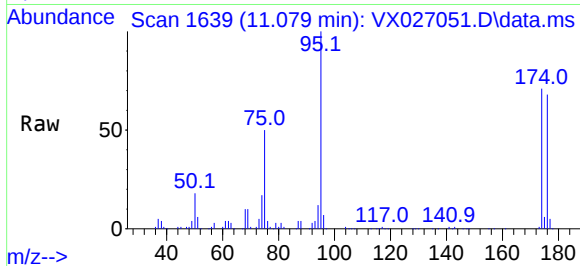

#78
n-propylbenzene
Concen: 0.238 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53

Tgt Ion: 91 Resp: 1604
Ion Ratio Lower Upper
91 100
120 23.1 11.6 34.7


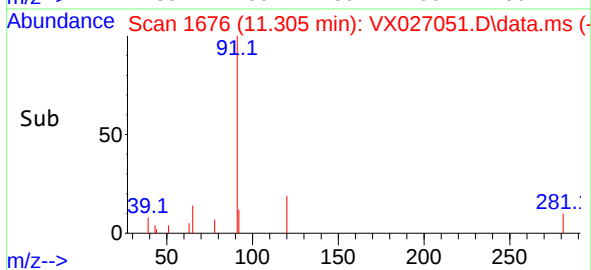
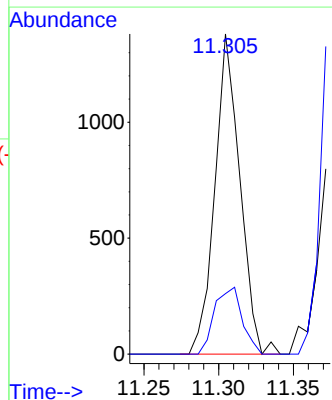
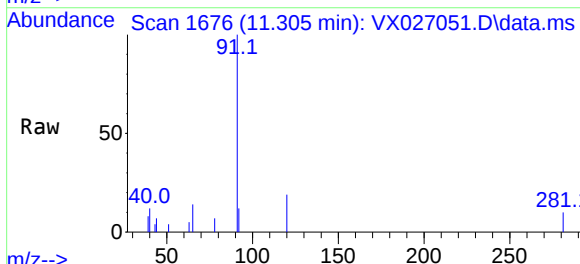




#79
2-Chlorotoluene
Concen: 0.557 ug/l
RT: 11.378 min Scan# 11
Delta R.T. 0.012 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53




Instrument :
MSVOA_X
ClientSampleId :
COP-1R


Tgt Ion: 91 Resp: 2318
Ion Ratio Lower Upper
91 100
126 1.1 16.4 49.2#

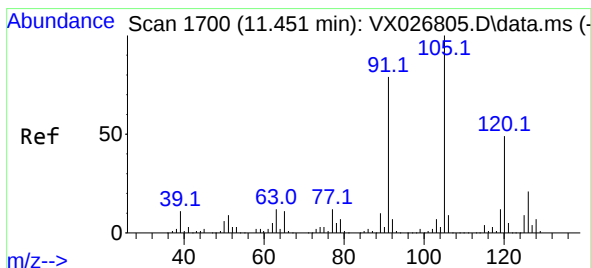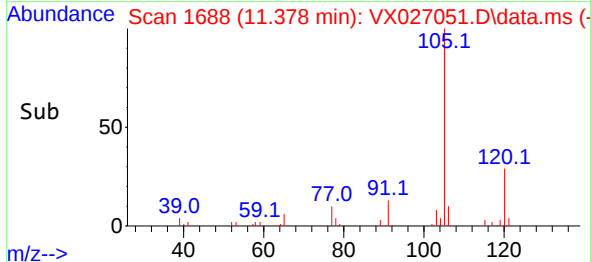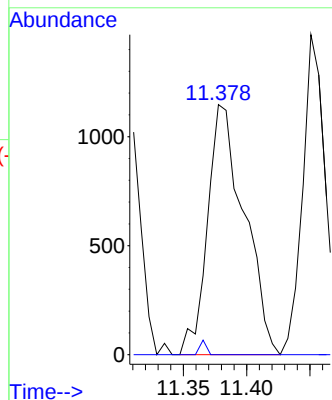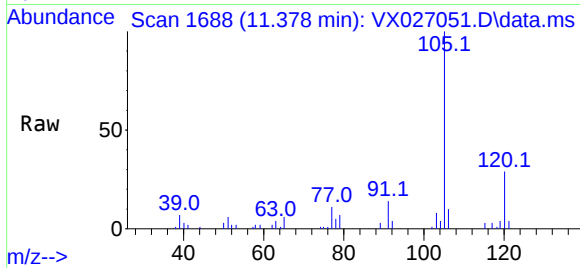

#80
1,3,5-Trimethylbenzene
Concen: 2.883 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53

Tgt Ion: 105 Resp: 14420
Ion Ratio Lower Upper
105 100
120 48.4 24.0 72.0


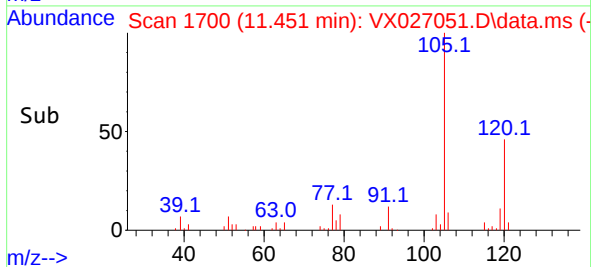
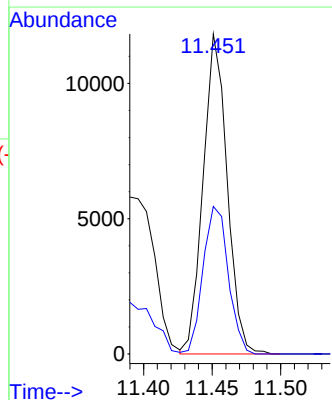
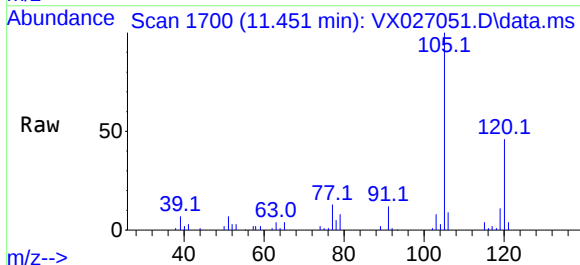




#81
trans-1,4-Dichloro-2-butene
Concen: 73.885 ug/l
RT: 11.079 min Scan# 11
Delta R.T. 0.061 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53




Instrument :
MSVOA_X
ClientSampleId :
COP-1R


Tgt Ion: 75 Resp: 40852
Ion Ratio Lower Upper
75 100
53 0.0 94.0 141.0#
89 0.0 37.0 55.4#

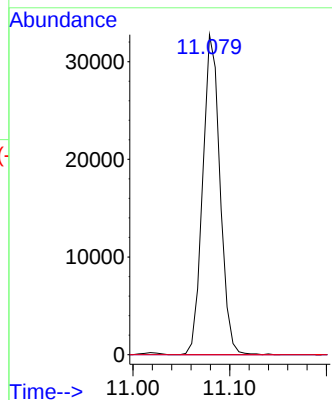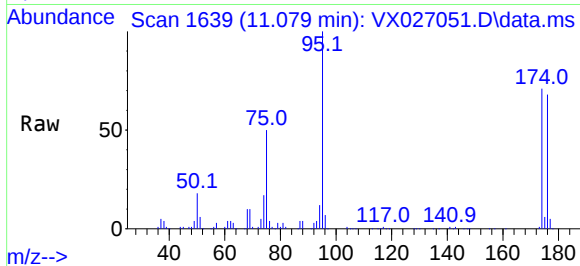

#82
4-Chlorotoluene
Concen: 0.385 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53

Tgt Ion: 91 Resp: 1797
Ion Ratio Lower Upper
91 100
126 0.0 14.1 42.4#


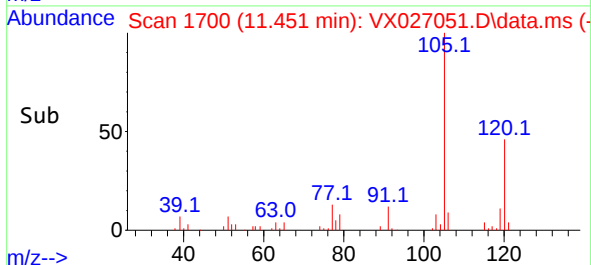
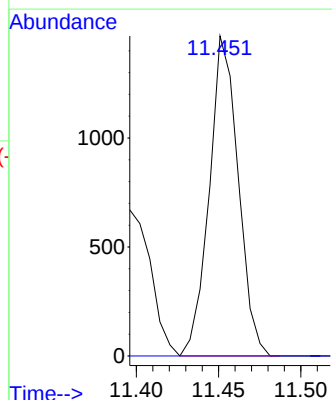
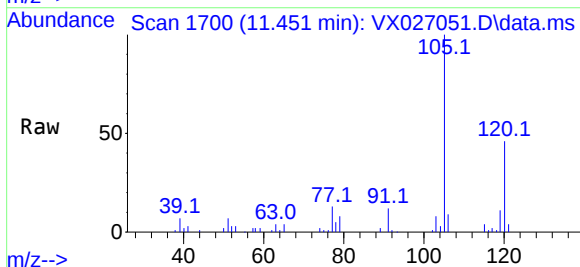




#84
1,2,4-Trimethylbenzene
Concen: 3.054 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53




Instrument :
MSVOA_X
ClientSampleId :
COP-1R


Tgt Ion:105 Resp: 15408
Ion Ratio Lower Upper
105 100
120 43.9 21.9 65.5

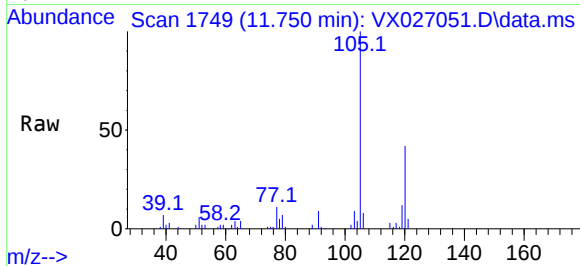

#85
sec-Butylbenzene
Concen: 2.550 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.140 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53

Tgt Ion:105 Resp: 15408
Ion Ratio Lower Upper
105 100
134 0.0 10.1 30.1#


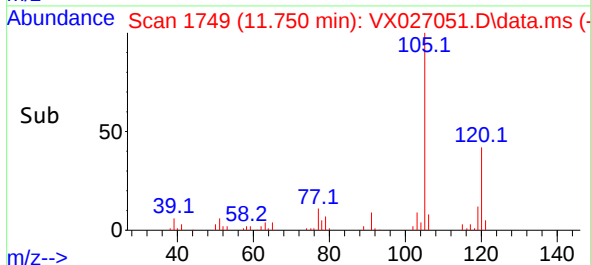

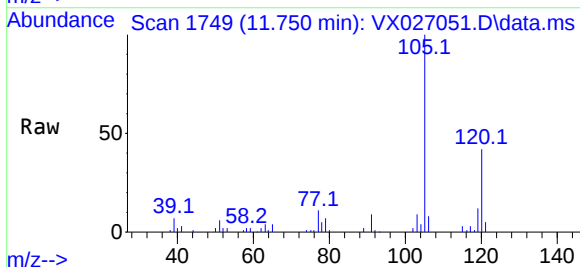




#86
p-Isopropyltoluene
Concen: 0.232 ug/l
RT: 12.012 min Scan# 1188
Delta R.T. -0.000 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53




Instrument :
MSVOA_X
ClientSampleId :
COP-1R


Tgt Ion:	119	Resp:	1188
Ion	Ratio	Lower	Upper
119	100		
134	36.0	13.0	39.0
91	36.6	12.6	37.6

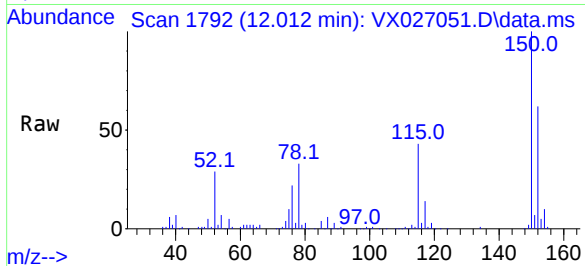

#89
n-Butylbenzene
Concen: 0.247 ug/l
RT: 12.317 min Scan# 1842
Delta R.T. -0.018 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53


Tgt Ion:	91	Resp:	1036
Ion	Ratio	Lower	Upper
91	100		
92	26.5	27.2	81.6#
134	112.7	13.1	39.1#

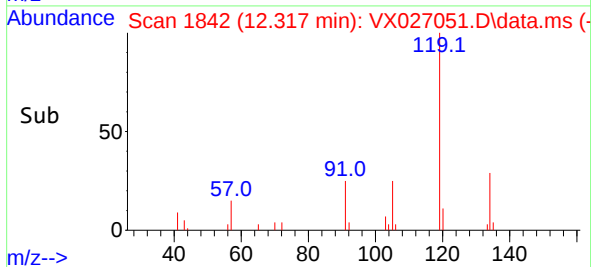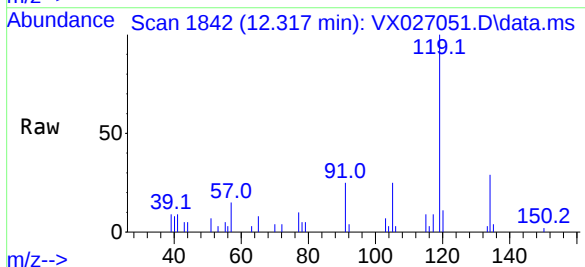

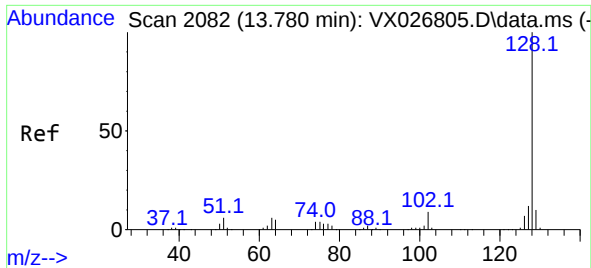

#95
Naphthalene
Concen: 1.667 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX027051.D
Acq: 16 Feb 2022 15:53

Instrument :
MSVOA_X
ClientSampleId :
COP-1R

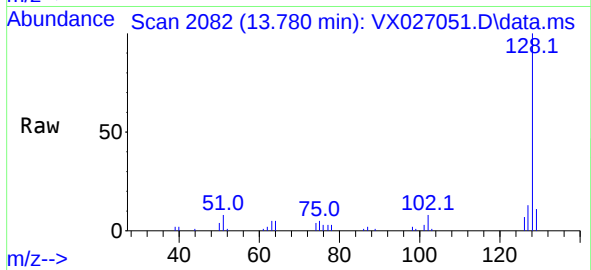

Tgt Ion:	128	Resp:	9411
Ion	Ratio	Lower	Upper
128	100		
127	12.5	10.3	15.5
129	11.7	8.7	13.1

