


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021622\
Data File : VX027043.D
Acq On : 16 Feb 2022 10:16
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Title : SW846 8260
Last Update : Tue Feb 08 07:07:46 2022

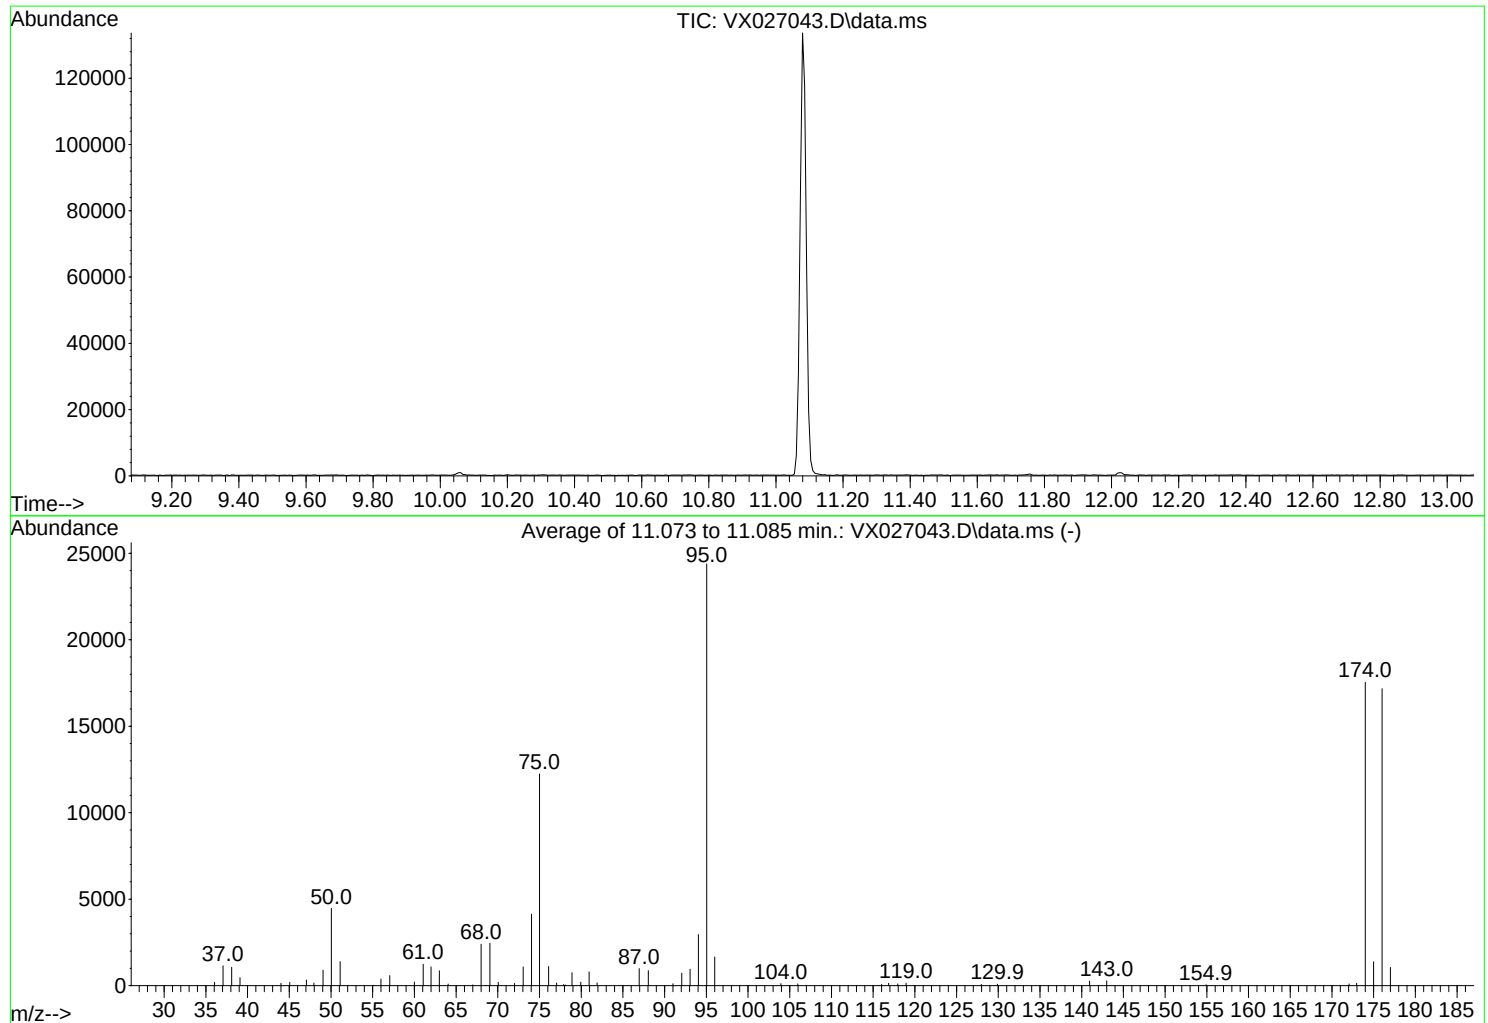

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	4467	PASS
75	95	30	60	50.2	12242	PASS
95	95	100	100	100.0	24389	PASS
96	95	5	9	6.8	1660	PASS
173	174	0.00	2	0.8	139	PASS
174	95	50	100	71.9	17537	PASS
175	174	5	9	7.9	1380	PASS
176	174	95	101	97.9	17170	PASS
177	176	5	9	6.2	1056	PASS