

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021624\
 Data File : VX040282.D
 Acq On : 16 Feb 2024 16:39
 Operator : JC/MD
 Sample : P1507-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW179D1-20240215

Quant Time: Feb 17 01:38:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020924W.M
 Quant Title : SW846 8260
 QLast Update : Mon Feb 12 00:21:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	70238	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	117287	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	114648	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	59283	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	47447	45.407	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	90.820%
35) Dibromofluoromethane	5.385	113	38436	46.926	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	93.860%
50) Toluene-d8	8.647	98	144234	47.075	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	94.160%
62) 4-Bromofluorobenzene	11.079	95	56860	45.503	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	91.000%
Target Compounds						
						Qvalue
9) 1,1,2-Trichlorotrifluo...	2.331	101	508	0.682	ug/l	# 92
12) 1,1-Dichloroethene	2.319	96	440	0.614	ug/l	# 71
19) Methyl tert-butyl Ether	3.117	73	1592	0.630	ug/l	95
27) cis-1,2-Dichloroethene	4.495	96	11995	12.874	ug/l	80
44) Trichloroethene	7.123	130	96213	108.708	ug/l	99
64) Tetrachloroethene	9.275	164	11023	13.720	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021624\
Data File : VX040282.D
Acq On : 16 Feb 2024 16:39
Operator : JC/MD
Sample : P1507-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW179D1-20240215

Quant Time: Feb 17 01:38:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020924W.M
Quant Title : SW846 8260
QLast Update : Mon Feb 12 00:21:14 2024
Response via : Initial Calibration




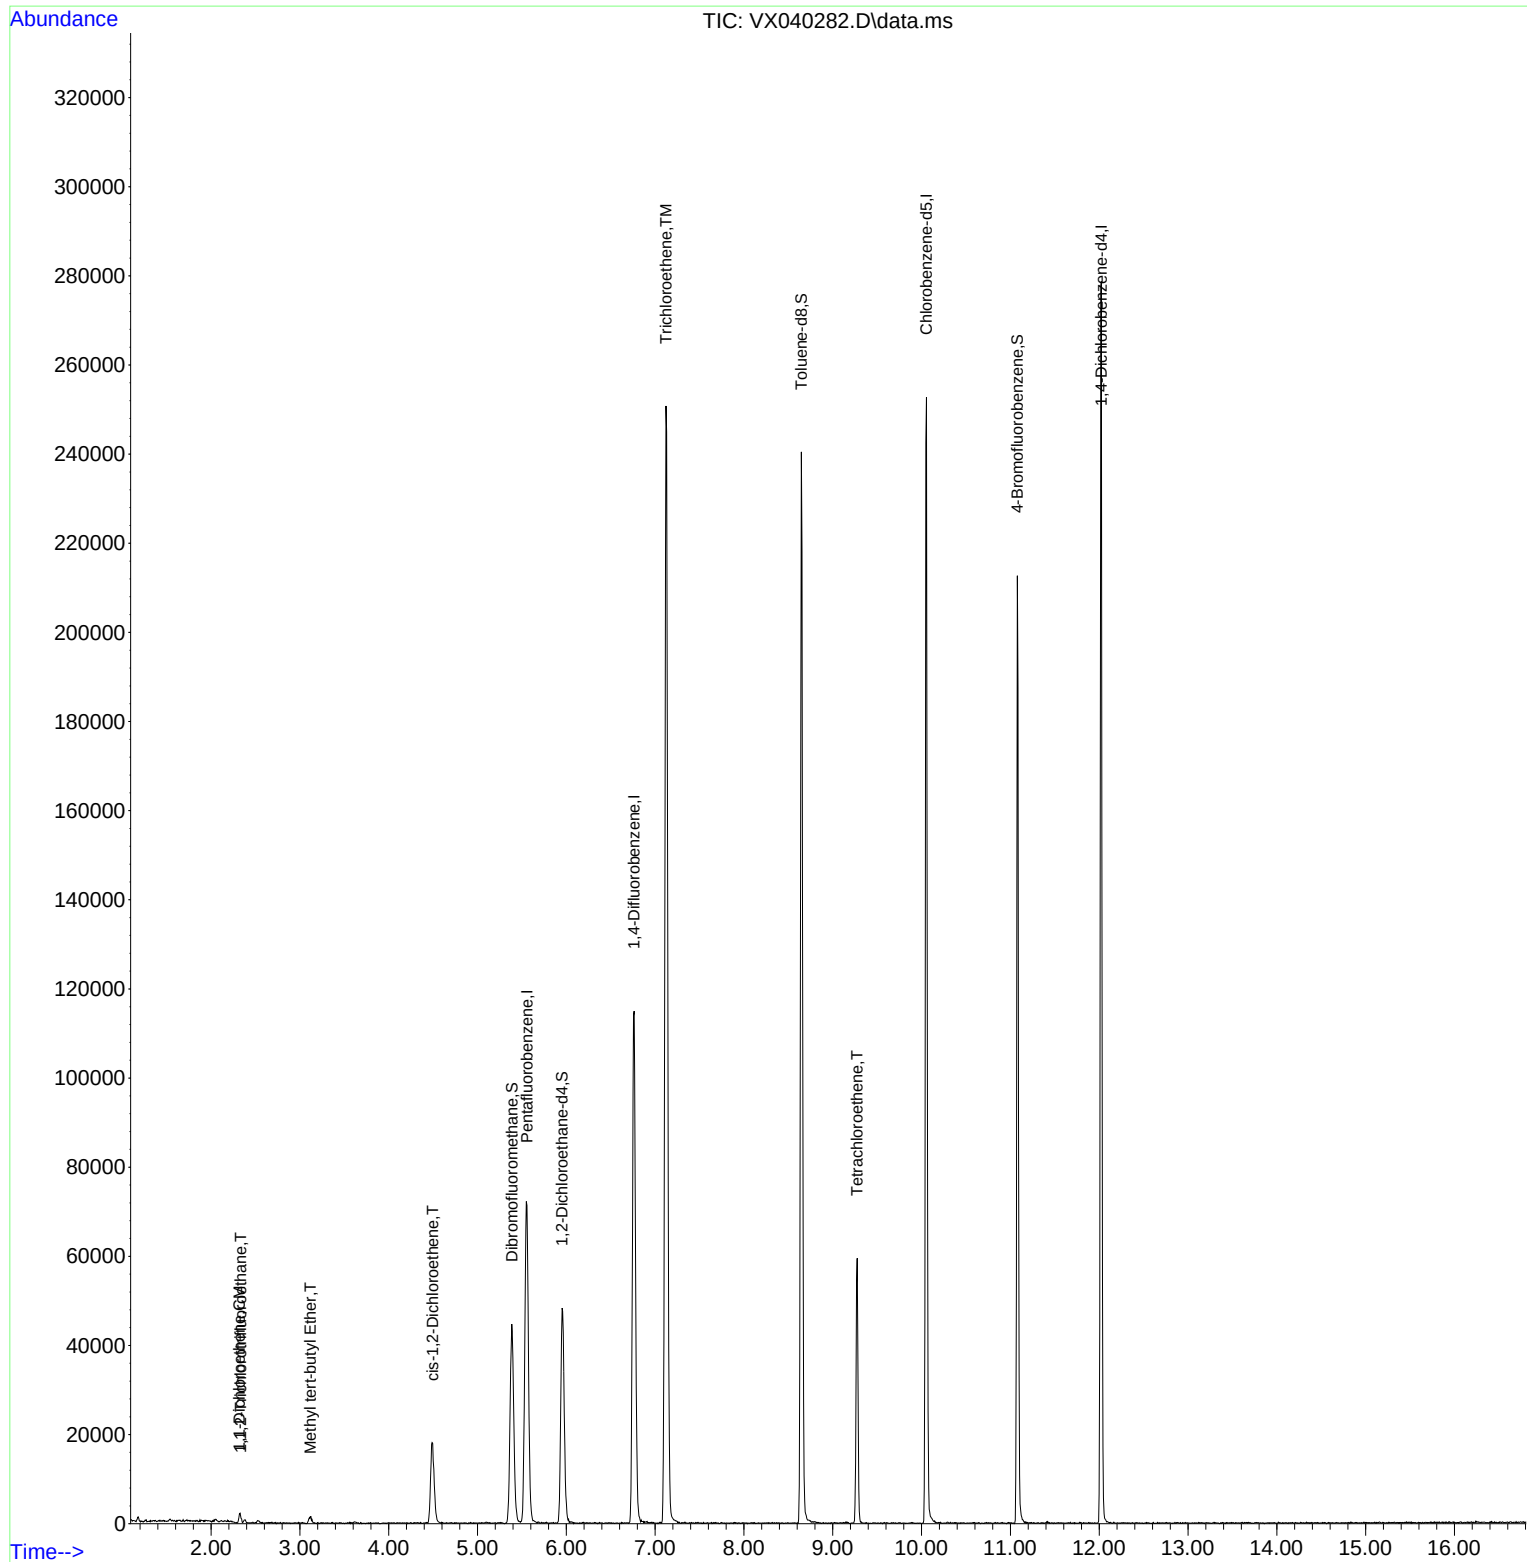


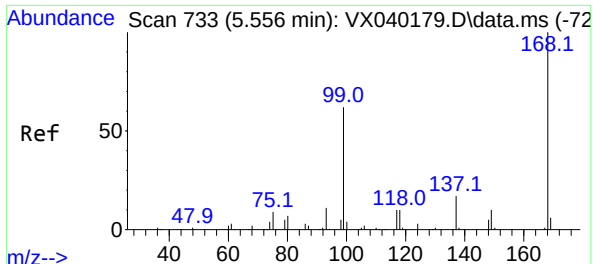

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX040282.D
Acq: 16 Feb 2024 16:39




Instrument :
MSVOA_X
ClientSampleId :
MW179D1-20240215


Tgt Ion:168 Resp: 70238
Ion Ratio Lower Upper
168 100
99 55.5 56.6 85.0#

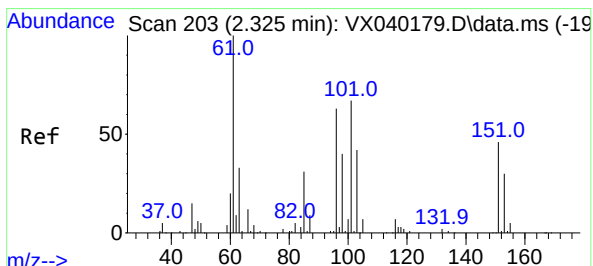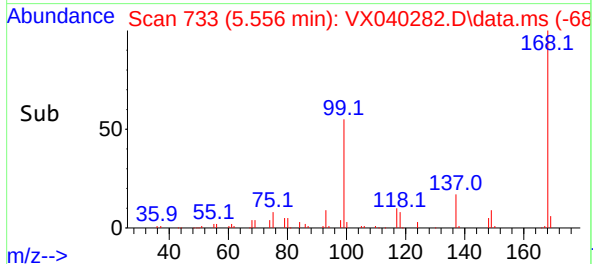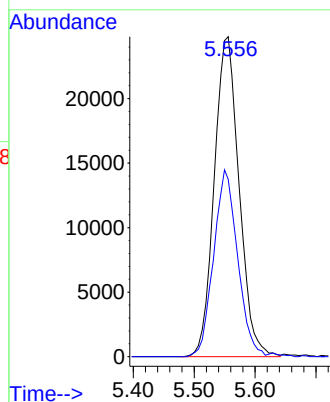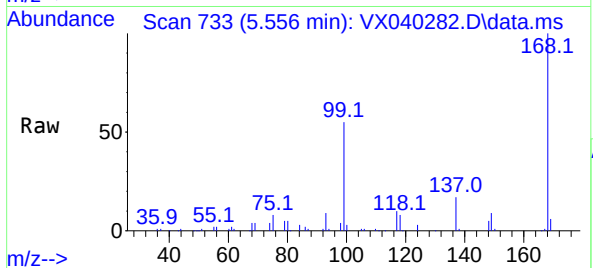

#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.682 ug/l
RT: 2.331 min Scan# 204
Delta R.T. 0.006 min
Lab File: VX040282.D
Acq: 16 Feb 2024 16:39

Tgt Ion:101 Resp: 508
Ion Ratio Lower Upper
101 100
85 36.4 37.0 55.6#
151 76.2 58.6 87.8

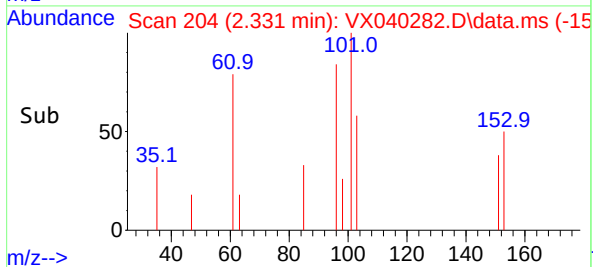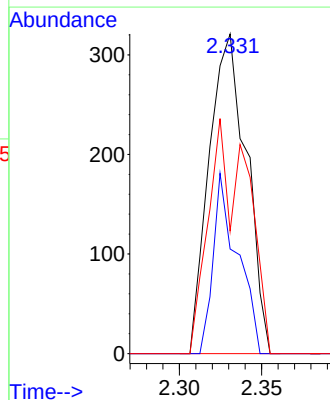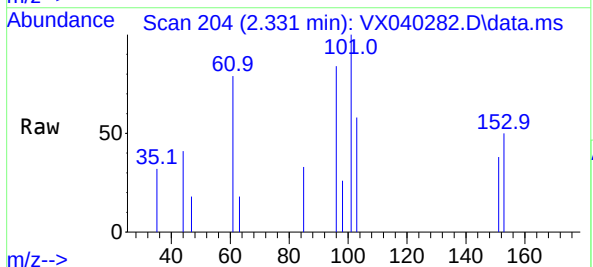

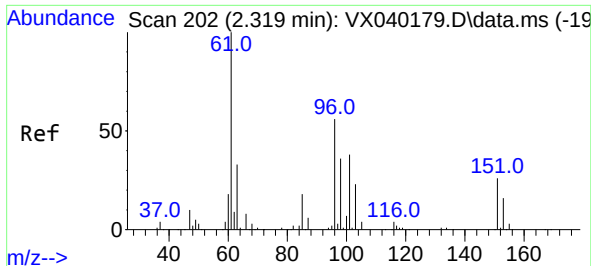

#12

1,1-Dichloroethene

Concen: 0.614 ug/l

RT: 2.319 min Scan# 20

Delta R.T. 0.000 min

Lab File: VX040282.D

Acq: 16 Feb 2024 16:39

Instrument :

MSVOA_X

ClientSampleId :

MW179D1-20240215





Tgt Ion: 96 Resp: 440

Ion Ratio Lower Upper

96 100

61 154.0 144.6 216.8

98 108.8 50.4 75.6#

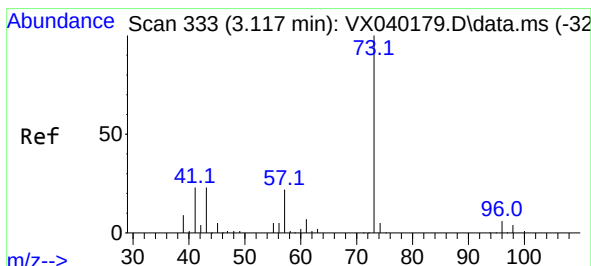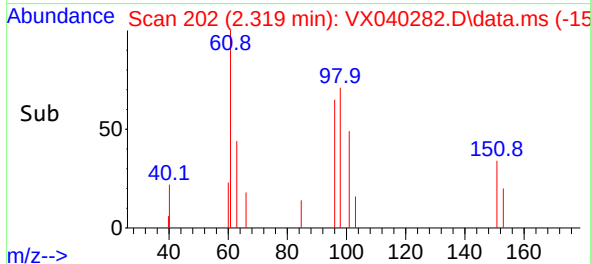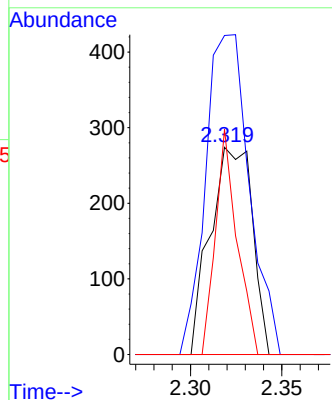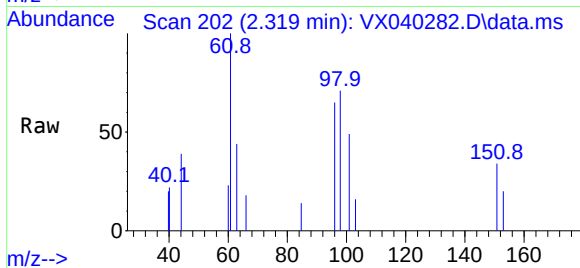

#19

Methyl tert-butyl Ether

Concen: 0.630 ug/l

RT: 3.117 min Scan# 333

Delta R.T. 0.000 min

Lab File: VX040282.D




Acq: 16 Feb 2024 16:39


Tgt Ion: 73 Resp: 1592

Ion Ratio Lower Upper

73 100

57 19.1 17.3 25.9


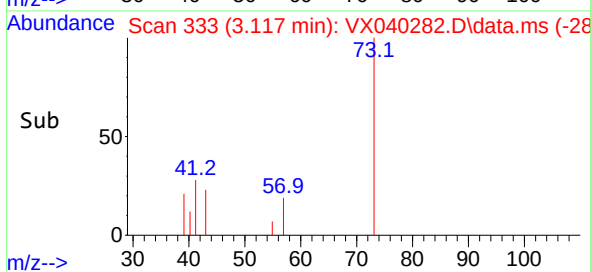
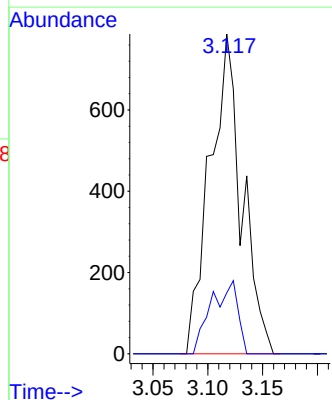
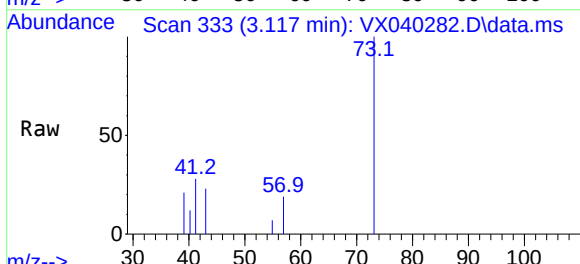


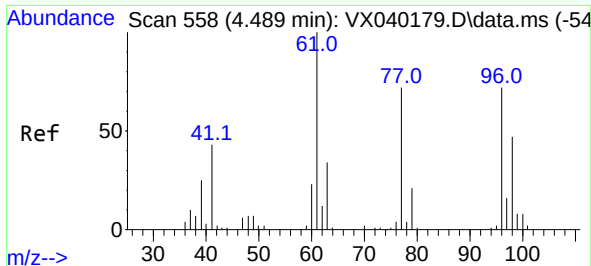

#27
cis-1,2-Dichloroethene
Concen: 12.874 ug/l
RT: 4.495 min Scan# 511
Delta R.T. 0.006 min
Lab File: VX040282.D
Acq: 16 Feb 2024 16:39




Instrument :
MSVOA_X
ClientSampleId :
MW179D1-20240215


Tgt Ion: 96 Resp: 11995
Ion Ratio Lower Upper
96 100
61 122.4 0.0 312.2
98 60.4 0.0 129.0

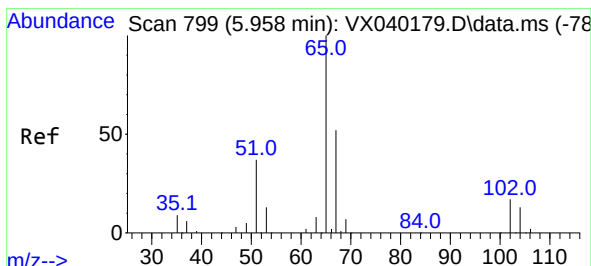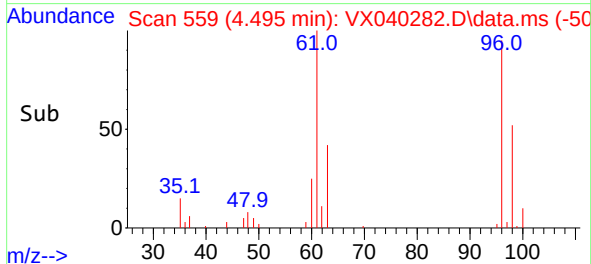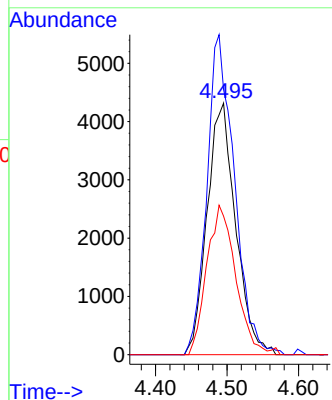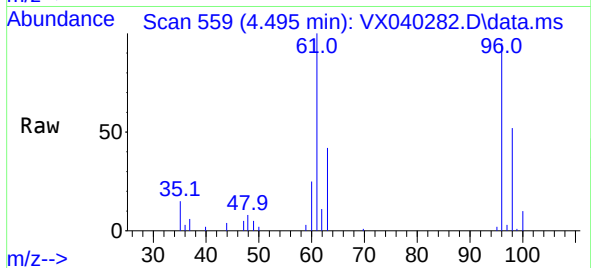

#33
1,2-Dichloroethane-d4
Concen: 45.407 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX040282.D
Acq: 16 Feb 2024 16:39

Tgt Ion: 65 Resp: 47447
Ion Ratio Lower Upper
65 100
67 52.8 0.0 100.2


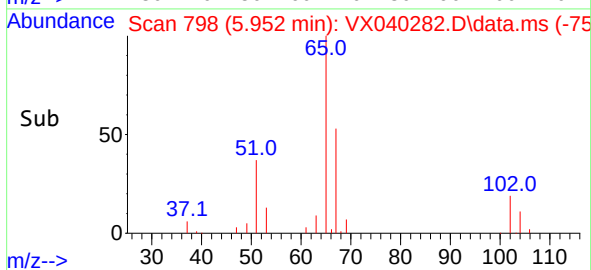
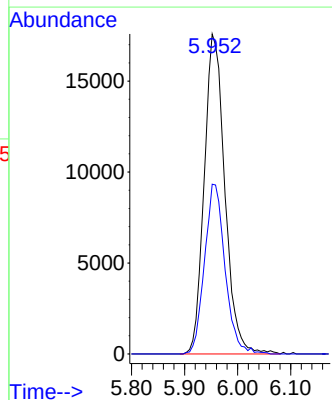
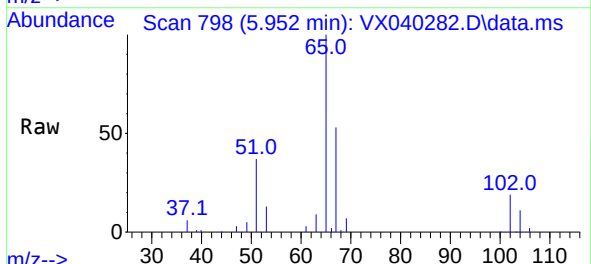


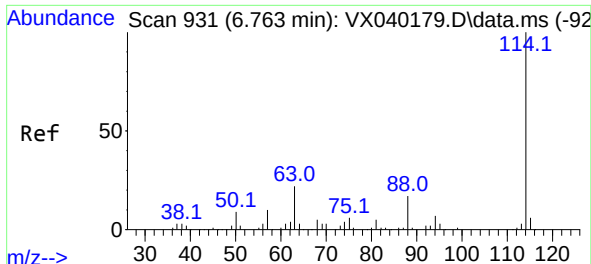

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX040282.D
Acq: 16 Feb 2024 16:39




Instrument :
MSVOA_X
ClientSampleId :
MW179D1-20240215


Tgt Ion:114 Resp: 117287
Ion Ratio Lower Upper
114 100
63 20.9 0.0 45.0
88 16.8 0.0 36.6

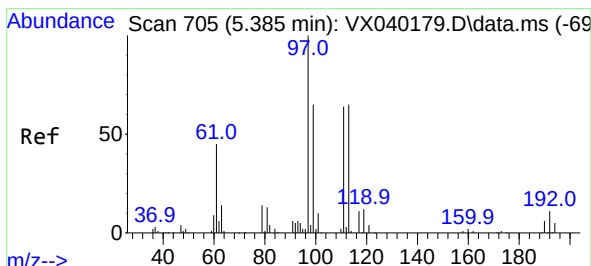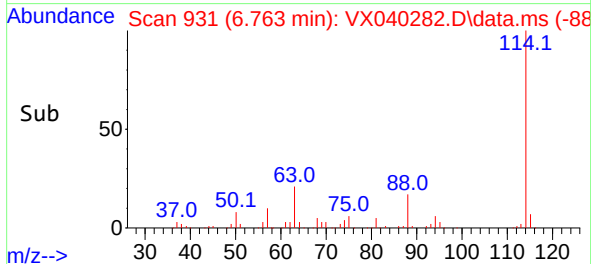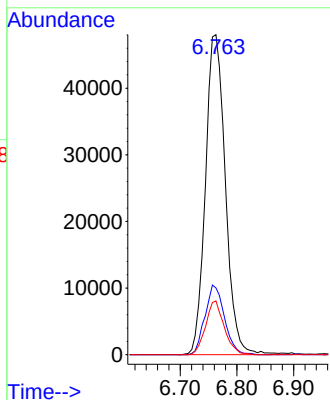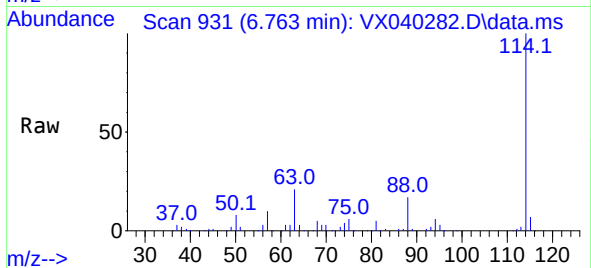

#35
Dibromofluoromethane
Concen: 46.926 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX040282.D
Acq: 16 Feb 2024 16:39

Tgt Ion:113 Resp: 38436
Ion Ratio Lower Upper
113 100
111 102.0 82.9 124.3
192 18.5 13.3 19.9


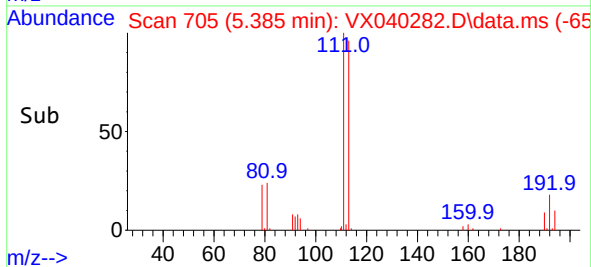
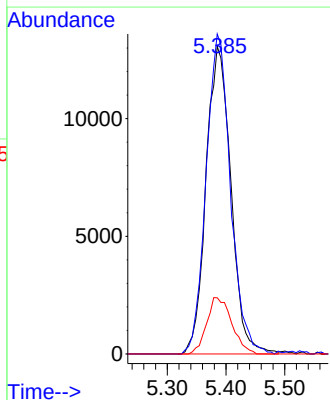
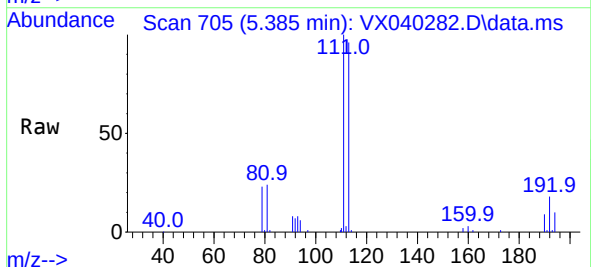


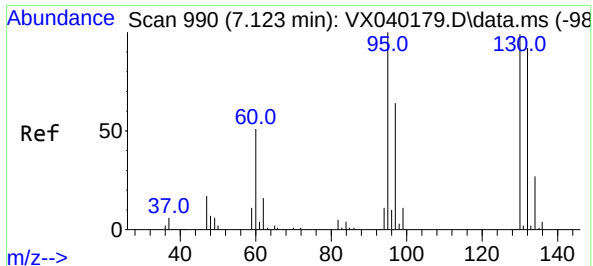

#44
Trichloroethene
Concen: 108.708 ug/l
RT: 7.123 min Scan# 990
Delta R.T. -0.006 min
Lab File: VX040282.D
Acq: 16 Feb 2024 16:39




Instrument :
MSVOA_X
ClientSampleId :
MW179D1-20240215


Tgt Ion:130 Resp: 96213
Ion Ratio Lower Upper
130 100
95 101.3 0.0 204.4

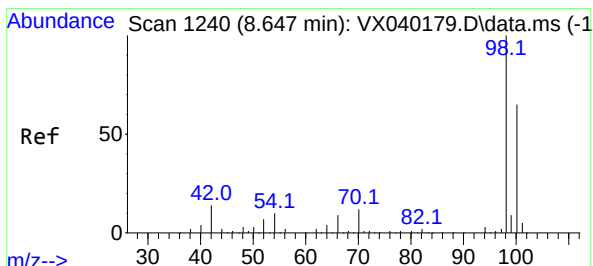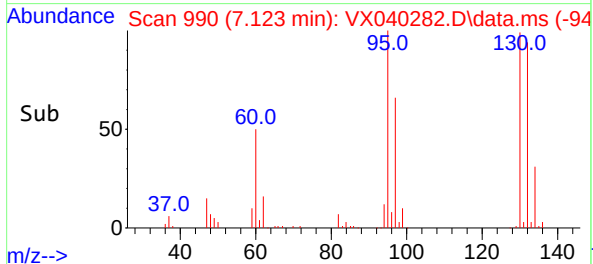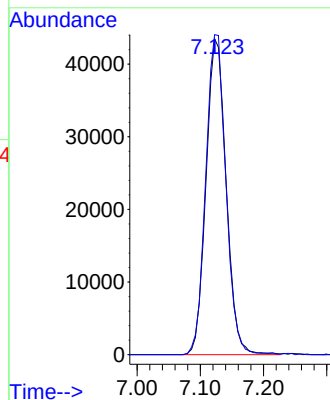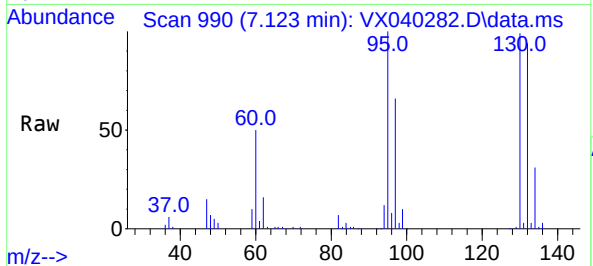

#50
Toluene-d8
Concen: 47.075 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.006 min
Lab File: VX040282.D
Acq: 16 Feb 2024 16:39

Tgt Ion: 98 Resp: 144234
Ion Ratio Lower Upper
98 100
100 63.9 53.1 79.7


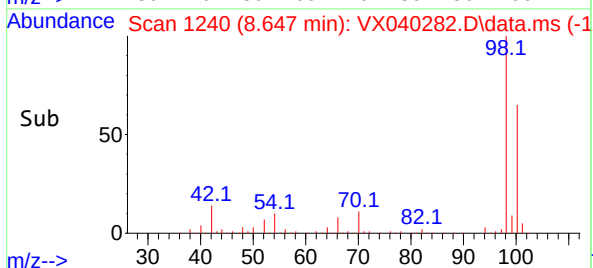
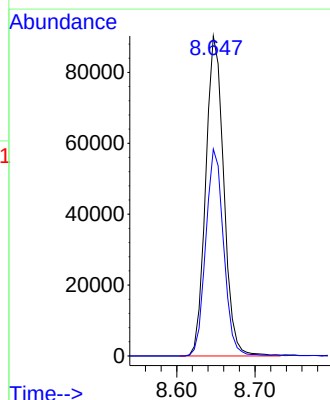
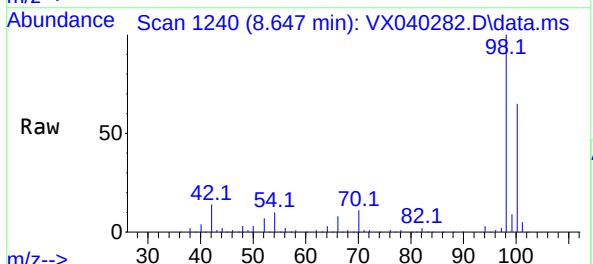


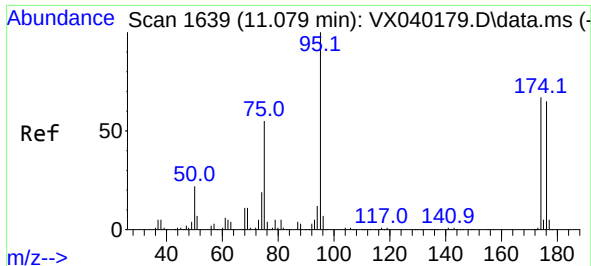

#62
4-Bromofluorobenzene
Concen: 45.503 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX040282.D
Acq: 16 Feb 2024 16:39




Instrument :
MSVOA_X
ClientSampleId :
MW179D1-20240215


Tgt Ion: 95 Resp: 56860
Ion Ratio Lower Upper
95 100
174 76.6 0.0 135.6
176 73.0 0.0 131.0

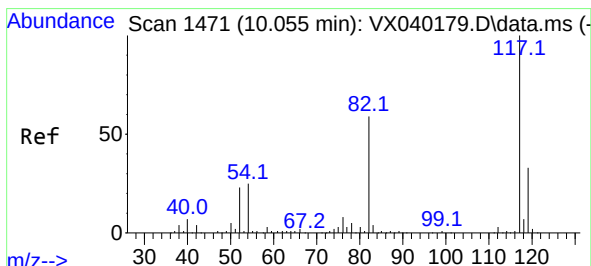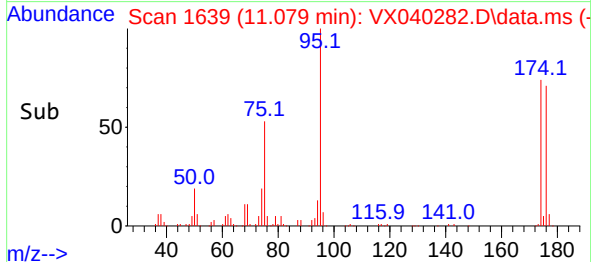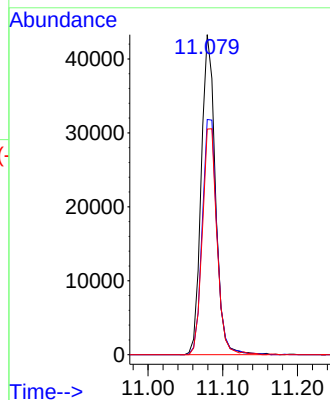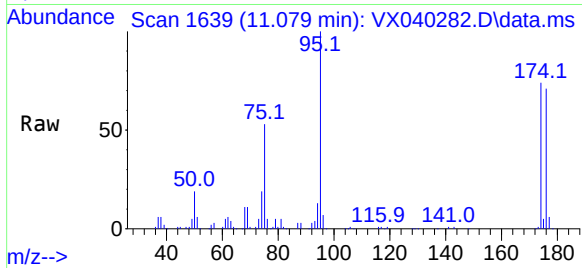

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX040282.D
Acq: 16 Feb 2024 16:39

Tgt Ion: 117 Resp: 114648
Ion Ratio Lower Upper
117 100
82 54.1 46.2 69.4
119 32.0 25.5 38.3

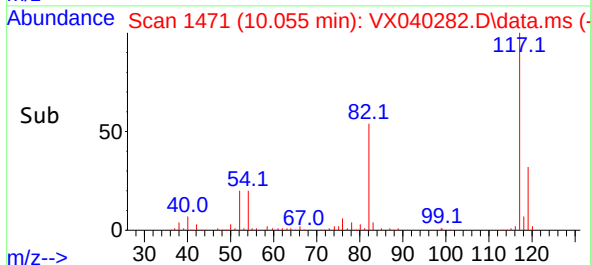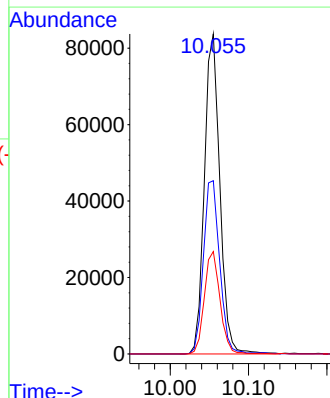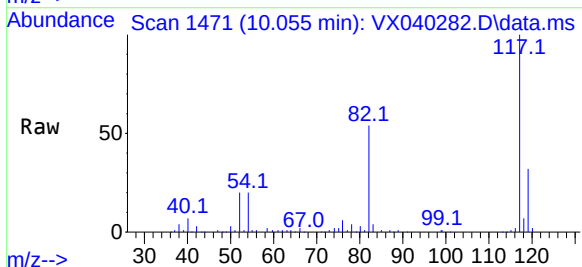




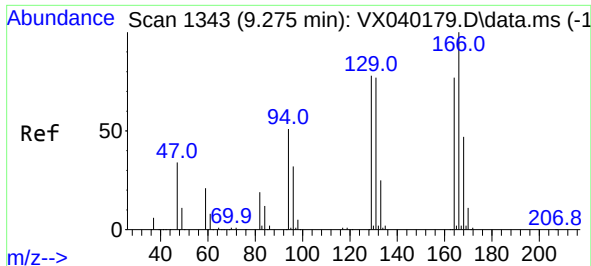


#64
Tetrachloroethene
Concen: 13.720 ug/l
RT: 9.275 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX040282.D
Acq: 16 Feb 2024 16:39

Instrument :
MSVOA_X
ClientSampleId :
MW179D1-20240215

Tgt Ion:164 Resp: 11023

Ion	Ratio	Lower	Upper
164	100		
166	116.2	102.7	154.1
129	91.7	80.4	120.6
131	90.3	76.5	114.7

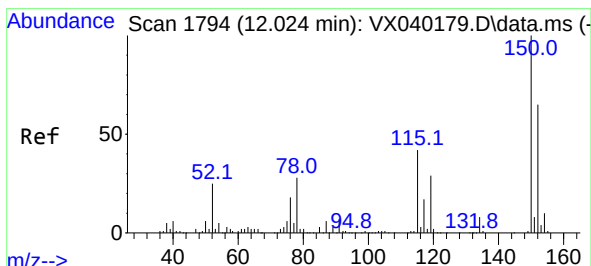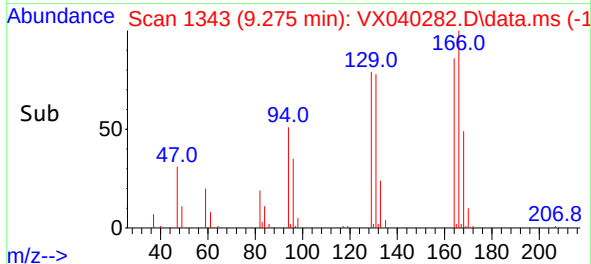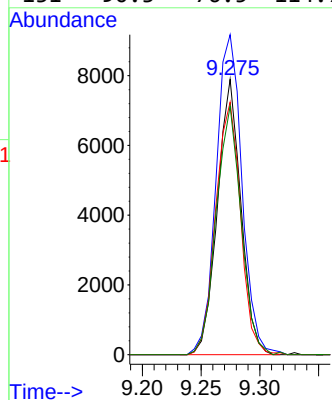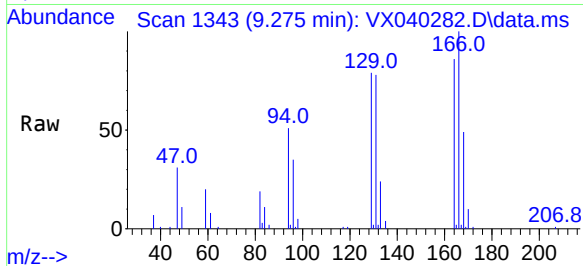

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX040282.D
Acq: 16 Feb 2024 16:39

Tgt Ion:152 Resp: 59283

Ion	Ratio	Lower	Upper
152	100		
115	60.5	43.3	129.9
150	154.8	0.0	345.0

