

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021722\
 Data File : VX027078.D
 Acq On : 17 Feb 2022 15:23
 Operator : JC/MD
 Sample : N1593-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-11R

Quant Time: Feb 18 03:50:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 08 07:07:46 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	110477	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	187138	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	164813	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	71705	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	70238	52.963	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 105.920%	
35) Dibromofluoromethane	5.391	113	58690	52.640	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 105.280%	
50) Toluene-d8	8.653	98	215189	52.580	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 105.160%	
62) 4-Bromofluorobenzene	11.085	95	77008	53.446	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 106.900%	
Target Compounds						
					Qvalue	
10) Methyl Iodide	2.452	142	67	2.295	ug/l #	37
11) Tert butyl alcohol	2.958	59	1344	5.610	ug/l #	75
13) Acrolein	2.343	56	1656	7.480	ug/l #	71
14) Allyl chloride	2.788	41	3292	1.644	ug/l #	65
15) Acrylonitrile	3.105	53	416	0.606	ug/l #	32
16) Acetone	2.343	43	4717	8.098	ug/l #	57
18) Methyl Acetate	2.788	43	9146	5.457	ug/l #	53
20) Methylene Chloride	2.794	84	276	0.219	ug/l #	63
30) Chloroform	5.171	83	967	0.427	ug/l #	18
31) Cyclohexane	5.549	56	2371	1.125	ug/l #	21
36) 1,1-Dichloropropene	5.556	75	8223	4.675	ug/l #	50
38) Carbon Tetrachloride	5.562	117	11201	6.073	ug/l #	17
39) Methylcyclohexane	7.366	83	634	0.294	ug/l #	20
40) Benzene	6.043	78	5375	1.049	ug/l	100
41) Methacrylonitrile	5.135	41	670	0.618	ug/l #	52
48) Methyl methacrylate	7.775	41	627	0.411	ug/l	90
52) Toluene	8.726	92	708	0.218	ug/l	85
55) 1,1,2-Trichloroethane	9.104	97	1661	1.352	ug/l #	21
56) Ethyl methacrylate	9.104	69	437	0.224	ug/l #	6
59) 2-Hexanone	9.451	43	570	0.418	ug/l	75
68) m/p-Xylenes	10.305	106	502	0.216	ug/l	95
73) Isopropylbenzene	10.963	105	2561	0.453	ug/l	100
76) 1,2,3-Trichloropropane	11.085	75	37391	23.821	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.615	105	4314	0.928	ug/l	75
81) trans-1,4-Dichloro-2-b...	11.085	75	37391	72.820	ug/l #	3
85) sec-Butylbenzene	11.890	105	5078	0.904	ug/l	86
86) p-Isopropyltoluene	12.182	119	3492	0.734	ug/l	96
89) n-Butylbenzene	12.317	91	2335	0.600	ug/l #	1
90) Hexachloroethane	12.615	117	3075	4.472	ug/l #	14
92) 1,2-Dibromo-3-Chloropr...	13.170	75	429	1.138	ug/l #	3


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX021722\
Data File : VX027078.D
Acq On : 17 Feb 2022 15:23
Operator : JC/MD
Sample : N1593-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-11R

Quant Time: Feb 18 03:50:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X020822W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 08 07:07:46 2022
Response via : Initial Calibration




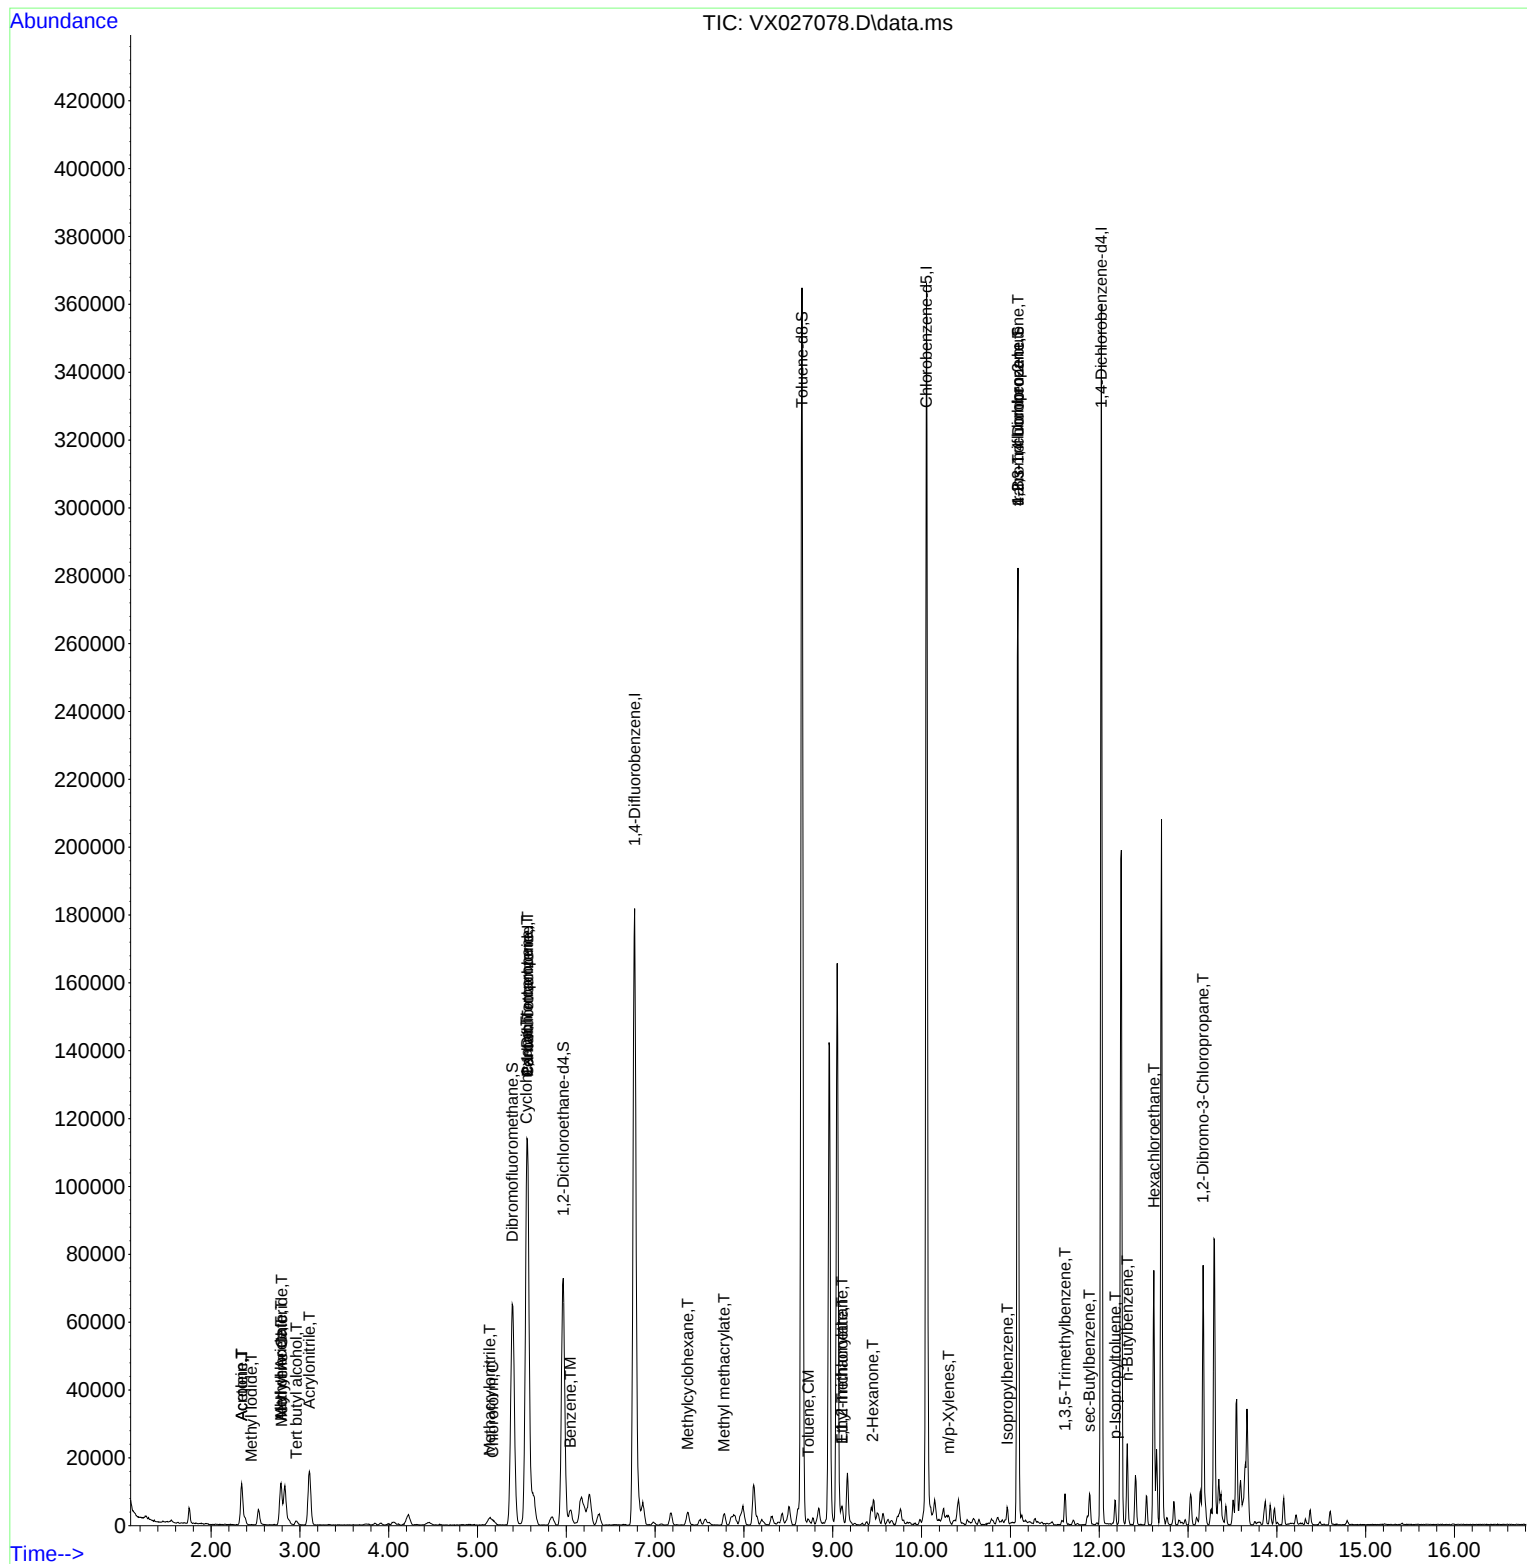


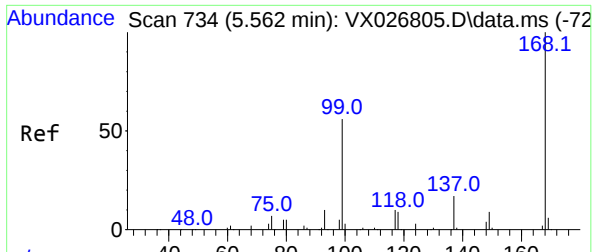

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-11R


Tgt Ion:168 Resp: 110477
Ion Ratio Lower Upper
168 100
99 56.6 50.3 75.5

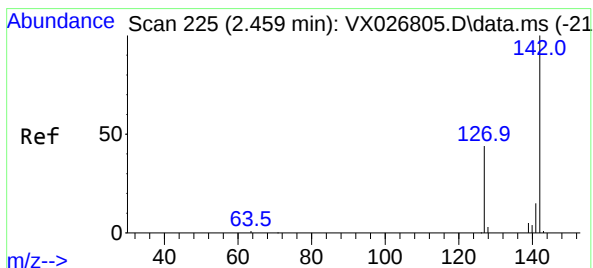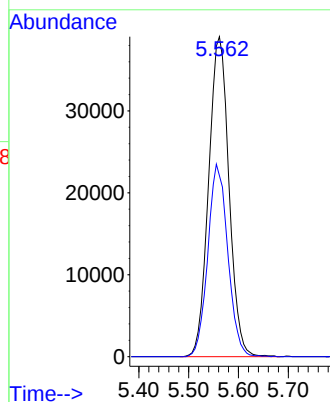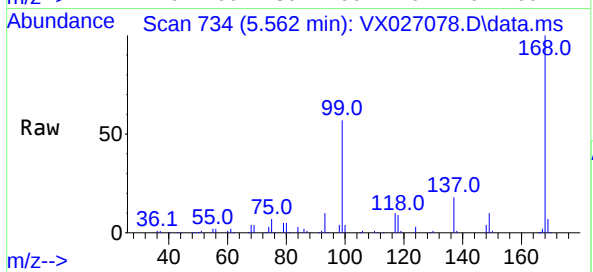

#10
Methyl Iodide
Concen: 2.295 ug/l
RT: 2.452 min Scan# 224
Delta R.T. -0.007 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23

Tgt Ion:142 Resp: 67
Ion Ratio Lower Upper
142 100
127 0.0 38.1 57.1#
141 0.0 11.2 16.8#





#11

Tert butyl alcohol

Concen: 5.610 ug/l

RT: 2.958 min Scan# 30

Delta R.T. -0.043 min

Lab File: VX027078.D

Acq: 17 Feb 2022 15:23

Instrument :

MSVOA_X

ClientSampleId :





MW-11R

Tgt Ion: 59 Resp: 1344

Ion Ratio Lower Upper

59 100

57 0.0 7.2 10.8#

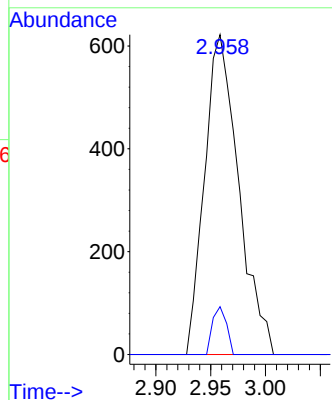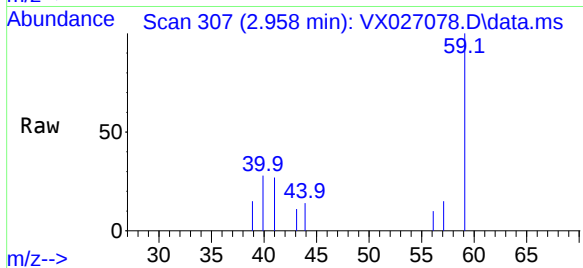

#13

Acrolein

Concen: 7.480 ug/l

RT: 2.343 min Scan# 206

Delta R.T. 0.103 min

Lab File: VX027078.D




Acq: 17 Feb 2022 15:23


Tgt Ion: 56 Resp: 1656

Ion Ratio Lower Upper

56 100

55 47.4 56.9 85.3#



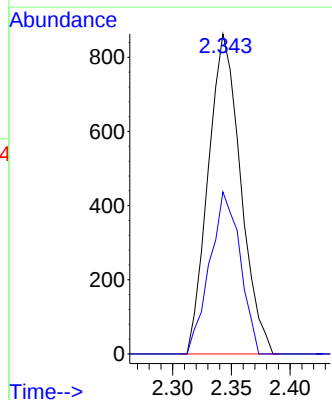
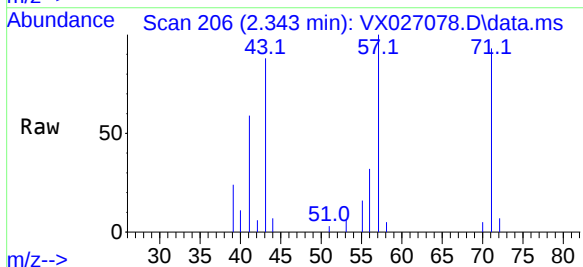




#14
 Allyl chloride
 Concen: 1.644 ug/l
 RT: 2.788 min Scan# 21
 Delta R.T. 0.122 min
 Lab File: VX027078.D
 Acq: 17 Feb 2022 15:23




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-11R


Tgt Ion: 41 Resp: 3292
 Ion Ratio Lower Upper
 41 100
 39 47.5 54.2 81.4#
 76 0.0 25.2 37.8#

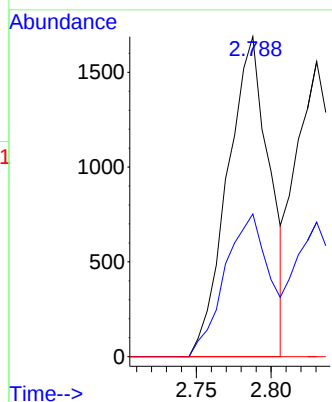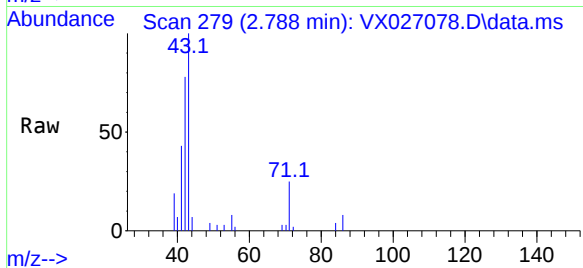

#15
 Acrylonitrile
 Concen: 0.606 ug/l
 RT: 3.105 min Scan# 331
 Delta R.T. 0.036 min
 Lab File: VX027078.D
 Acq: 17 Feb 2022 15:23

Tgt Ion: 53 Resp: 416
 Ion Ratio Lower Upper
 53 100
 52 0.0 66.6 100.0#
 51 44.7 29.5 44.3#



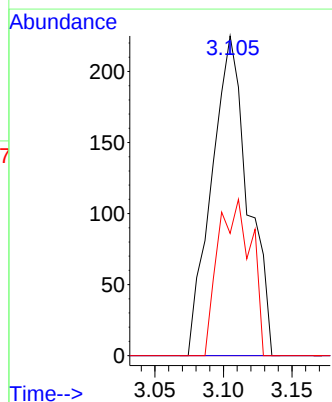
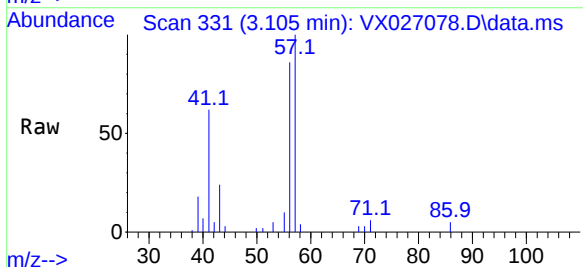




#16
Acetone
Concen: 8.098 ug/l
RT: 2.343 min Scan# 206
Delta R.T. -0.043 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-11R


Tgt Ion: 43 Resp: 4717
Ion Ratio Lower Upper
43 100
58 5.9 23.0 34.6#

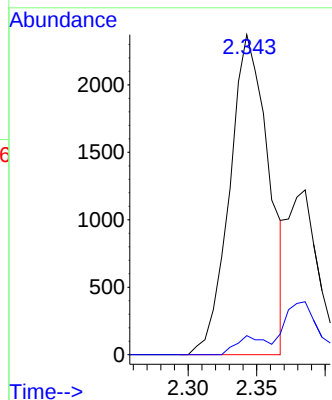

#18
Methyl Acetate
Concen: 5.457 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.079 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23

Tgt Ion: 43 Resp: 9146
Ion Ratio Lower Upper
43 100
74 0.0 18.3 27.5#

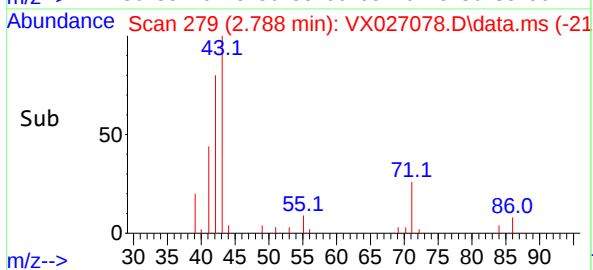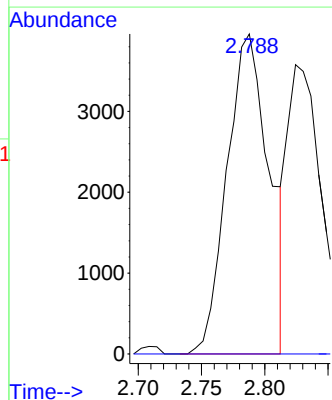







#20
Methylene Chloride
Concen: 0.219 ug/l
RT: 2.794 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23

Instrument :
MSVOA_X
ClientSampleId :
MW-11R

Tgt Ion: 84 Resp: 276




Ion	Ratio	Lower	Upper
84	100		
49	69.4	101.5	152.3#
51	66.5	31.2	46.8#
86	67.9	51.3	76.9

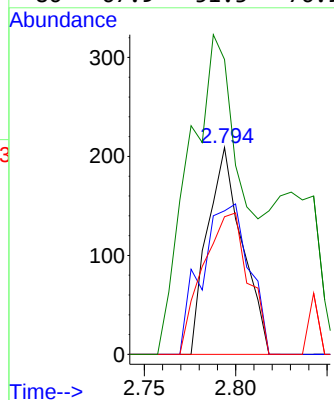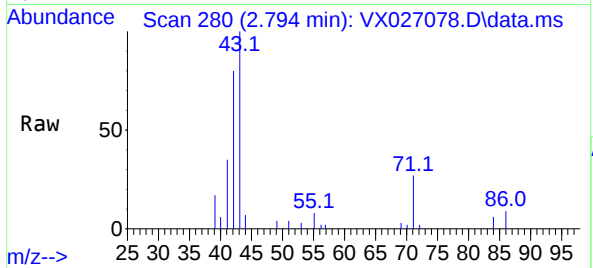


#30
Chloroform
Concen: 0.427 ug/l
RT: 5.171 min Scan# 670
Delta R.T. 0.073 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23

Tgt Ion: 83 Resp: 967


Ion	Ratio	Lower	Upper
83	100		
85	0.0	51.6	77.4#

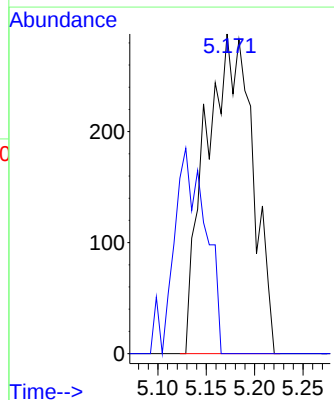






#31
Cyclohexane
Concen: 1.125 ug/l
RT: 5.549 min Scan# 71
Delta R.T. 0.073 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23

Instrument :
MSVOA_X
ClientSampleId :
MW-11R



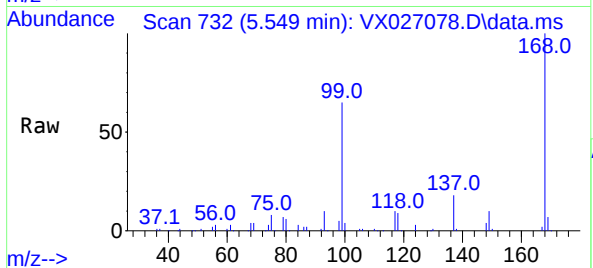



Tgt Ion: 56 Resp: 2371
Ion Ratio Lower Upper
56 100
69 143.4 25.8 38.6#
84 117.7 68.9 103.3#

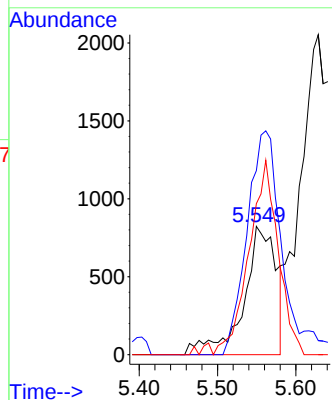

#33
1,2-Dichloroethane-d4
Concen: 52.963 ug/l
RT: 5.964 min Scan# 800
Delta R.T. -0.000 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23

Tgt Ion: 65 Resp: 70238
Ion Ratio Lower Upper
65 100
67 52.1 0.0 100.8


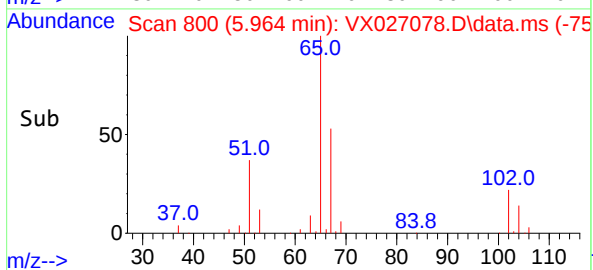
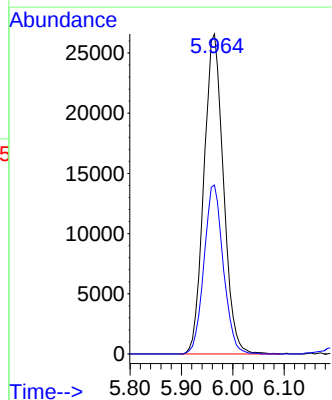



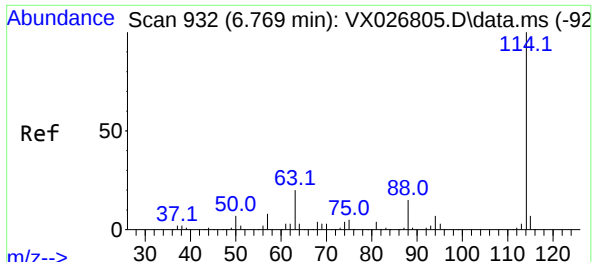

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-11R


Tgt Ion:114 Resp: 187138
Ion Ratio Lower Upper
114 100
63 19.7 0.0 42.8
88 15.5 0.0 33.0

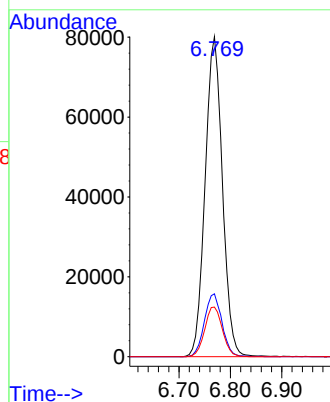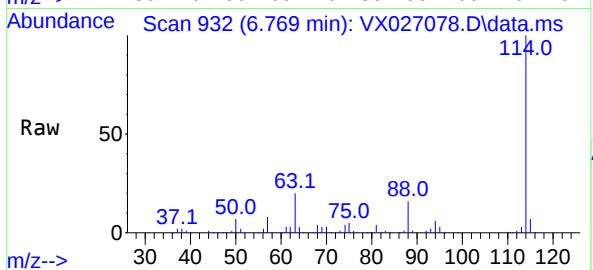

#35
Dibromofluoromethane
Concen: 52.640 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.000 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23


Tgt Ion:113 Resp: 58690
Ion Ratio Lower Upper
113 100
111 101.0 81.2 121.8
192 19.5 15.0 22.4





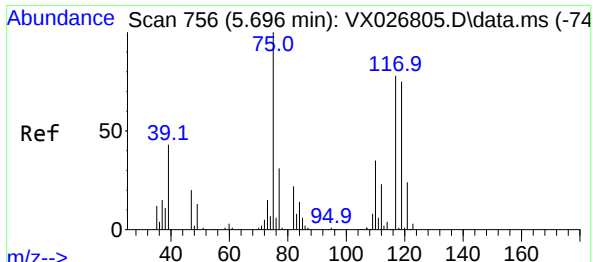


#36
1,1-Dichloropropene
Concen: 4.675 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.140 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23


Instrument :
MSVOA_X
ClientSampleId :
MW-11R

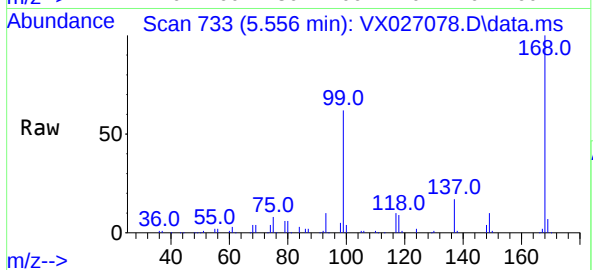



Tgt Ion: 75 Resp: 8223
Ion Ratio Lower Upper
75 100
110 9.2 17.2 51.6#
77 0.0 24.6 36.8#

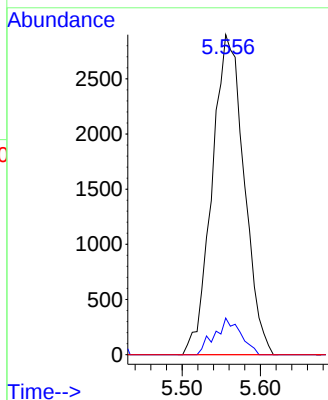


#38
Carbon Tetrachloride
Concen: 6.073 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.122 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23



Tgt Ion: 117 Resp: 11201
Ion Ratio Lower Upper
117 100
119 5.2 74.7 112.1#
121 0.0 25.4 38.0#

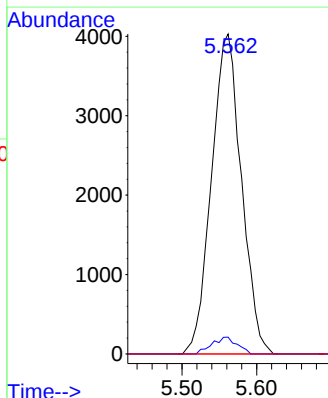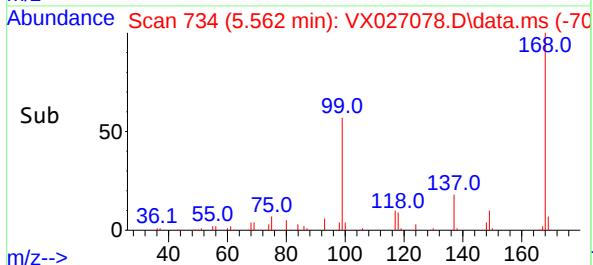



#39

Methylcyclohexane

Concen: 0.294 ug/l

RT: 7.366 min Scan# 10

Delta R.T. -0.018 min

Lab File: VX027078.D

Acq: 17 Feb 2022 15:23

Instrument :

MSVOA_X

ClientSampleId :

MW-11R





Tgt Ion: 83 Resp: 634

Ion Ratio Lower Upper

83 100

55 173.5 63.6 95.4#

98 24.3 38.4 57.6#

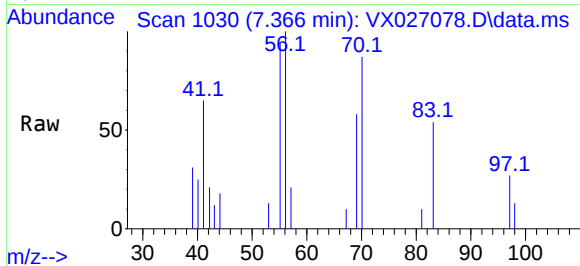

#40

Benzene

Concen: 1.049 ug/l

RT: 6.043 min Scan# 813

Delta R.T. -0.000 min

Lab File: VX027078.D




Acq: 17 Feb 2022 15:23


Tgt Ion: 78 Resp: 5375

Ion Ratio Lower Upper

78 100

77 23.6 18.9 28.3

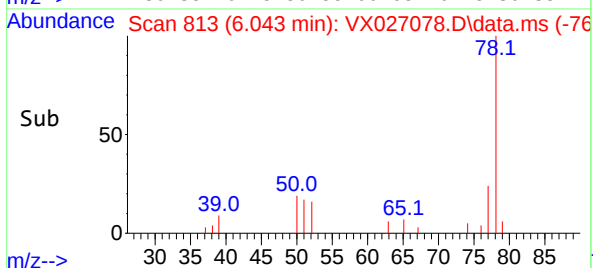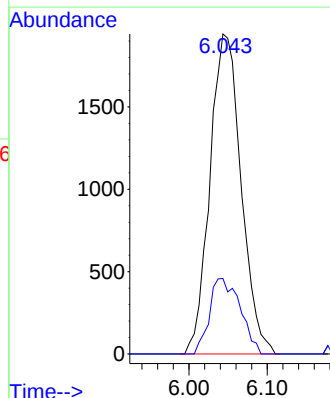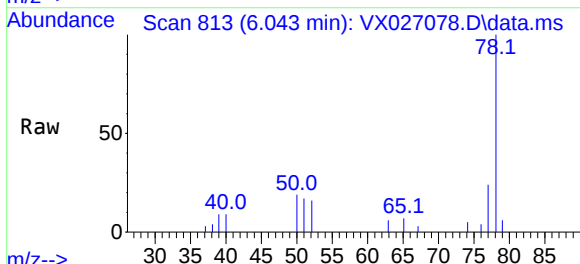







#41
Methacrylonitrile
Concen: 0.618 ug/l
RT: 5.135 min Scan# 61
Delta R.T. 0.213 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23

Instrument :
MSVOA_X
ClientSampleId :
MW-11R

Tgt Ion: 41 Resp: 670




Ion	Ratio	Lower	Upper
41	100		
39	54.9	45.4	68.0
67	0.0	53.2	79.8#
52	0.0	23.0	34.6#

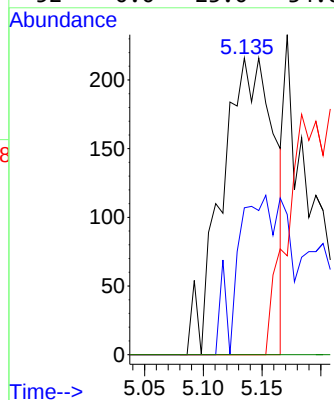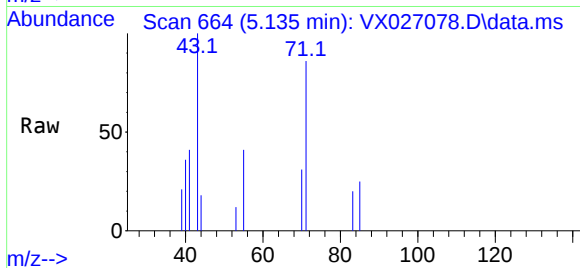


#48
Methyl methacrylate
Concen: 0.411 ug/l
RT: 7.775 min Scan# 1097
Delta R.T. 0.079 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23

Tgt Ion: 41 Resp: 627

Ion	Ratio	Lower	Upper
41	100		
69	64.0	62.2	93.4
39	58.2	45.4	68.0



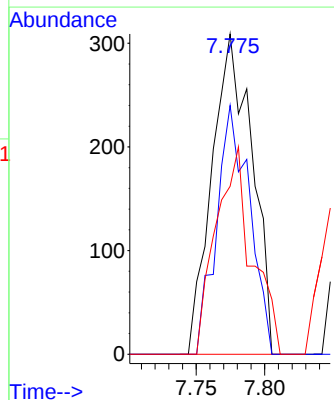
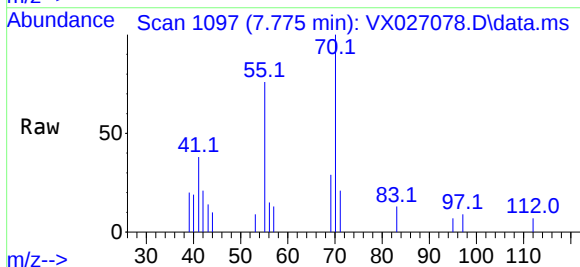




#50
Toluene-d8
Concen: 52.580 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-11R


Tgt Ion: 98 Resp: 215189
Ion Ratio Lower Upper
98 100
100 66.4 53.2 79.8

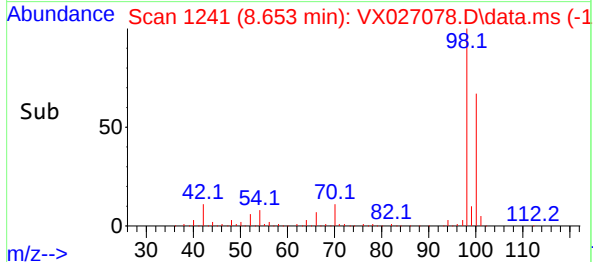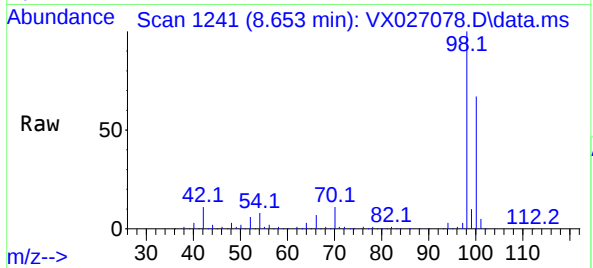

#52
Toluene
Concen: 0.218 ug/l
RT: 8.726 min Scan# 1253
Delta R.T. 0.006 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23

Tgt Ion: 92 Resp: 708
Ion Ratio Lower Upper
92 100
91 149.4 135.7 203.5

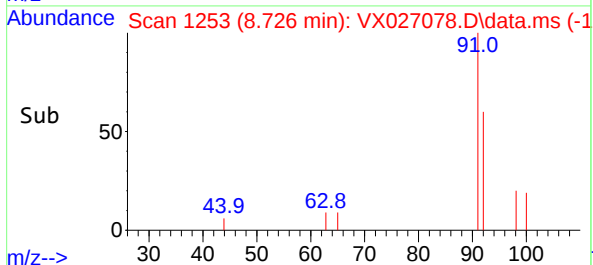







#55
1,1,2-Trichloroethane
Concen: 1.352 ug/l
RT: 9.104 min Scan# 1315
Delta R.T. -0.049 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23

Instrument :
MSVOA_X
ClientSampleId :
MW-11R

Tgt Ion: 97 Resp: 1661




Ion	Ratio	Lower	Upper
97	100		
83	12.5	68.4	102.6#
85	0.0	44.0	66.0#
99	0.0	49.8	74.6#

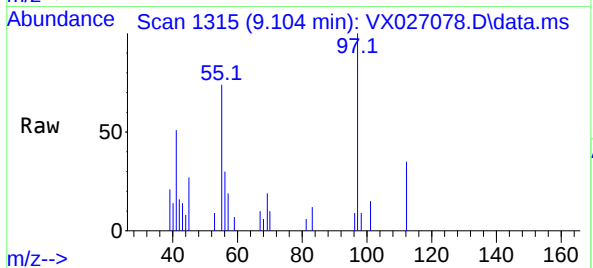


#56
Ethyl methacrylate
Concen: 0.224 ug/l
RT: 9.104 min Scan# 1315
Delta R.T. -0.012 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23

Tgt Ion: 69 Resp: 437

Ion	Ratio	Lower	Upper
69	100		
41	0.0	57.2	85.8#
39	104.3	30.9	46.3#


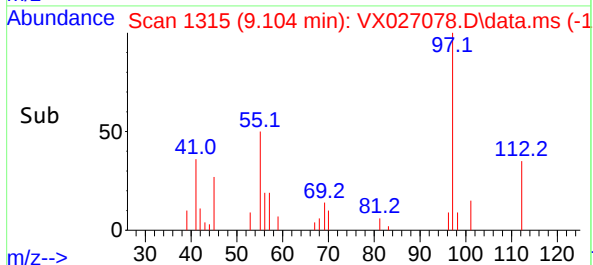
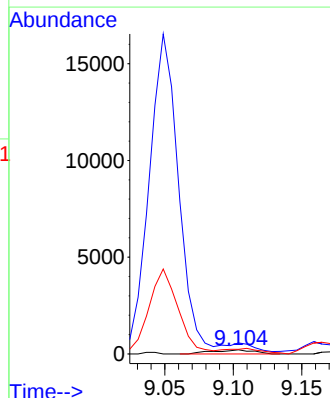





#59
2-Hexanone
Concen: 0.418 ug/l
RT: 9.451 min Scan# 11
Delta R.T. 0.018 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-11R


Tgt Ion: 43 Resp: 570
Ion Ratio Lower Upper
43 100
58 34.9 26.4 79.2

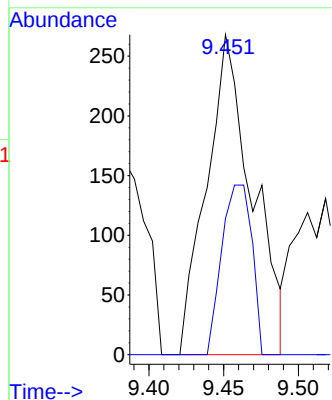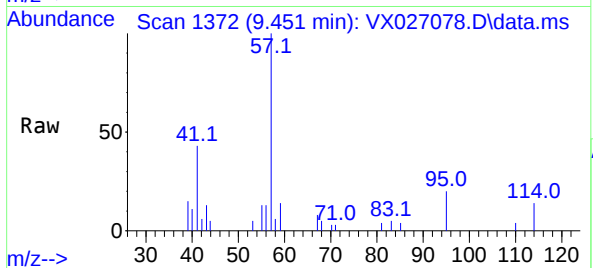

#62
4-Bromofluorobenzene
Concen: 53.446 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23

Tgt Ion: 95 Resp: 77008
Ion Ratio Lower Upper
95 100
174 76.5 0.0 148.6
176 74.0 0.0 141.4


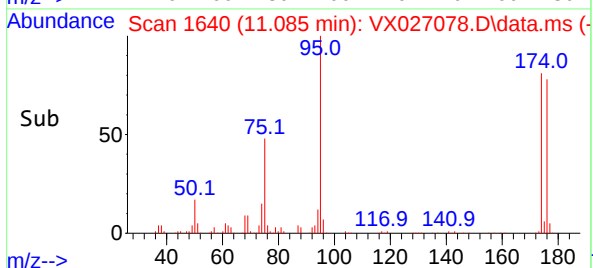
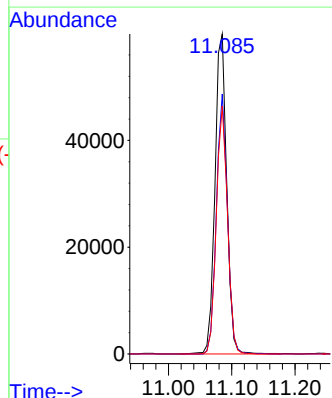



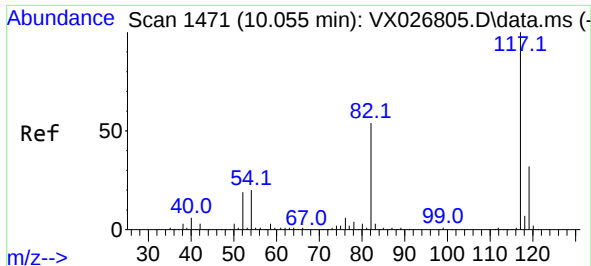

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-11R


Tgt Ion:117 Resp: 164813
Ion Ratio Lower Upper
117 100
82 55.0 45.2 67.8
119 30.9 26.2 39.2

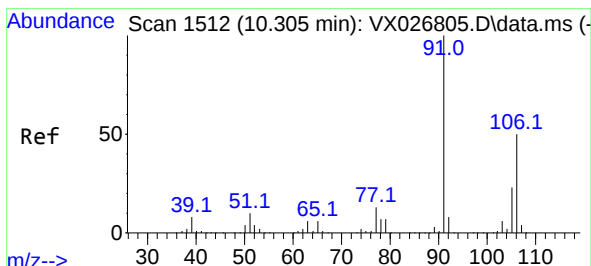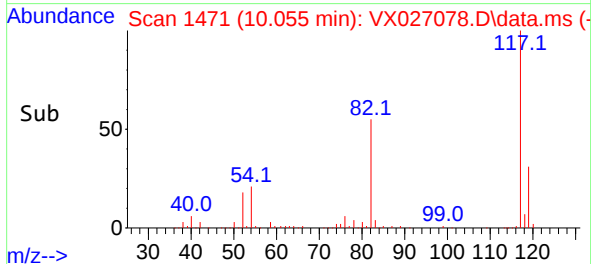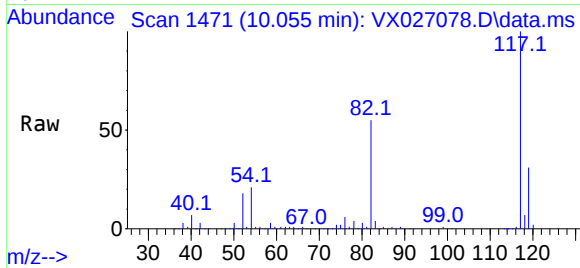

#68
m/p-Xylenes
Concen: 0.216 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23

Tgt Ion:106 Resp: 502
Ion Ratio Lower Upper
106 100
91 214.7 165.3 247.9


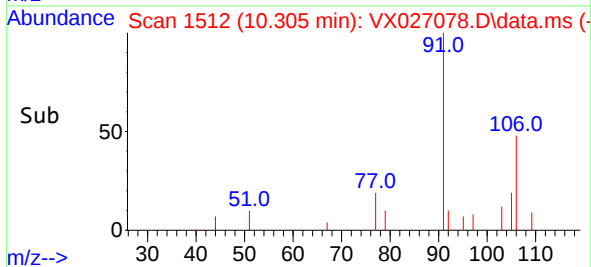

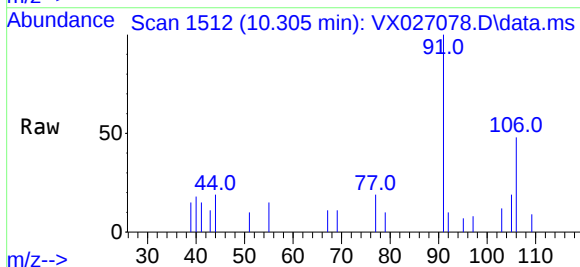


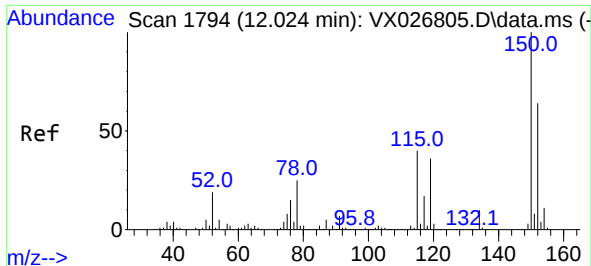

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-11R


Tgt Ion:152 Resp: 71705
Ion Ratio Lower Upper
152 100
115 60.0 44.2 132.6
150 156.7 0.0 348.2

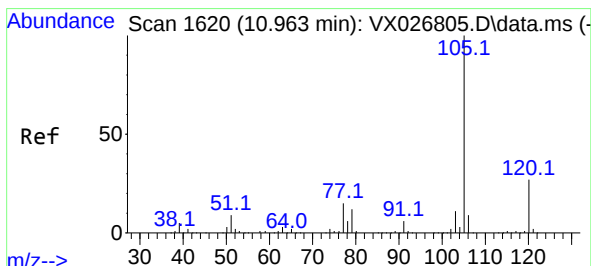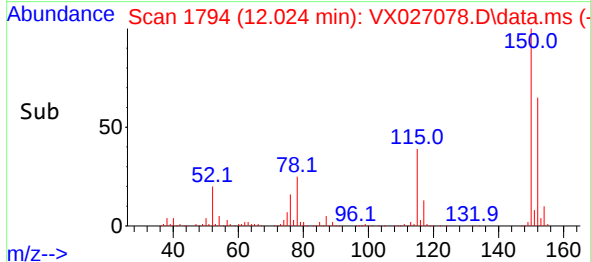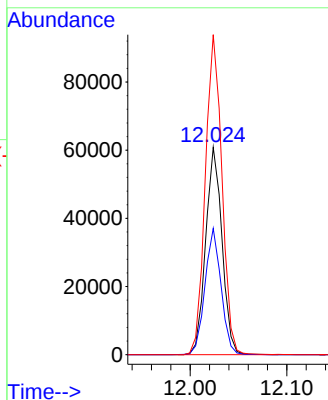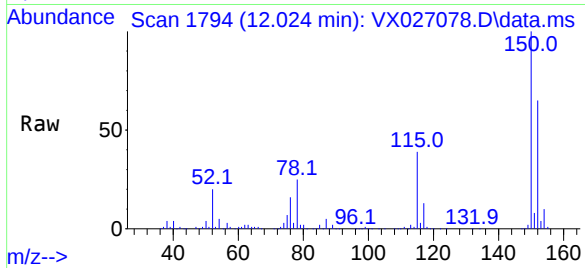

#73
Isopropylbenzene
Concen: 0.453 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. -0.000 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23

Tgt Ion:105 Resp: 2561
Ion Ratio Lower Upper
105 100
120 25.8 13.1 39.1


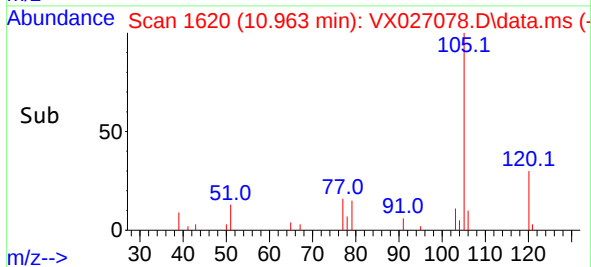
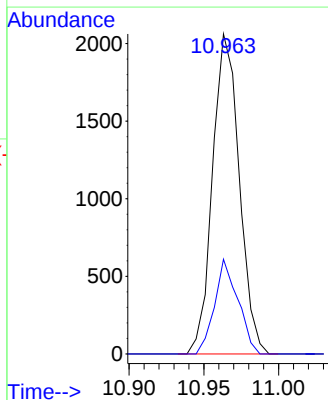
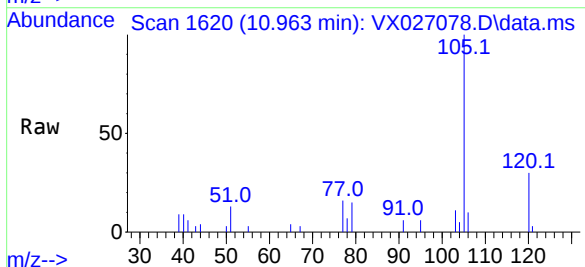


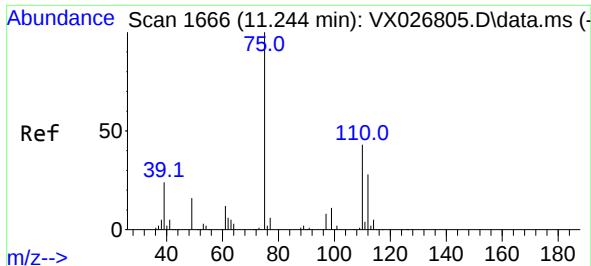

#76
1,2,3-Trichloropropane
Concen: 23.821 ug/l
RT: 11.085 min Scan# 11085
Delta R.T. -0.159 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-11R


Tgt Ion: 75 Resp: 37391
Ion Ratio Lower Upper
75 100
77 1.3 18.3 54.8#

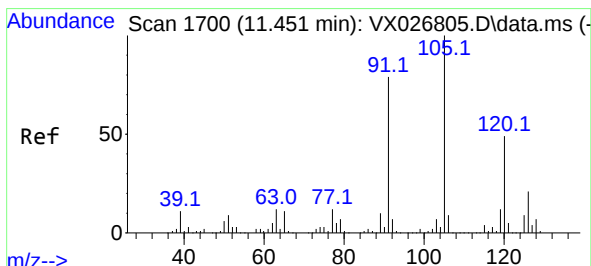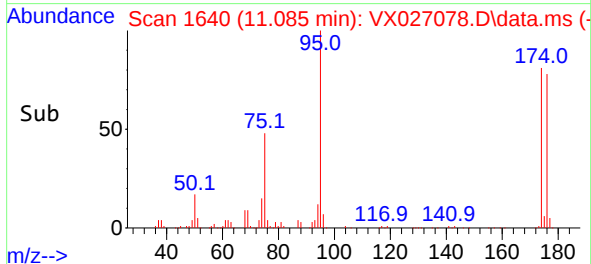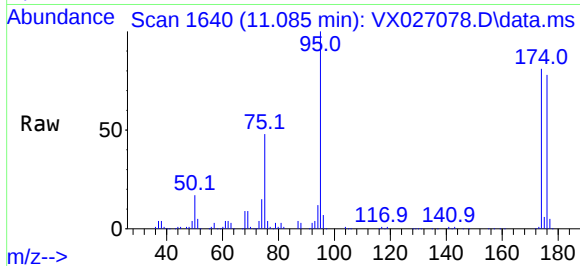

#80
1,3,5-Trimethylbenzene
Concen: 0.928 ug/l
RT: 11.615 min Scan# 1727
Delta R.T. 0.164 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23

Tgt Ion:105 Resp: 4314
Ion Ratio Lower Upper
105 100
120 31.4 24.0 72.0


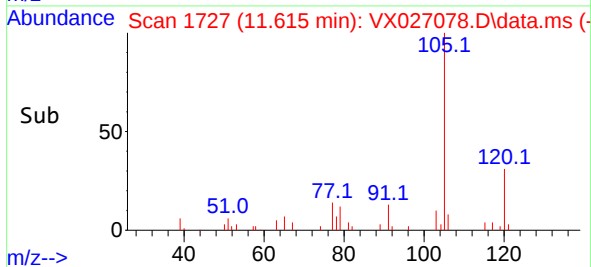

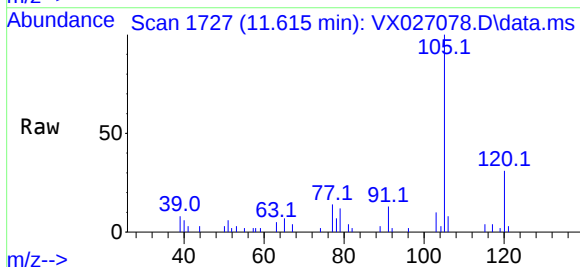


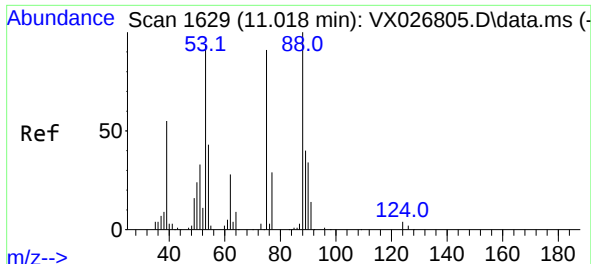

#81
trans-1,4-Dichloro-2-butene
Concen: 72.820 ug/l
RT: 11.085 min Scan# 1629
Delta R.T. 0.067 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23




Instrument :
MSVOA_X
ClientSampleId :
MW-11R


Tgt Ion: 75 Resp: 37391
Ion Ratio Lower Upper
75 100
53 0.0 94.0 141.0#
89 0.0 37.0 55.4#

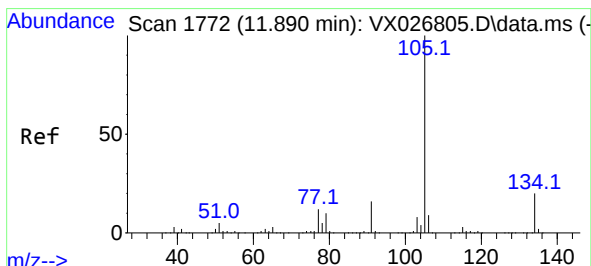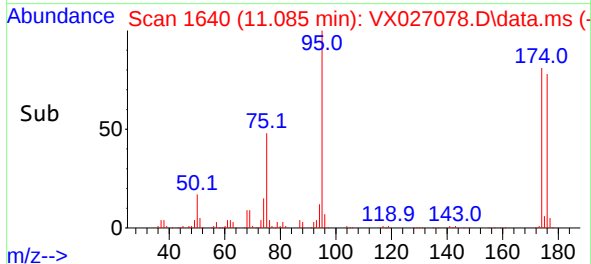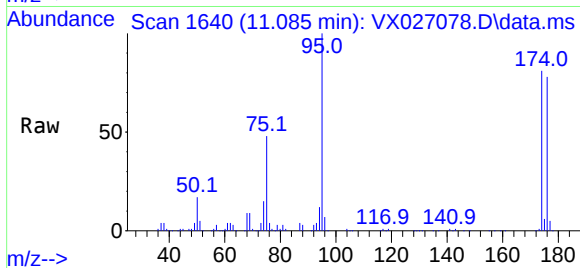

#85
sec-Butylbenzene
Concen: 0.904 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. -0.000 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23

Tgt Ion: 105 Resp: 5078
Ion Ratio Lower Upper
105 100
134 26.5 10.1 30.1

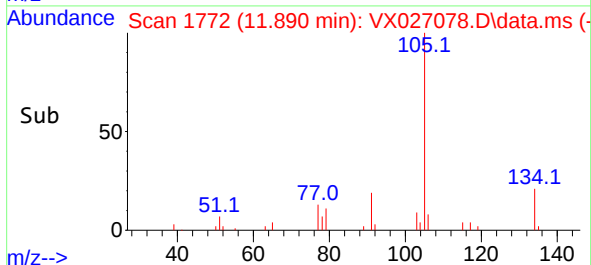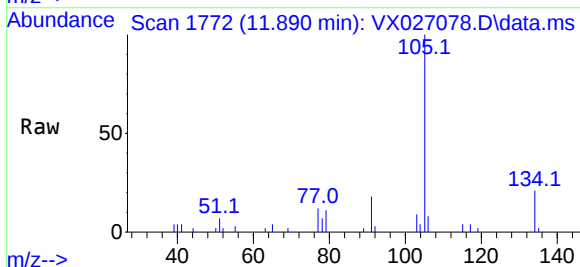

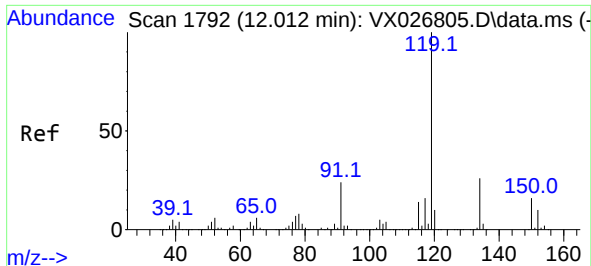

#86

p-Isopropyltoluene

Concen: 0.734 ug/l

RT: 12.182 min Scan# 119

Delta R.T. 0.171 min

Lab File: VX027078.D

Acq: 17 Feb 2022 15:23

Instrument :

MSVOA_X

ClientSampleId :

MW-11R





Tgt Ion:119 Resp: 3492

Ion Ratio Lower Upper

119 100

134 29.0 13.0 39.0

91 25.6 12.6 37.6

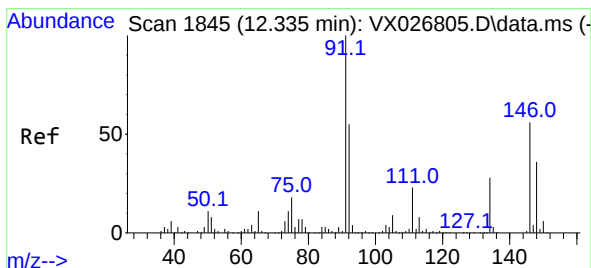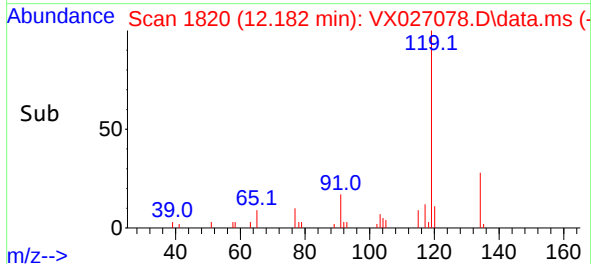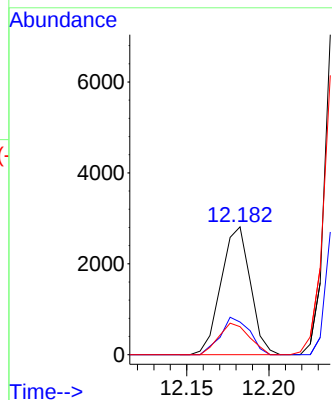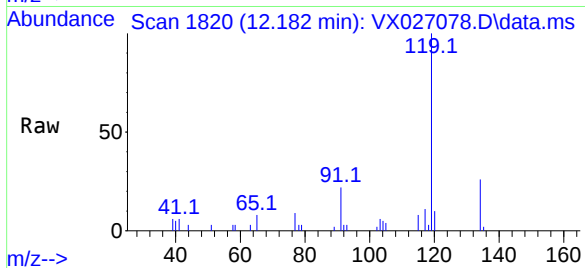

#89

n-Butylbenzene

Concen: 0.600 ug/l

RT: 12.317 min Scan# 1842

Delta R.T. -0.018 min

Lab File: VX027078.D

Acq: 17 Feb 2022 15:23




Tgt Ion: 91 Resp: 2335


Ion Ratio Lower Upper

91 100

92 11.6 27.2 81.6#

134 124.0 13.1 39.1#


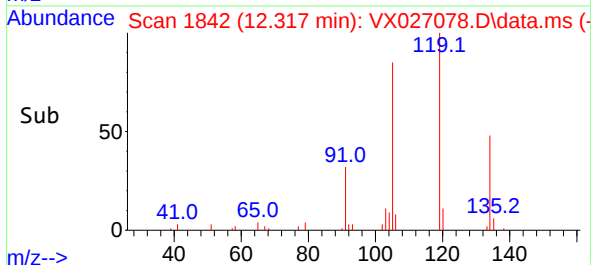
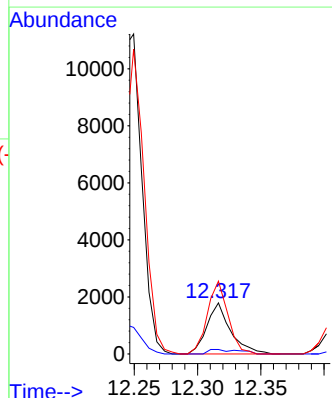
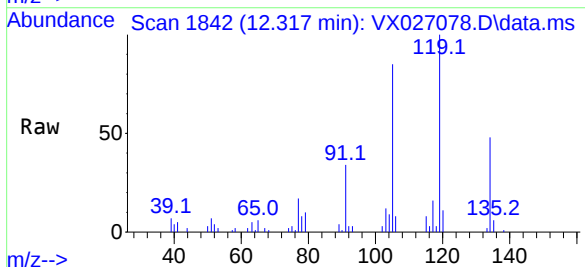


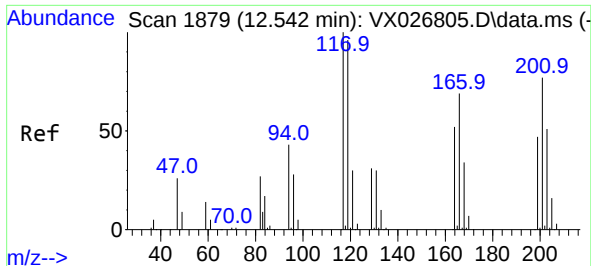

#90
Hexachloroethane
Concen: 4.472 ug/l
RT: 12.615 min Scan# 1879
Delta R.T. 0.073 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23

Instrument : MSVOA_X
ClientSampleId : MW-11R

Tgt Ion:117 Resp: 3075
Ion Ratio Lower Upper
117 100
201 0.0 35.6 106.8#

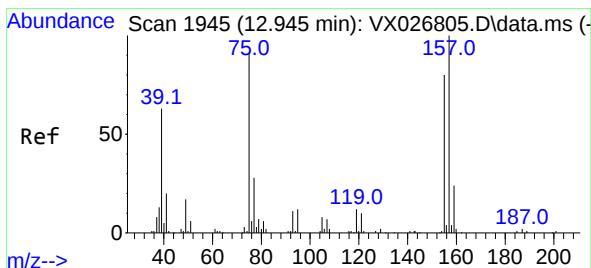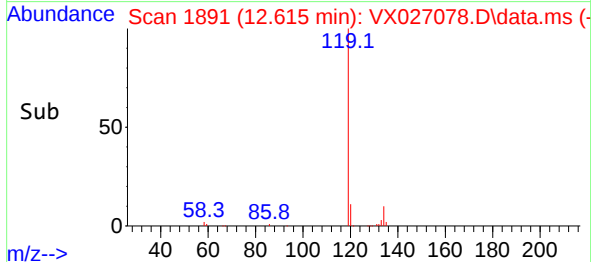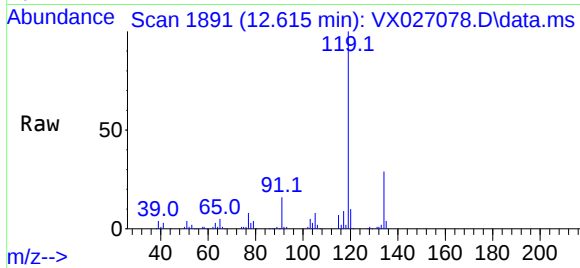

#92
1,2-Dibromo-3-Chloropropane
Concen: 1.138 ug/l
RT: 13.170 min Scan# 1982
Delta R.T. 0.225 min
Lab File: VX027078.D
Acq: 17 Feb 2022 15:23

Tgt Ion: 75 Resp: 429
Ion Ratio Lower Upper
75 100
155 0.0 40.0 119.9#
157 0.0 51.6 154.8#

